


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN073118\
Data File : VN050201.D
Acq On : 31 Jul 2018 7:43
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Title : SW846 8260
Last Update : Thu Jul 26 18:10:10 2018

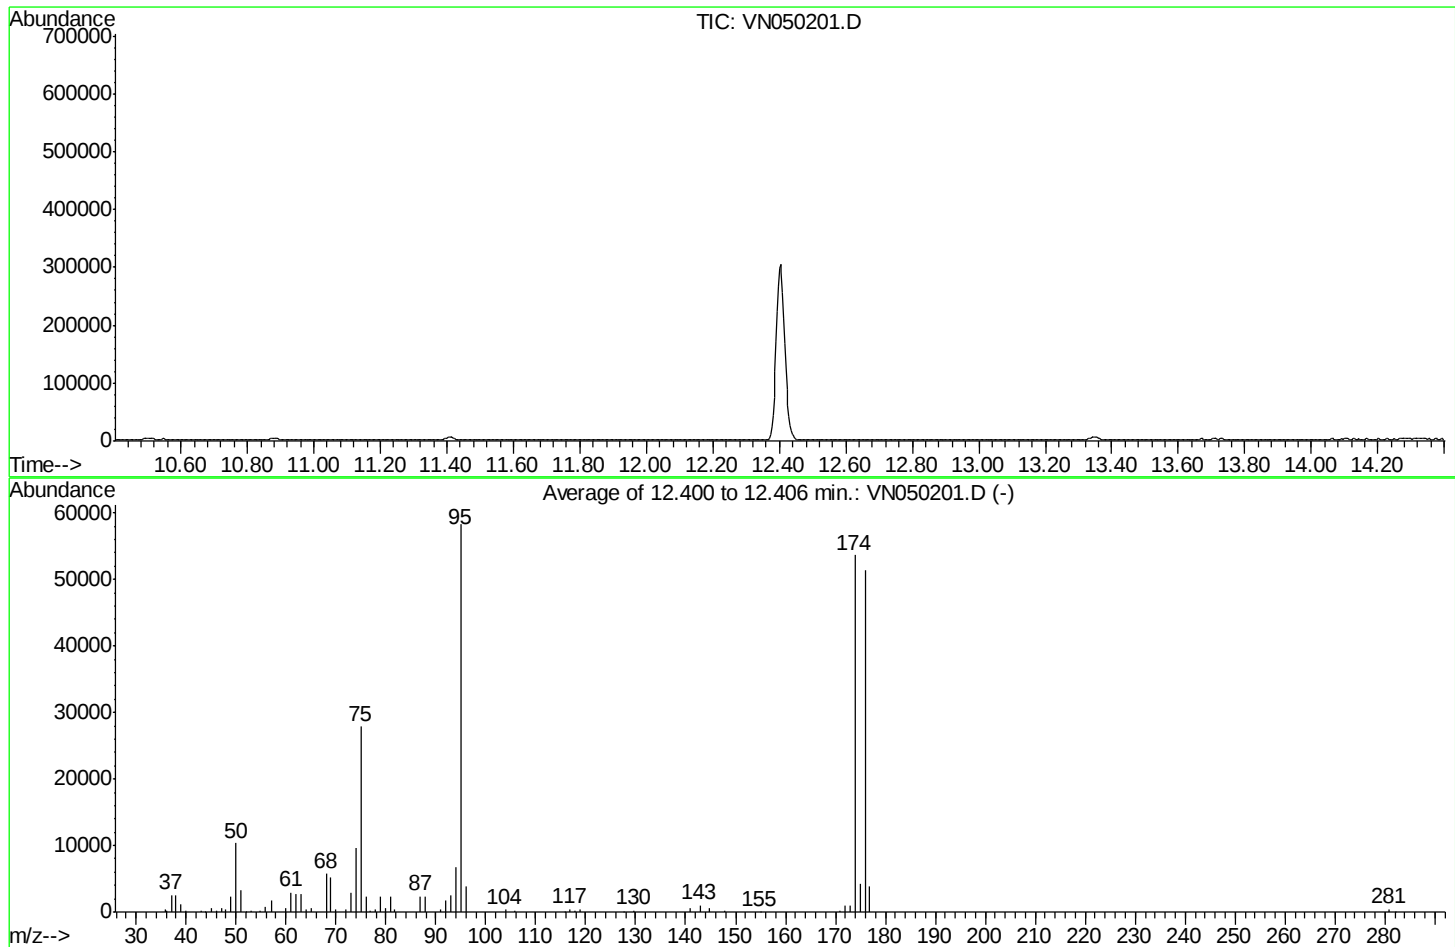

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	10357	PASS
75	95	30	60	47.8	27882	PASS
95	95	100	100	100.0	58290	PASS
96	95	5	9	6.7	3899	PASS
173	174	0.00	2	1.7	888	PASS
174	95	50	100	92.0	53629	PASS
175	174	5	9	7.8	4184	PASS
176	174	95	101	95.9	51410	PASS
177	176	5	9	7.4	3823	PASS