

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN073120\
 Data File : VN062678.D
 Acq On : 31 Jul 2020 12:16
 Operator : JC/MD
 Sample : PB130640ZHE#01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130640ZHE#01

Quant Time: Aug 01 06:03:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072120W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 21 18:48:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	131307	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	235398	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	241387	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	83254	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	113578	55.68	ug/l	0.00
Spiked Amount			Recovery	=	111.36%	
35) Dibromofluoromethane	7.55	113	80487	52.05	ug/l	0.00
Spiked Amount			Recovery	=	104.10%	
50) Toluene-d8	10.06	98	318119	51.56	ug/l	0.00
Spiked Amount			Recovery	=	103.12%	
62) 4-Bromofluorobenzene	12.38	95	114191	50.62	ug/l	0.00
Spiked Amount			Recovery	=	101.24%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
8) Diethyl Ether	3.38	74	930	0.920	ug/l	96
11) Tert butyl alcohol	4.74	59	150	0.462	ug/l #	73
16) Acetone	3.78	43	15517	20.215	ug/l	95
18) Methyl Acetate	4.28	43	1942	0.999	ug/l	95
20) Methylene Chloride	4.50	84	16324	8.867	ug/l	93
25) 2-Butanone	6.80	43	1016	0.869	ug/l #	52
31) Cyclohexane	7.63	56	3250	1.081	ug/l #	15
36) 1,1-Dichloropropene	7.62	75	12095	4.820	ug/l #	51
38) Carbon Tetrachloride	7.63	117	14157	5.870	ug/l #	16
43) Isopropyl Acetate	8.13	43	48852	11.204	ug/l #	89
45) 1,2-Dichloropropane	9.24	63	1137	0.533	ug/l #	44
48) Methyl methacrylate	9.15	41	2813	1.357	ug/l #	15
51) 4-Methyl-2-Pentanone	9.95	43	6187	2.372	ug/l	91
54) cis-1,3-Dichloropropene	9.87	75	19990	6.266	ug/l #	64
56) Ethyl methacrylate	10.52	69	882	2.046	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	3452	1.101	ug/l #	42
59) 2-Hexanone	10.74	43	55048	29.920	ug/l #	54
71) Bromoform	12.38	173	612	0.428	ug/l #	1
74) N-amyl acetate	12.01	43	2255	0.767	ug/l #	47
76) 1,2,3-Trichloropropane	12.38	75	63752	30.084	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	2098	0.384	ug/l	88
81) trans-1,4-Dichloro-2-buten	12.38	75	63752	83.748	ug/l #	12
93) 1,2,4-Trichlorobenzene	14.89	180	111	3.178	ug/l #	32
95) Naphthalene	15.12	128	1133	4.044	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN073120\
Data File : VN062678.D
Acq On : 31 Jul 2020 12:16
Operator : JC/MD
Sample : PB130640ZHE#01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB130640ZHE#01

Quant Time: Aug 01 06:03:50 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072120W.M
Quant Title : SW846 8260
QLast Update : Tue Jul 21 18:48:59 2020
Response via : Initial Calibration

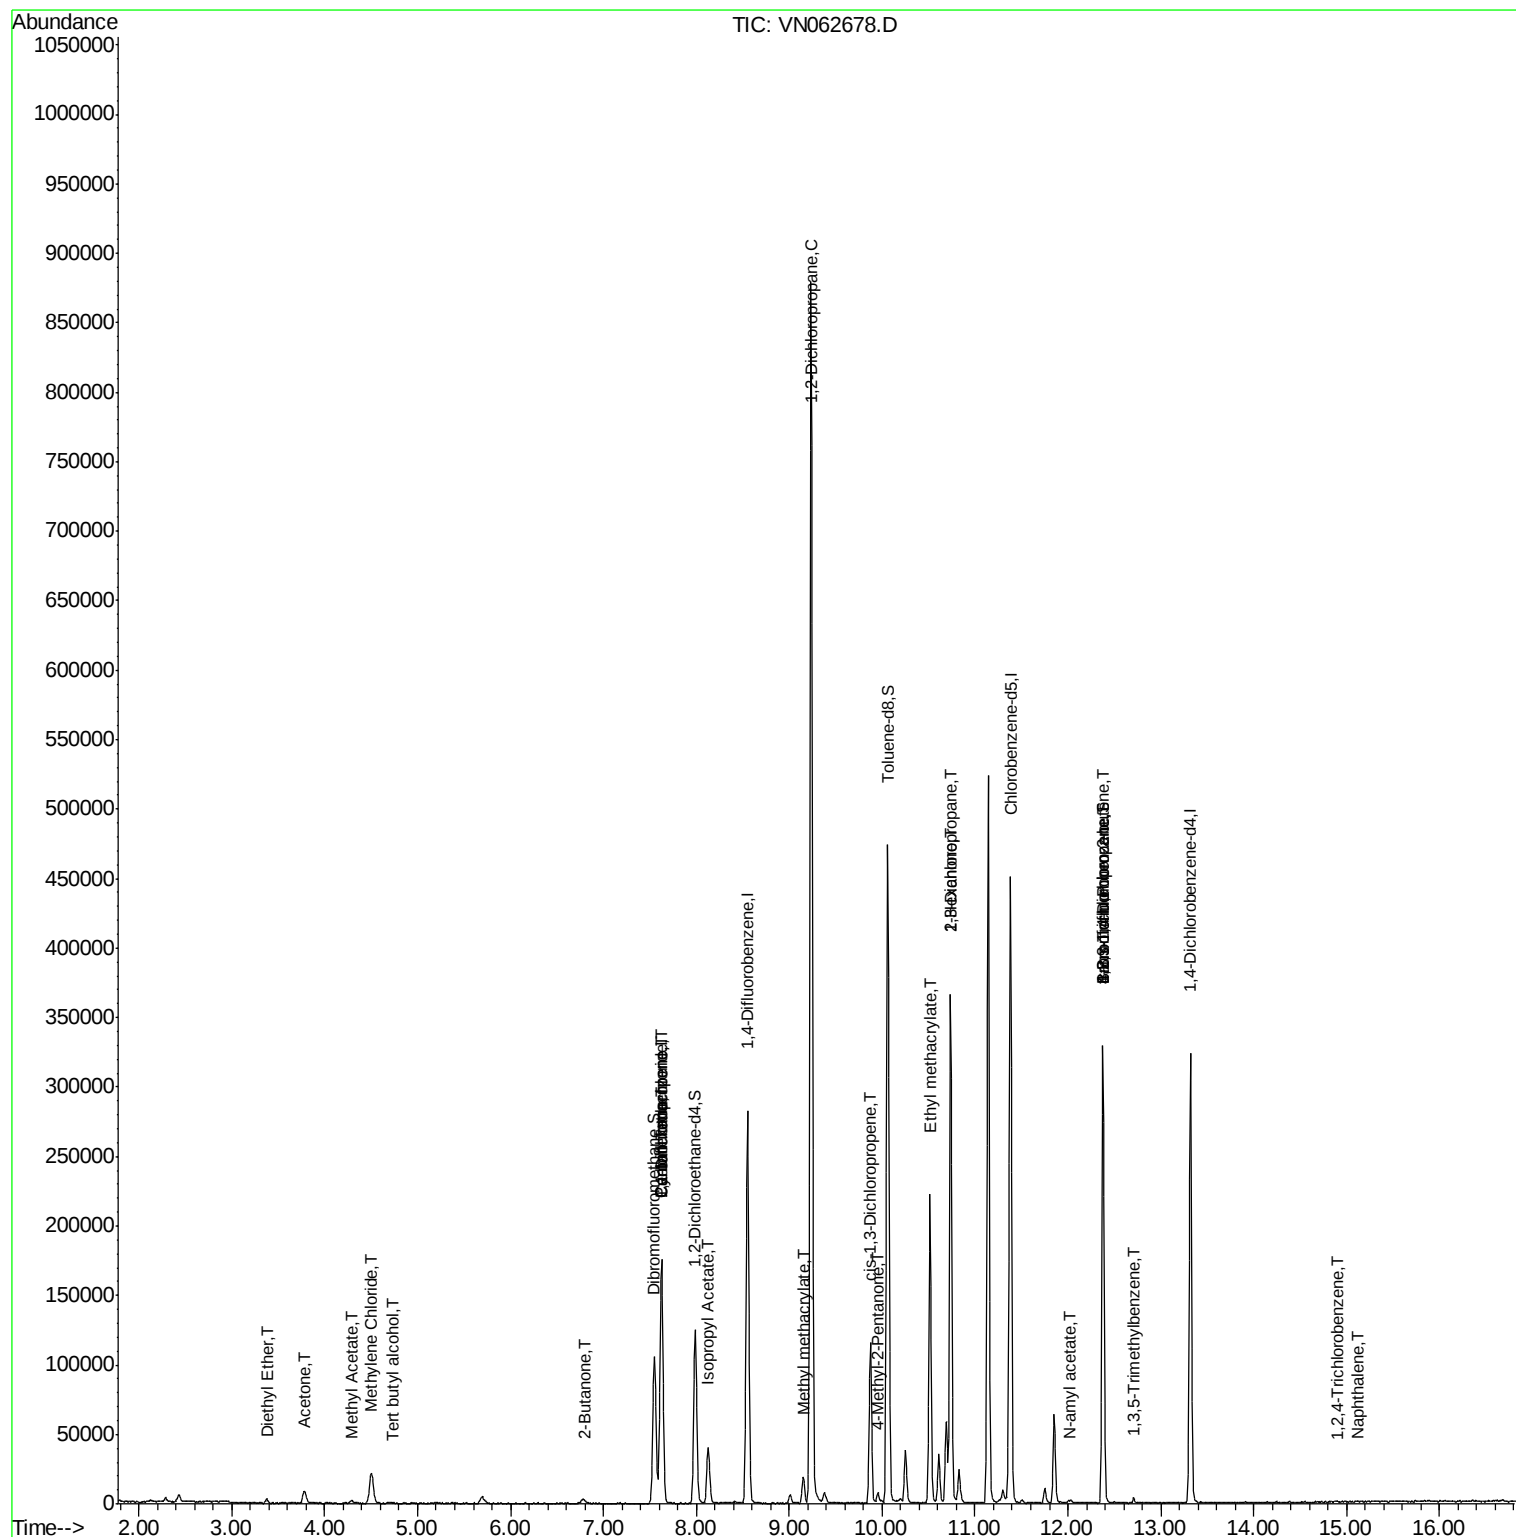

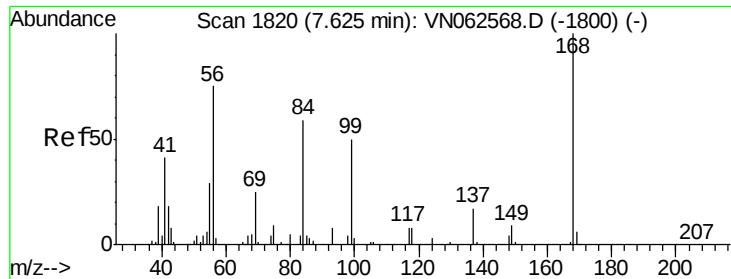

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1821

Delta R.T. 0.00 min

Lab File: VN062678.D

Acq: 31 Jul 2020 12:16

Instrument :

MSVOA_N

ClientSampleId :


PB130640ZHE#01

Tot Ion:168 Resp: 131307

Ion Ratio Lower Upper

168 100

99 65.6 48.4 72.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

60000

50000

40000



30000

20000

10000

0

Time-->



#8

Diethyl Ether

Concen: 0.920 ug/l

RT: 3.38 min Scan# 499

Delta R.T. 0.01 min

Lab File: VN062678.D


Acq: 31 Jul 2020 12:16

Tgt Ion: 74 Resp: 930

Ion Ratio Lower Upper

74 100

45 114.8 55.3 165.8



Abundance Ion 74.00 (73.70 to 74.70): VN

Ion 45.00 (44.70 to 45.70): VN

3.38


600


400

200

0

Time-->









#11

Tert butyl alcohol
 Concen: 0.462 ug/l
 RT: 4.74 min Scan# 923
 Delta R.T. 0.01 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130640ZHE#01




Tot Ion: 59 Resp: 150
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.2 12.2#

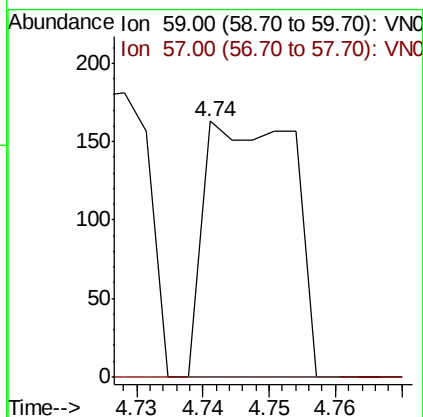


#16

Acetone
 Concen: 20.215 ug/l
 RT: 3.78 min Scan# 624
 Delta R.T. 0.01 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Tgt Ion: 43 Resp: 15517
 Ion Ratio Lower Upper
 43 100
 58 27.9 24.6 37.0



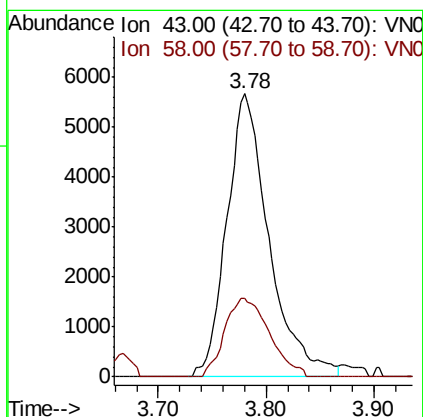





#18
Methyl Acetate
Concen: 0.999 ug/l
RT: 4.28 min Scan# 781
Delta R.T. 0.00 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16




Instrument :
MSVOA_N
ClientSampleId :
PB130640ZHE#01


Tot Ion: 43 Resp: 1942
Ion Ratio Lower Upper
43 100
74 23.2 16.6 24.8

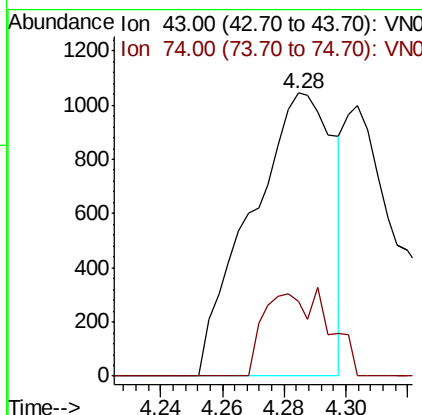

#20
Methylene Chloride
Concen: 8.867 ug/l
RT: 4.50 min Scan# 848
Delta R.T. -0.00 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16

Tgt Ion: 84 Resp: 16324
Ion Ratio Lower Upper
84 100
49 128.9 109.4 164.0
51 38.6 33.6 50.4
86 56.2 51.4 77.2


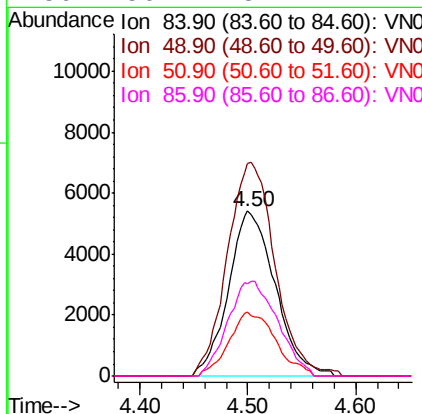






#25
2-Butanone
Concen: 0.869 ug/l
RT: 6.80 min Scan# 1563
Delta R.T. 0.01 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16




Instrument :
MSVOA_N
ClientSampleId :
PB130640ZHE#01


Tot Ion: 43 Resp: 1016
Ion Ratio Lower Upper
43 100
72 0.0 19.0 28.6#

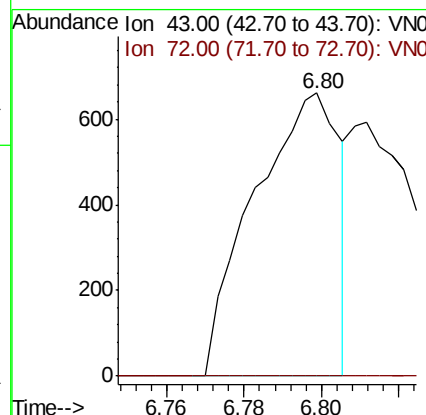

#31
Cyclohexane
Concen: 1.081 ug/l
RT: 7.63 min Scan# 1820
Delta R.T. 0.01 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16

Tgt Ion: 56 Resp: 3250
Ion Ratio Lower Upper
56 100
69 168.6 25.3 37.9#
84 91.7 61.0 91.4#



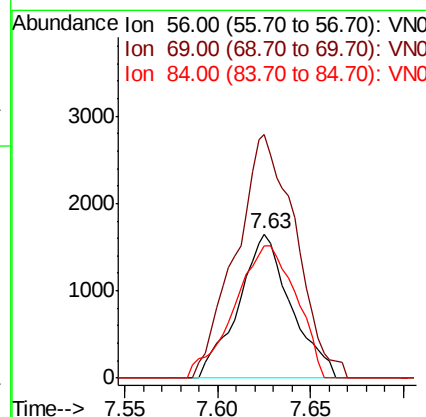



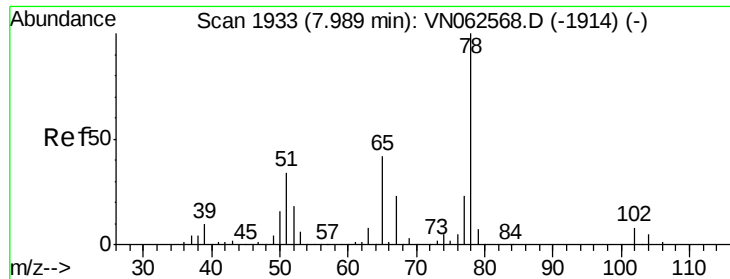

#33
 1,2-Dichloroethane-d4
 Concen: 55.681 ug/l
 RT: 7.99 min Scan# 1933
 Delta R.T. -0.00 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130640ZHE#01


Tot Ion: 65 Resp: 113578
 Ion Ratio Lower Upper
 65 100
 67 51.1 0.0 106.0

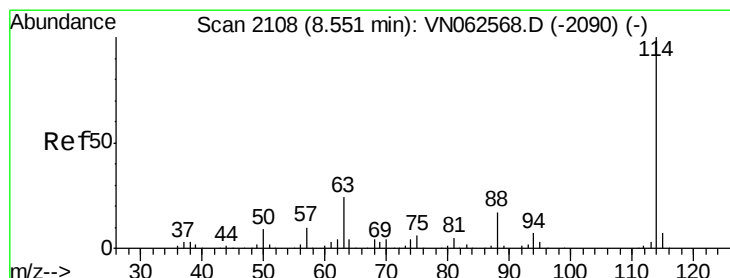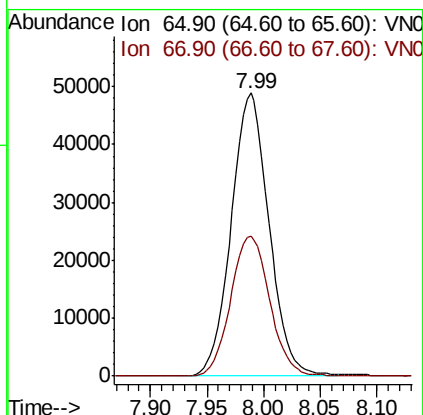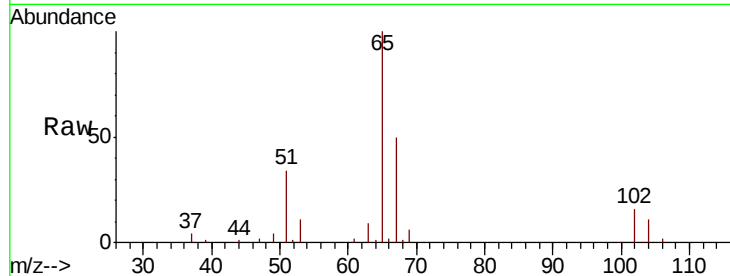

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. -0.00 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Tgt Ion: 114 Resp: 235398
 Ion Ratio Lower Upper
 114 100
 63 24.1 0.0 48.4
 88 17.7 0.0 33.8


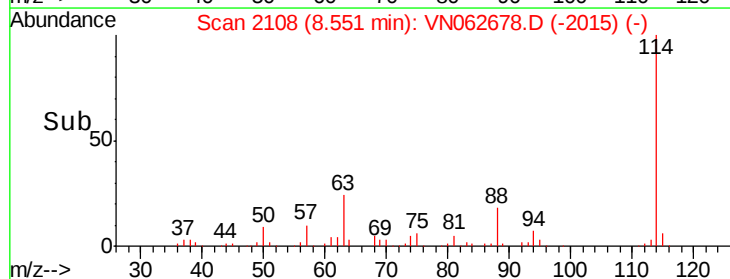
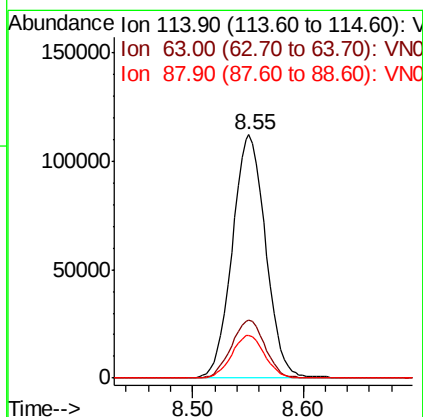
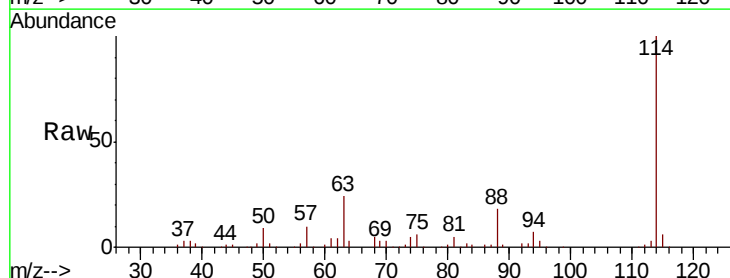




#35
 Dibromofluoromethane
 Concen: 52.054 ug/l
 RT: 7.55 min Scan# 1796
 Delta R.T. -0.00 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130640ZHE#01


Tot Ion:113 Resp: 80487
 Ion Ratio Lower Upper
 113 100
 111 102.5 82.7 124.1
 192 18.4 14.8 22.2

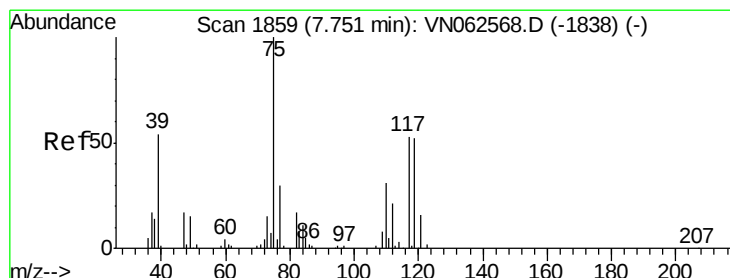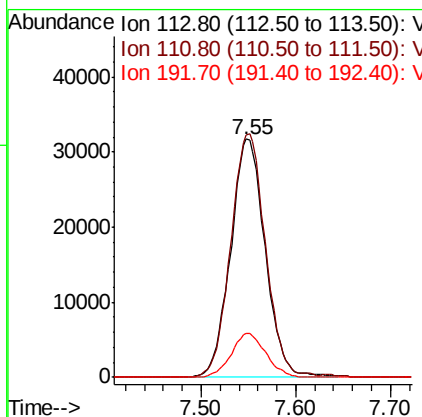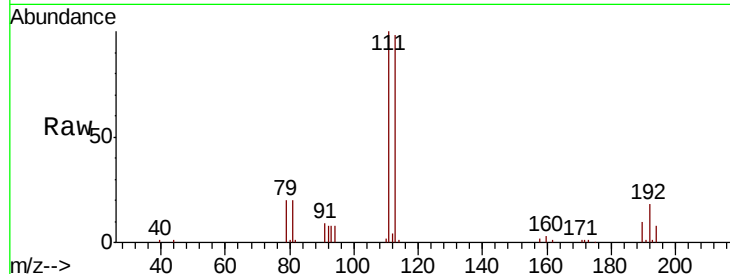

#36
 1,1-Dichloropropene
 Concen: 4.820 ug/l
 RT: 7.62 min Scan# 1819
 Delta R.T. -0.13 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Tgt Ion: 75 Resp: 12095
 Ion Ratio Lower Upper
 75 100
 110 8.8 16.0 48.0#
 77 0.0 24.6 36.8#

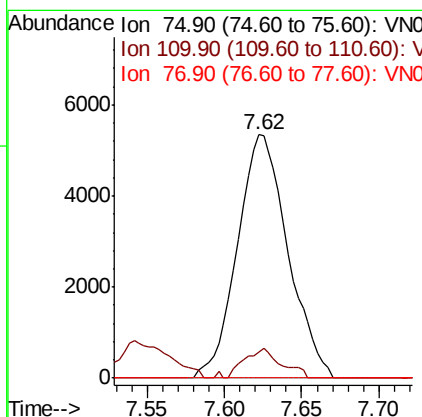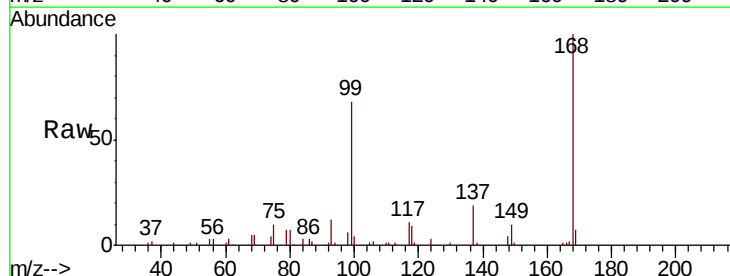


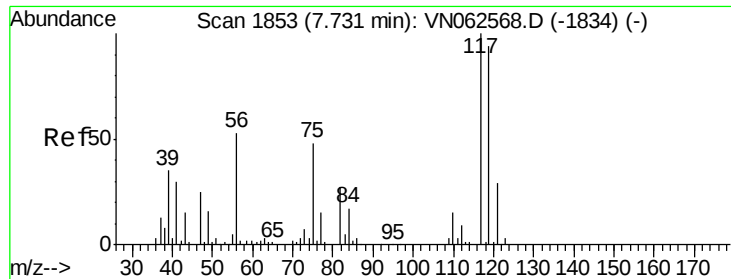




#38
Carbon Tetrachloride
Concen: 5.870 ug/l
RT: 7.63 min Scan# 1821
Delta R.T. -0.10 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16

Instrument :
MSVOA_N
ClientSampleId :
PB130640ZHE#01

Tot Ion:117 Resp: 14157
Ion Ratio Lower Upper
117 100
119 4.0 74.8 112.2#
121 0.0 23.0 34.6#




Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V


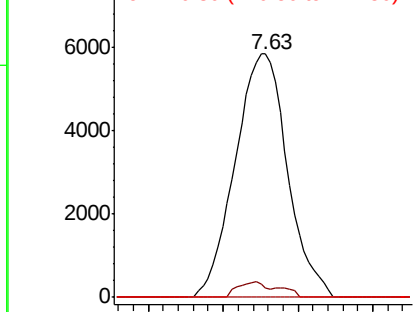



#43
Isopropyl Acetate
Concen: 11.204 ug/l
RT: 8.13 min Scan# 1976
Delta R.T. -0.00 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16

Tgt Ion: 43 Resp: 48852
Ion Ratio Lower Upper
43 100
61 18.6 20.8 31.2#
87 12.3 9.2 13.8



Abundance Ion 43.00 (42.70 to 43.70): V
Ion 61.00 (60.70 to 61.70): V
Ion 87.00 (86.70 to 87.70): V




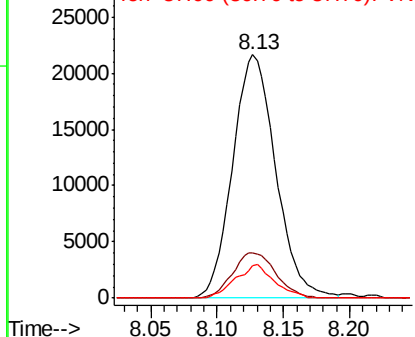


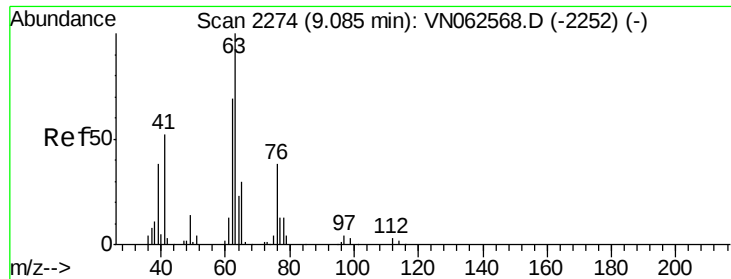

#45
 1,2-Dichloropropane
 Concen: 0.533 ug/l
 RT: 9.24 min Scan# 2322
 Delta R.T. 0.15 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130640ZHE#01


Tot Ion: 63 Resp: 1137
 Ion Ratio Lower Upper
 63 100
 65 0.0 24.4 36.6#

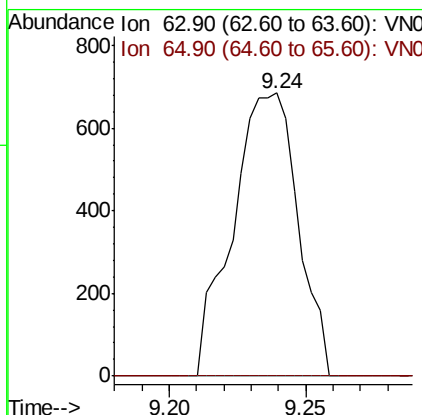

#48
 Methyl methacrylate
 Concen: 1.357 ug/l
 RT: 9.15 min Scan# 2293
 Delta R.T. -0.02 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Tgt Ion: 41 Resp: 2813
 Ion Ratio Lower Upper
 41 100
 69 0.0 64.4 96.6#
 39 0.0 43.5 65.3#


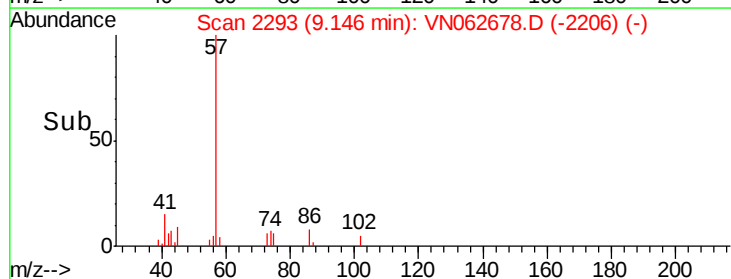
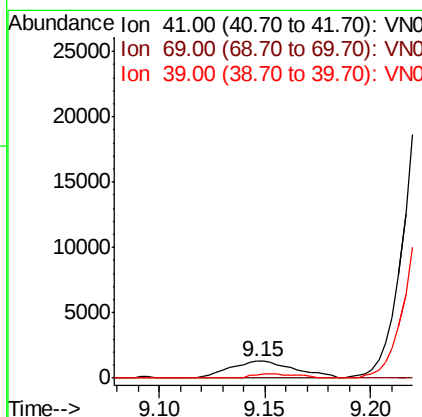





#50
Toluene-d8
Concen: 51.564 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. -0.00 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16




Instrument :
MSVOA_N
ClientSampleId :
PB130640ZHE#01


Tot Ion: 98 Resp: 318119
Ion Ratio Lower Upper
98 100
100 64.1 50.9 76.3

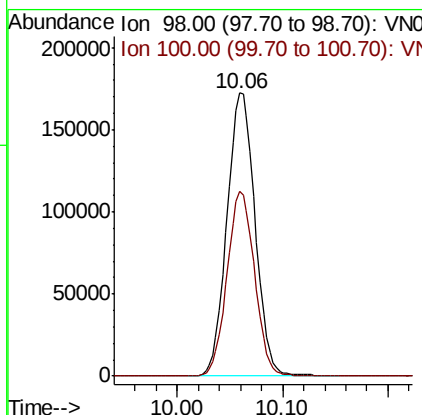

#51
4-Methyl-2-Pentanone
Concen: 2.372 ug/l
RT: 9.95 min Scan# 2544
Delta R.T. -0.00 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16

Tgt Ion: 43 Resp: 6187
Ion Ratio Lower Upper
43 100
58 31.6 29.8 44.6

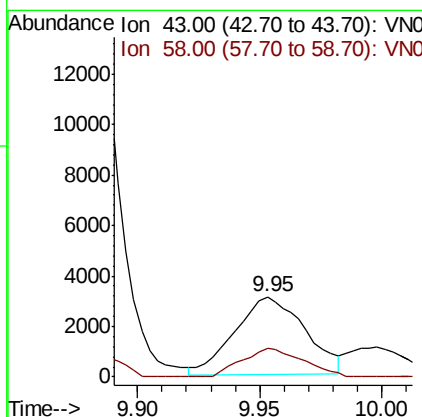

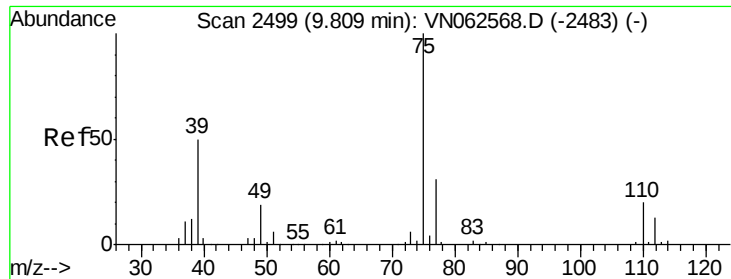


#54




cis-1,3-Dichloropropene
 Concen: 6.266 ug/l
 RT: 9.87 min Scan# 2519
 Delta R.T. 0.06 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130640ZHE#01

Tot Ion: 75 Resp: 19990
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.0 37.6#
 39 33.9 39.8 59.8#




Abundance Ion 74.90 (74.60 to 75.60): VNO
 Ion 76.90 (76.60 to 77.60): VNO
 Ion 39.00 (38.70 to 39.70): VNO

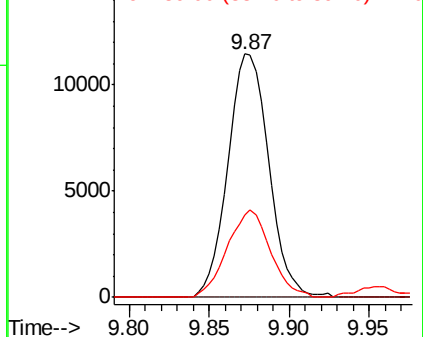



#56


Ethyl methacrylate
 Concen: 2.046 ug/l
 RT: 10.52 min Scan# 2720
 Delta R.T. 0.12 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Tgt Ion: 69 Resp: 882
 Ion Ratio Lower Upper
 69 100
 41 4772.2 57.2 85.8#
 39 1992.1 28.6 43.0#



Abundance Ion 69.00 (68.70 to 69.70): VNO
 Ion 41.00 (40.70 to 41.70): VNO
 Ion 39.00 (38.70 to 39.70): VNO

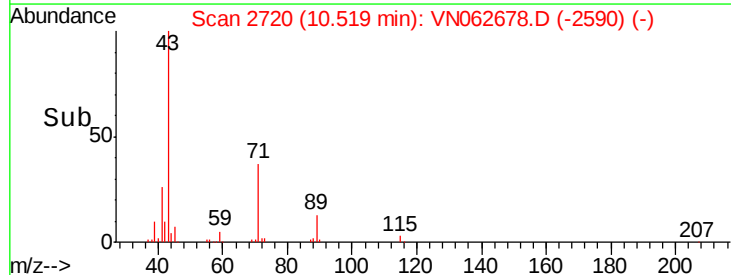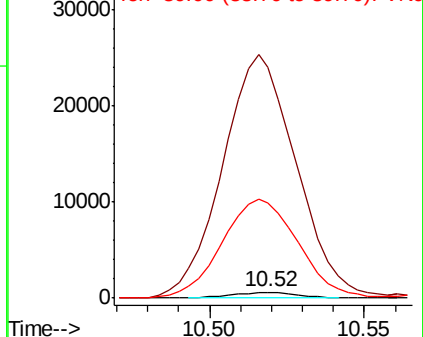



#57

1,3-Dichloropropane

Concen: 1.101 ug/l

RT: 10.74 min Scan# 2788

Delta R.T. 0.06 min

Lab File: VN062678.D

Acq: 31 Jul 2020 12:16

Instrument :

MSVOA_N

ClientSampleId :


PB130640ZHE#01

Tot Ion: 76 Resp: 3452

Ion Ratio Lower Upper

76 100

78 0.0 26.3 39.5#

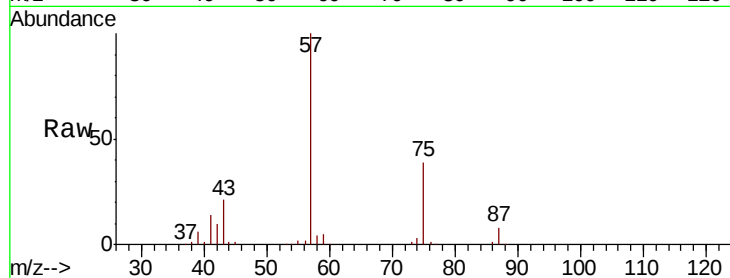

Abundance Ion 75.90 (75.60 to 76.60): VN062568.D (-2754) (-)

Ion 77.90 (77.60 to 78.60): VN062568.D (-2754) (-)

10.74

2500

2000

1500

1000



500

0

Time-->

10.70

10.75

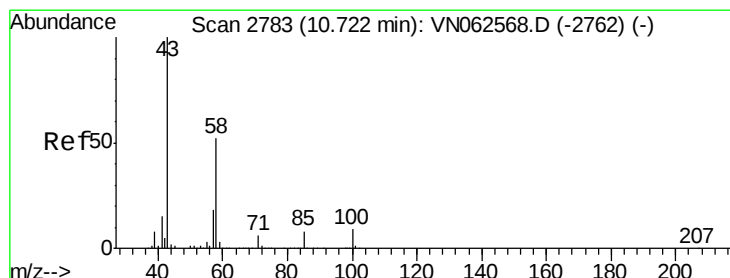

#59

2-Hexanone

Concen: 29.920 ug/l

RT: 10.74 min Scan# 2788

Delta R.T. 0.02 min

Lab File: VN062678.D


Acq: 31 Jul 2020 12:16

Tgt Ion: 43 Resp: 55048

Ion Ratio Lower Upper

43 100

58 19.3 26.0 78.0#

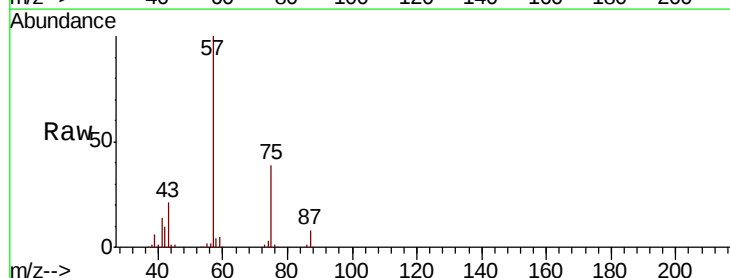

Abundance Ion 43.00 (42.70 to 43.70): VN062568.D (-2762) (-)

Ion 58.00 (57.70 to 58.70): VN062568.D (-2762) (-)

40000

30000

20000

10000


0


Time-->

10.70

10.75

10.80









#62
4-Bromofluorobenzene
Concen: 50.622 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. -0.00 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16

Instrument :
MSVOA_N
ClientSampleId :
PB130640ZHE#01

Tot Ion: 95 Resp: 114191
Ion Ratio Lower Upper
95 100
174 73.1 0.0 144.6
176 69.8 0.0 139.4

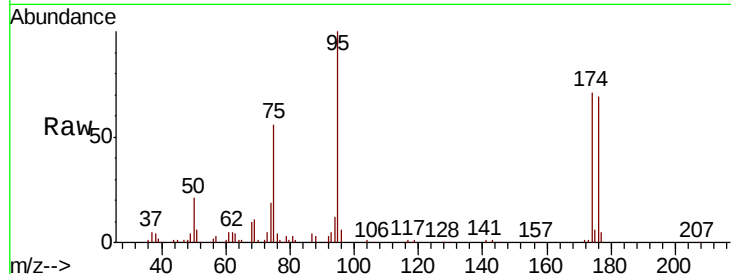


Abundance Ion 94.90 (94.60 to 95.60): VN062678.D (-3205) (-)
Ion 173.80 (173.50 to 174.50): VN062678.D (-3205) (-)
Ion 175.80 (175.50 to 176.50): VN062678.D (-3205) (-)


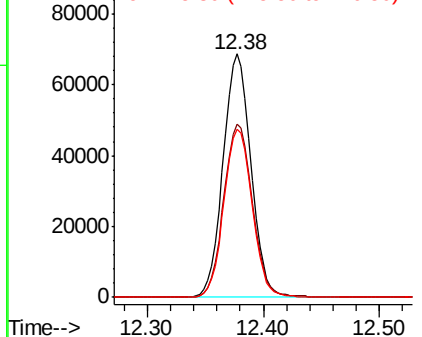



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. -0.00 min
Lab File: VN062678.D
Acq: 31 Jul 2020 12:16

Tgt Ion: 117 Resp: 241387
Ion Ratio Lower Upper
117 100
82 62.6 49.0 73.6
119 32.5 25.4 38.2



Abundance Ion 116.90 (116.60 to 117.60): VN062678.D (-2895) (-)
Ion 82.00 (81.70 to 82.70): VN062678.D (-2895) (-)
Ion 118.90 (118.60 to 119.60): VN062678.D (-2895) (-)

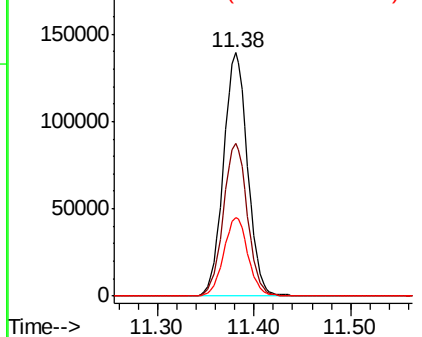



#71

Bromoform

Concen: 0.428 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.28 min

Lab File: VN062678.D

Acq: 31 Jul 2020 12:16

Instrument :

MSVOA_N

ClientSampleId :

PB130640ZHE#01


Tot Ion:173 Resp: 612

Ion Ratio Lower Upper

173 100

175 893.8 24.1 72.2#




254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

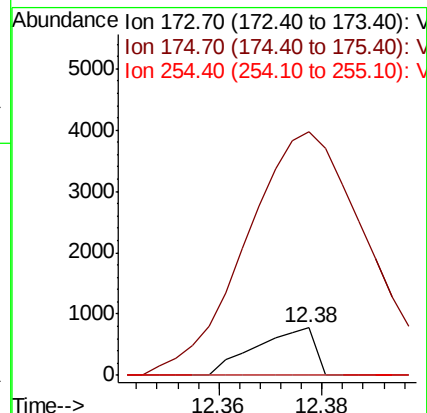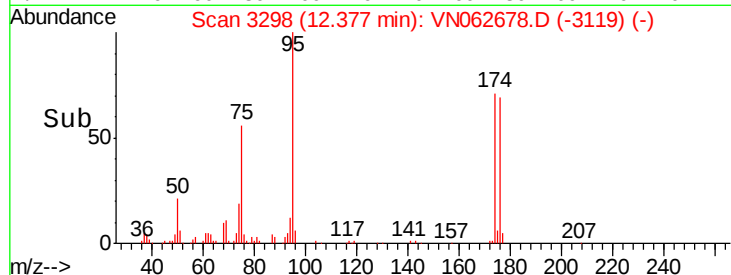

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN062678.D

Acq: 31 Jul 2020 12:16


Tgt Ion:152 Resp: 83254

Ion Ratio Lower Upper

152 100

115 64.0 31.8 95.4



150 158.7 0.0 351.4




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

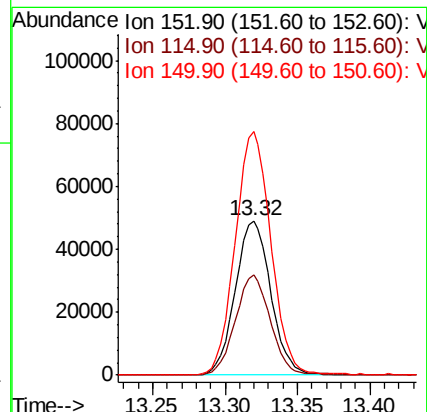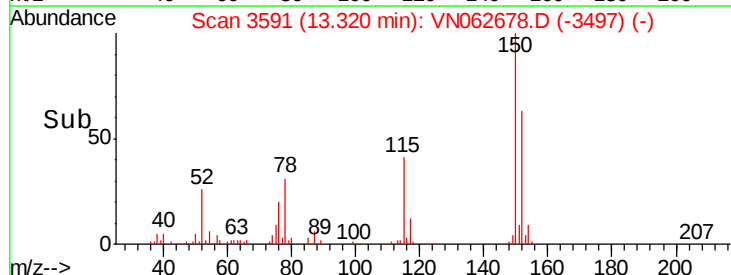

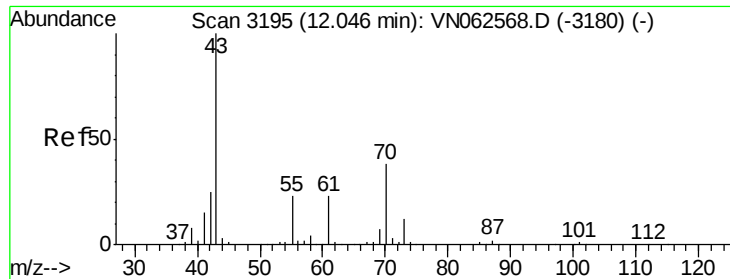

#74

N-amvl acetate

Concen: 0.767 ug/l

RT: 12.01 min Scan# 3185

Delta R.T. -0.03 min

Lab File: VN062678.D

Acq: 31 Jul 2020 12:16

Instrument :

MSVOA_N

ClientSampleId :

PB130640ZHE#01

Tot Ion: 43 Resp: 2255


Ion Ratio Lower Upper

43 100

70 0.0 30.5 45.7#

55 3.0 19.0 28.6#

61 0.0 18.4 27.6#



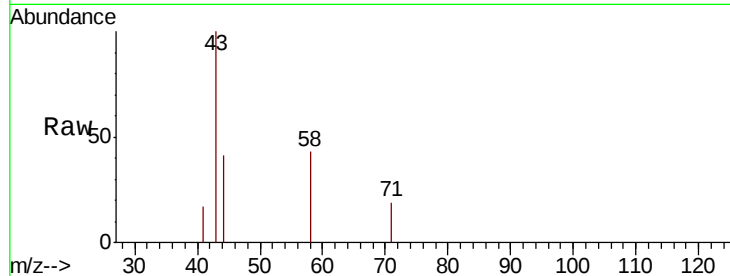


Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

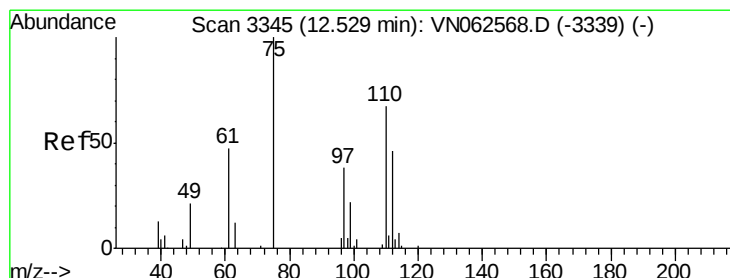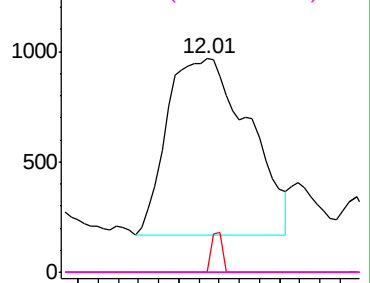

#76

1,2,3-Trichloropropane

Concen: 30.084 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.15 min

Lab File: VN062678.D


Acq: 31 Jul 2020 12:16

Tgt Ion: 75 Resp: 63752

Ion Ratio Lower Upper



75 100


77 0.8 0.0 0.0#

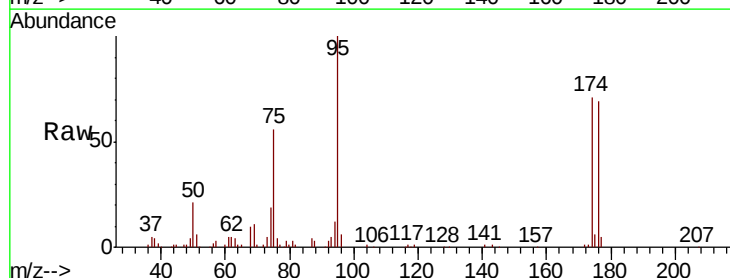

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0




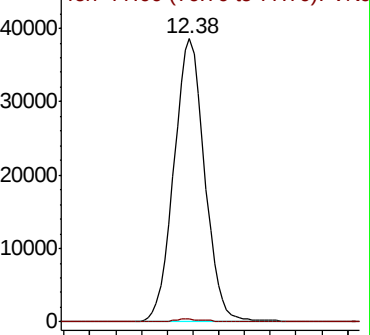


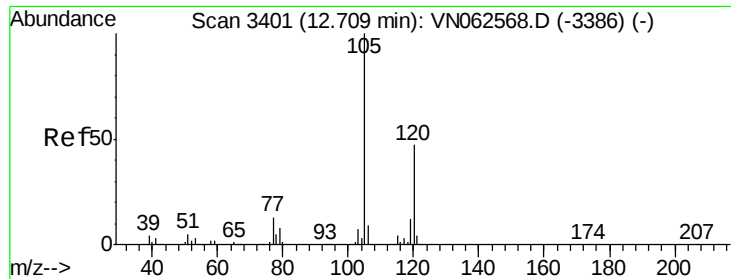

#80
 1,3,5-Trimethylbenzene
 Concen: 0.384 ug/l
 RT: 12.71 min Scan# 3401
 Delta R.T. -0.00 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130640ZHE#01


Tot Ion:105 Resp: 2098
 Ion Ratio Lower Upper
 105 100
 120 38.8 23.2 69.6

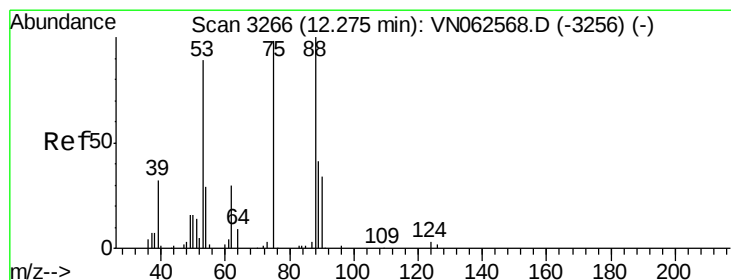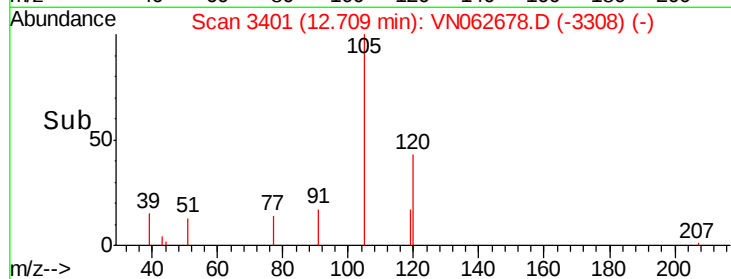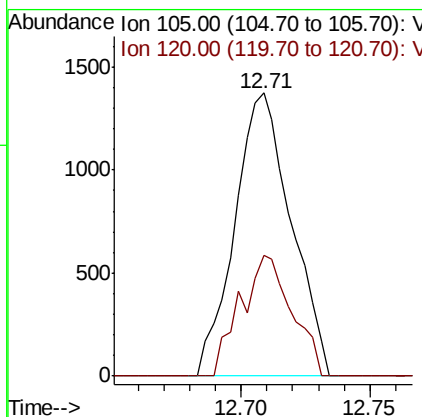

#81
 trans-1,4-Dichloro-2-butene
 Concen: 83.748 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. 0.10 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Tgt Ion: 75 Resp: 63752
 Ion Ratio Lower Upper
 75 100
 53 0.0 75.4 113.0#
 89 0.0 34.5 51.7#



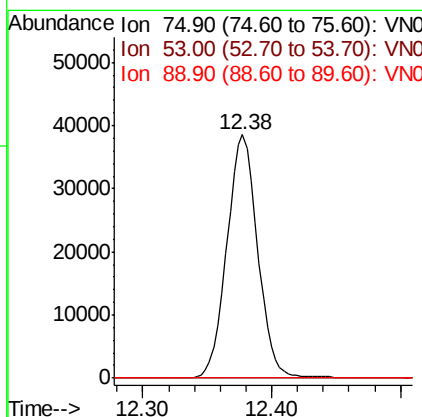





#93
 1,2,4-Trichlorobenzene
 Concen: 3.178 ug/l
 RT: 14.89 min Scan# 4080
 Delta R.T. 0.01 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130640ZHE#01

Tot Ion:180 Resp: 111
 Ion Ratio Lower Upper
 180 100
 182 26.1 47.8 143.3#
 145 0.0 15.3 45.9#

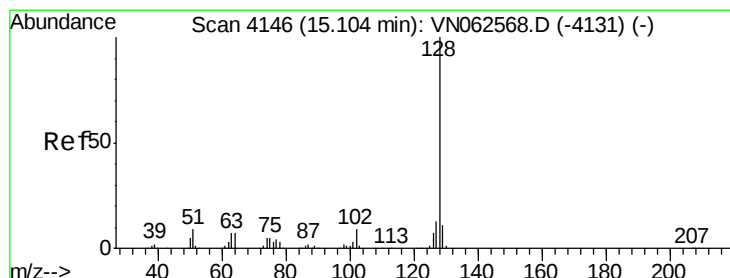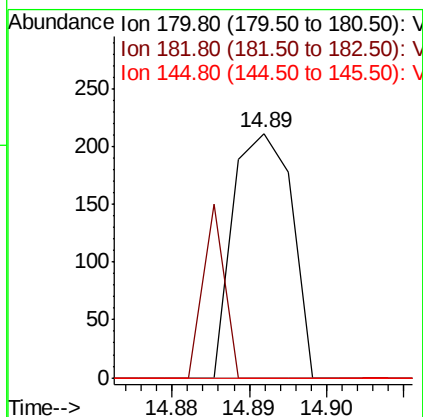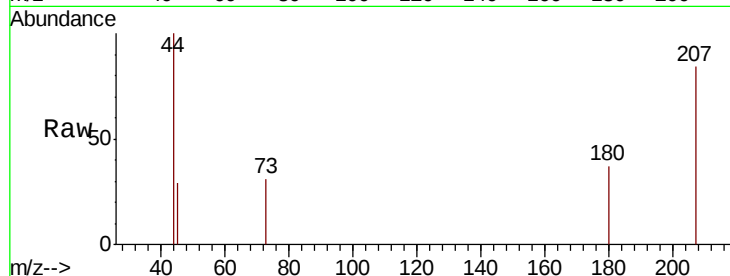

#95
 Naphthalene
 Concen: 4.044 ug/l
 RT: 15.12 min Scan# 4150
 Delta R.T. 0.01 min
 Lab File: VN062678.D
 Acq: 31 Jul 2020 12:16

Tgt Ion:128 Resp: 1133
 Ion Ratio Lower Upper
 128 100
 127 0.0 10.4 15.6#
 129 0.0 8.7 13.1#

