


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN073120\
 Data File : VN062671.D
 Acq On : 31 Jul 2020 8:45
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072120W.M
 Title : SW846 8260
 Last Update : Tue Jul 21 18:48:59 2020

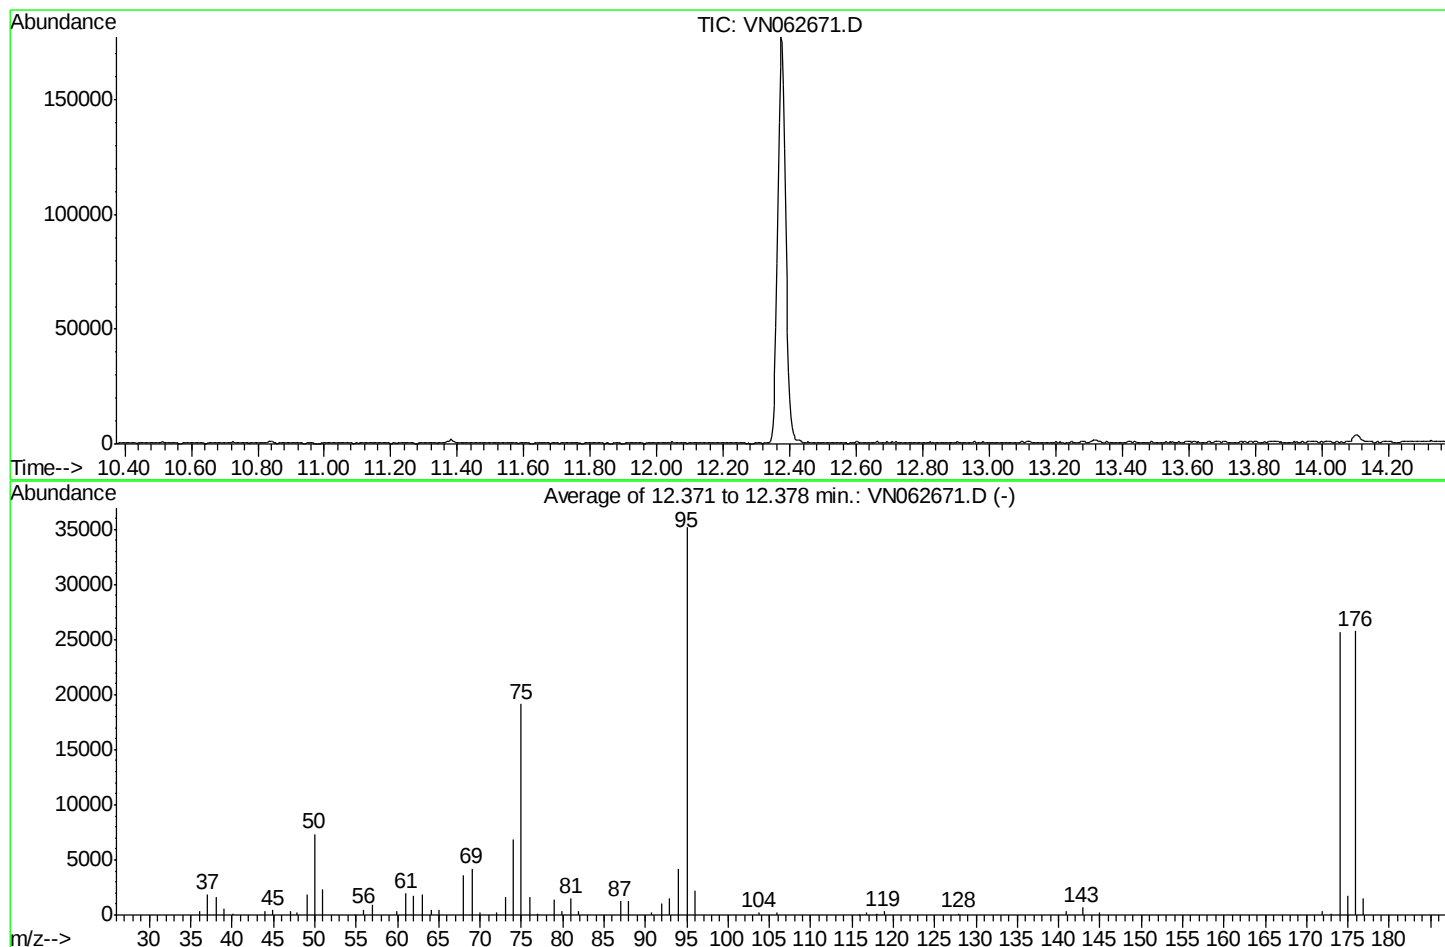

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	7321	PASS
75	95	30	60	54.4	19130	PASS
95	95	100	100	100.0	35168	PASS
96	95	5	9	6.4	2266	PASS
173	174	0.00	2	0.6	143	PASS
174	95	50	100	72.8	25613	PASS
175	174	5	9	7.0	1790	PASS
176	174	95	101	100.5	25730	PASS
177	176	5	9	5.8	1495	PASS