


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN073120\
Data File : VN062699.D
Acq On : 31 Jul 2020 21:09
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072120W.M
Title : SW846 8260
Last Update : Tue Jul 21 18:48:59 2020

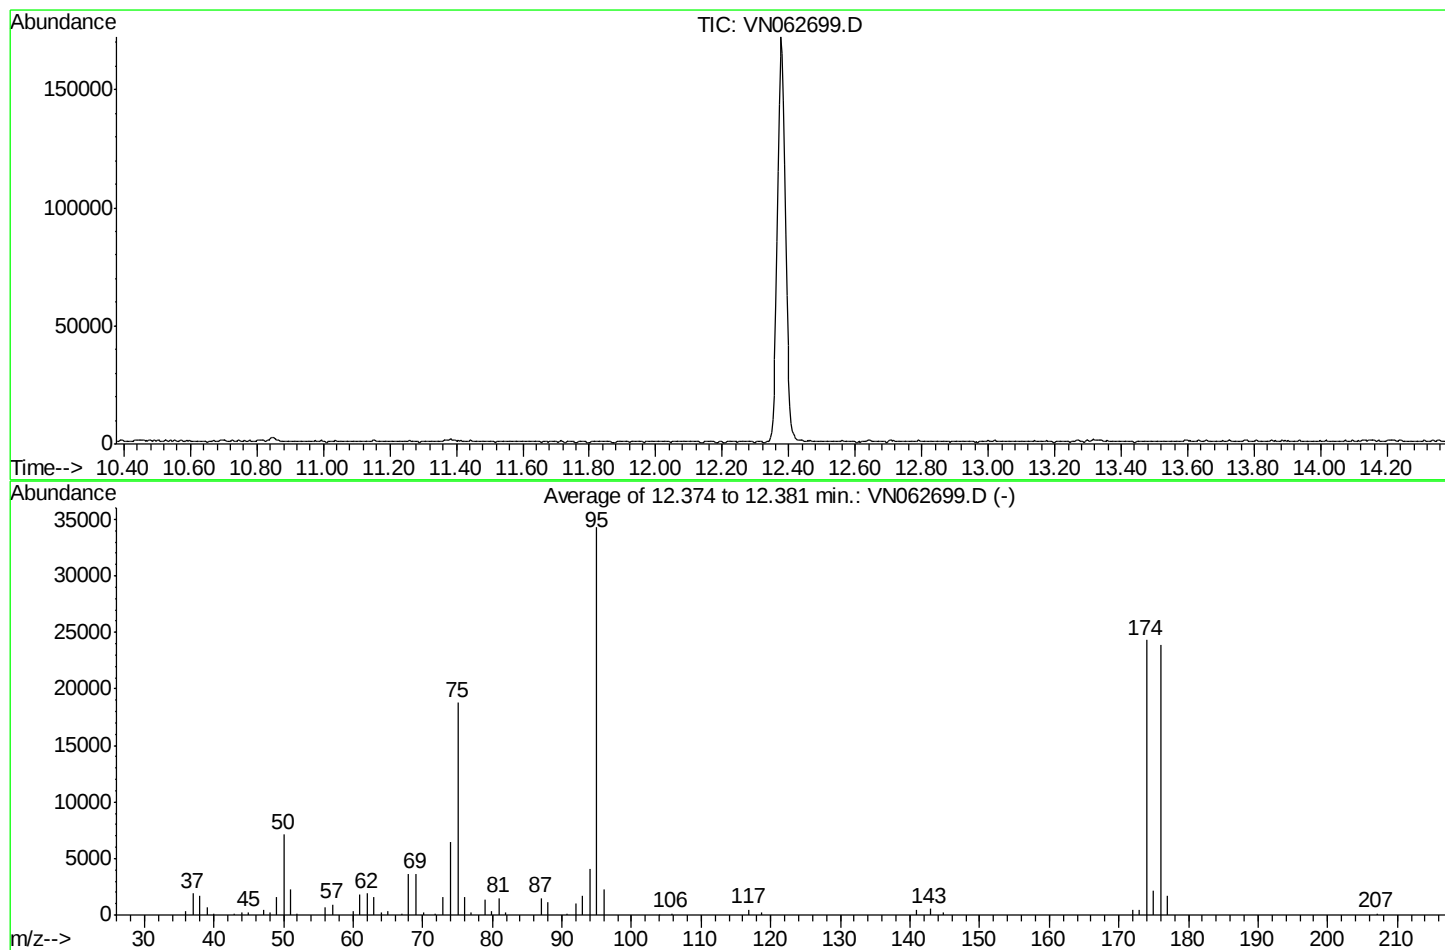

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	7125	PASS
75	95	30	60	54.8	18789	PASS
95	95	100	100	100.0	34293	PASS
96	95	5	9	6.7	2291	PASS
173	174	0.00	2	1.9	451	PASS
174	95	50	100	71.0	24336	PASS
175	174	5	9	8.7	2121	PASS
176	174	95	101	98.3	23917	PASS
177	176	5	9	7.1	1707	PASS