

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN073123\
 Data File : VN078706.D
 Acq On : 31 Jul 2023 15:35
 Operator : JC\MD
 Sample : 03813-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PLAUDERVILLE-1

Quant Time: Aug 01 01:18:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 10 16:13:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	677815	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	1222492	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	1113305	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	347705	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	440004	48.422	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	96.840%		
35) Dibromofluoromethane	8.171	113	416862	50.232	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	100.460%		
50) Toluene-d8	10.571	98	1549378	49.422	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	98.840%		
62) 4-Bromofluorobenzene	12.853	95	484234	50.146	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	100.300%		
Target Compounds						Qvalue
3) Chloromethane	2.371	50	2764	0.306	ug/l #	80
5) Bromomethane	2.971	94	3770	Below Cal	#	55
6) Chloroethane	3.106	64	942	Below Cal	#	43
11) Tert butyl alcohol	5.536	59	1025	0.732	ug/l #	72
13) Acrolein	4.200	56	562	0.408	ug/l #	51
16) Acetone	4.447	43	174870	61.780	ug/l	99
18) Methyl Acetate	5.036	43	4169	0.348	ug/l #	88
20) Methylene Chloride	5.283	84	44611	4.379	ug/l	93
25) 2-Butanone	7.500	43	94875	21.293	ug/l	93
29) Tetrahydrofuran	7.859	42	2940	1.006	ug/l #	77
31) Cyclohexane	8.229	56	13981	1.138	ug/l #	13
36) 1,1-Dichloropropene	8.229	75	53412	4.457	ug/l #	48
37) Ethyl Acetate	7.571	43	36485	3.653	ug/l	96
38) Carbon Tetrachloride	8.235	117	70845	5.440	ug/l #	15
43) Isopropyl Acetate	8.700	43	605163	36.798	ug/l #	80
48) Methyl methacrylate	9.671	41	15341	2.014	ug/l #	3
49) 1,4-Dioxane	9.700	88	349	2.100	ug/l #	30
51) 4-Methyl-2-Pentanone	10.453	43	422001	43.141	ug/l	92
54) cis-1,3-Dichloropropene	10.365	75	208294	15.037	ug/l #	63
57) 1,3-Dichloropropane	11.212	76	21761	1.476	ug/l #	44
59) 2-Hexanone	11.176	43	463638	66.690	ug/l #	19
74) N-amyl acetate	12.494	43	4340	0.385	ug/l #	48
75) 1,1,2,2-Tetrachloroethane	12.941	83	982	Below Cal	#	96
76) 1,2,3-Trichloropropane	12.853	75	238205	28.343	ug/l #	1
77) Bromobenzene	12.994	156	216	Below Cal	#	1
81) trans-1,4-Dichloro-2-b...	12.853	75	238205	74.479	ug/l #	15
90) Hexachloroethane	14.329	117	280	Below Cal	#	50
92) 1,2-Dibromo-3-Chloropr...	14.700	75	339	Below Cal	#	4
94) Hexachlorobutadiene	15.500	225	219	Below Cal	#	59
95) Naphthalene	15.647	128	2881	0.212	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN073123\
Data File : VN078706.D
Acq On : 31 Jul 2023 15:35
Operator : JC\MD
Sample : 03813-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1

Quant Time: Aug 01 01:18:52 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 10 16:13:53 2023
Response via : Initial Calibration

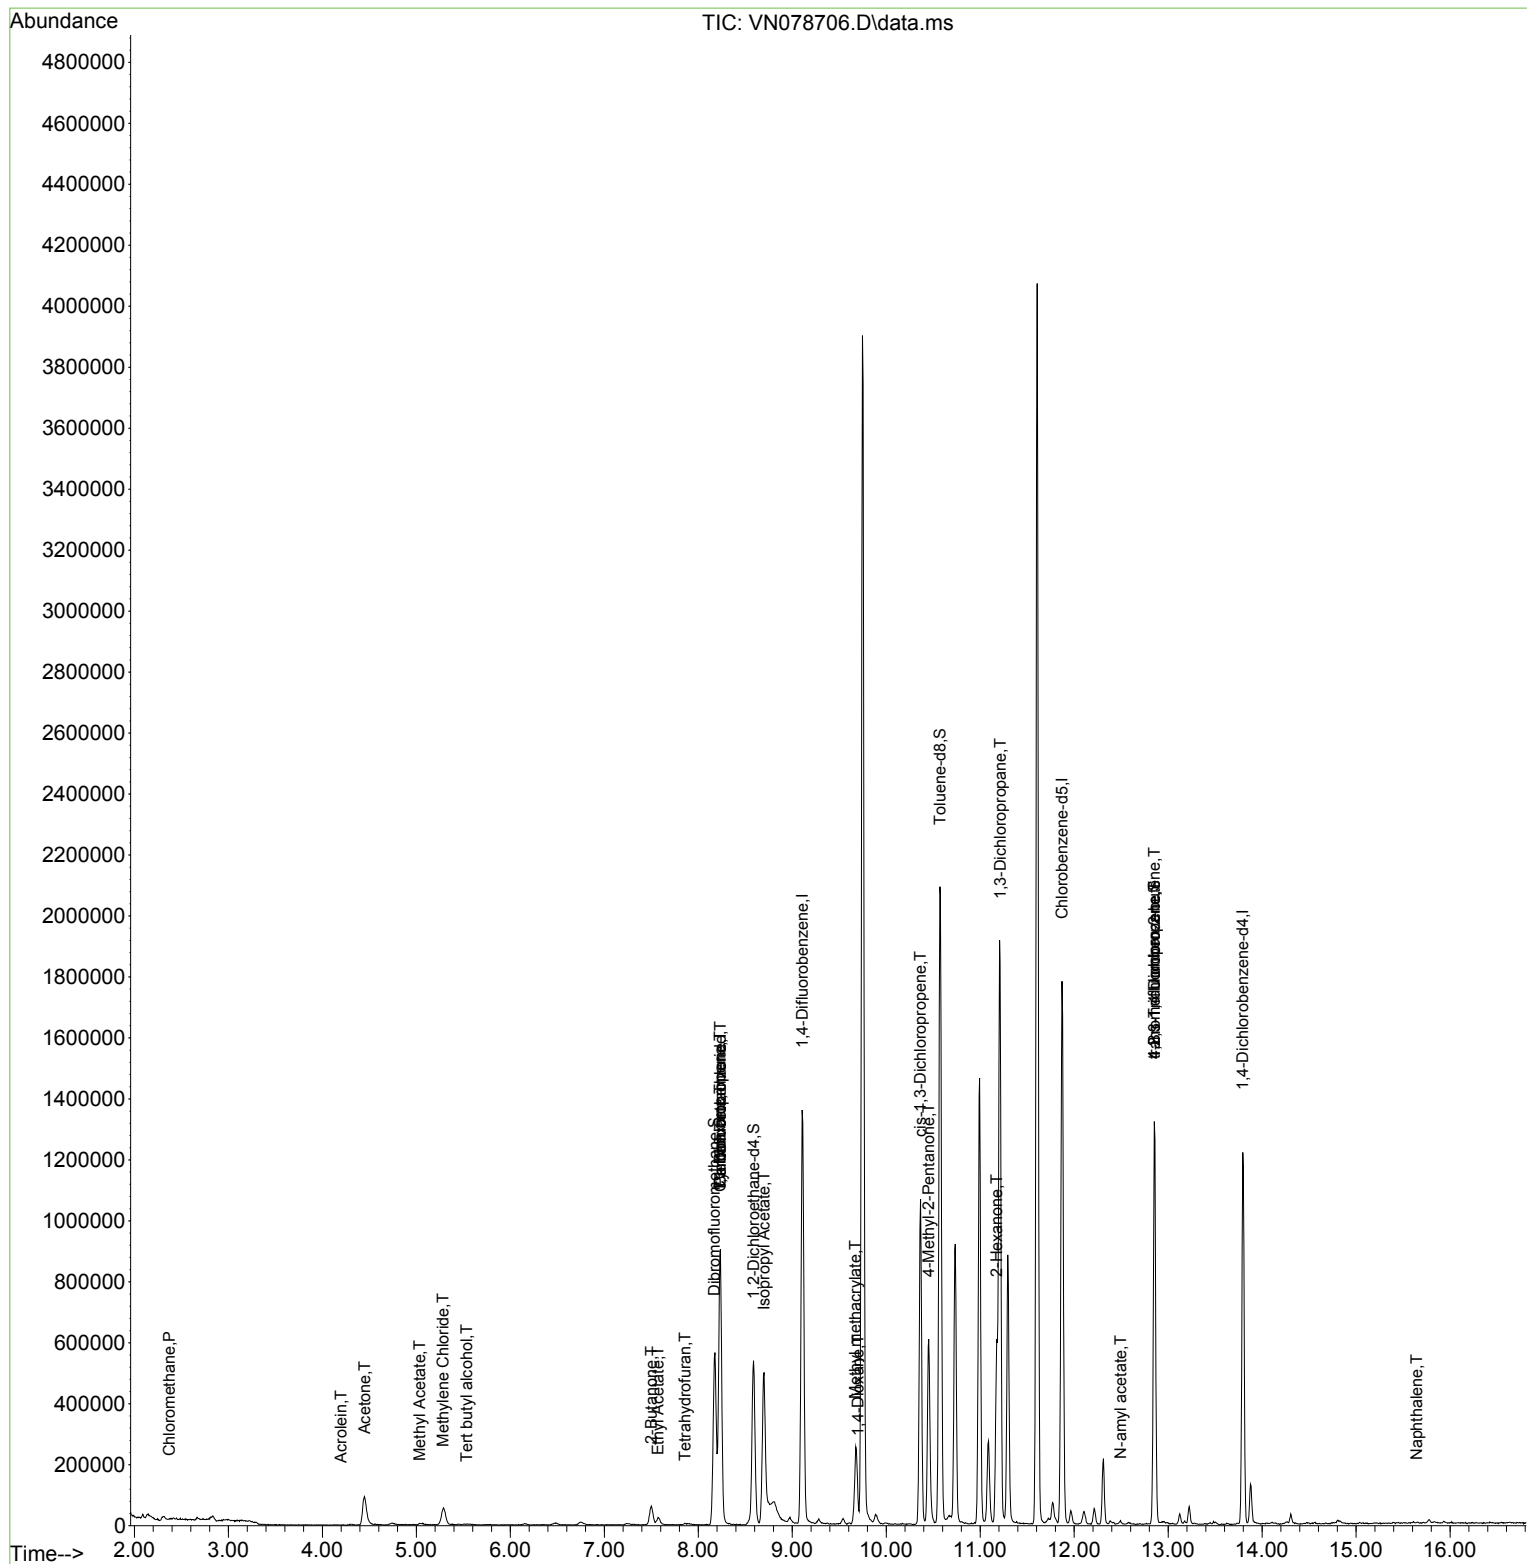



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. 0.005 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35

Instrument :

MSVOA_N

ClientSampleId :





PLAUDERVILLE-1

Tgt Ion:168 Resp: 677815

Ion Ratio Lower Upper

168 100

99 59.6 53.0 79.6

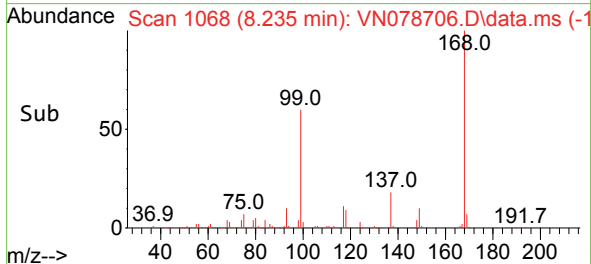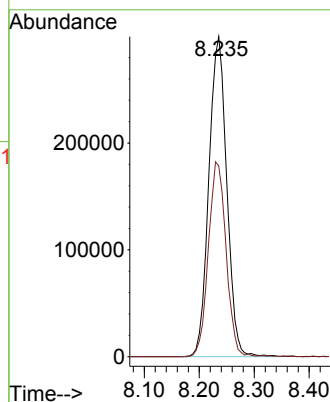

#3

Chloromethane

Concen: 0.306 ug/l

RT: 2.371 min Scan# 71

Delta R.T. 0.000 min

Lab File: VN078706.D




Acq: 31 Jul 2023 15:35


Tgt Ion: 50 Resp: 2764

Ion Ratio Lower Upper

50 100

52 21.6 26.5 39.7#


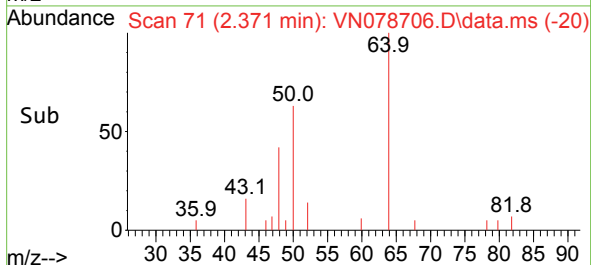
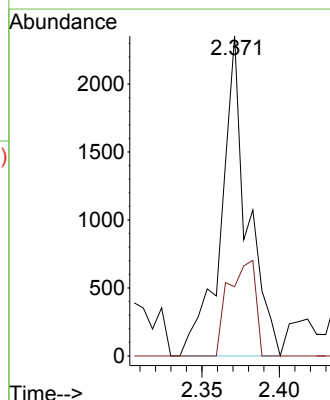





#5
Bromomethane
Concen: Below Cal
RT: 2.971 min Scan# 11
Delta R.T. 0.017 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion: 94 Resp: 3770
Ion Ratio Lower Upper
94 100
96 48.8 73.1 109.7#

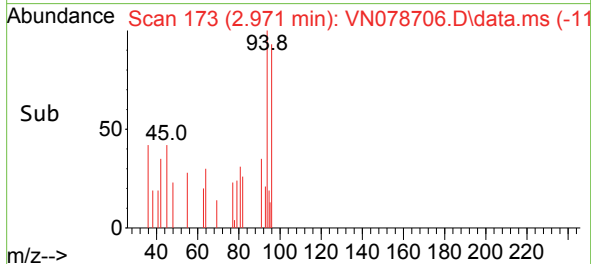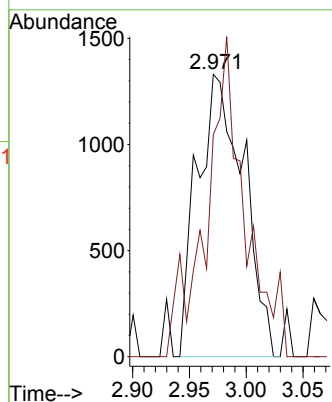

#6
Chloroethane
Concen: Below Cal
RT: 3.106 min Scan# 196
Delta R.T. -0.012 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion: 64 Resp: 942
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#



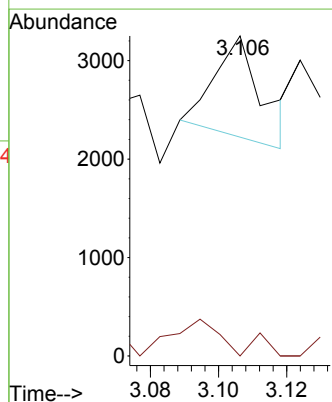





#11
Tert butyl alcohol
Concen: 0.732 ug/l
RT: 5.536 min Scan# 609
Delta R.T. -0.000 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion: 59 Resp: 1025
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

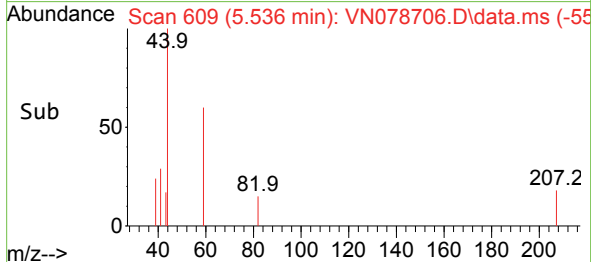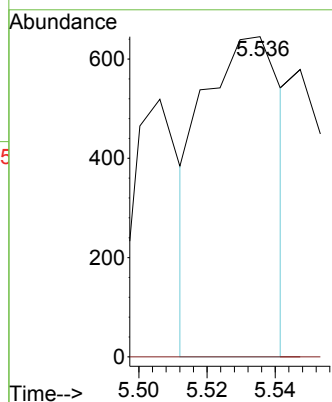

#13
Acrolein
Concen: 0.408 ug/l
RT: 4.200 min Scan# 382
Delta R.T. 0.011 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion: 56 Resp: 562
Ion Ratio Lower Upper
56 100
55 28.6 54.5 81.7#


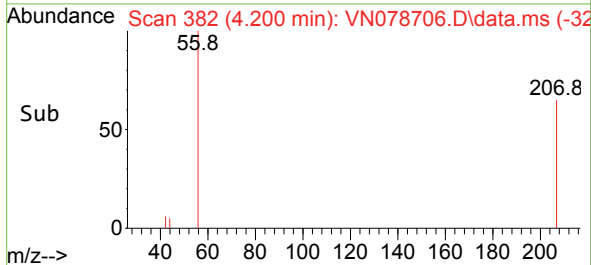
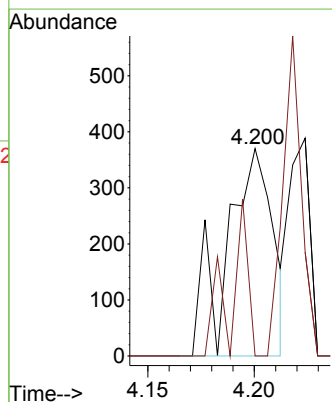





#16
Acetone
Concen: 61.780 ug/l
RT: 4.447 min Scan# 41
Delta R.T. 0.005 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion: 43 Resp: 174870
Ion Ratio Lower Upper
43 100
58 34.2 28.0 42.0

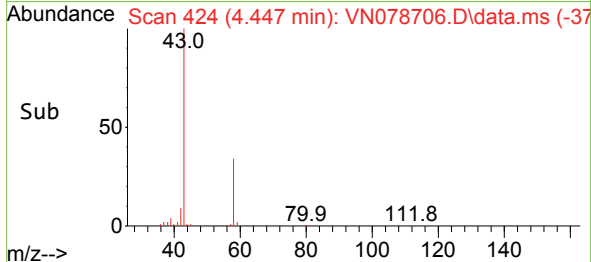

#18
Methyl Acetate
Concen: 0.348 ug/l
RT: 5.036 min Scan# 524
Delta R.T. -0.000 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion: 43 Resp: 4169
Ion Ratio Lower Upper
43 100
74 25.9 26.2 39.4#


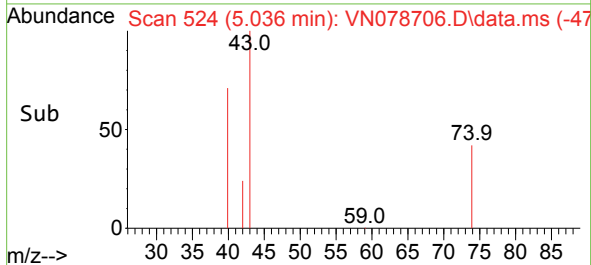






#20
Methylene Chloride
Concen: 4.379 ug/l
RT: 5.283 min Scan# 501
Delta R.T. -0.000 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion:	84	Resp:	44611
Ion	Ratio	Lower	Upper
84	100		
49	94.6	79.7	119.5
51	30.1	25.2	37.8
86	57.7	53.3	79.9

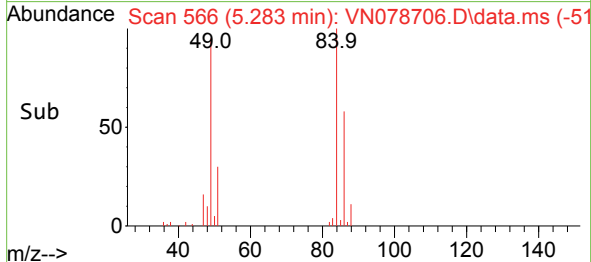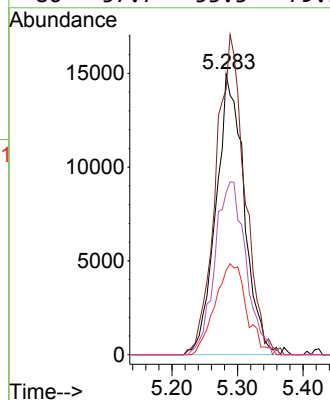

#25
2-Butanone
Concen: 21.293 ug/l
RT: 7.500 min Scan# 943
Delta R.T. 0.011 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion:	43	Resp:	94875
Ion	Ratio	Lower	Upper
43	100		
72	33.7	30.2	45.2

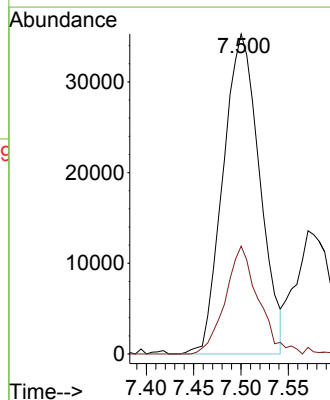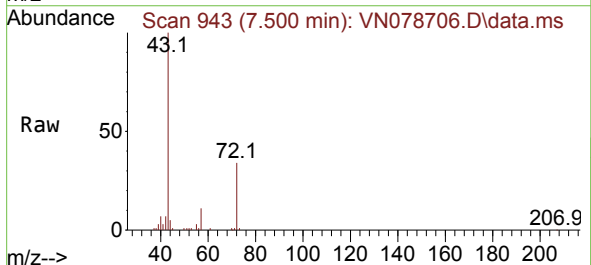



#29

Tetrahydrofuran

Concen: 1.006 ug/l

RT: 7.859 min Scan# 1004

Delta R.T. 0.012 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35

Instrument :

MSVOA_N

ClientSampleId :

PLAUDERVILLE-1





Tgt Ion: 42 Resp: 2940

Ion Ratio Lower Upper

42 100

72 43.8 49.8 74.6#

71 43.1 47.4 71.2#

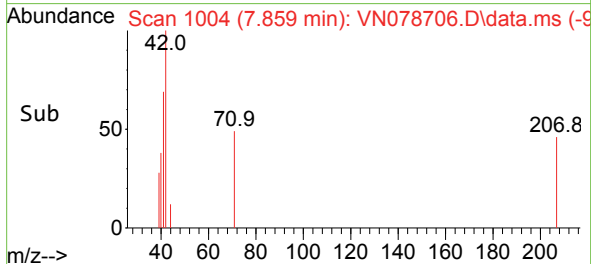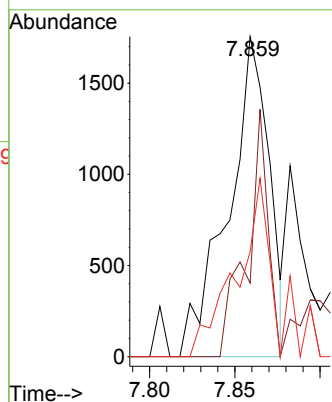

#31

Cyclohexane

Concen: 1.138 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.036 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35




Tgt Ion: 56 Resp: 13981


Ion Ratio Lower Upper

56 100

69 161.2 26.8 40.2#

84 144.1 81.8 122.6#

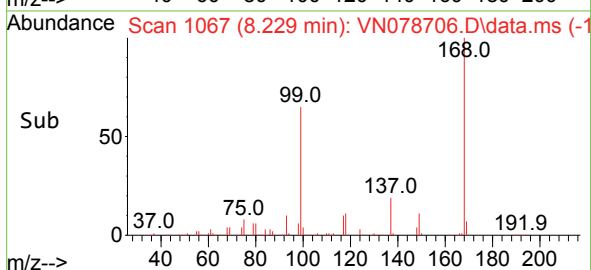



#33

1,2-Dichloroethane-d4

Concen: 48.422 ug/l

RT: 8.588 min Scan# 1127

Delta R.T. 0.005 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35

Instrument :

MSVOA_N

ClientSampleId :





PLAUDERVILLE-1

Tgt Ion: 65 Resp: 440004

Ion Ratio Lower Upper

65 100

67 55.2 0.0 106.6

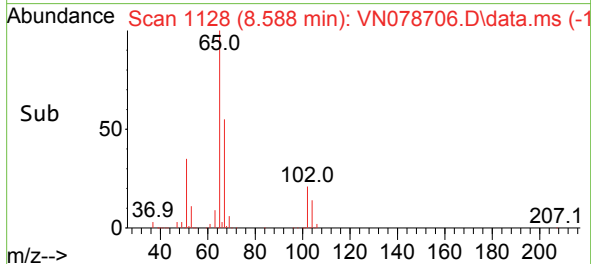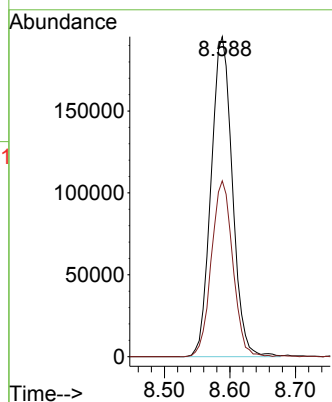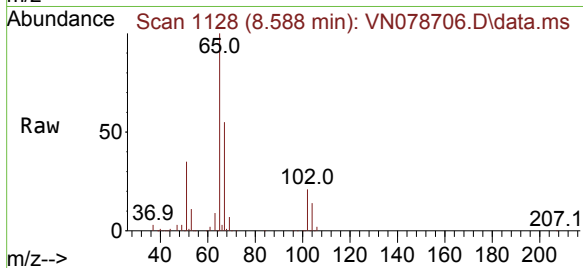

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.000 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35




Tgt Ion: 114 Resp: 1222492


Ion Ratio Lower Upper

114 100

63 20.0 0.0 36.4

88 16.1 0.0 30.6


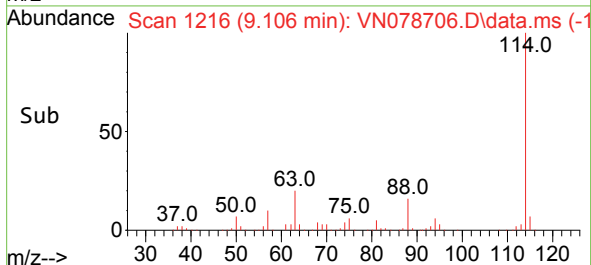

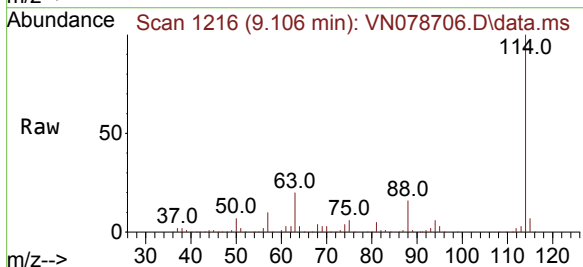




#35
Dibromofluoromethane
Concen: 50.232 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.006 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion:113 Resp: 416862
Ion Ratio Lower Upper
113 100
111 104.6 82.6 123.8
192 18.2 12.7 19.1

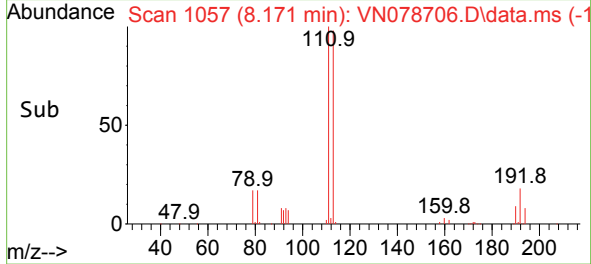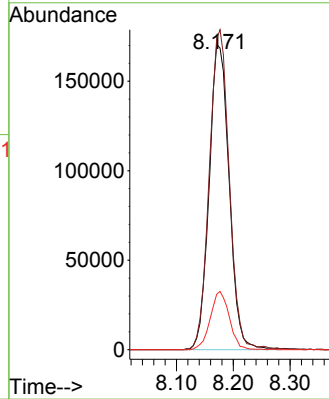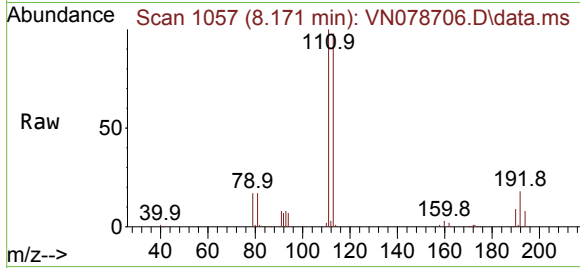

#36
1,1-Dichloropropene
Concen: 4.457 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.148 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion: 75 Resp: 53412
Ion Ratio Lower Upper
75 100
110 9.3 19.1 57.3#
77 0.0 25.0 37.4#


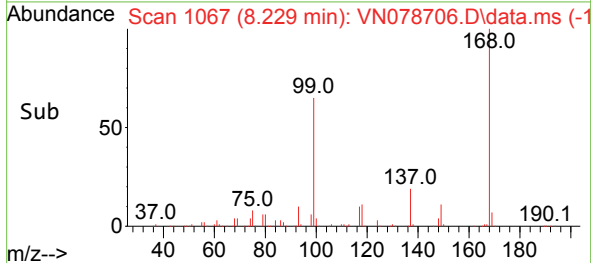
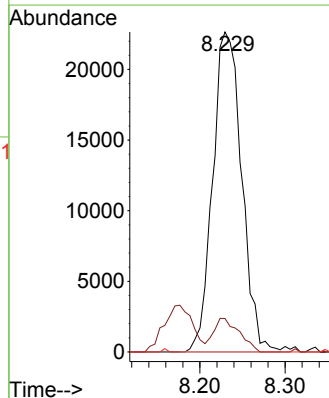
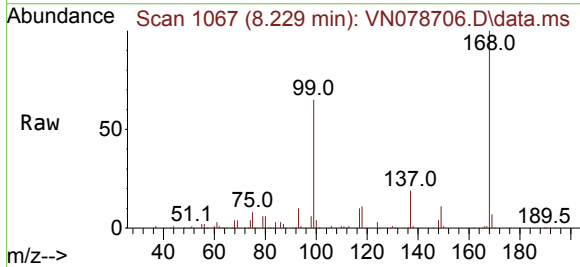




#37
Ethyl Acetate
Concen: 3.653 ug/l
RT: 7.571 min Scan# 91
Delta R.T. -0.000 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion: 43 Resp: 36485
Ion Ratio Lower Upper
43 100
61 14.8 13.2 19.8
70 12.6 11.3 16.9

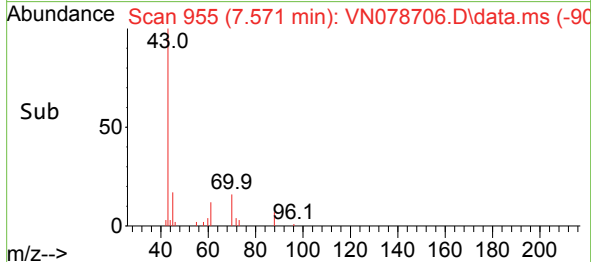

#38
Carbon Tetrachloride
Concen: 5.440 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.130 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion: 117 Resp: 70845
Ion Ratio Lower Upper
117 100
119 4.7 77.3 115.9#
121 0.0 23.3 34.9#




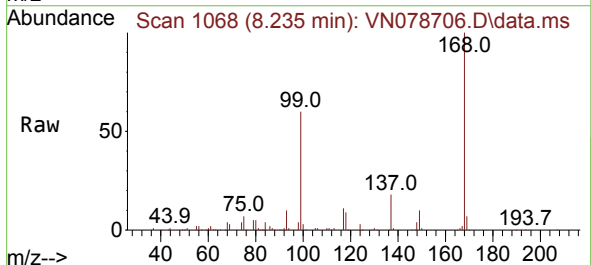




#43
Isopropyl Acetate
Concen: 36.798 ug/l
RT: 8.700 min Scan# 1146
Delta R.T. 0.006 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion: 43 Resp: 605163
Ion Ratio Lower Upper
43 100
61 17.9 24.7 37.1#
87 11.9 14.6 21.8#

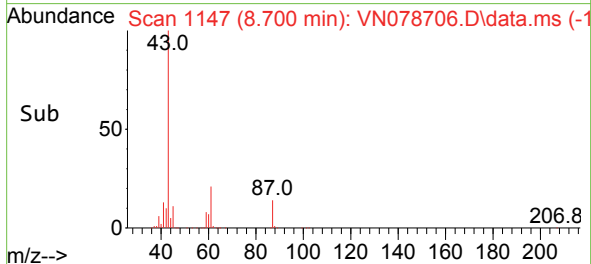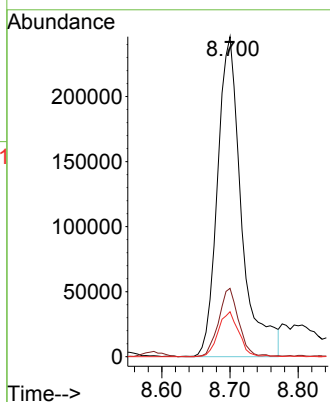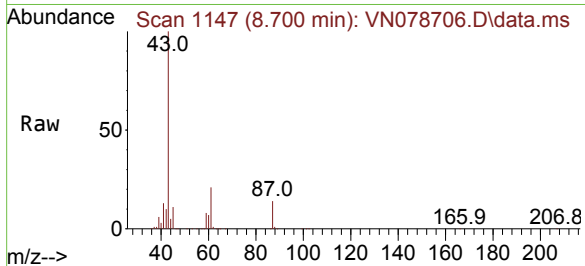

#48
Methyl methacrylate
Concen: 2.014 ug/l
RT: 9.671 min Scan# 1312
Delta R.T. -0.017 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion: 41 Resp: 15341
Ion Ratio Lower Upper
41 100
69 1.4 90.4 135.6#
39 0.0 54.6 81.8#

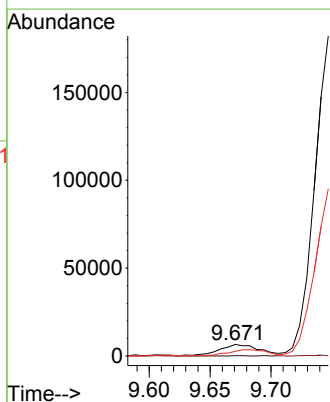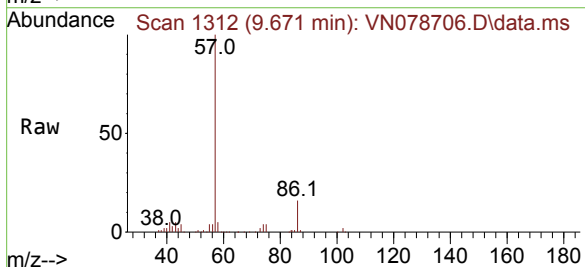



#49

1,4-Dioxane

Concen: 2.100 ug/l

RT: 9.700 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35

Instrument :

MSVOA_N

ClientSampleId :

PLAUDERVILLE-1





Tgt Ion: 88 Resp: 349

Ion Ratio Lower Upper

88 100

43 0.0 17.0 25.6#

58 0.0 47.0 70.4#

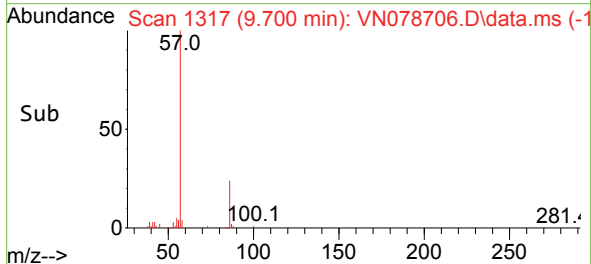

#50

Toluene-d8

Concen: 49.422 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. -0.000 min

Lab File: VN078706.D




Acq: 31 Jul 2023 15:35


Tgt Ion: 98 Resp: 1549378

Ion Ratio Lower Upper

98 100

100 63.7 52.0 78.0


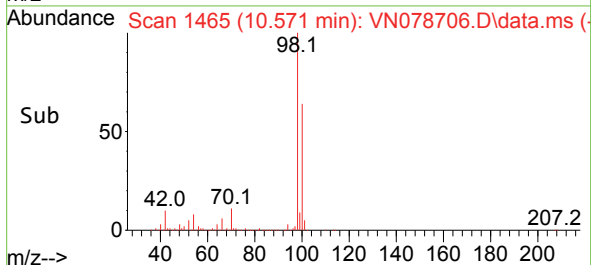
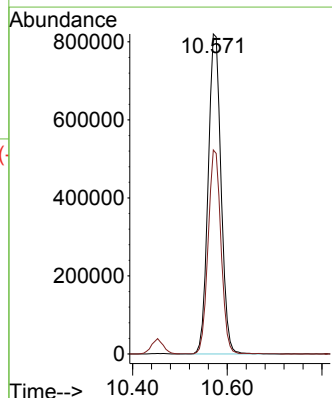
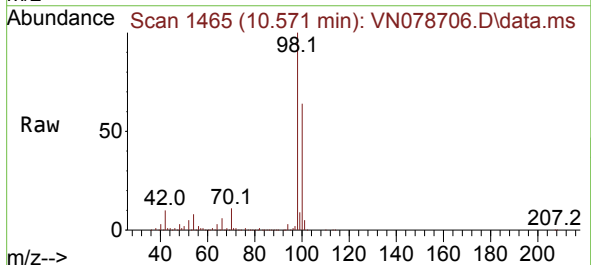




#51
4-Methyl-2-Pentanone
Concen: 43.141 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. -0.000 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion: 43 Resp: 422001
Ion Ratio Lower Upper
43 100
58 40.3 36.6 54.8

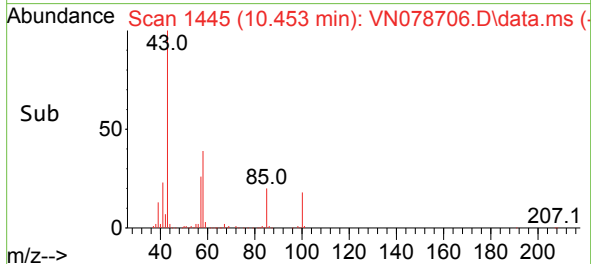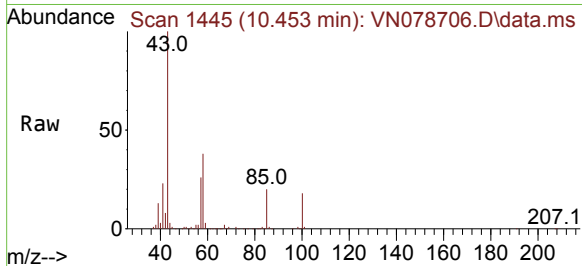

#54
cis-1,3-Dichloropropene
Concen: 15.037 ug/l
RT: 10.365 min Scan# 1430
Delta R.T. 0.047 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion: 75 Resp: 208294
Ion Ratio Lower Upper
75 100
77 0.9 26.1 39.1#
39 27.0 31.6 47.4#

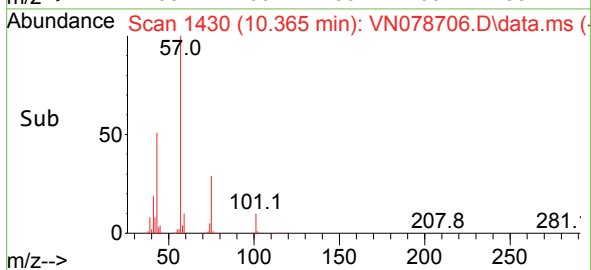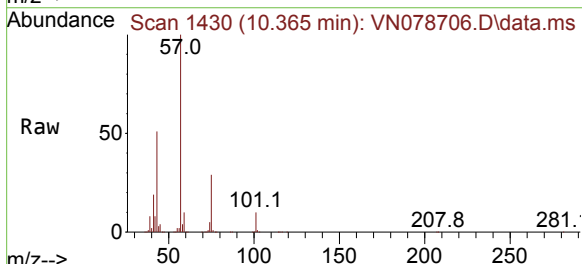



#57

1,3-Dichloropropane

Concen: 1.476 ug/l

RT: 11.212 min Scan# 1574

Delta R.T. 0.041 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35

Instrument :

MSVOA_N

ClientSampleId :





PLAUDERVILLE-1

Tgt Ion: 76 Resp: 21761

Ion Ratio Lower Upper

76 100

78 1.1 26.1 39.1#

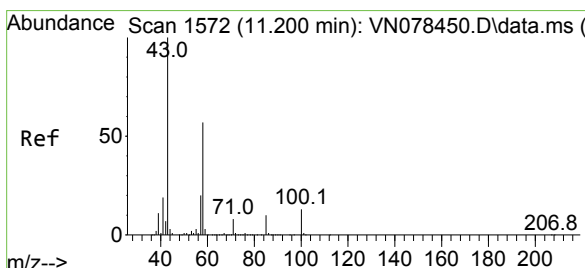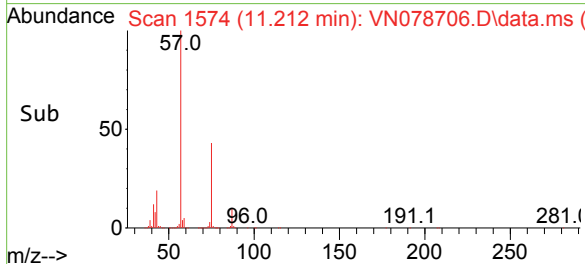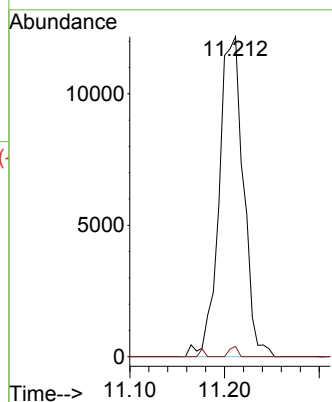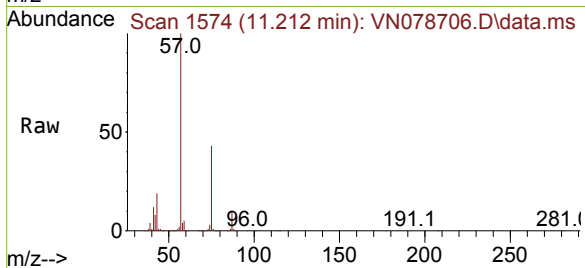

#59

2-Hexanone

Concen: 66.690 ug/l

RT: 11.176 min Scan# 1568

Delta R.T. -0.024 min

Lab File: VN078706.D




Acq: 31 Jul 2023 15:35


Tgt Ion: 43 Resp: 463638

Ion Ratio Lower Upper

43 100

58 0.0 31.7 95.1#


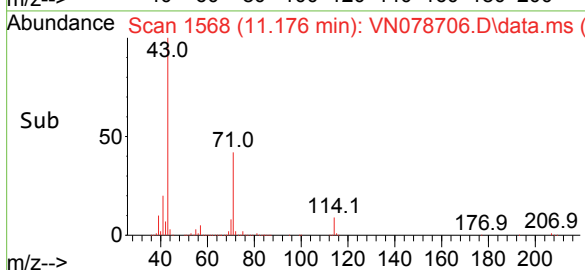

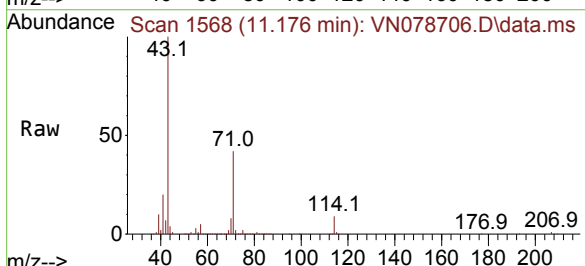


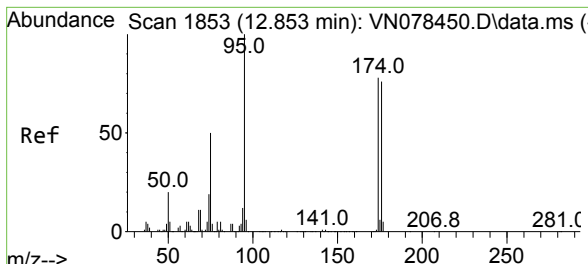

#62
 4-Bromofluorobenzene
 Concen: 50.146 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.000 min
 Lab File: VN078706.D
 Acq: 31 Jul 2023 15:35




Instrument :
 MSVOA_N
 ClientSampleId :
 PLAUDERVILLE-1


Tgt Ion:	95	Resp:	484234
Ion	Ratio	Lower	Upper
95	100		
174	75.6	0.0	143.8
176	71.5	0.0	135.8

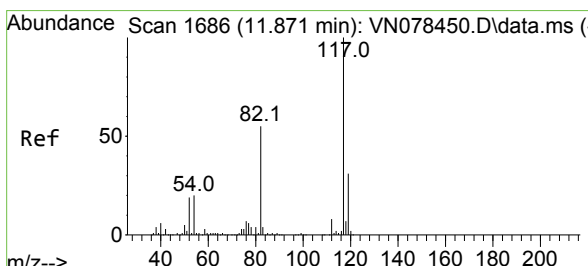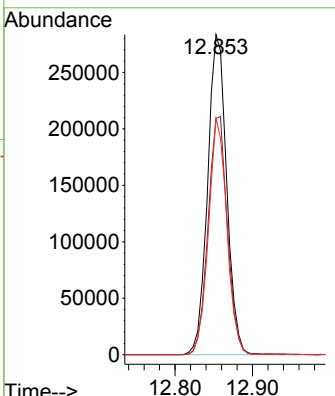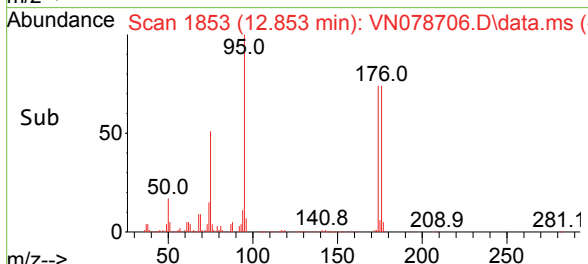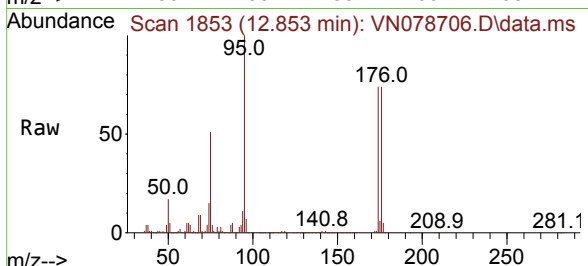

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 11.870 min Scan# 1686
 Delta R.T. -0.001 min
 Lab File: VN078706.D
 Acq: 31 Jul 2023 15:35

Tgt Ion:	117	Resp:	1113305
Ion	Ratio	Lower	Upper
117	100		
82	57.9	44.0	66.0
119	30.9	25.6	38.4


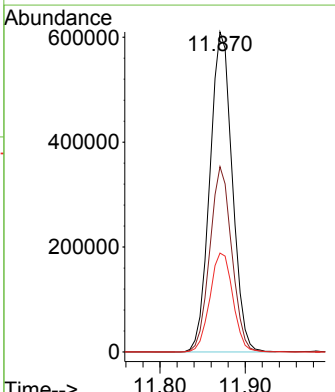
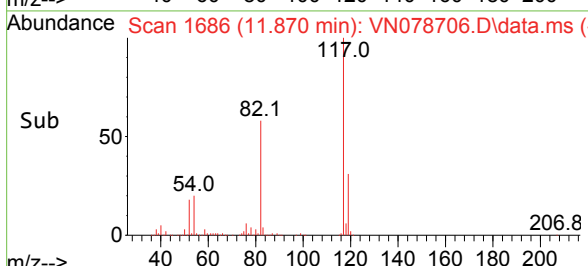
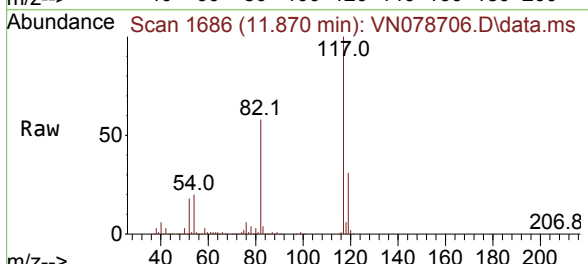


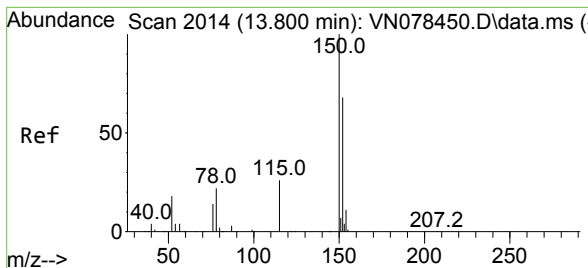

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 20
Delta R.T. -0.006 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion:152 Resp: 347705
Ion Ratio Lower Upper
152 100
115 60.9 32.3 96.8
150 156.9 0.0 355.8

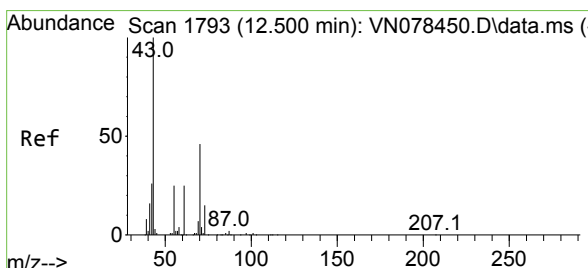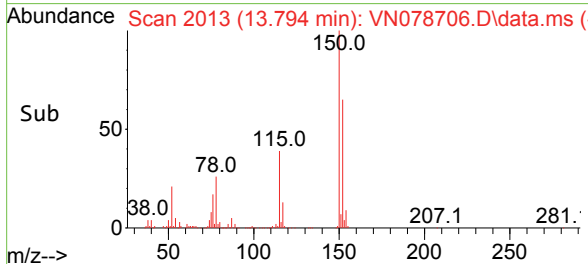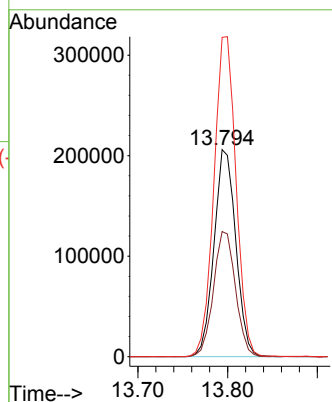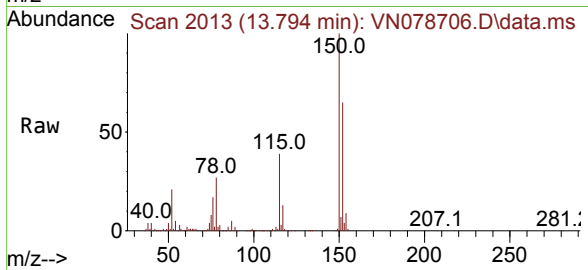

#74
N-ethyl acetate
Concen: 0.385 ug/l
RT: 12.494 min Scan# 1792
Delta R.T. -0.006 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion: 43 Resp: 4340
Ion Ratio Lower Upper
43 100
70 8.7 43.4 65.2#
55 13.0 21.4 32.0#
61 0.0 22.8 34.2#


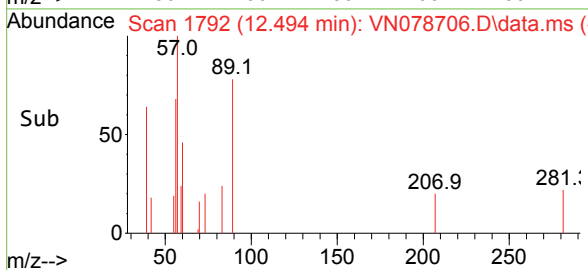

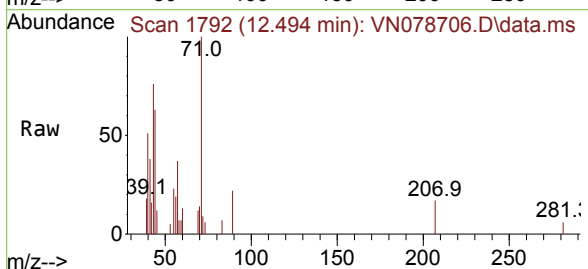




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.941 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1


Tgt Ion: 83 Resp: 982
Ion Ratio Lower Upper
83 100
131 0.0 5.0 15.0#
85 64.3 31.9 95.7

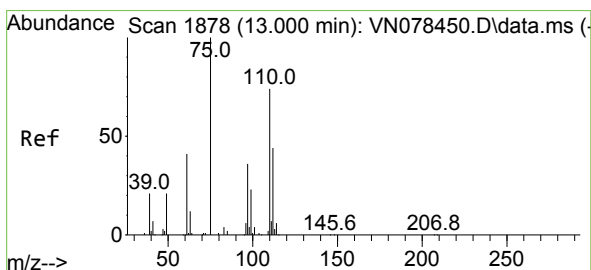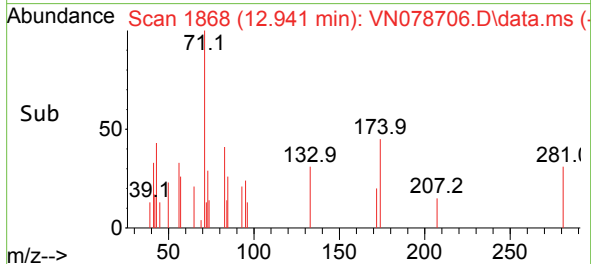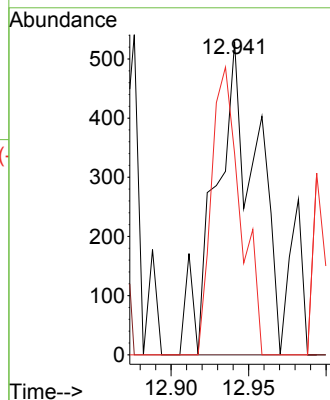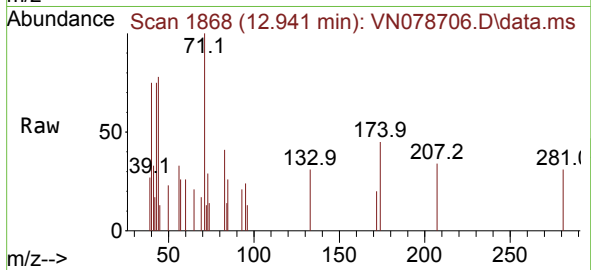

#76
1,2,3-Trichloropropane
Concen: 28.343 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion: 75 Resp: 238205
Ion Ratio Lower Upper
75 100
77 1.1 84.5 253.5#

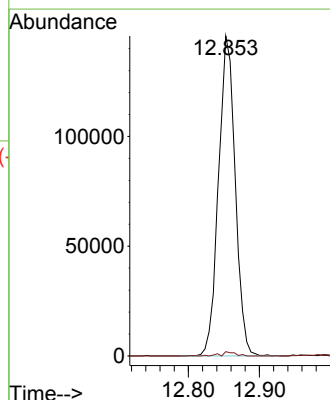

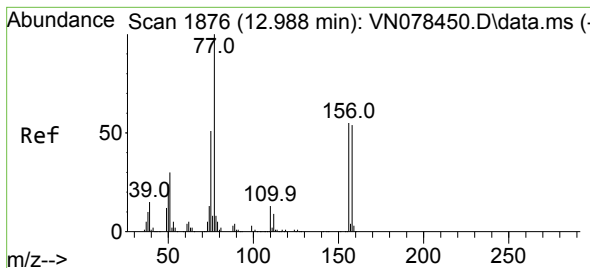

#77

Bromobenzene

Concen: Below Cal

RT: 12.994 min Scan# 1877

Delta R.T. 0.006 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35

Instrument :

MSVOA_N

ClientSampleId :

PLAUDERVILLE-1





Tgt Ion:156 Resp: 216

Ion Ratio Lower Upper

156 100

77 456.9 107.7 323.3#

158 233.8 48.4 145.3#

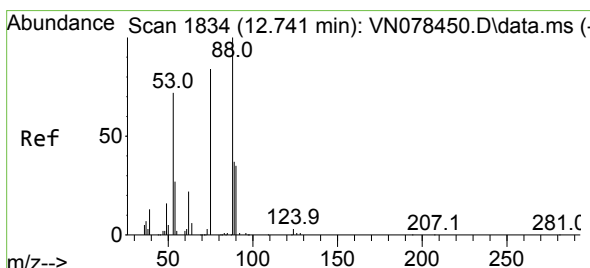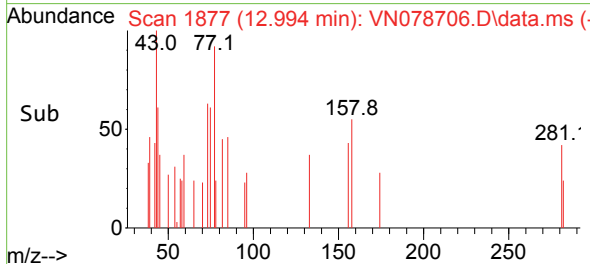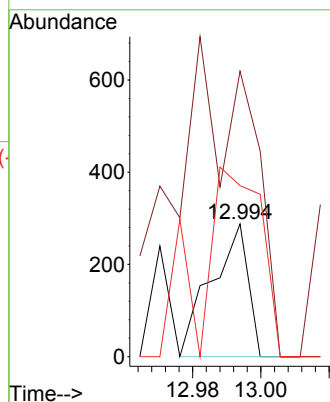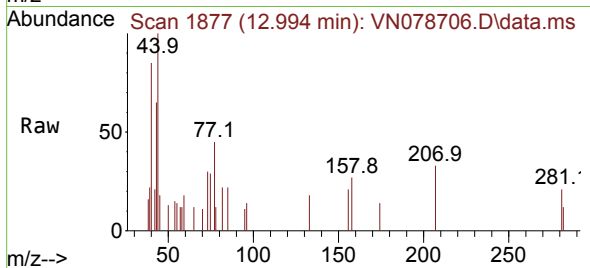

#81

trans-1,4-Dichloro-2-butene

Concen: 74.479 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35




Tgt Ion: 75 Resp: 238205


Ion Ratio Lower Upper

75 100

53 0.2 67.4 101.2#

89 0.0 38.8 58.2#

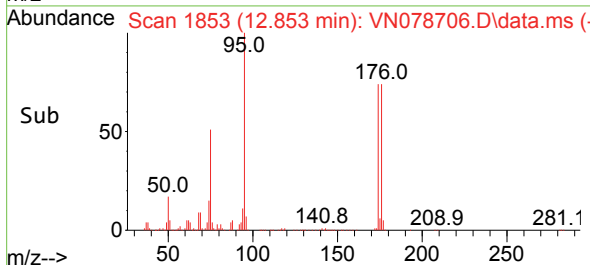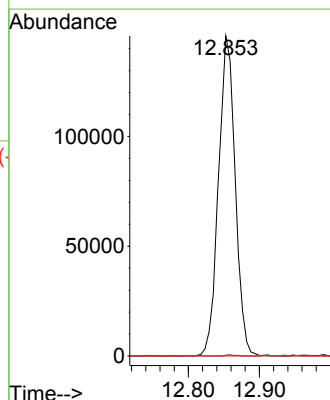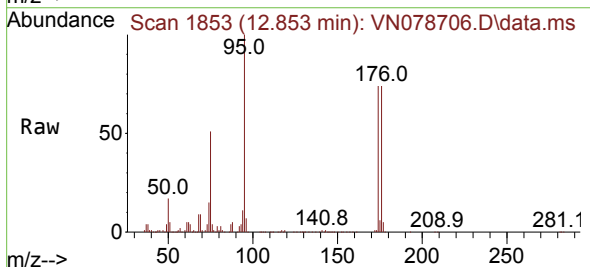



#90

Hexachloroethane

Concen: Below Cal

RT: 14.329 min Scan# 2105

Delta R.T. -0.006 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35

Instrument :

MSVOA_N

ClientSampleId :





PLAUDERVILLE-1

Tgt Ion:117 Resp: 280

Ion Ratio Lower Upper

117 100

201 21.1 29.3 88.0#

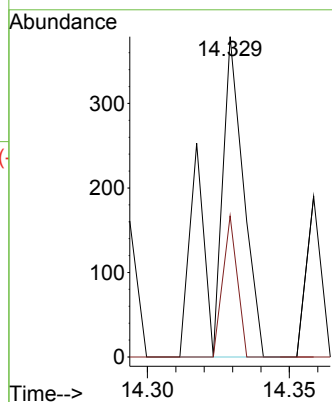

#92

1,2-Dibromo-3-Chloropropane

Concen: Below Cal

RT: 14.700 min Scan# 2167

Delta R.T. -0.023 min

Lab File: VN078706.D

Acq: 31 Jul 2023 15:35




Tgt Ion: 75 Resp: 339


Ion Ratio Lower Upper

75 100

155 0.0 39.1 117.2#

157 0.0 50.3 150.9#


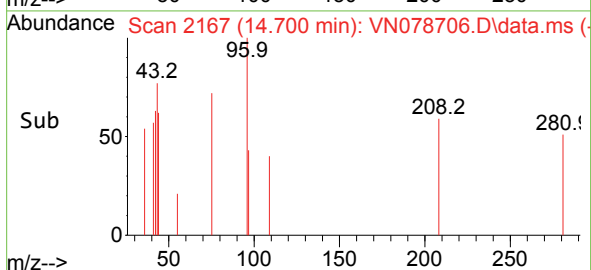






#94
Hexachlorobutadiene
Concen: Below Cal
RT: 15.500 min Scan# 219
Delta R.T. -0.006 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-1

Tgt Ion:225 Resp: 219
Ion Ratio Lower Upper
225 100
223 36.1 31.3 93.8
227 100.5 31.9 95.9#

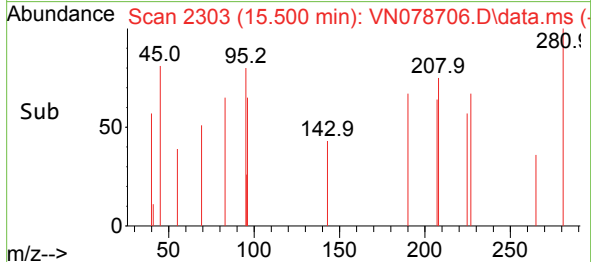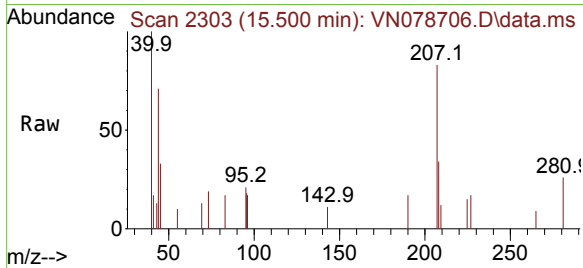

#95
Naphthalene
Concen: 0.212 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. -0.000 min
Lab File: VN078706.D
Acq: 31 Jul 2023 15:35

Tgt Ion:128 Resp: 2881
Ion Ratio Lower Upper
128 100
127 13.2 10.0 15.0
129 10.3 8.7 13.1

