

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN073123\
 Data File : VN078707.D
 Acq On : 31 Jul 2023 15:59
 Operator : JC\MD
 Sample : 03813-05
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PLAUDERVILLE-2

Quant Time: Aug 01 01:19:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 10 16:13:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	678448	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	1246656	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	1135431	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	389156	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	450387	49.519	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	99.040%		
35) Dibromofluoromethane	8.177	113	421488	49.805	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.620%		
50) Toluene-d8	10.576	98	1557517	48.719	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	97.440%		
62) 4-Bromofluorobenzene	12.853	95	512715	52.067	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	104.140%		
Target Compounds						Qvalue
3) Chloromethane	2.377	50	3230	0.357	ug/l	92
5) Bromomethane	2.959	94	1163	Below Cal	#	49
6) Chloroethane	3.095	64	775	Below Cal	#	43
11) Tert butyl alcohol	5.536	59	1663	1.186	ug/l #	72
13) Acrolein	4.183	56	484	0.351	ug/l #	42
16) Acetone	4.447	43	171039	60.370	ug/l	94
18) Methyl Acetate	5.047	43	5548	0.463	ug/l	89
20) Methylene Chloride	5.289	84	43802	4.272	ug/l	95
25) 2-Butanone	7.500	43	99974	22.417	ug/l	89
29) Tetrahydrofuran	7.865	42	3485	1.191	ug/l #	63
31) Cyclohexane	8.235	56	14015	1.140	ug/l #	1
36) 1,1-Dichloropropene	8.230	75	55736	4.561	ug/l #	48
37) Ethyl Acetate	7.577	43	35533	3.488	ug/l #	94
38) Carbon Tetrachloride	8.230	117	71347	5.372	ug/l #	17
42) 1,2-Dichloroethane	8.700	62	4699	0.382	ug/l	84
43) Isopropyl Acetate	8.700	43	681919	40.662	ug/l #	79
48) Methyl methacrylate	9.671	41	12911	1.662	ug/l #	33
49) 1,4-Dioxane	9.682	88	234	1.381	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	431953	43.303	ug/l	94
54) cis-1,3-Dichloropropene	10.365	75	223313	15.808	ug/l #	64
57) 1,3-Dichloropropane	11.206	76	25763	1.714	ug/l #	42
59) 2-Hexanone	11.176	43	491806	69.371	ug/l #	19
74) N-amyl acetate	12.494	43	5522	0.438	ug/l #	45
75) 1,1,2,2-Tetrachloroethane	12.935	83	694	Below Cal	#	82
76) 1,2,3-Trichloropropane	12.853	75	251850	26.774	ug/l #	1
77) Bromobenzene	12.988	156	417	Below Cal	#	50
81) trans-1,4-Dichloro-2-b...	12.853	75	251850	70.358	ug/l #	15
90) Hexachloroethane	14.335	117	328	Below Cal	#	21
92) 1,2-Dibromo-3-Chloropr...	14.723	75	263	Below Cal	#	4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN073123\
Data File : VN078707.D
Acq On : 31 Jul 2023 15:59
Operator : JC\MD
Sample : 03813-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2

Quant Time: Aug 01 01:19:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 10 16:13:53 2023
Response via : Initial Calibration




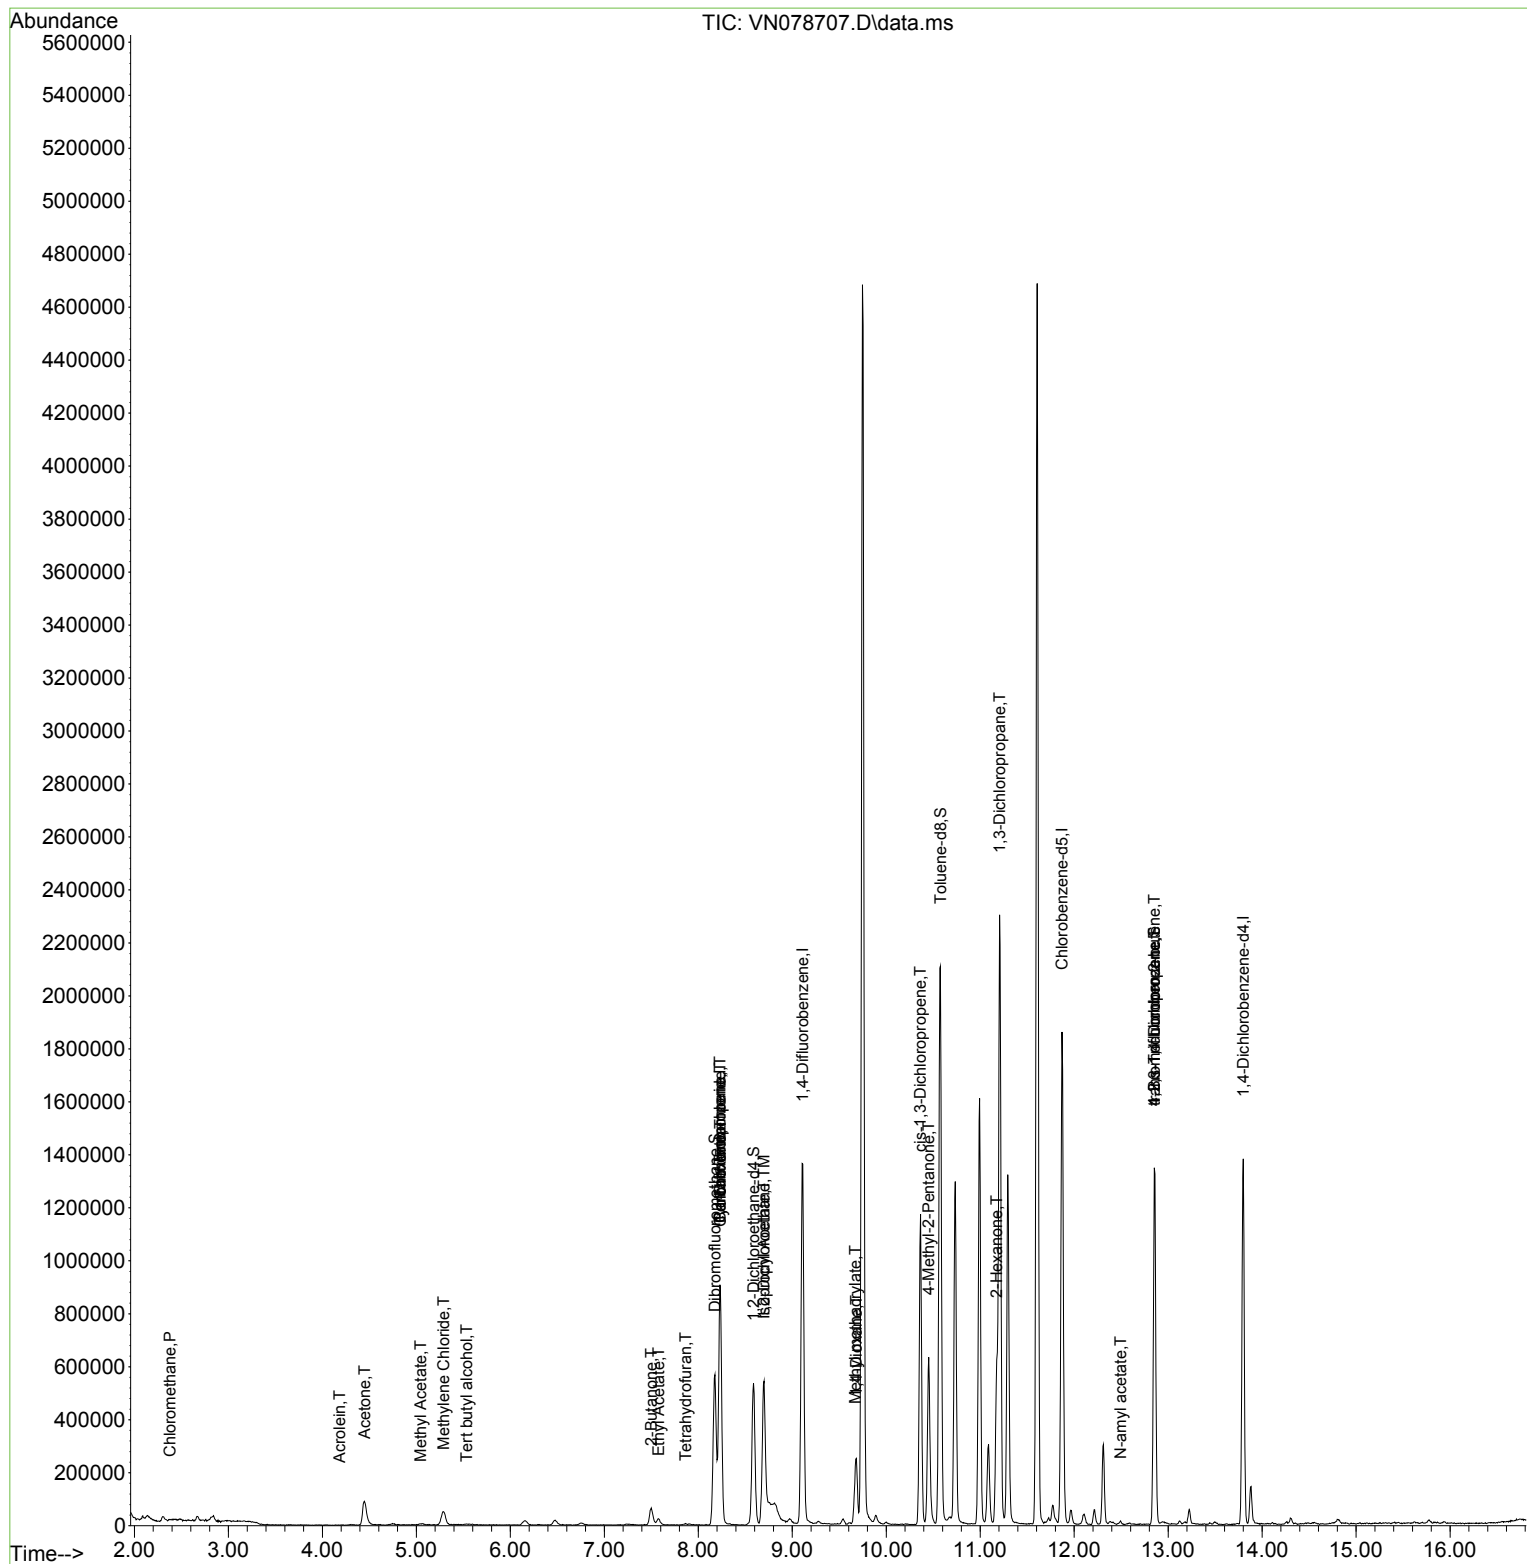




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2


Tgt Ion:168 Resp: 678448
Ion Ratio Lower Upper
168 100
99 60.2 53.0 79.6

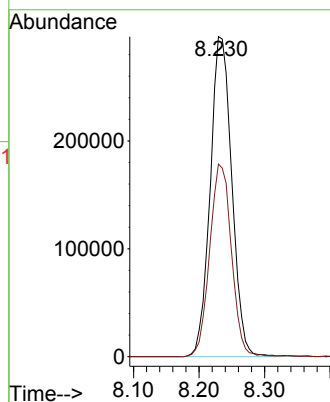

#3
Chloromethane
Concen: 0.357 ug/l
RT: 2.377 min Scan# 72
Delta R.T. 0.006 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59

Tgt Ion: 50 Resp: 3230
Ion Ratio Lower Upper
50 100
52 28.4 26.5 39.7


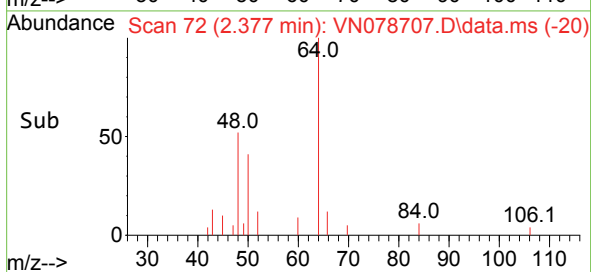
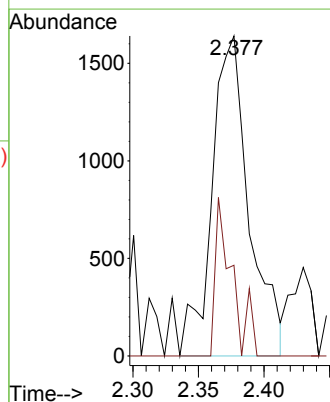





#5
Bromomethane
Concen: Below Cal
RT: 2.959 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2


Tgt Ion: 94 Resp: 1163
Ion Ratio Lower Upper
94 100
96 42.8 73.1 109.7#

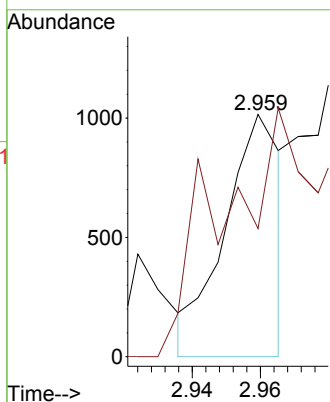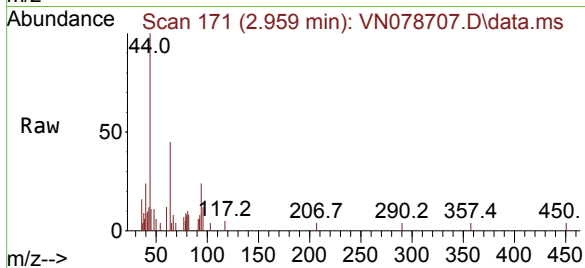

#6
Chloroethane
Concen: Below Cal
RT: 3.095 min Scan# 194
Delta R.T. -0.023 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59

Tgt Ion: 64 Resp: 775
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#



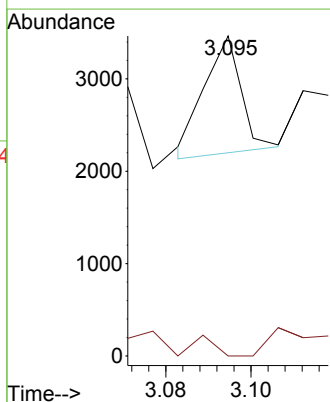
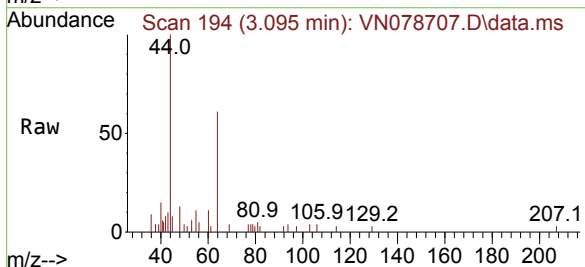




#11
Tert butyl alcohol
Concen: 1.186 ug/l
RT: 5.536 min Scan# 609
Delta R.T. -0.000 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2


Tgt Ion: 59 Resp: 1663
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#



#13
Acrolein
Concen: 0.351 ug/l
RT: 4.183 min Scan# 379
Delta R.T. -0.006 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59

Tgt Ion: 56 Resp: 484
Ion Ratio Lower Upper
56 100
55 21.5 54.5 81.7#


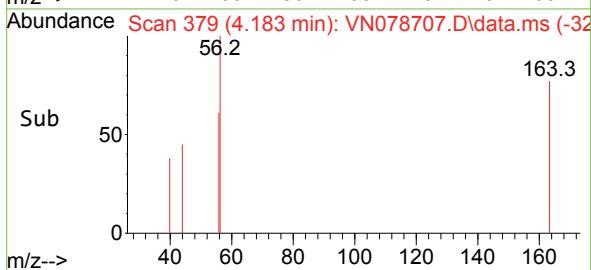






#16
Acetone
Concen: 60.370 ug/l
RT: 4.447 min Scan# 41
Delta R.T. 0.005 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2


Tgt Ion: 43 Resp: 171039
Ion Ratio Lower Upper
43 100
58 31.7 28.0 42.0

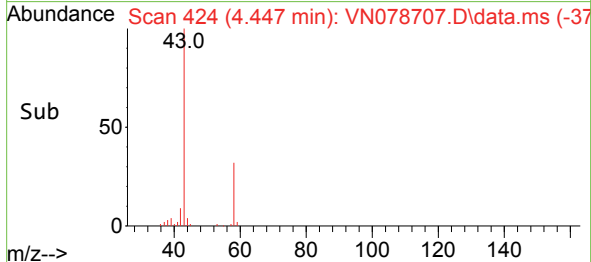

#18
Methyl Acetate
Concen: 0.463 ug/l
RT: 5.047 min Scan# 526
Delta R.T. 0.011 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59

Tgt Ion: 43 Resp: 5548
Ion Ratio Lower Upper
43 100
74 38.7 26.2 39.4




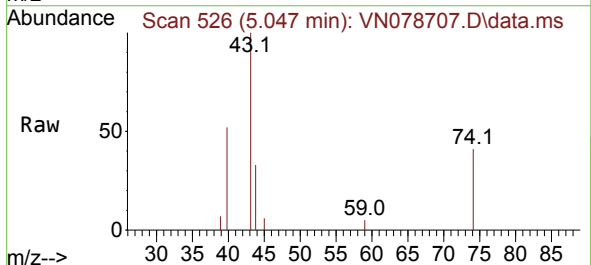




#20
Methylene Chloride
Concen: 4.272 ug/l
RT: 5.289 min Scan# 501
Delta R.T. 0.006 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2


Tgt Ion:	84	Resp:	43802
Ion	Ratio	Lower	Upper
84	100		
49	101.9	79.7	119.5
51	27.9	25.2	37.8
86	59.0	53.3	79.9

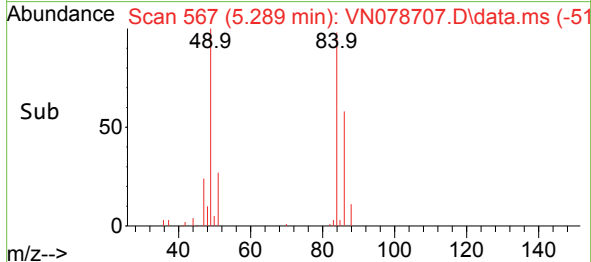

#25
2-Butanone
Concen: 22.417 ug/l
RT: 7.500 min Scan# 943
Delta R.T. 0.011 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59

Tgt Ion:	43	Resp:	99974
Ion	Ratio	Lower	Upper
43	100		
72	31.1	30.2	45.2

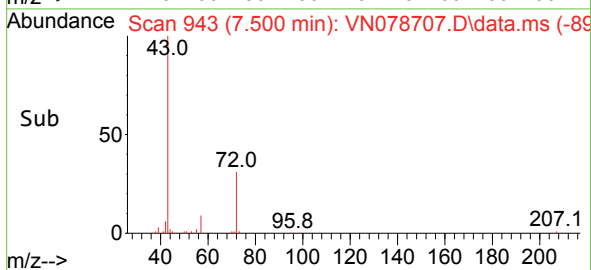



#29

Tetrahydrofuran

Concen: 1.191 ug/l

RT: 7.865 min Scan# 1005

Delta R.T. 0.018 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59

Instrument :

MSVOA_N

ClientSampleId :

PLAUDERVILLE-2





Tgt Ion: 42 Resp: 3485

Ion Ratio Lower Upper

42 100

72 33.1 49.8 74.6#

71 32.6 47.4 71.2#

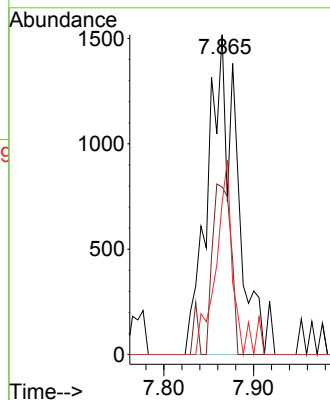

#31

Cyclohexane

Concen: 1.140 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.030 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59




Tgt Ion: 56 Resp: 14015


Ion Ratio Lower Upper

56 100

69 179.5 26.8 40.2#

84 177.4 81.8 122.6#

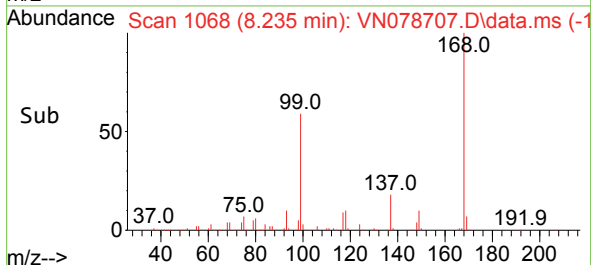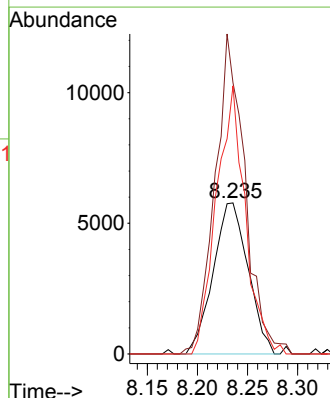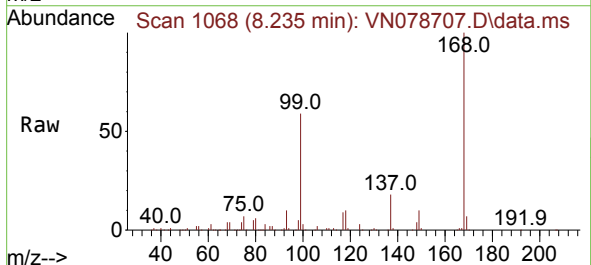



#33

1,2-Dichloroethane-d4

Concen: 49.519 ug/l

RT: 8.588 min Scan# 1127

Delta R.T. 0.005 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59

Instrument :

MSVOA_N

ClientSampleId :





PLAUDERVILLE-2

Tgt Ion: 65 Resp: 450387

Ion Ratio Lower Upper

65 100

67 53.6 0.0 106.6

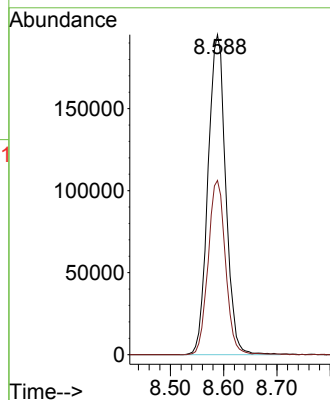

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1217

Delta R.T. 0.006 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59




Tgt Ion: 114 Resp: 1246656


Ion Ratio Lower Upper

114 100

63 19.0 0.0 36.4

88 15.5 0.0 30.6


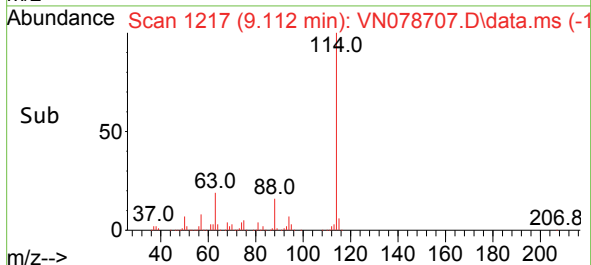
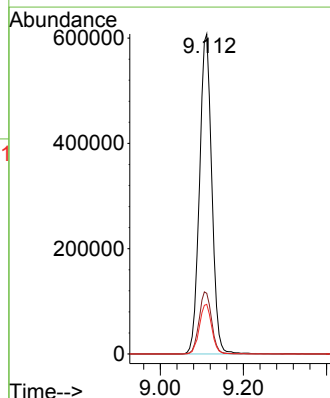





#35
Dibromofluoromethane
Concen: 49.805 ug/l
RT: 8.177 min Scan# 1058
Delta R.T. -0.000 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2


Tgt Ion:113 Resp: 421488
Ion Ratio Lower Upper
113 100
111 104.9 82.6 123.8
192 18.0 12.7 19.1

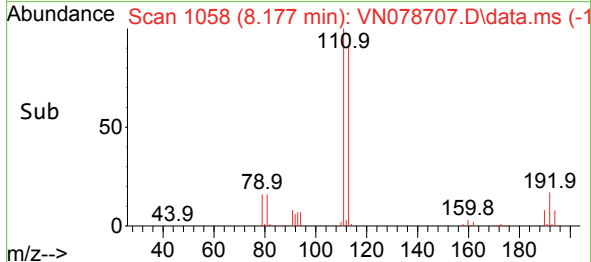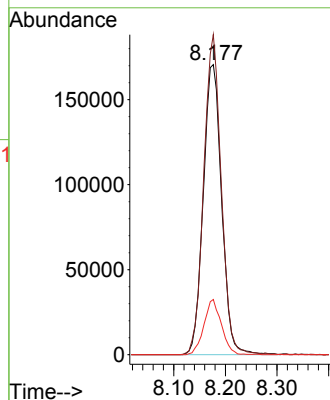

#36
1,1-Dichloropropene
Concen: 4.561 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59

Tgt Ion: 75 Resp: 55736
Ion Ratio Lower Upper
75 100
110 9.2 19.1 57.3#
77 0.0 25.0 37.4#

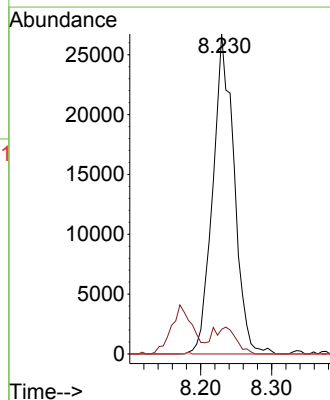



#37

Ethyl Acetate

Concen: 3.488 ug/l

RT: 7.577 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN078707.D


Acq: 31 Jul 2023 15:59

Instrument :

MSVOA_N

ClientSampleId :

PLAUDERVILLE-2

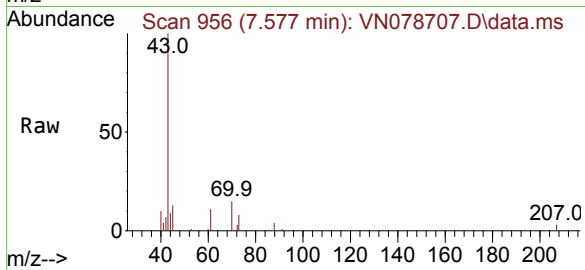




Tgt Ion: 43 Resp: 35533

Ion Ratio Lower Upper

43 100

61 12.9 13.2 19.8#

70 13.2 11.3 16.9

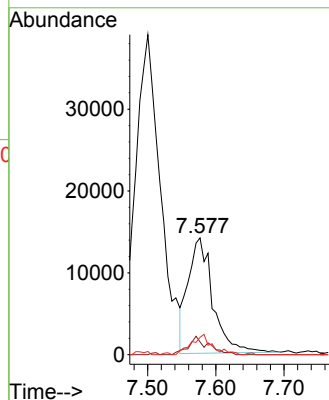

#38

Carbon Tetrachloride

Concen: 5.372 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.135 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59




Tgt Ion: 117 Resp: 71347


Ion Ratio Lower Upper

117 100

119 6.3 77.3 115.9#

121 0.0 23.3 34.9#

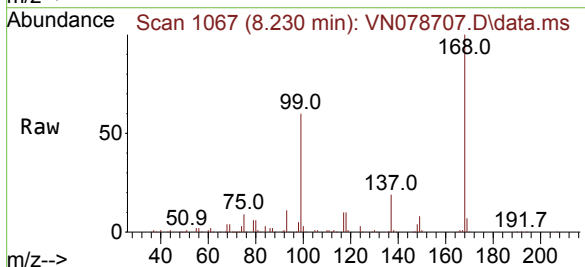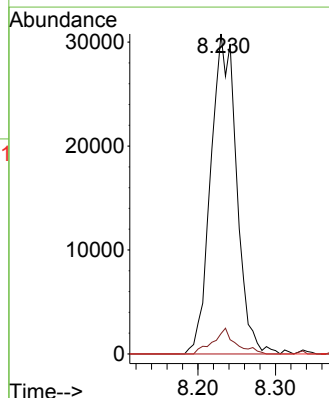



#42

1,2-Dichloroethane

Concen: 0.382 ug/l

RT: 8.700 min Scan# 1147

Delta R.T. 0.023 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59

Instrument :

MSVOA_N

ClientSampleId :





PLAUDERVILLE-2

Tgt Ion: 62 Resp: 4699

Ion Ratio Lower Upper

62 100

98 4.1 0.0 19.8

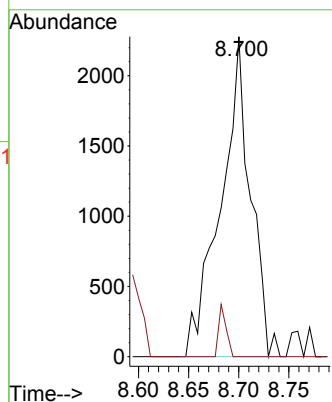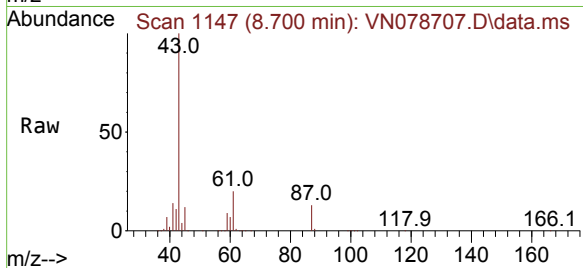

#43

Isopropyl Acetate

Concen: 40.662 ug/l

RT: 8.700 min Scan# 1147

Delta R.T. 0.006 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59




Tgt Ion: 43 Resp: 681919


Ion Ratio Lower Upper

43 100

61 17.5 24.7 37.1#

87 11.2 14.6 21.8#

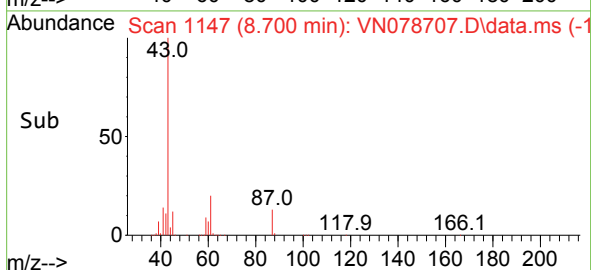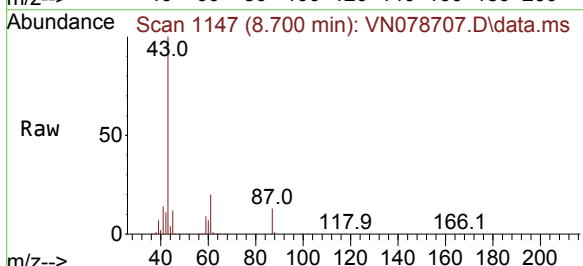



#48

Methyl methacrylate

Concen: 1.662 ug/l

RT: 9.671 min Scan# 11

Delta R.T. -0.017 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59

Instrument :

MSVOA_N

ClientSampleId :

PLAUDERVILLE-2





Tgt Ion: 41 Resp: 12911

Ion Ratio Lower Upper

41 100

69 1.5 90.4 135.6#

39 63.2 54.6 81.8

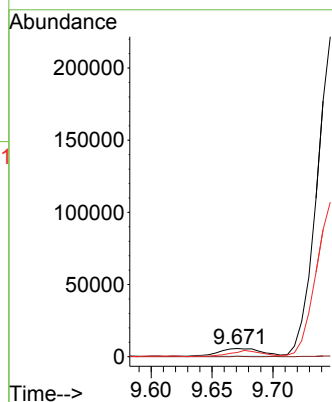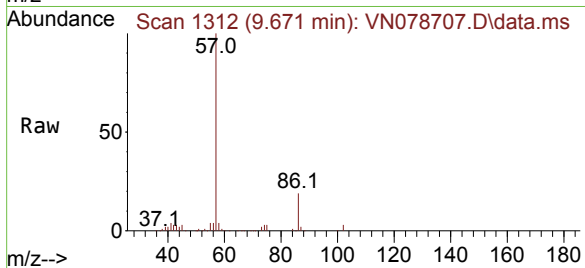

#49

1,4-Dioxane

Concen: 1.381 ug/l

RT: 9.682 min Scan# 1314

Delta R.T. -0.018 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59




Tgt Ion: 88 Resp: 234


Ion Ratio Lower Upper

88 100

43 0.0 17.0 25.6#

58 5288.5 47.0 70.4#


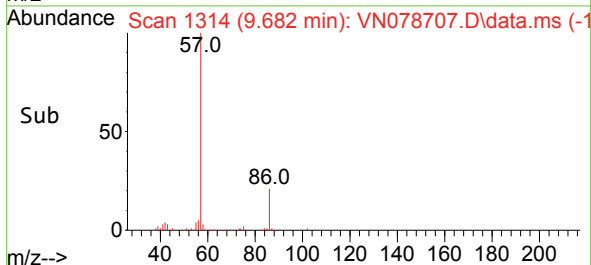

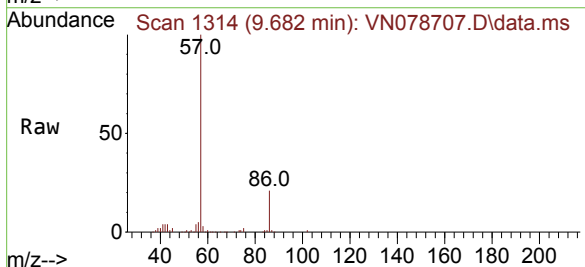




#50
Toluene-d8
Concen: 48.719 ug/l
RT: 10.576 min Scan# 1466
Delta R.T. 0.005 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2


Tgt Ion: 98 Resp: 1557517
Ion Ratio Lower Upper
98 100
100 63.6 52.0 78.0

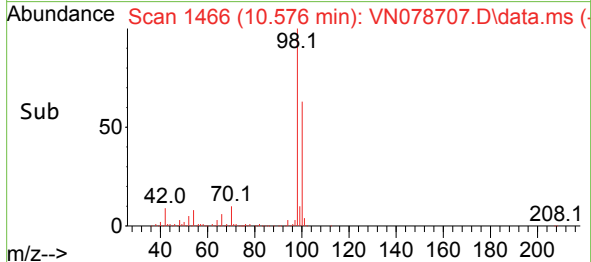

#51
4-Methyl-2-Pentanone
Concen: 43.303 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. -0.000 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59

Tgt Ion: 43 Resp: 431953
Ion Ratio Lower Upper
43 100
58 42.1 36.6 54.8




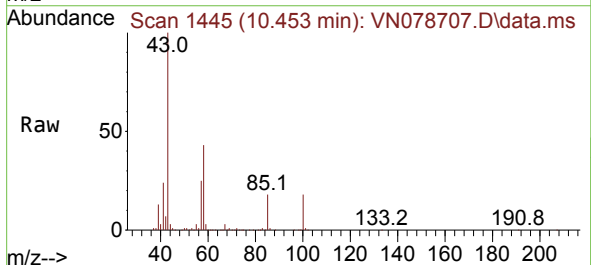


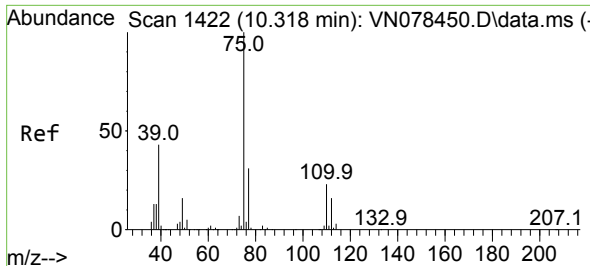

#54
 cis-1,3-Dichloropropene
 Concen: 15.808 ug/l
 RT: 10.365 min Scan# 1422
 Delta R.T. 0.047 min
 Lab File: VN078707.D
 Acq: 31 Jul 2023 15:59




Instrument :
 MSVOA_N
 ClientSampleId :
 PLAUDERVILLE-2


Tgt Ion: 75 Resp: 223313
 Ion Ratio Lower Upper
 75 100
 77 0.6 26.1 39.1#
 39 27.7 31.6 47.4#

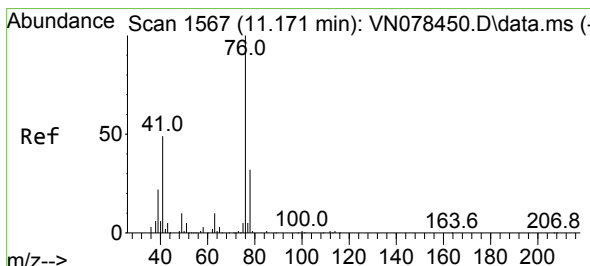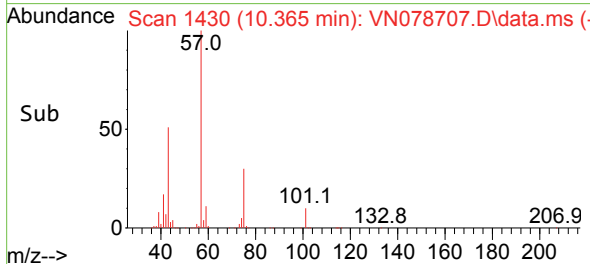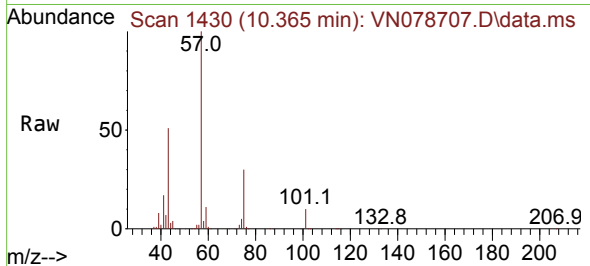

#57
 1,3-Dichloropropane
 Concen: 1.714 ug/l
 RT: 11.206 min Scan# 1573
 Delta R.T. 0.035 min
 Lab File: VN078707.D
 Acq: 31 Jul 2023 15:59

Tgt Ion: 76 Resp: 25763
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.1 39.1#


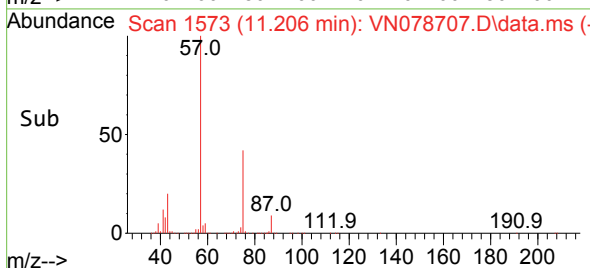
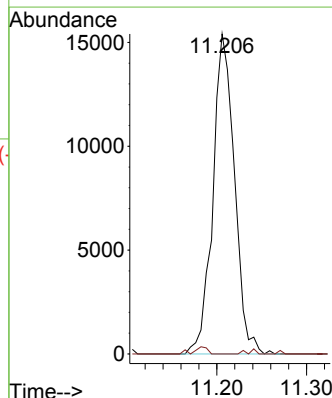
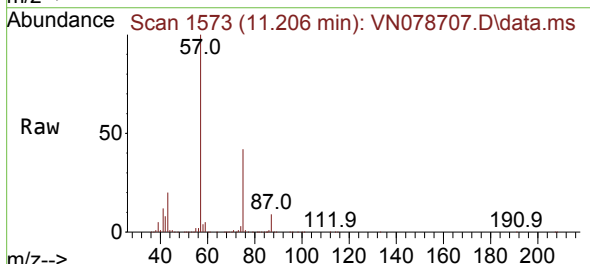




#59
2-Hexanone
Concen: 69.371 ug/l
RT: 11.176 min Scan# 11176
Delta R.T. -0.024 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2


Tgt Ion: 43 Resp: 491806
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#

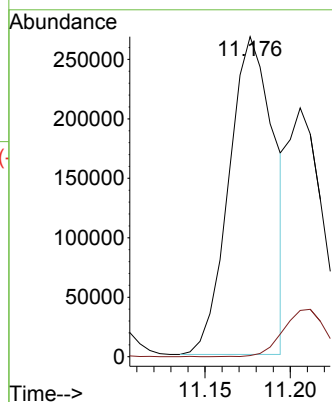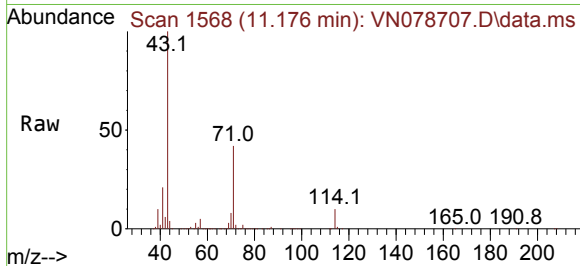

#62
4-Bromofluorobenzene
Concen: 52.067 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59

Tgt Ion: 95 Resp: 512715
Ion Ratio Lower Upper
95 100
174 75.1 0.0 143.8
176 72.2 0.0 135.8

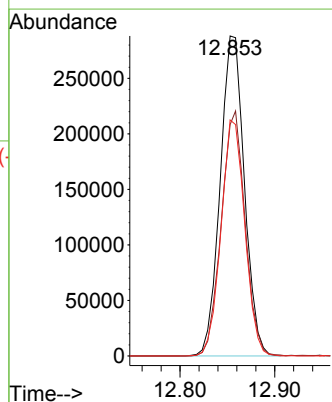

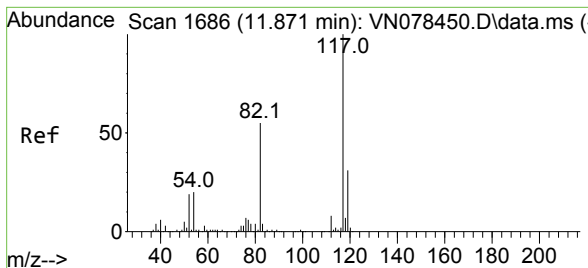

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.871 min Scan# 1

Delta R.T. -0.001 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59

Instrument :

MSVOA_N

ClientSampleId :

PLAUDERVILLE-2





Tgt Ion:117 Resp: 1135431

Ion Ratio Lower Upper

117 100

82 58.1 44.0 66.0

119 32.8 25.6 38.4

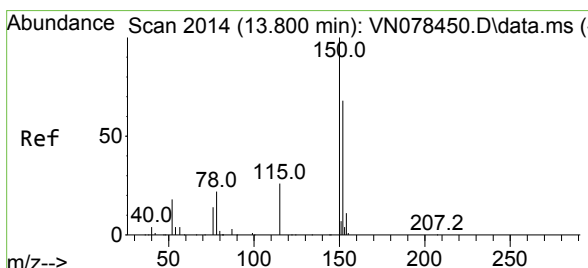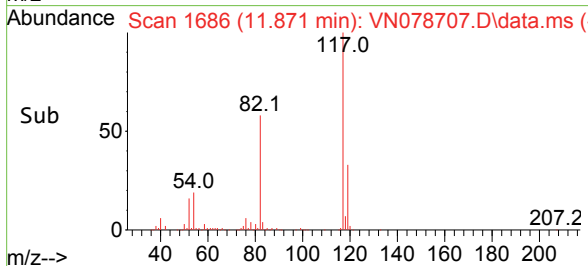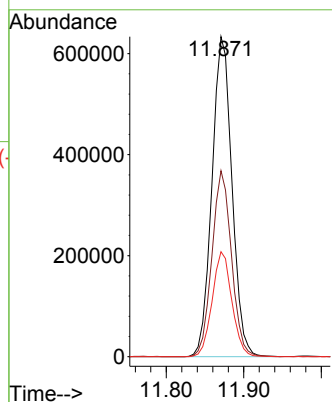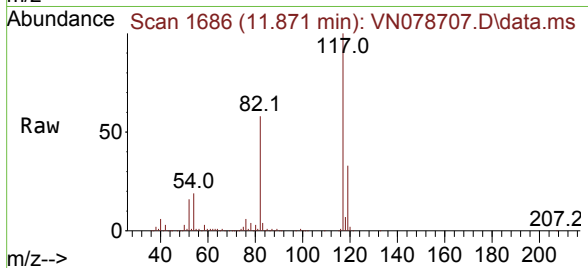

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.800 min Scan# 2014

Delta R.T. -0.000 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59




Tgt Ion:152 Resp: 389156


Ion Ratio Lower Upper

152 100

115 62.4 32.3 96.8

150 157.6 0.0 355.8


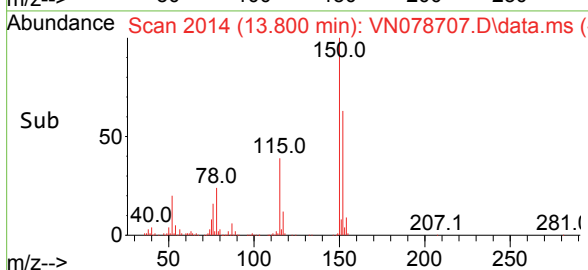

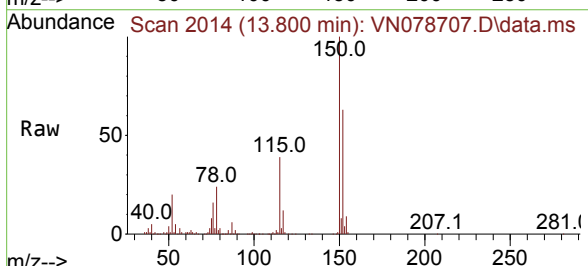




#74
N-amy1 acetate
Concen: 0.438 ug/l
RT: 12.494 min Scan# 1
Delta R.T. -0.006 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59




Instrument :
MSVOA_N
ClientSampleId :
PLAUDERVILLE-2


Tgt Ion: 43	Resp: 5522
Ion Ratio	Lower Upper
43	100
70	4.9 43.4 65.2#
55	12.8 21.4 32.0#
61	0.0 22.8 34.2#

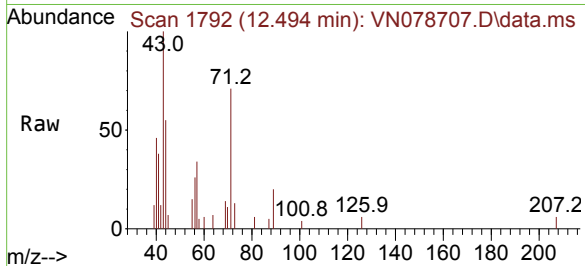

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.935 min Scan# 1867
Delta R.T. -0.006 min
Lab File: VN078707.D
Acq: 31 Jul 2023 15:59

Tgt Ion: 83	Resp: 694
Ion Ratio	Lower Upper
83	100
131	0.0 5.0 15.0#
85	76.9 31.9 95.7

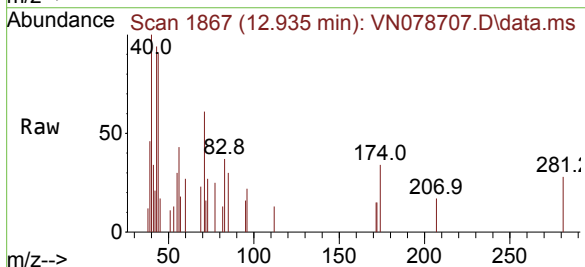



#76

1,2,3-Trichloropropane

Concen: 26.774 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59

Instrument :

MSVOA_N

ClientSampleId :





PLAUDERVILLE-2

Tgt Ion: 75 Resp: 251850

Ion Ratio Lower Upper

75 100

77 1.6 84.5 253.5#

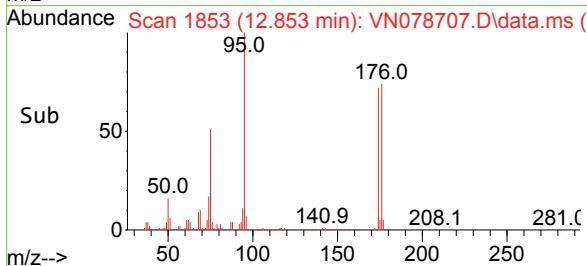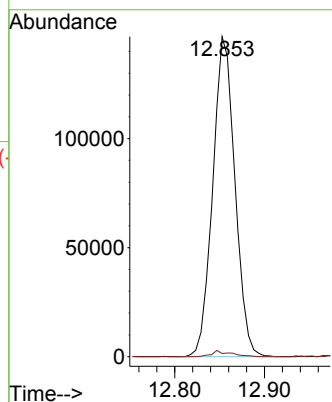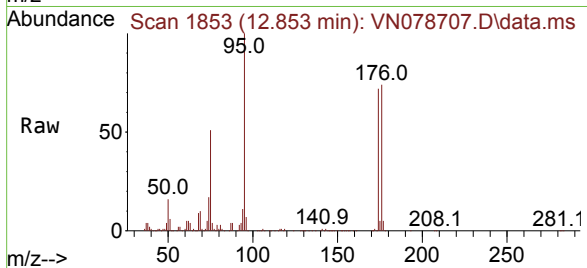

#77

Bromobenzene

Concen: Below Cal

RT: 12.988 min Scan# 1876

Delta R.T. 0.000 min

Lab File: VN078707.D

Acq: 31 Jul 2023 15:59




Tgt Ion:156 Resp: 417


Ion Ratio Lower Upper

156 100

77 325.9 107.7 323.3#

158 102.6 48.4 145.3


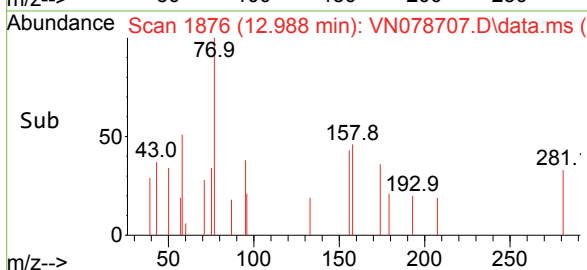

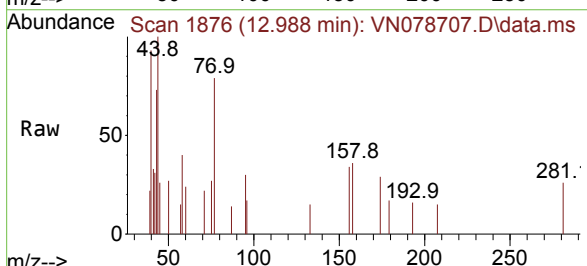


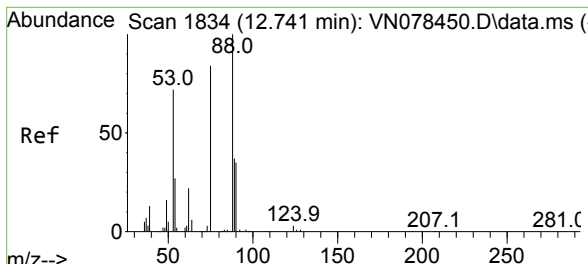

#81
 trans-1,4-Dichloro-2-butene
 Concen: 70.358 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. 0.112 min
 Lab File: VN078707.D
 Acq: 31 Jul 2023 15:59




Instrument :
 MSVOA_N
 ClientSampleId :
 PLAUDERVILLE-2


Tgt Ion:	75	Resp:	251850
Ion Ratio	Lower	Upper	
75	100		
53	0.0	67.4	101.2#
89	0.0	38.8	58.2#

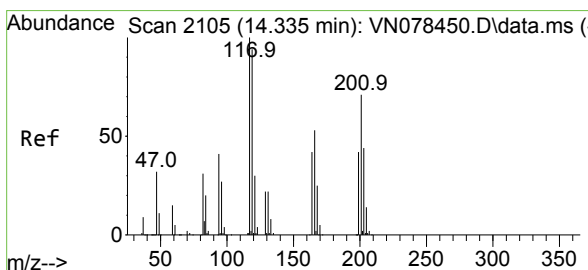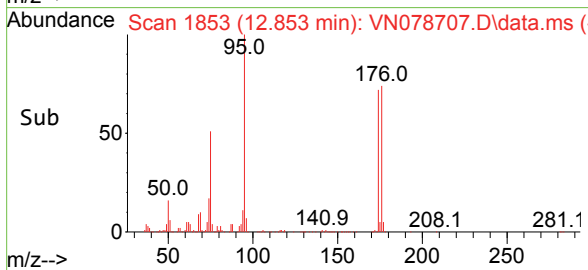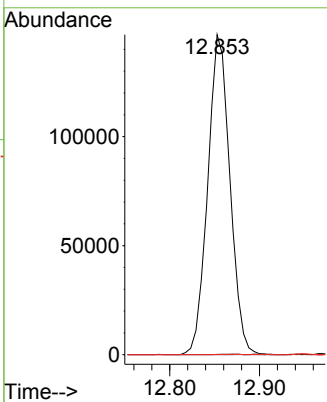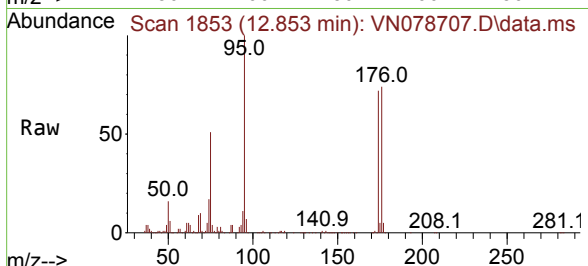

#90
 Hexachloroethane
 Concen: Below Cal
 RT: 14.335 min Scan# 2105
 Delta R.T. 0.000 min
 Lab File: VN078707.D
 Acq: 31 Jul 2023 15:59

Tgt Ion:	117	Resp:	328
Ion Ratio	Lower	Upper	
117	100		
201	0.0	29.3	88.0#

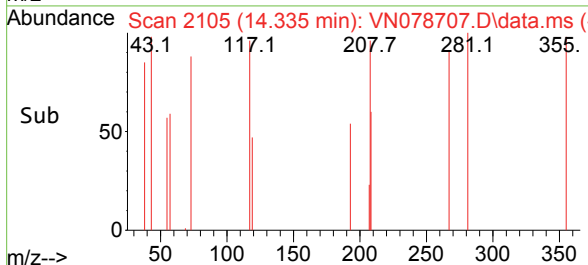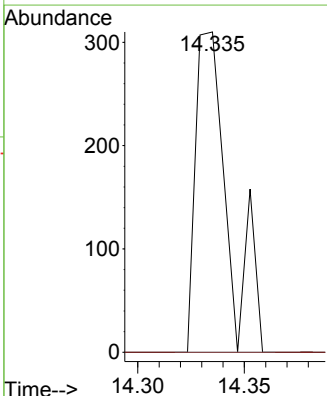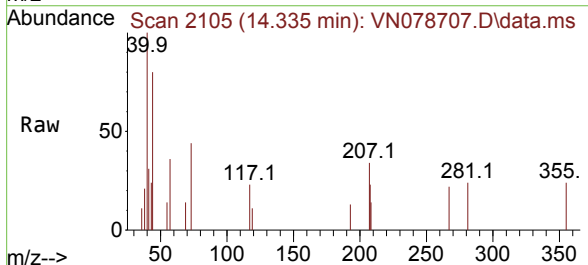



#92

1,2-Dibromo-3-Chloropropane

Concen: Below Cal

RT: 14.723 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN078707.D


Acq: 31 Jul 2023 15:59

Instrument :

MSVOA_N

ClientSampleId :

PLAUDERVILLE-2

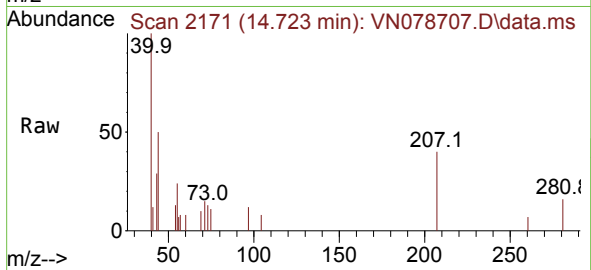

Tgt Ion: 75 Resp: 263

Ion Ratio Lower Upper

75 100

155 0.0 39.1 117.2#

157 0.0 50.3 150.9#

