
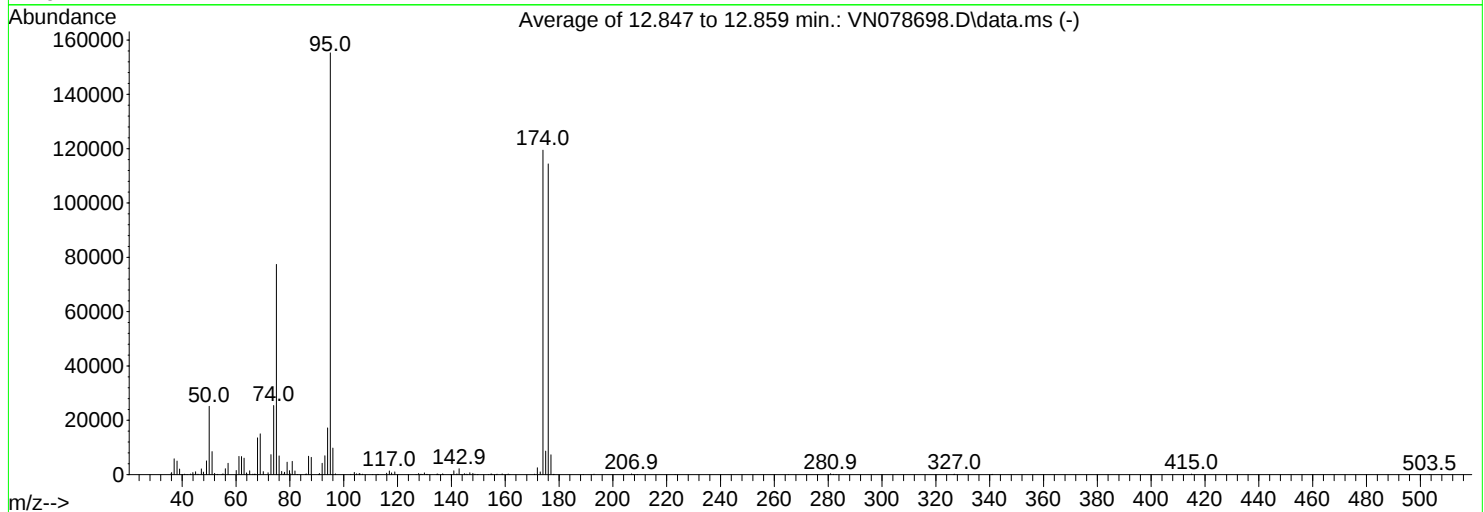


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN073123\
Data File : VN078698.D
Acq On : 31 Jul 2023 09:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

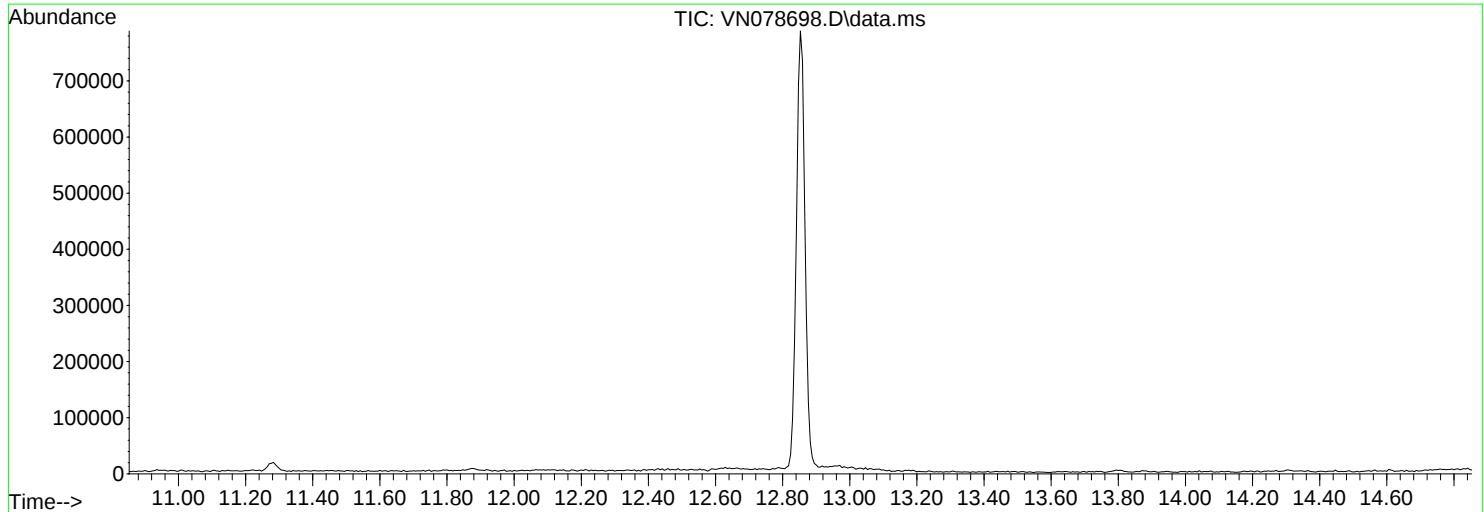

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	25152	PASS
75	95	30	60	49.9	77419	PASS
95	95	100	100	100.0	155285	PASS
96	95	5	9	6.3	9779	PASS
173	174	0.00	2	0.9	1027	PASS
174	95	50	100	76.9	119448	PASS
175	174	5	9	7.2	8651	PASS
176	174	95	101	95.8	114421	PASS
177	176	5	9	6.4	7320	PASS

Average of 12.847 to 12.859 min.: VN078698.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	350	45.85	198	57.05	4208	68.00	1358
36.05	784	47.10	2105	60.05	1532	69.00	1500
37.00	5835	47.90	940	61.05	6735	70.10	109
38.05	5032	49.00	5067	62.00	6687	71.90	72
39.00	2067	50.00	25152	63.00	6046	72.95	7377
39.95	63	51.10	8470	63.90	663	73.95	25461
40.90	165	52.05	456	64.10	176	75.00	77419
41.80	56	53.05	145	65.05	1429	76.00	6904
43.15	220	54.80	134	66.25	161	76.95	1172
43.95	748	55.15	306	66.90	182	77.70	159
44.95	1061	56.00	2206	67.10	211	78.00	882

Average of 12.847 to 12.859 min.: VN078698.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	4585	90.95	402	106.00	309	127.85	425
79.85	1452	92.00	4195	106.95	176	128.50	74
80.10	286	93.00	6954	110.80	62	128.70	195
80.90	4865	94.00	17228	112.70	127	129.20	75
81.90	1353	95.00	155285	112.90	55	129.95	645
82.80	50	96.00	9779	115.95	562	130.70	114
85.80	71	96.95	300	116.95	1348	131.20	101
86.05	297	102.65	117	117.80	658	134.60	165
86.95	6756	103.95	808	118.95	1004	134.85	231
87.95	6341	104.75	297	124.00	89	135.10	113
90.70	119	105.75	446	126.90	73	136.75	295

Average of 12.847 to 12.859 min.: VN078698.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
137.00	116	148.00	502	161.15	238	189.00	55
139.80	70	148.75	194	161.70	53	193.00	166
140.90	1422	149.70	68	170.95	175	206.95	322
142.05	272	149.90	67	171.95	2543	207.70	59
142.90	2171	153.80	83	173.00	1027	209.10	64
143.60	70	154.70	221	174.00	119448	223.10	68
144.85	378	155.00	243	175.05	8651	265.20	78
145.10	123	156.70	51	176.00	114421	280.90	344
145.75	185	156.95	202	177.00	7320	282.00	111
146.00	63	158.85	310	177.90	110	282.90	84
146.85	737	160.70	53	178.10	109	326.70	110

Average of 12.847 to 12.859 min.: VN078698.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
327.00	162						
340.60	91						
341.05	127						
415.00	253						
503.50	92						

Instrument :

MSVOA_N

ClientSampleId :

BFB