

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080119\
 Data File : VN057034.D
 Acq On : 1 Aug 2019 14:01
 Operator : JC/SP
 Sample : K4097-03
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-VPB203-GW-458-460

Quant Time: Aug 02 05:44:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 27 01:33:29 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	569731	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.58	114	817502	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	673498	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	178051	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.02	65	341234	58.51	ug/l	0.00
Spiked Amount 50.000			Recovery	=	117.02%	
35) Dibromofluoromethane	7.58	113	304899	58.26	ug/l	0.00
Spiked Amount 50.000			Recovery	=	116.52%	
50) Toluene-d8	10.08	98	1152525	57.75	ug/l	0.00
Spiked Amount 50.000			Recovery	=	115.50%	
62) 4-Bromofluorobenzene	12.40	95	296491	45.64	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.28%	
Target Compounds						
16) Acetone	3.81	43	5562	2.633	ug/l	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN080119\
Data File : VN057034.D
Acq On : 1 Aug 2019 14:01
Operator : JC/SP
Sample : K4097-03
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB203-GW-458-460

Quant Time: Aug 02 05:44:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Quant Title : SW846 8260
QLast Update : Sat Jul 27 01:33:29 2019
Response via : Initial Calibration

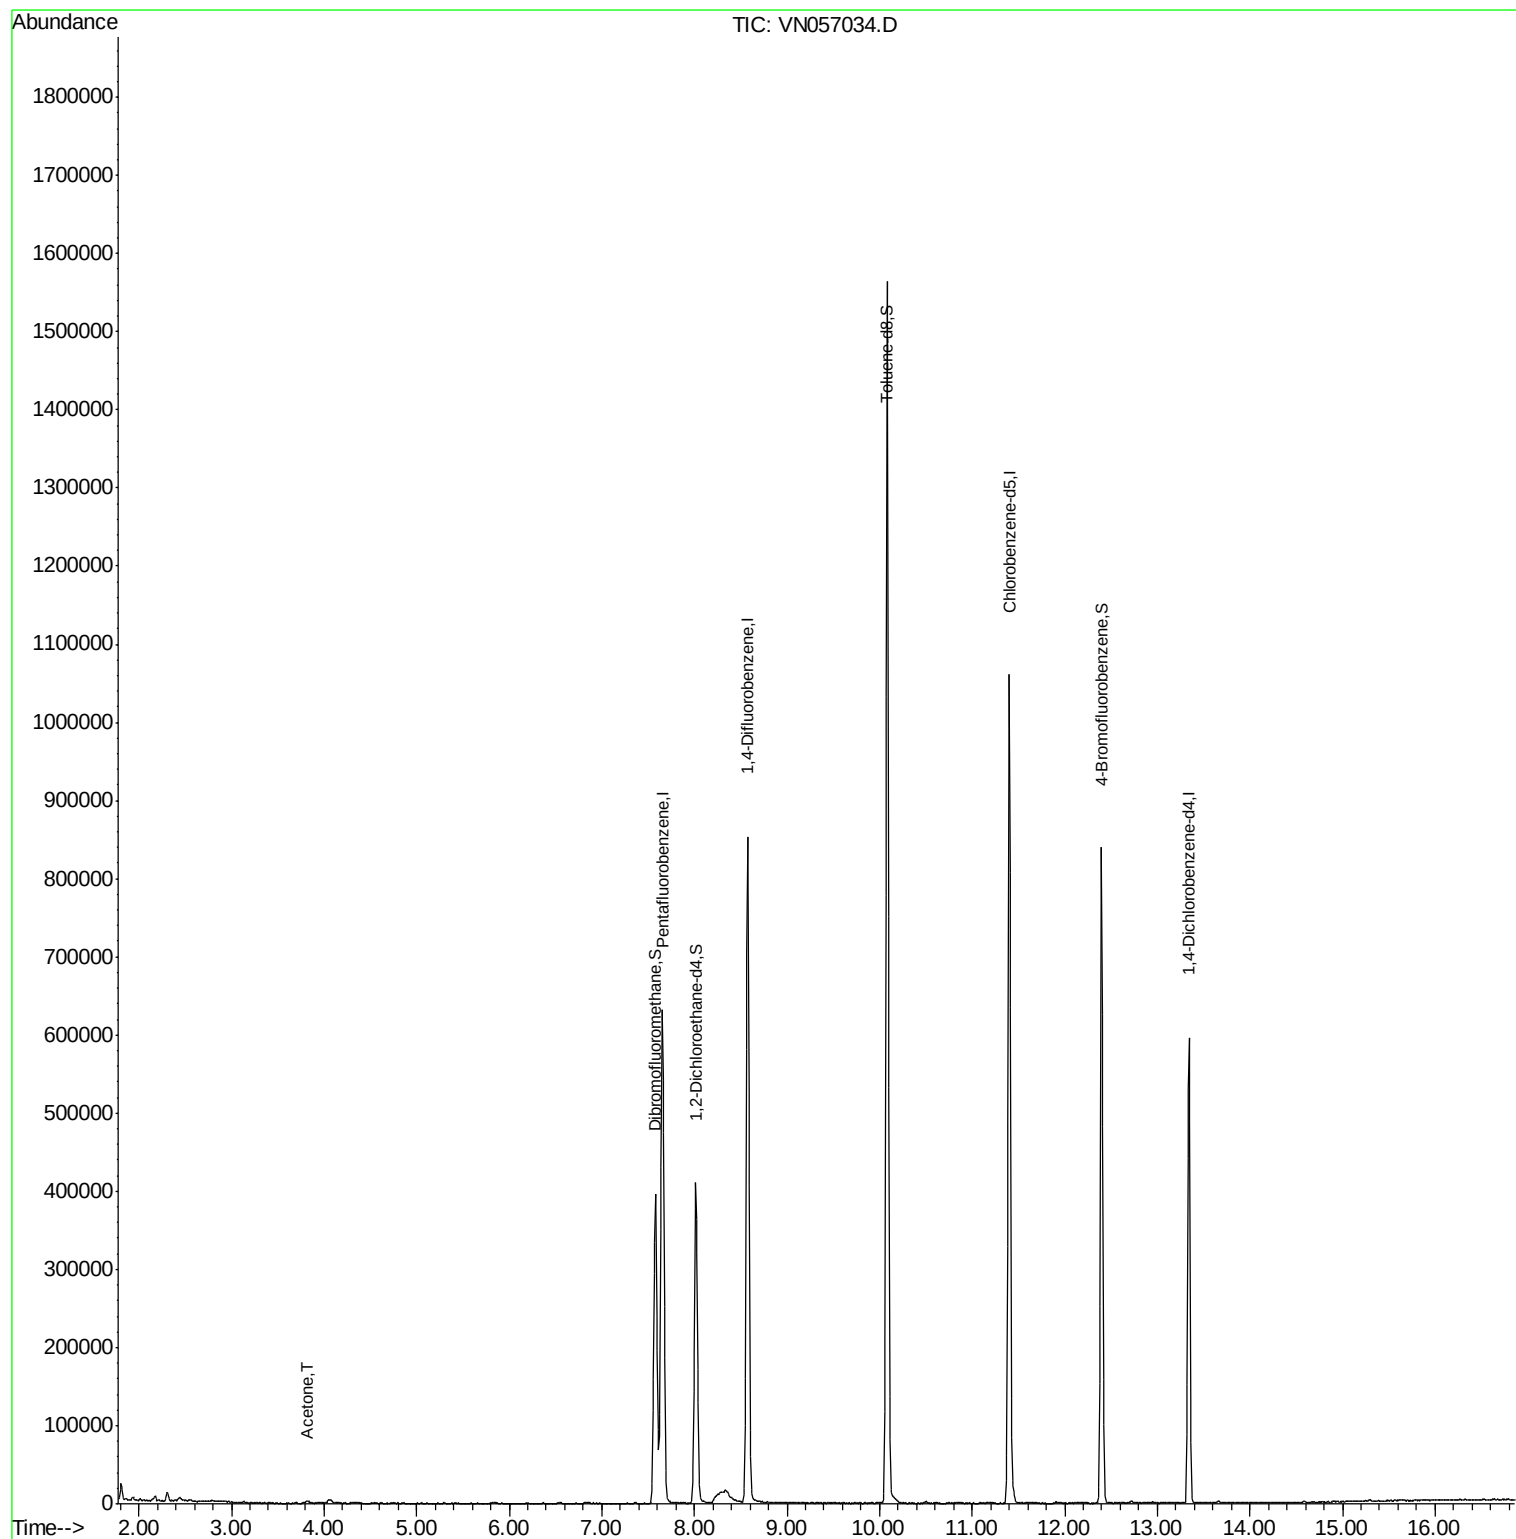

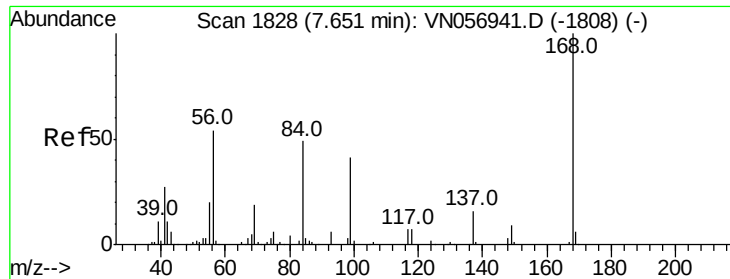

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.65 min Scan# 1829

Delta R.T. 0.00 min

Lab File: VN057034.D

Acq: 1 Aug 2019 14:01

Instrument :

MSVOA_N

ClientSampleId :


BP-VPB203-GW-458-460

Tot Ion:168 Resp: 569731

Ion Ratio Lower Upper




168 100

99 49.5 39.0 58.4

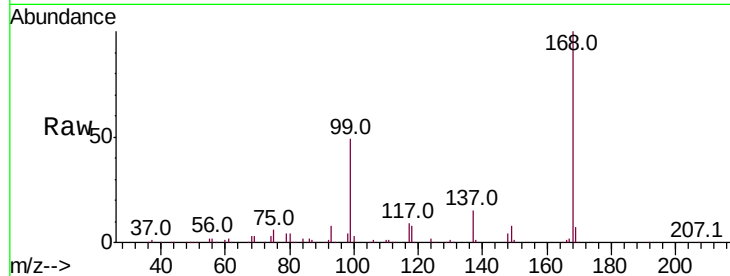

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

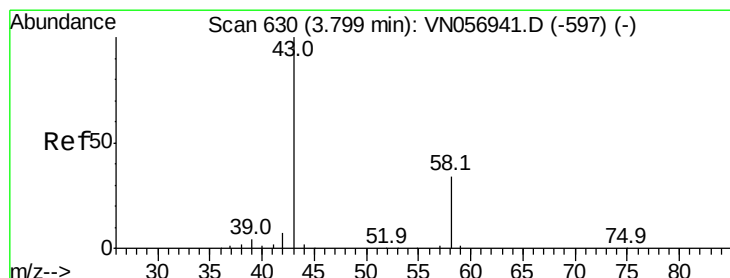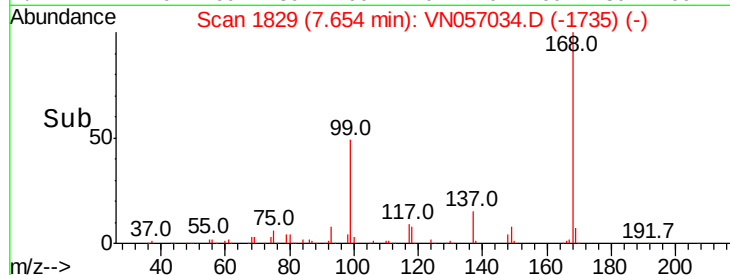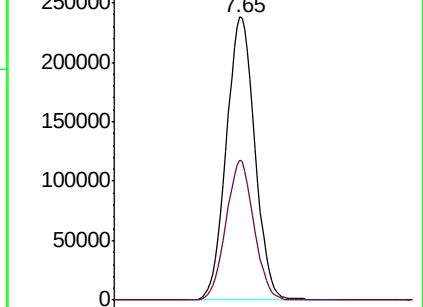

#16

Acetone

Concen: 2.633 ug/l

RT: 3.81 min Scan# 634

Delta R.T. 0.01 min

Lab File: VN057034.D


Acq: 1 Aug 2019 14:01

Tgt Ion: 43 Resp: 5562

Ion Ratio Lower Upper



43 100


58 30.3 27.2 40.8

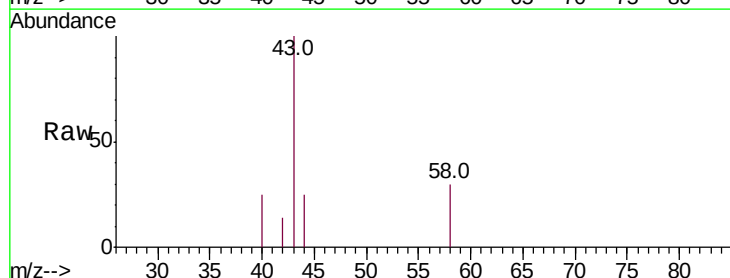

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0



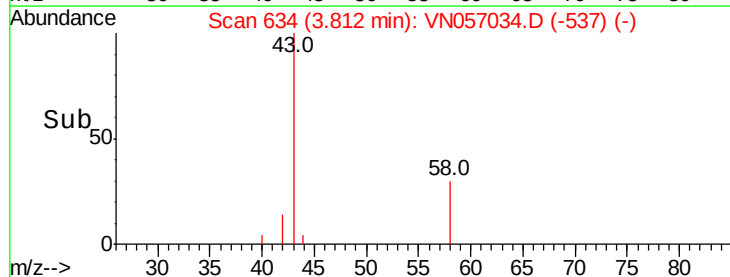
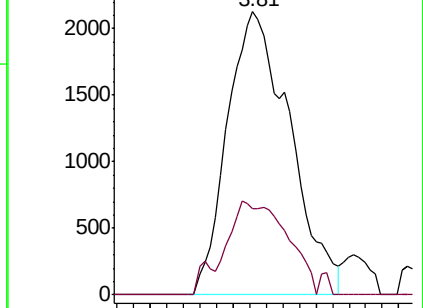


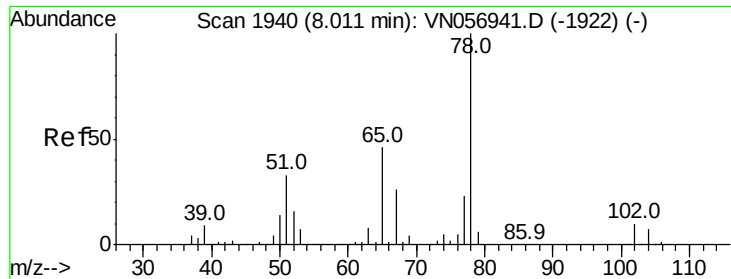

#33
 1,2-Dichloroethane-d4
 Concen: 58.510 ug/l
 RT: 8.02 min Scan# 1942
 Delta R.T. 0.01 min
 Lab File: VN057034.D
 Acq: 1 Aug 2019 14:01




Instrument :
 MSVOA_N
 ClientSampleId :
 BP-VPB203-GW-458-460


Tot Ion: 65 Resp: 341234
 Ion Ratio Lower Upper
 65 100
 67 54.8 0.0 112.0

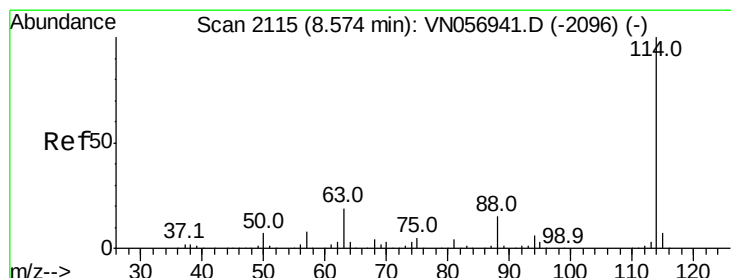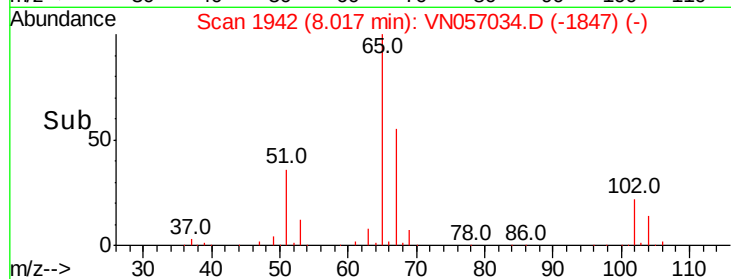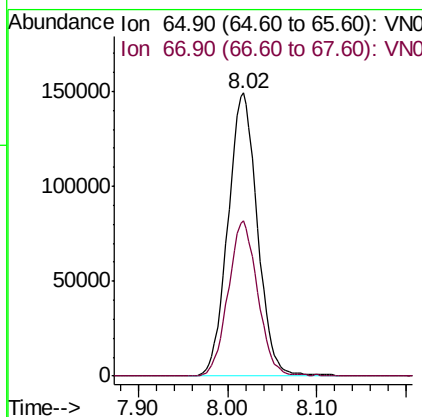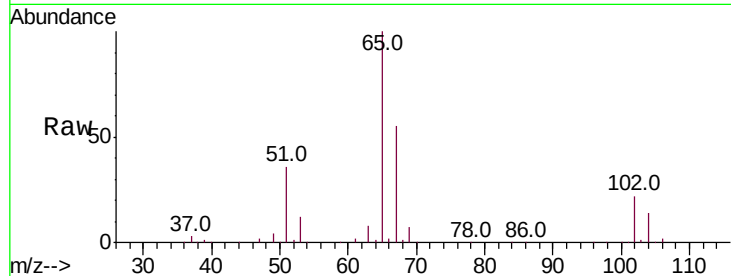

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.58 min Scan# 2116
 Delta R.T. 0.00 min
 Lab File: VN057034.D
 Acq: 1 Aug 2019 14:01

Tgt Ion: 114 Resp: 817502
 Ion Ratio Lower Upper
 114 100
 63 18.9 0.0 38.0
 88 15.2 0.0 30.0


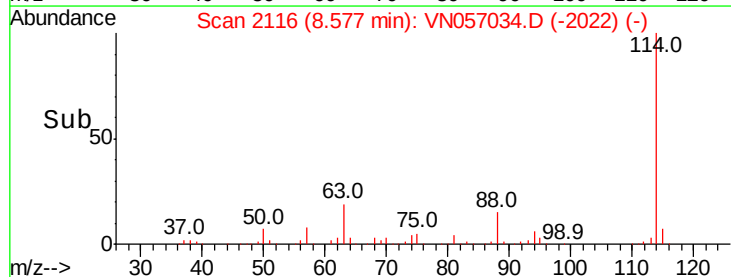
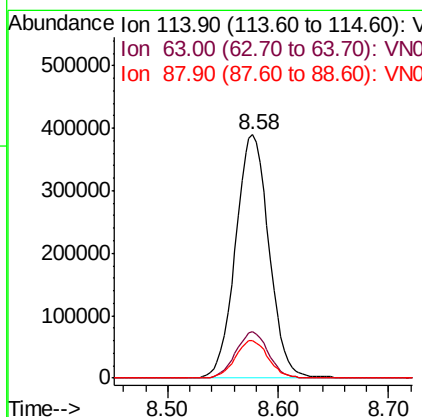
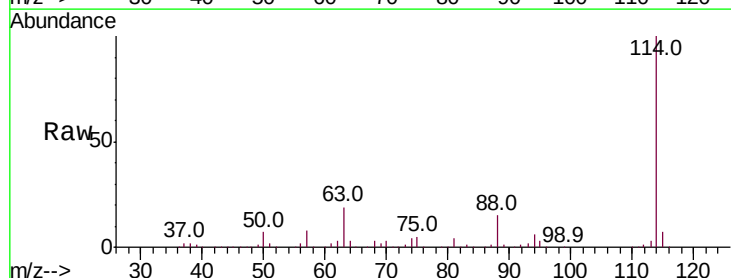


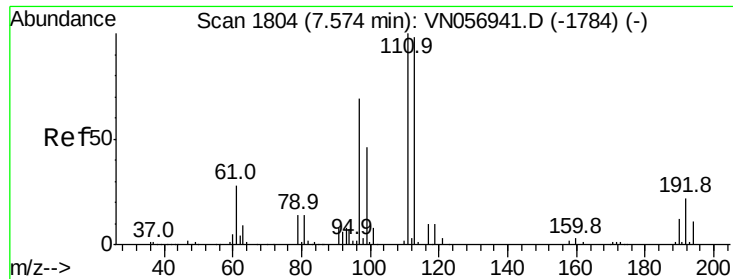

#35
 Dibromofluoromethane
 Concen: 58.260 ug/l
 RT: 7.58 min Scan# 1806
 Delta R.T. 0.01 min
 Lab File: VN057034.D
 Acq: 1 Aug 2019 14:01




Instrument :
 MSVOA_N
 ClientSampleId :
 BP-VPB203-GW-458-460


Tot Ion:113 Resp: 304899
 Ion Ratio Lower Upper
 113 100
 111 102.7 82.0 123.0
 192 23.4 18.4 27.6

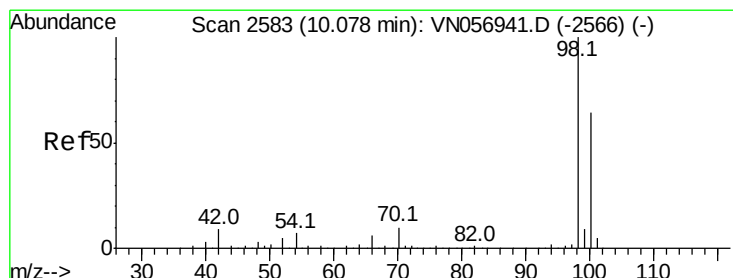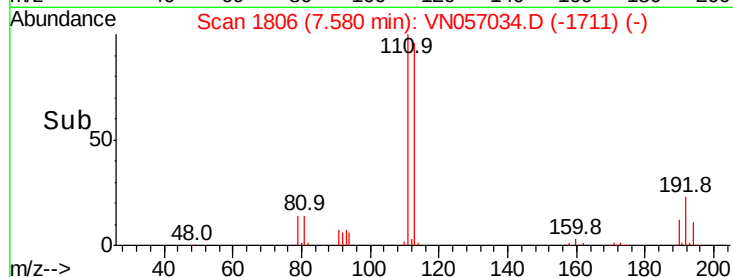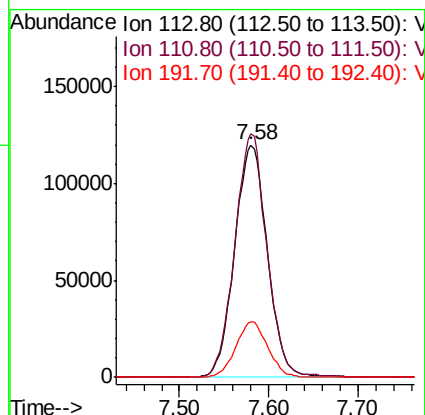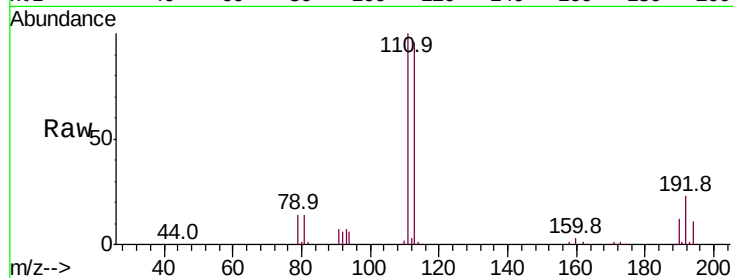

#50
 Toluene-d8
 Concen: 57.749 ug/l
 RT: 10.08 min Scan# 2584
 Delta R.T. 0.00 min
 Lab File: VN057034.D
 Acq: 1 Aug 2019 14:01

Tgt Ion: 98 Resp: 1152525
 Ion Ratio Lower Upper
 98 100
 100 64.1 51.3 76.9

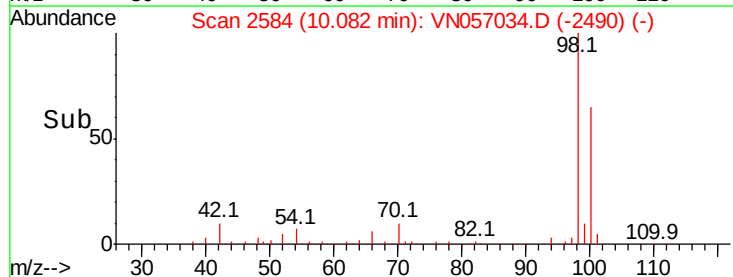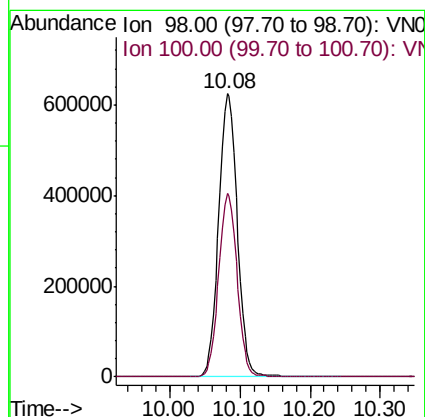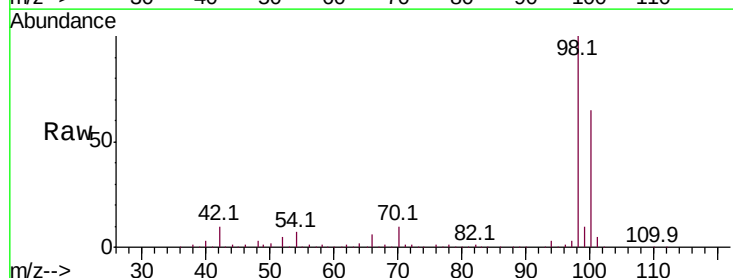

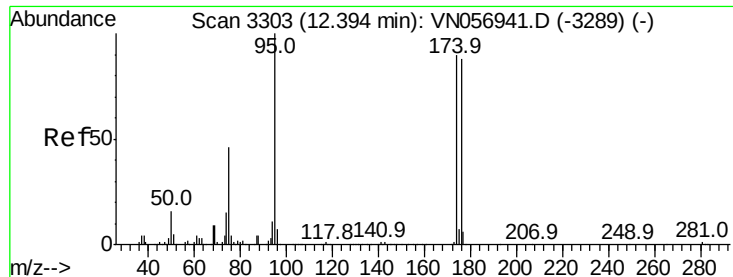

#62

4-Bromofluorobenzene

Concen: 45.635 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. 0.00 min

Lab File: VN057034.D

Acq: 1 Aug 2019 14:01

Instrument :

MSVOA_N

ClientSampleId :

BP-VPB203-GW-458-460


Tot Ion: 95 Resp: 296491

Ion Ratio Lower Upper

95 100

174 94.7 0.0 182.2




176 90.7 0.0 179.4

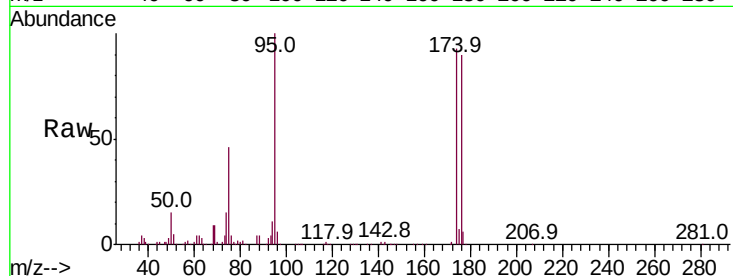

Abundance Ion 94.90 (94.60 to 95.60): VN056941.D (-3289) (-)

Ion 173.80 (173.50 to 174.50): VN056941.D (-3289) (-)

Ion 175.80 (175.50 to 176.50): VN056941.D (-3289) (-)

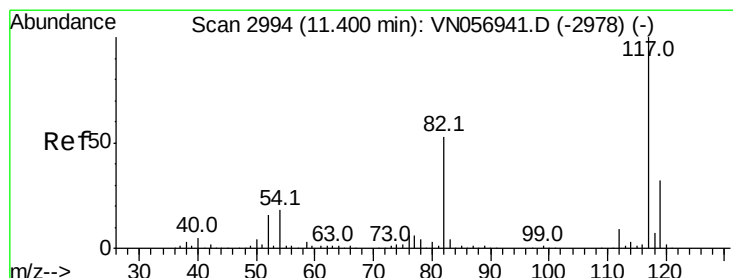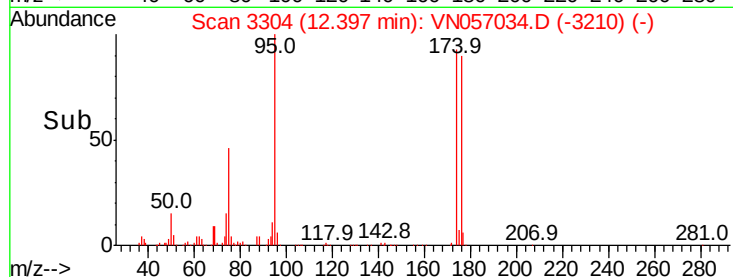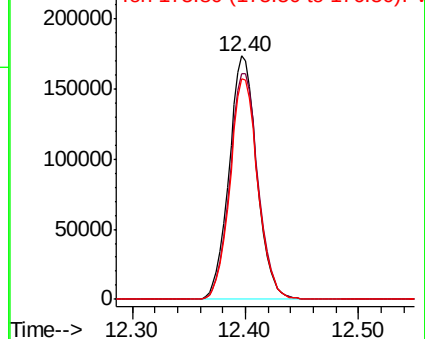

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.40 min Scan# 2994

Delta R.T. -0.00 min

Lab File: VN057034.D

Acq: 1 Aug 2019 14:01


Tgt Ion: 117 Resp: 673498

Ion Ratio Lower Upper

117 100

82 51.7 42.2 63.4



119 31.9 25.8 38.6

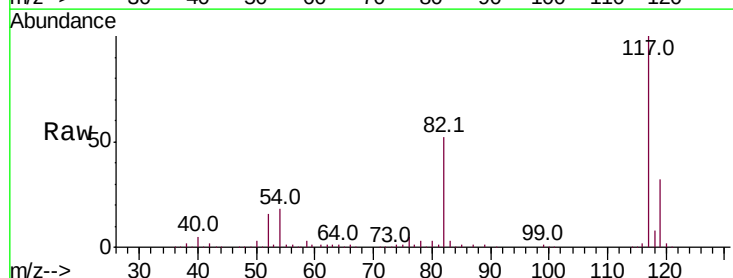


Abundance Ion 116.90 (116.60 to 117.60): VN056941.D (-2978) (-)

Ion 82.00 (81.70 to 82.70): VN056941.D (-2978) (-)

Ion 118.90 (118.60 to 119.60): VN056941.D (-2978) (-)

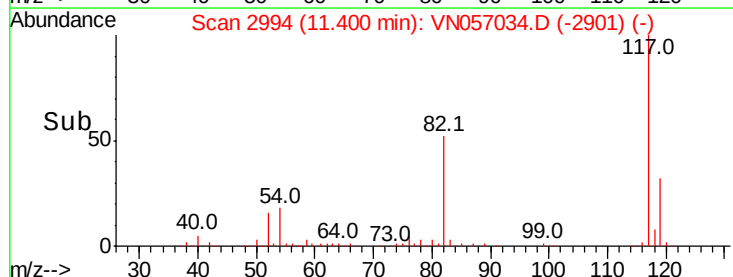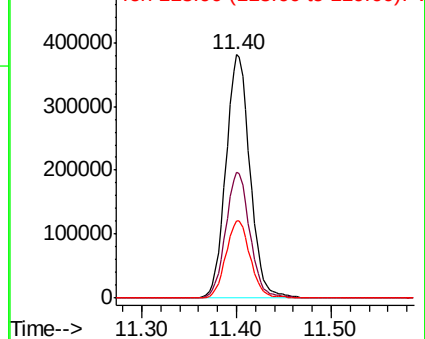

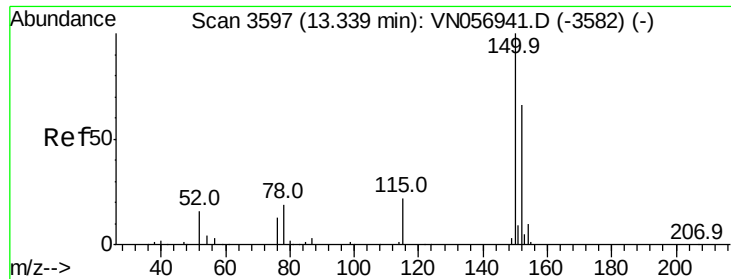

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. 0.00 min

Lab File: VN057034.D

Acq: 1 Aug 2019 14:01

Instrument :

MSVOA_N

ClientSampleId :

BP-VPB203-GW-458-460


Tot Ion:152 Resp: 178051

Ion Ratio Lower Upper

152 100

115 55.4 28.2 84.6

150 160.1 0.0 349.4

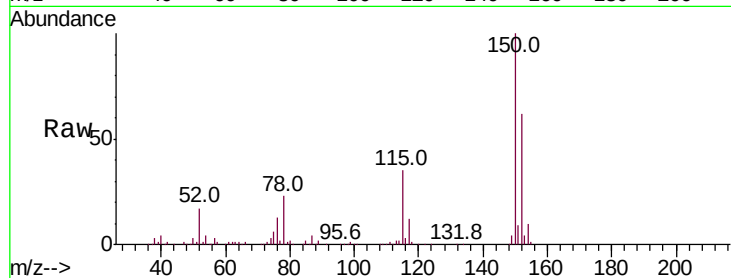

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

