


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080119\
Data File : VN057022.D
Acq On : 1 Aug 2019 8:19
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Title : SW846 8260
Last Update : Sat Jul 27 01:33:29 2019

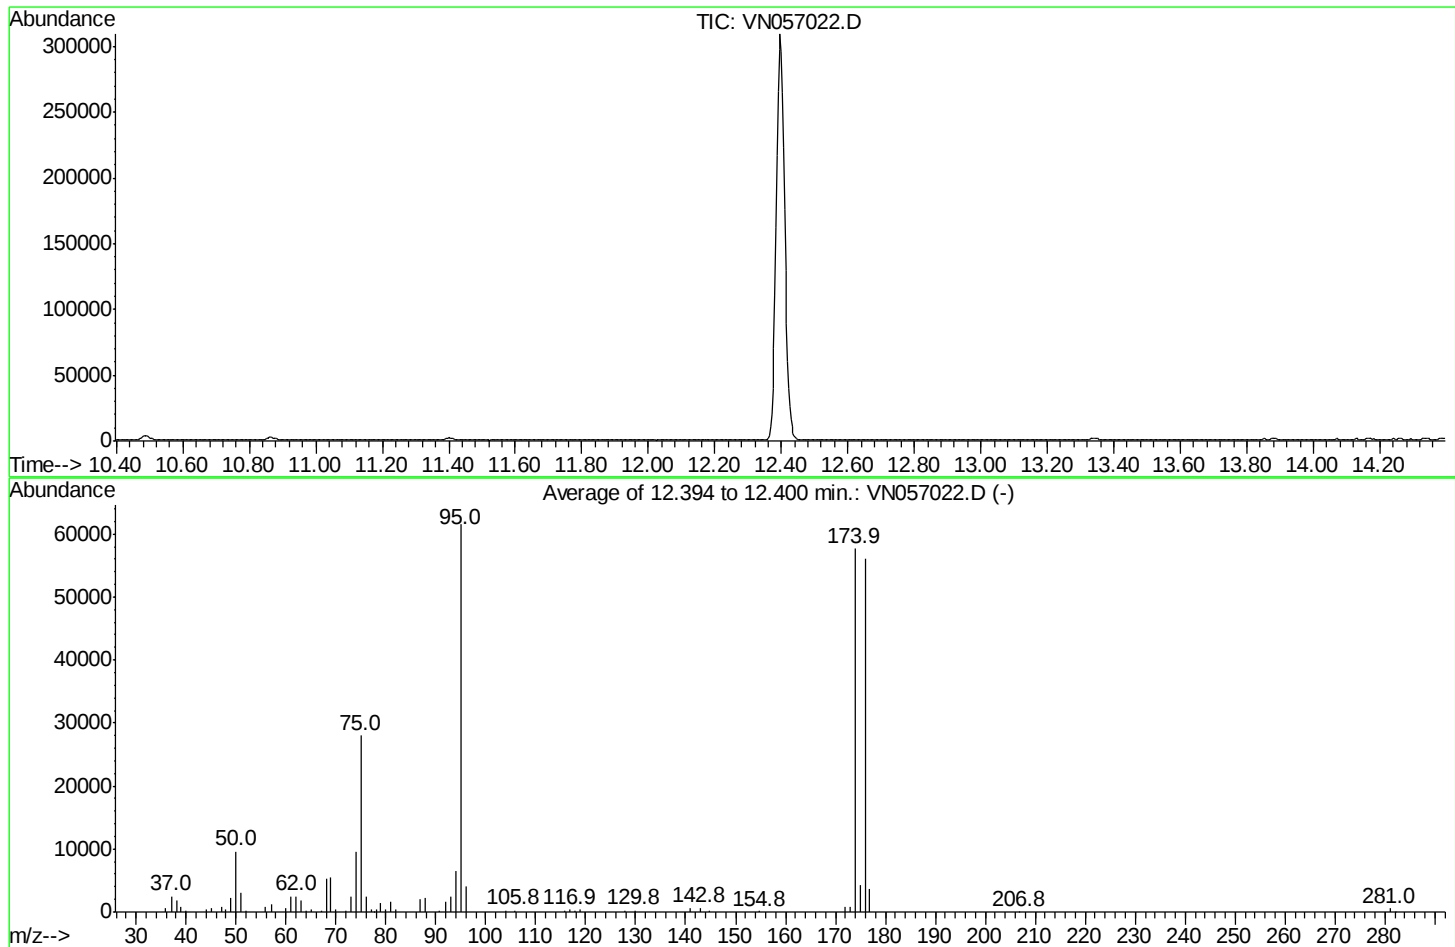

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9602	PASS
75	95	30	60	45.5	27970	PASS
95	95	100	100	100.0	61530	PASS
96	95	5	9	6.6	4051	PASS
173	174	0.00	2	1.4	802	PASS
174	95	50	100	93.8	57698	PASS
175	174	5	9	7.5	4305	PASS
176	174	95	101	97.2	56058	PASS
177	176	5	9	6.6	3672	PASS