


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN080122\  
Data File : VN073651.D  
Acq On : 01 Aug 2022 10:52  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N072822W.M  
Title : SW846 8260  
Last Update : Fri Jul 29 02:20:25 2022

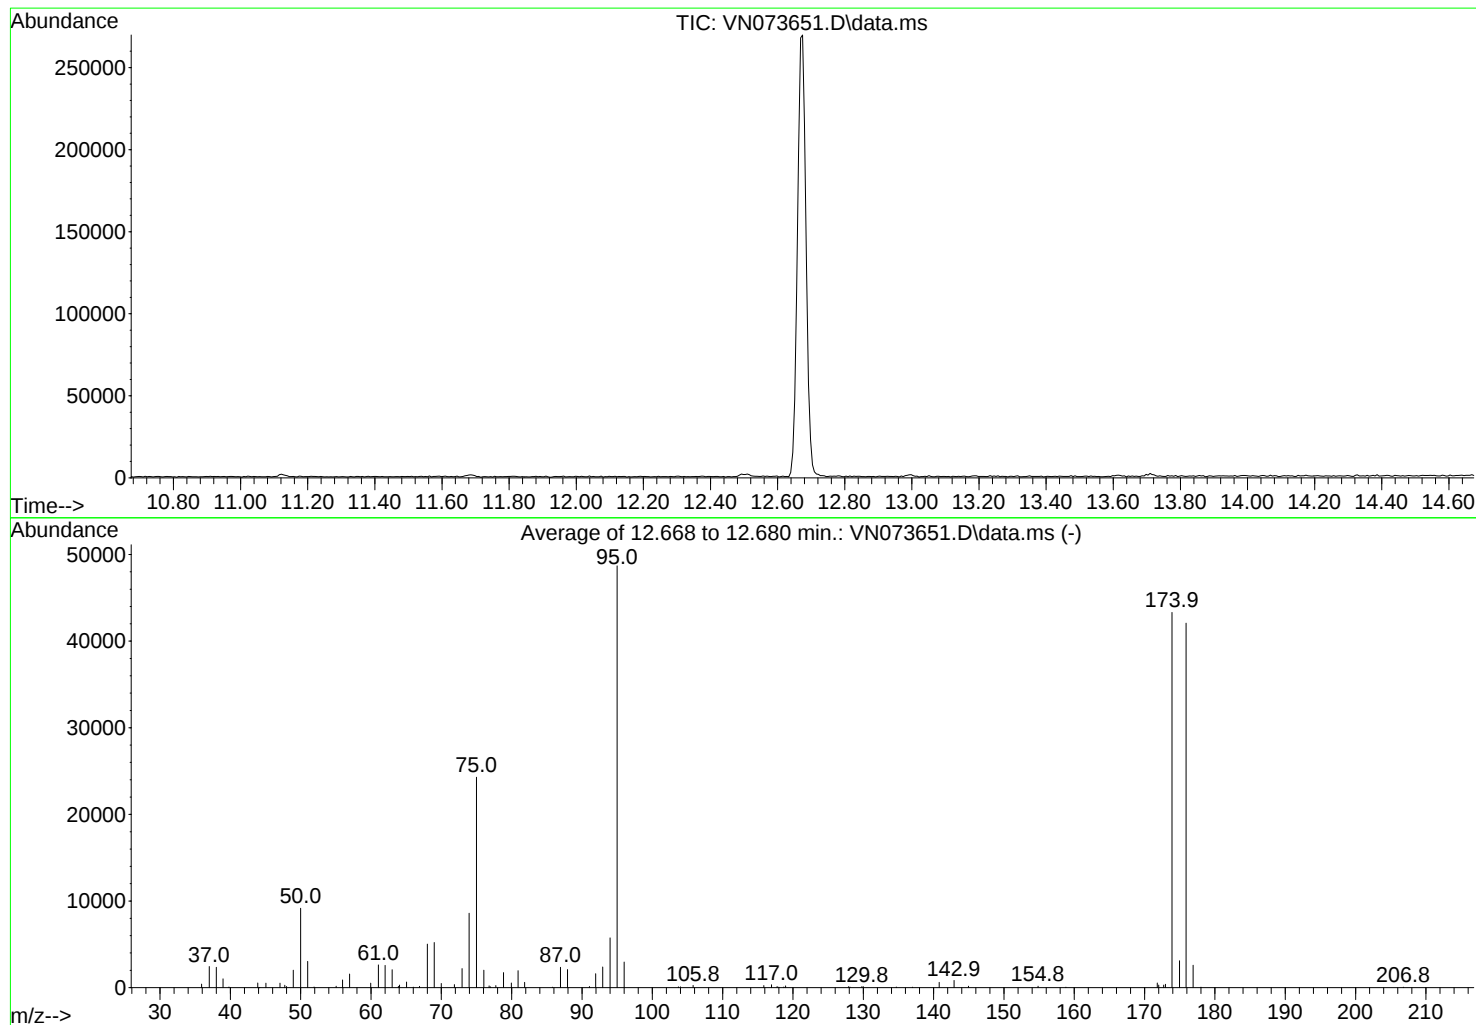

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1825

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.8         | 9167       | PASS                |
| 75             | 95              | 30              | 60              | 49.9         | 24291      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 48693      | PASS                |
| 96             | 95              | 5               | 9               | 6.1          | 2961       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.9          | 380        | PASS                |
| 174            | 95              | 50              | 100             | 89.0         | 43323      | PASS                |
| 175            | 174             | 5               | 9               | 7.2          | 3111       | PASS                |
| 176            | 174             | 95              | 101             | 97.1         | 42075      | PASS                |
| 177            | 176             | 5               | 9               | 6.2          | 2595       | PASS                |