
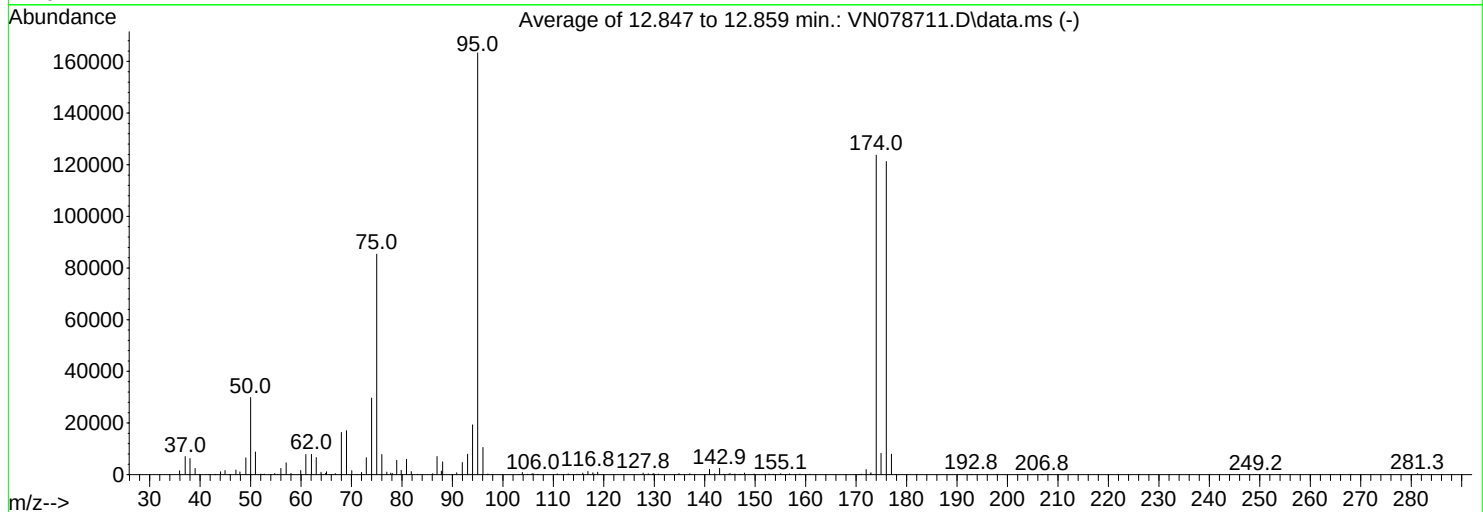


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080123\
Data File : VN078711.D
Acq On : 01 Aug 2023 12:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080123W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Aug 02 04:51:47 2023

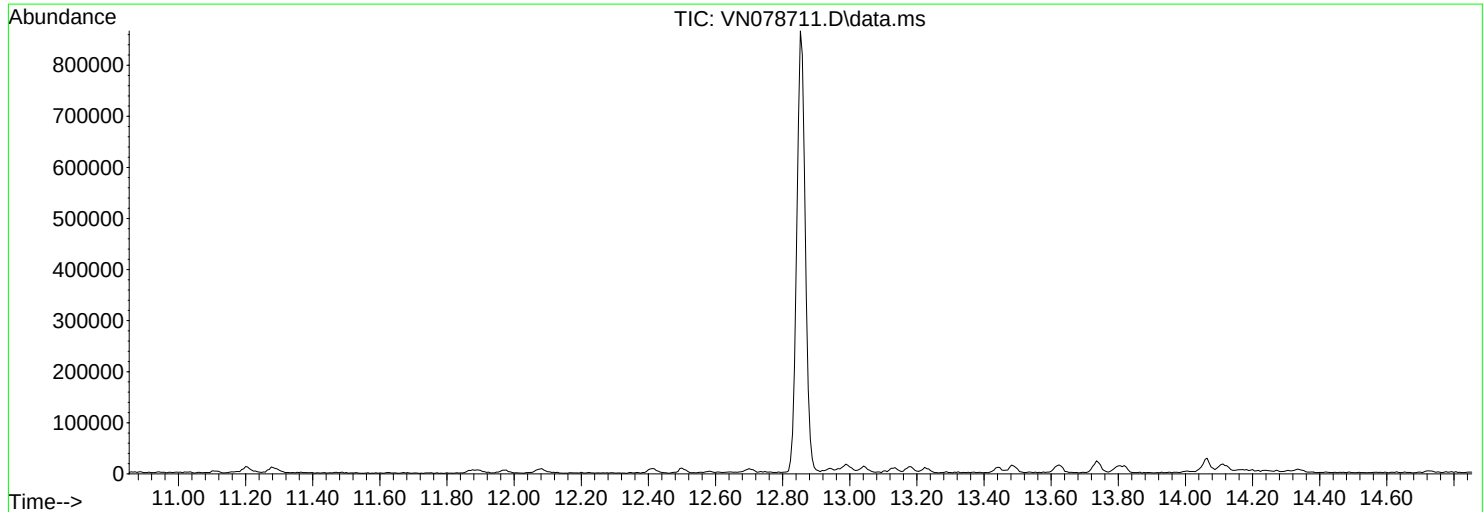

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	29861	PASS
75	95	30	60	52.3	85403	PASS
95	95	100	100	100.0	163328	PASS
96	95	5	9	6.4	10526	PASS
173	174	0.00	2	0.6	759	PASS
174	95	50	100	75.8	123731	PASS
175	174	5	9	6.6	8218	PASS
176	174	95	101	98.0	121248	PASS
177	176	5	9	6.5	7916	PASS