

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080218\
 Data File : VN050301.D
 Acq On : 3 Aug 2018 7:31
 Operator : MD\SY
 Sample : J4303-08
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-A04

Quant Time: Aug 03 08:19:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 26 18:10:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	690150	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1131513	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	947872	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	371736	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	474395	49.27	ug/l	0.00
Spiked Amount			Recovery	=	98.54%	
35) Dibromofluoromethane	7.59	113	427759	46.30	ug/l	0.00
Spiked Amount			Recovery	=	92.60%	
50) Toluene-d8	10.09	98	1532338	45.12	ug/l	0.00
Spiked Amount			Recovery	=	90.24%	
62) 4-Bromofluorobenzene	12.40	95	440180	39.36	ug/l	0.00
Spiked Amount			Recovery	=	78.72%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.06	50	3150	0.29	ug/l	# 86
5) Bromomethane	2.56	94	254	Below	Cal	99
8) Diethyl Ether	3.41	74	2500	0.51	ug/l	82
11) Tert butyl alcohol	4.78	59	182	0.26	ug/l	# 72
16) Acetone	3.83	43	12264	1.08	ug/l	95
18) Methyl Acetate	4.33	43	16440	0.24	ug/l	99
20) Methylene Chloride	4.55	84	1306	Below	Cal	# 85
31) Cyclohexane	7.66	56	12610	0.88	ug/l	# 1
36) 1,1-Dichloropropene	7.67	75	48009	3.77	ug/l	# 48
38) Carbon Tetrachloride	7.67	117	62072	4.59	ug/l	# 16
43) Isopropyl Acetate	8.27	43	294294	16.81	ug/l	# 61
56) Ethyl methacrylate	10.44	69	2058	2.19	ug/l	# 1
59) 2-Hexanone	10.77	43	300	5.22	ug/l	# 24
70) Styrene	11.96	104	31	0.92	ug/l	# 1
71) Bromoform	12.40	173	1502	0.22	ug/l	# 1
75) 1,1,2,2-Tetrachloroethane	12.49	83	233	Below	Cal	# 25
76) 1,2,3-Trichloropropane	12.40	75	214347	31.03	ug/l	# 100
81) trans-1,4-Dichloro-2-buten	12.40	75	214347	98.41	ug/l	# 13
86) p-Isopropyltoluene	13.44	119	5864	0.26	ug/l	# 84
92) 1,2-Dibromo-3-Chloropropan	14.44	75	59	Below	Cal	# 1
95) Naphthalene	15.10	128	1563	4.50	ug/l	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080218\
Data File : VN050301.D
Acq On : 3 Aug 2018 7:31
Operator : MD\SY
Sample : J4303-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-A04

Quant Time: Aug 03 08:19:06 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 26 18:10:10 2018
Response via : Initial Calibration

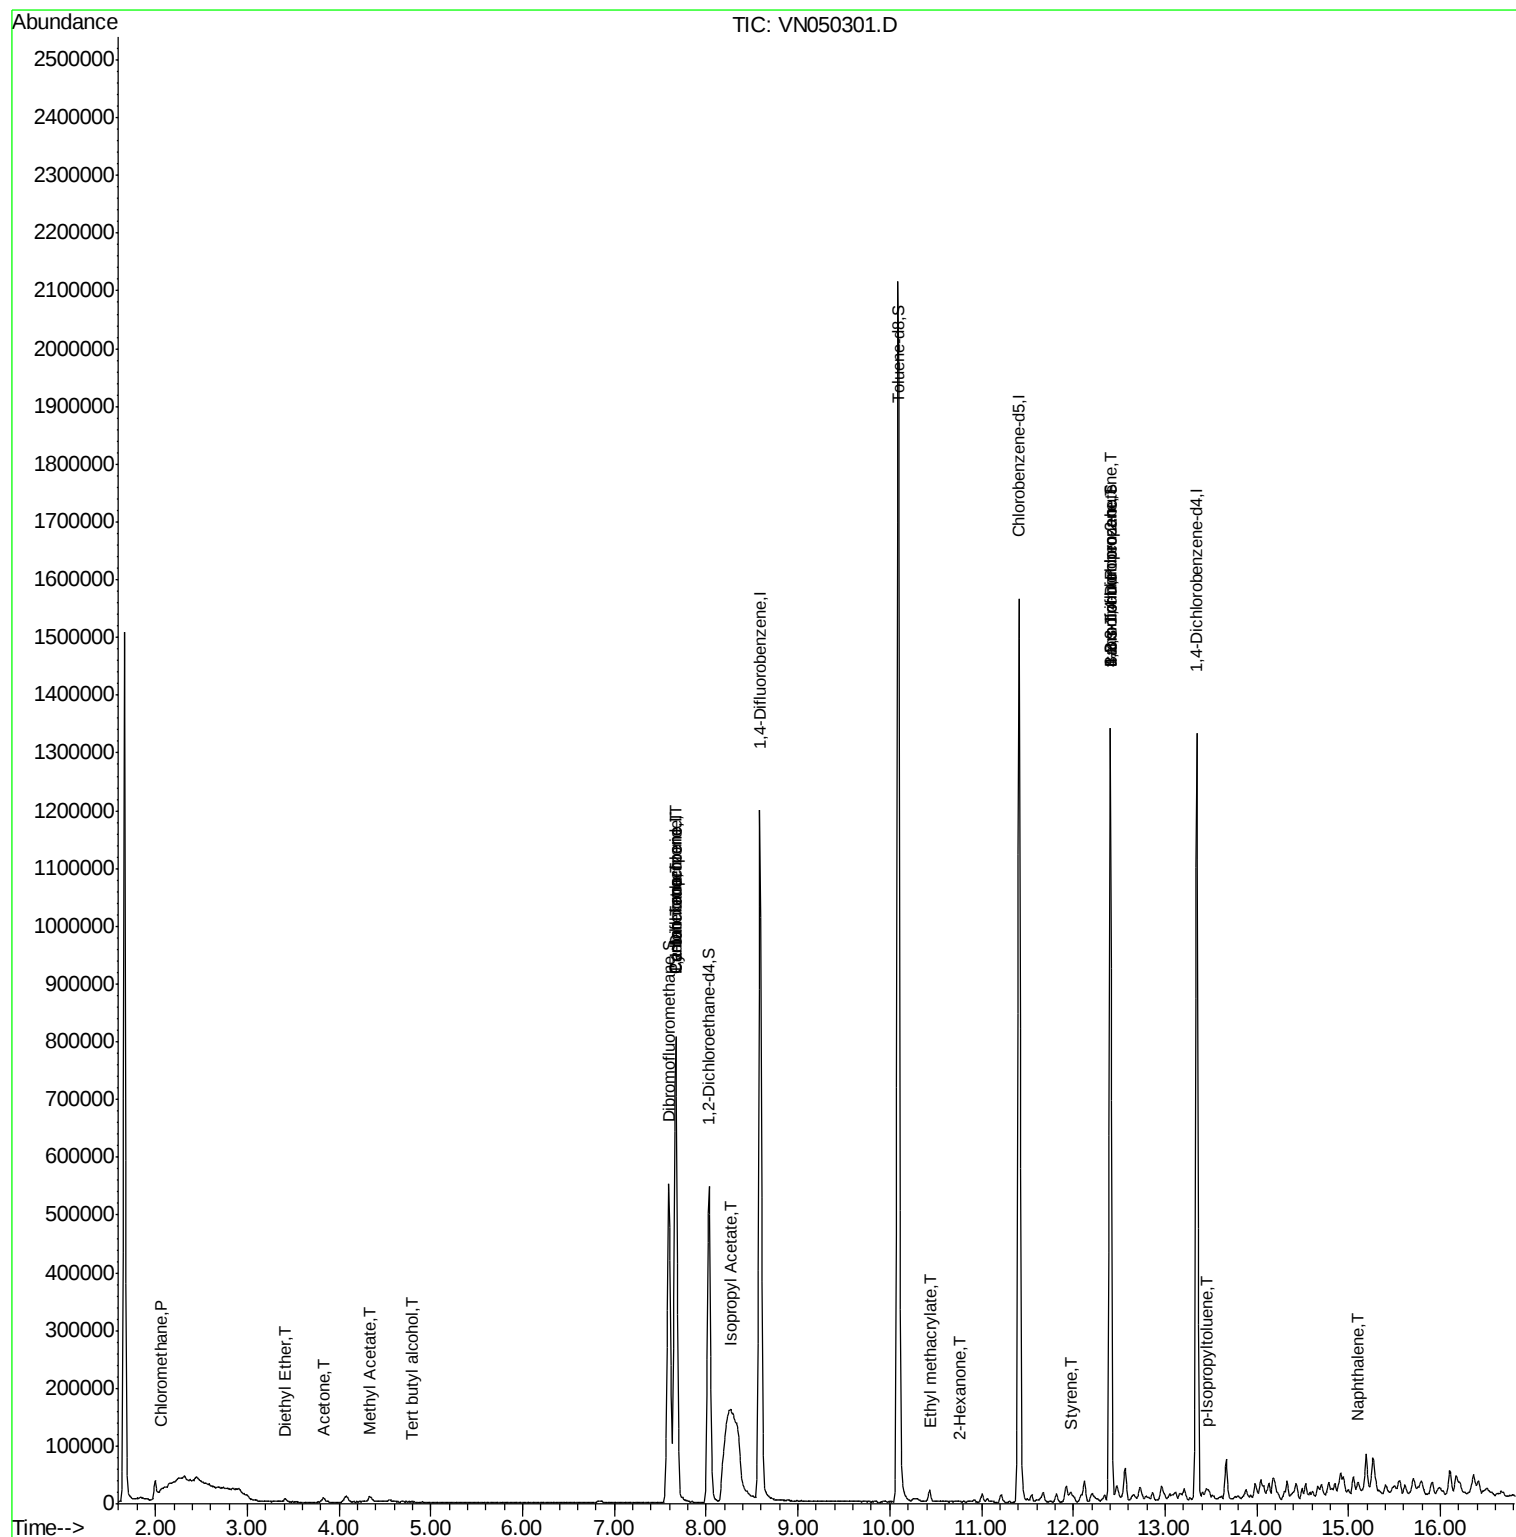

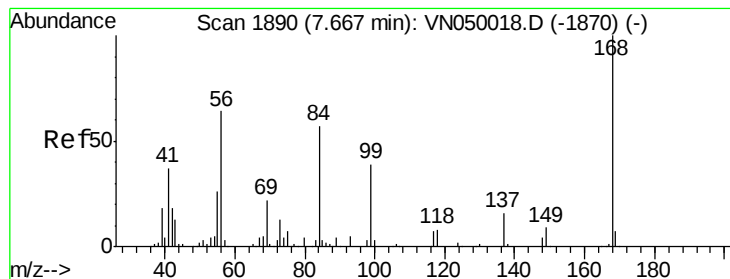

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31

Instrument :

MSVOA_N

ClientSampleId :


MW-A04

Tot Ion:168 Resp: 690150

Ion Ratio Lower Upper

168 100

99 52.0 40.0 60.0



Abundance Ion 167.90 (167.60 to 168.60): VN050018.D (-1870) (-)

Ion 98.90 (98.60 to 99.60): VN050018.D (-1870) (-)

7.67



300000

200000

100000

0

Time-->



#3

Chloromethane

Concen: 0.29 ug/l

RT: 2.06 min Scan# 145

Delta R.T. 0.00 min

Lab File: VN050301.D


Acq: 3 Aug 2018 7:31

Tgt Ion: 50 Resp: 3150

Ion Ratio Lower Upper

50 100

52 40.3 25.9 38.9#



Abundance Ion 49.90 (49.60 to 50.60): VN050018.D (-133) (-)

Ion 51.90 (51.60 to 52.60): VN050018.D (-133) (-)

2.06


1500


1000

500

0

Time-->



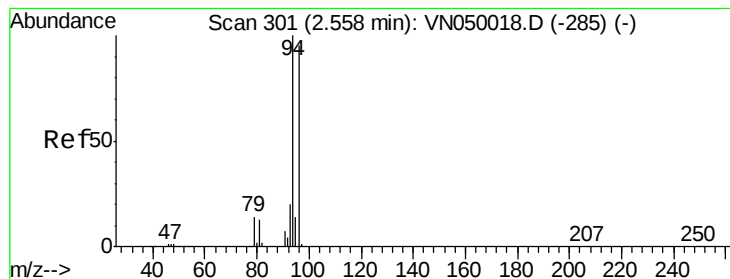

#5

Bromomethane

Concen: Below Cal

RT: 2.56 min Scan# 302

Delta R.T. 0.01 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31

Instrument :

MSVOA_N

ClientSampleId :


MW-A04

Tot Ion: 94 Resp: 254

Ion Ratio Lower Upper

94 100

96 94.3 74.6 112.0



Abundance Ion 93.90 (93.60 to 94.60): VN0

Ion 95.90 (95.60 to 96.60): VN0

250

200

150


100

50


0

2.54 2.55 2.56 2.57

2.56



Time-->



#8

Diethyl Ether

Concen: 0.51 ug/l

RT: 3.41 min Scan# 567

Delta R.T. 0.00 min

Lab File: VN050301.D


Acq: 3 Aug 2018 7:31

Tgt Ion: 74 Resp: 2500

Ion Ratio Lower Upper

74 100

45 112.3 47.6 142.8



Abundance Ion 74.00 (73.70 to 74.70): VN0

Ion 45.00 (44.70 to 45.70): VN0

1500


1000

500


0

3.35 3.40 3.45

3.41



Time-->




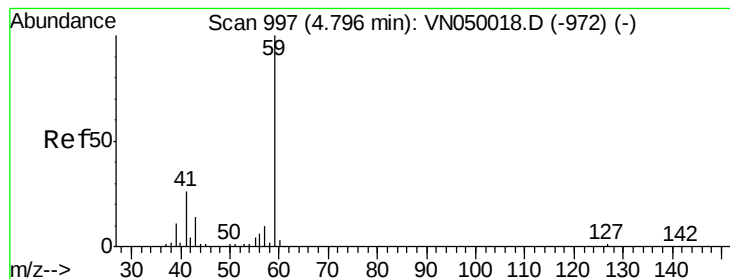


#11

Tert butyl alcohol
 Concen: 0.26 ug/l
 RT: 4.78 min Scan# 992
 Delta R.T. -0.03 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-A04




Tot Ion: 59 Resp: 182
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.5 12.7#

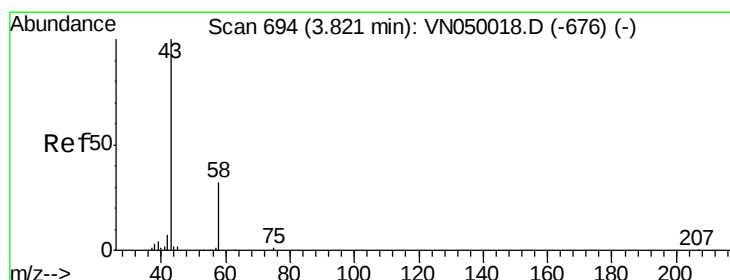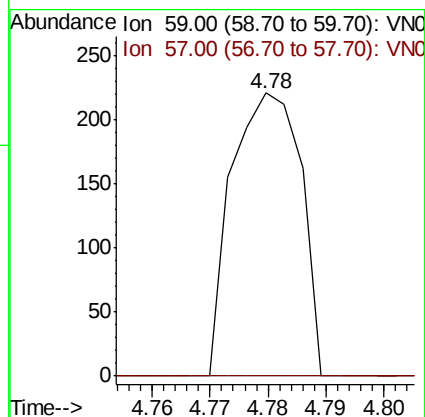


#16

Acetone
 Concen: 1.08 ug/l
 RT: 3.83 min Scan# 696
 Delta R.T. 0.00 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31

Tgt Ion: 43 Resp: 12264
 Ion Ratio Lower Upper
 43 100
 58 35.1 25.8 38.8



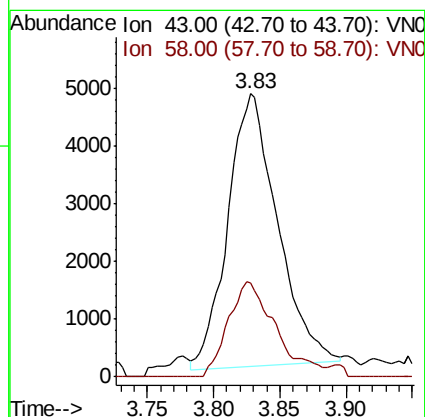





#18
Methyl Acetate
Concen: 0.24 ug/l
RT: 4.33 min Scan# 853
Delta R.T. 0.00 min
Lab File: VN050301.D
Acq: 3 Aug 2018 7:31




Instrument :
MSVOA_N
ClientSampled :
MW-A04


Tot Ion: 43 Resp: 16440
Ion Ratio Lower Upper
43 100
74 23.5 19.2 28.8

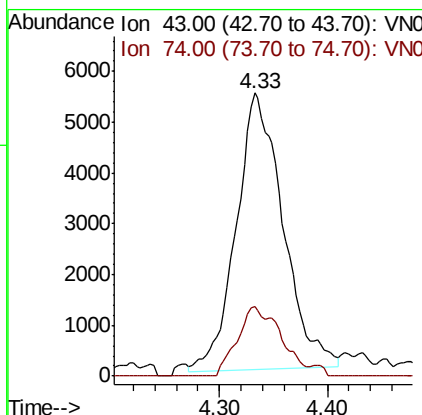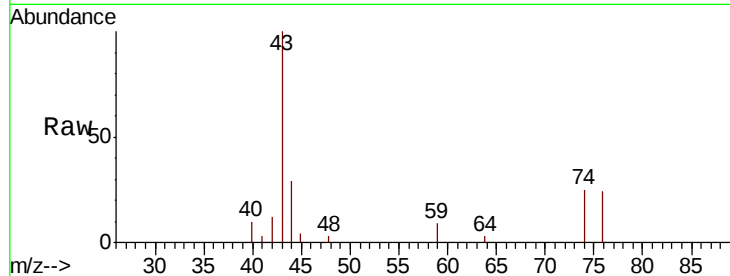

#20
Methylene Chloride
Concen: Below Cal
RT: 4.55 min Scan# 921
Delta R.T. 0.00 min
Lab File: VN050301.D
Acq: 3 Aug 2018 7:31

Tgt Ion: 84 Resp: 1306
Ion Ratio Lower Upper
84 100
49 99.8 94.8 142.2
51 52.1 28.3 42.5#
86 67.7 51.0 76.6

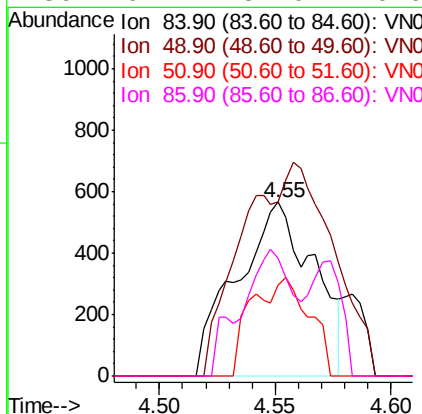

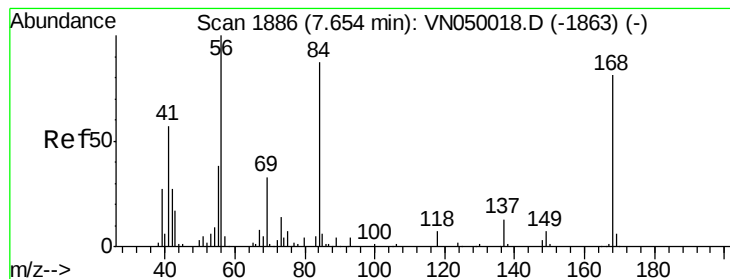

#31

Cyclohexane

Concen: 0.88 ug/l

RT: 7.66 min Scan# 1889

Delta R.T. 0.01 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31

Instrument :

MSVOA_N

ClientSampled :

MW-A04


Tot Ion: 56 Resp: 12610

Ion Ratio Lower Upper

56 100

69 187.0 26.2 39.4#




84 147.9 67.4 101.0#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

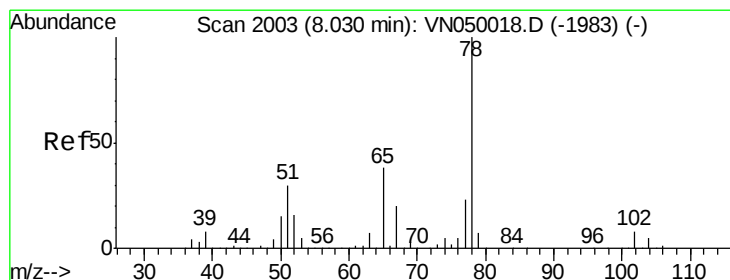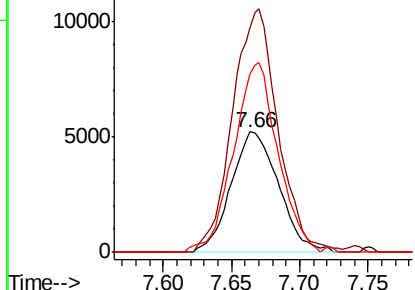

#33

1,2-Dichloroethane-d4

Concen: 49.27 ug/l

RT: 8.03 min Scan# 2003

Delta R.T. 0.00 min

Lab File: VN050301.D


Acq: 3 Aug 2018 7:31

Tgt Ion: 65 Resp: 474395

Ion Ratio Lower Upper



65 100


67 53.5 0.0 108.4



Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0




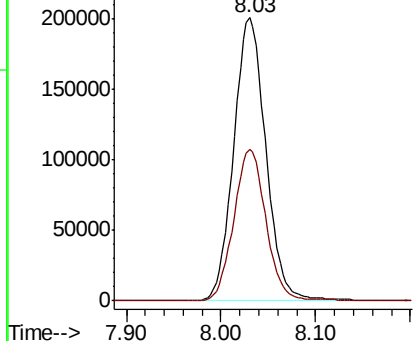




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2177
 Delta R.T. 0.00 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-A04


Tot Ion:114 Resp: 1131513
 Ion Ratio Lower Upper
 114 100
 63 20.1 0.0 40.0
 88 15.1 0.0 31.2

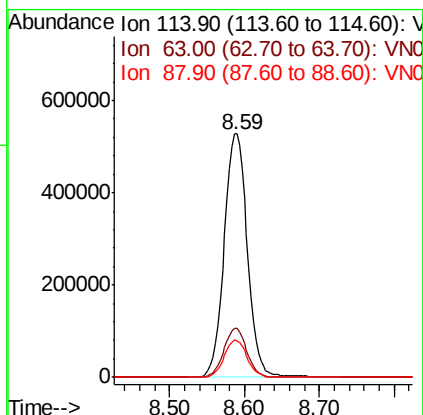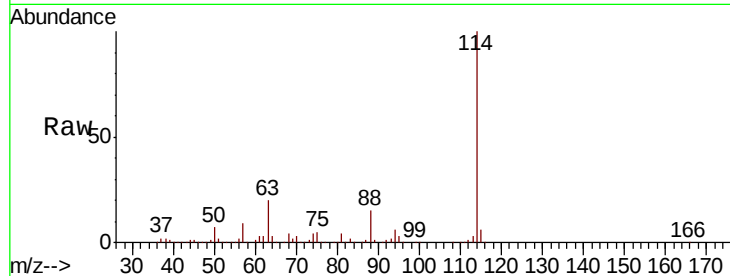

#35
 Dibromofluoromethane
 Concen: 46.30 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. 0.00 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31

Tgt Ion:113 Resp: 427759
 Ion Ratio Lower Upper
 113 100
 111 103.0 80.7 121.1
 192 22.5 17.8 26.6


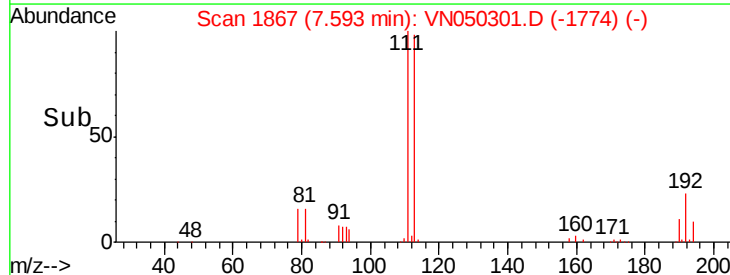
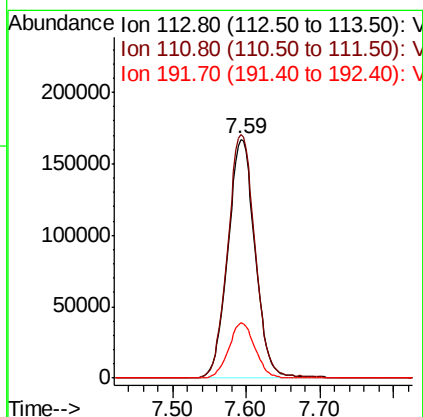



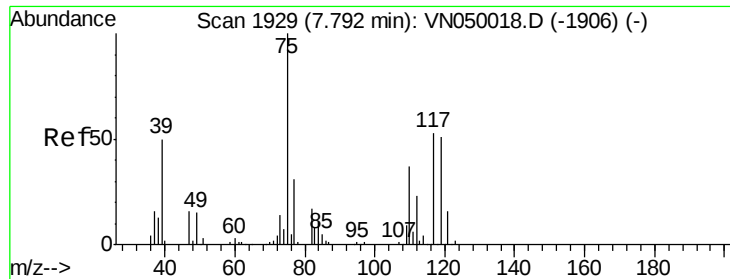

#36
 1,1-Dichloropropene
 Concen: 3.77 ug/l
 RT: 7.67 min Scan# 1890
 Delta R.T. -0.13 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31




Instrument :
 MSVOA_N
 ClientSampled :
 MW-A04


Tot Ion: 75 Resp: 48009
 Ion Ratio Lower Upper
 75 100
 110 8.9 18.4 55.2#
 77 0.0 25.3 37.9#

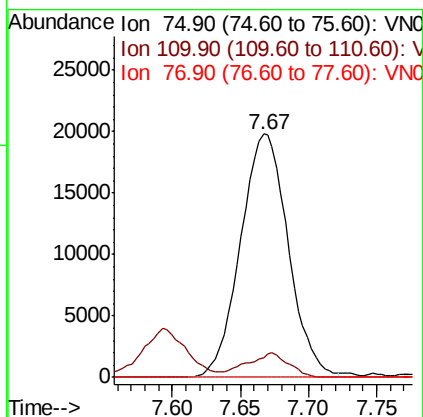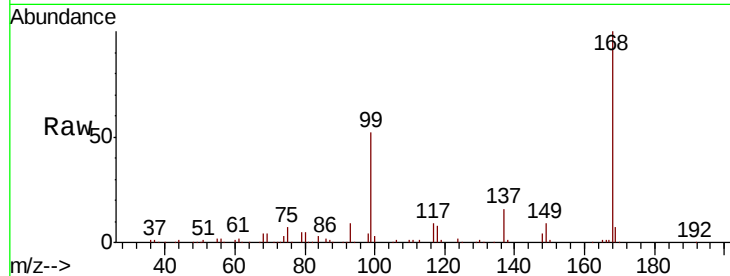

#38
 Carbon Tetrachloride
 Concen: 4.59 ug/l
 RT: 7.67 min Scan# 1890
 Delta R.T. -0.11 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31

Tgt Ion: 117 Resp: 62072
 Ion Ratio Lower Upper
 117 100
 119 6.0 77.4 116.0#
 121 0.0 23.9 35.9#

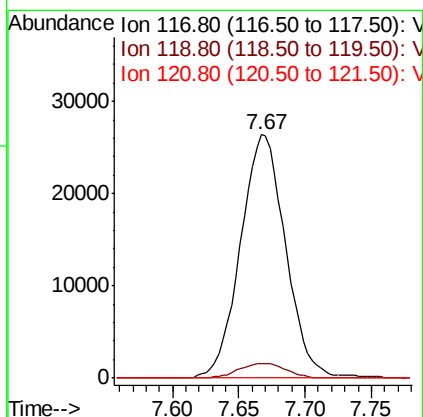




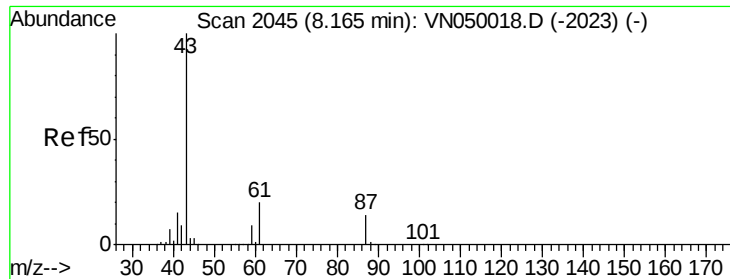


#43

Isopropyl Acetate
 Concen: 16.81 ug/l
 RT: 8.27 min Scan# 2077
 Delta R.T. 0.10 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-A04




Tot Ion: 43 Resp: 294294
 Ion Ratio Lower Upper
 43 100
 61 0.1 15.8 23.6#
 87 0.0 10.3 15.5#

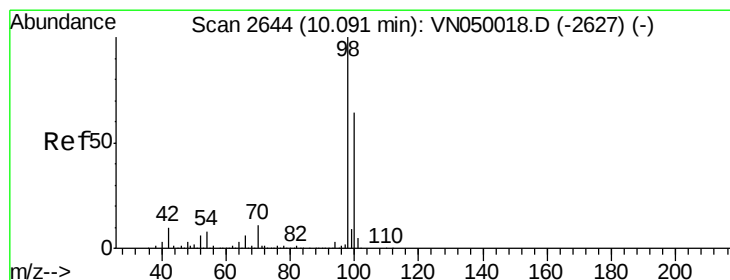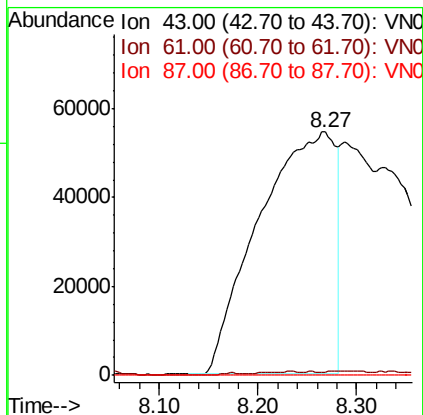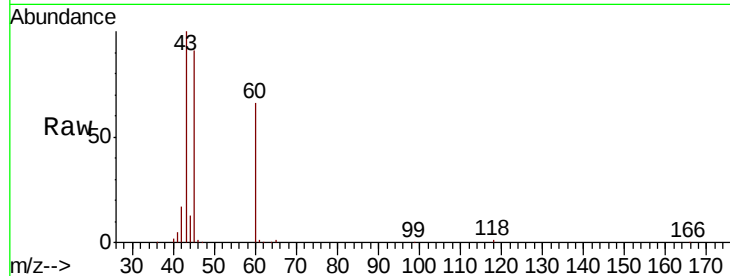


#50

Toluene-d8
 Concen: 45.12 ug/l
 RT: 10.09 min Scan# 2644
 Delta R.T. -0.00 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31

Tgt Ion: 98 Resp: 1532338
 Ion Ratio Lower Upper
 98 100
 100 63.4 50.7 76.1

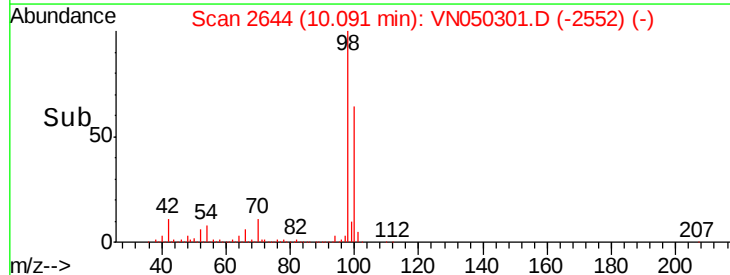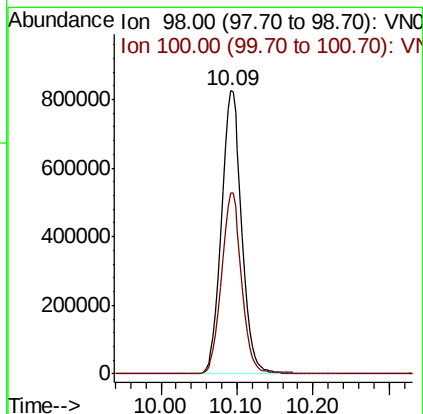

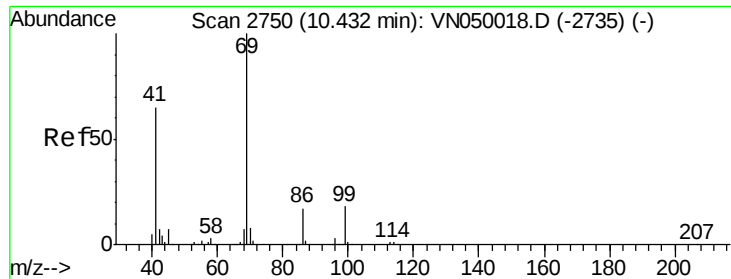

#56

Ethyl methacrylate

Concen: 2.19 ug/l

RT: 10.44 min Scan# 2752

Delta R.T. 0.01 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31

Instrument :

MSVOA_N

ClientSampled :

MW-A04


Tot Ion: 69 Resp: 2058

Ion Ratio Lower Upper

69 100

41 156.3 51.0 76.4#


39 89.8 26.6 40.0#

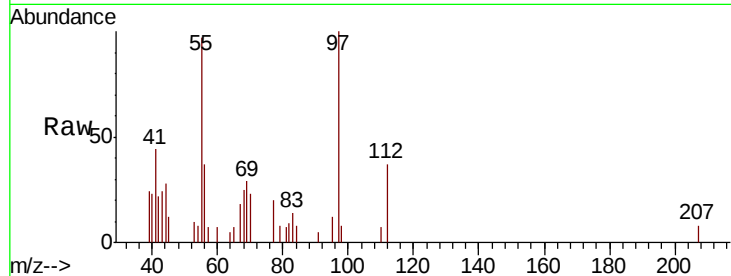



Abundance Ion 69.00 (68.70 to 69.70): VN050018.D (-2735) (-)

Ion 41.00 (40.70 to 41.70): VN050018.D (-2735) (-)

Ion 39.00 (38.70 to 39.70): VN050018.D (-2735) (-)

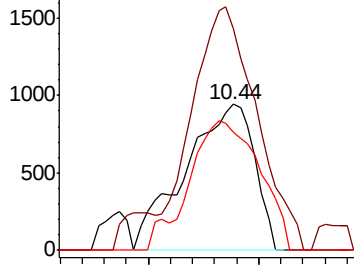

Time-->

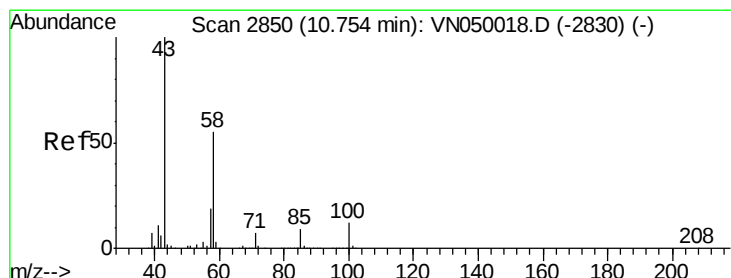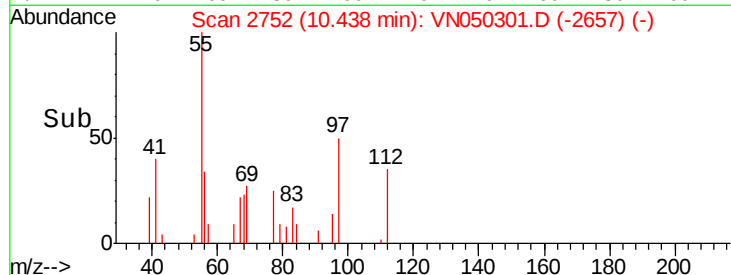

#59

2-Hexanone

Concen: 5.22 ug/l

RT: 10.77 min Scan# 2854

Delta R.T. 0.01 min

Lab File: VN050301.D


Acq: 3 Aug 2018 7:31

Tgt Ion: 43 Resp: 300

Ion Ratio Lower Upper

43 100

58 0.0 27.6 82.7#

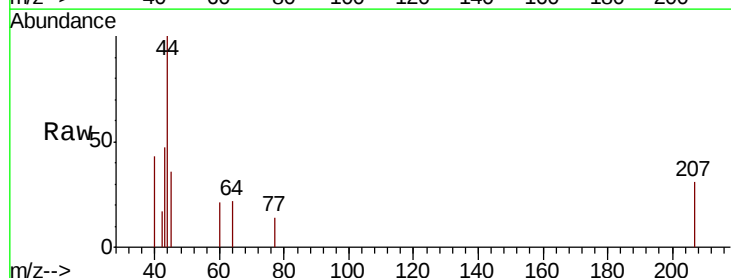

Abundance Ion 43.00 (42.70 to 43.70): VN050018.D (-2830) (-)

Ion 58.00 (57.70 to 58.70): VN050018.D (-2830) (-)

Ion 41.00 (40.70 to 41.70): VN050018.D (-2830) (-)

Ion 39.00 (38.70 to 39.70): VN050018.D (-2830) (-)

Ion 37.00 (36.70 to 37.70): VN050018.D (-2830) (-)

Ion 35.00 (34.70 to 35.70): VN050018.D (-2830) (-)

Ion 33.00 (32.70 to 33.70): VN050018.D (-2830) (-)

Ion 31.00 (30.70 to 31.70): VN050018.D (-2830) (-)

Ion 29.00 (28.70 to 29.70): VN050018.D (-2830) (-)

Ion 27.00 (26.70 to 27.70): VN050018.D (-2830) (-)

Ion 25.00 (24.70 to 25.70): VN050018.D (-2830) (-)

Ion 23.00 (22.70 to 23.70): VN050018.D (-2830) (-)

Ion 21.00 (20.70 to 21.70): VN050018.D (-2830) (-)

Ion 19.00 (18.70 to 19.70): VN050018.D (-2830) (-)

Ion 17.00 (16.70 to 17.70): VN050018.D (-2830) (-)

Ion 15.00 (14.70 to 15.70): VN050018.D (-2830) (-)

Ion 13.00 (12.70 to 13.70): VN050018.D (-2830) (-)

Ion 11.00 (10.70 to 11.70): VN050018.D (-2830) (-)

Ion 9.00 (8.70 to 9.70): VN050018.D (-2830) (-)

Ion 7.00 (6.70 to 7.70): VN050018.D (-2830) (-)

Ion 5.00 (4.70 to 5.70): VN050018.D (-2830) (-)

Ion 3.00 (2.70 to 3.70): VN050018.D (-2830) (-)

Ion 1.00 (0.70 to 1.70): VN050018.D (-2830) (-)

Ion 0.00 (0.00 to 0.00): VN050018.D (-2830) (-)

Ion 0.00 (0.00 to 0.00): VN050018.D (-2830) (-)

Ion 0.00 (0.00 to 0.00): VN050018.D (-2830) (-)

Ion 0.00 (0.00 to 0.00): VN050018.D (-2830) (-)



Ion 0.00 (0.00 to 0.00): VN050018.D (-2830) (-)

Ion 0.00 (0.00 to 0.00): VN050018.D (-2830) (-)


Ion 0.00 (0.00 to 0.00): VN050018.D (-2830) (-)

Ion 0.00 (0.00 to 0.00): VN050018.D (-2830) (-)

Ion 0.00 (0.00 to 0.00): VN050018.D (-2830) (-)

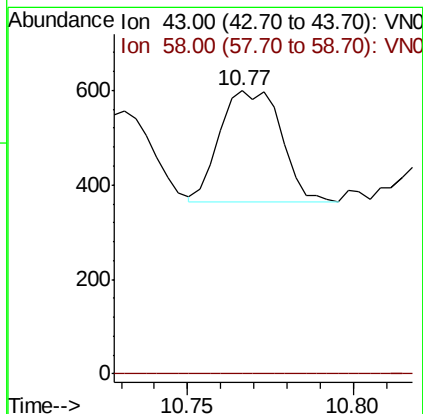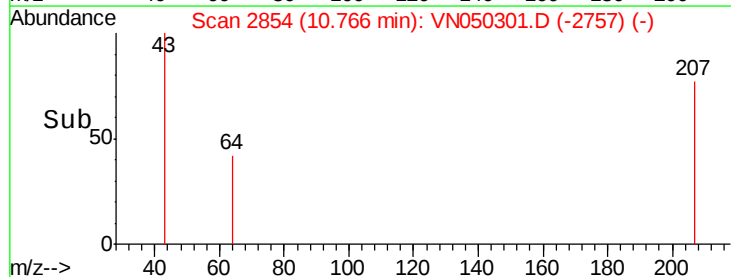

Time-->

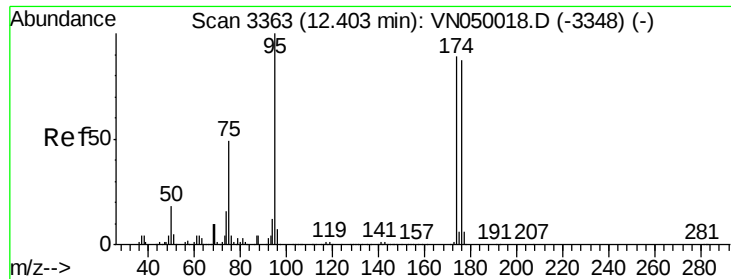

#62

4-Bromofluorobenzene

Concen: 39.36 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31

Instrument :

MSVOA_N

ClientSampleId :

MW-A04


Tot Ion: 95 Resp: 440180

Ion Ratio Lower Upper

95 100

174 91.1 0.0 178.2

176 88.3 0.0 173.4

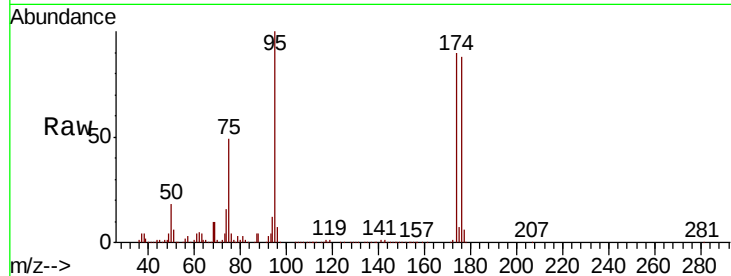


Abundance Ion 94.90 (94.60 to 95.60): VN050018.D (-3348) (-)

Ion 173.80 (173.50 to 174.50): VN050018.D (-3348) (-)

Ion 175.80 (175.50 to 176.50): VN050018.D (-3348) (-)

Time-->

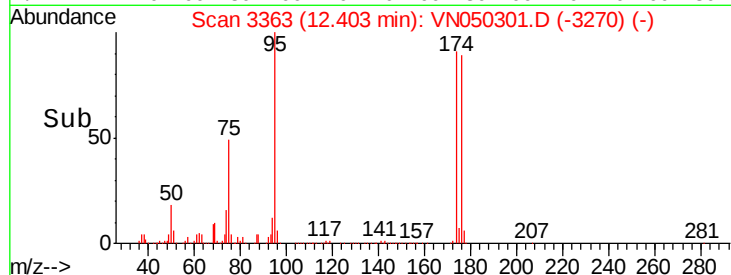


Abundance Ion 94.90 (94.60 to 95.60): VN050301.D (-3270) (-)

Ion 173.80 (173.50 to 174.50): VN050301.D (-3270) (-)

Ion 175.80 (175.50 to 176.50): VN050301.D (-3270) (-)

Time-->

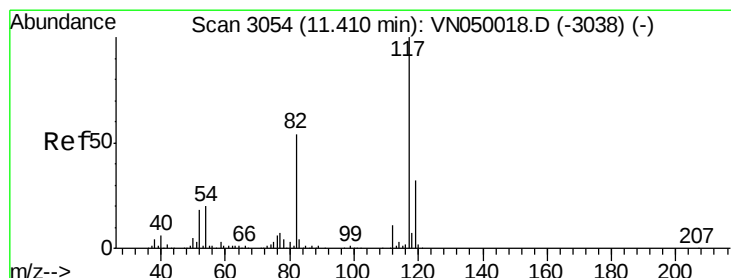

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.41 min Scan# 3054

Delta R.T. 0.00 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31


Tgt Ion: 117 Resp: 947872

Ion Ratio Lower Upper

117 100

82 53.7 43.7 65.5

119 32.4 26.1 39.1

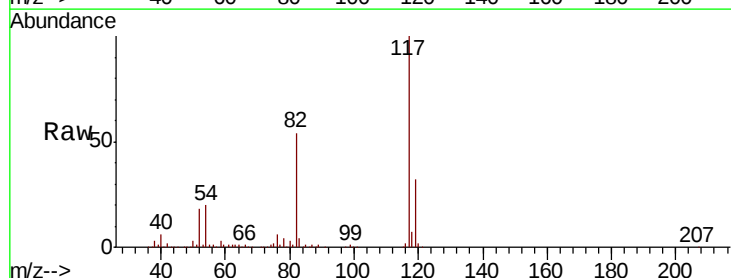


Abundance Ion 116.90 (116.60 to 117.60): VN050018.D (-3038) (-)

Ion 82.00 (81.70 to 82.70): VN050018.D (-3038) (-)

Ion 118.90 (118.60 to 119.60): VN050018.D (-3038) (-)

Time-->

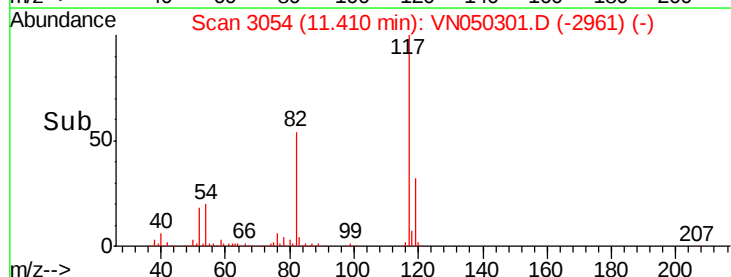


Abundance Ion 116.90 (116.60 to 117.60): VN050301.D (-2961) (-)

Ion 82.00 (81.70 to 82.70): VN050301.D (-2961) (-)

Ion 118.90 (118.60 to 119.60): VN050301.D (-2961) (-)


Time-->






#70
Stvrene
Concen: 0.92 ug/l
RT: 11.96 min Scan# 3226
Delta R.T. -0.00 min
Lab File: VN050301.D
Acq: 3 Aug 2018 7:31

Instrument :
MSVOA_N
ClientSampleId :
MW-A04

Tot Ion:104 Resp: 31
Ion Ratio Lower Upper
104 100
78 441.9 39.3 58.9#
103 0.0 45.0 67.6#

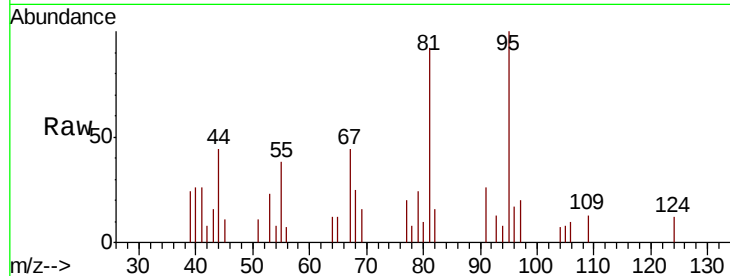


Abundance Ion 104.00 (103.70 to 104.70): V
Ion 78.00 (77.70 to 78.70): VN
Ion 103.00 (102.70 to 103.70): V

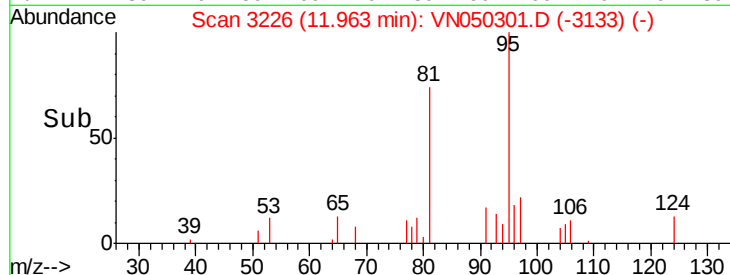
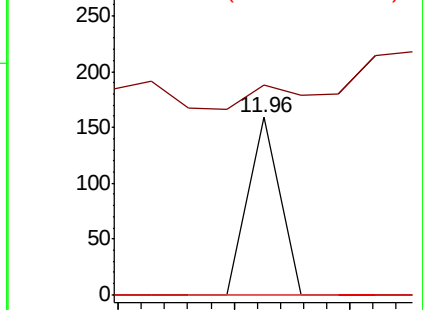



#71
Bromoform
Concen: 0.22 ug/l
RT: 12.40 min Scan# 3362
Delta R.T. 0.27 min
Lab File: VN050301.D
Acq: 3 Aug 2018 7:31

Tgt Ion:173 Resp: 1502
Ion Ratio Lower Upper
173 100
175 1727.8 24.1 72.2#
254 0.0 0.2 0.2#



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

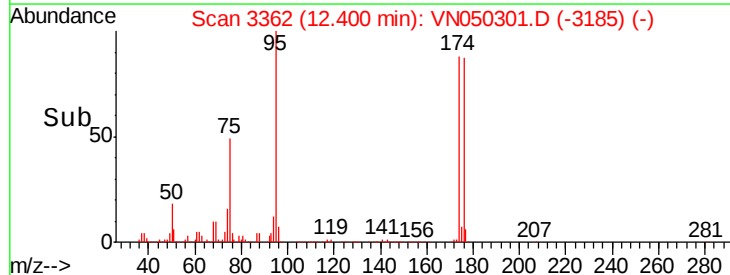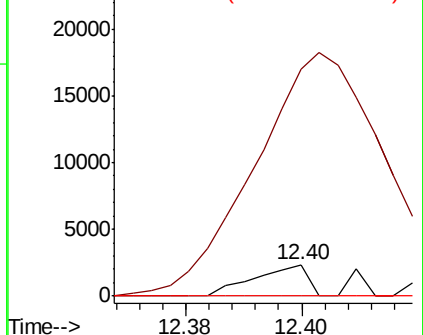

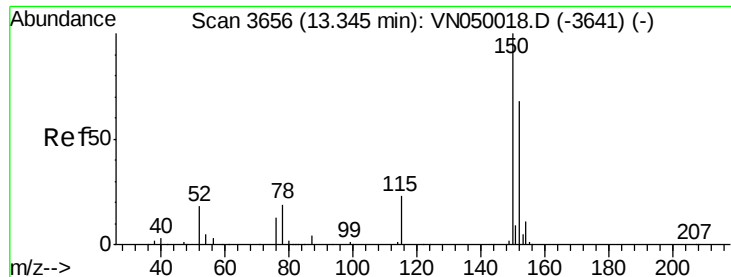

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.35 min Scan# 3656

Delta R.T. 0.00 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31

Instrument :

MSVOA_N

ClientSampleId :

MW-A04


Tot Ion:152 Resp: 371736

Ion Ratio Lower Upper

152 100

115 55.7 27.8 83.3




150 157.9 0.0 348.6

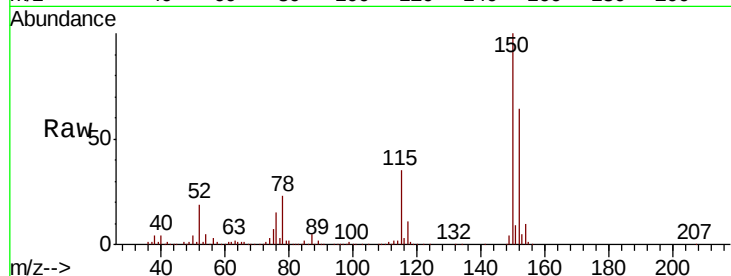

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

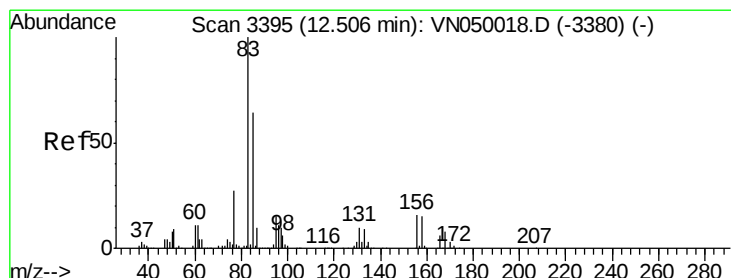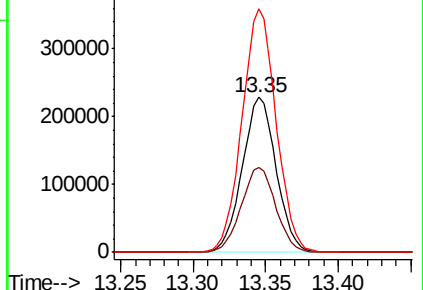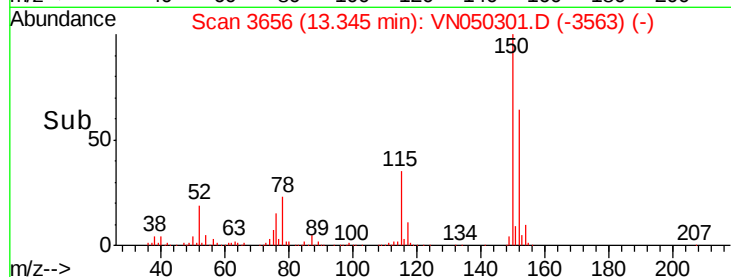

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.49 min Scan# 3389

Delta R.T. -0.02 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31


Tgt Ion: 83 Resp: 233

Ion Ratio Lower Upper

83 100

131 0.0 5.1 15.3#



85 0.0 32.3 96.8#

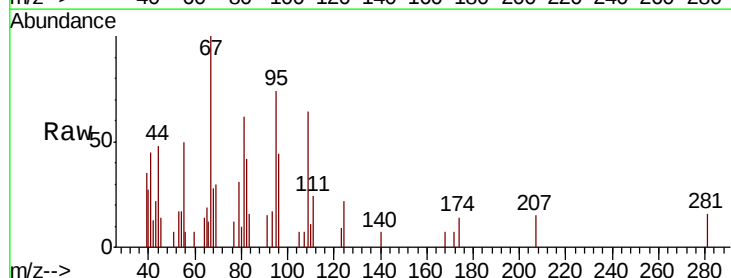


Abundance Ion 82.90 (82.60 to 83.60): V

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): V

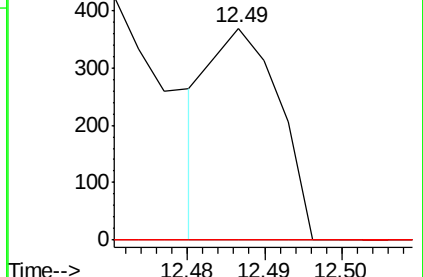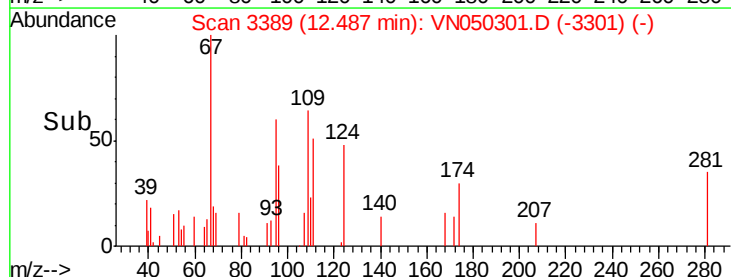



#76

1,2,3-Trichloropropane

Concen: 31.03 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. -0.15 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31

Instrument :

MSVOA_N

ClientSampleId :





MW-A04

Tot Ion: 75 Resp: 214347

Ion Ratio Lower Upper

75 100

77 1.4 0.0 0.0#

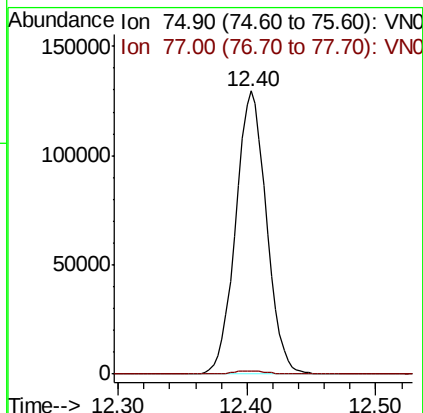

#81

trans-1,4-Dichloro-2-butene

Concen: 98.41 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.10 min

Lab File: VN050301.D

Acq: 3 Aug 2018 7:31




Tgt Ion: 75 Resp: 214347


Ion Ratio Lower Upper

75 100

53 0.3 73.5 110.3#

89 0.0 36.0 54.0#


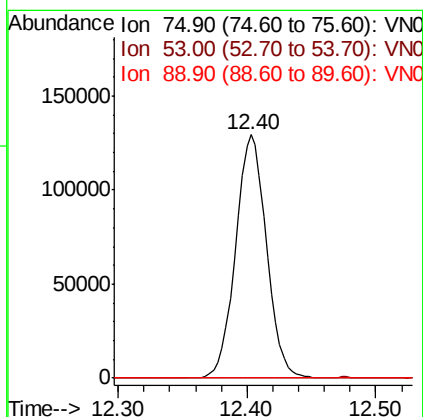




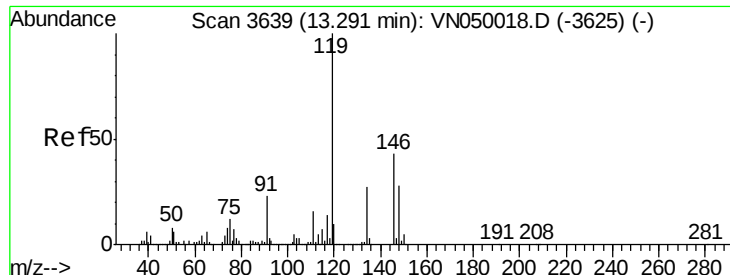

#86
 p-Isopropyltoluene
 Concen: 0.26 ug/l
 RT: 13.44 min Scan# 3687
 Delta R.T. 0.15 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-A04


Tot Ion	Ratio	Lower	Upper
119	100		
134	26.1	13.3	39.8
91	39.5	11.4	34.2#

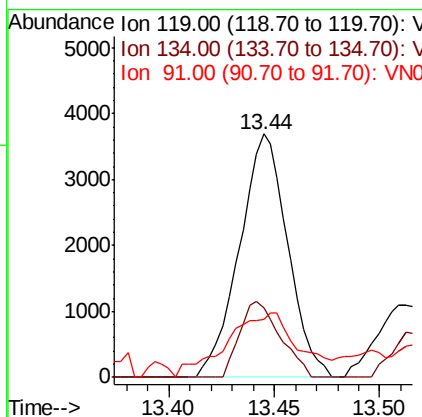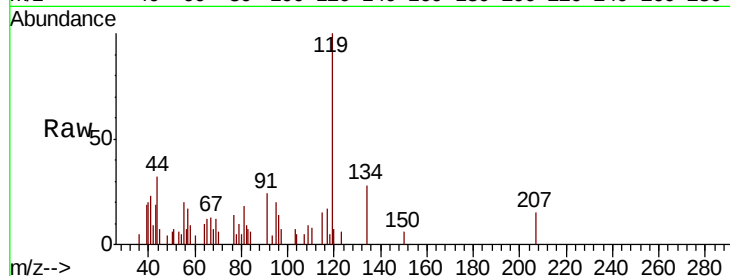

#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 14.44 min Scan# 3996
 Delta R.T. 0.17 min
 Lab File: VN050301.D
 Acq: 3 Aug 2018 7:31

Tgt Ion	Ratio	Lower	Upper
75	100		
155	0.0	44.8	134.4#
157	0.0	57.2	171.6#

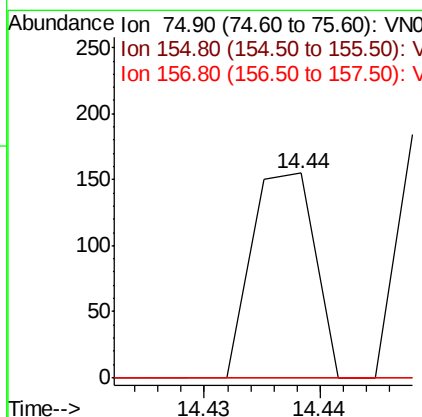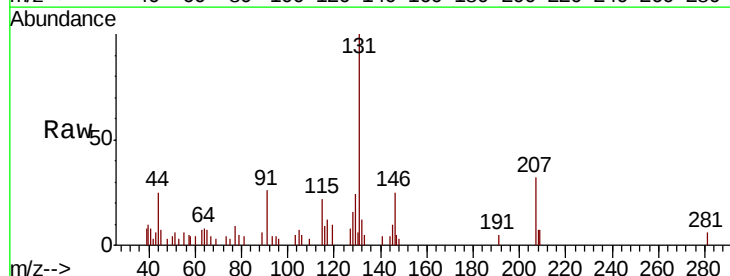


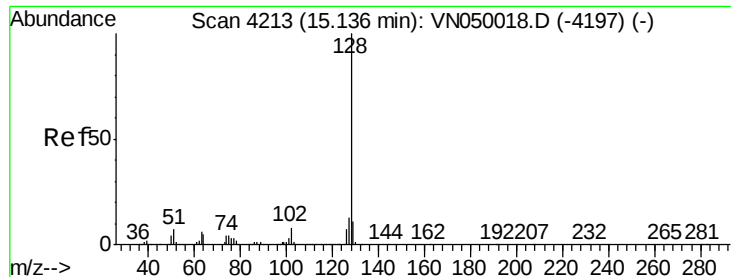

#95
Naphthalene
Concen: 4.50 ug/l
RT: 15.10 min Scan# 4203
Delta R.T. -0.03 min
Lab File: VN050301.D
Acq: 3 Aug 2018 7:31

Instrument :
MSVOA_N
ClientSampleId :
MW-A04

Tot Ion:128 Resp: 1563
Ion Ratio Lower Upper
128 100
127 27.2 10.4 15.6#
129 103.3 8.8 13.2#

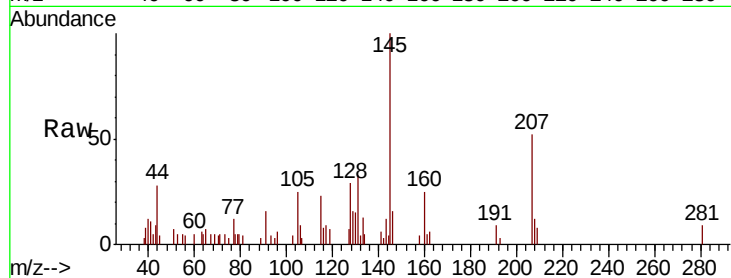

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

