


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080218\
Data File : VN050278.D
Acq On : 2 Aug 2018 21:09
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Title : SW846 8260
Last Update : Thu Jul 26 18:10:10 2018

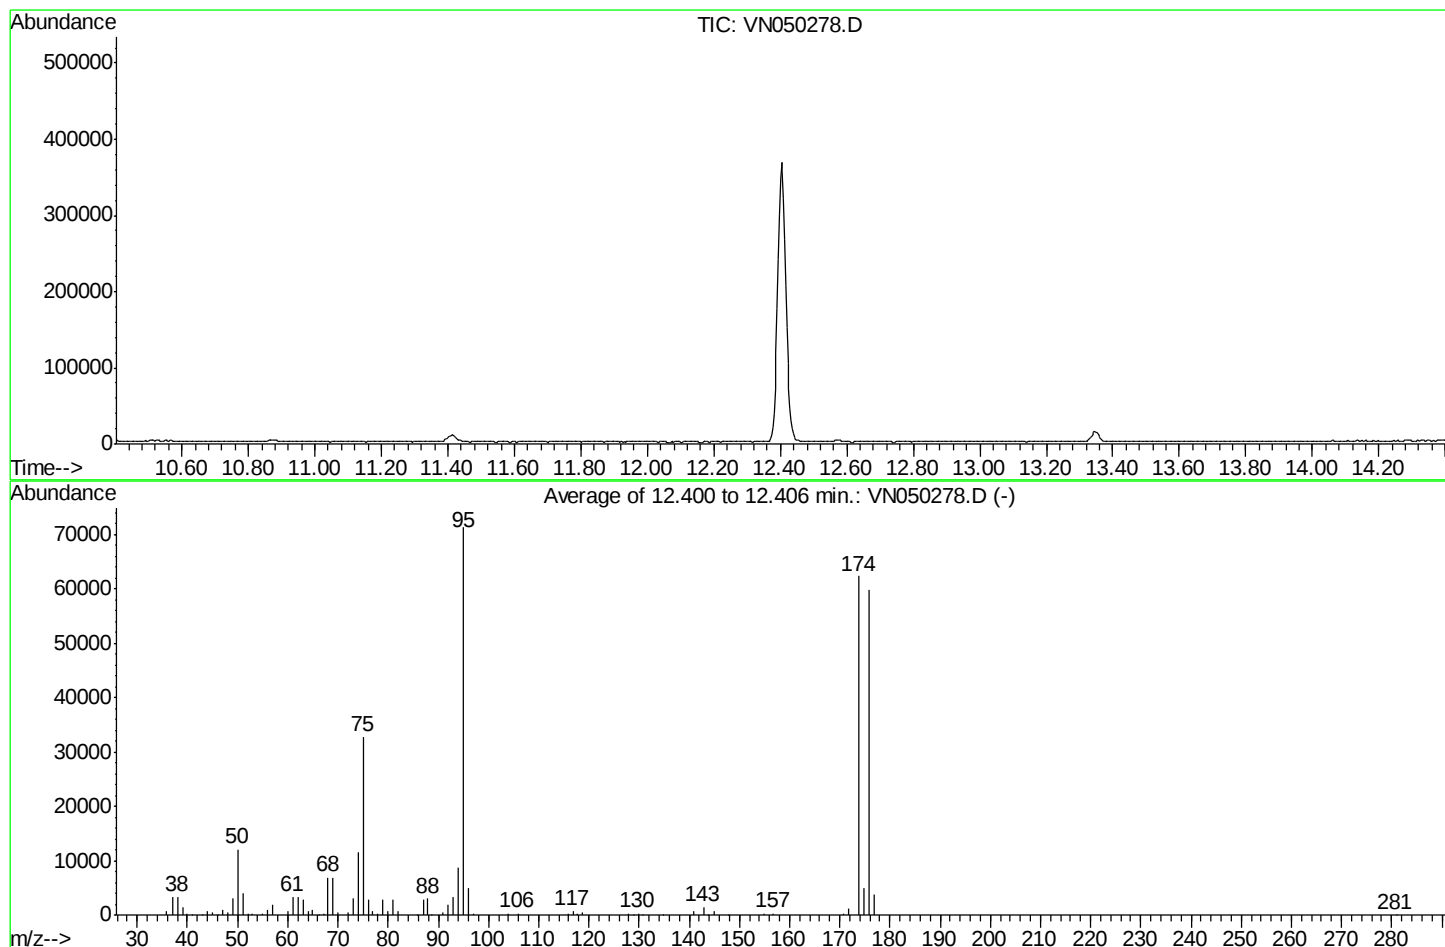

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	12083	PASS
75	95	30	60	46.0	32797	PASS
95	95	100	100	100.0	71317	PASS
96	95	5	9	6.9	4928	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.4	62301	PASS
175	174	5	9	7.8	4878	PASS
176	174	95	101	96.2	59933	PASS
177	176	5	9	6.4	3860	PASS