


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN080219\
Data File : VN057050.D
Acq On : 2 Aug 2019 8:21
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Title : SW846 8260
Last Update : Sat Jul 27 01:33:29 2019

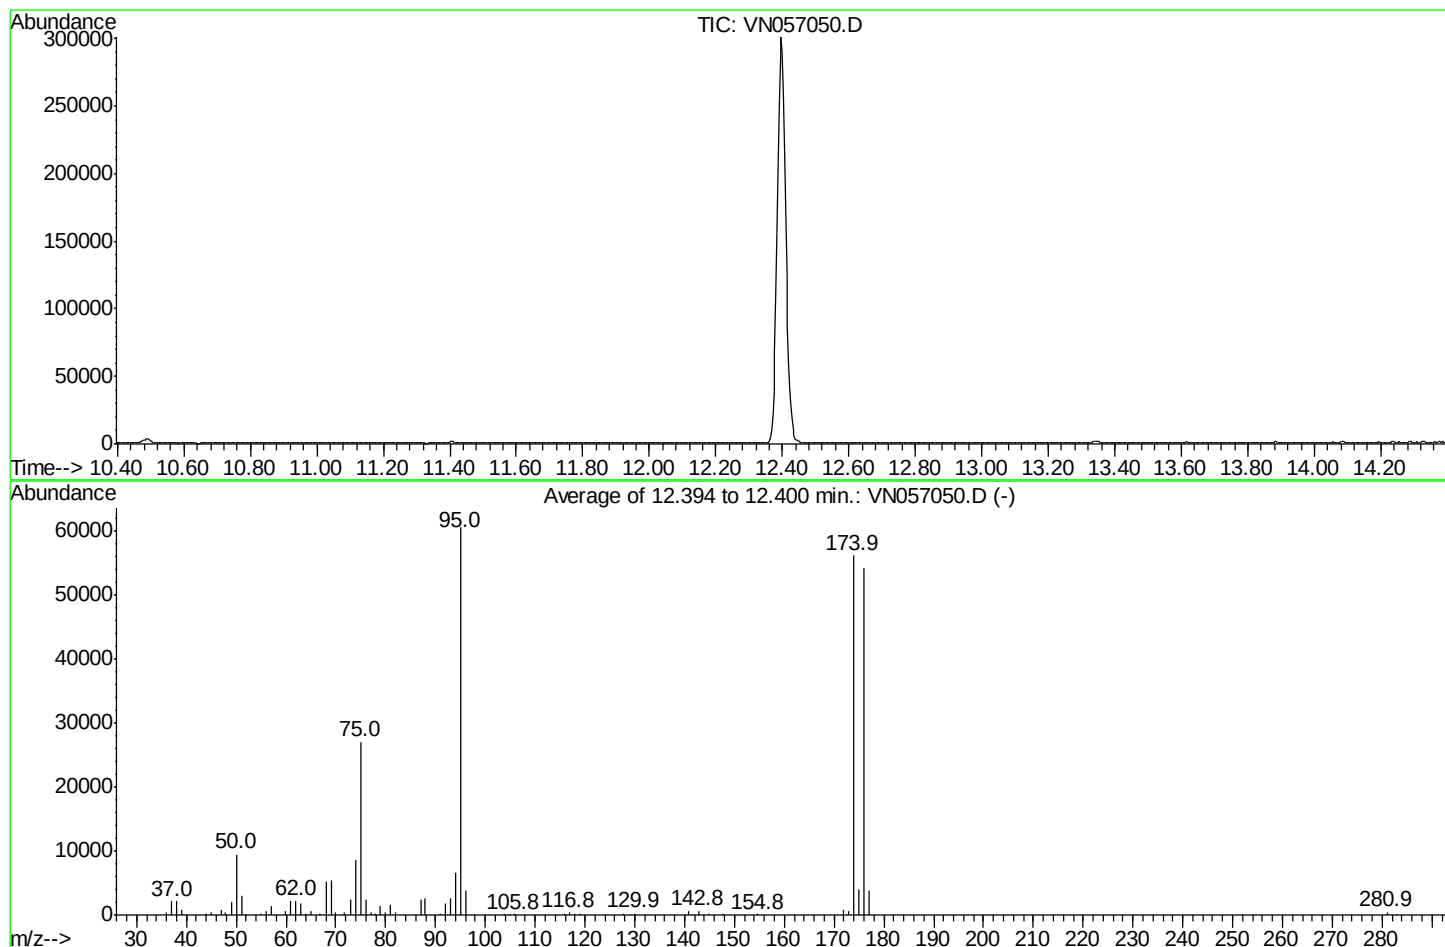

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	9481	PASS
75	95	30	60	44.7	27096	PASS
95	95	100	100	100.0	60573	PASS
96	95	5	9	6.1	3711	PASS
173	174	0.00	2	0.9	516	PASS
174	95	50	100	92.8	56197	PASS
175	174	5	9	7.0	3908	PASS
176	174	95	101	96.4	54192	PASS
177	176	5	9	7.0	3781	PASS