

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080222\
 Data File : VN073689.D
 Acq On : 02 Aug 2022 16:01
 Operator : JC\MD
 Sample : N3971-15
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-23R

Quant Time: Aug 03 02:07:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 29 02:20:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	364748	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	572090	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	539462	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	246833	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	210659	47.392	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	94.780%
35) Dibromofluoromethane	7.951	113	197306	54.924	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	109.840%
50) Toluene-d8	10.380	98	655364	46.360	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	92.720%
62) 4-Bromofluorobenzene	12.674	95	242912	51.195	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.400%


Target Compounds				Qvalue		
3) Chloromethane	2.269	50	1516	Below Cal		100
6) Chloroethane	3.034	64	1081	Below Cal	#	42
11) Tert butyl alcohol	5.292	59	5440	5.675	ug/l #	72
13) Acrolein	3.934	56	811	0.853	ug/l #	1
14) Allyl chloride	4.722	41	1201	0.217	ug/l #	70
16) Acetone	4.228	43	41119	17.223	ug/l	98
18) Methyl Acetate	4.775	43	1634	0.275	ug/l #	57
19) Methyl tert-butyl Ether	5.534	73	23293	1.970	ug/l #	84
20) Methylene Chloride	5.028	84	2114	Below Cal	#	76
25) 2-Butanone	7.269	43	3331	0.898	ug/l	91
29) Tetrahydrofuran	7.633	42	1637	0.698	ug/l	91
31) Cyclohexane	8.022	56	50393	7.615	ug/l #	82
36) 1,1-Dichloropropene	8.022	75	26643	5.204	ug/l #	53
37) Ethyl Acetate	7.339	43	53746	7.971	ug/l	99
38) Carbon Tetrachloride	8.022	117	34450	6.625	ug/l #	17
39) Methylcyclohexane	9.392	83	2581	0.422	ug/l	99
40) Benzene	8.392	78	62605	3.765	ug/l	99
51) 4-Methyl-2-Pentanone	10.269	43	1619	0.248	ug/l #	62
52) Toluene	10.451	92	6533	0.643	ug/l	97
56) Ethyl methacrylate	10.492	69	1437	0.246	ug/l #	39
58) 2-Chloroethyl Vinyl ether	9.904	63	59	9.960	ug/l #	44
67) Ethyl Benzene	11.786	91	58513	3.027	ug/l	97
68) m/p-Xylenes	11.898	106	6607	0.896	ug/l	95
73) Isopropylbenzene	12.521	105	35567	1.968	ug/l	99
76) 1,2,3-Trichloropropane	12.674	75	123727	25.802	ug/l #	1
78) n-propylbenzene	12.863	91	31102	1.530	ug/l	99
79) 2-Chlorotoluene	12.863	91	31102	2.451	ug/l #	40
81) trans-1,4-Dichloro-2-b...	12.674	75	123727	64.960	ug/l #	11
82) 4-Chlorotoluene	12.863	91	31102	2.586	ug/l #	40
84) 1,2,4-Trimethylbenzene	13.304	105	2974	0.203	ug/l	95
90) Hexachloroethane	14.168	117	911	0.320	ug/l #	9
95) Naphthalene	15.433	128	41344	2.948	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080222\
Data File : VN073689.D
Acq On : 02 Aug 2022 16:01
Operator : JC\MD
Sample : N3971-15
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-23R

Quant Time: Aug 03 02:07:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 29 02:20:25 2022
Response via : Initial Calibration




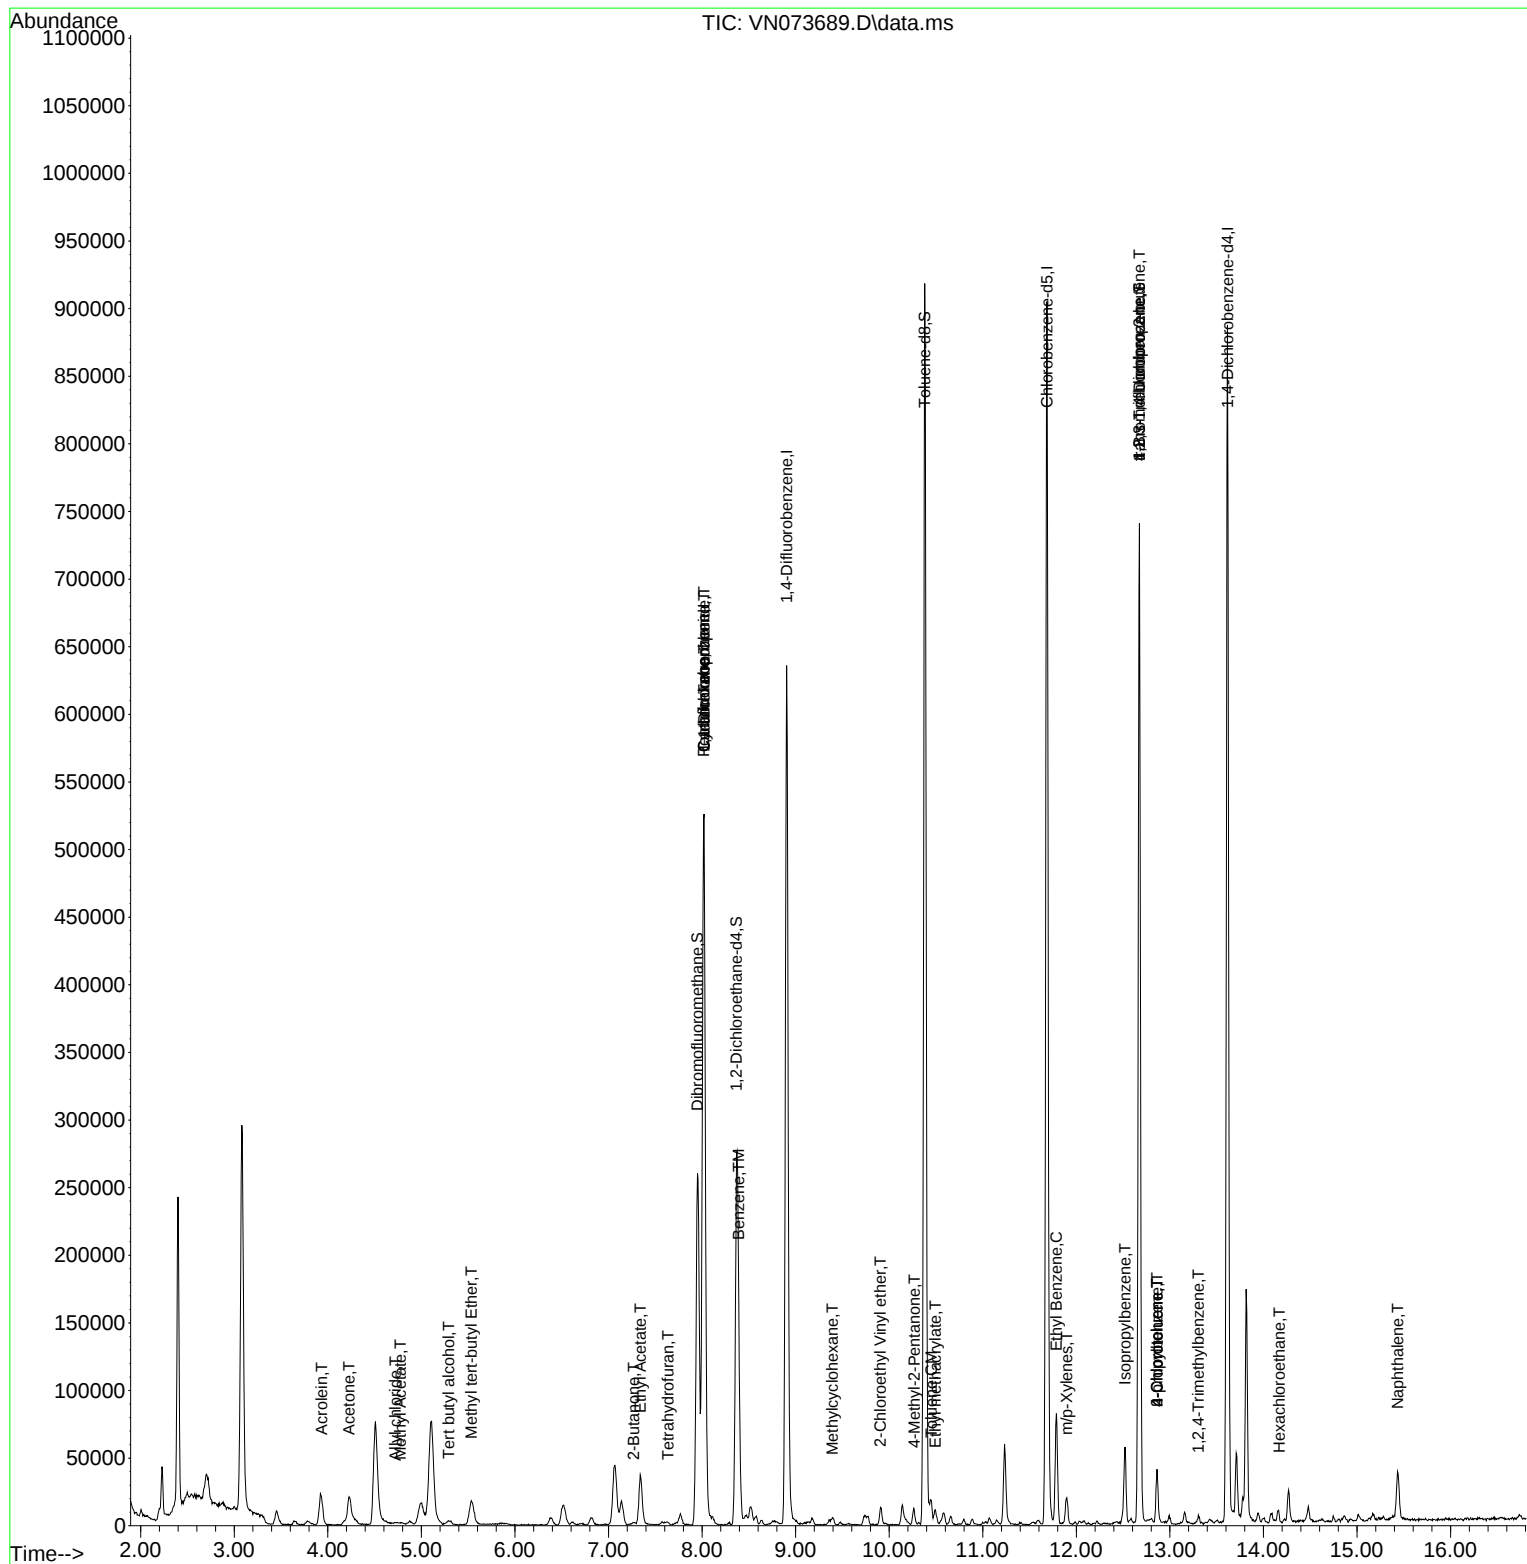




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion:168 Resp: 364748
Ion Ratio Lower Upper
168 100
99 51.9 42.3 63.5

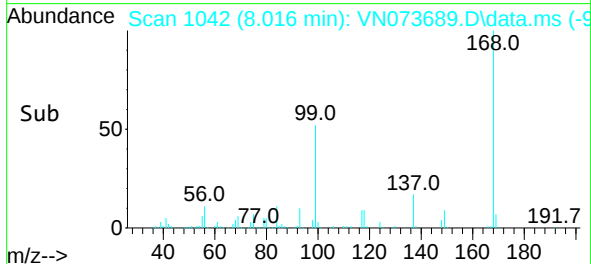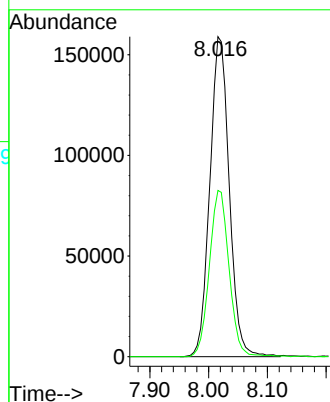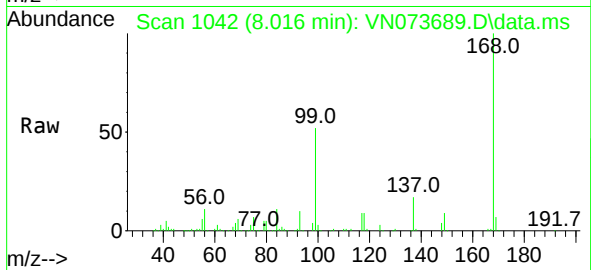

#3
Chloromethane
Concen: Below Cal
RT: 2.269 min Scan# 65
Delta R.T. 0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 50 Resp: 1516
Ion Ratio Lower Upper
50 100
52 32.0 25.7 38.5


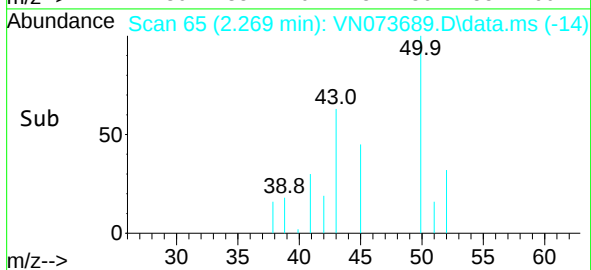
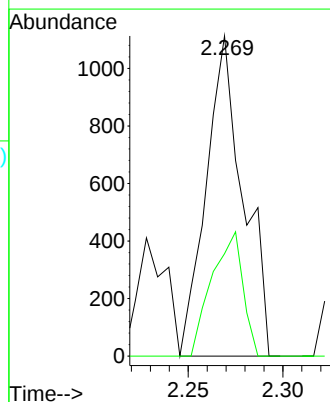
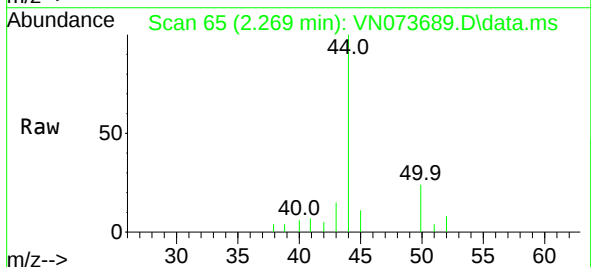




#6
Chloroethane
Concen: Below Cal
RT: 3.034 min Scan# 11
Delta R.T. 0.077 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion: 64 Resp: 1081
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

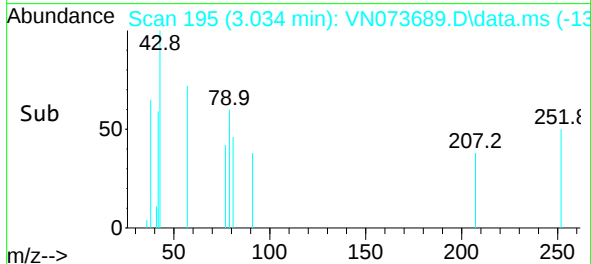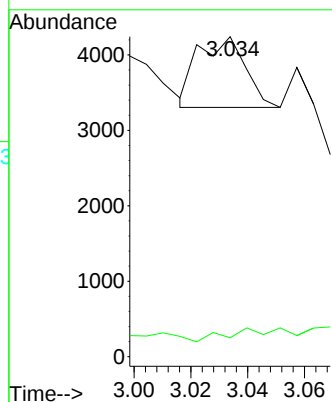

#11
Tert butyl alcohol
Concen: 5.675 ug/l
RT: 5.292 min Scan# 579
Delta R.T. 0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 59 Resp: 5440
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


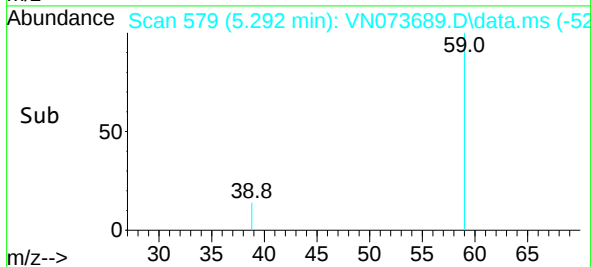
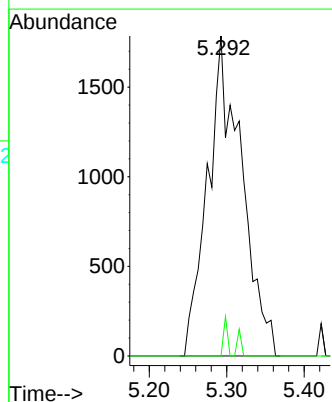
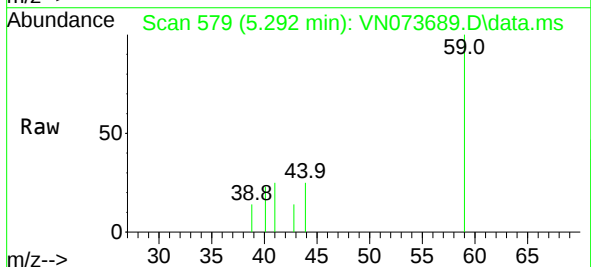




#13
Acrolein
Concen: 0.853 ug/l
RT: 3.934 min Scan# 34
Delta R.T. -0.047 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion: 56 Resp: 811
Ion Ratio Lower Upper
56 100
55 2429.8 54.8 82.2#

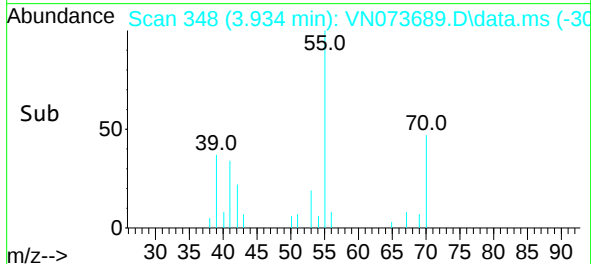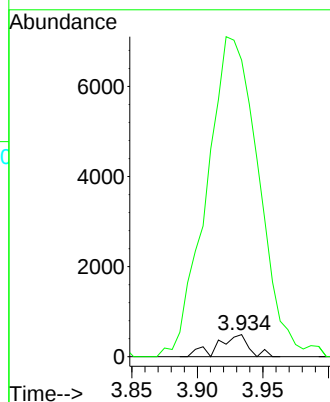

#14
Allyl chloride
Concen: 0.217 ug/l
RT: 4.722 min Scan# 482
Delta R.T. -0.041 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 41 Resp: 1201
Ion Ratio Lower Upper
41 100
39 47.0 53.2 79.8#
76 13.9 29.9 44.9#


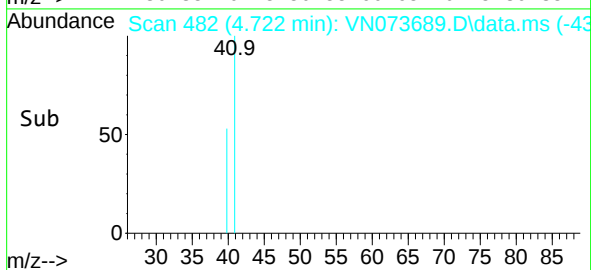
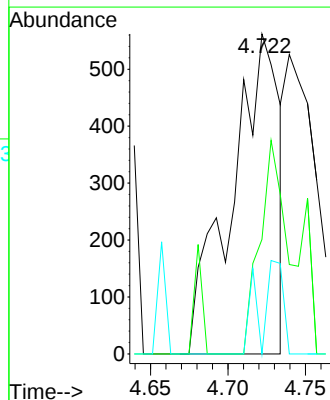
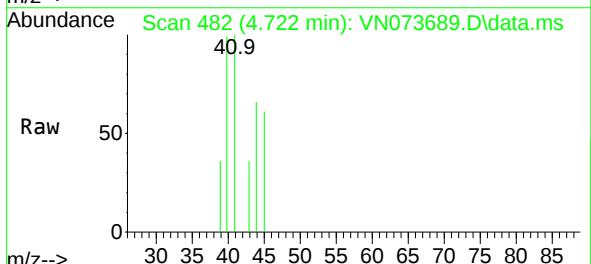




#16
Acetone
Concen: 17.223 ug/l
RT: 4.228 min Scan# 396
Delta R.T. 0.006 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion: 43 Resp: 41119
Ion Ratio Lower Upper
43 100
58 31.3 26.0 39.0

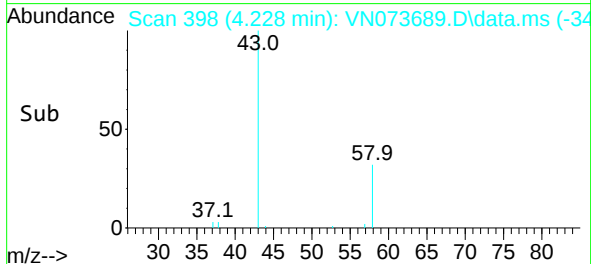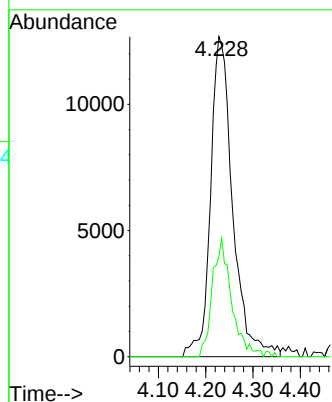

#18
Methyl Acetate
Concen: 0.275 ug/l
RT: 4.775 min Scan# 491
Delta R.T. -0.006 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 43 Resp: 1634
Ion Ratio Lower Upper
43 100
74 5.0 21.6 32.4#

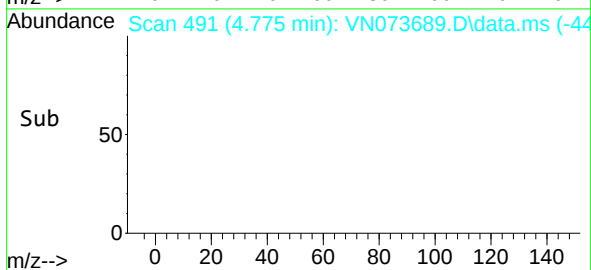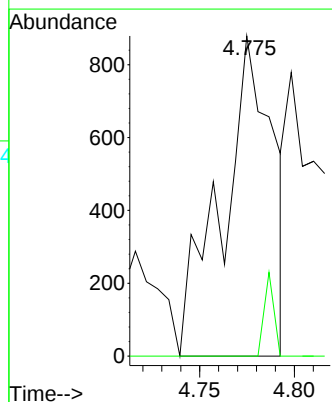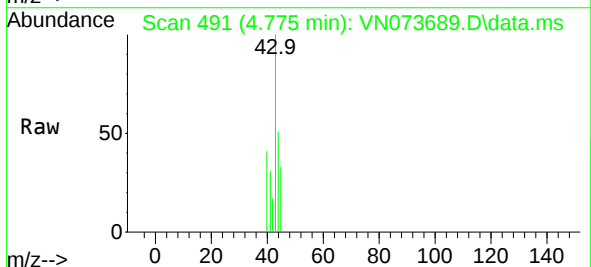

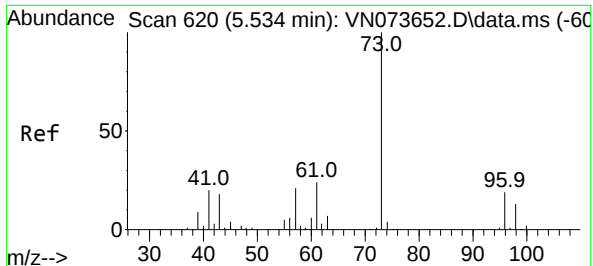

#19

Methyl tert-butyl Ether

Concen: 1.970 ug/l

RT: 5.534 min Scan# 61

Delta R.T. -0.000 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01

Instrument :

MSVOA_N

ClientSampleId :





MW-23R

Tgt Ion: 73 Resp: 23293

Ion Ratio Lower Upper

73 100

57 29.7 17.6 26.4#

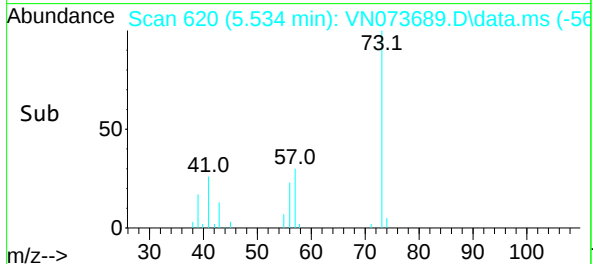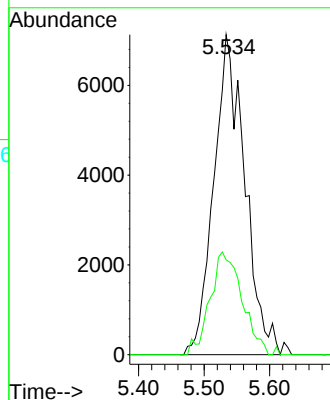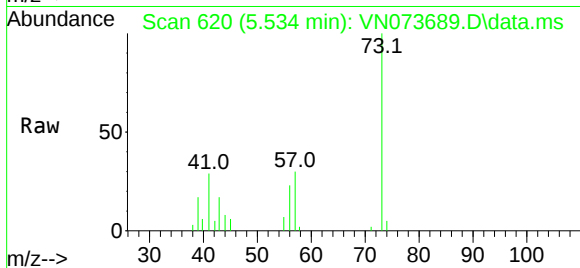

#20

Methylene Chloride

Concen: Below Cal

RT: 5.028 min Scan# 534

Delta R.T. 0.018 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01

Tgt Ion: 84 Resp: 2114




Ion Ratio Lower Upper


84 100

49 74.2 88.3 132.5#

51 36.7 28.2 42.2

86 49.4 50.6 76.0#

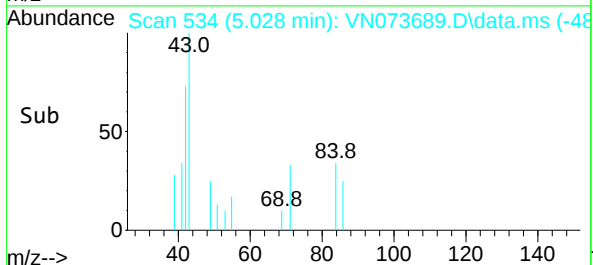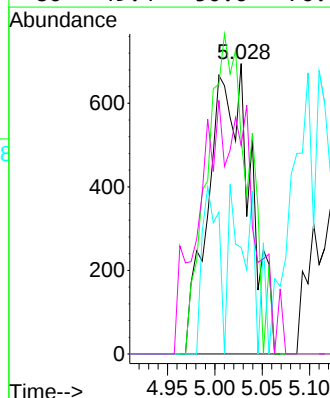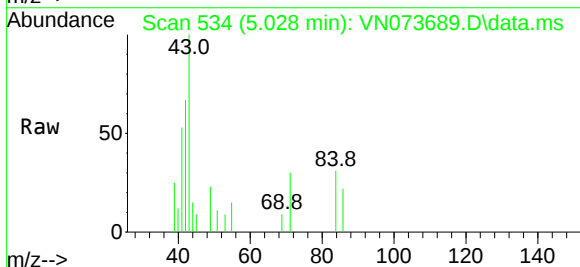

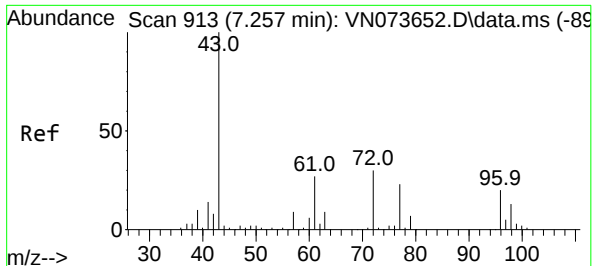

#25

2-Butanone

Concen: 0.898 ug/l

RT: 7.269 min Scan# 913

Delta R.T. 0.012 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01

Instrument :

MSVOA_N

ClientSampleId :





MW-23R

Tgt Ion: 43 Resp: 3331

Ion Ratio Lower Upper

43 100

72 24.9 23.7 35.5

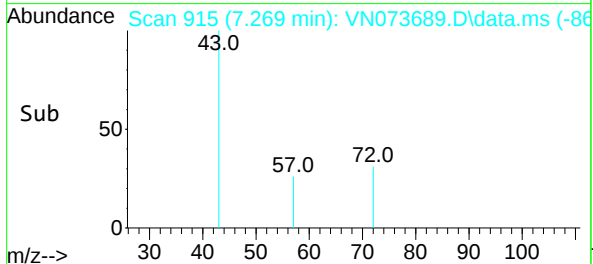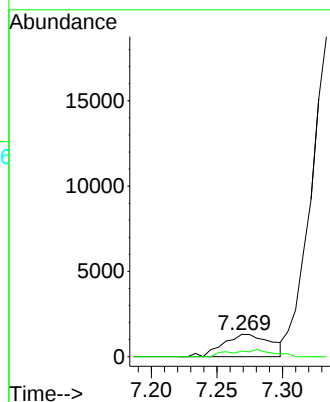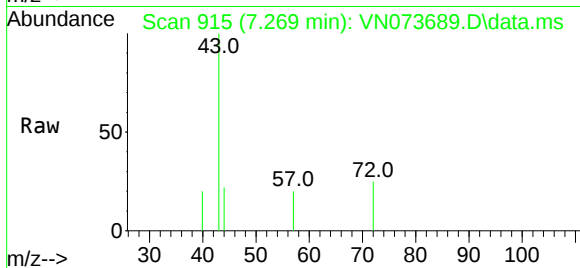

#29

Tetrahydrofuran

Concen: 0.698 ug/l

RT: 7.633 min Scan# 977

Delta R.T. 0.023 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01




Tgt Ion: 42 Resp: 1637


Ion Ratio Lower Upper

42 100

72 55.8 39.7 59.5

71 39.9 36.6 55.0

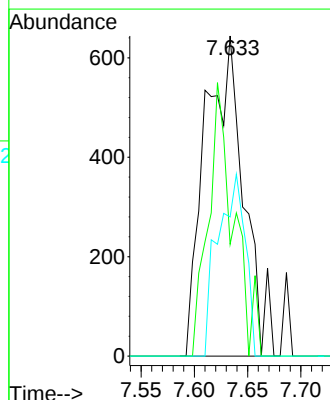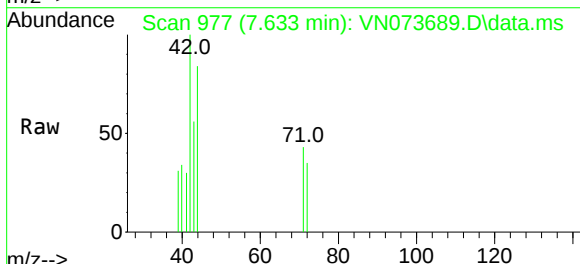



#31

Cyclohexane

Concen: 7.615 ug/l

RT: 8.022 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01

Instrument :

MSVOA_N

ClientSampleId :

MW-23R





Tgt Ion: 56 Resp: 50393

Ion Ratio Lower Upper

56 100

69 51.1 27.8 41.8#

84 110.8 76.9 115.3

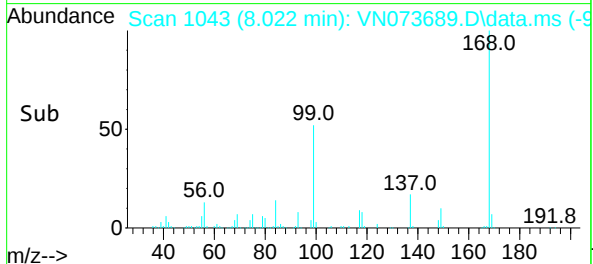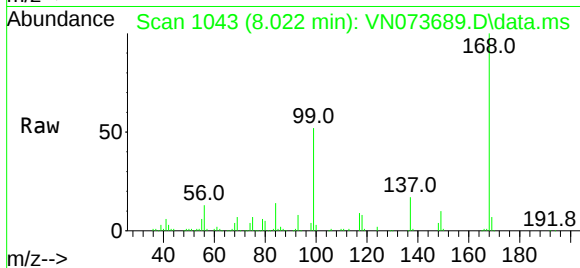

#33

1,2-Dichloroethane-d4

Concen: 47.392 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. -0.000 min

Lab File: VN073689.D




Acq: 02 Aug 2022 16:01


Tgt Ion: 65 Resp: 210659

Ion Ratio Lower Upper

65 100

67 53.5 0.0 104.8

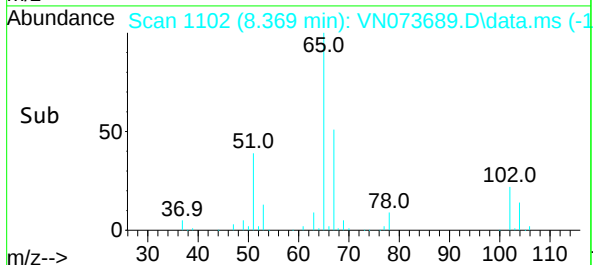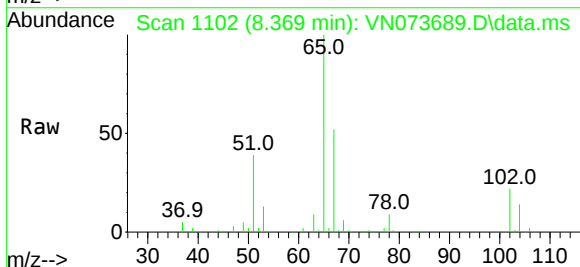

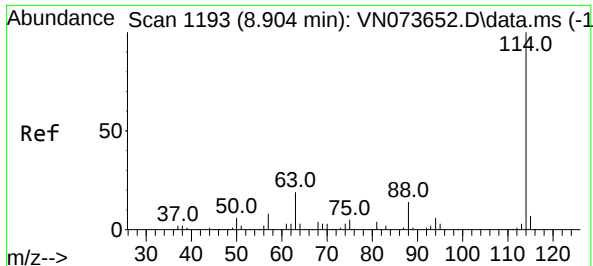

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01

Instrument :

MSVOA_N

ClientSampleId :

MW-23R





Tgt Ion:114 Resp: 572090

Ion Ratio Lower Upper

114 100

63 19.0 0.0 40.0

88 14.8 0.0 32.6

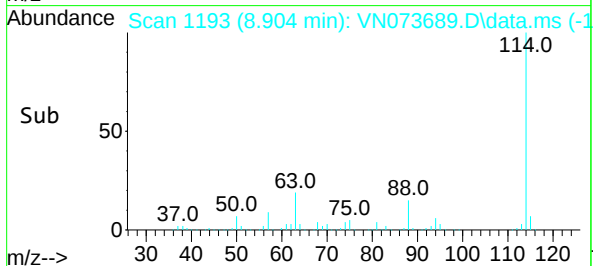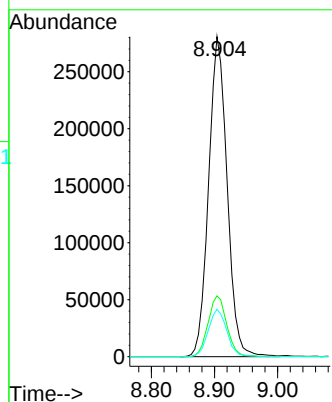

#35

Dibromofluoromethane

Concen: 54.924 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. -0.000 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01




Tgt Ion:113 Resp: 197306


Ion Ratio Lower Upper

113 100

111 101.6 81.4 122.0

192 20.8 17.0 25.6

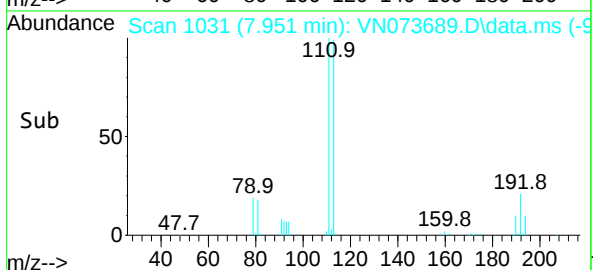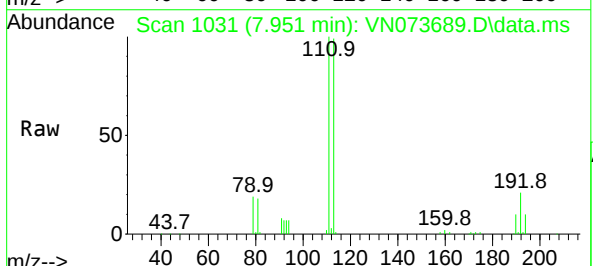

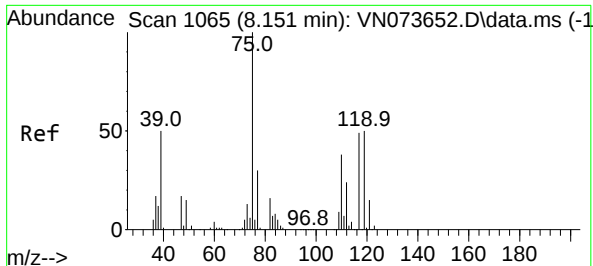

#36

1,1-Dichloropropene

Concen: 5.204 ug/l

RT: 8.022 min Scan# 1043

Delta R.T. -0.129 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01

Instrument :

MSVOA_N

ClientSampleId :

MW-23R





Tgt Ion: 75 Resp: 26643

Ion Ratio Lower Upper

75 100

110 9.7 18.3 54.8#

77 4.1 25.1 37.7#

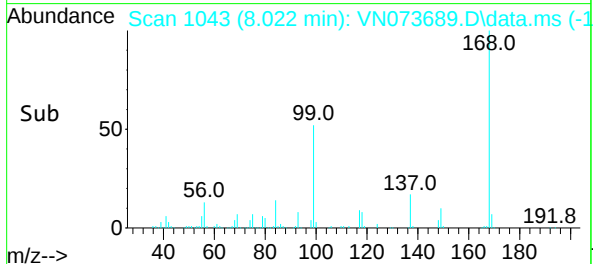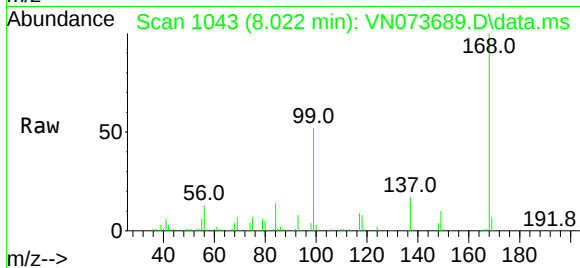

#37

Ethyl Acetate

Concen: 7.971 ug/l

RT: 7.339 min Scan# 927

Delta R.T. -0.000 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01




Tgt Ion: 43 Resp: 53746


Ion Ratio Lower Upper

43 100

61 15.5 11.8 17.6

70 11.5 9.3 13.9


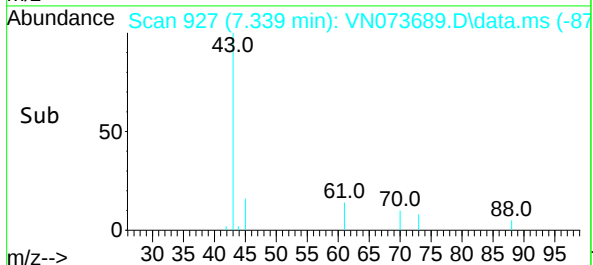
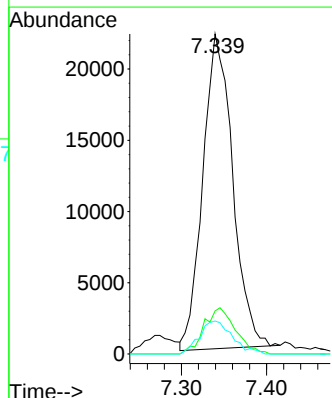
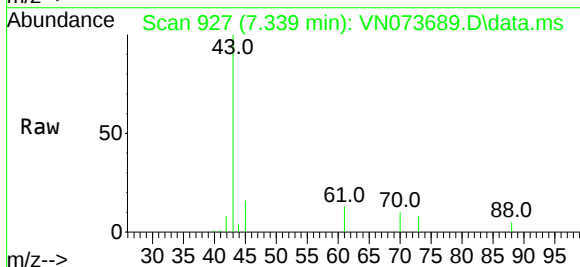


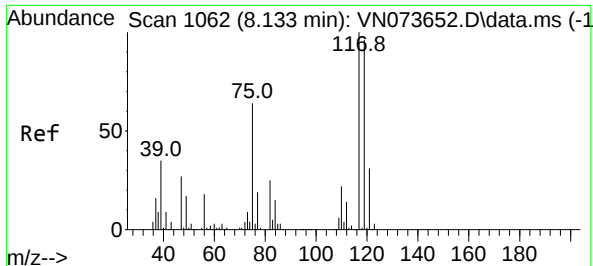

#38
Carbon Tetrachloride
Concen: 6.625 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. -0.112 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion:117 Resp: 34450
Ion Ratio Lower Upper
117 100
119 5.7 75.8 113.8#
121 0.0 24.6 37.0#

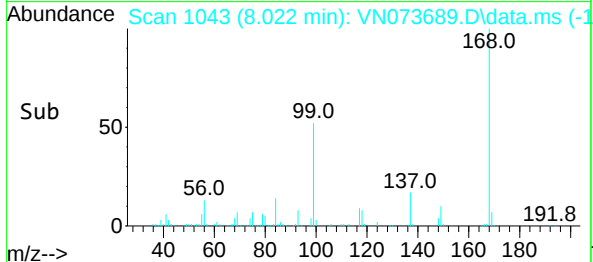

#39
Methylcyclohexane
Concen: 0.422 ug/l
RT: 9.392 min Scan# 1276
Delta R.T. -0.006 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 83 Resp: 2581
Ion Ratio Lower Upper
83 100
55 72.1 57.8 86.8
98 50.4 39.4 59.2


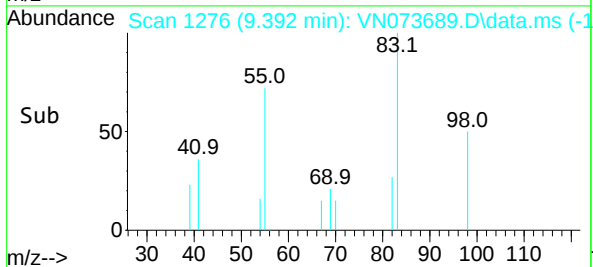

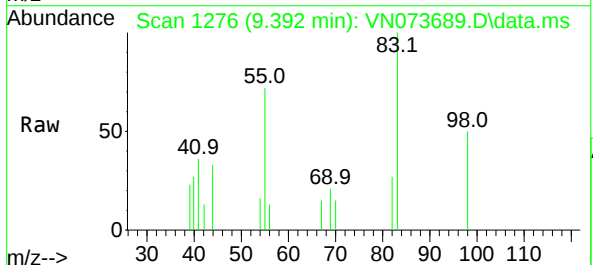


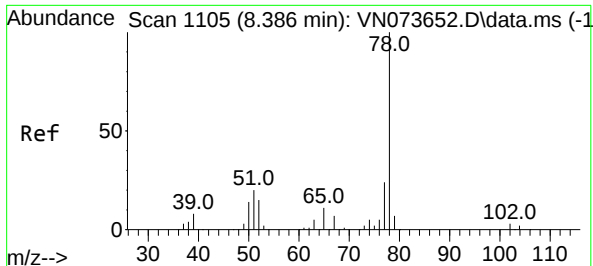

#40
Benzene
Concen: 3.765 ug/l
RT: 8.392 min Scan# 1106
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion: 78 Resp: 62605
Ion Ratio Lower Upper
78 100
77 23.8 19.4 29.0

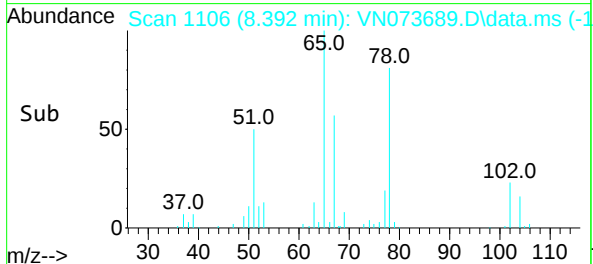

#50
Toluene-d8
Concen: 46.360 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 98 Resp: 655364
Ion Ratio Lower Upper
98 100
100 64.3 52.6 78.8

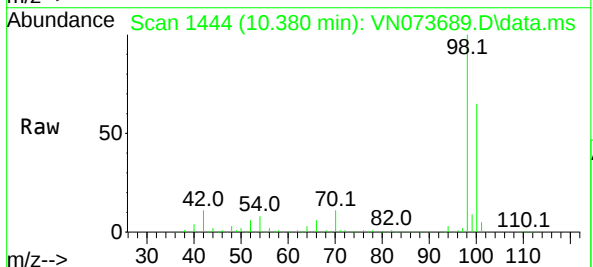



#51

4-Methyl-2-Pentanone

Concen: 0.248 ug/l

RT: 10.269 min Scan# 1425

Delta R.T. -0.006 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01

Instrument :

MSVOA_N

ClientSampleId :





MW-23R

Tgt Ion: 43 Resp: 1619

Ion Ratio Lower Upper

43 100

58 18.2 34.1 51.1#

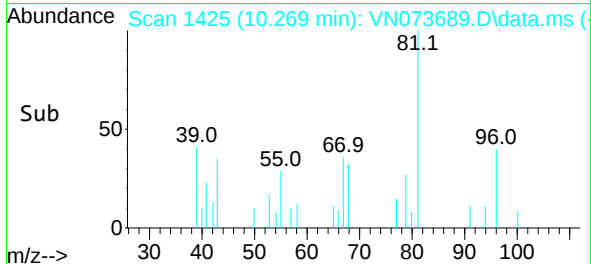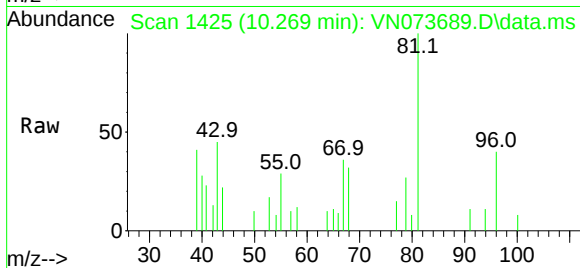

#52

Toluene

Concen: 0.643 ug/l

RT: 10.451 min Scan# 1456

Delta R.T. 0.006 min

Lab File: VN073689.D




Acq: 02 Aug 2022 16:01


Tgt Ion: 92 Resp: 6533

Ion Ratio Lower Upper

92 100

91 169.5 138.6 207.8


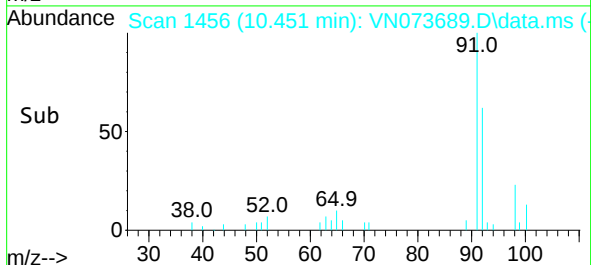

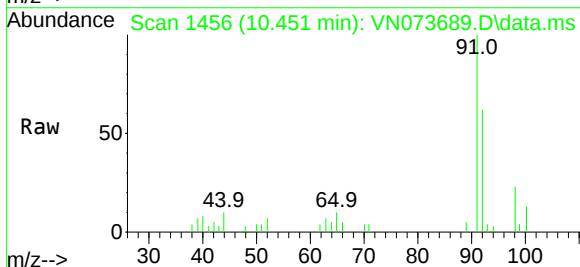




#56
Ethyl methacrylate
Concen: 0.246 ug/l
RT: 10.492 min Scan# 1499
Delta R.T. -0.212 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion: 69 Resp: 1437
Ion Ratio Lower Upper
69 100
41 122.6 47.8 71.6#
39 46.4 27.3 40.9#

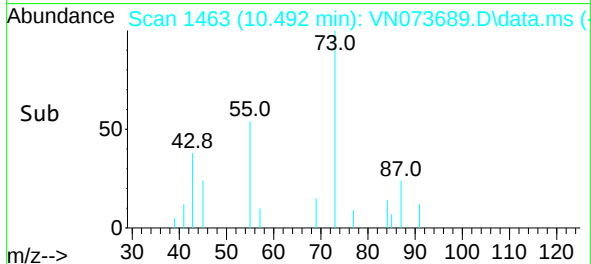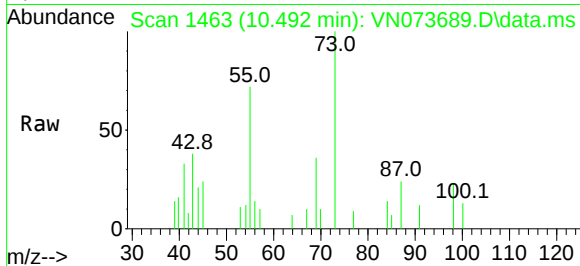

#58
2-Chloroethyl Vinyl ether
Concen: 9.960 ug/l
RT: 9.904 min Scan# 1363
Delta R.T. -0.076 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 63 Resp: 59
Ion Ratio Lower Upper
63 100
106 0.0 24.6 36.8#



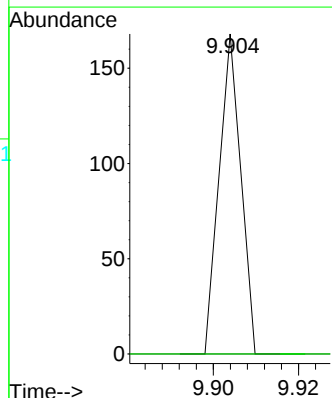
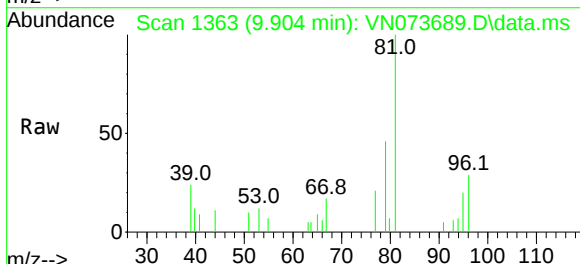




#62
4-Bromofluorobenzene
Concen: 51.195 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion: 95 Resp: 242912
Ion Ratio Lower Upper
95 100
174 87.8 0.0 167.6
176 83.9 0.0 163.4

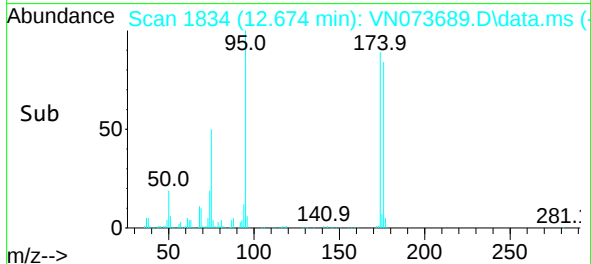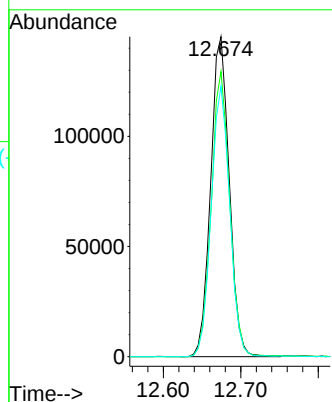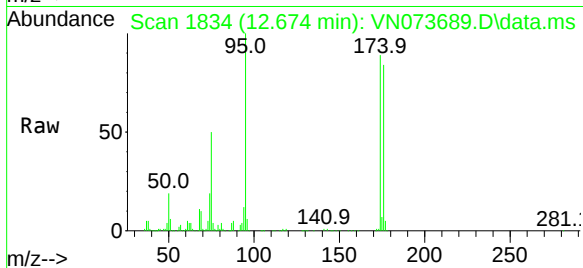

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 117 Resp: 539462
Ion Ratio Lower Upper
117 100
82 52.9 44.2 66.2
119 31.6 25.4 38.0


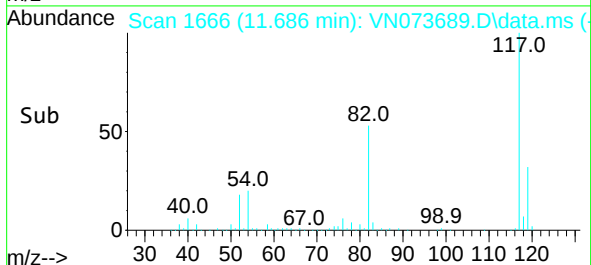

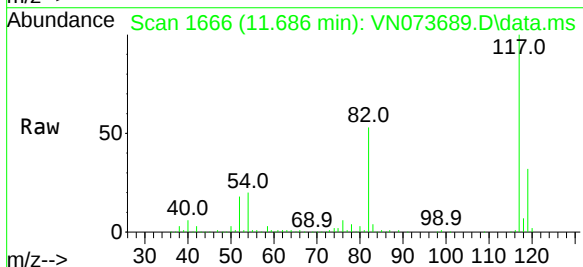


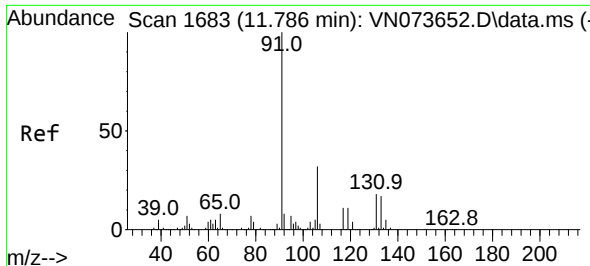

#67
Ethyl Benzene
Concen: 3.027 ug/l
RT: 11.786 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion: 91 Resp: 58513
Ion Ratio Lower Upper
91 100
106 29.5 24.9 37.3

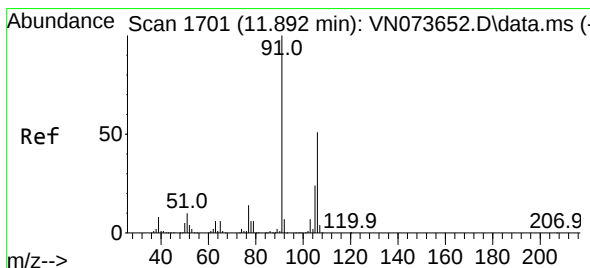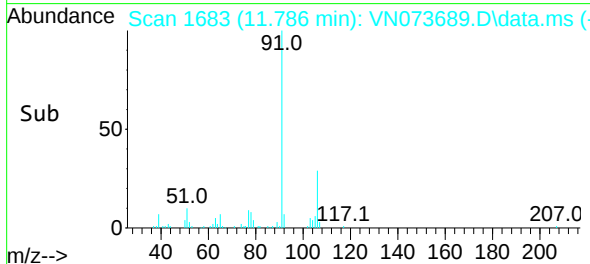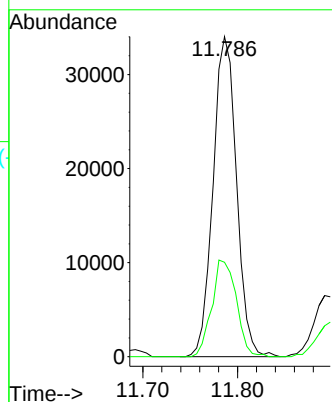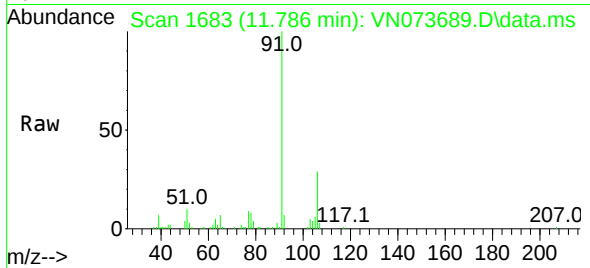

#68
m/p-Xylenes
Concen: 0.896 ug/l
RT: 11.898 min Scan# 1702
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 106 Resp: 6607
Ion Ratio Lower Upper
106 100
91 206.5 158.9 238.3


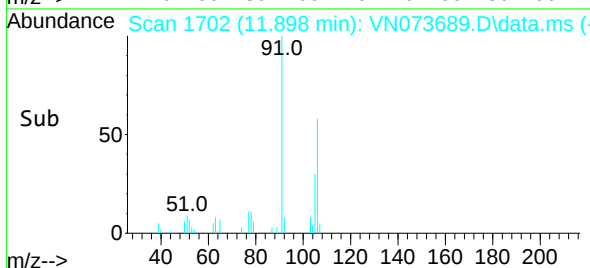

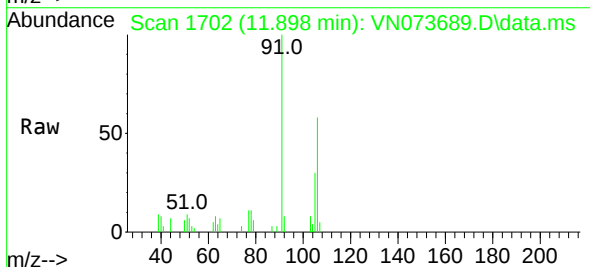


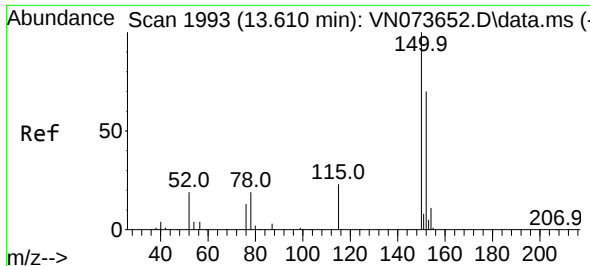

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion:152 Resp: 246833
Ion Ratio Lower Upper
152 100
115 57.0 28.9 86.7
150 156.9 0.0 356.2

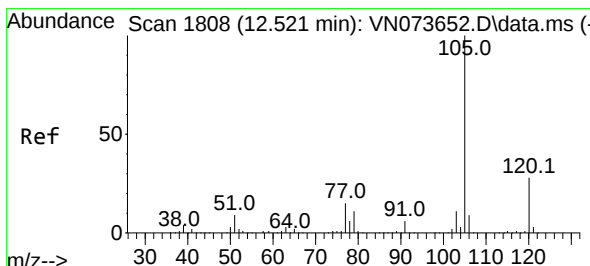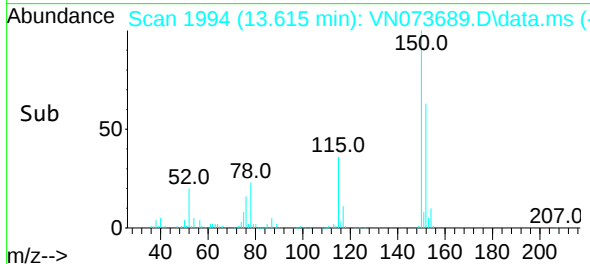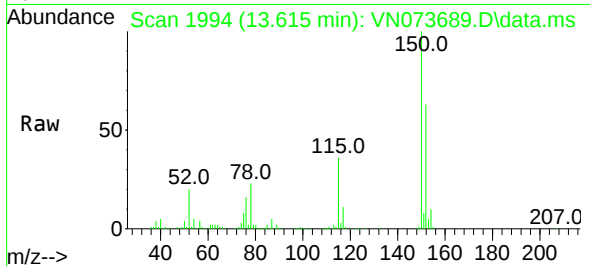

#73
Isopropylbenzene
Concen: 1.968 ug/l
RT: 12.521 min Scan# 1808
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion:105 Resp: 35567
Ion Ratio Lower Upper
105 100
120 26.6 13.5 40.4


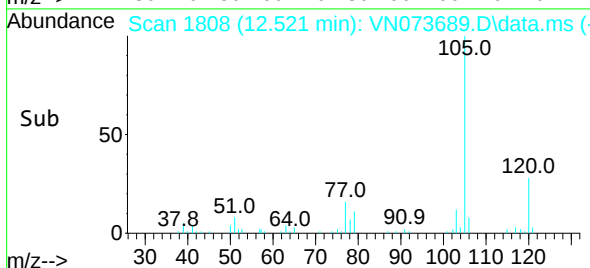
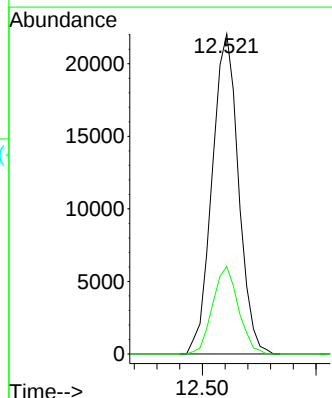
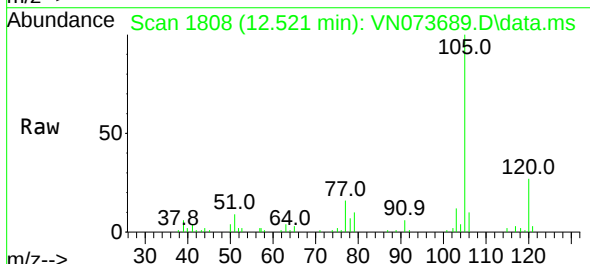




#76
1,2,3-Trichloropropane
Concen: 25.802 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.147 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion: 75 Resp: 123727
Ion Ratio Lower Upper
75 100
77 1.5 98.5 295.5#

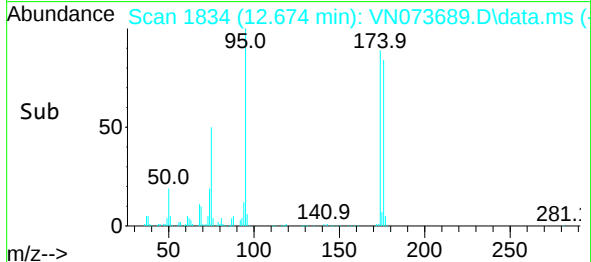

#78
n-propylbenzene
Concen: 1.530 ug/l
RT: 12.863 min Scan# 1866
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 91 Resp: 31102
Ion Ratio Lower Upper
91 100
120 23.4 11.9 35.5

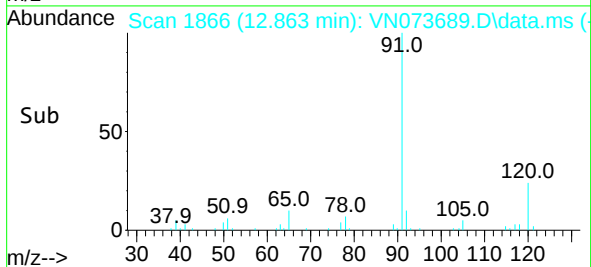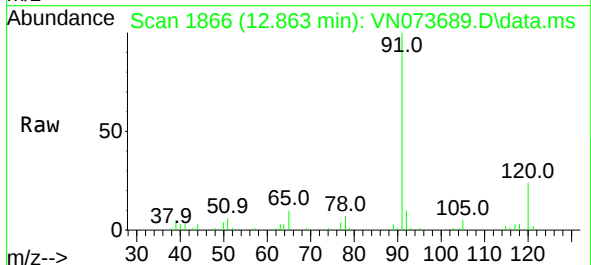



#79

2-Chlorotoluene

Concen: 2.451 ug/l

RT: 12.863 min Scan# 1866

Delta R.T. -0.088 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01

Instrument :

MSVOA_N

ClientSampleId :





MW-23R

Tgt Ion: 91 Resp: 31102

Ion Ratio Lower Upper

91 100

126 0.0 17.3 51.9#

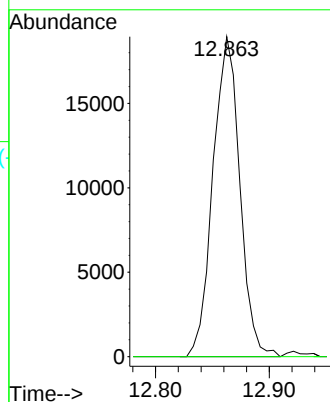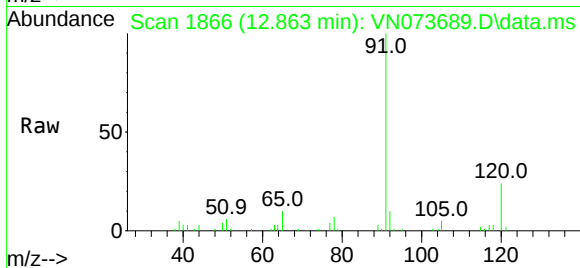

#81

trans-1,4-Dichloro-2-butene

Concen: 64.960 ug/l

RT: 12.674 min Scan# 1834

Delta R.T. 0.106 min

Lab File: VN073689.D

Acq: 02 Aug 2022 16:01




Tgt Ion: 75 Resp: 123727


Ion Ratio Lower Upper

75 100

53 0.2 78.0 117.0#

89 0.0 37.2 55.8#


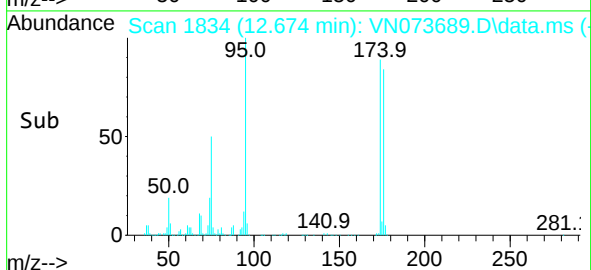
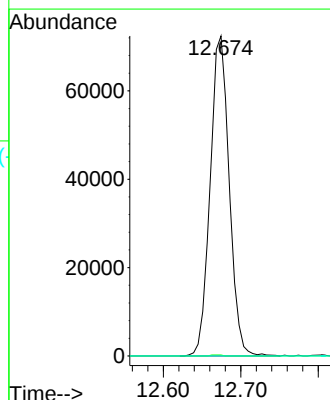
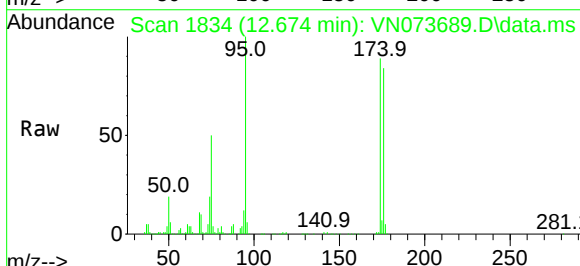




#82
4-Chlorotoluene
Concen: 2.586 ug/l
RT: 12.863 min Scan# 1897
Delta R.T. -0.182 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01




Instrument :
MSVOA_N
ClientSampleId :
MW-23R


Tgt Ion: 91 Resp: 31102
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

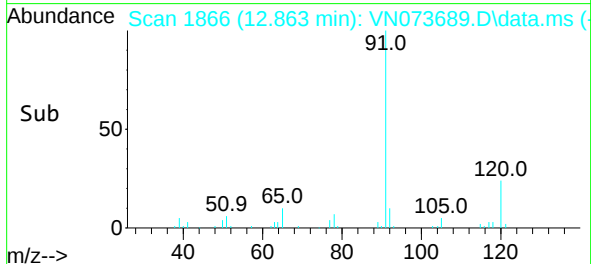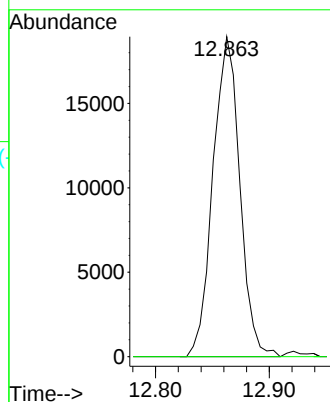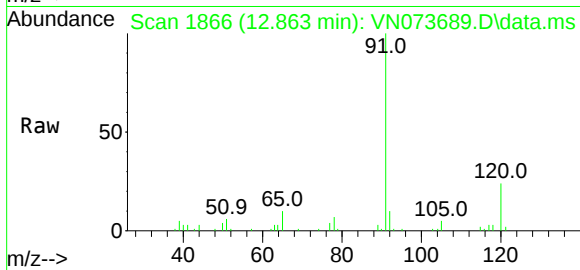

#84
1,2,4-Trimethylbenzene
Concen: 0.203 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. -0.006 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion: 105 Resp: 2974
Ion Ratio Lower Upper
105 100
120 43.3 23.3 69.8


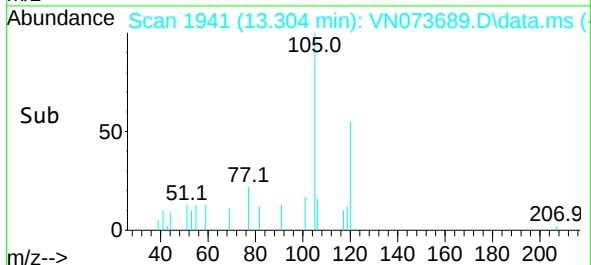
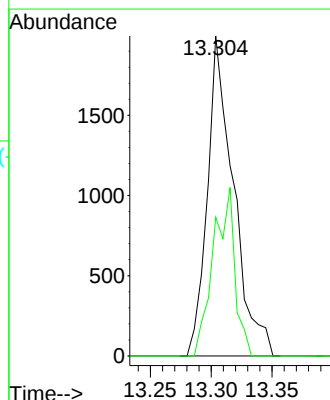
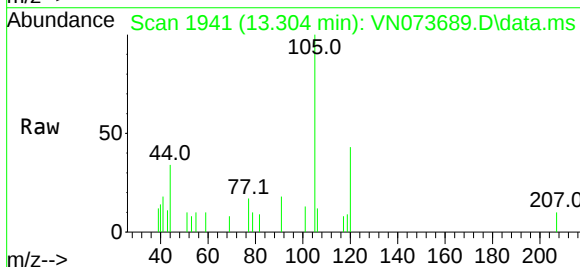




#90
Hexachloroethane
Concen: 0.320 ug/l
RT: 14.168 min Scan# 2088
Delta R.T. 0.018 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Instrument :
MSVOA_N
ClientSampleId :
MW-23R

Tgt Ion:117 Resp: 911
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

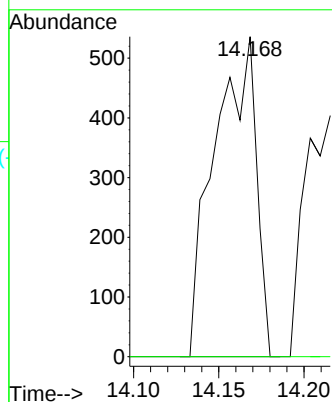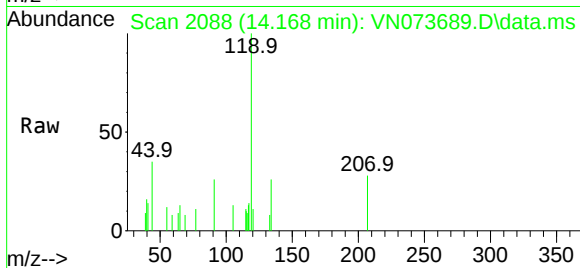

#95
Naphthalene
Concen: 2.948 ug/l
RT: 15.433 min Scan# 2303
Delta R.T. -0.000 min
Lab File: VN073689.D
Acq: 02 Aug 2022 16:01

Tgt Ion:128 Resp: 41344
Ion Ratio Lower Upper
128 100
127 13.4 10.3 15.5
129 10.2 8.6 13.0

