


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080222\
Data File : VN073675.D
Acq On : 02 Aug 2022 09:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Title : SW846 8260
Last Update : Fri Jul 29 02:20:25 2022

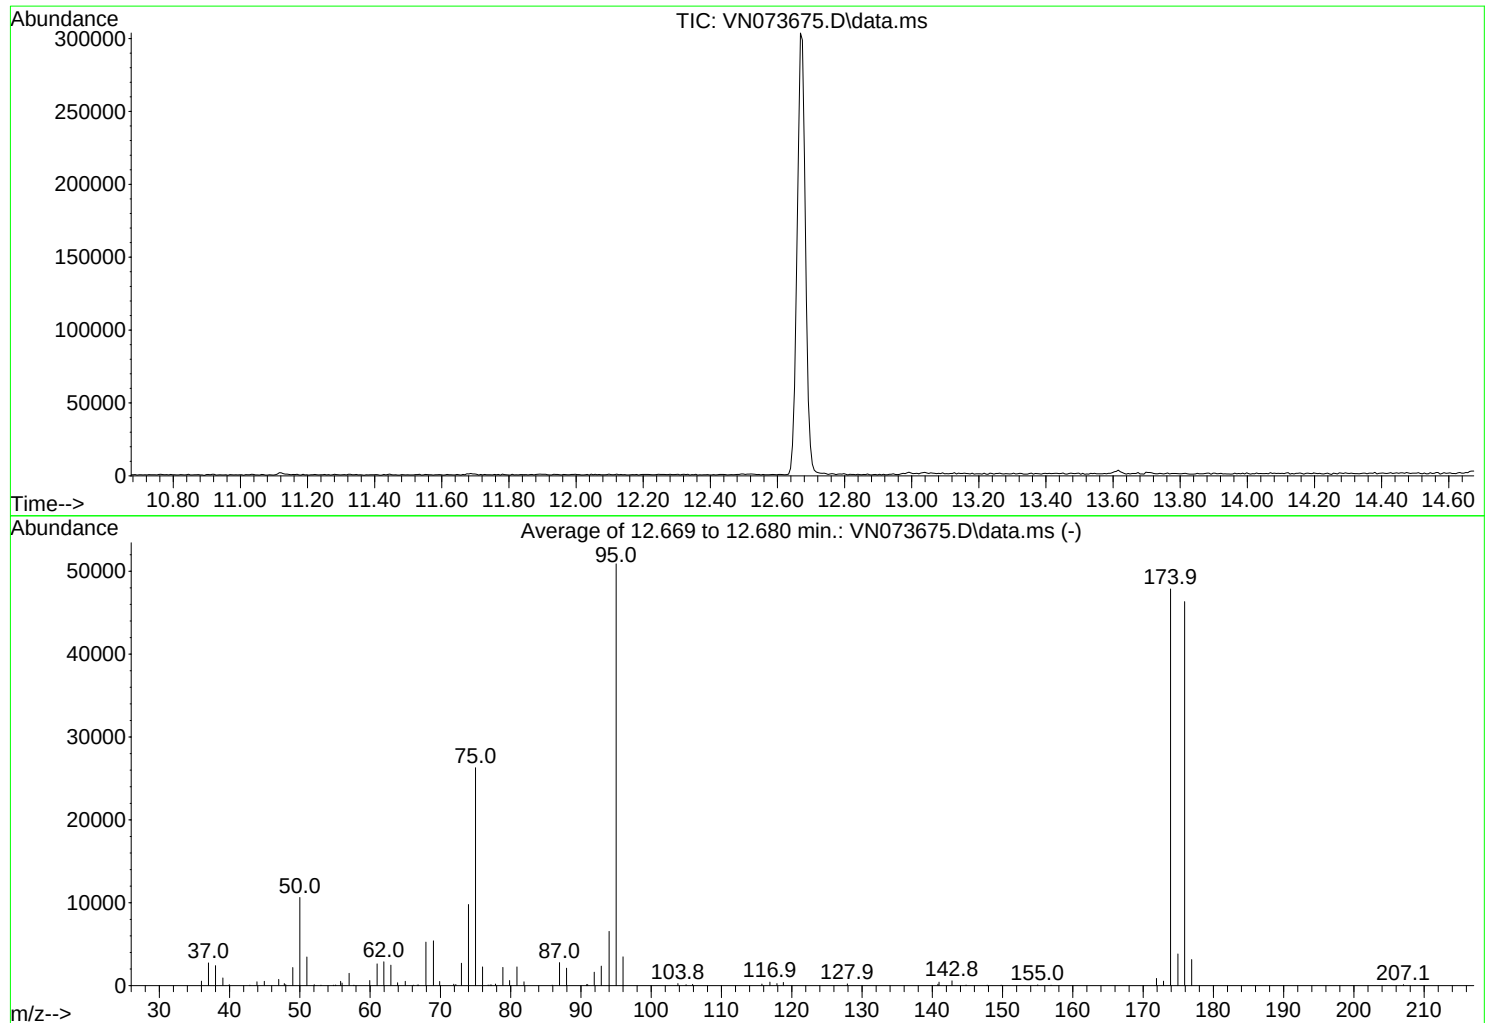

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1824

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	10636	PASS
75	95	30	60	51.7	26299	PASS
95	95	100	100	100.0	50896	PASS
96	95	5	9	6.8	3482	PASS
173	174	0.00	2	1.1	545	PASS
174	95	50	100	94.1	47869	PASS
175	174	5	9	8.0	3831	PASS
176	174	95	101	96.8	46328	PASS
177	176	5	9	6.8	3157	PASS