
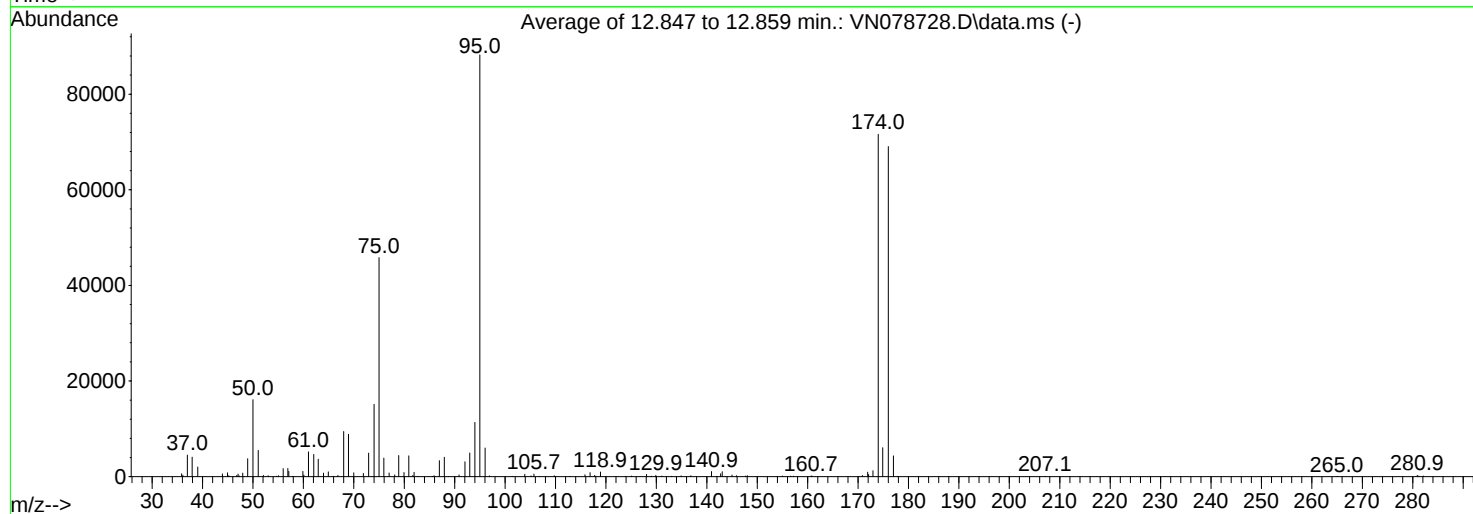


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080223\
Data File : VN078728.D
Acq On : 02 Aug 2023 09:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080123W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Aug 02 04:51:47 2023

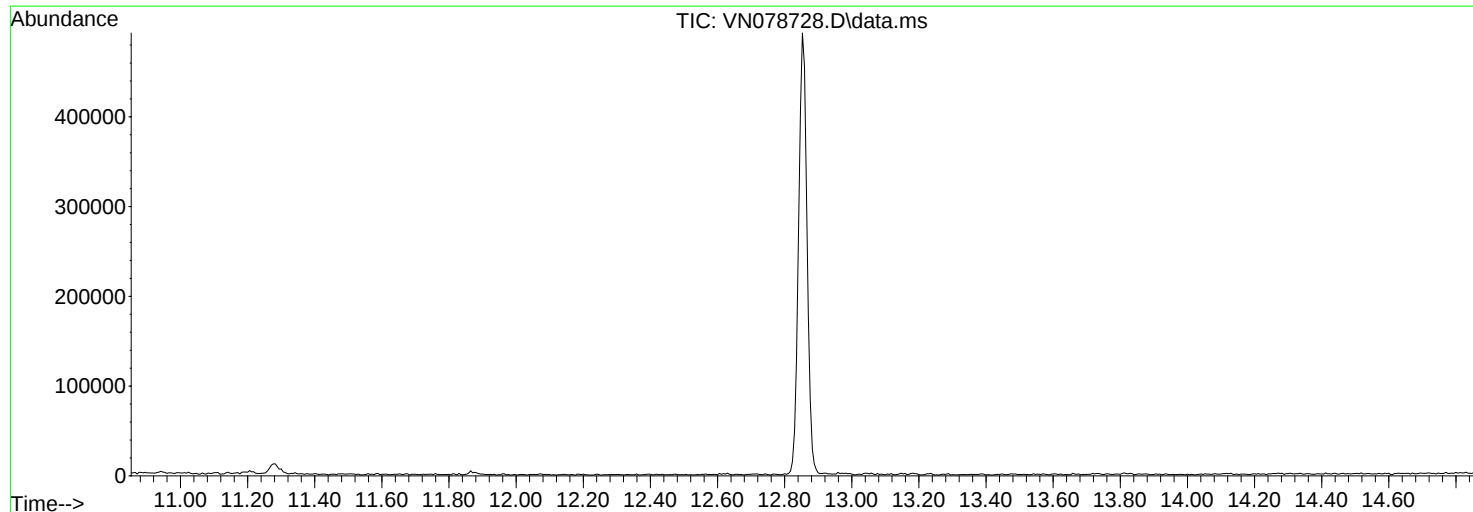

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	16101	PASS
75	95	30	60	51.9	45821	PASS
95	95	100	100	100.0	88229	PASS
96	95	5	9	6.8	5987	PASS
173	174	0.00	2	1.7	1242	PASS
174	95	50	100	81.2	71629	PASS
175	174	5	9	8.5	6067	PASS
176	174	95	101	96.4	69037	PASS
177	176	5	9	6.3	4369	PASS