

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080318\
 Data File : VN050344.D
 Acq On : 4 Aug 2018 5:04
 Operator : MD\SY
 Sample : J4313-06
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 C-7

Quant Time: Aug 04 05:37:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 26 18:10:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	652817	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1072362	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	907515	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	362002	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	456688	50.14	ug/l	0.00
Spiked Amount			Recovery	=	100.28%	
35) Dibromofluoromethane	7.59	113	405663	46.33	ug/l	0.00
Spiked Amount			Recovery	=	92.66%	
50) Toluene-d8	10.09	98	1461943	45.42	ug/l	0.00
Spiked Amount			Recovery	=	90.84%	
62) 4-Bromofluorobenzene	12.40	95	411085	38.79	ug/l	0.00
Spiked Amount			Recovery	=	77.58%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.06	50	3858	0.38	ug/l	98
5) Bromomethane	2.57	94	3991	Below	Cal	91
13) Acrolein	3.62	56	1041	1.93	ug/l #	56
16) Acetone	3.82	43	42963	15.96	ug/l	93
18) Methyl Acetate	4.34	43	13338	Below	Cal	100
20) Methylene Chloride	4.55	84	54584	5.65	ug/l	95
25) 2-Butanone	6.84	43	5999	1.73	ug/l	91
28) Bromochloromethane	7.38	49	3367	0.49	ug/l #	10
29) Tetrahydrofuran	7.22	42	1295	0.58	ug/l #	49
30) Chloroform	7.37	83	44439	2.88	ug/l	99
31) Cyclohexane	7.67	56	12172	0.90	ug/l #	1
36) 1,1-Dichloropropene	7.67	75	45380	3.76	ug/l #	48
38) Carbon Tetrachloride	7.67	117	57100	4.45	ug/l #	16
41) Methacrylonitrile	7.22	41	605	2.88	ug/l #	27
43) Isopropyl Acetate	8.17	43	142814	8.04	ug/l #	92
47) Bromodichloromethane	9.40	83	9082	0.71	ug/l	90
48) Methyl methacrylate	9.18	41	2938	0.40	ug/l #	26
49) 1,4-Dioxane	9.20	88	60	0.61	ug/l #	1
51) 4-Methyl-2-Pentanone	9.99	43	2651	0.32	ug/l #	59
56) Ethyl methacrylate	10.63	69	191	2.05	ug/l #	1
59) 2-Hexanone	10.77	43	3416	5.72	ug/l #	54
70) Styrene	11.97	104	75	0.93	ug/l #	25
75) 1,1,2,2-Tetrachloroethane	12.40	83	214	Below	Cal #	1
76) 1,2,3-Trichloropropane	12.40	75	202212	30.06	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	202212	95.34	ug/l #	13
92) 1,2-Dibromo-3-Chloropropan	14.50	75	32	Below	Cal #	1
95) Naphthalene	15.14	128	33654	6.27	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080318\
Data File : VN050344.D
Acq On : 4 Aug 2018 5:04
Operator : MD\SY
Sample : J4313-06
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
C-7

Quant Time: Aug 04 05:37:47 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 26 18:10:10 2018
Response via : Initial Calibration

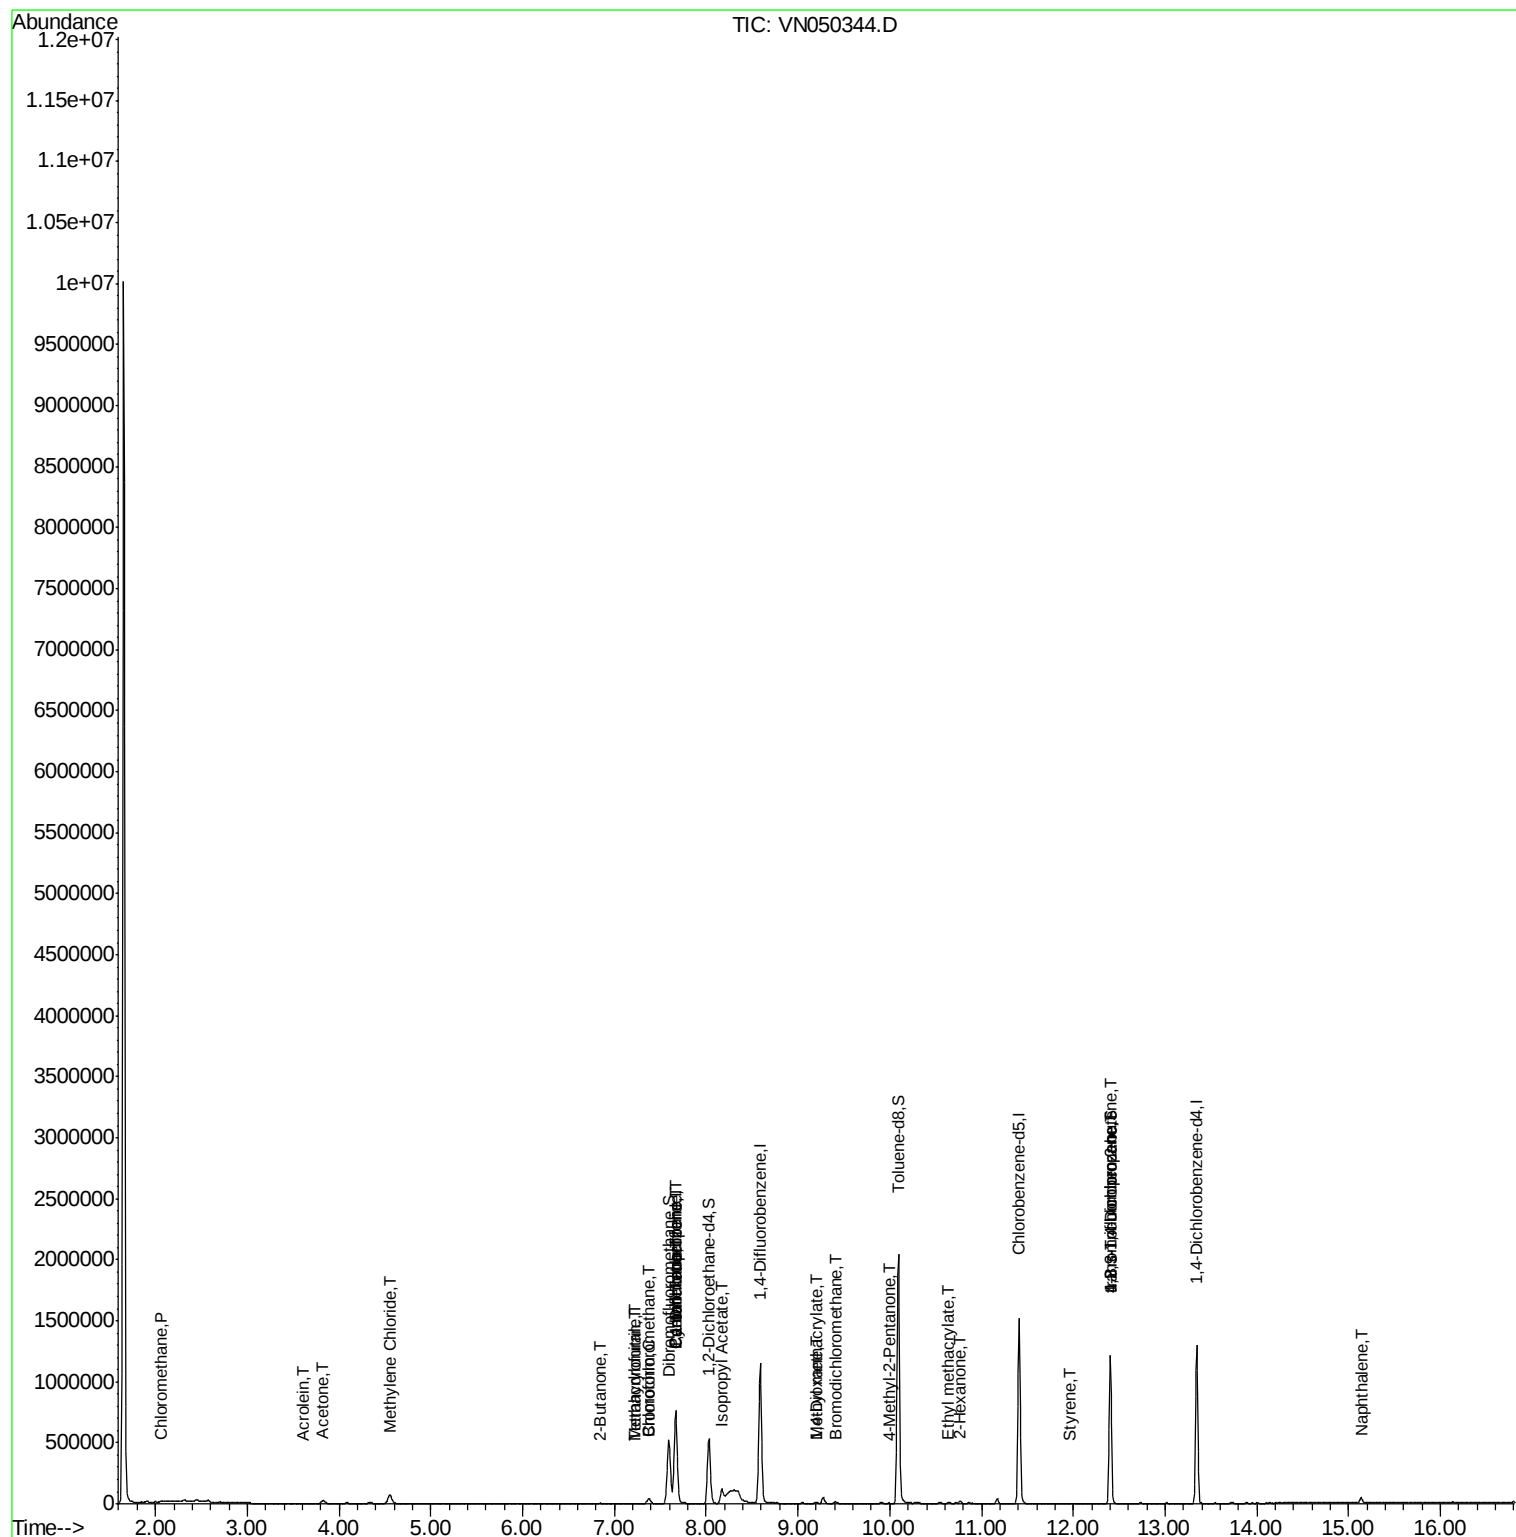

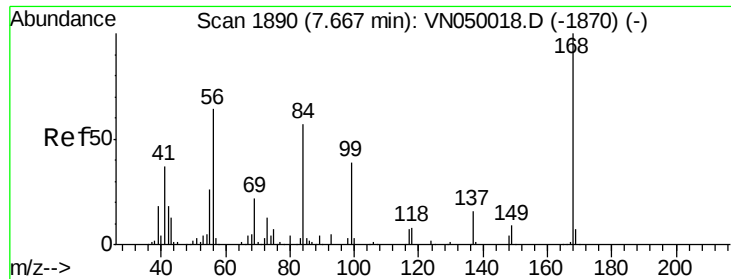

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04


Instrument :
MSVOA_N
ClientSampleId :
C-7

Tot Ion:168 Resp: 652817

Ion Ratio Lower Upper

168 100

99 51.5 40.0 60.0



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.67

250000

200000



150000

100000

50000

0

Time-->



#3

Chloromethane

Concen: 0.38 ug/l

RT: 2.06 min Scan# 145

Delta R.T. 0.00 min

Lab File: VN050344.D


Acq: 4 Aug 2018 5:04

Tgt Ion: 50 Resp: 3858

Ion Ratio Lower Upper

50 100

52 33.3 25.9 38.9



Abundance Ion 49.90 (49.60 to 50.60): VNO

Ion 51.90 (51.60 to 52.60): VNO

2.06

3000

2500

2000


1500


1000

500

0

Time-->





#5

Bromomethane

Concen: Below Cal

RT: 2.57 min Scan# 304

Delta R.T. 0.02 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04

Instrument :

MSVOA_N

ClientSampled :


C-7

Tot Ion: 94 Resp: 3991

Ion Ratio Lower Upper




94 100

96 102.3 74.6 112.0

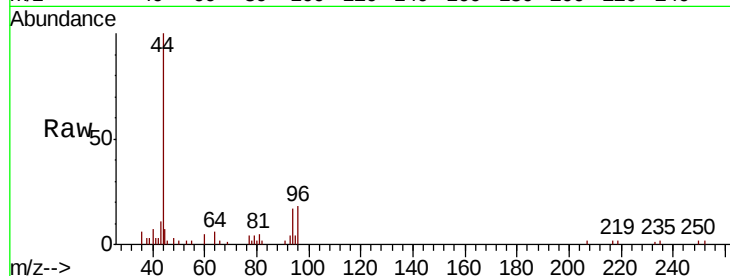

Abundance Ion 93.90 (93.60 to 94.60): VN0

Ion 95.90 (95.60 to 96.60): VN0

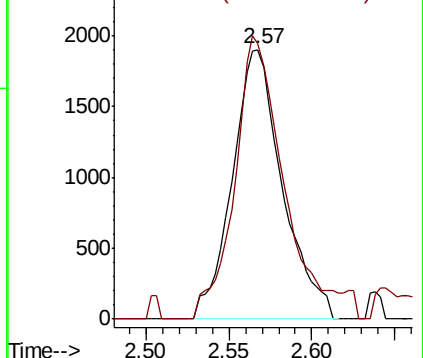

#13

Acrolein

Concen: 1.93 ug/l

RT: 3.62 min Scan# 630

Delta R.T. 0.01 min

Lab File: VN050344.D


Acq: 4 Aug 2018 5:04

Tgt Ion: 56 Resp: 1041

Ion Ratio Lower Upper



56 100


55 33.3 55.8 83.6#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

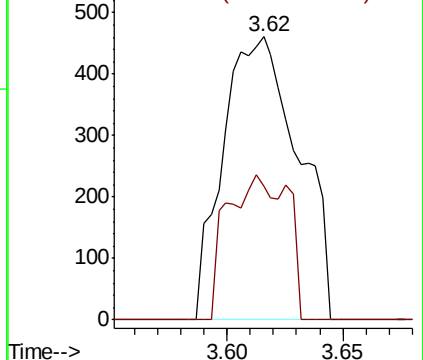



#16

Acetone

Concen: 15.96 ug/l

RT: 3.82 min Scan# 695

Delta R.T. 0.00 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04

Instrument :

MSVOA_N

ClientSampleId :


C-7

Tot Ion: 43 Resp: 42963

Ion Ratio Lower Upper




43 100

58 28.6 25.8 38.8

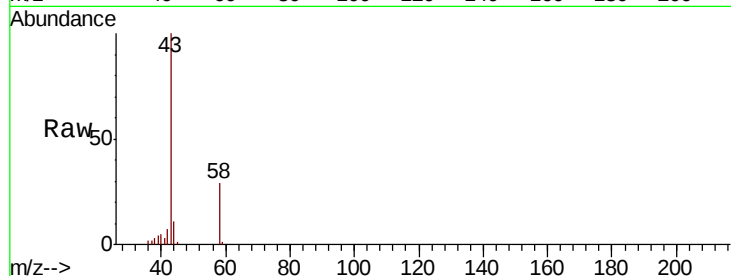

Abundance Ion 43.00 (42.70 to 43.70): VN050018.D (-676) (-)

Ion 58.00 (57.70 to 58.70): VN050018.D (-676) (-)

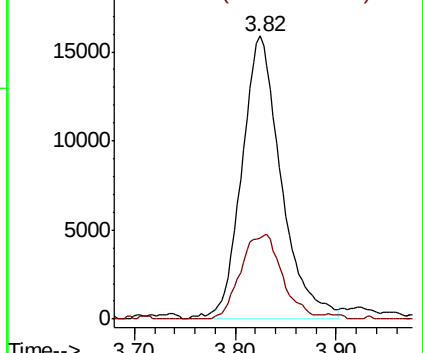

#20

Methylene Chloride

Concen: 5.65 ug/l

RT: 4.55 min Scan# 921

Delta R.T. 0.00 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04

Tgt Ion: 84 Resp: 54584


Ion Ratio Lower Upper

84 100

49 111.8 94.8 142.2

51 35.6 28.3 42.5

86 59.0 51.0 76.6






Abundance Ion 83.90 (83.60 to 84.60): VN050018.D (-896) (-)

Ion 48.90 (48.60 to 49.60): VN050018.D (-896) (-)

Ion 50.90 (50.60 to 51.60): VN050018.D (-896) (-)

Ion 85.90 (85.60 to 86.60): VN050018.D (-896) (-)




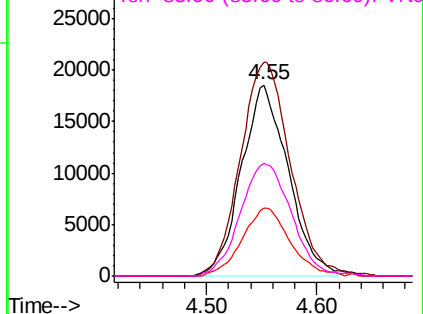




#25
2-Butanone
Concen: 1.73 ug/l
RT: 6.84 min Scan# 1634
Delta R.T. 0.00 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04




Instrument :
MSVOA_N
ClientSampled :
C-7


Tot Ion: 43 Resp: 5999
Ion Ratio Lower Upper
43 100
72 22.2 21.5 32.3

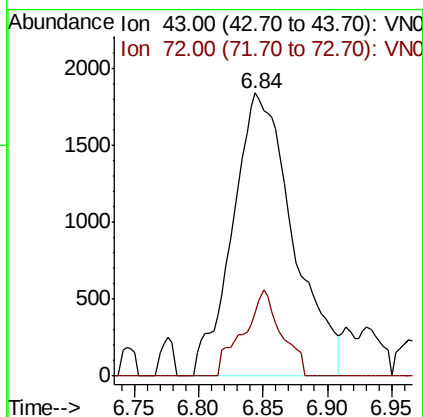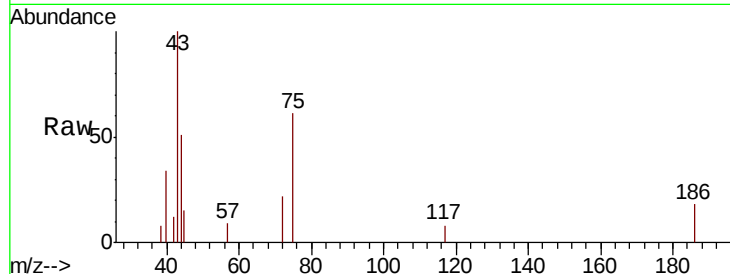

#28
Bromochloromethane
Concen: 0.49 ug/l
RT: 7.38 min Scan# 1800
Delta R.T. 0.18 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04

Tgt Ion: 49 Resp: 3367
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.0
130 0.0 66.3 99.5#

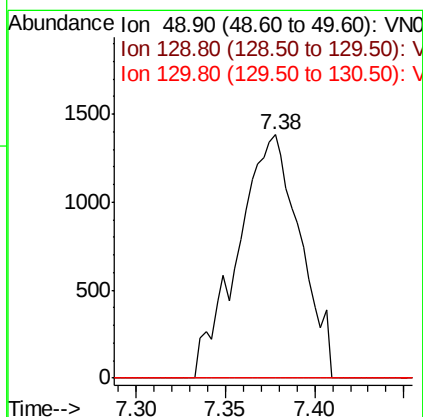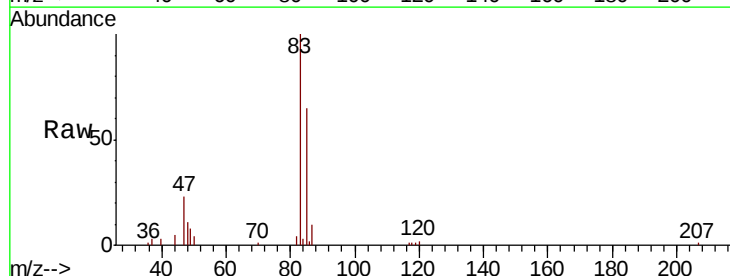



#29

Tetrahydrofuran

Concen: 0.58 ug/l

RT: 7.22 min Scan# 1751

Delta R.T. 0.00 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04

Instrument :

MSVOA_N

ClientSampled :

C-7





Tot Ion: 42 Resp: 1295

Ion Ratio Lower Upper

42 100

72 16.5 35.9 53.9#

71 4.6 33.7 50.5#

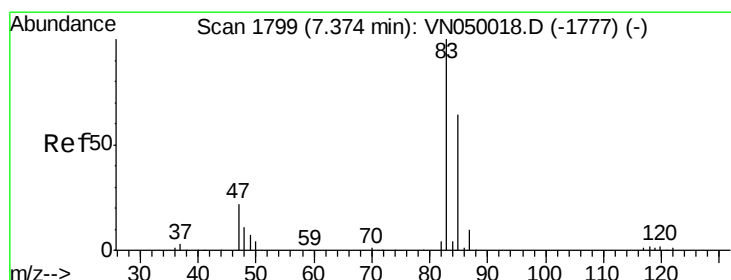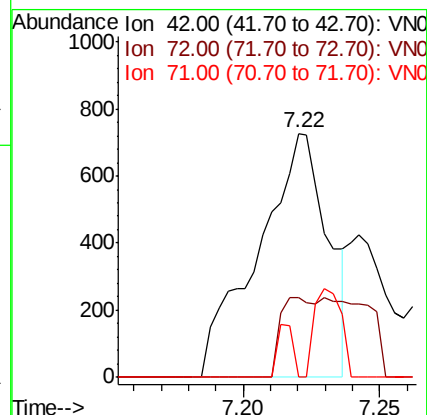

#30

Chloroform

Concen: 2.88 ug/l

RT: 7.37 min Scan# 1799

Delta R.T. 0.00 min

Lab File: VN050344.D




Acq: 4 Aug 2018 5:04


Tgt Ion: 83 Resp: 44439

Ion Ratio Lower Upper

83 100

85 66.3 52.5 78.7

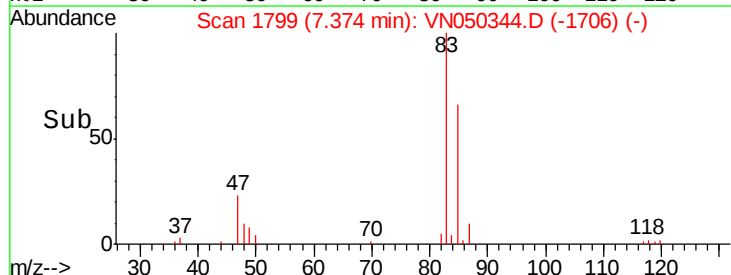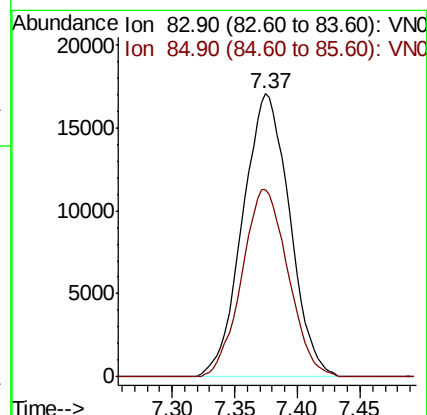







#31
Cyclohexane
Concen: 0.90 ug/l
RT: 7.67 min Scan# 1890
Delta R.T. 0.01 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04

Instrument :
MSVOA_N
ClientSampled :
C-7

Tot Ion: 56 Resp: 12172
Ion Ratio Lower Upper
56 100
69 188.0 26.2 39.4#
84 151.0 67.4 101.0#

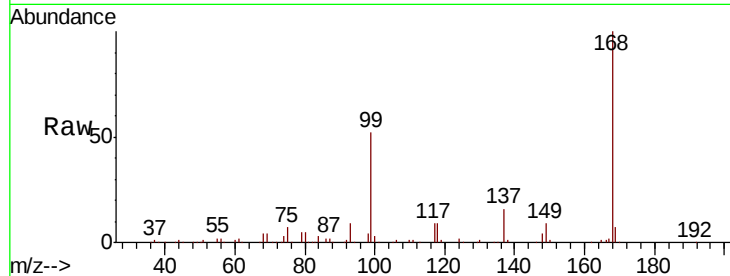


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0


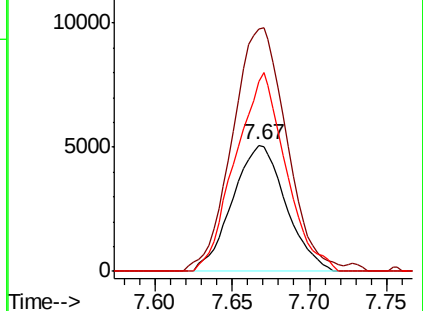



#33
1,2-Dichloroethane-d4
Concen: 50.14 ug/l
RT: 8.03 min Scan# 2003
Delta R.T. 0.00 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04

Tgt Ion: 65 Resp: 456688
Ion Ratio Lower Upper
65 100
67 53.3 0.0 108.4



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

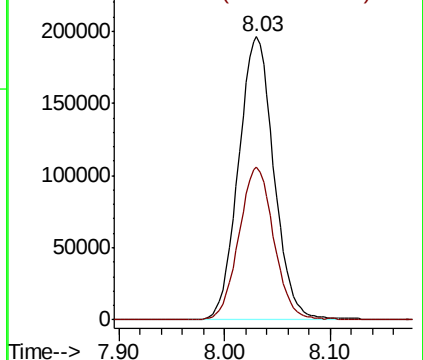







#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2177
 Delta R.T. 0.00 min
 Lab File: VN050344.D
 Acq: 4 Aug 2018 5:04

Instrument :
 MSVOA_N
 ClientSampleId :
 C-7

Tot Ion:114 Resp: 1072362




Ion	Ratio	Lower	Upper
114	100		
63	19.5	0.0	40.0
88	15.2	0.0	31.2

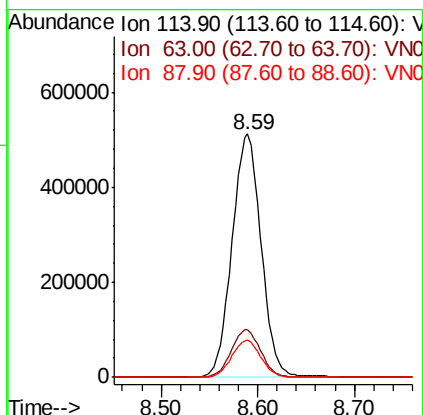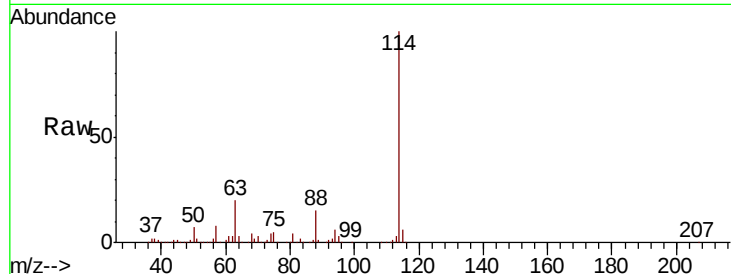


#35
 Dibromofluoromethane
 Concen: 46.33 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. 0.00 min
 Lab File: VN050344.D
 Acq: 4 Aug 2018 5:04

Tgt Ion:113 Resp: 405663

Ion	Ratio	Lower	Upper
113	100		
111	102.6	80.7	121.1
192	22.0	17.8	26.6



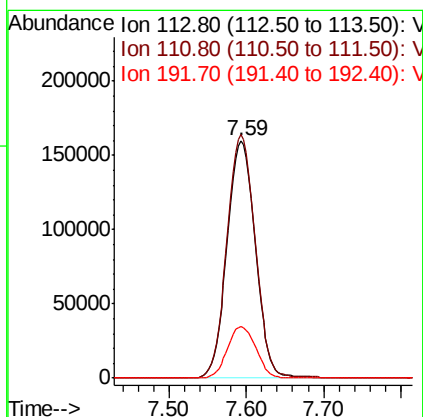
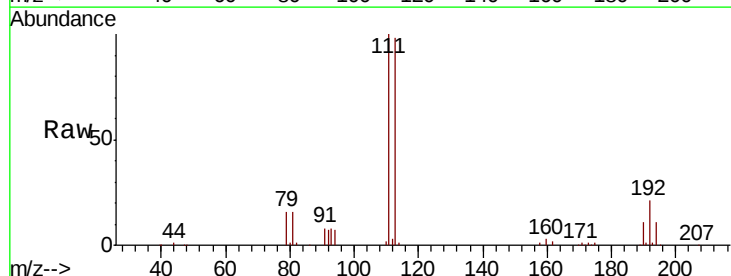


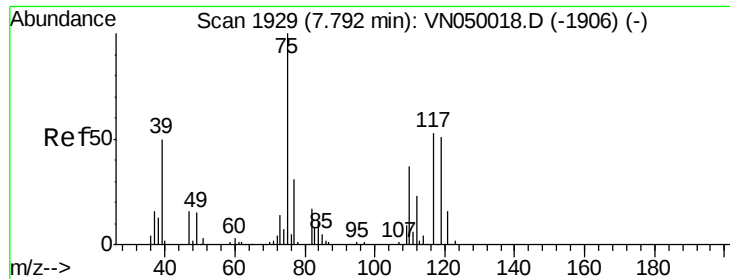

#36
 1,1-Dichloropropene
 Concen: 3.76 ug/l
 RT: 7.67 min Scan# 1890
 Delta R.T. -0.13 min
 Lab File: VN050344.D
 Acq: 4 Aug 2018 5:04




Instrument :
 MSVOA_N
 ClientSampled :
 C-7


Tot Ion	75	Resp	45380
Ion Ratio	Lower	Upper	
75	100		
110	8.9	18.4	55.2#
77	0.0	25.3	37.9#

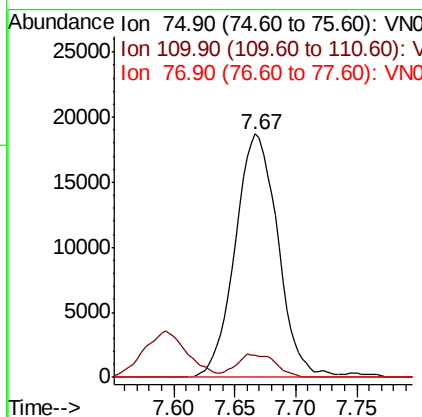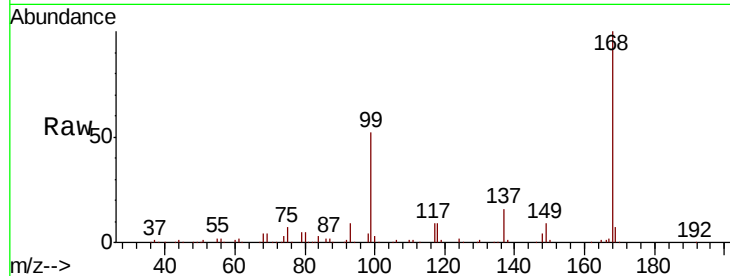

#38
 Carbon Tetrachloride
 Concen: 4.45 ug/l
 RT: 7.67 min Scan# 1891
 Delta R.T. -0.11 min
 Lab File: VN050344.D
 Acq: 4 Aug 2018 5:04

Tgt Ion	117	Resp	57100
Ion Ratio	Lower	Upper	
117	100		
119	6.2	77.4	116.0#
121	0.0	23.9	35.9#



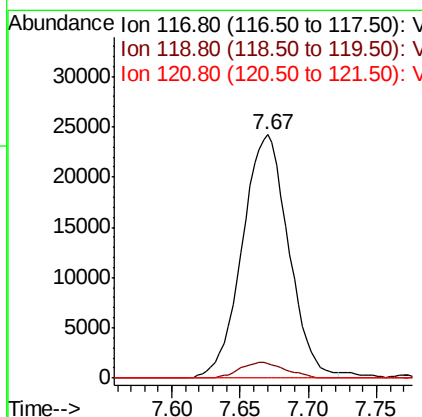



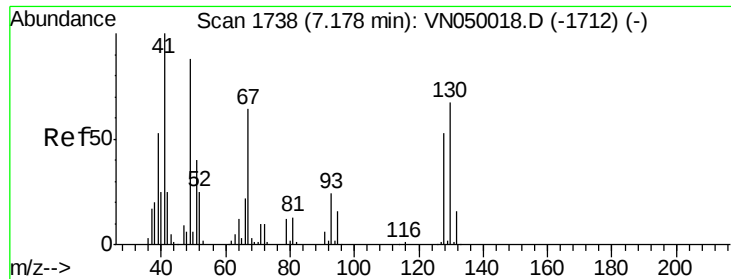

#41
Methacrylonitrile
Concen: 2.88 ug/l
RT: 7.22 min Scan# 1752
Delta R.T. 0.05 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04




Instrument :
MSVOA_N
ClientSampled :
C-7


Tot Ion: 41 Resp: 605
Ion Ratio Lower Upper
41 100
39 43.1 55.8 83.6#
67 0.0 84.3 126.5#
52 0.0 34.2 51.2#

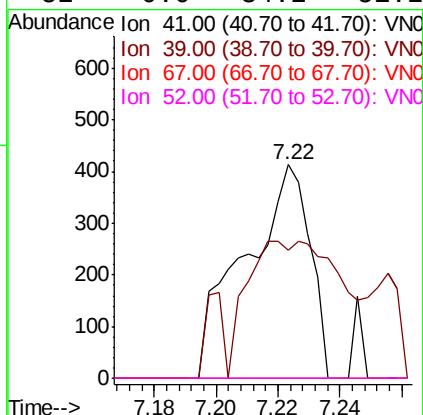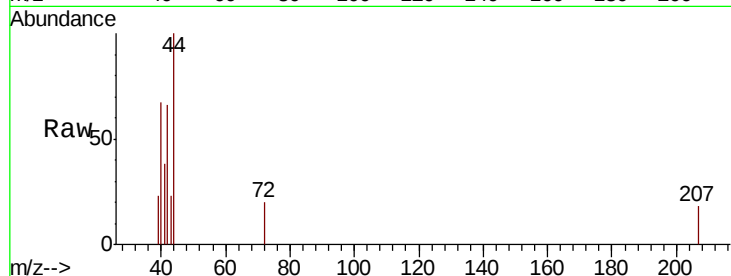

#43
Isopropyl Acetate
Concen: 8.04 ug/l
RT: 8.17 min Scan# 2047
Delta R.T. 0.00 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04

Tgt Ion: 43 Resp: 142814
Ion Ratio Lower Upper
43 100
61 15.8 15.8 23.6
87 10.2 10.3 15.5#

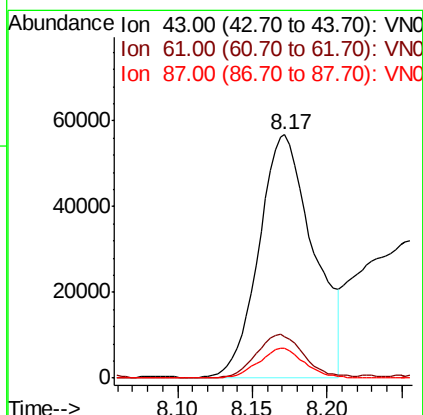

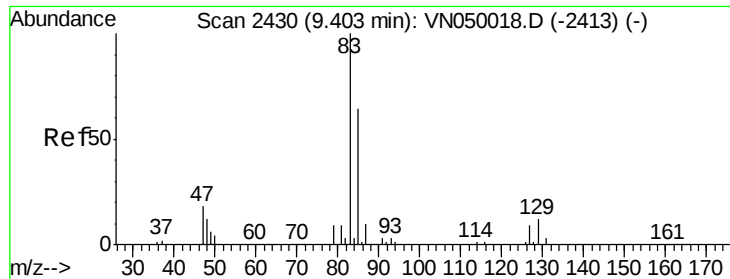

#47

Bromodichloromethane

Concen: 0.71 ug/l

RT: 9.40 min Scan# 2430

Delta R.T. -0.00 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04

Instrument :
MSVOA_N
ClientSampled :
C-7


Tot Ion: 83 Resp: 9082

Ion Ratio Lower Upper




83 100

85 55.2 51.1 76.7

127 7.9 7.0 10.4

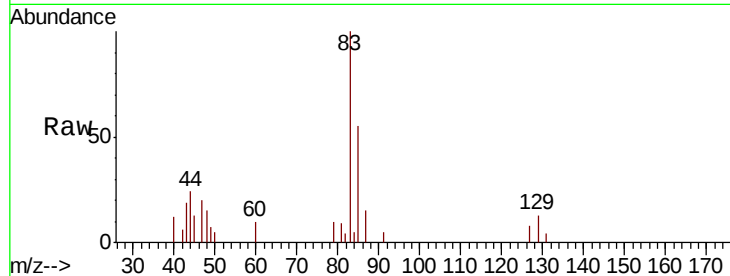

Abundance Ion 82.90 (82.60 to 83.60): VN0
Ion 84.90 (84.60 to 85.60): VN0
Ion 126.80 (126.50 to 127.50): V

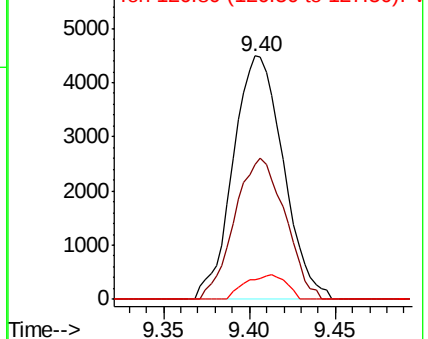

#48

Methyl methacrylate

Concen: 0.40 ug/l

RT: 9.18 min Scan# 2362

Delta R.T. -0.02 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04


Tgt Ion: 41 Resp: 2938

Ion Ratio Lower Upper



41 100


69 0.0 70.6 105.8#

39 25.4 43.9 65.9#



Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0

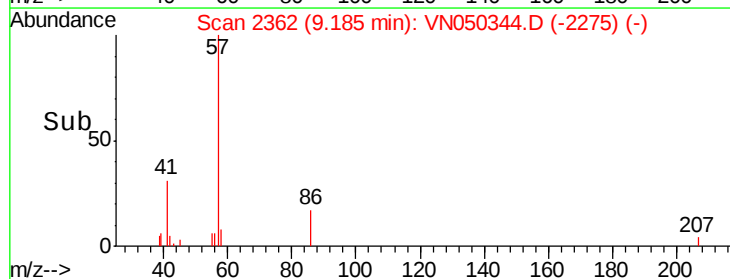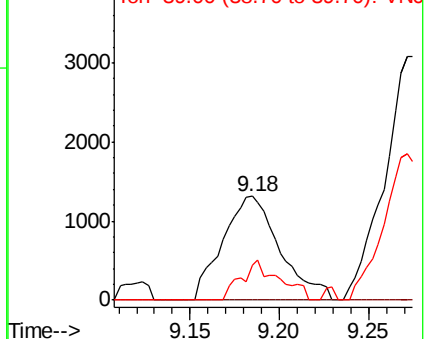


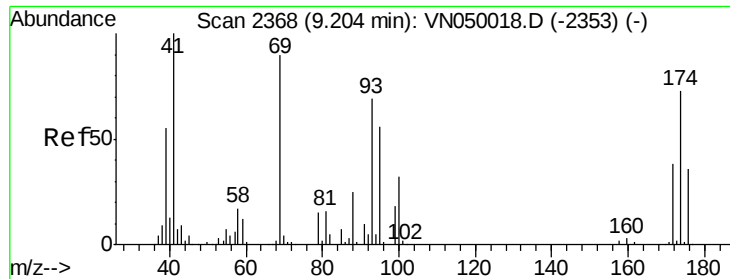




#49
1,4-Dioxane
Concen: 0.61 ug/l
RT: 9.20 min Scan# 2368
Delta R.T. 0.00 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04

Instrument :
MSVOA_N
ClientSampled :
C-7

Tot Ion: 88 Resp: 60
Ion Ratio Lower Upper
88 100
43 0.0 26.9 40.3#
58 298.3 57.3 85.9#

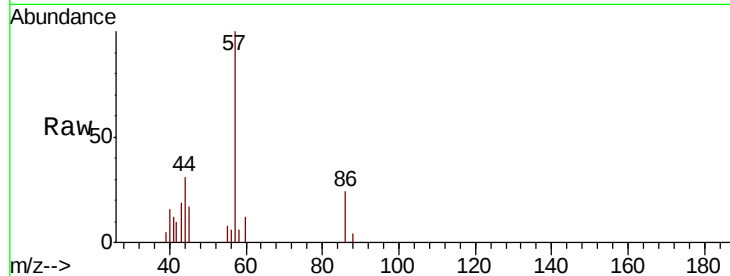


Abundance Ion 88.00 (87.70 to 88.70): VN0
Ion 43.00 (42.70 to 43.70): VN0
Ion 58.00 (57.70 to 58.70): VN0


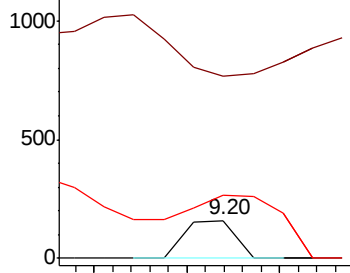



#50
Toluene-d8
Concen: 45.42 ug/l
RT: 10.09 min Scan# 2645
Delta R.T. 0.00 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04

Tgt Ion: 98 Resp: 1461943
Ion Ratio Lower Upper
98 100
100 62.9 50.7 76.1



Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0

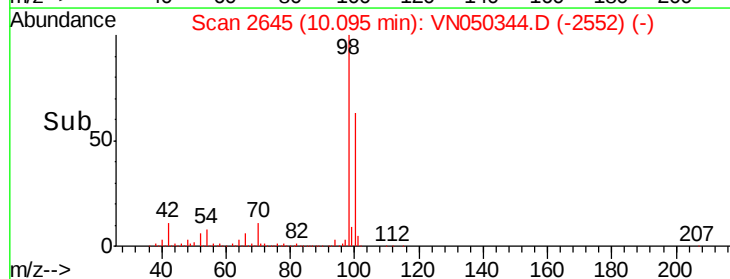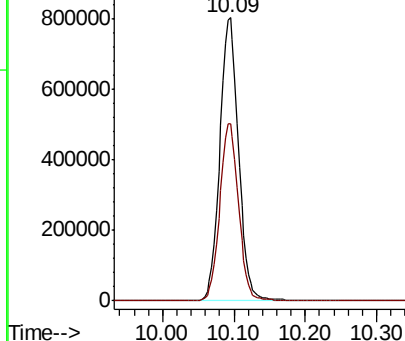



#51

4-Methyl-2-Pentanone

Concen: 0.32 ug/l

RT: 9.99 min Scan# 2613

Delta R.T. 0.00 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04

Instrument :

MSVOA_N

ClientSampled :


C-7

Tot Ion: 43 Resp: 2651

Ion Ratio Lower Upper




43 100

58 14.9 31.9 47.9#

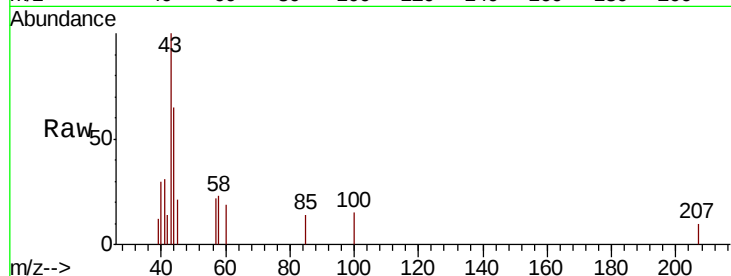

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

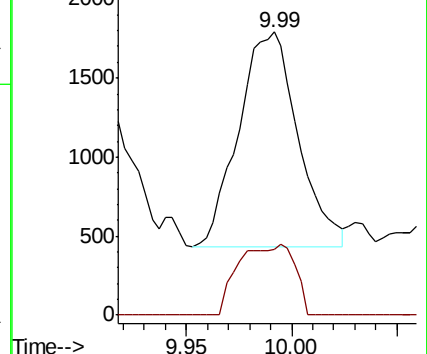

#56

Ethyl methacrylate

Concen: 2.05 ug/l

RT: 10.63 min Scan# 2813

Delta R.T. 0.20 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04


Tgt Ion: 69 Resp: 191

Ion Ratio Lower Upper

69 100

41 1007.9 51.0 76.4#



39 473.8 26.6 40.0#




Abundance Ion 69.00 (68.70 to 69.70): VN0

Ion 41.00 (40.70 to 41.70): VN0

Ion 39.00 (38.70 to 39.70): VN0



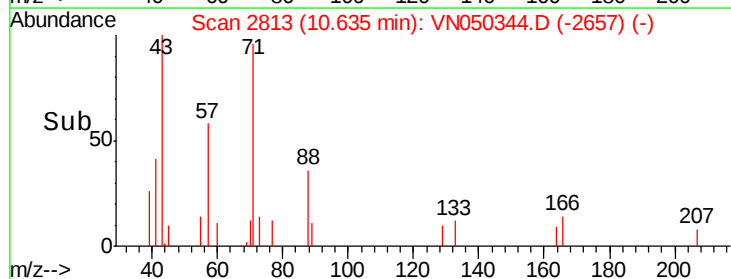
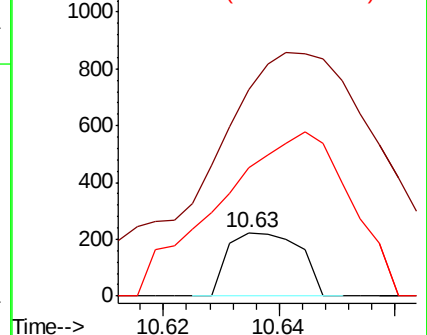




#59
2-Hexanone
Concen: 5.72 ug/l
RT: 10.77 min Scan# 2854
Delta R.T. 0.01 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04




Instrument :
MSVOA_N
ClientSampled :
C-7


Tot Ion: 43 Resp: 3416
Ion Ratio Lower Upper
43 100
58 21.7 27.6 82.7#

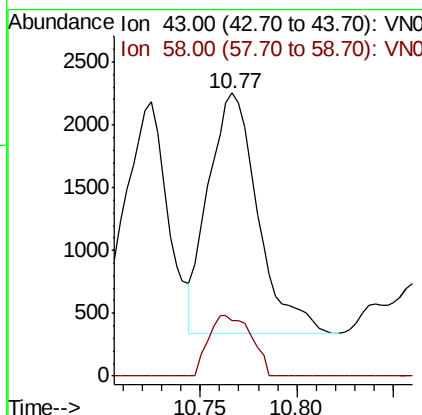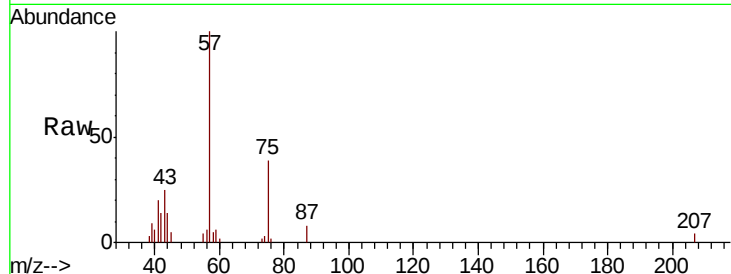

#62
4-Bromofluorobenzene
Concen: 38.79 ug/l
RT: 12.40 min Scan# 3363
Delta R.T. 0.00 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04

Tgt Ion: 95 Resp: 411085
Ion Ratio Lower Upper
95 100
174 91.5 0.0 178.2
176 87.0 0.0 173.4



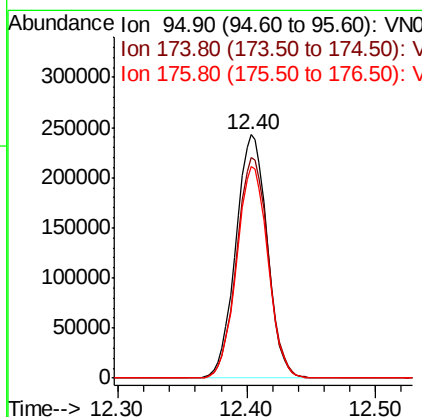
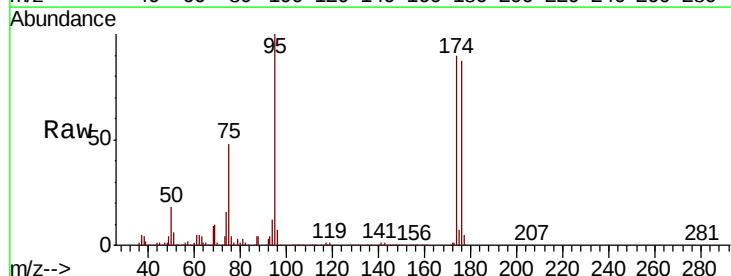


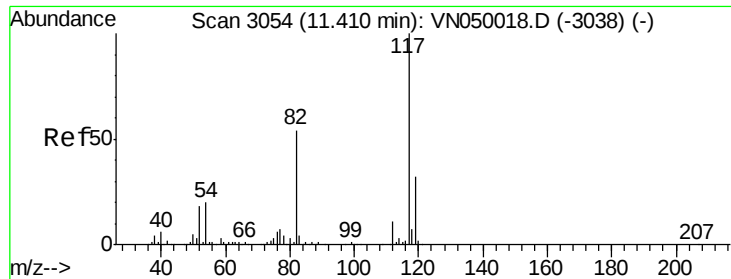

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. 0.00 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04




Instrument :
MSVOA_N
ClientSampleId :
C-7


Tot Ion	Ratio	Lower	Upper
117	100		
82	53.5	43.7	65.5
119	32.6	26.1	39.1

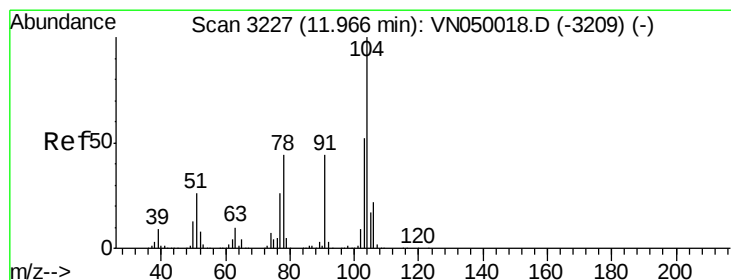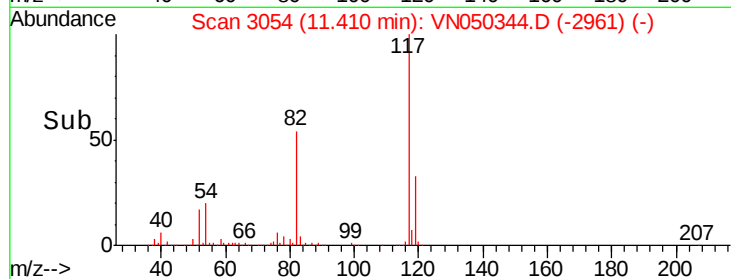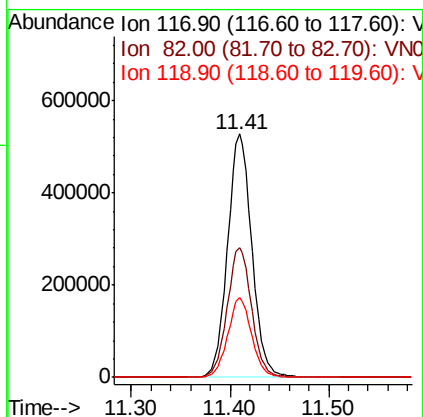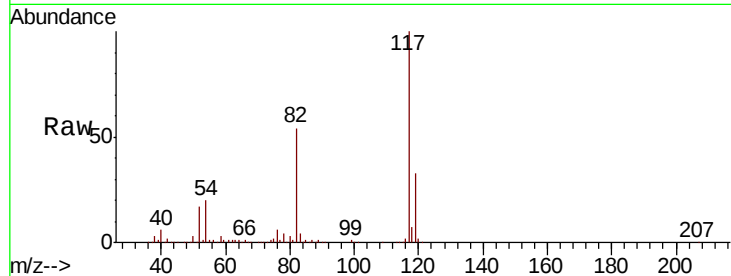

#70
Styrene
Concen: 0.93 ug/l
RT: 11.97 min Scan# 3229
Delta R.T. 0.01 min
Lab File: VN050344.D
Acq: 4 Aug 2018 5:04

Tgt Ion	Ratio	Lower	Upper
104	100		
78	0.0	39.3	58.9#
103	0.0	45.0	67.6#

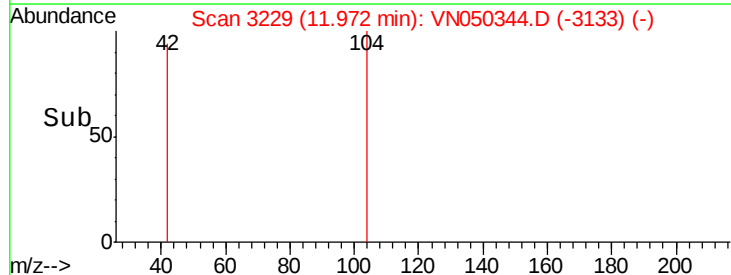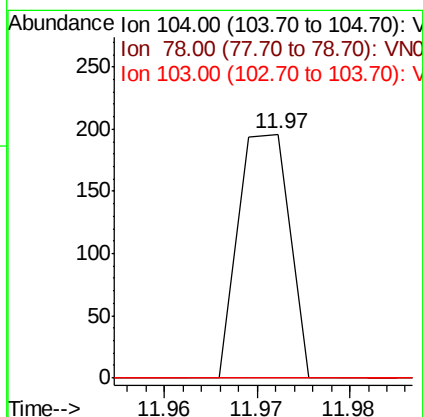



#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.35 min Scan# 3656

Delta R.T. 0.00 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04

Instrument :

MSVOA_N

ClientSampleId :

C-7


Tot Ion:152 Resp: 362002

Ion Ratio Lower Upper

152 100

115 55.7 27.8 83.3




150 157.3 0.0 348.6

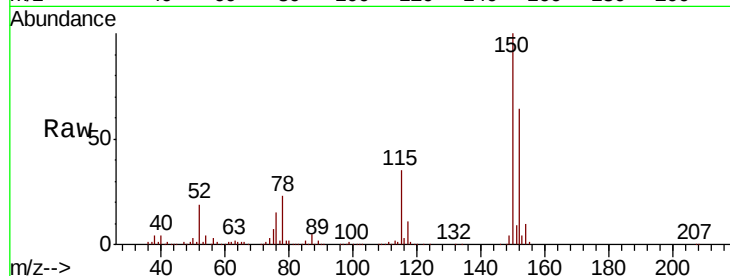

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

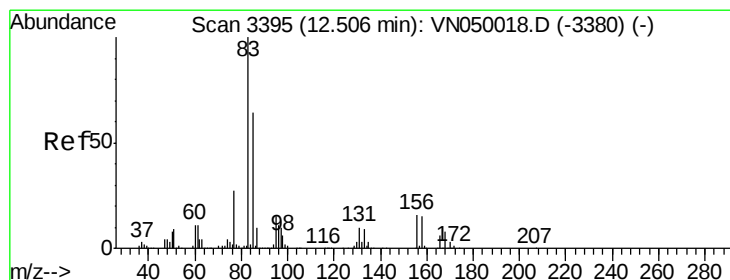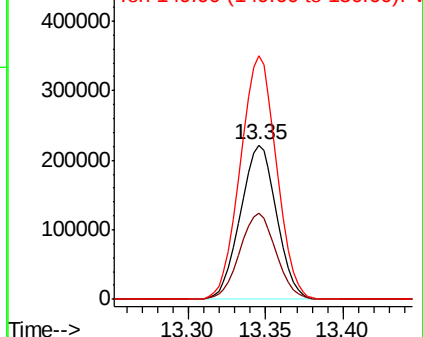

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.40 min Scan# 3361

Delta R.T. -0.11 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04


Tgt Ion: 83 Resp: 214

Ion Ratio Lower Upper

83 100

131 237.9 5.1 15.3#



85 0.0 32.3 96.8#




Abundance Ion 82.90 (82.60 to 83.60): VNO

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): VNO

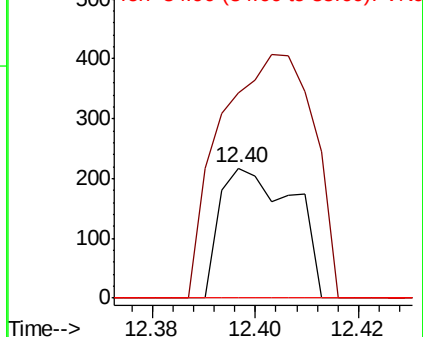



#76

1,2,3-Trichloropropane

Concen: 30.06 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. -0.15 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04

Instrument :

MSVOA_N

ClientSampled :





C-7

Tot Ion: 75 Resp: 202212

Ion Ratio Lower Upper

75 100

77 1.3 0.0 0.0#

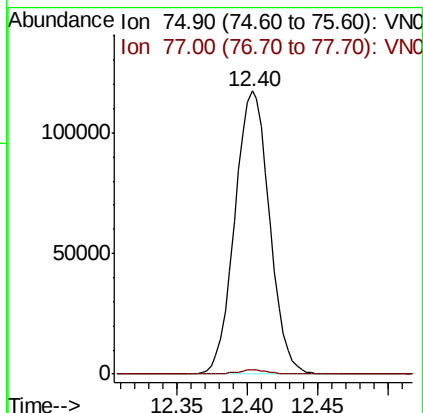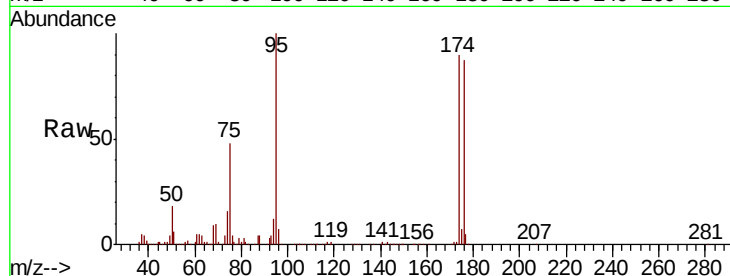

#81

trans-1,4-Dichloro-2-butene

Concen: 95.34 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.10 min

Lab File: VN050344.D

Acq: 4 Aug 2018 5:04




Tgt Ion: 75 Resp: 202212


Ion Ratio Lower Upper

75 100

53 0.3 73.5 110.3#

89 0.0 36.0 54.0#



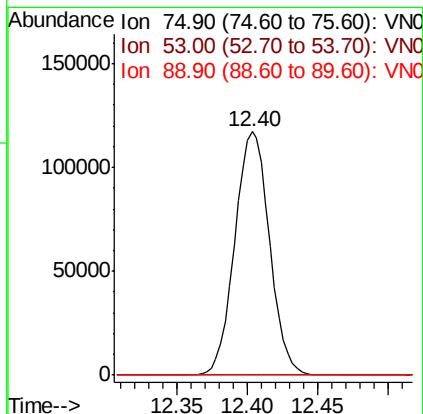





#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 14.50 min Scan# 4016
 Delta R.T. 0.23 min
 Lab File: VN050344.D
 Acq: 4 Aug 2018 5:04

Instrument :
 MSVOA_N
 ClientSampleId :
 C-7

Tot Ion: 75 Resp: 32
 Ion Ratio Lower Upper
 75 100
 155 0.0 44.8 134.4#
 157 0.0 57.2 171.6#

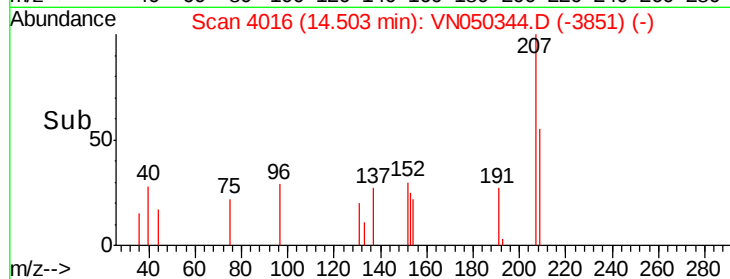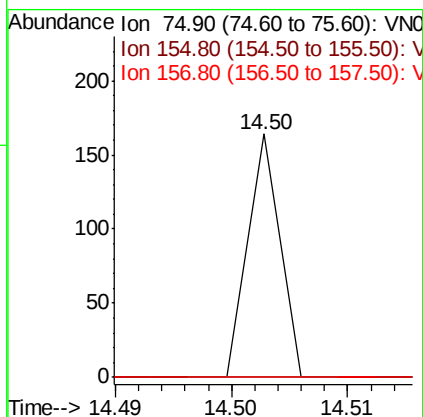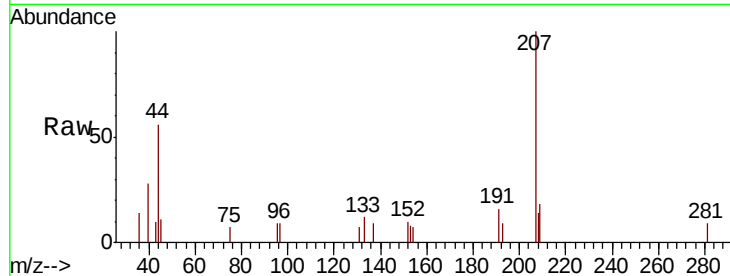

#95
 Naphthalene
 Concen: 6.27 ug/l
 RT: 15.14 min Scan# 4213
 Delta R.T. 0.00 min
 Lab File: VN050344.D
 Acq: 4 Aug 2018 5:04

Tgt Ion: 128 Resp: 33654
 Ion Ratio Lower Upper
 128 100
 127 13.0 10.4 15.6
 129 11.0 8.8 13.2

