

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080318\  
 Data File : VN050345.D  
 Acq On : 4 Aug 2018 5:29  
 Operator : MD\SY  
 Sample : J4313-08  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8

Quant Time: Aug 04 06:41:14 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N072418W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Jul 26 18:10:10 2018  
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	677158	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1125221	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	982474	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	424351	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	479943	50.80	ug/l	0.00
Spiked Amount				50.000		
Recovery				=		101.60%
35) Dibromofluoromethane	7.59	113	417956	45.49	ug/l	0.00
Spiked Amount				50.000		
Recovery				=		90.98%
50) Toluene-d8	10.09	98	1542214	45.66	ug/l	0.00
Spiked Amount				50.000		
Recovery				=		91.32%
62) 4-Bromofluorobenzene	12.40	95	465481	41.85	ug/l	0.00
Spiked Amount				50.000		
Recovery				=		83.70%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.06	50	3670	0.35	ug/l	100
5) Bromomethane	2.56	94	3922	Below Cal		98
13) Acrolein	3.60	56	286	0.51	ug/l #	36
14) Allyl chloride	4.55	41	4751	0.39	ug/l #	24
16) Acetone	3.82	43	43720	15.57	ug/l	94
18) Methyl Acetate	4.34	43	12862	Below Cal		97
20) Methylene Chloride	4.55	84	121862	13.64	ug/l	99
25) 2-Butanone	6.84	43	4939	1.37	ug/l #	85
28) Bromochloromethane	7.37	49	2404	0.34	ug/l #	10
30) Chloroform	7.37	83	34096	2.13	ug/l	97
31) Cyclohexane	7.67	56	12253	0.87	ug/l #	1
36) 1,1-Dichloropropene	7.67	75	48282	3.81	ug/l #	48
37) Ethyl Acetate	6.84	43	4939	0.56	ug/l #	67
38) Carbon Tetrachloride	7.67	117	60769	4.52	ug/l #	17
41) Methacrylonitrile	7.20	41	152	2.78	ug/l #	25
43) Isopropyl Acetate	8.17	43	195351	10.84	ug/l	95
47) Bromodichloromethane	9.41	83	6593	0.49	ug/l	94
48) Methyl methacrylate	9.18	41	5119	0.67	ug/l #	25
51) 4-Methyl-2-Pentanone	9.99	43	2316	0.27	ug/l #	83
56) Ethyl methacrylate	10.27	69	214	2.05	ug/l #	21
59) 2-Hexanone	10.77	43	5789	6.06	ug/l #	60
68) m/p-Xylenes	11.62	106	8241	0.55	ug/l	98
70) Styrene	11.95	104	108	0.93	ug/l #	1
71) Bromoform	12.41	173	4774	0.69	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.40	83	192	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.40	75	221175	28.05	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.73	105	9029	0.35	ug/l	96
81) trans-1,4-Dichloro-2-buten	12.40	75	221175	88.96	ug/l #	13
84) 1,2,4-Trimethylbenzene	13.04	105	24980	0.96	ug/l	98
92) 1,2-Dibromo-3-Chloropropan	14.25	75	63	Below Cal	#	1
95) Naphthalene	15.13	128	10001	4.89	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080318\  
 Data File : VN050345.D  
 Acq On : 4 Aug 2018 5:29  
 Operator : MD\SY  
 Sample : J4313-08  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 Client Sample Id :  
 C-8

Quant Time: Aug 04 06:41:14 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N072418W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Jul 26 18:10:10 2018  
 Response via : Initial Calibration




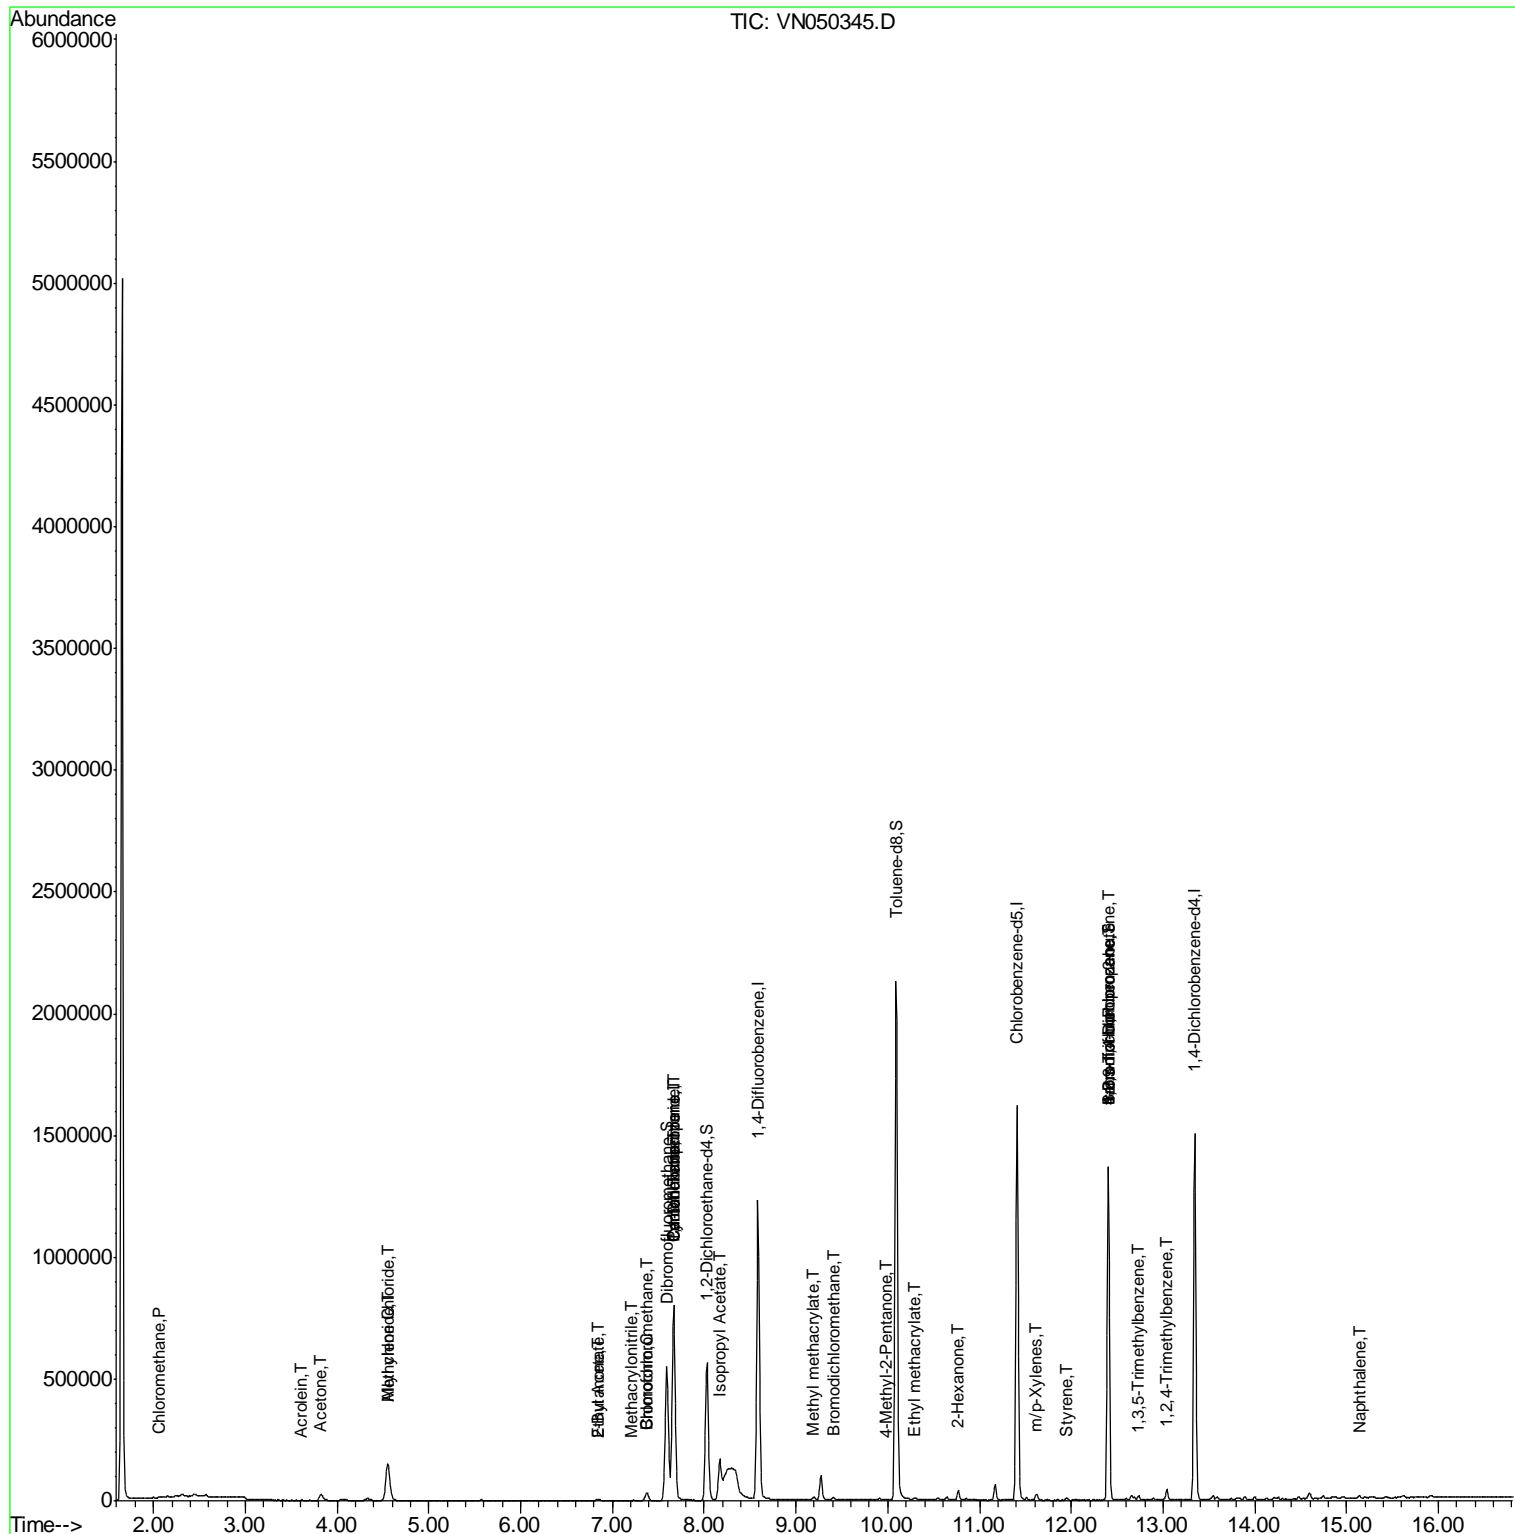




#1  
 Pentafluorobenzene  
 Concen: 50.00 ug/l  
 RT: 7.67 min Scan# 1891  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion: 168 Resp: 677158  
 Ion Ratio Lower Upper  
 168 100  
 99 51.0 40.0 60.0

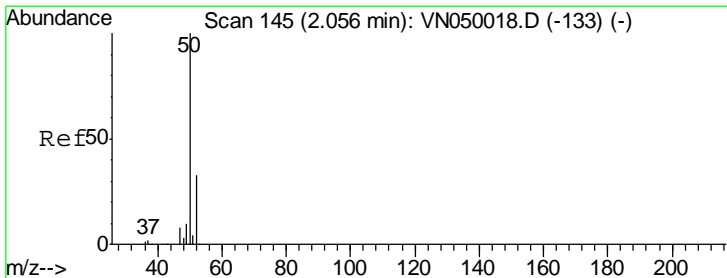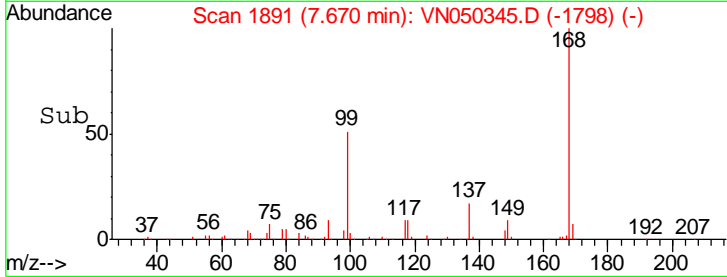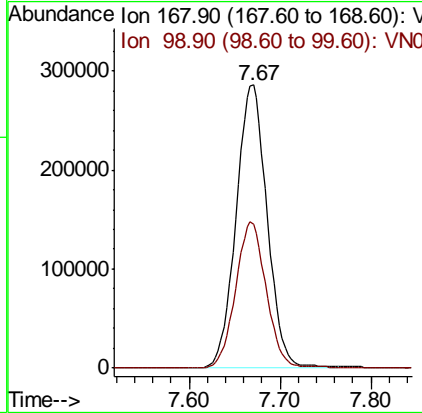

#3  
 Chloromethane  
 Concen: 0.35 ug/l  
 RT: 2.06 min Scan# 146  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion: 50 Resp: 3670  
 Ion Ratio Lower Upper  
 50 100  
 52 32.4 25.9 38.9


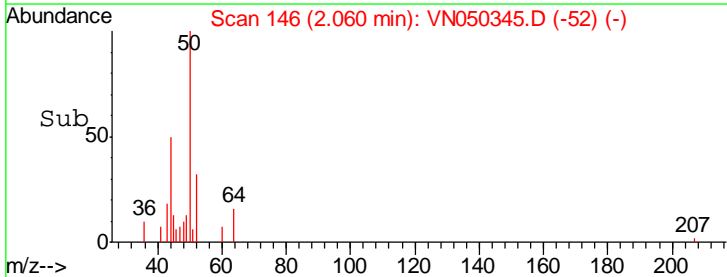
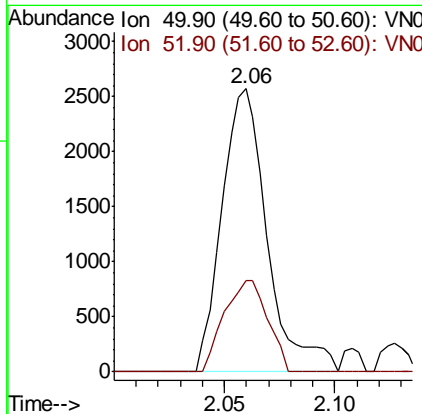
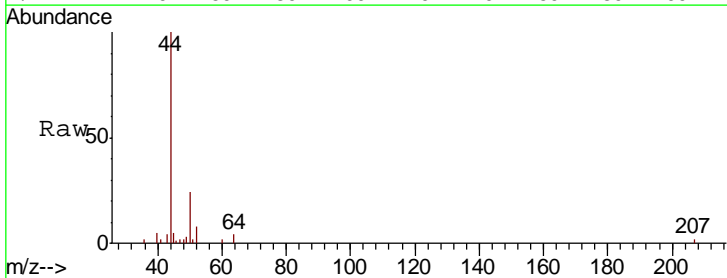




#5  
 Bromomethane  
 Concen: Below Cal  
 RT: 2.56 min Scan# 302  
 Delta R.T. 0.01 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion: 94 Resp: 3922  
 Ion Ratio Lower Upper  
 94 100  
 96 91.6 74.6 112.0

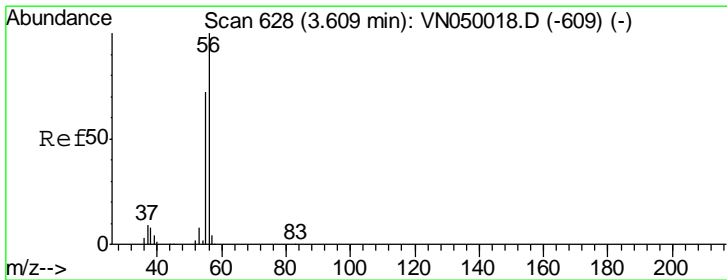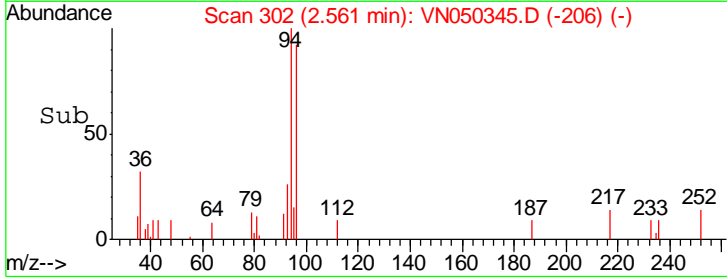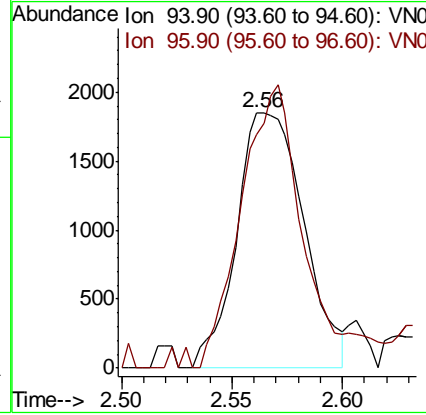

#13  
 Acrolein  
 Concen: 0.51 ug/l  
 RT: 3.60 min Scan# 625  
 Delta R.T. -0.01 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion: 56 Resp: 286  
 Ion Ratio Lower Upper  
 56 100  
 55 122.4 55.8 83.6#


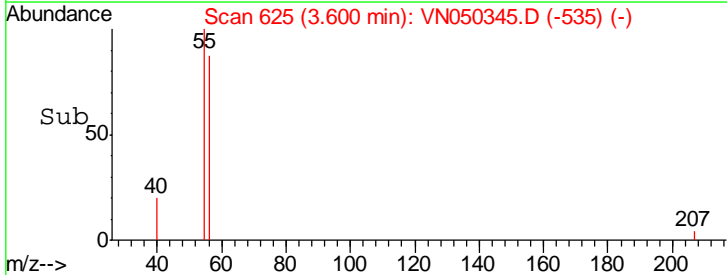
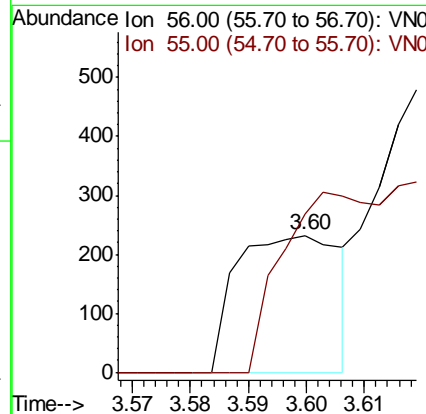
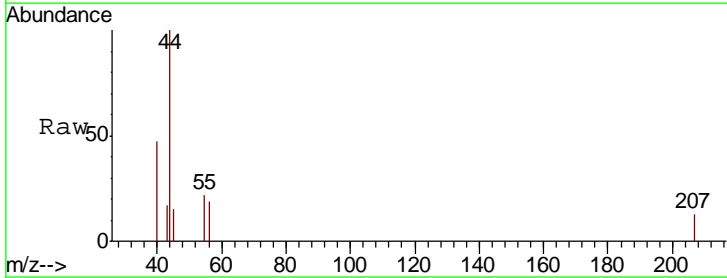


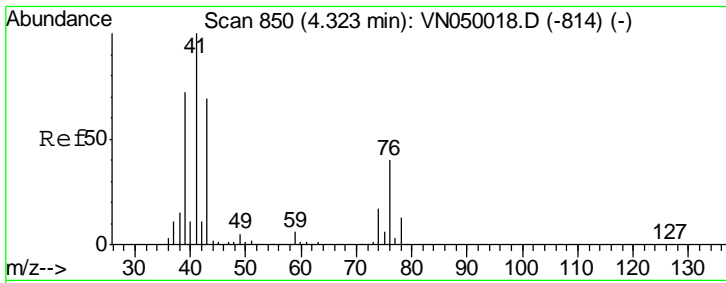

#14  
 Allvl chloride  
 Concen: 0.39 ug/l  
 RT: 4.55 min Scan# 922  
 Delta R.T. 0.23 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
41	100		
39	0.0	54.2	81.4#
76	0.0	29.0	43.6#

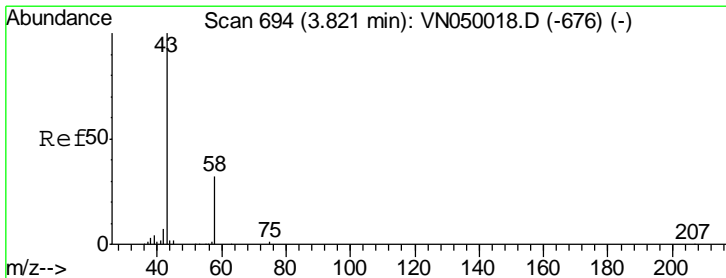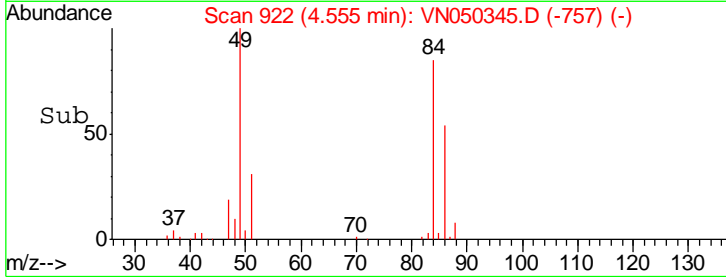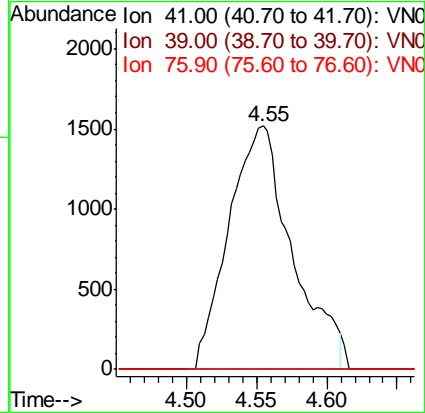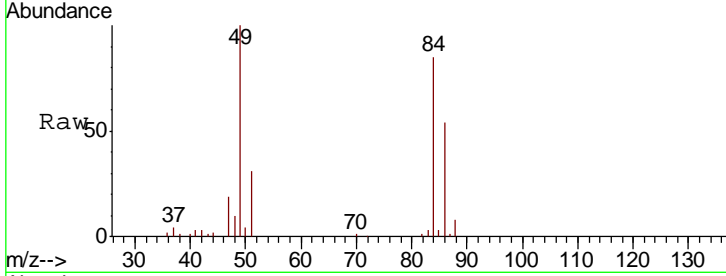

#16  
 Acetone  
 Concen: 15.57 ug/l  
 RT: 3.82 min Scan# 694  
 Delta R.T. -0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
43	100		
58	35.7	25.8	38.8

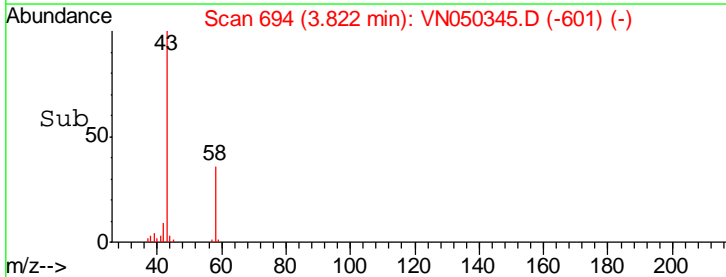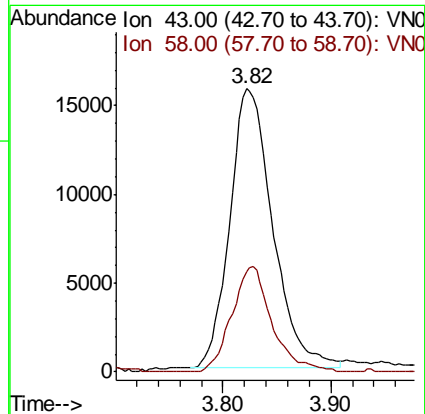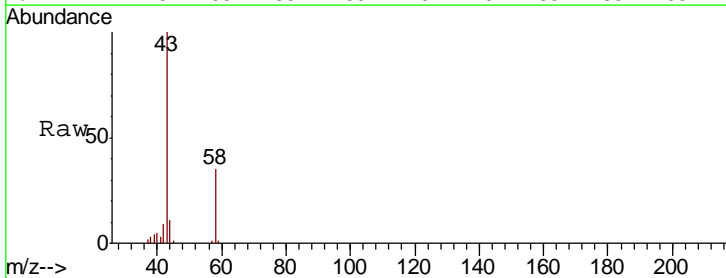


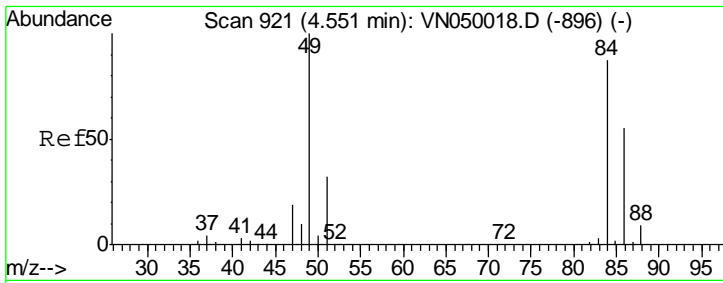




#20  
 Methylene Chloride  
 Concen: 13.64 ug/l  
 RT: 4.55 min Scan# 922  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8

Tgt Ion	Resp	Lower	Upper
84	121862		
49	118.1	94.8	142.2
51	36.8	28.3	42.5
86	64.0	51.0	76.6




Abundance Ion 83.90 (83.60 to 84.60): VNC  
 Ion 48.90 (48.60 to 49.60): VNC  
 Ion 50.90 (50.60 to 51.60): VNC  
 Ion 85.90 (85.60 to 86.60): VNC

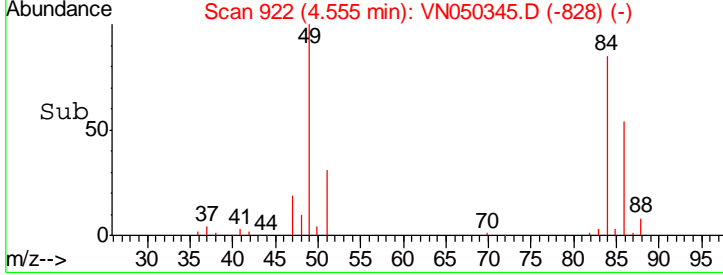
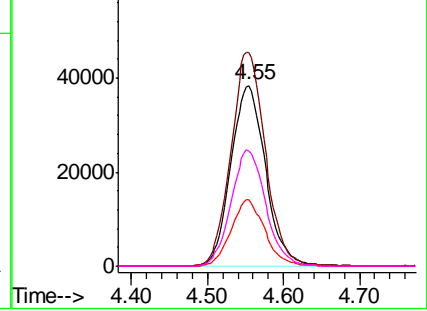



#25  
 2-Butanone  
 Concen: 1.37 ug/l  
 RT: 6.84 min Scan# 1634  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
43	4939		
72	19.3	21.5	32.3#



Abundance Ion 43.00 (42.70 to 43.70): VNC  
 Ion 72.00 (71.70 to 72.70): VNC


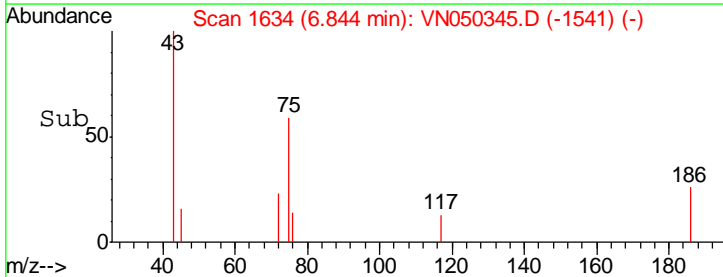
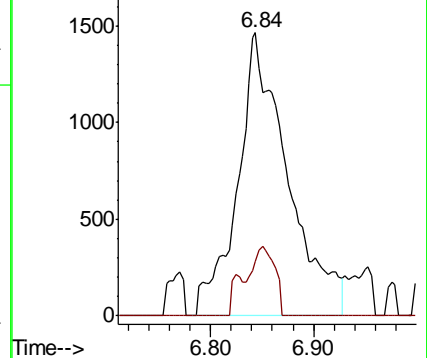




#28  
 Bromochloromethane  
 Concen: 0.34 ug/l  
 RT: 7.37 min Scan# 1798  
 Delta R.T. 0.17 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29





Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
49	100		
129	0.0	0.0	4.0
130	0.0	66.3	99.5#

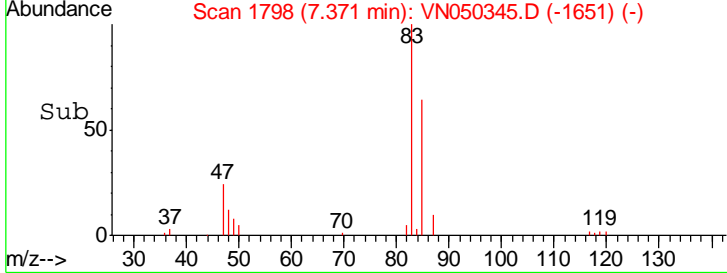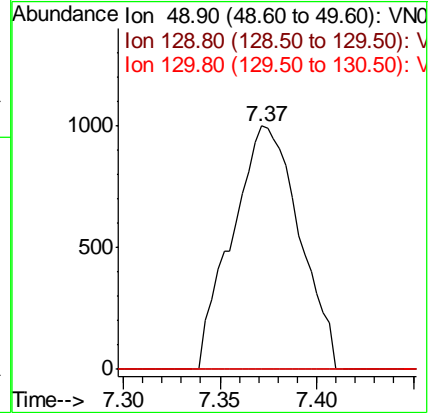

#30  
 Chloroform  
 Concen: 2.13 ug/l  
 RT: 7.37 min Scan# 1799  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
83	100		
85	68.3	52.5	78.7

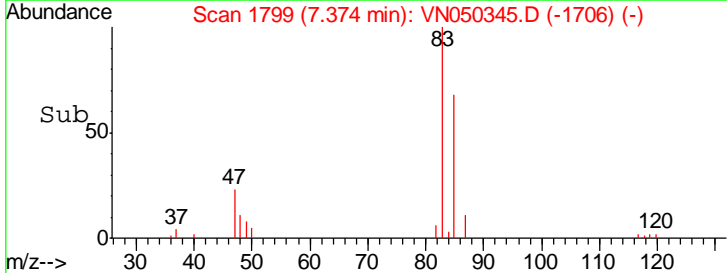

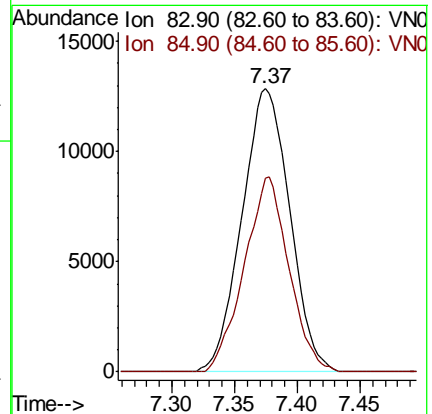
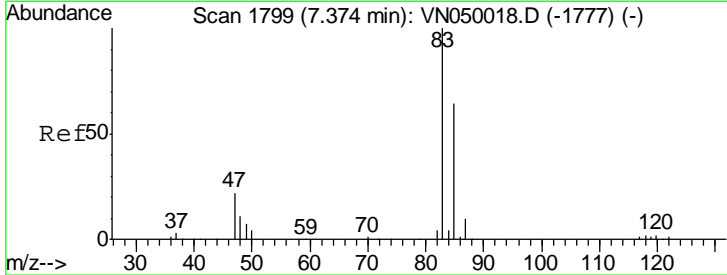




#31  
 Cyclohexane  
 Concen: 0.87 ug/l  
 RT: 7.67 min Scan# 1890  
 Delta R.T. 0.01 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8

Tgt Ion	Resp	Lower	Upper
56	12253		
69	175.9	26.2	39.4#
84	138.8	67.4	101.0#

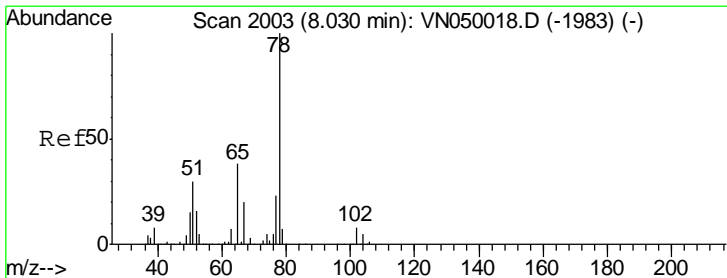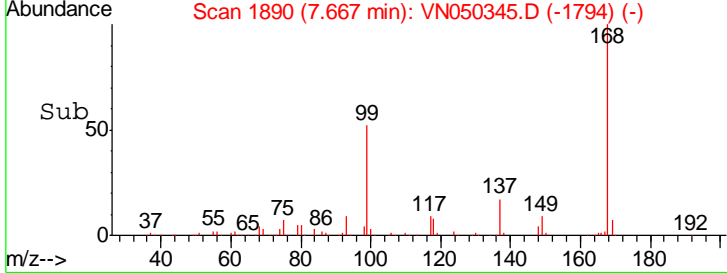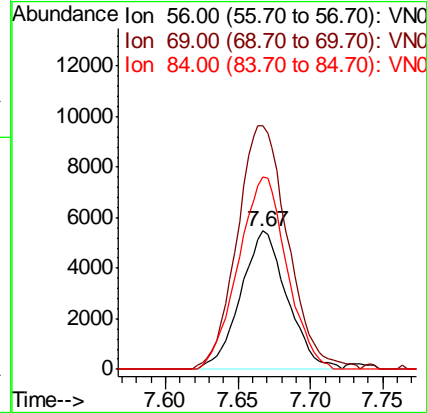


#33  
 1,2-Dichloroethane-d4  
 Concen: 50.80 ug/l  
 RT: 8.03 min Scan# 2003  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
65	479943		
67	54.0	0.0	108.4

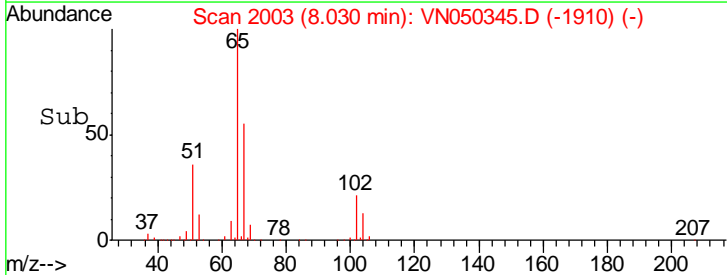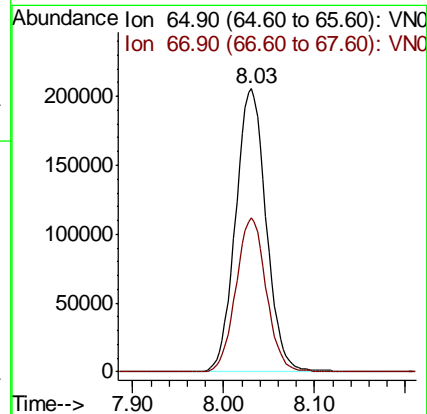









#34  
 1,4-Difluorobenzene  
 Concen: 50.00 ug/l  
 RT: 8.59 min Scan# 2176  
 Delta R.T. -0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
114	1125221		
63	19.8	0.0	40.0
88	15.2	0.0	31.2

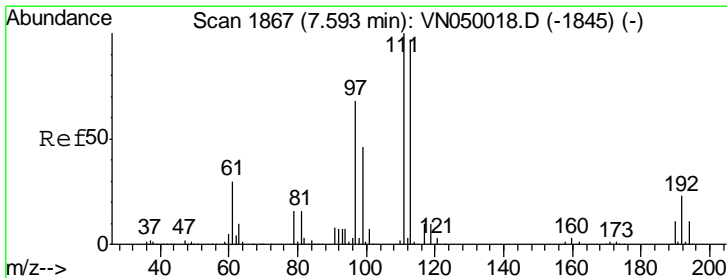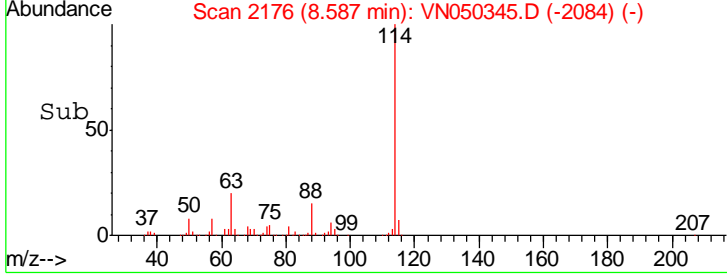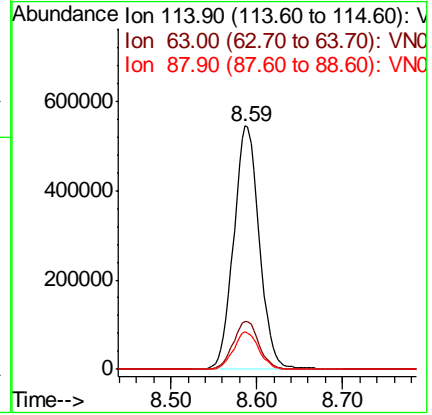

#35  
 Dibromofluoromethane  
 Concen: 45.49 ug/l  
 RT: 7.59 min Scan# 1867  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
113	417956		
111	102.9	80.7	121.1
192	22.4	17.8	26.6


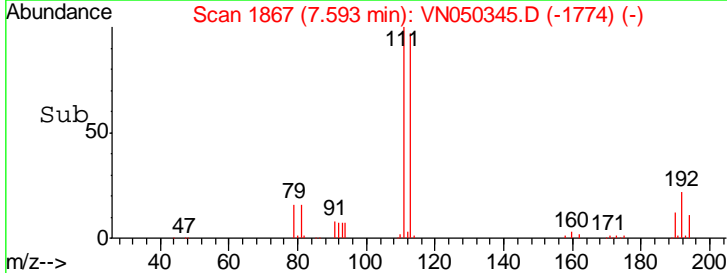
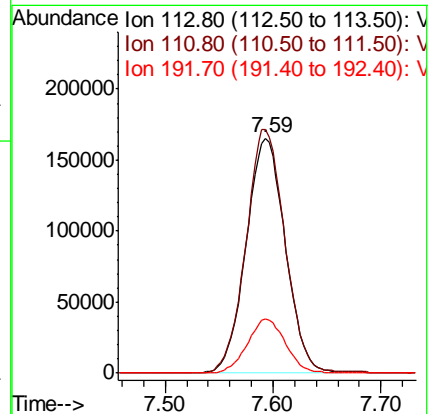
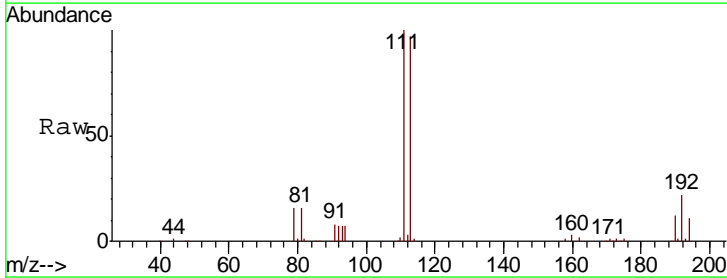




#36  
 1,1-Dichloropropene  
 Concen: 3.81 ug/l  
 RT: 7.67 min Scan# 1890  
 Delta R.T. -0.13 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
75	48282		
110	8.0	18.4	55.2#
77	0.1	25.3	37.9#

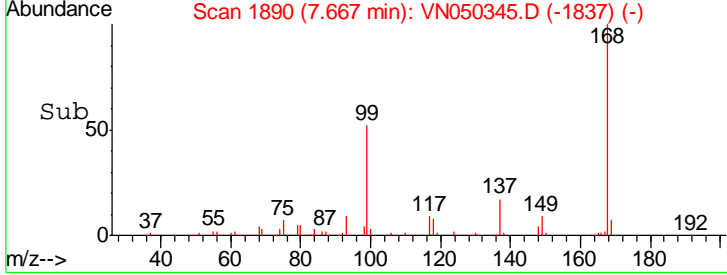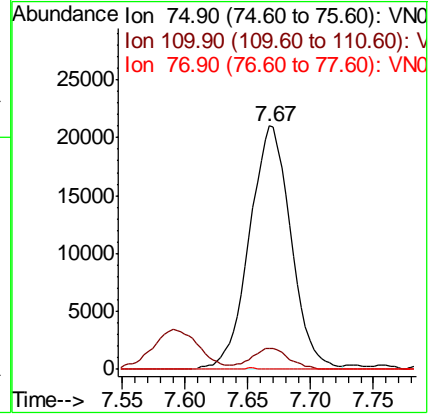

#37  
 Ethyl Acetate  
 Concen: 0.56 ug/l  
 RT: 6.84 min Scan# 1634  
 Delta R.T. -0.09 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
43	4939		
61	0.0	11.8	17.8#
70	0.0	8.4	12.6#


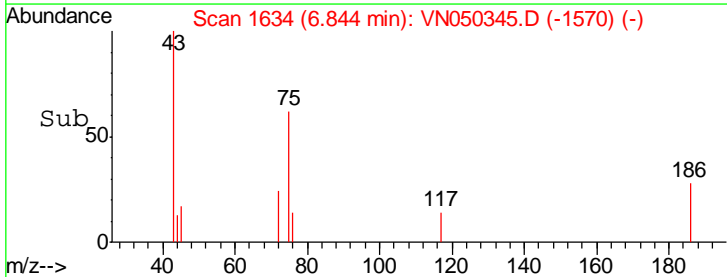
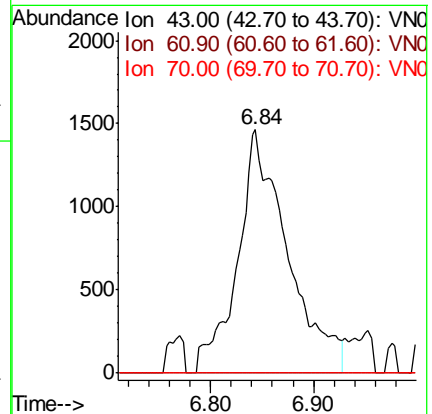





#38  
 Carbon Tetrachloride  
 Concen: 4.52 ug/l  
 RT: 7.67 min Scan# 1890  
 Delta R.T. -0.11 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
117	100		
119	7.1	77.4	116.0#
121	0.0	23.9	35.9#

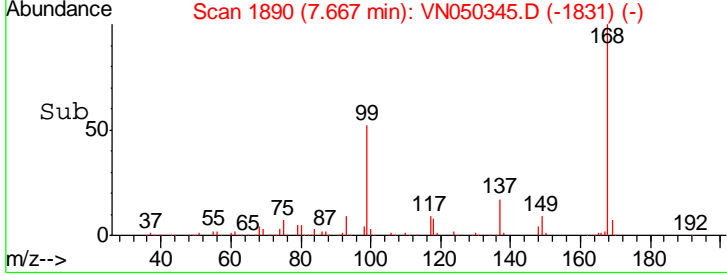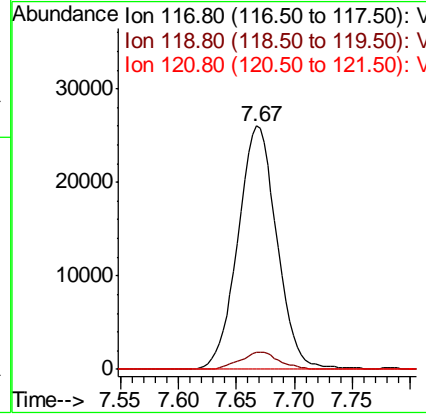

#41  
 Methacrylonitrile  
 Concen: 2.78 ug/l  
 RT: 7.20 min Scan# 1744  
 Delta R.T. 0.02 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
41	100		
39	38.8	55.8	83.6#
67	0.0	84.3	126.5#
52	0.0	34.2	51.2#


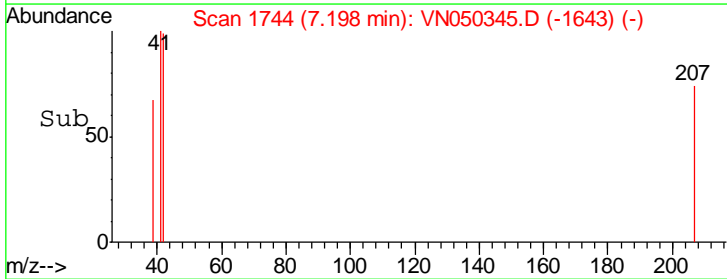
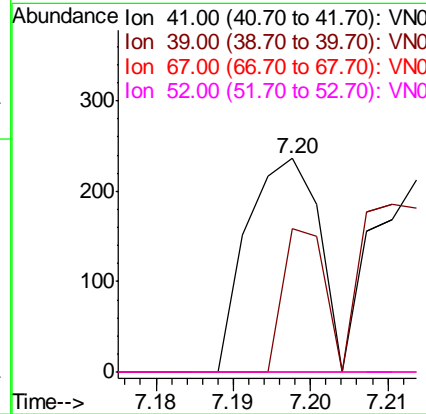



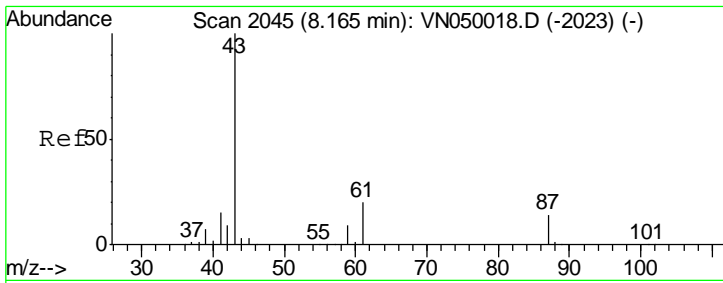

#43  
 Isopropyl Acetate  
 Concen: 10.84 ug/l  
 RT: 8.17 min Scan# 2046  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
43	195351		
61	17.1	15.8	23.6
87	11.5	10.3	15.5

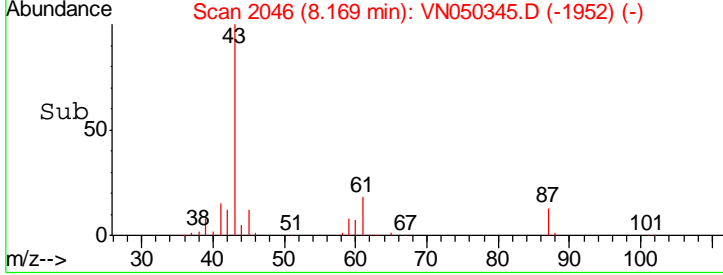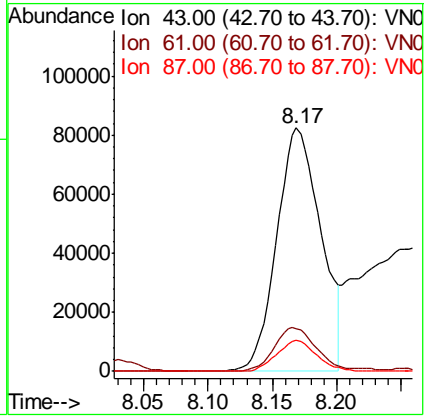

#47  
 Bromodichloromethane  
 Concen: 0.49 ug/l  
 RT: 9.41 min Scan# 2432  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
83	6593		
85	68.5	51.1	76.7
127	7.2	7.0	10.4


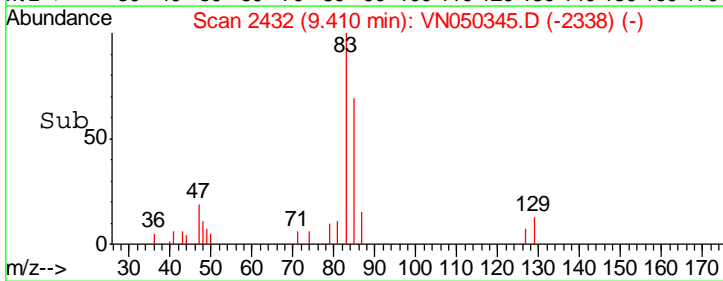
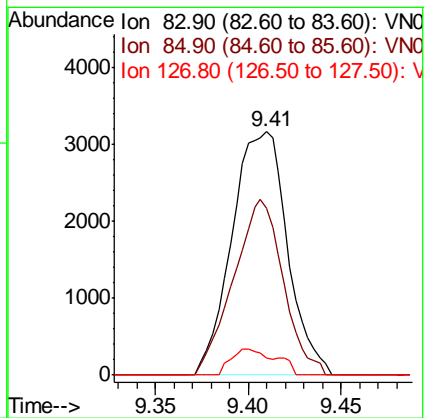



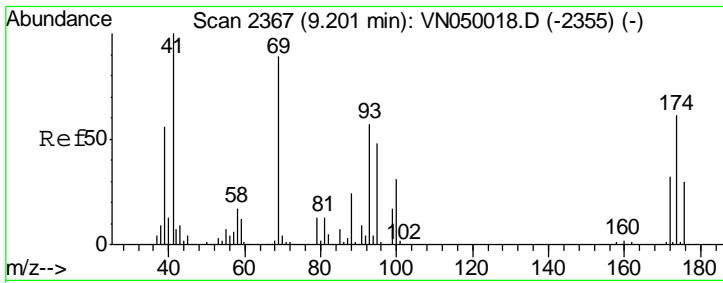

#48  
 Methyl methacrylate  
 Concen: 0.67 ug/l  
 RT: 9.18 min Scan# 2361  
 Delta R.T. -0.02 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
41	100		
69	0.0	70.6	105.8#
39	22.8	43.9	65.9#

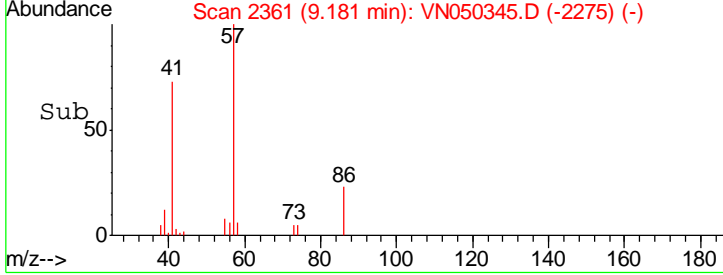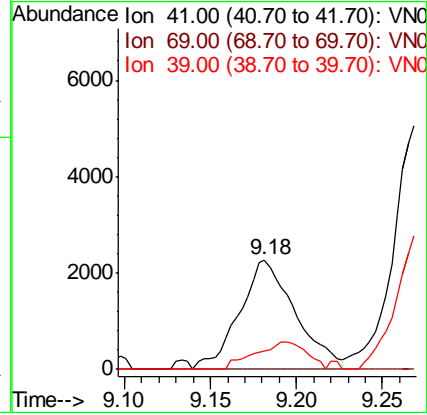

#50  
 Toluene-d8  
 Concen: 45.66 ug/l  
 RT: 10.09 min Scan# 2644  
 Delta R.T. -0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
98	100		
100	63.5	50.7	76.1


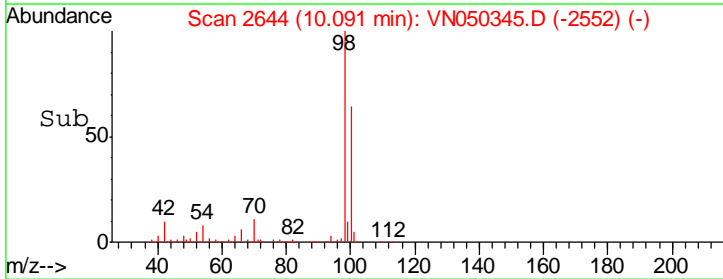
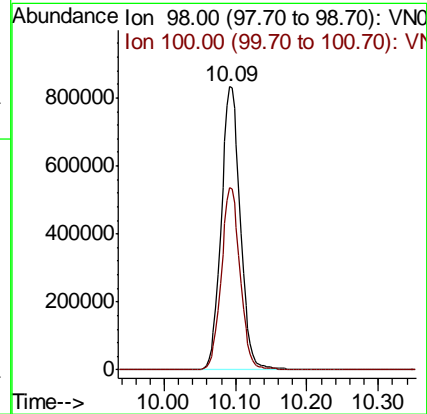





#51  
 4-Methyl-2-Pentanone  
 Concen: 0.27 ug/l  
 RT: 9.99 min Scan# 2611  
 Delta R.T. -0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
43	100		
58	29.3	31.9	47.9#

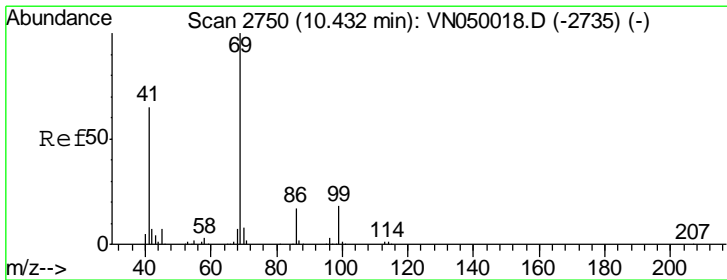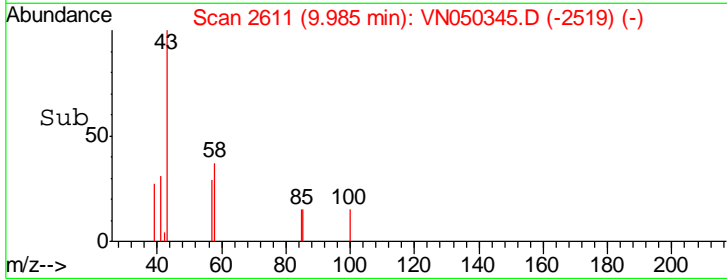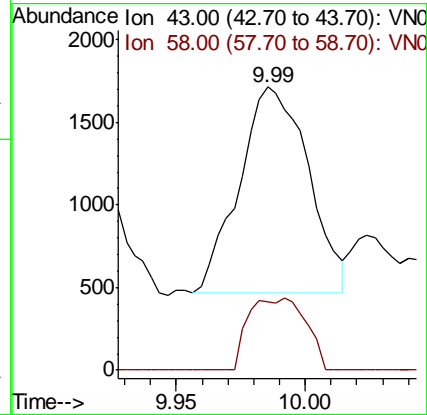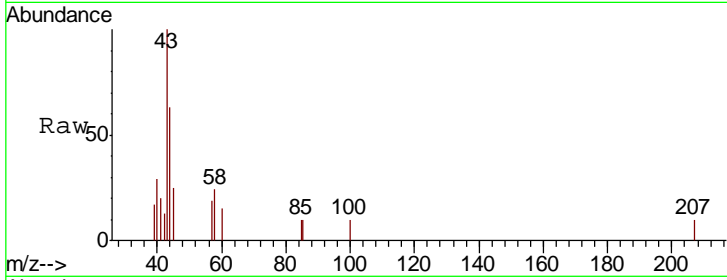

#56  
 Ethyl methacrylate  
 Concen: 2.05 ug/l  
 RT: 10.27 min Scan# 2701  
 Delta R.T. -0.16 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
69	100		
41	142.1	51.0	76.4#
39	54.7	26.6	40.0#


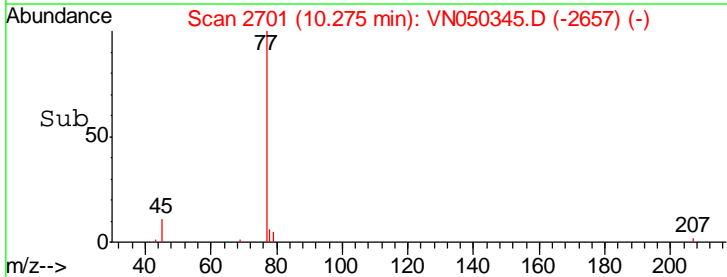
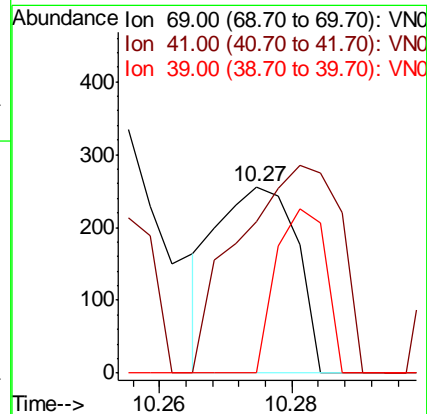
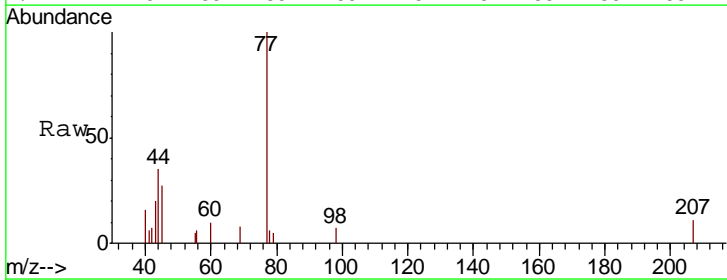




#59  
 2-Hexanone  
 Concen: 6.06 ug/l  
 RT: 10.77 min Scan# 2854  
 Delta R.T. 0.01 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument : MSVOA\_N  
 Client Sampled : C-8


Tgt Ion	Resp	Lower	Upper
43	100		
58	26.3	27.6	82.7#

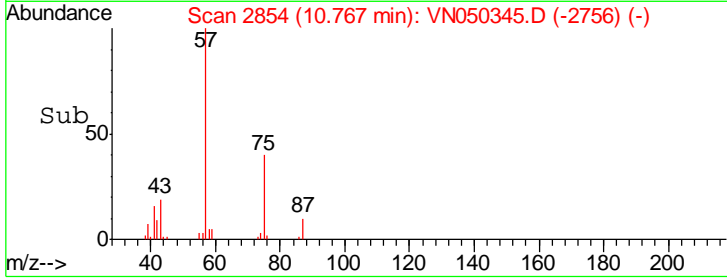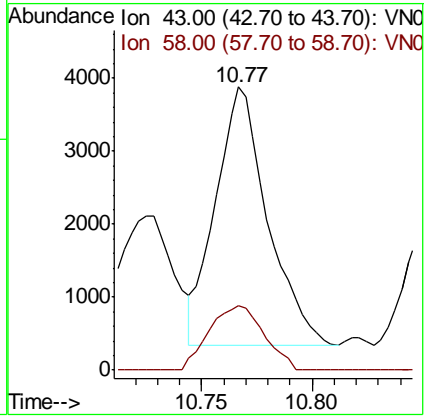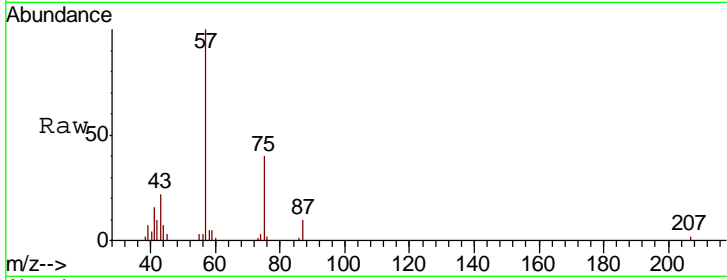

#62  
 4-Bromofluorobenzene  
 Concen: 41.85 ug/l  
 RT: 12.40 min Scan# 3363  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
95	100		
174	90.5	0.0	178.2
176	86.5	0.0	173.4


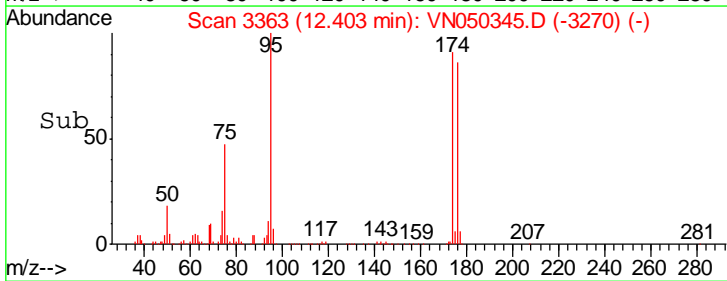
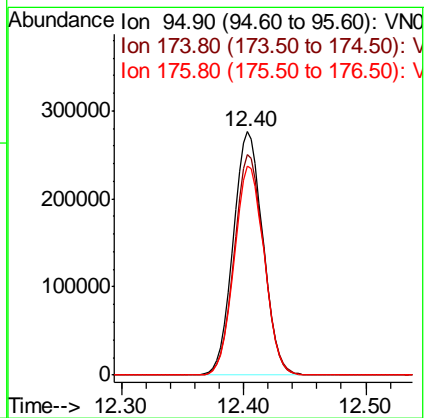





#63  
 Chlorobenzene-d5  
 Concen: 50.00 ug/l  
 RT: 11.41 min Scan# 3054  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument : MSVOA\_N  
 ClientSampled : C-8

Tgt Ion	Resp	Lower	Upper
117	100		
82	53.5	43.7	65.5
119	32.6	26.1	39.1

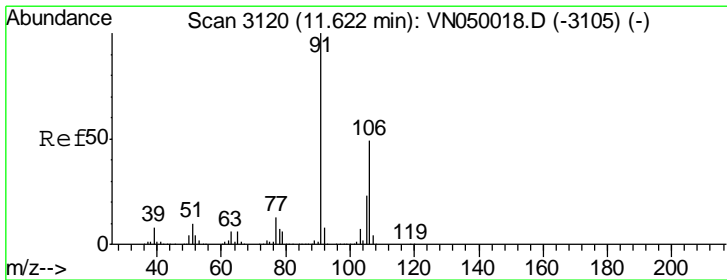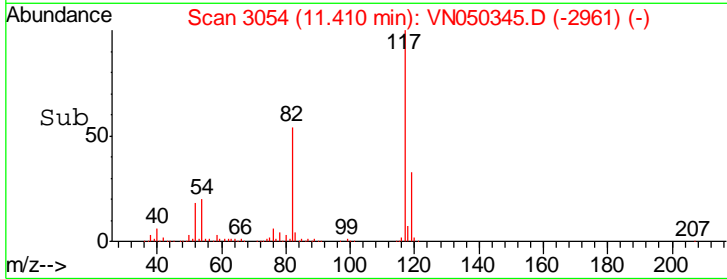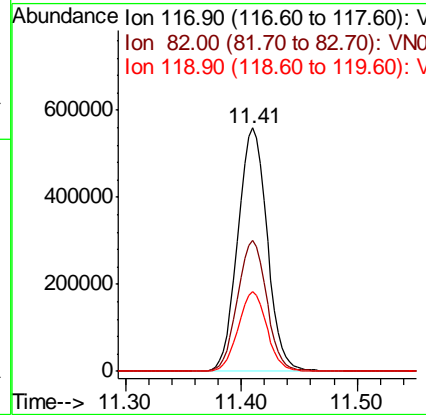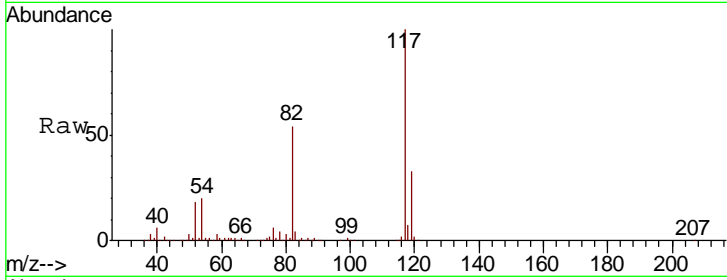


#68  
 m/p-Xylenes  
 Concen: 0.55 ug/l  
 RT: 11.62 min Scan# 3119  
 Delta R.T. -0.01 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
106	100		
91	200.2	162.2	243.2

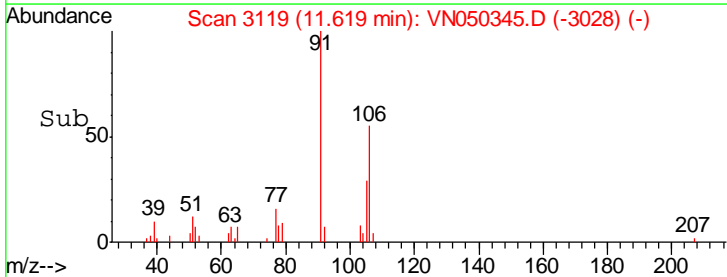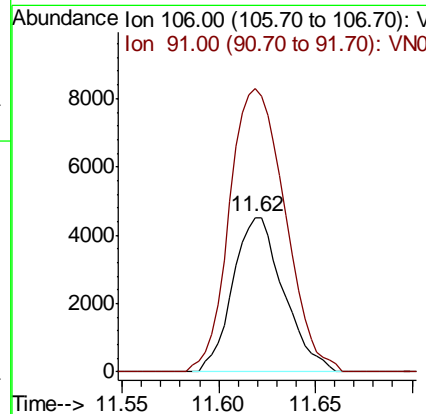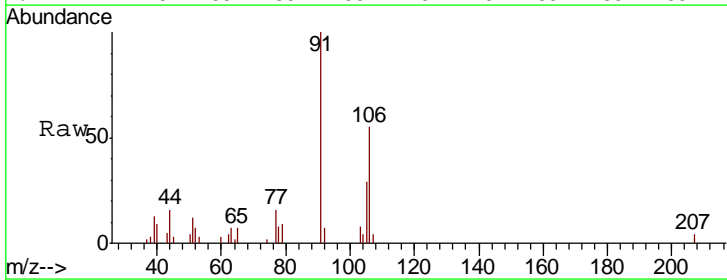









#70  
 Styrene  
 Concen: 0.93 ug/l  
 RT: 11.95 min Scan# 3222  
 Delta R.T. -0.02 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
104	108		
78	309.3	39.3	58.9#
103	375.0	45.0	67.6#

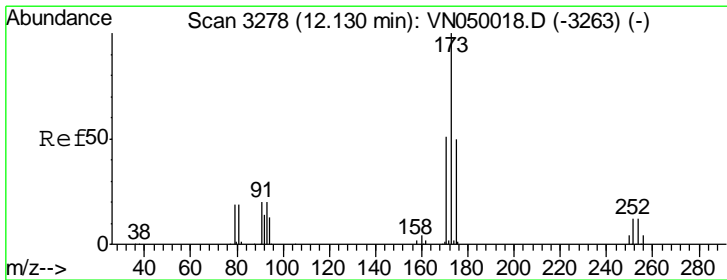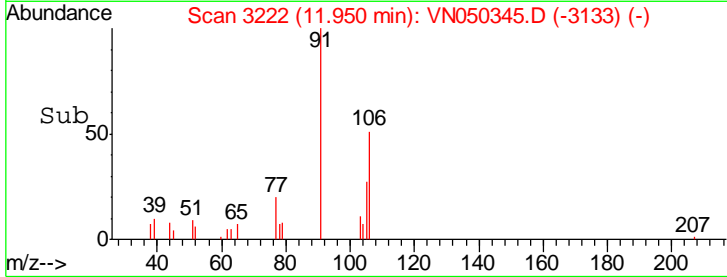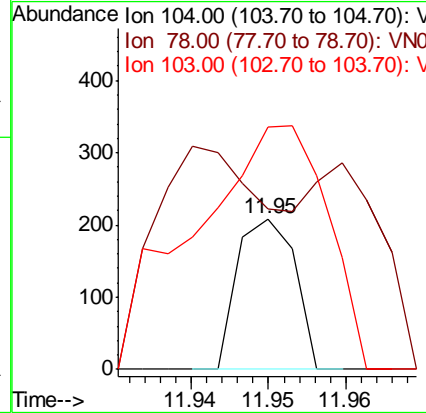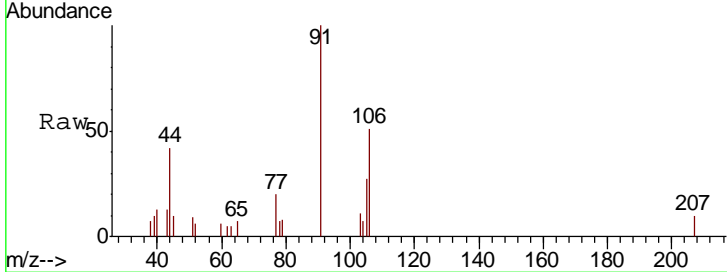

#71  
 Bromoform  
 Concen: 0.69 ug/l  
 RT: 12.41 min Scan# 3364  
 Delta R.T. 0.28 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
173	4774		
175	565.9	24.1	72.2#
254	0.0	0.2	0.2#


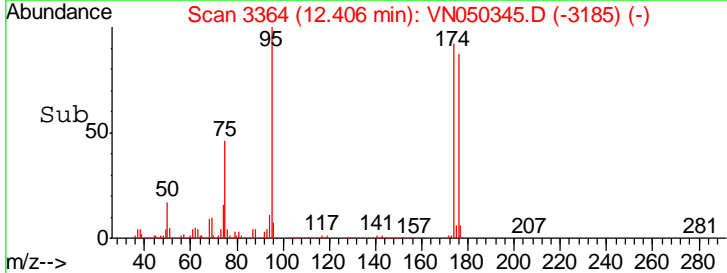
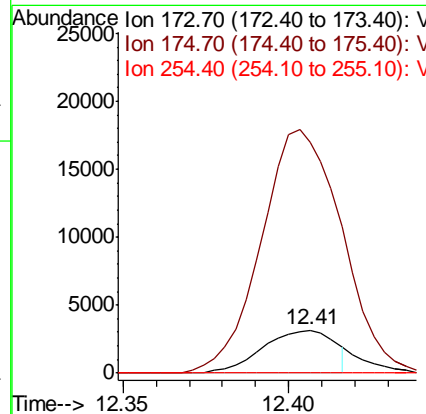



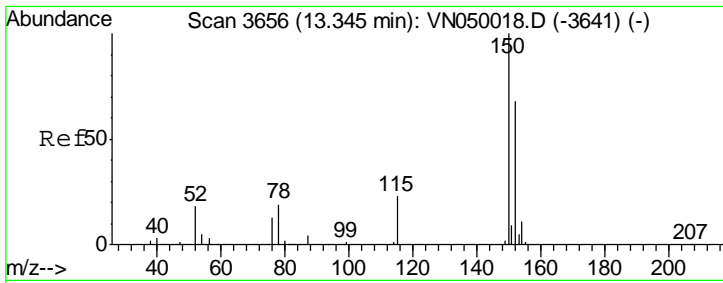

#72  
 1,4-Dichlorobenzene-d4  
 Concen: 50.00 ug/l  
 RT: 13.35 min Scan# 3656  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument :  
 MSVOA\_N  
 ClientSampled :  
 C-8


Tgt Ion	Resp	Lower	Upper
152	100		
115	56.5	27.8	83.3
150	157.8	0.0	348.6

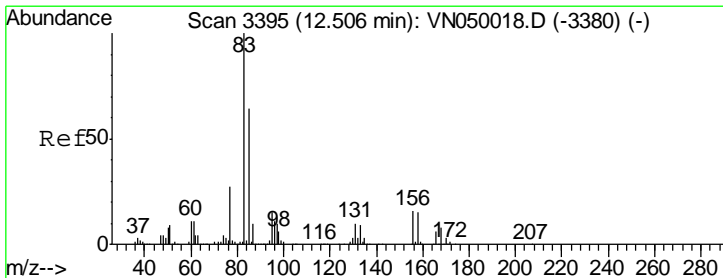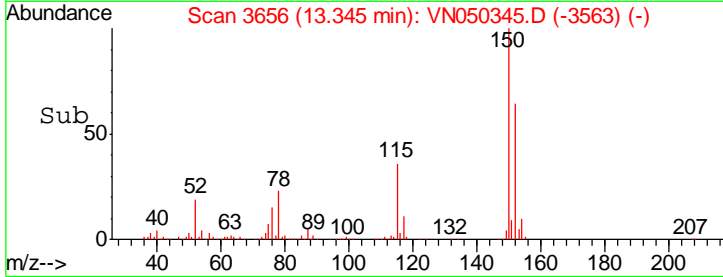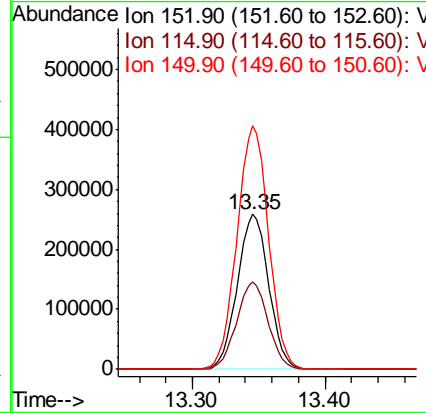

#75  
 1,1,2,2-Tetrachloroethane  
 Concen: Below Cal  
 RT: 12.40 min Scan# 3361  
 Delta R.T. -0.11 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
83	100		
131	268.8	5.1	15.3#
85	0.0	32.3	96.8#


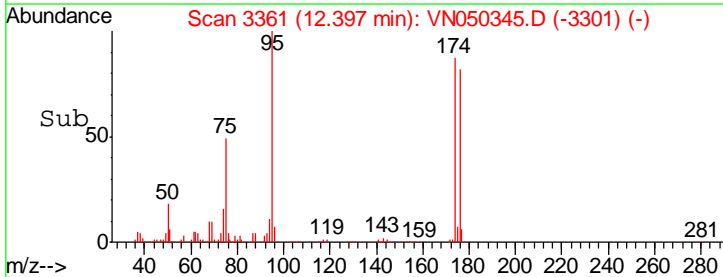
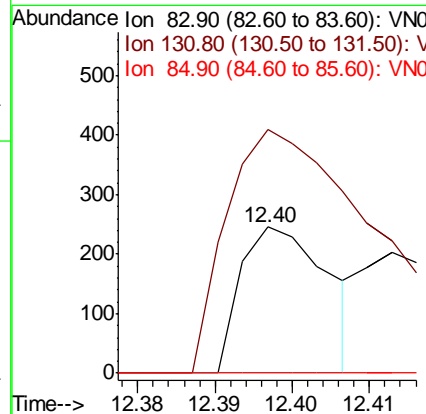
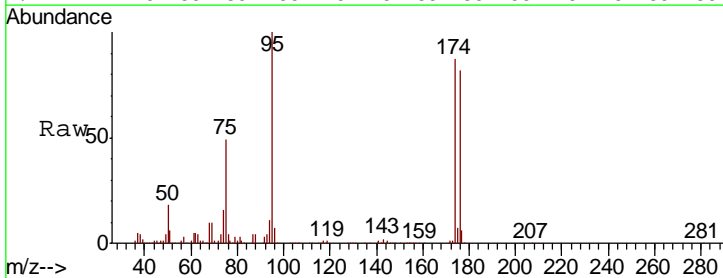


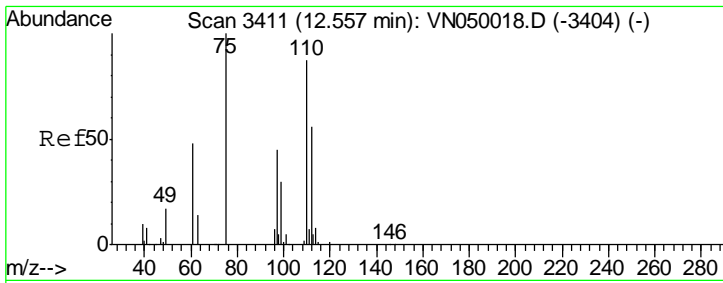

#76  
 1,2,3-Trichloropropane  
 Concen: 28.05 ug/l  
 RT: 12.40 min Scan# 3363  
 Delta R.T. -0.15 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument : MSVOA\_N  
 Client Sampled : C-8


Tgt Ion: 75 Resp: 221175  
 Ion Ratio Lower Upper  
 75 100  
 77 1.2 0.0 0.0#

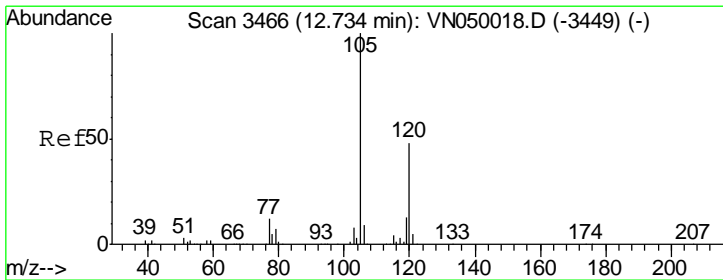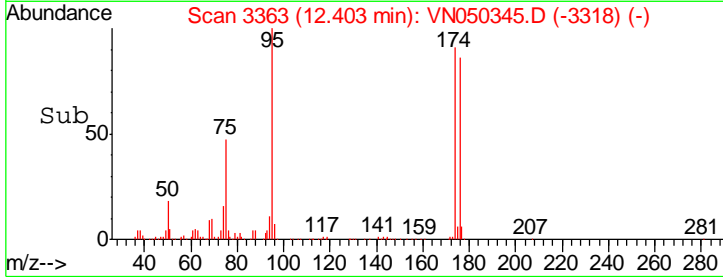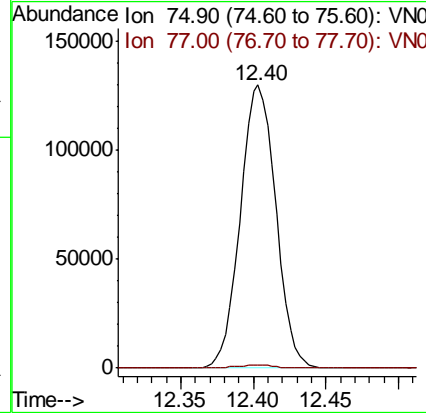

#80  
 1,3,5-Trimethylbenzene  
 Concen: 0.35 ug/l  
 RT: 12.73 min Scan# 3466  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion: 105 Resp: 9029  
 Ion Ratio Lower Upper  
 105 100  
 120 51.3 24.4 73.2


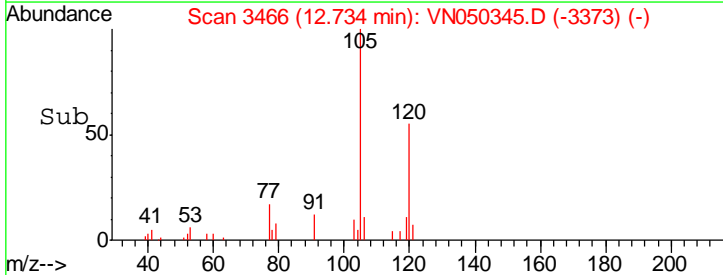
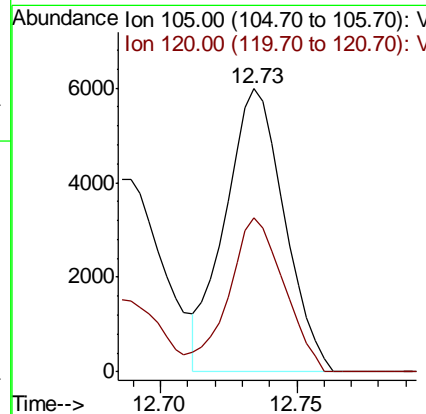



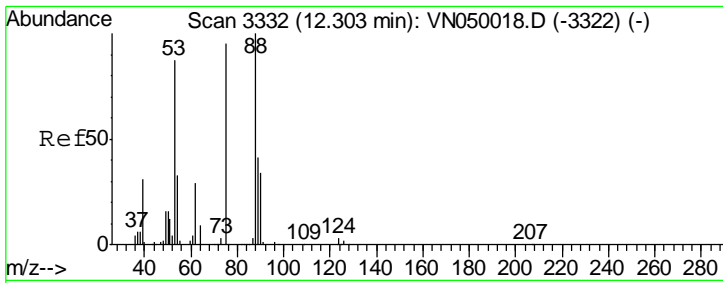

#81  
 trans-1,4-Dichloro-2-butene  
 Concen: 88.96 ug/l  
 RT: 12.40 min Scan# 3363  
 Delta R.T. 0.10 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29




Instrument : MSVOA\_N  
 ClientSampled : C-8


Tgt Ion	Resp	Lower	Upper
75	100		
53	0.2	73.5	110.3#
89	0.0	36.0	54.0#

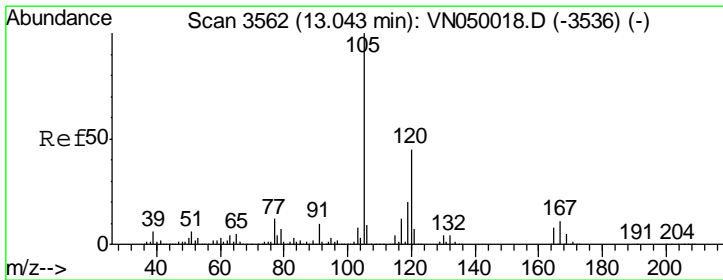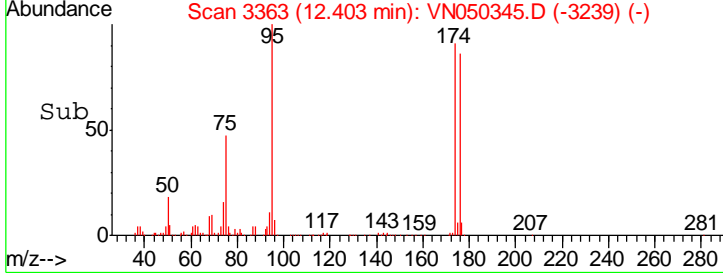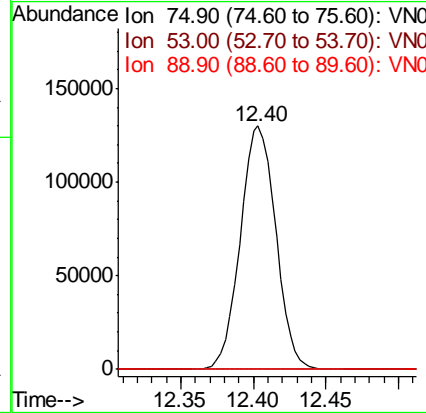

#84  
 1,2,4-Trimethylbenzene  
 Concen: 0.96 ug/l  
 RT: 13.04 min Scan# 3562  
 Delta R.T. 0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
105	100		
120	44.5	22.9	68.7

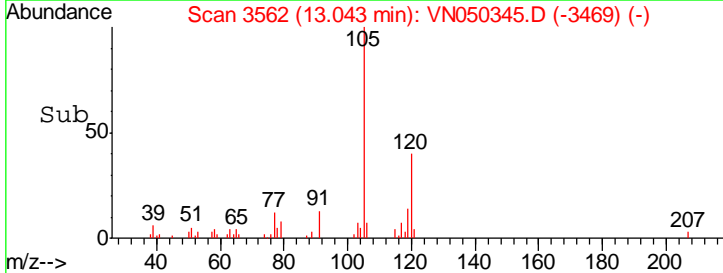
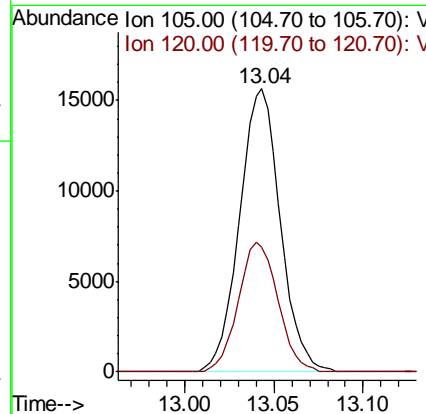



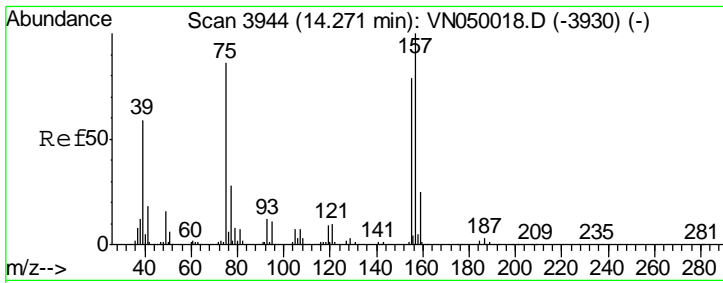

#92  
 1,2-Dibromo-3-Chloropropane  
 Concen: Below Cal  
 RT: 14.25 min Scan# 3936  
 Delta R.T. -0.03 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Instrument : MSVOA\_N  
 ClientSampled : C-8

Tgt Ion	Resp	Lower	Upper
75	100		
155	0.0	44.8	134.4#
157	0.0	57.2	171.6#

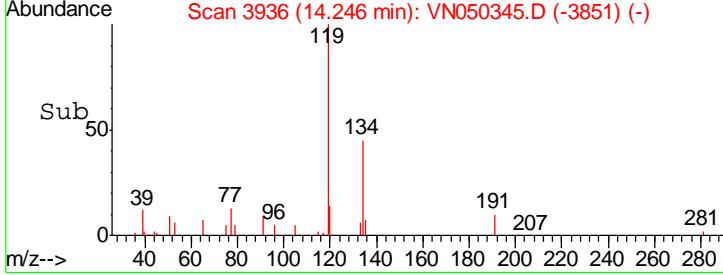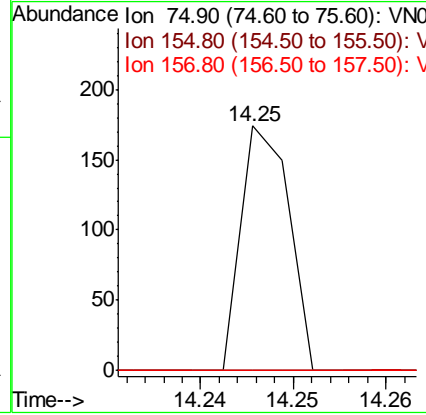

#95  
 Naphthalene  
 Concen: 4.89 ug/l  
 RT: 15.13 min Scan# 4212  
 Delta R.T. -0.00 min  
 Lab File: VN050345.D  
 Acq: 4 Aug 2018 5:29

Tgt Ion	Resp	Lower	Upper
128	100		
127	12.8	10.4	15.6
129	11.8	8.8	13.2

