


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN080318\  
 Data File : VN050328.D  
 Acq On : 3 Aug 2018 21:37  
 Operator : MD\SY  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N072418W.M  
 Title : SW846 8260  
 Last Update : Thu Jul 26 18:10:10 2018

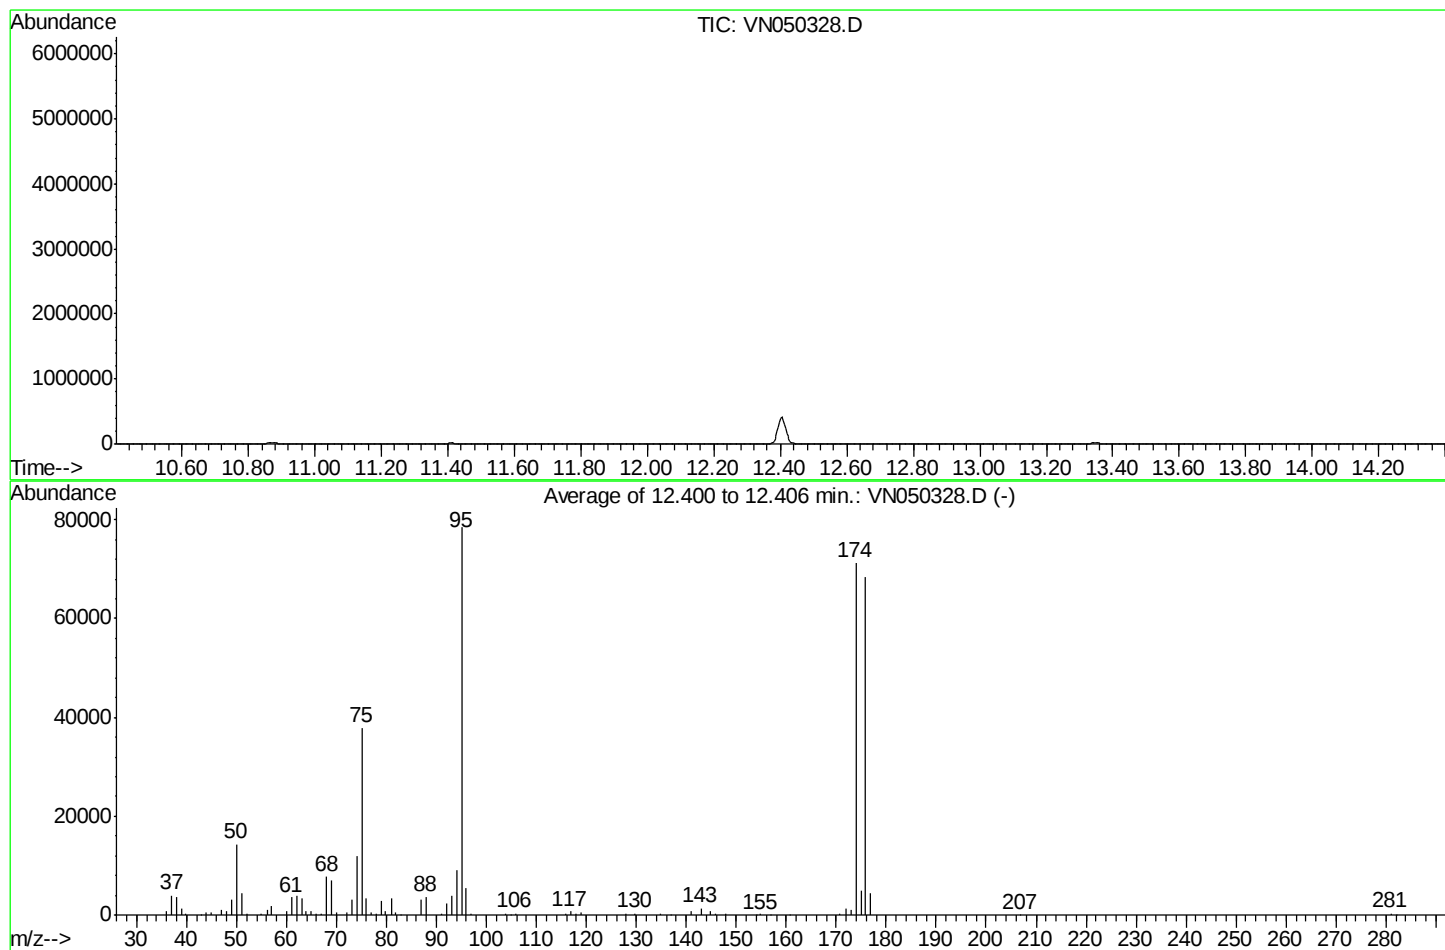

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.2      | 14266   | PASS             |
| 75          | 95           | 30           | 60           | 48.3      | 37866   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 78458   | PASS             |
| 96          | 95           | 5            | 9            | 7.0       | 5505    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.5       | 1101    | PASS             |
| 174         | 95           | 50           | 100          | 90.9      | 71314   | PASS             |
| 175         | 174          | 5            | 9            | 7.1       | 5053    | PASS             |
| 176         | 174          | 95           | 101          | 95.9      | 68384   | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 4457    | PASS             |