


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080321\
 Data File : VN067974.D
 Acq On : 3 Aug 2021 9:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
 Title : SW846 8260
 Last Update : Thu Jul 29 15:02:35 2021

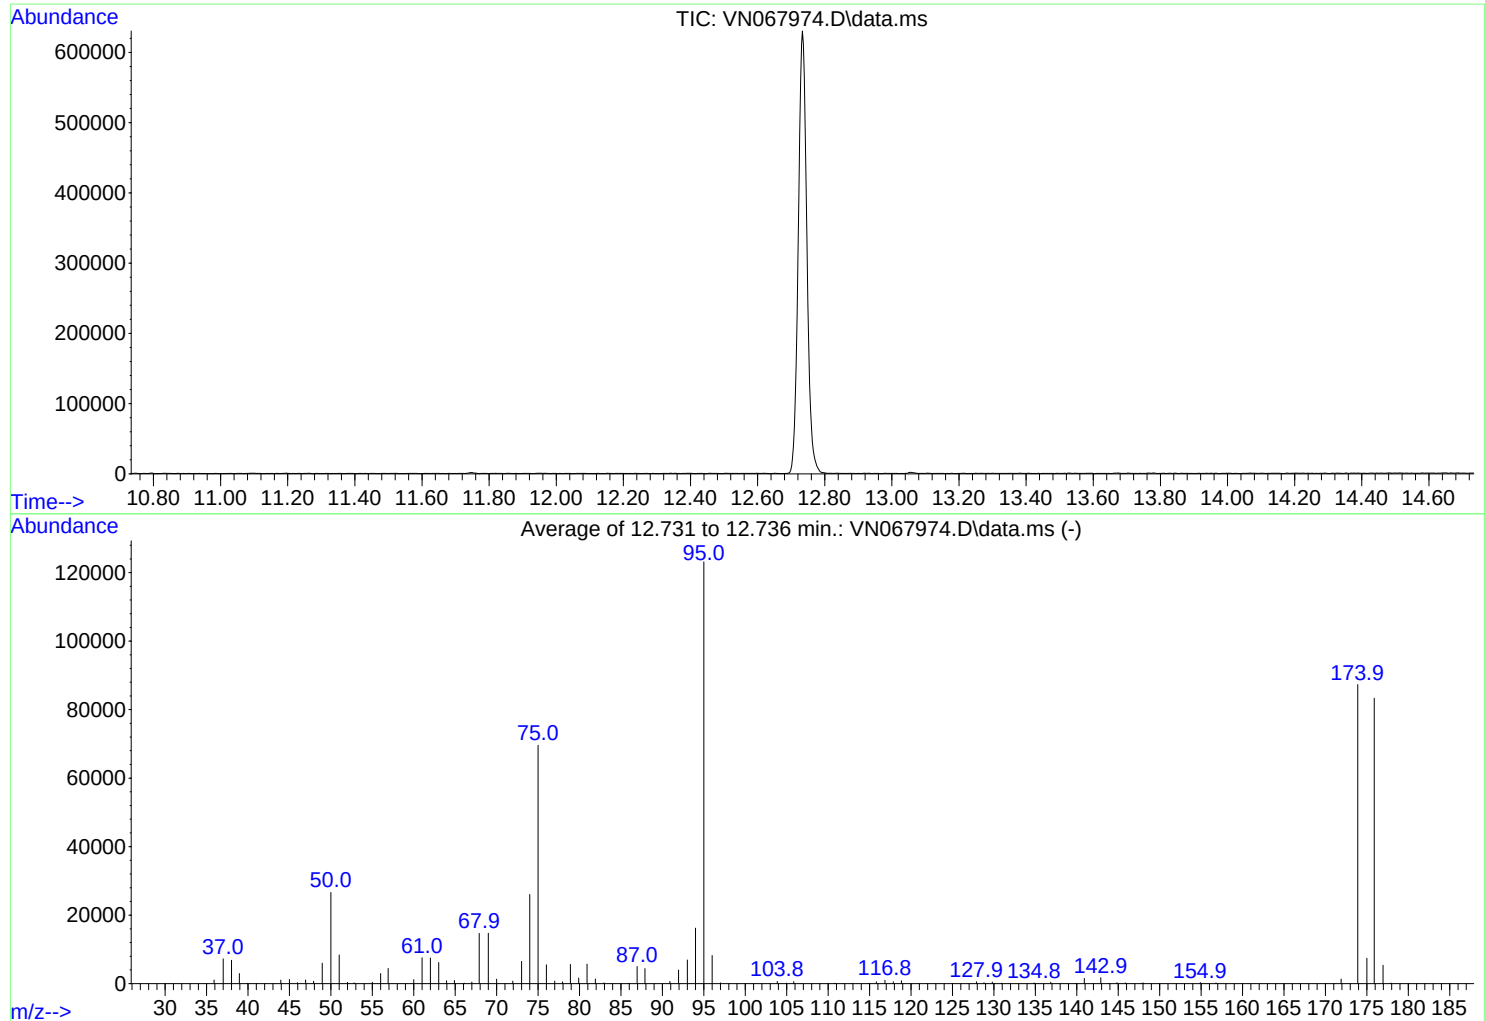

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3987

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	26637	PASS
75	95	30	60	56.5	69589	PASS
95	95	100	100	100.0	123149	PASS
96	95	5	9	6.7	8219	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.9	87293	PASS
175	174	5	9	8.5	7450	PASS
176	174	95	101	95.5	83328	PASS
177	176	5	9	6.5	5390	PASS