

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080322\
 Data File : VN073718.D
 Acq On : 03 Aug 2022 17:52
 Operator : JC\MD
 Sample : N3972-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SPN-15

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Title : SW846 8260

Signal : TIC: VN073718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.205	47	54	62	rBV5	10347	29285	1.79%	0.290%
2	2.710	133	140	150	rVB6	19166	54983	3.36%	0.544%
3	3.081	195	203	213	rVB5	24865	58760	3.59%	0.582%
4	4.228	381	398	413	rBV2	25250	83870	5.12%	0.830%
5	4.510	435	446	458	rBV	89150	277401	16.94%	2.746%
6	4.998	519	529	537	rBV6	7026	23759	1.45%	0.235%
7	7.345	918	928	942	rVB2	22088	58256	3.56%	0.577%
8	7.622	967	975	986	rBB2	10064	26412	1.61%	0.261%
9	7.951	1021	1031	1037	rBV	256610	632454	38.63%	6.260%
10	8.016	1037	1042	1056	rVB	431053	962651	58.79%	9.528%
11	8.375	1093	1103	1123	rBV	257247	595842	36.39%	5.897%
12	8.904	1181	1193	1212	rBV	616946	1263663	77.18%	12.507%
13	10.381	1436	1444	1463	rBV	917960	1637372	100.00%	16.206%
14	10.586	1472	1479	1485	rBV3	11214	21910	1.34%	0.217%
15	10.657	1485	1491	1498	rVB3	10072	17879	1.09%	0.177%
16	11.233	1582	1589	1599	rBV	32398	62359	3.81%	0.617%
17	11.686	1658	1666	1679	rBV	916956	1560287	95.29%	15.443%
18	12.492	1796	1803	1811	rBV5	7421	16560	1.01%	0.164%
19	12.674	1826	1834	1845	rBV	725985	1197077	73.11%	11.848%
20	13.616	1985	1994	2005	rBV	899777	1473878	90.01%	14.588%
21	13.710	2005	2010	2018	rVB2	30326	48936	2.99%	0.484%


Sum of corrected areas: 10103594

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080322\
Data File : VN073718.D
Acq On : 03 Aug 2022 17:52
Operator : JC\MD
Sample : N3972-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SPN-15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

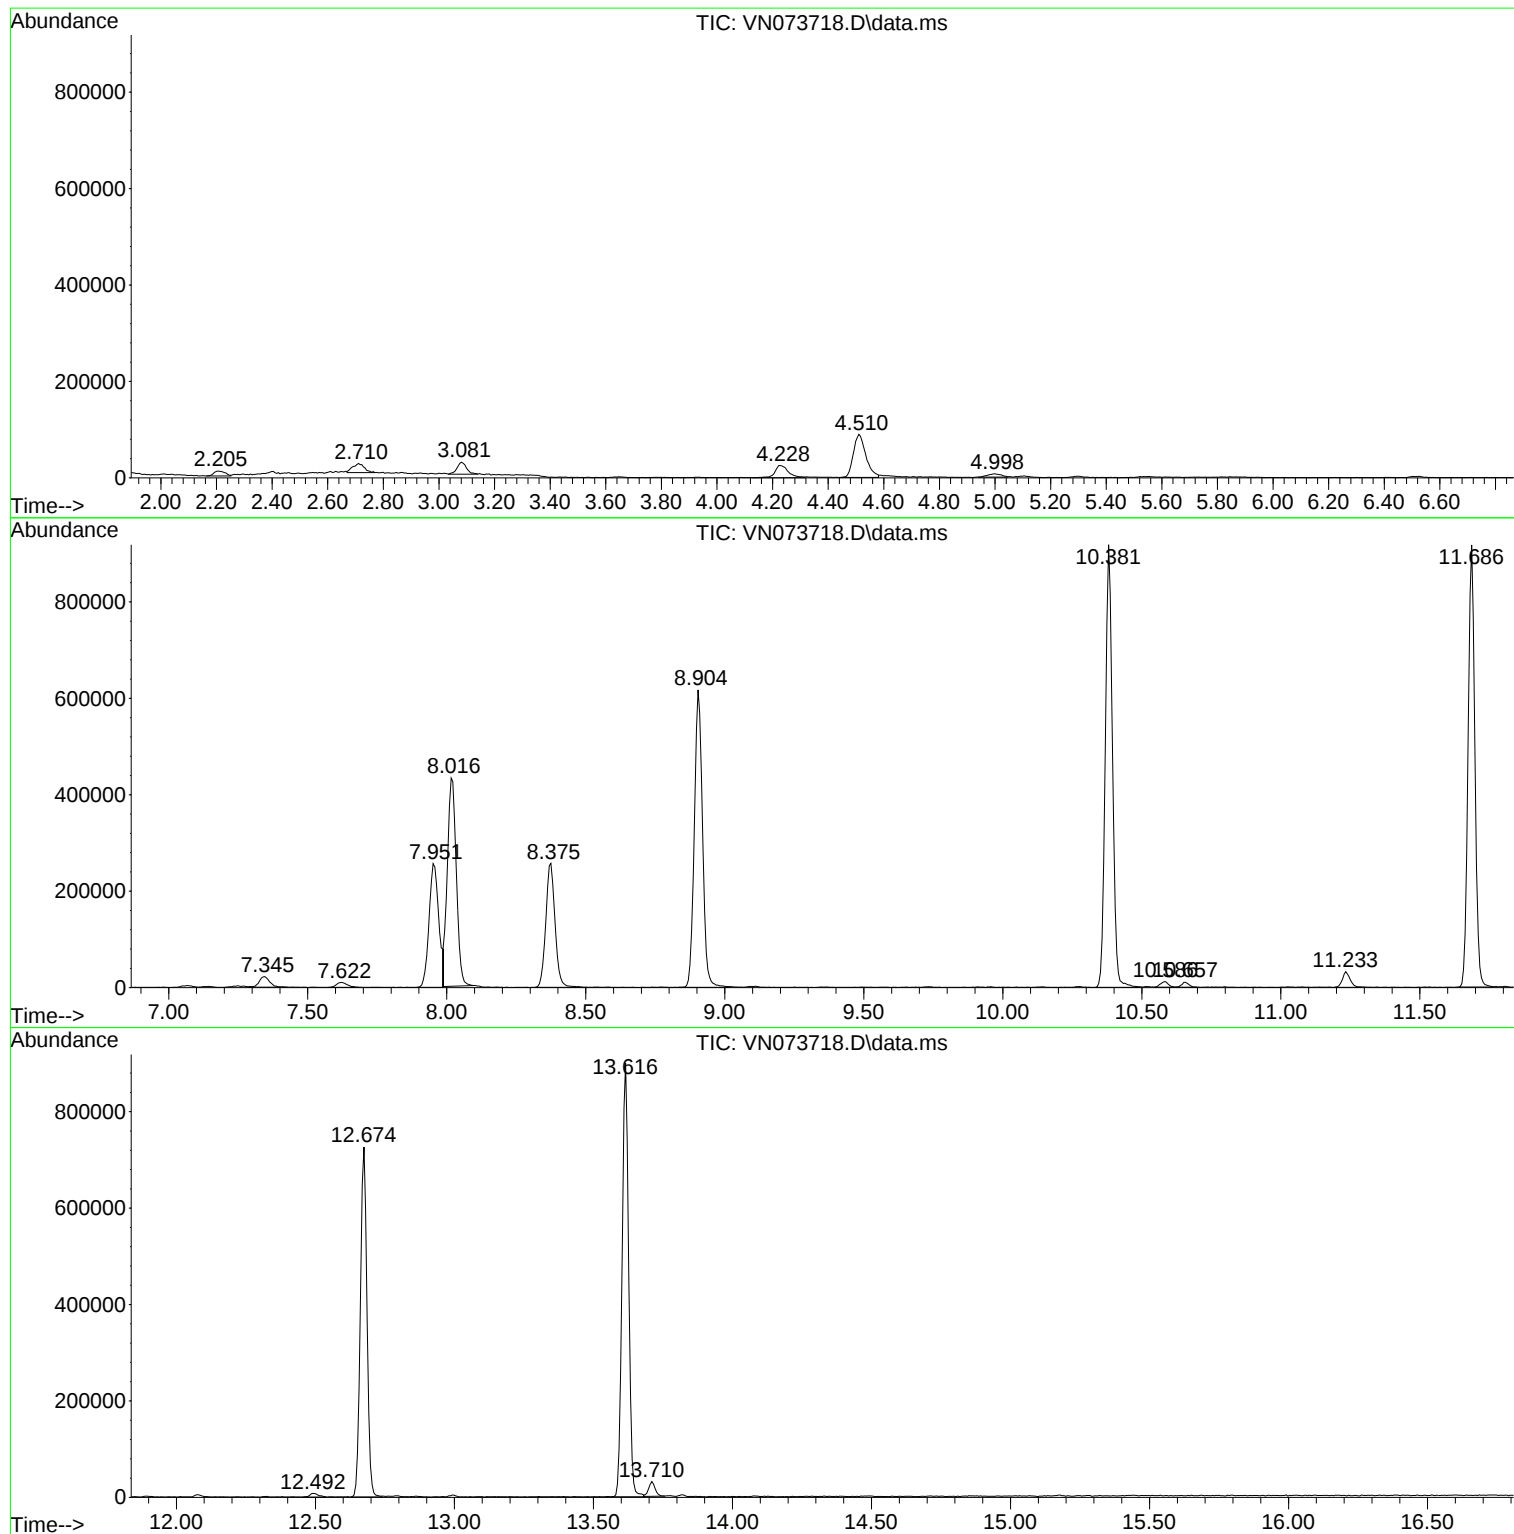

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080322\
Data File : VN073718.D
Acq On : 03 Aug 2022 17:52
Operator : JC\MD
Sample : N3972-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SPN-15










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.510	14.41 ug/l	277401	Pentafluorobenzene	8.022

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
3			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4			Ethylamine	45	C2H7N	000075-04-7	5
5			Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

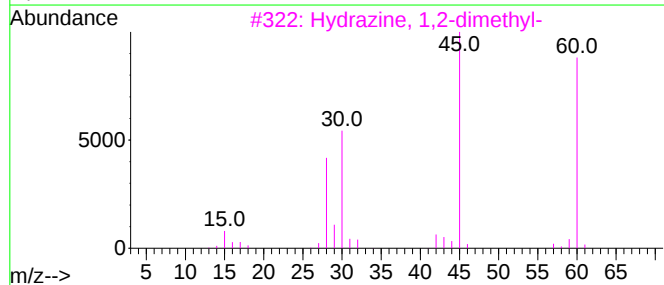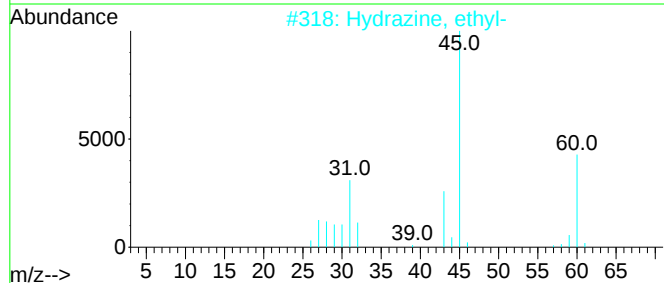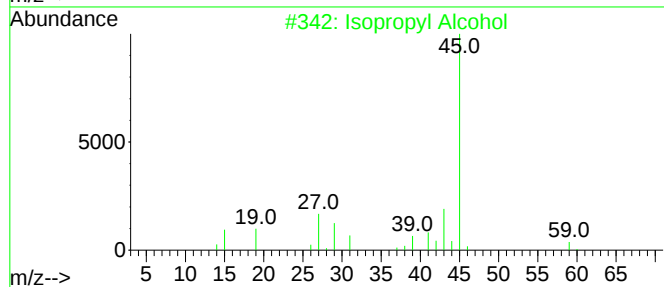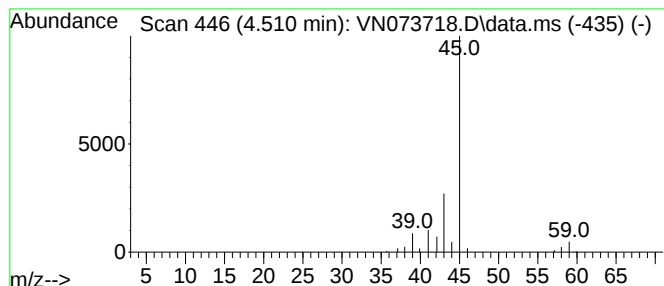

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080322\
Data File : VN073718.D
Acq On : 03 Aug 2022 17:52
Operator : JC\MD
Sample : N3972-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SPN-15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	4.510	14.4	ug/l	277401	1	8.022	962651	50.0