
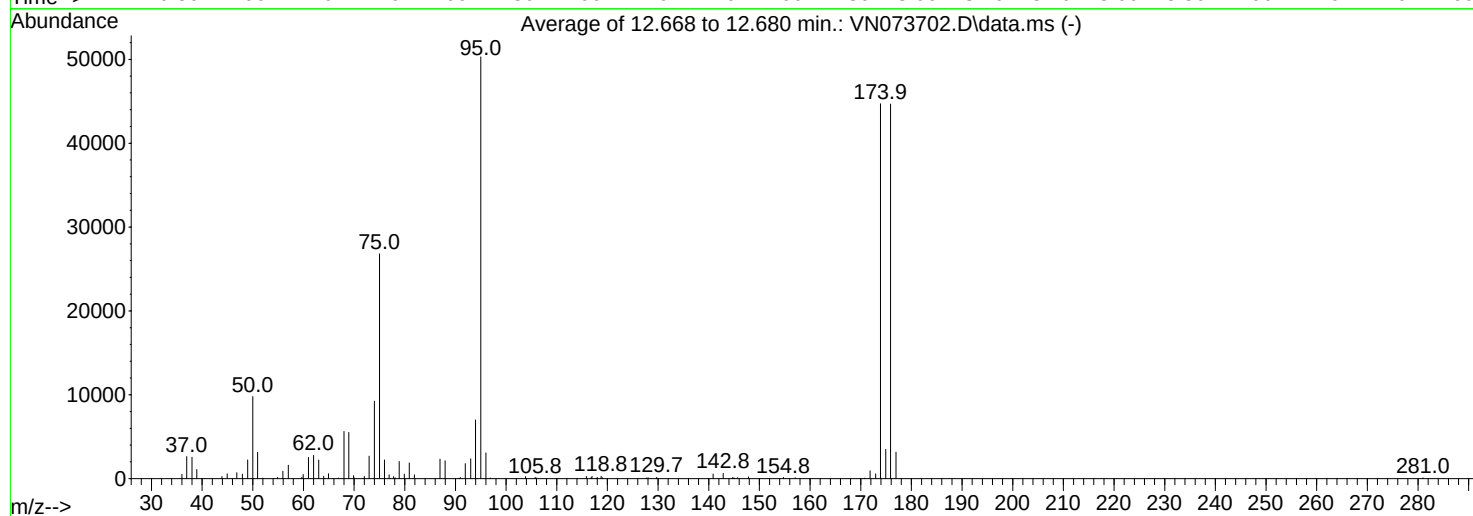


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080322\
 Data File : VN073702.D
 Acq On : 03 Aug 2022 10:44
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Title : SW846 8260
 Last Update : Fri Jul 29 02:20:25 2022

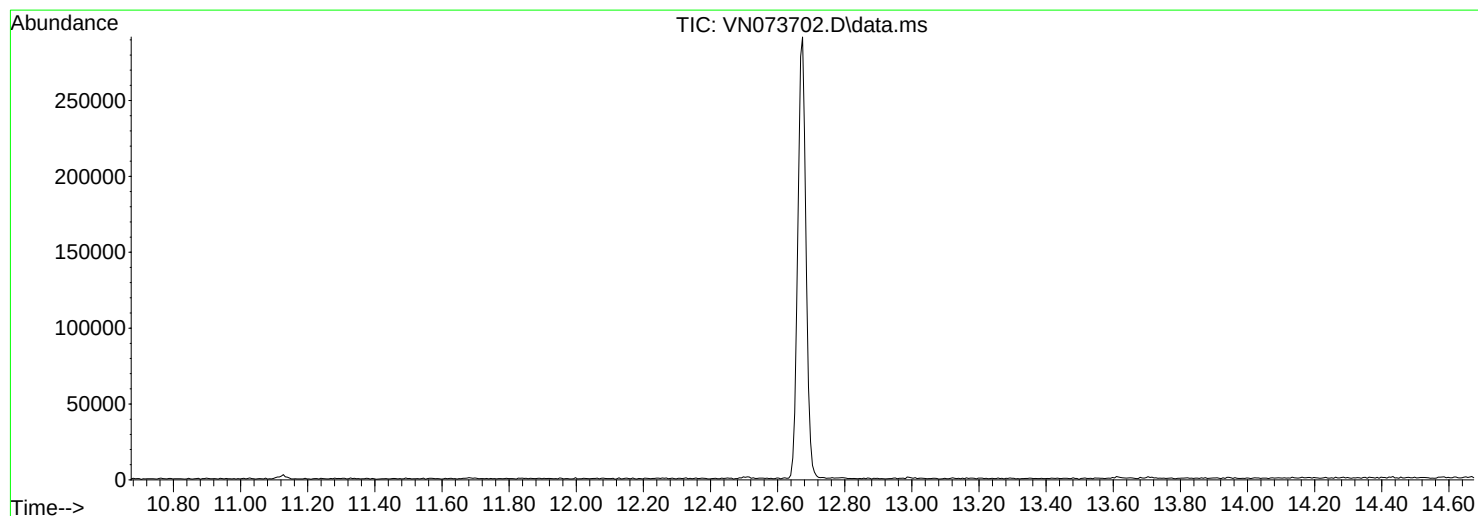

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	9795	PASS
75	95	30	60	53.3	26800	PASS
95	95	100	100	100.0	50299	PASS
96	95	5	9	6.1	3071	PASS
173	174	0.00	2	1.3	567	PASS
174	95	50	100	88.9	44709	PASS
175	174	5	9	7.8	3497	PASS
176	174	95	101	99.9	44672	PASS
177	176	5	9	7.1	3176	PASS