

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080323\
 Data File : VN078745.D
 Acq On : 03 Aug 2023 12:07
 Operator : JC\MD
 Sample : VN0803WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0803WBL01

Quant Time: Aug 04 06:30:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080123W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Aug 02 04:51:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.824	128	104365	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.106	114	645752	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.871	117	412289	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.588	65	258999	33.107	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	110.367%#
60) 4-Bromofluorobenzene	12.859	95	131512	21.285	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	70.933%
63) Toluene-d8	10.571	98	611584	30.028	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	100.100%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080323\
Data File : VN078745.D
Acq On : 03 Aug 2023 12:07
Operator : JC\MD
Sample : VN0803WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0803WBL01

Quant Time: Aug 04 06:30:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080123W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Aug 02 04:51:47 2023
Response via : Initial Calibration




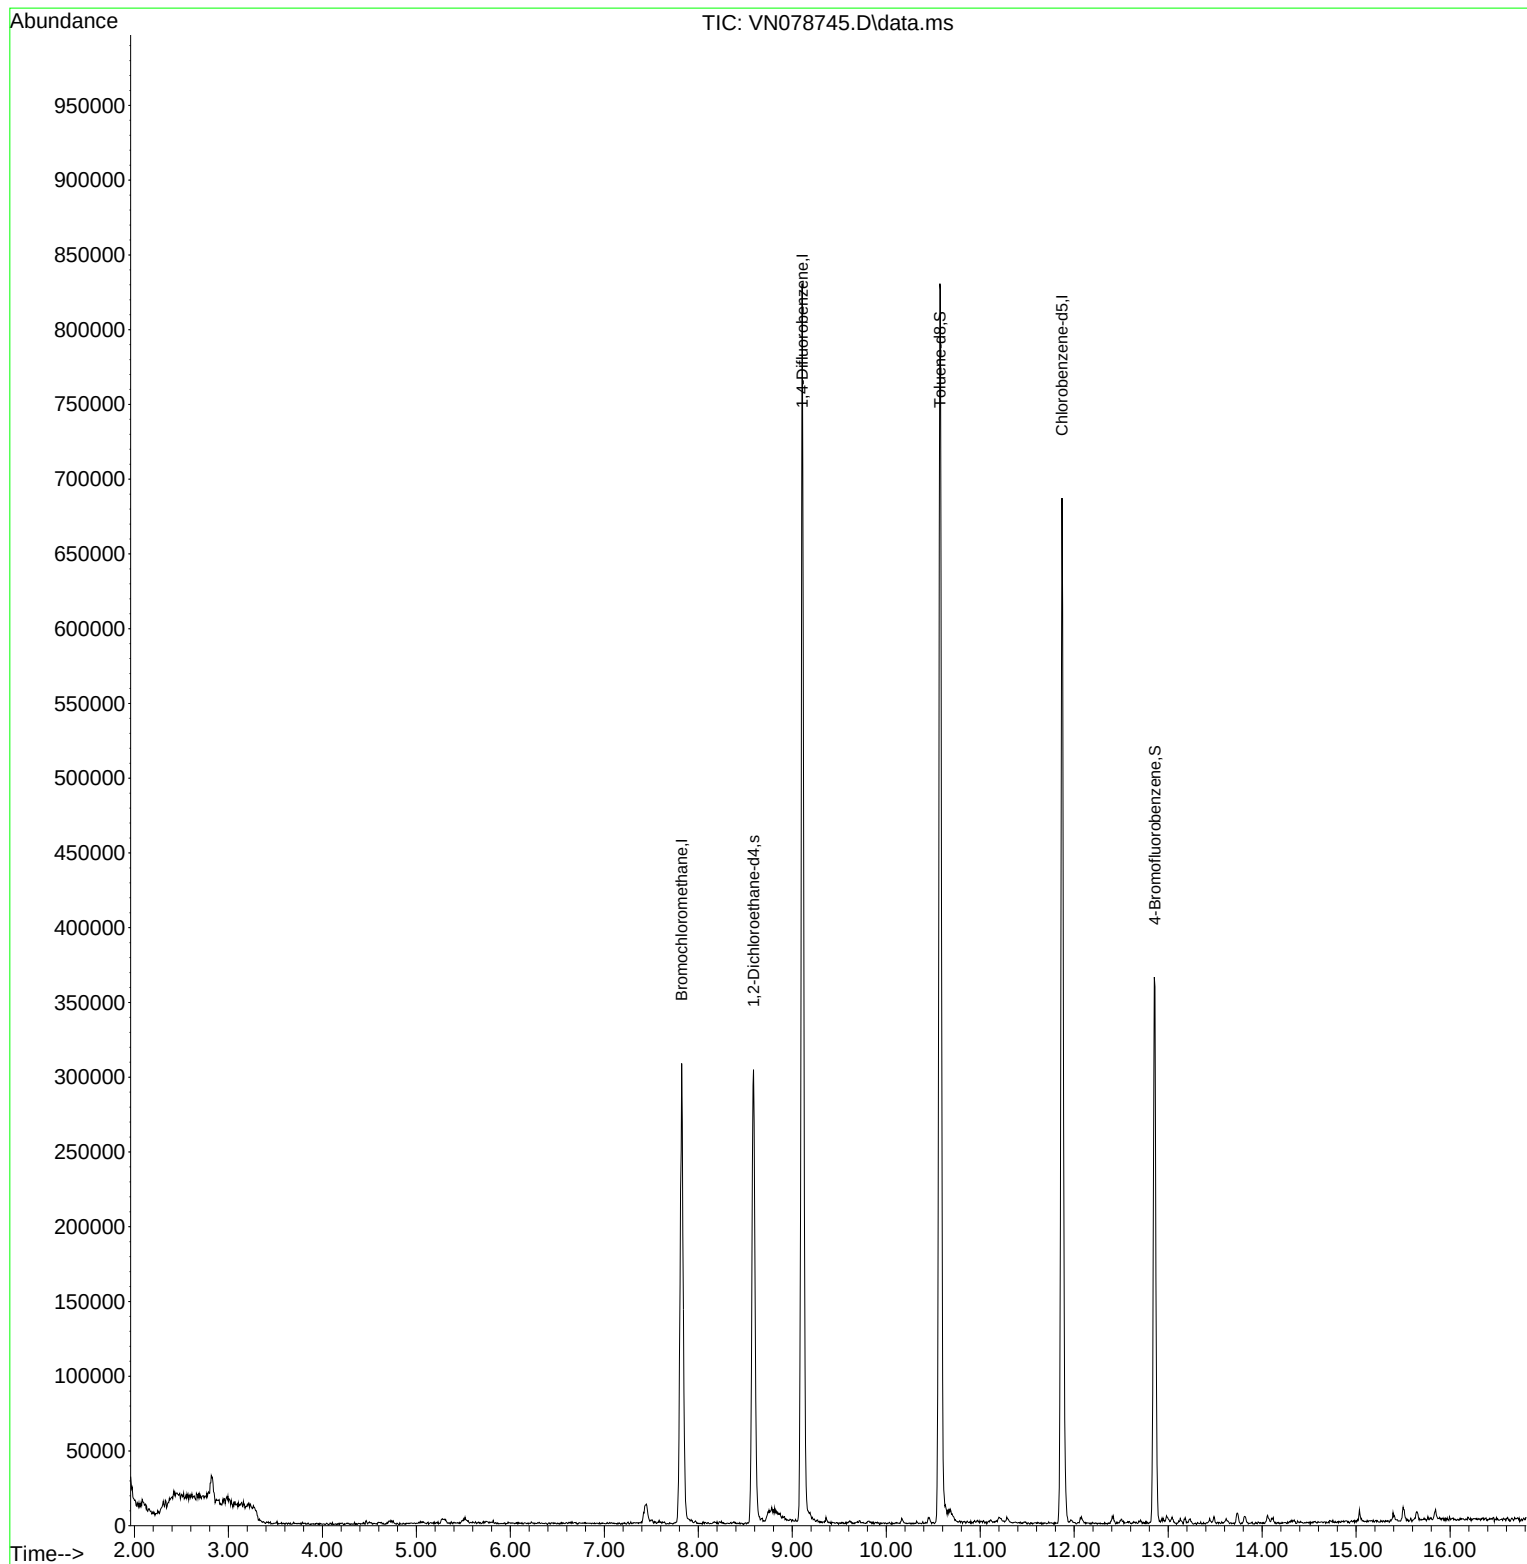


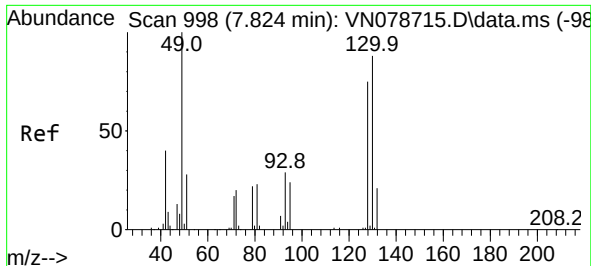

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.824 min Scan# 998
Delta R.T. -0.000 min
Lab File: VN078745.D
Acq: 03 Aug 2023 12:07




Instrument :
MSVOA_N
ClientSampleId :
VN0803WBL01


Tgt Ion:128 Resp: 104365
Ion Ratio Lower Upper
128 100
49 144.3 0.0 370.8
130 126.5 0.0 307.0

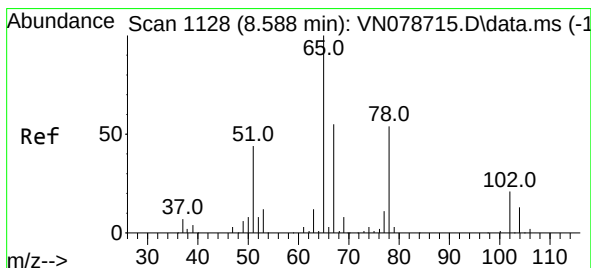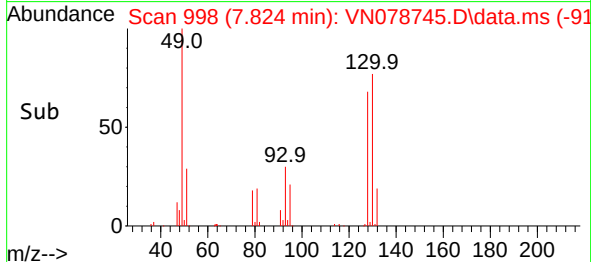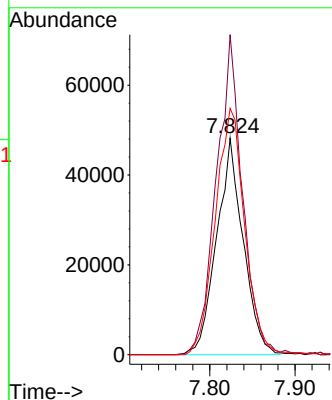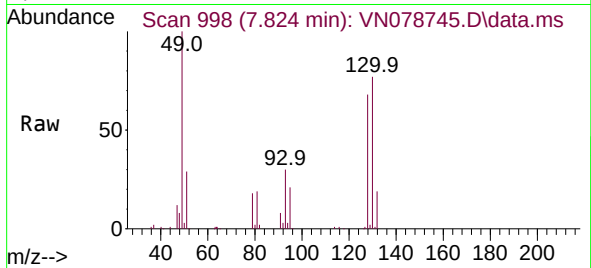

#27
1,2-Dichloroethane-d4
Concen: 33.107 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VN078745.D
Acq: 03 Aug 2023 12:07

Tgt Ion: 65 Resp: 258999
Ion Ratio Lower Upper
65 100
67 51.9 42.9 64.3

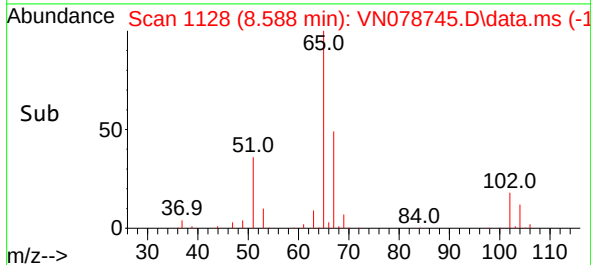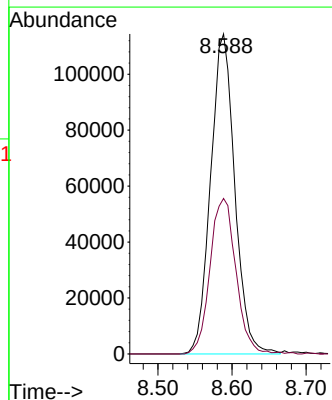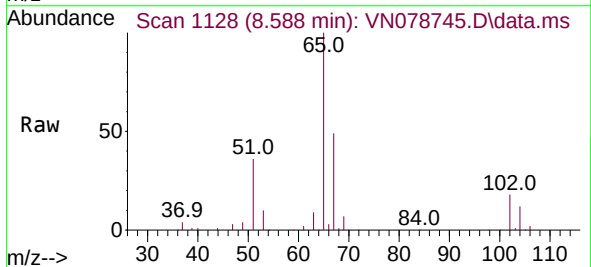

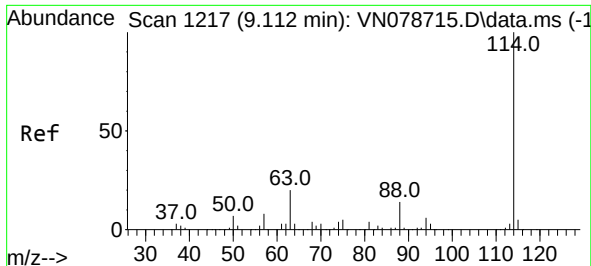

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN078745.D

Acq: 03 Aug 2023 12:07

Instrument :

MSVOA_N

ClientSampleId :

VN0803WBL01





Tgt Ion:114 Resp: 645752

Ion Ratio Lower Upper

114 100

63 19.8 15.2 22.8

88 15.9 12.5 18.7

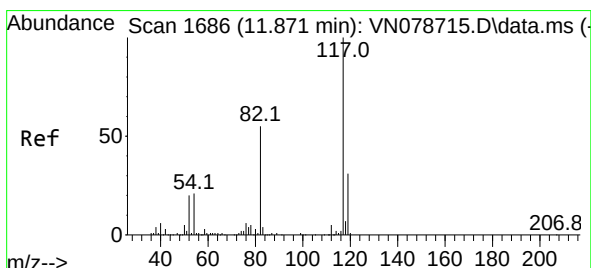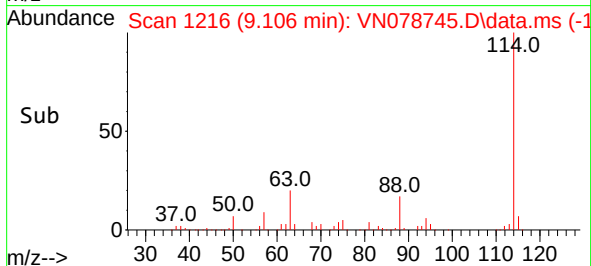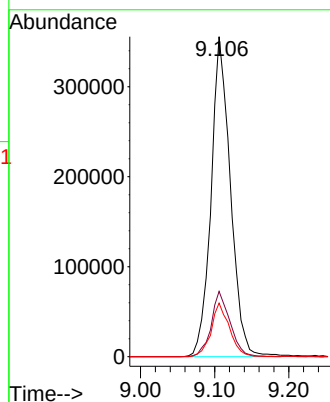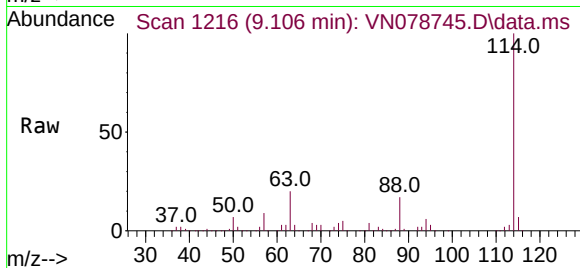

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.871 min Scan# 1686

Delta R.T. -0.000 min

Lab File: VN078745.D

Acq: 03 Aug 2023 12:07




Tgt Ion:117 Resp: 412289


Ion Ratio Lower Upper

117 100

82 56.1 43.9 65.9

119 32.2 26.2 39.4


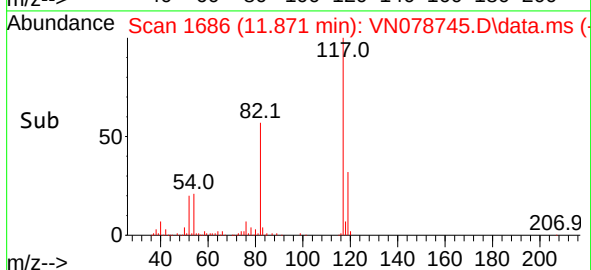
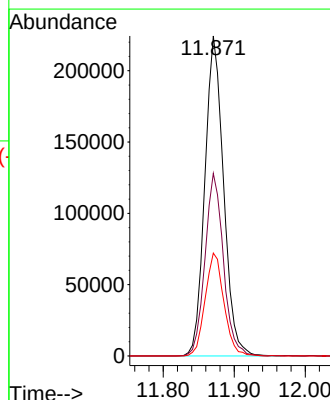
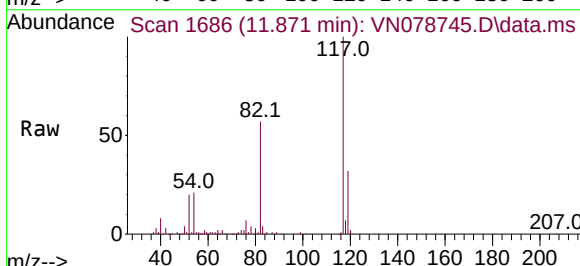


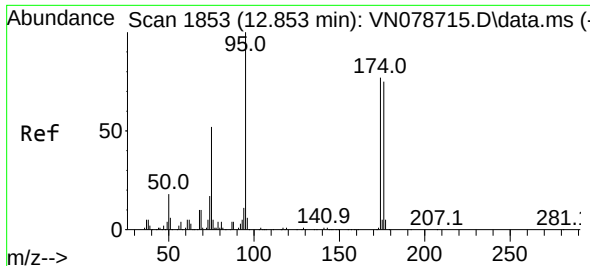

#60
4-Bromofluorobenzene
Concen: 21.285 ug/l
RT: 12.859 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN078745.D
Acq: 03 Aug 2023 12:07

Instrument :
MSVOA_N
ClientSampleId :
VN0803WBL01

Tgt Ion: 95 Resp: 131512
Ion Ratio Lower Upper
95 100
174 82.5 61.7 92.5
176 76.7 58.1 87.1

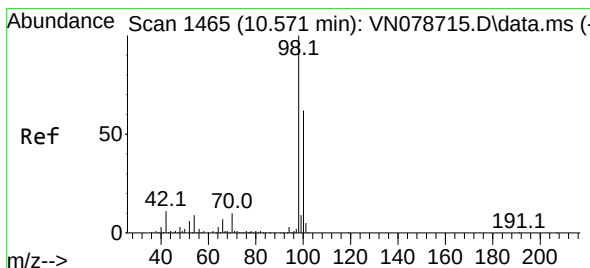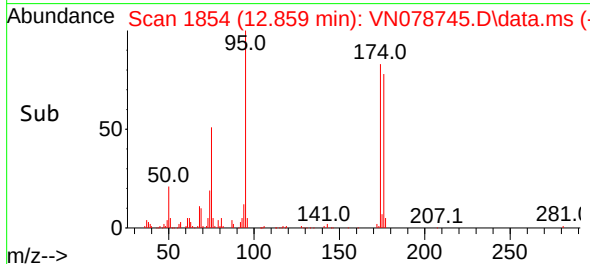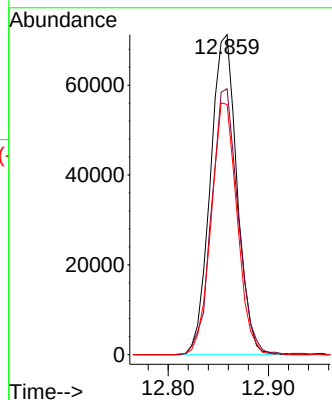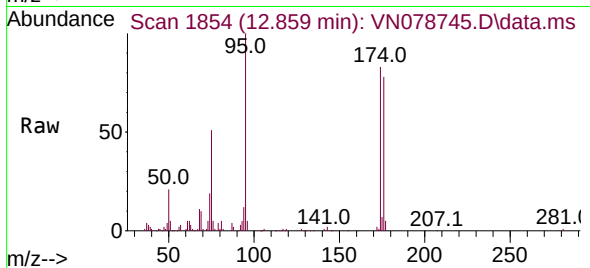

#63
Toluene-d8
Concen: 30.028 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN078745.D
Acq: 03 Aug 2023 12:07

Tgt Ion: 98 Resp: 611584
Ion Ratio Lower Upper
98 100
100 63.0 49.7 74.5

