

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080323\
 Data File : VN078746.D
 Acq On : 03 Aug 2023 12:31
 Operator : JC\MD
 Sample : VN0803WBL02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0803WBL02

Quant Time: Aug 04 06:30:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080123W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Aug 02 04:51:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.824	128	112199	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.106	114	604420	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.870	117	394108	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.588	65	271600	32.294	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	107.633%
60) 4-Bromofluorobenzene	12.853	95	112722	19.085	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	63.633%
63) Toluene-d8	10.571	98	605750	31.114	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	103.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080323\
Data File : VN078746.D
Acq On : 03 Aug 2023 12:31
Operator : JC\MD
Sample : VN0803WBL02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0803WBL02

Quant Time: Aug 04 06:30:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080123W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Aug 02 04:51:47 2023
Response via : Initial Calibration




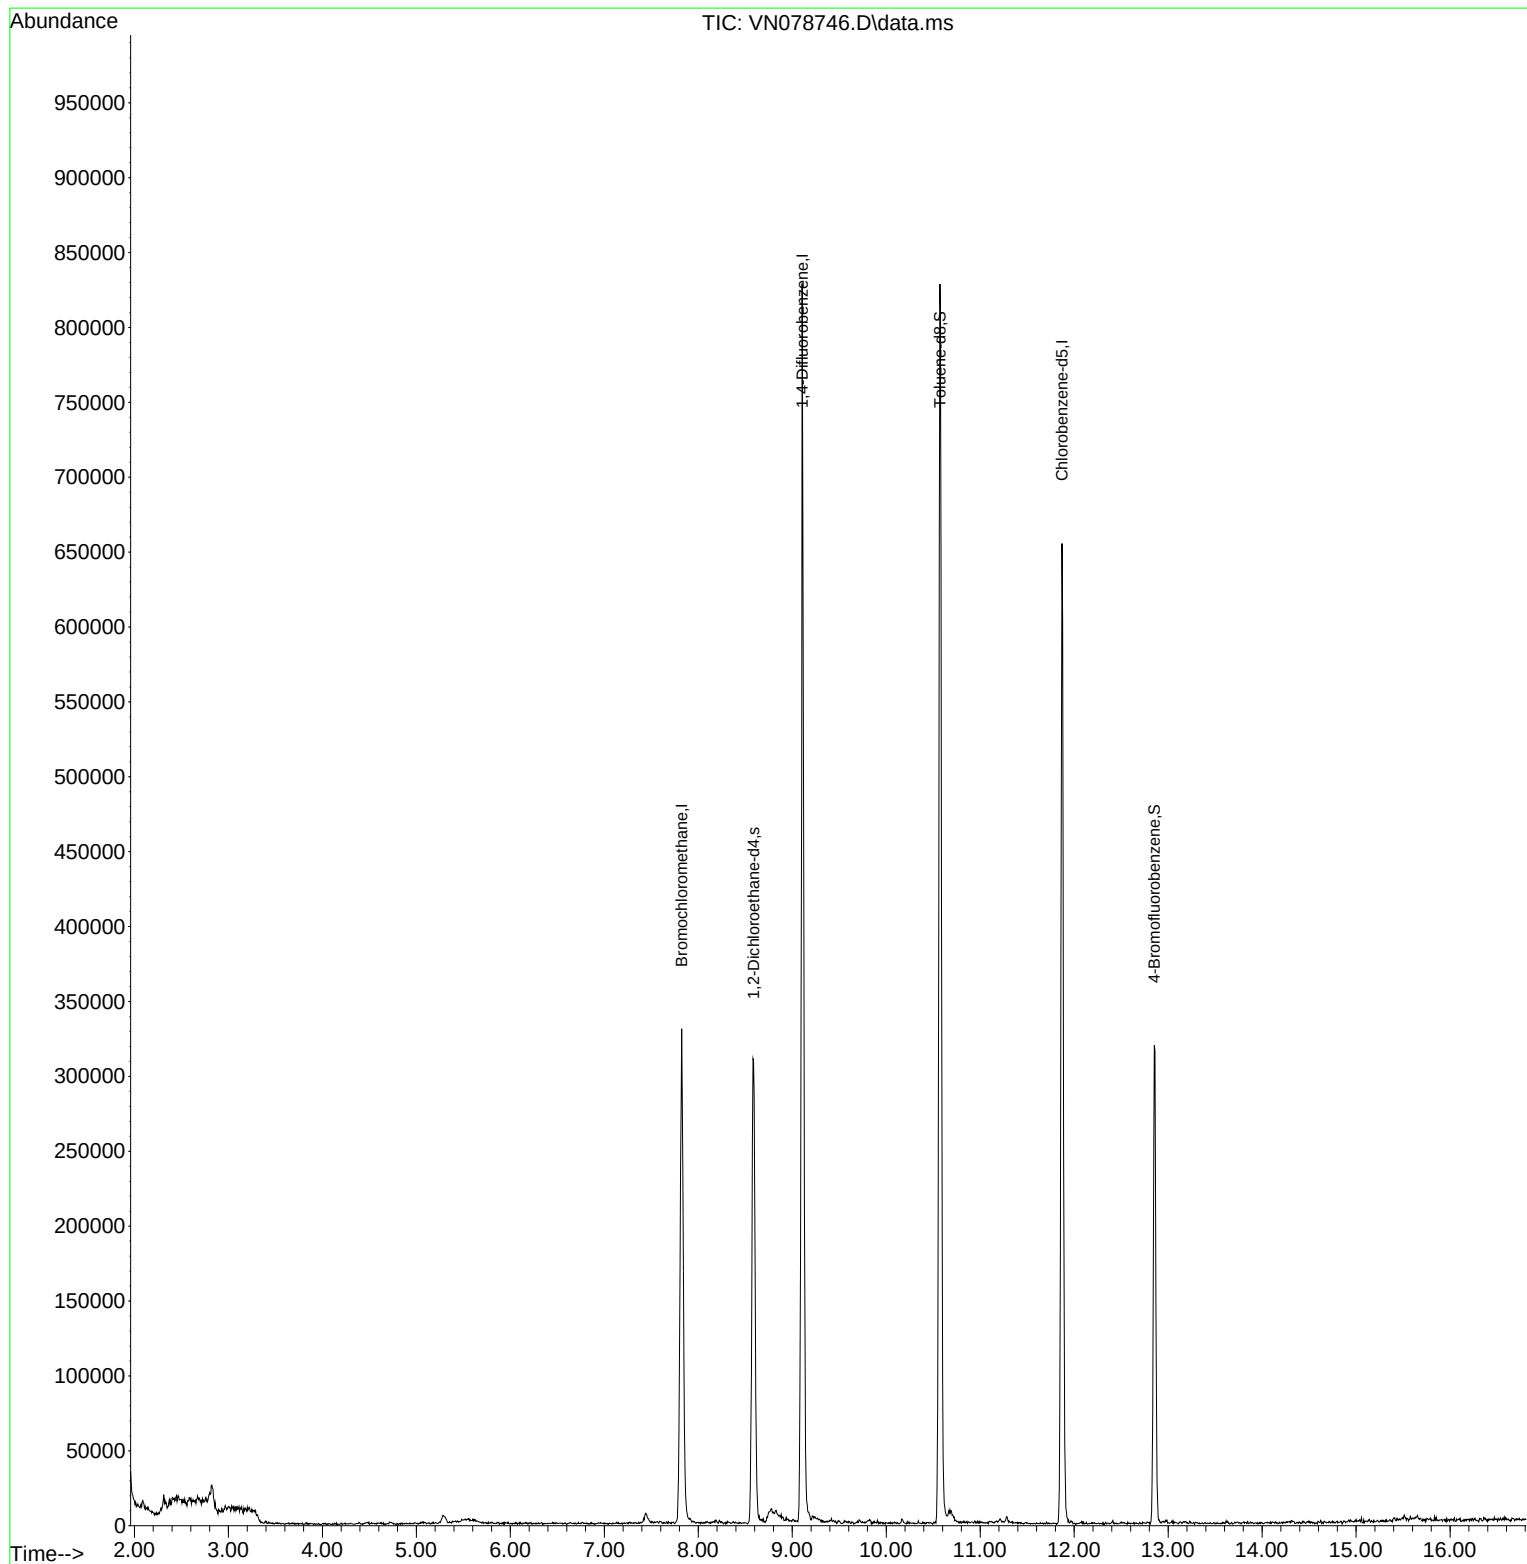


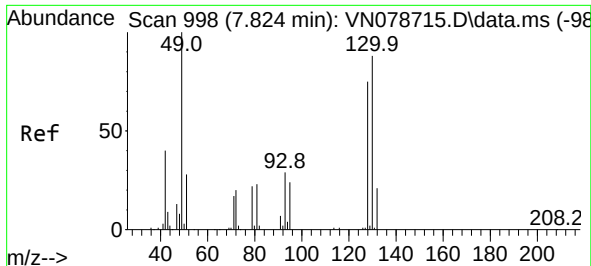

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.824 min Scan# 998
Delta R.T. -0.000 min
Lab File: VN078746.D
Acq: 03 Aug 2023 12:31




Instrument :
MSVOA_N
ClientSampleId :
VN0803WBL02


Tgt Ion:128 Resp: 112199
Ion Ratio Lower Upper
128 100
49 150.4 0.0 370.8
130 127.8 0.0 307.0

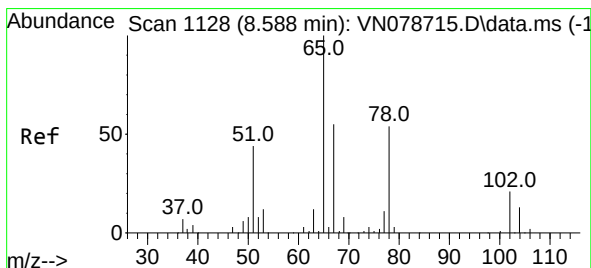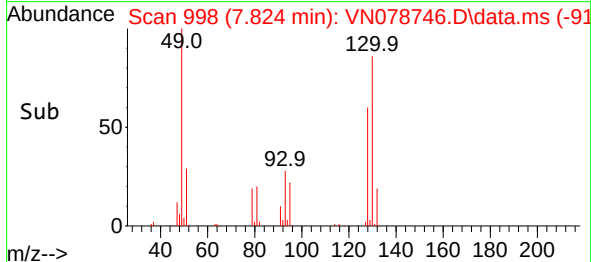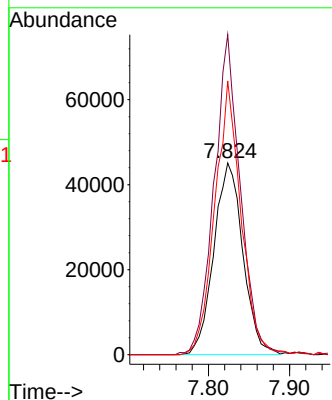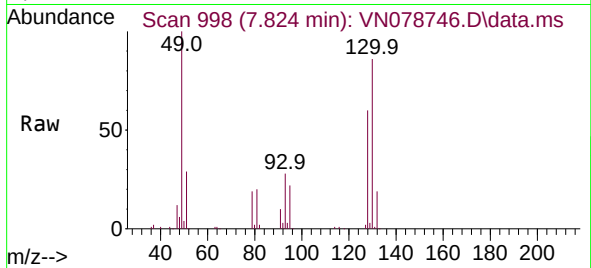

#27
1,2-Dichloroethane-d4
Concen: 32.294 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VN078746.D
Acq: 03 Aug 2023 12:31

Tgt Ion: 65 Resp: 271600
Ion Ratio Lower Upper
65 100
67 52.5 42.9 64.3


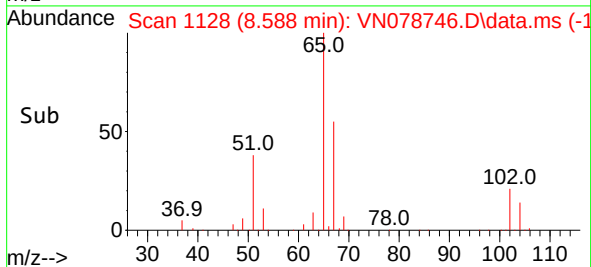
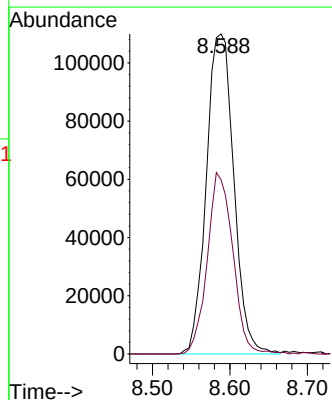
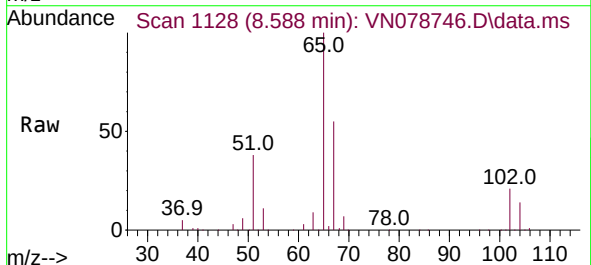


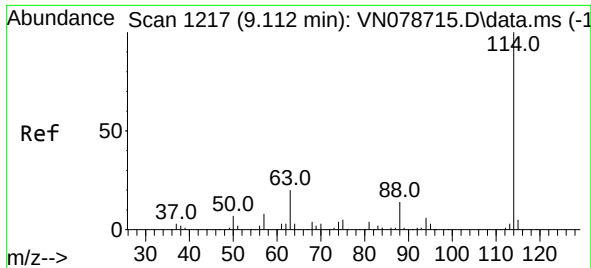

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN078746.D
Acq: 03 Aug 2023 12:31




Instrument :
MSVOA_N
ClientSampleId :
VN0803WBL02


Tgt Ion:114 Resp: 604420
Ion Ratio Lower Upper
114 100
63 19.5 15.2 22.8
88 15.5 12.5 18.7

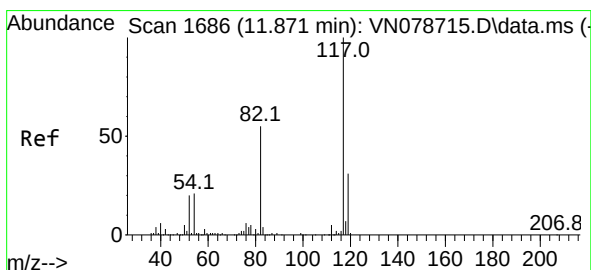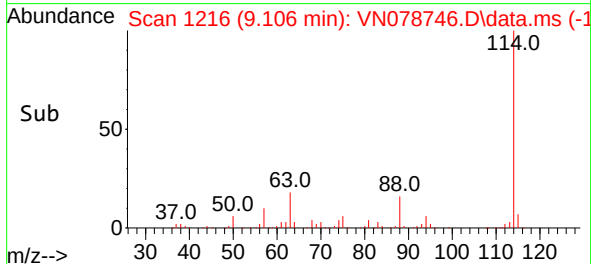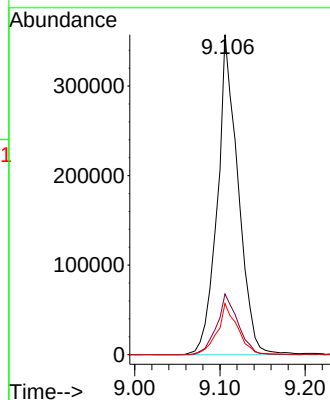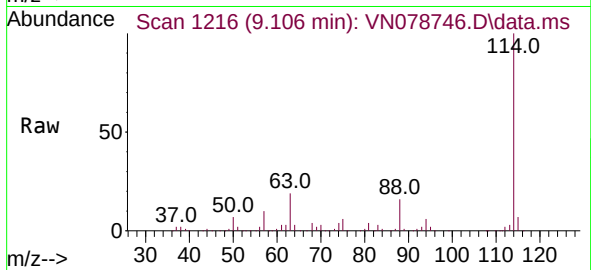

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.870 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VN078746.D
Acq: 03 Aug 2023 12:31

Tgt Ion:117 Resp: 394108
Ion Ratio Lower Upper
117 100
82 55.5 43.9 65.9
119 31.3 26.2 39.4


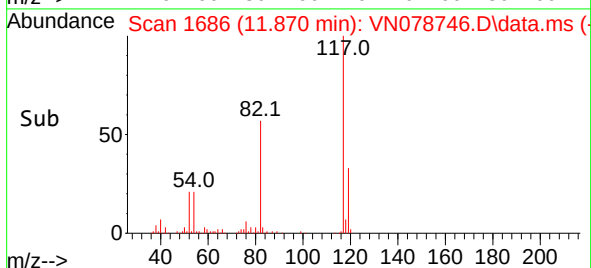
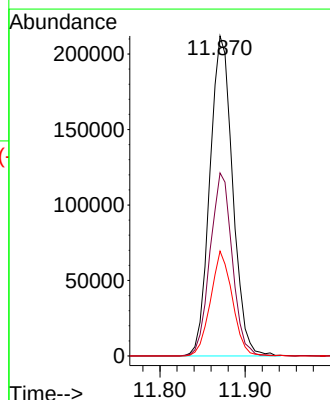
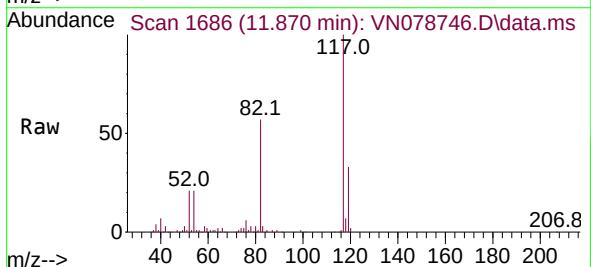


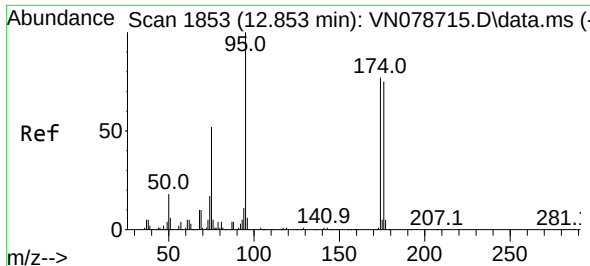

#60
4-Bromofluorobenzene
Concen: 19.085 ug/l
RT: 12.853 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN078746.D
Acq: 03 Aug 2023 12:31

Instrument :
MSVOA_N
ClientSampleId :
VN0803WBL02

Tgt Ion: 95 Resp: 112722
Ion Ratio Lower Upper
95 100
174 84.9 61.7 92.5
176 79.1 58.1 87.1

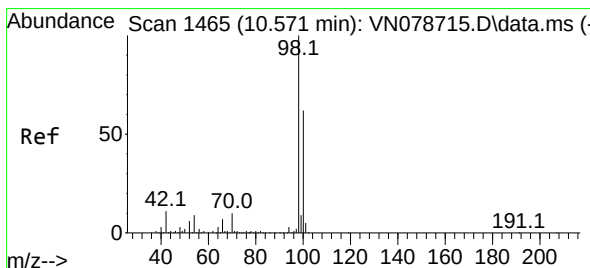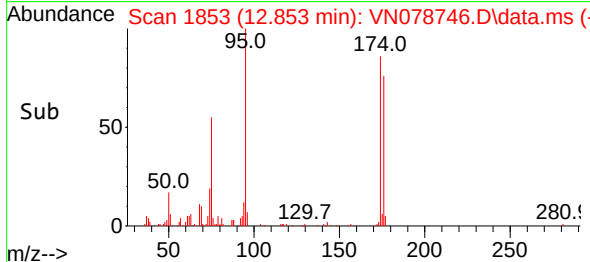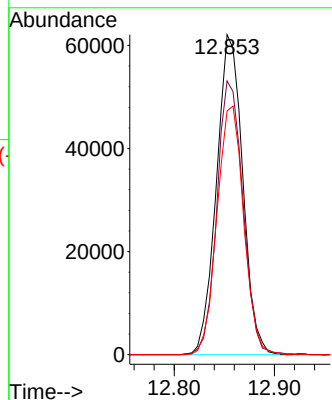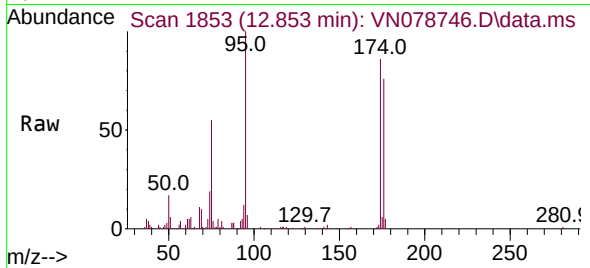

#63
Toluene-d8
Concen: 31.114 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN078746.D
Acq: 03 Aug 2023 12:31

Tgt Ion: 98 Resp: 605750
Ion Ratio Lower Upper
98 100
100 62.1 49.7 74.5

