
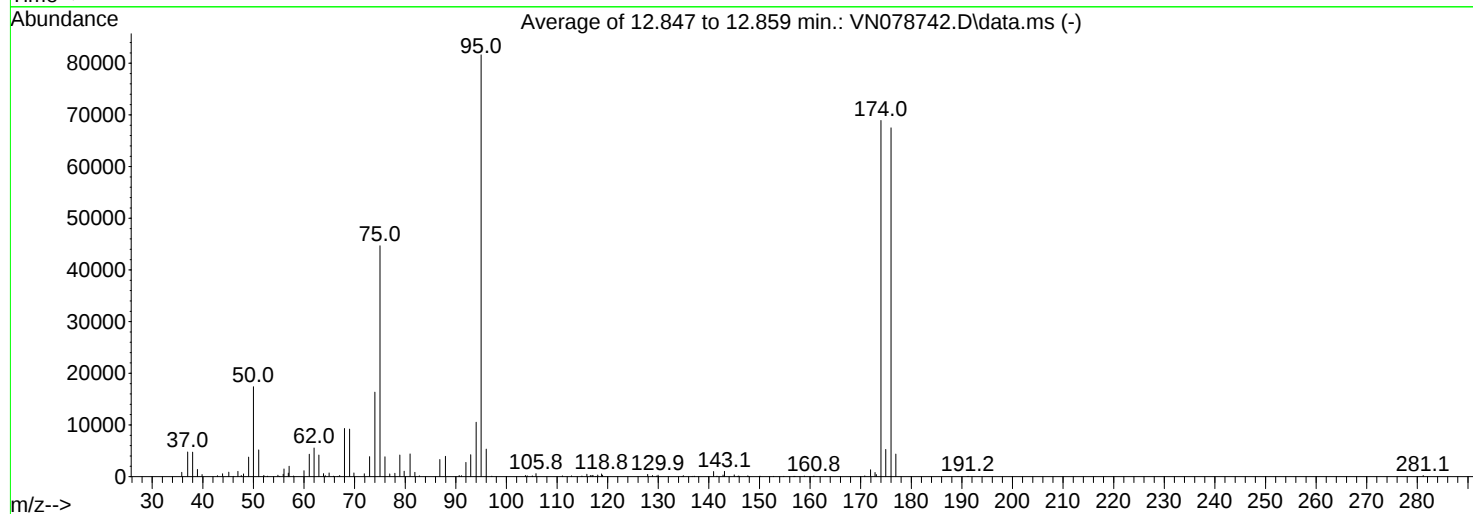


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080323\
Data File : VN078742.D
Acq On : 03 Aug 2023 10:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080123W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Aug 02 04:51:47 2023

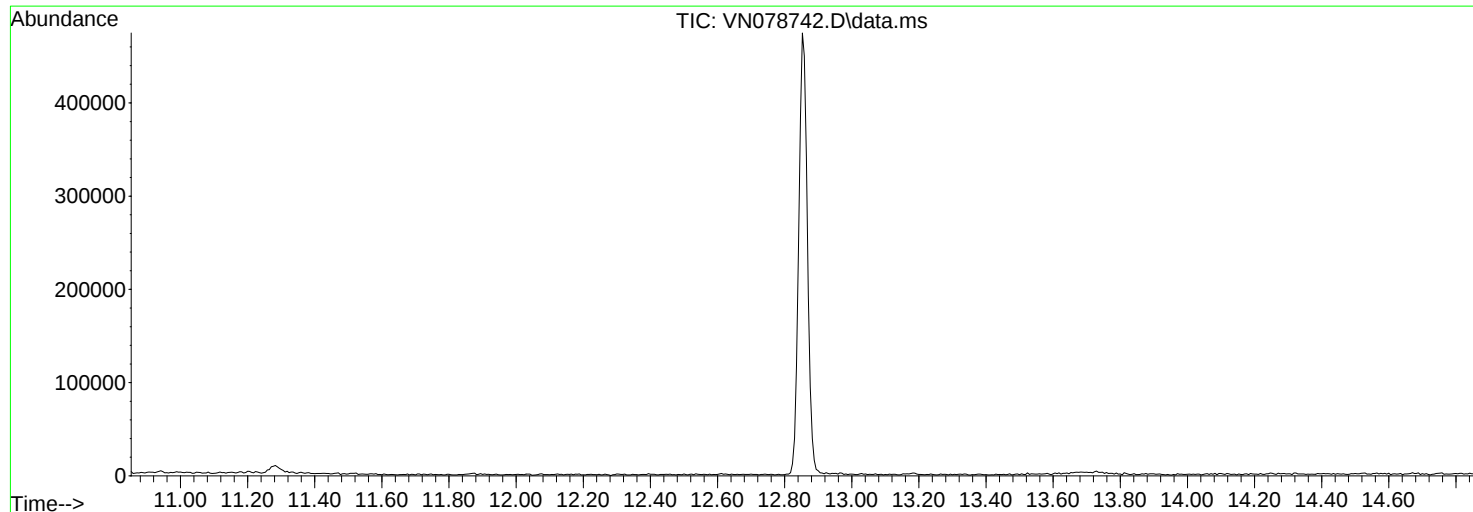

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	17405	PASS
75	95	30	60	54.7	44675	PASS
95	95	100	100	100.0	81624	PASS
96	95	5	9	6.5	5327	PASS
173	174	0.00	2	1.2	809	PASS
174	95	50	100	84.4	68920	PASS
175	174	5	9	7.6	5254	PASS
176	174	95	101	97.9	67501	PASS
177	176	5	9	6.5	4370	PASS