

Data File : VN050361.D
Acq On : 4 Aug 2018 12:53
Operator : MD\SY
Sample : J4328-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-22

Quant Time: Aug 11 00:39:39 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 26 18:10:10 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	646291	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1021557	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	909020	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	393190	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	441308	48.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.88%	
35) Dibromofluoromethane	7.59	113	396279	47.51	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.02%	
50) Toluene-d8	10.09	98	1446710	47.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.36%	
62) 4-Bromofluorobenzene	12.40	95	436995	43.28	ug/l	0.00
Spiked Amount 50.000			Recovery	=	86.56%	
Target Compounds						
19) Methyl tert-butyl Ether	5.05	73	64565	3.253	ug/l	93
39) Methylcyclohexane	9.08	83	30540	2.579	ug/l	91
65) Chlorobenzene	11.44	112	54516	2.374	ug/l	95
91) 1,2-Dichlorobenzene	13.65	146	9096	0.635	ug/l	94
95) Naphthalene	15.14	128	12073	5.028	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VN050361.D
Acq On : 4 Aug 2018 12:53
Operator : MD\SY
Sample : J4328-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-22

Quant Time: Aug 11 00:39:39 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 26 18:10:10 2018
Response via : Initial Calibration

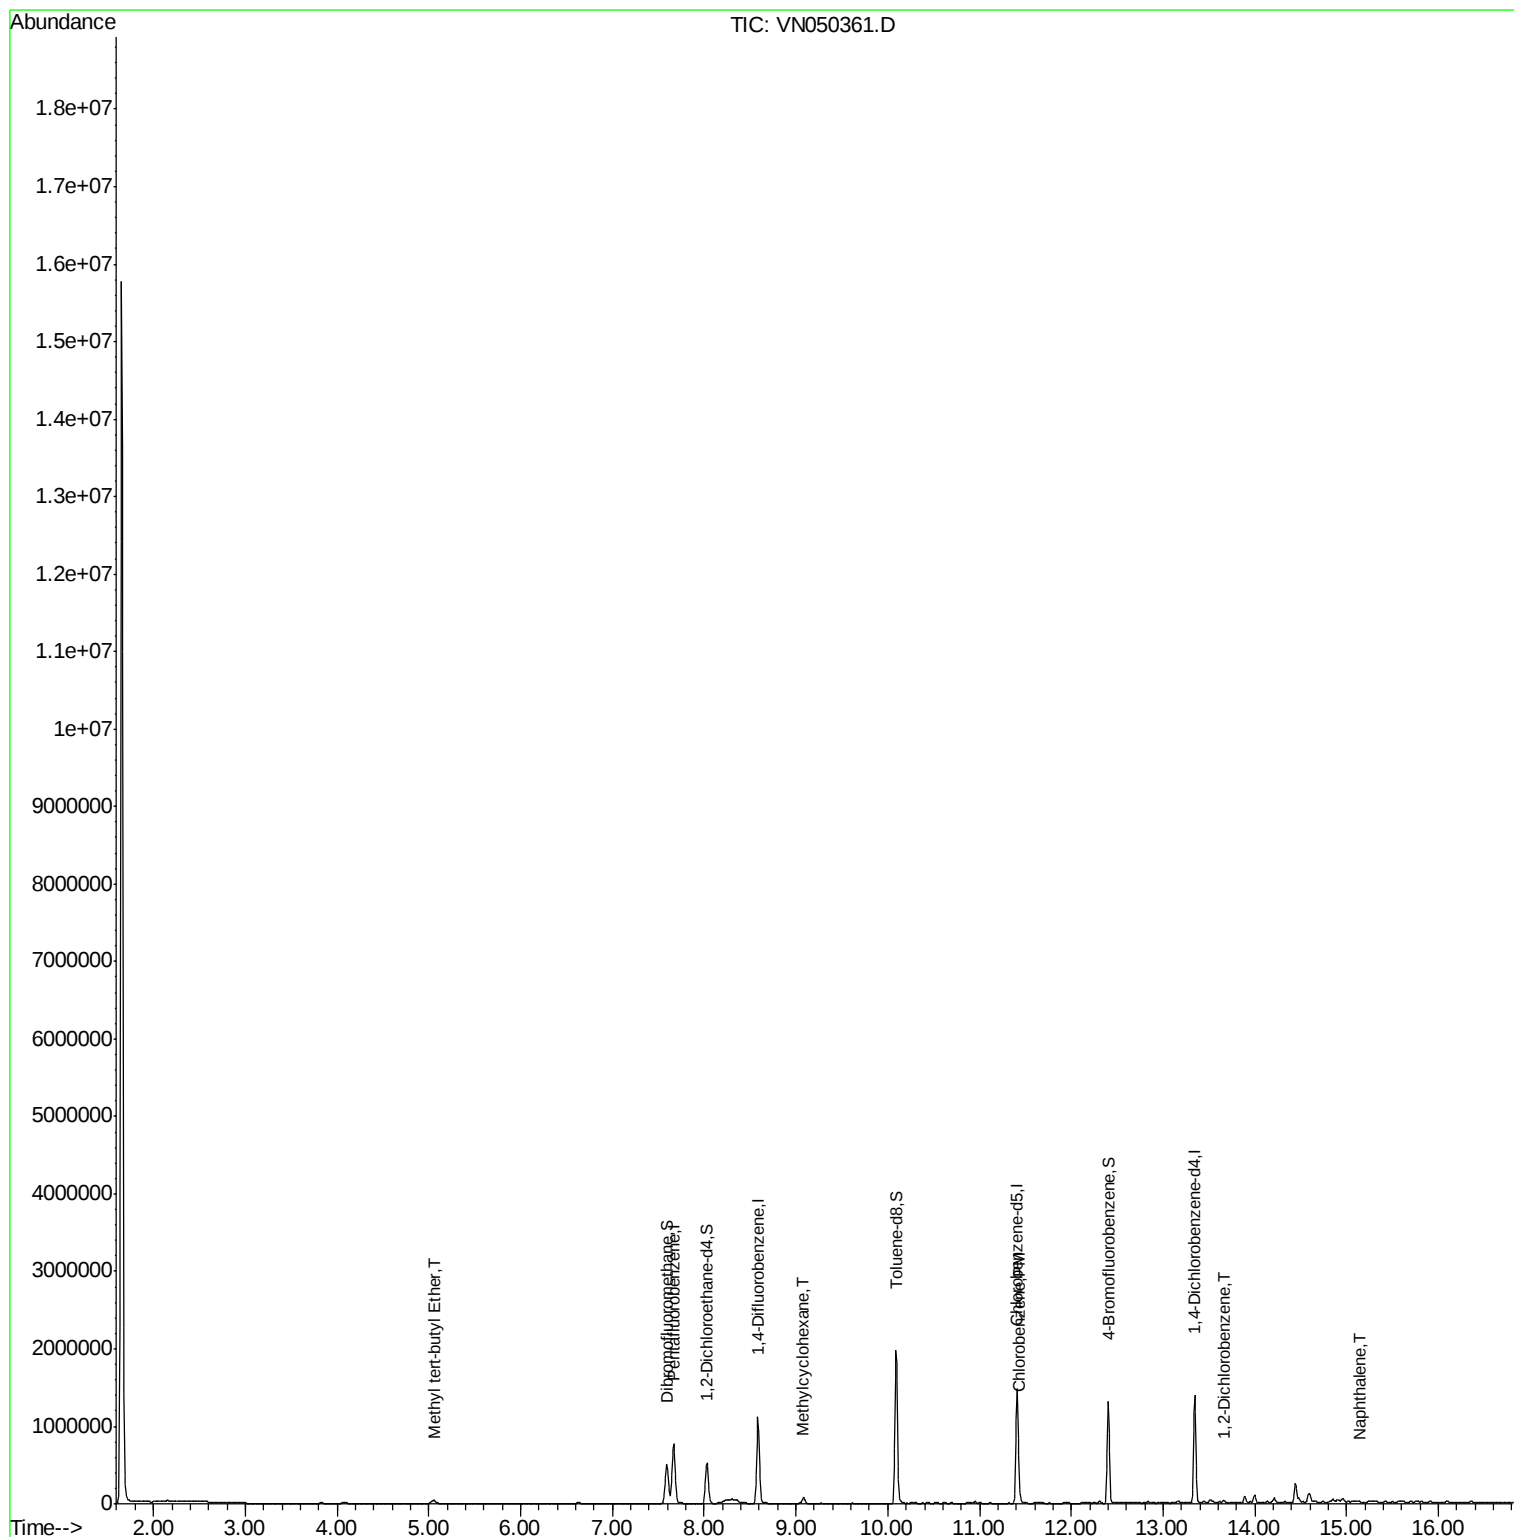



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1890

Delta R.T. -0.00 min

Lab File: VN050361.D

Acq: 4 Aug 2018 12:53

Instrument :

MSVOA_N

ClientSampled :


MW-22

Tgt Ion:168 Resp: 646291

Ion Ratio Lower Upper

168 100

99 52.0 40.0 60.0

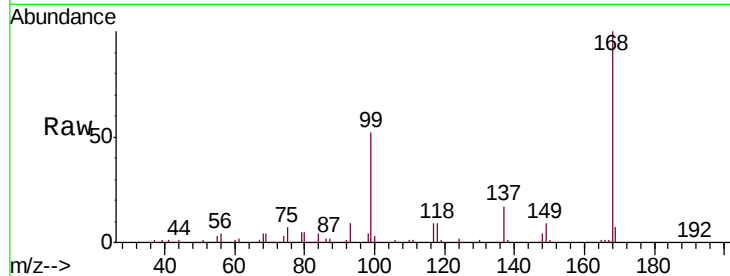

Abundance Ion 167.90 (167.60 to 168.60): VN050018.D (-1870) (-)

Ion 98.90 (98.60 to 99.60): VN050018.D (-1870) (-)

7.67

250000

200000

150000



100000

50000

0

7.60 7.70 7.80

Time-->

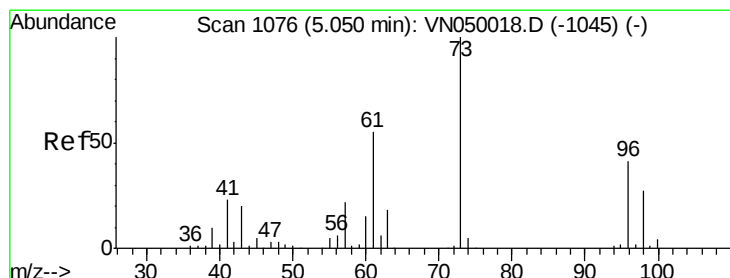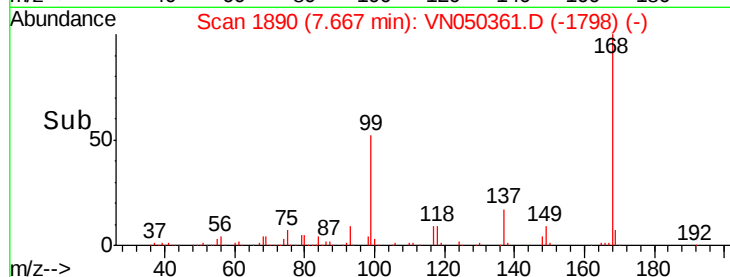

#19

Methyl tert-butyl Ether

Concen: 3.253 ug/l

RT: 5.05 min Scan# 1077

Delta R.T. 0.00 min

Lab File: VN050361.D


Acq: 4 Aug 2018 12:53

Tgt Ion: 73 Resp: 64565

Ion Ratio Lower Upper

73 100

57 25.7 18.0 27.0

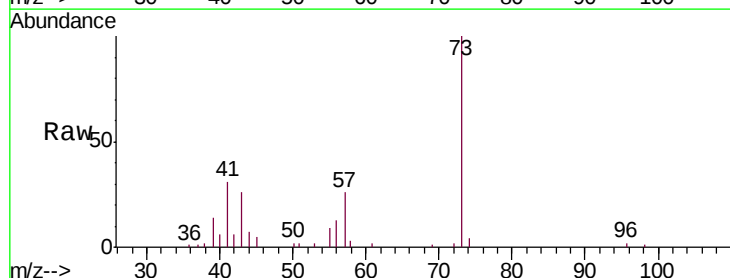

Abundance Ion 73.00 (72.70 to 73.70): VN050018.D (-1045) (-)

Ion 57.00 (56.70 to 57.70): VN050018.D (-1045) (-)

5.05

20000

15000


10000


5000

0

4.90 5.00 5.10

Time-->

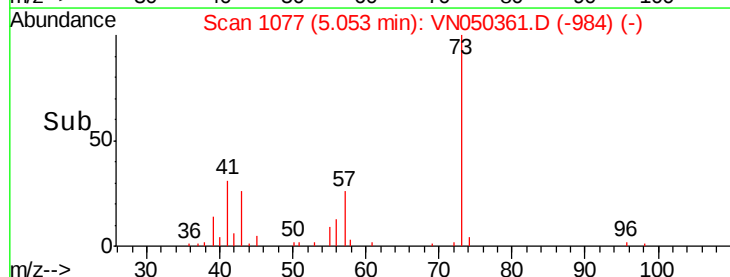

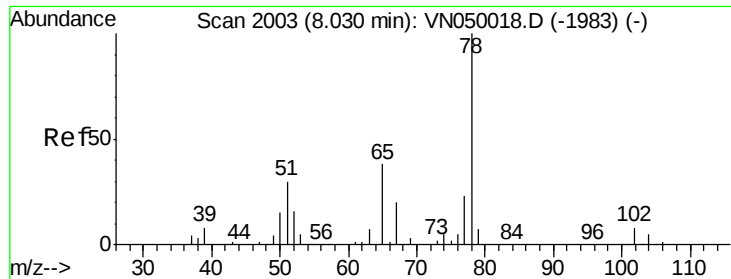

#33

1,2-Dichloroethane-d4

Concen: 48.940 ug/l

RT: 8.03 min Scan# 2003

Delta R.T. 0.00 min

Lab File: VN050361.D

Acq: 4 Aug 2018 12:53

Instrument :

MSVOA_N

ClientSampleId :


MW-22

Tgt Ion: 65 Resp: 441308

Ion Ratio Lower Upper

65 100

67 54.0 0.0 108.4

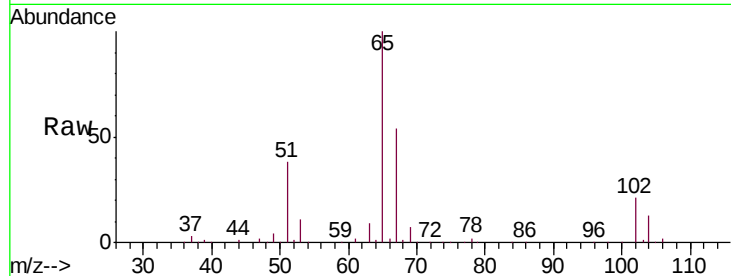

Abundance Ion 64.90 (64.60 to 65.60): VN050018.D (-1983) (-)

Ion 66.90 (66.60 to 67.60): VN050018.D (-1983) (-)

8.03

200000

150000



100000

50000

0

8.00 8.10

Time-->

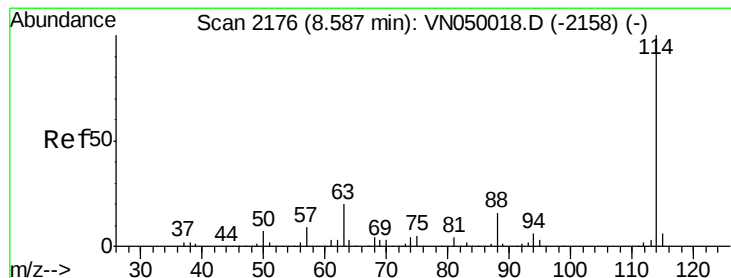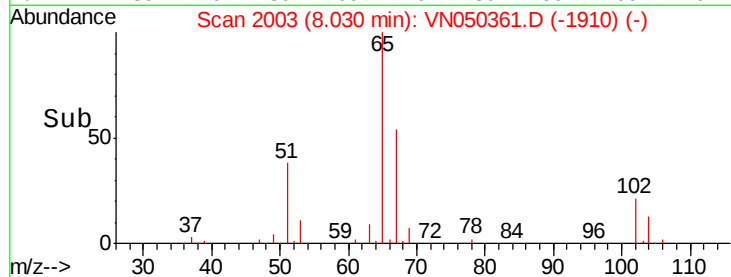

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2176

Delta R.T. -0.00 min

Lab File: VN050361.D

Acq: 4 Aug 2018 12:53


Tgt Ion: 114 Resp: 1021557

Ion Ratio Lower Upper

114 100

63 20.5 0.0 40.0

88 15.5 0.0 31.2

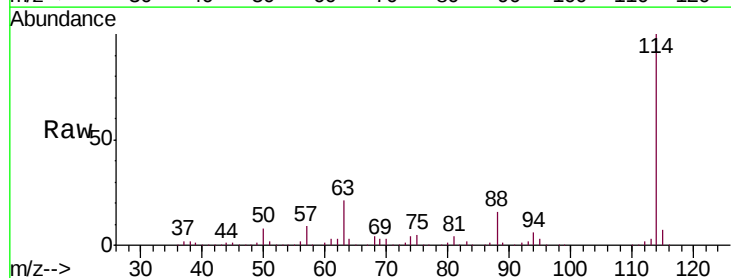

Abundance Ion 113.90 (113.60 to 114.60): VN050018.D (-2158) (-)

Ion 63.00 (62.70 to 63.70): VN050018.D (-2158) (-)

Ion 87.90 (87.60 to 88.60): VN050018.D (-2158) (-)

8.59

600000

500000

400000

300000


200000


100000

0

8.50 8.60 8.70

Time-->




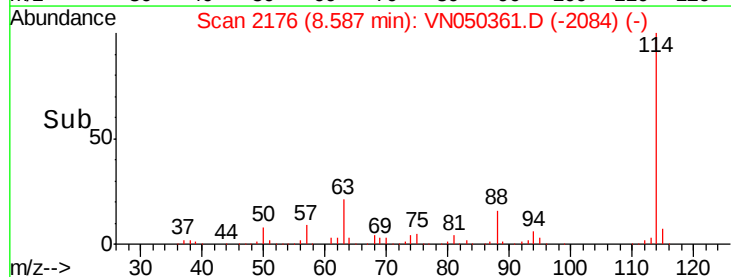


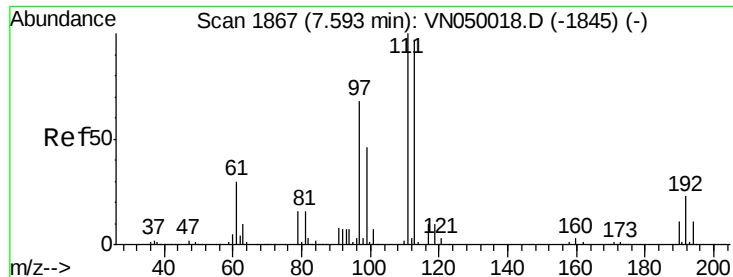

#35
Dibromofluoromethane
Concen: 47.511 ug/l
RT: 7.59 min Scan# 1867
Delta R.T. 0.00 min
Lab File: VN050361.D
Acq: 4 Aug 2018 12:53




Instrument :
MSVOA_N
ClientSampled :
MW-22


Tgt Ion: 113 Resp: 396279
Ion Ratio Lower Upper
113 100
111 101.6 80.7 121.1
192 22.4 17.8 26.6

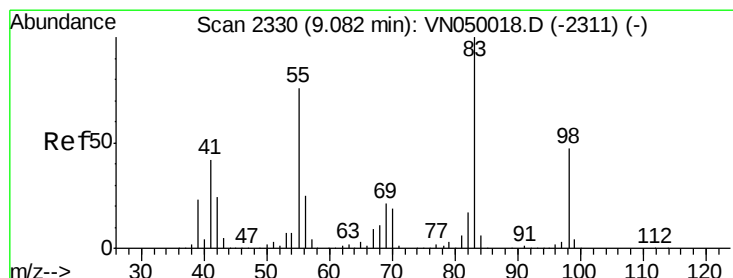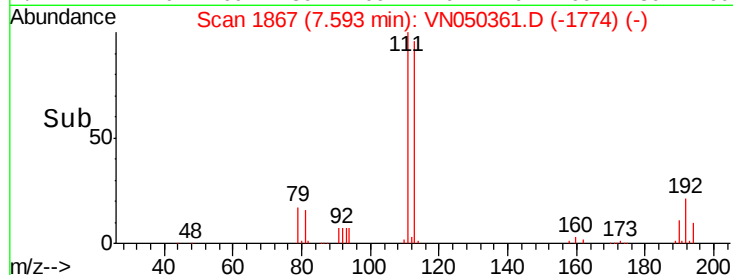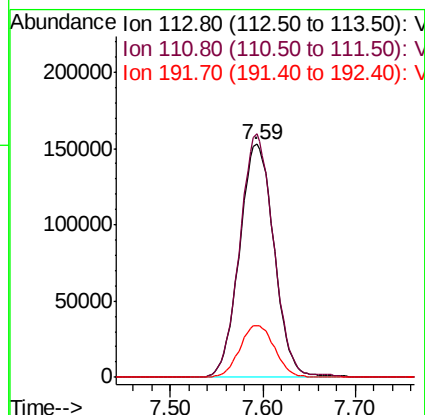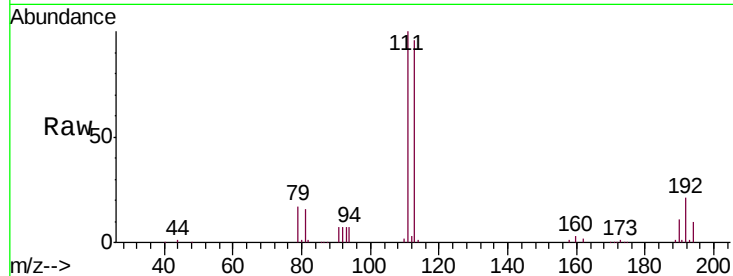

#39
Methylcyclohexane
Concen: 2.579 ug/l
RT: 9.08 min Scan# 2330
Delta R.T. -0.00 min
Lab File: VN050361.D
Acq: 4 Aug 2018 12:53

Tgt Ion: 83 Resp: 30540
Ion Ratio Lower Upper
83 100
55 87.5 61.8 92.8
98 48.0 36.5 54.7


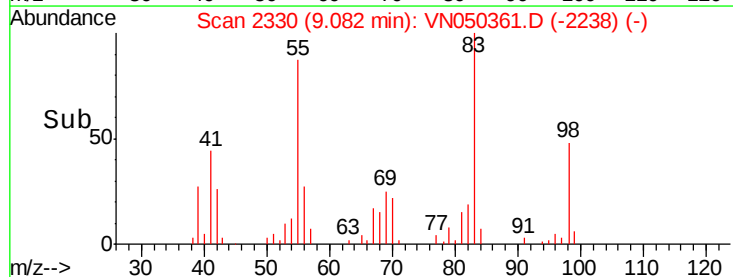
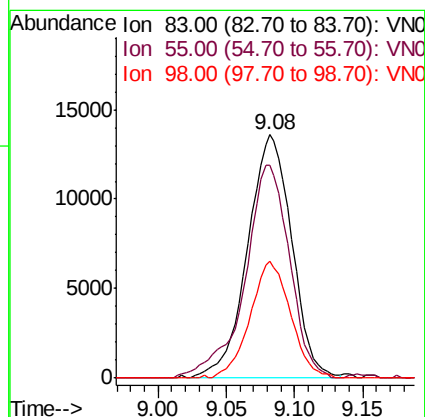
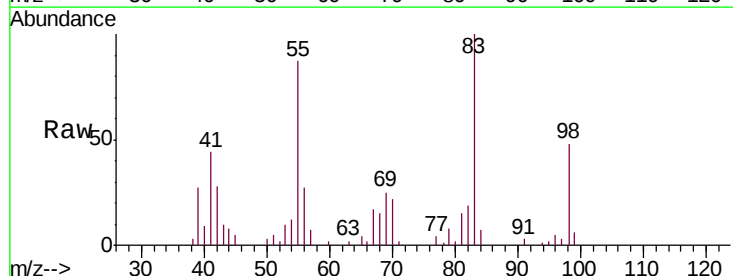


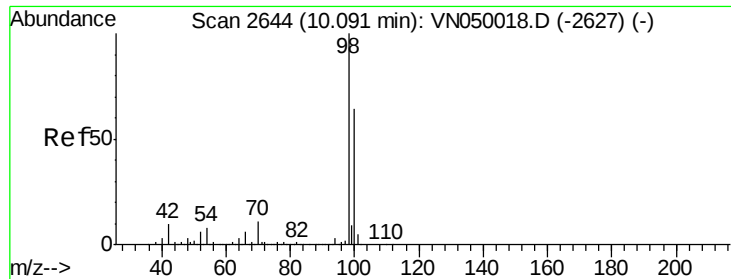

#50
Toluene-d8
Concen: 47.179 ug/l
RT: 10.09 min Scan# 2644
Delta R.T. -0.00 min
Lab File: VN050361.D
Acq: 4 Aug 2018 12:53




Instrument :
MSVOA_N
ClientSampleId :
MW-22


Tgt Ion: 98 Resp: 1446710
Ion Ratio Lower Upper
98 100
100 63.0 50.7 76.1

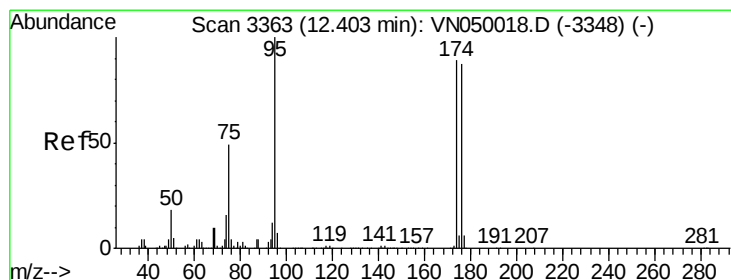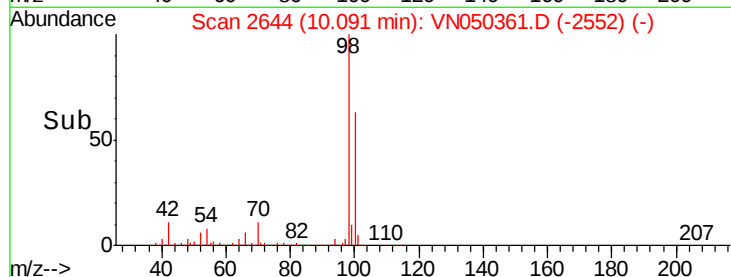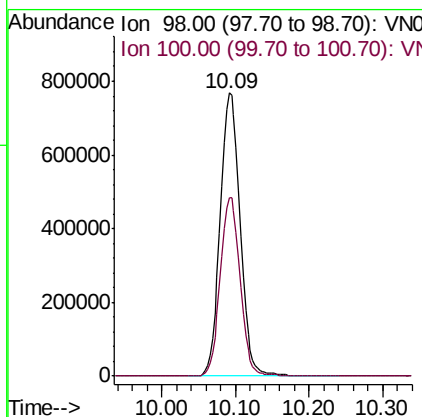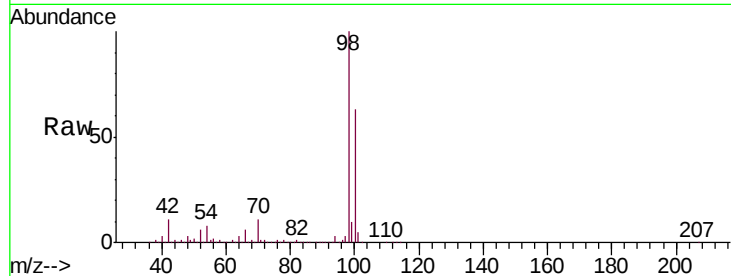

#62
4-Bromofluorobenzene
Concen: 43.280 ug/l
RT: 12.40 min Scan# 3363
Delta R.T. 0.00 min
Lab File: VN050361.D
Acq: 4 Aug 2018 12:53

Tgt Ion: 95 Resp: 436995
Ion Ratio Lower Upper
95 100
174 90.7 0.0 178.2
176 86.7 0.0 173.4


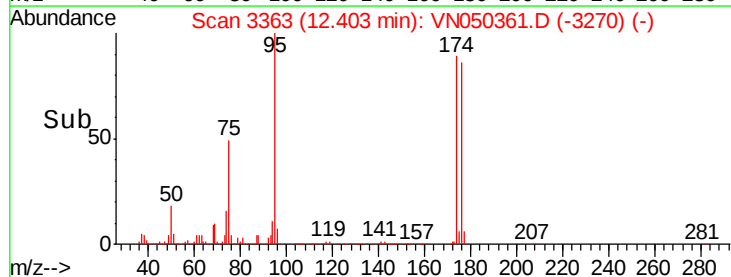
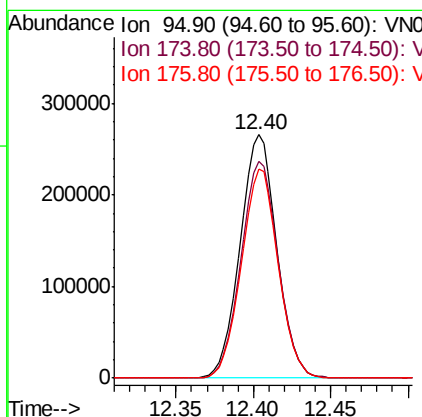
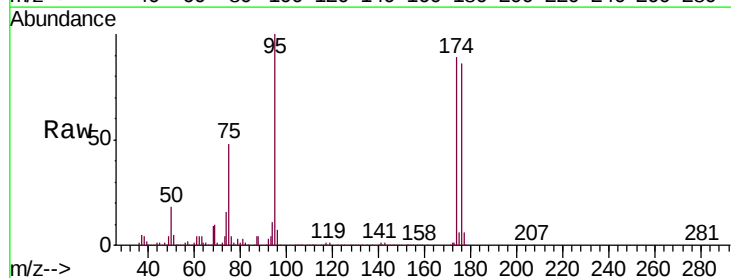


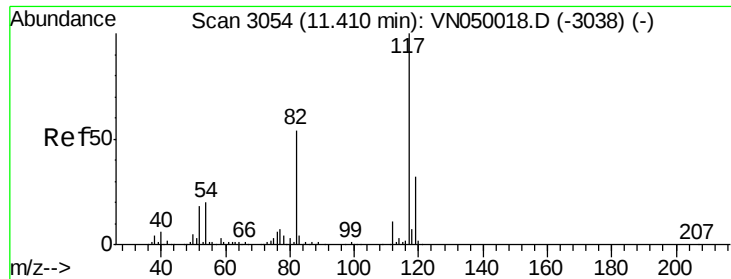

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. 0.00 min
Lab File: VN050361.D
Acq: 4 Aug 2018 12:53




Instrument :
MSVOA_N
ClientSampleId :
MW-22


Tgt Ion	Ratio	Lower	Upper
117	100		
82	53.3	43.7	65.5
119	32.6	26.1	39.1

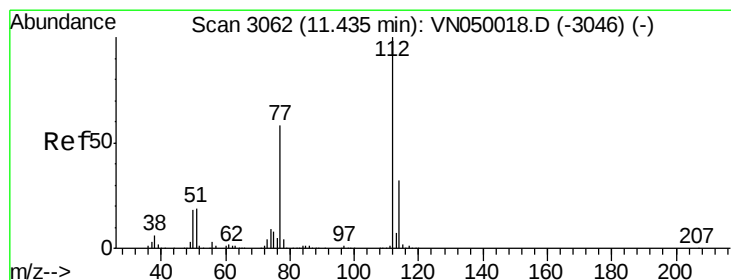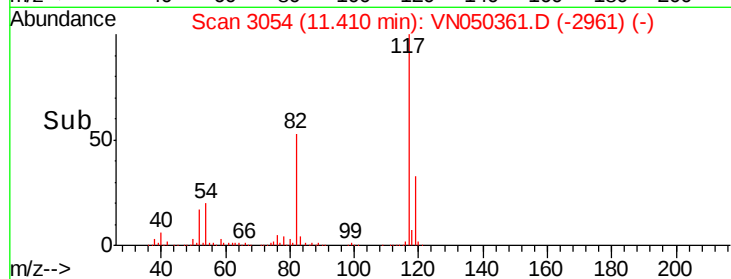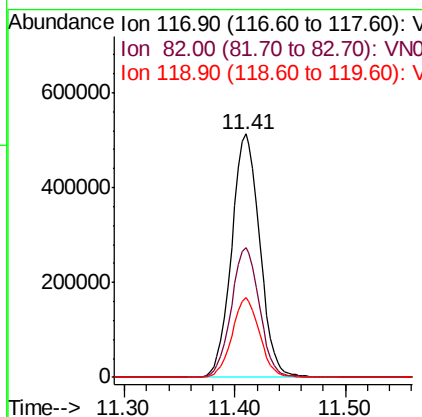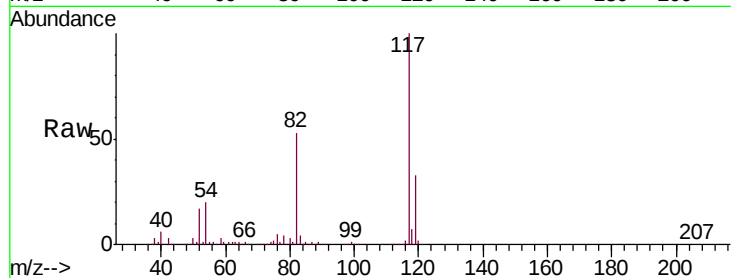

#65
Chlorobenzene
Concen: 2.374 ug/l
RT: 11.44 min Scan# 3062
Delta R.T. 0.00 min
Lab File: VN050361.D
Acq: 4 Aug 2018 12:53

Tgt Ion	Ratio	Lower	Upper
112	100		
114	35.0	25.6	38.4

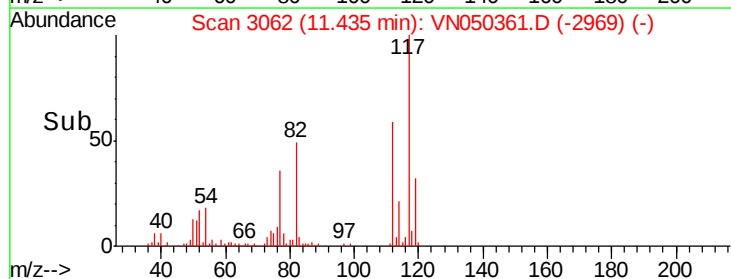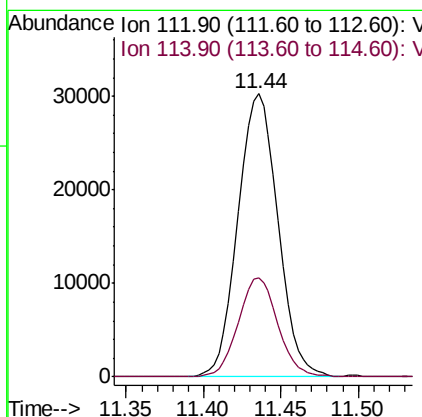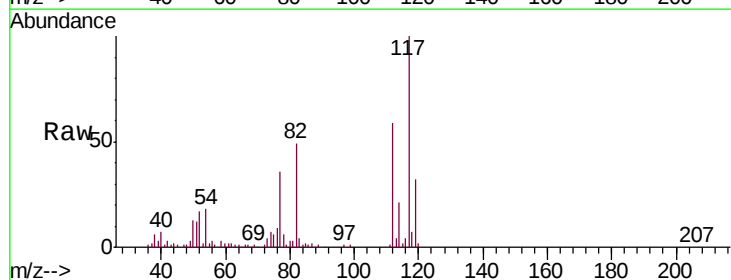

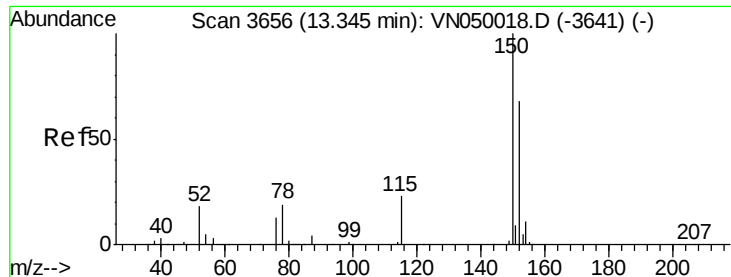

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3656

Delta R.T. 0.00 min

Lab File: VN050361.D

Acq: 4 Aug 2018 12:53

Instrument :

MSVOA_N

ClientSampleId :

MW-22


Tgt Ion:152 Resp: 393190

Ion Ratio Lower Upper

152 100

115 56.3 27.8 83.3




150 156.7 0.0 348.6

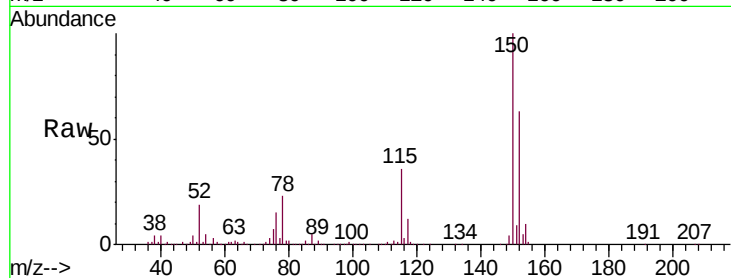

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

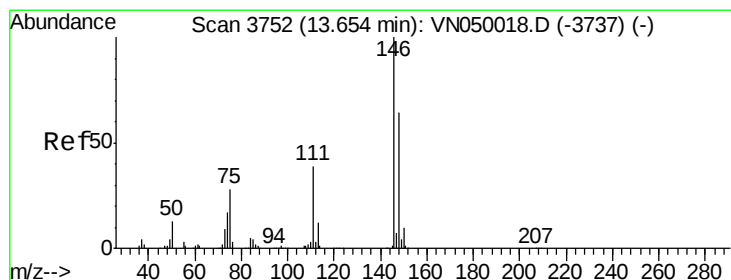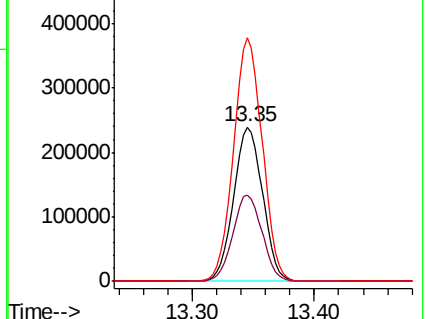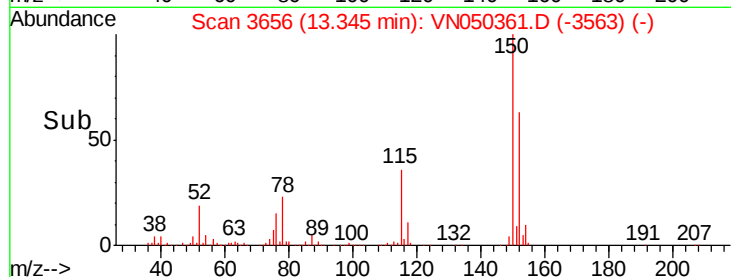

#91

1,2-Dichlorobenzene

Concen: 0.635 ug/l

RT: 13.65 min Scan# 3752

Delta R.T. 0.00 min

Lab File: VN050361.D

Acq: 4 Aug 2018 12:53


Tgt Ion:146 Resp: 9096

Ion Ratio Lower Upper

146 100

111 39.0 19.6 58.7



148 57.2 32.1 96.3

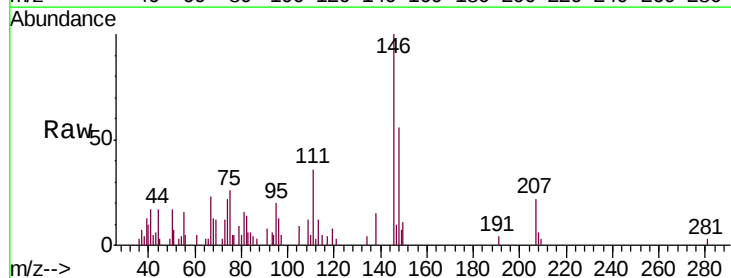


Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V

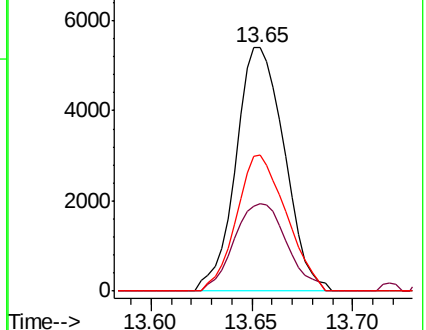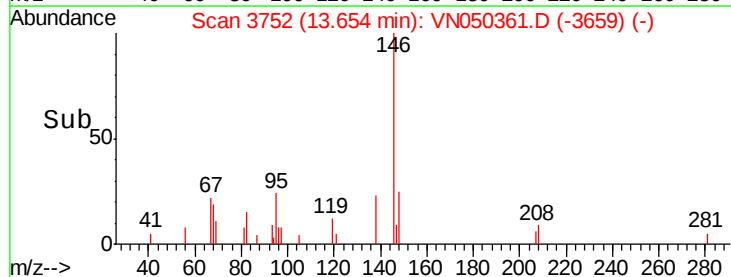

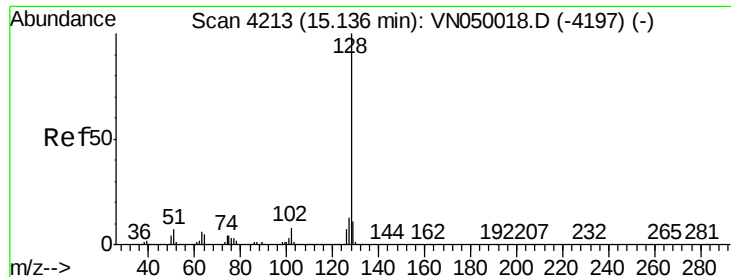

#95
Naphthalene
Concen: 5.028 ug/l
RT: 15.14 min Scan# 4213
Delta R.T. 0.00 min
Lab File: VN050361.D
Acq: 4 Aug 2018 12:53

Instrument :
MSVOA_N
ClientSampleId :
MW-22

Tgt Ion	Ratio	Lower	Upper
128	100		
127	14.2	10.4	15.6
129	11.6	8.8	13.2

