

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080422\
 Data File : VN073729.D
 Acq On : 04 Aug 2022 12:03
 Operator : JC\MD
 Sample : VN0804WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0804WBL01

Quant Time: Aug 05 00:24:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 29 02:20:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	372468	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	604275	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	569349	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	266911	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	222905	49.107	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.220%
35) Dibromofluoromethane	7.957	113	206045	54.301	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	108.600%
50) Toluene-d8	10.380	98	679859	45.531	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	91.060%
62) 4-Bromofluorobenzene	12.674	95	247042	49.598	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080422\
Data File : VN073729.D
Acq On : 04 Aug 2022 12:03
Operator : JC\MD
Sample : VN0804WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0804WBL01

Quant Time: Aug 05 00:24:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 29 02:20:25 2022
Response via : Initial Calibration




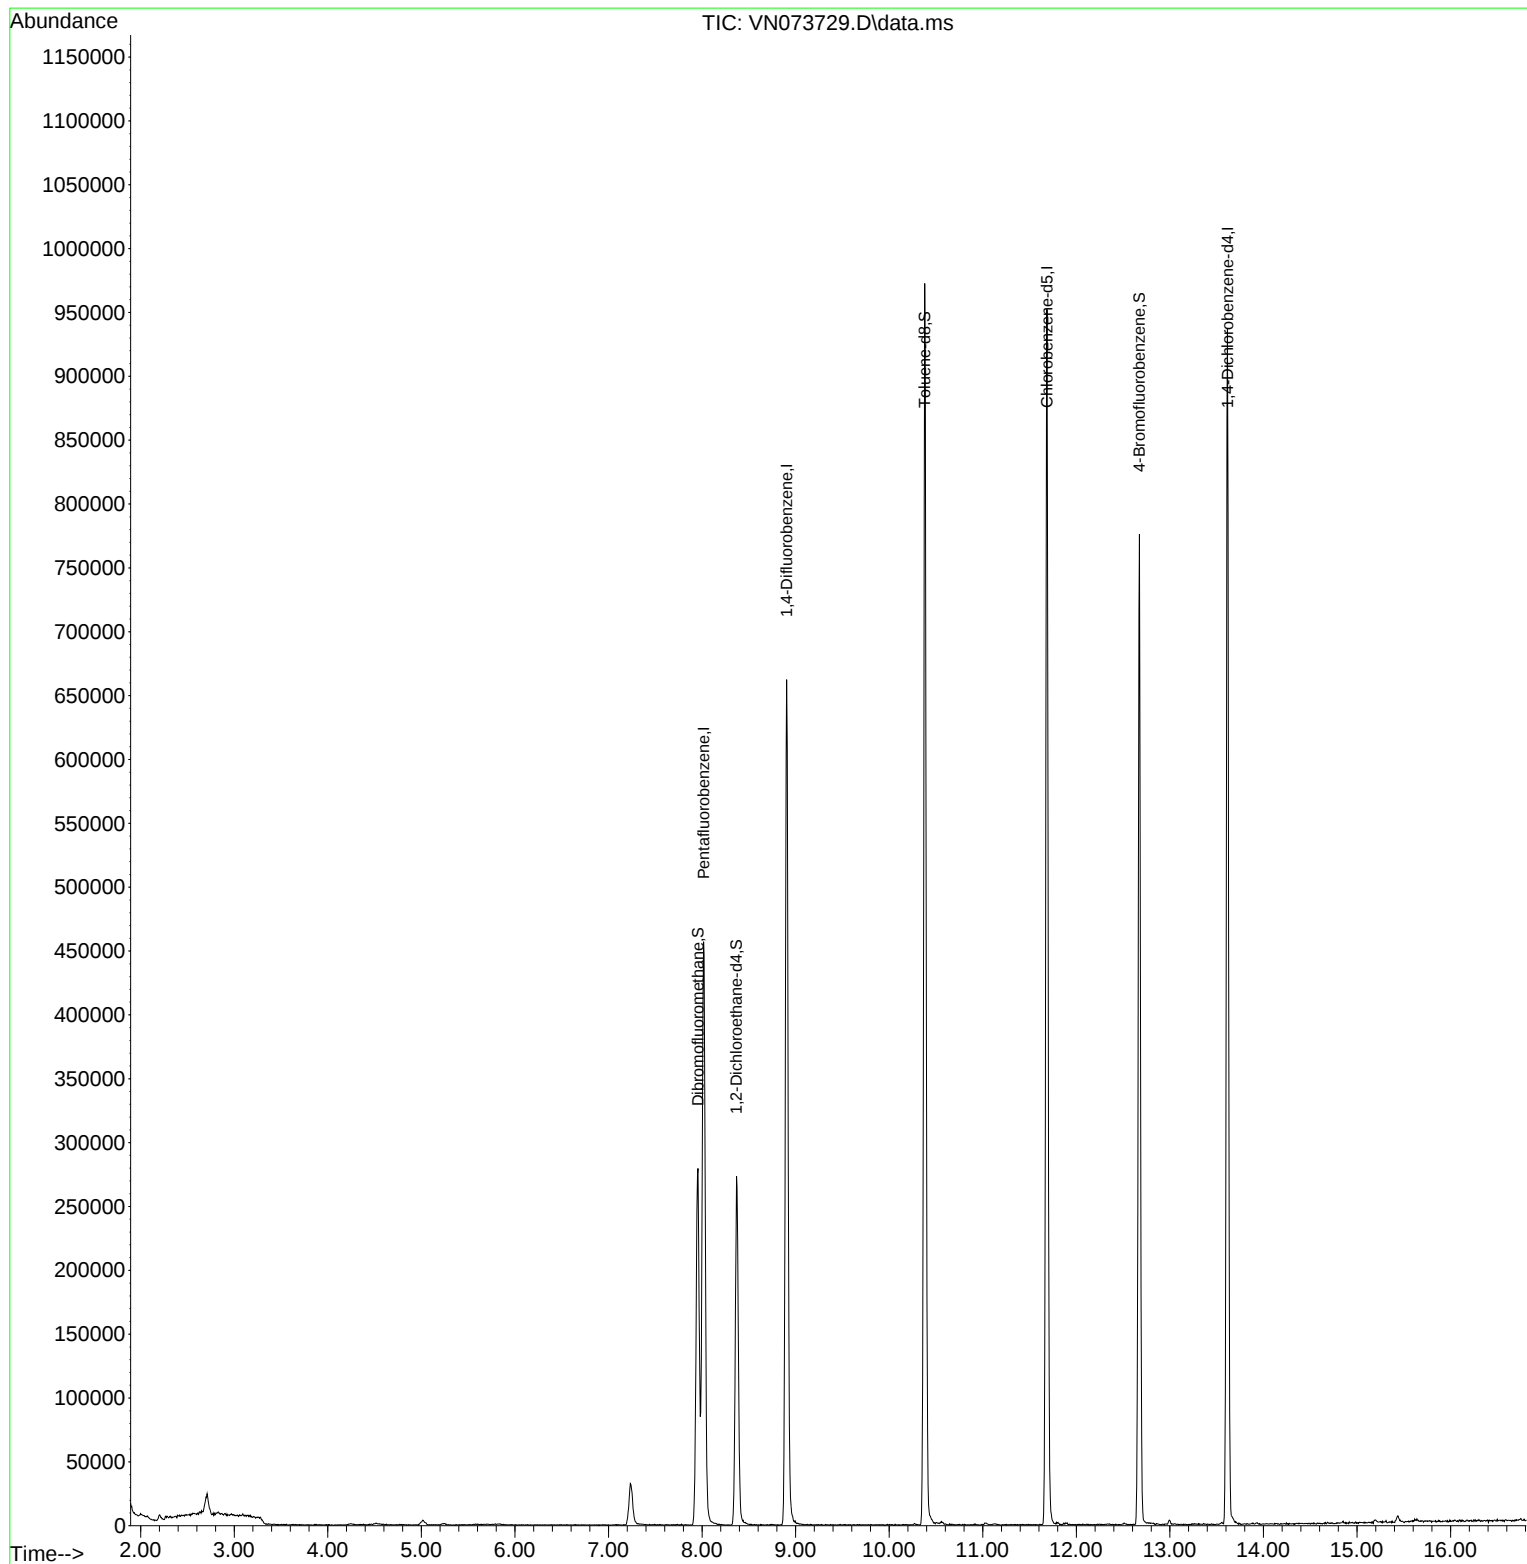


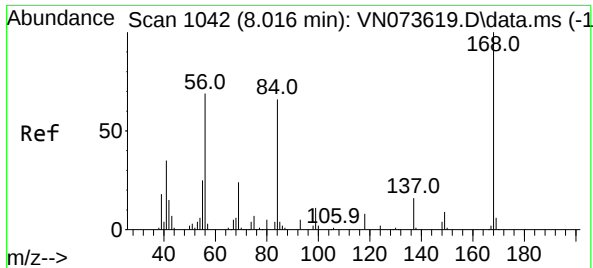

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073729.D
Acq: 04 Aug 2022 12:03




Instrument :
MSVOA_N
ClientSampleId :
VN0804WBL01


Tgt Ion:168 Resp: 372468
Ion Ratio Lower Upper
168 100
99 53.6 42.3 63.5

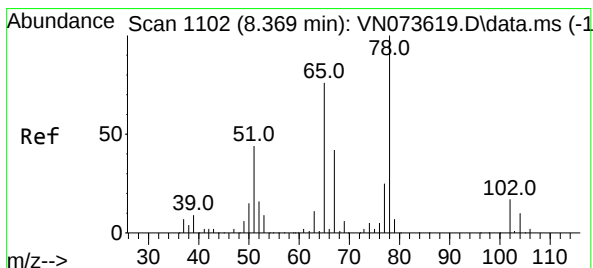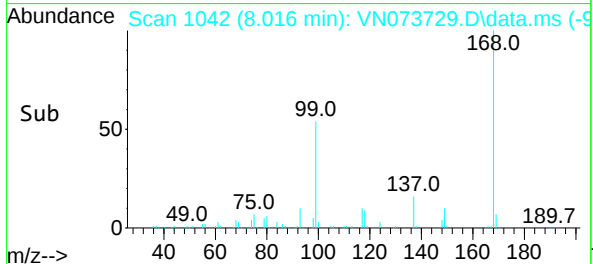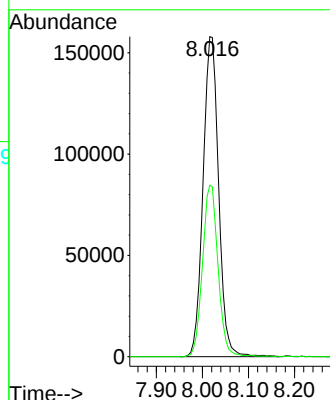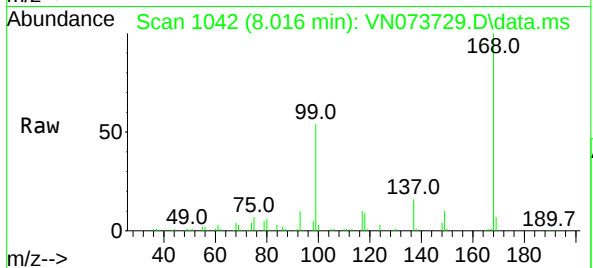

#33
1,2-Dichloroethane-d4
Concen: 49.107 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN073729.D
Acq: 04 Aug 2022 12:03

Tgt Ion: 65 Resp: 222905
Ion Ratio Lower Upper
65 100
67 53.9 0.0 104.8

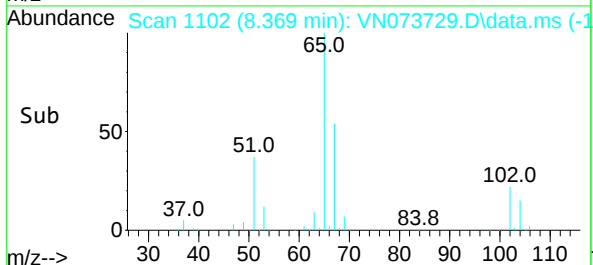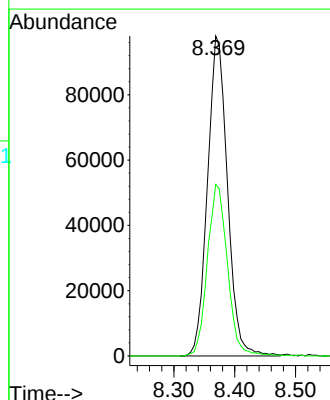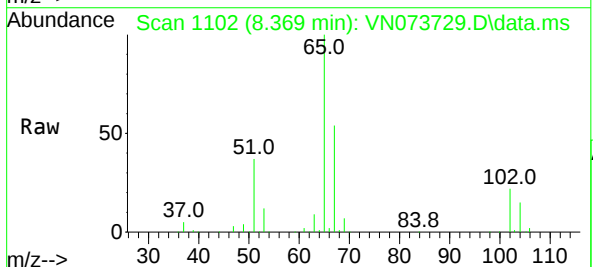

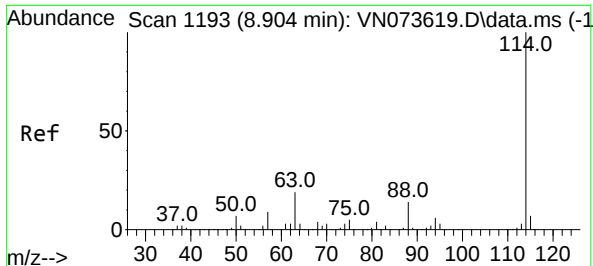

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VN073729.D

Acq: 04 Aug 2022 12:03

Instrument :

MSVOA_N

ClientSampleId :

VN0804WBL01





Tgt Ion:114 Resp: 604275

Ion Ratio Lower Upper

114 100

63 20.3 0.0 40.0

88 14.7 0.0 32.6

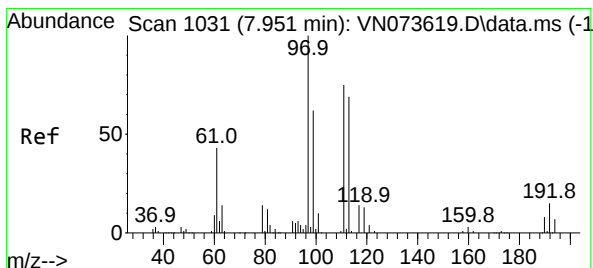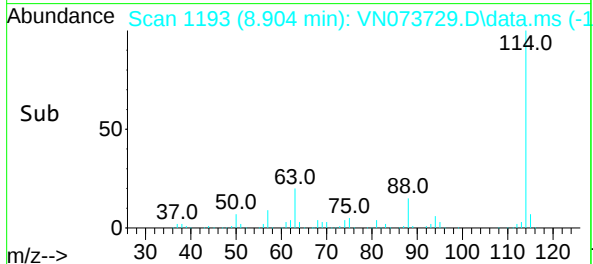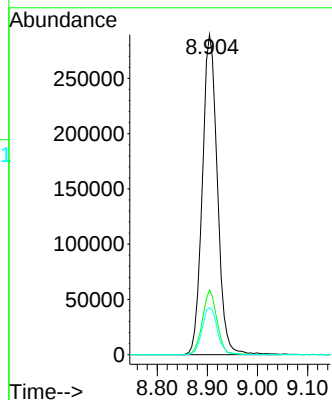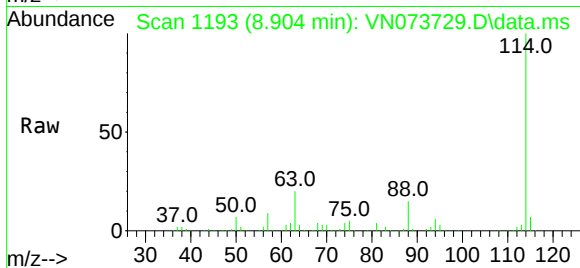

#35

Dibromofluoromethane

Concen: 54.301 ug/l

RT: 7.957 min Scan# 1032

Delta R.T. 0.006 min

Lab File: VN073729.D

Acq: 04 Aug 2022 12:03




Tgt Ion:113 Resp: 206045


Ion Ratio Lower Upper

113 100

111 104.1 81.4 122.0

192 20.7 17.0 25.6


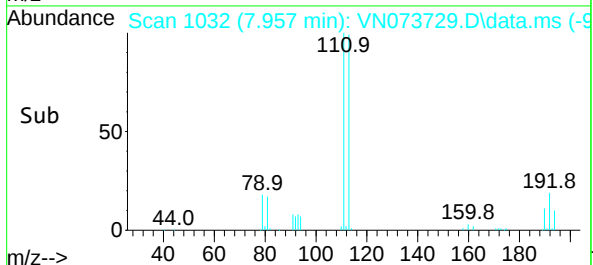
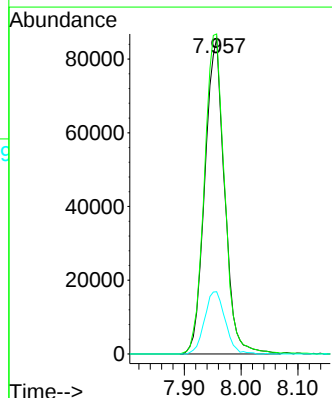
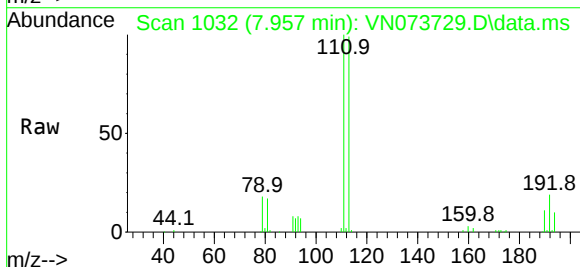


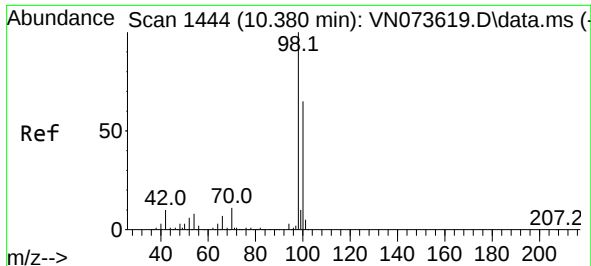

#50
Toluene-d8
Concen: 45.531 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. -0.000 min
Lab File: VN073729.D
Acq: 04 Aug 2022 12:03




Instrument :
MSVOA_N
ClientSampleId :
VN0804WBL01


Tgt Ion: 98 Resp: 679859
Ion Ratio Lower Upper
98 100
100 64.0 52.6 78.8

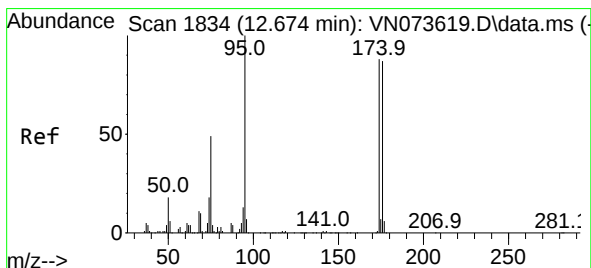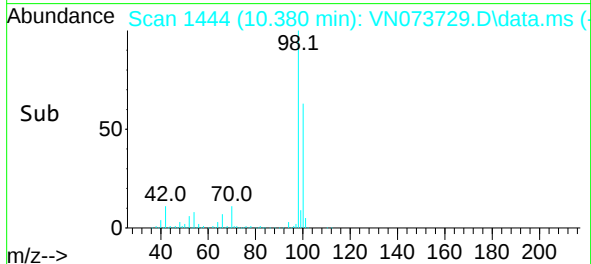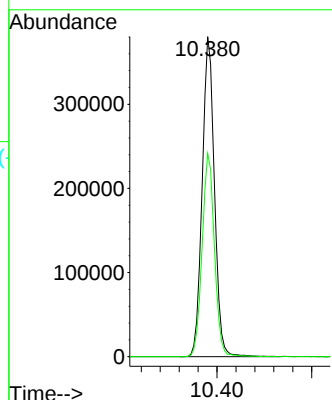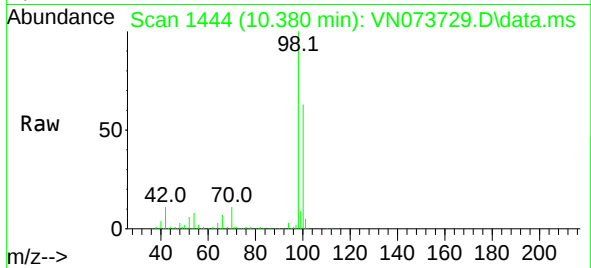

#62
4-Bromofluorobenzene
Concen: 49.598 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN073729.D
Acq: 04 Aug 2022 12:03

Tgt Ion: 95 Resp: 247042
Ion Ratio Lower Upper
95 100
174 91.4 0.0 167.6
176 87.3 0.0 163.4


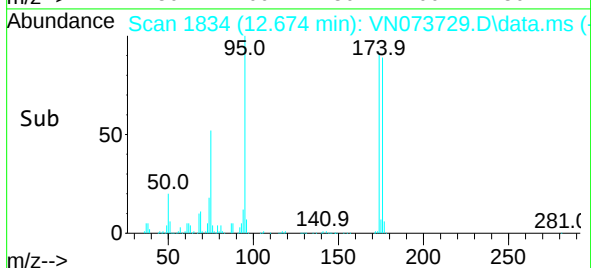
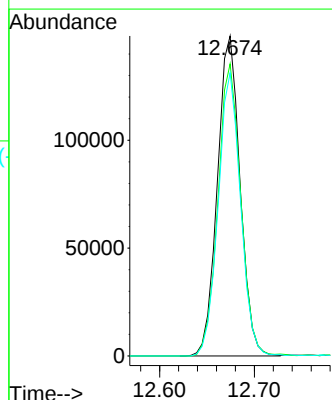
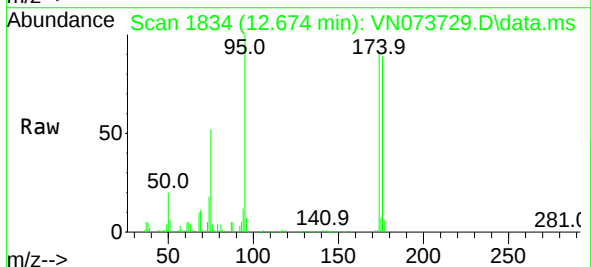


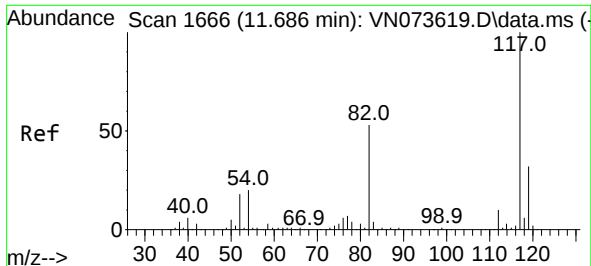

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN073729.D
Acq: 04 Aug 2022 12:03

Instrument :
MSVOA_N
ClientSampleId :
VN0804WBL01

Tgt Ion:117 Resp: 569349
Ion Ratio Lower Upper
117 100
82 53.3 44.2 66.2
119 33.3 25.4 38.0

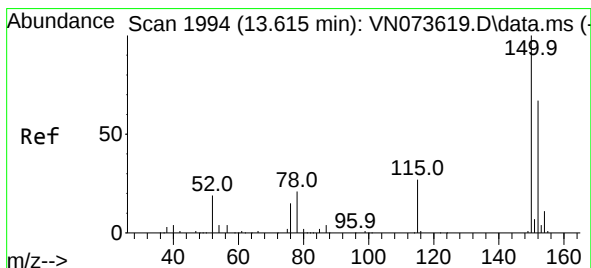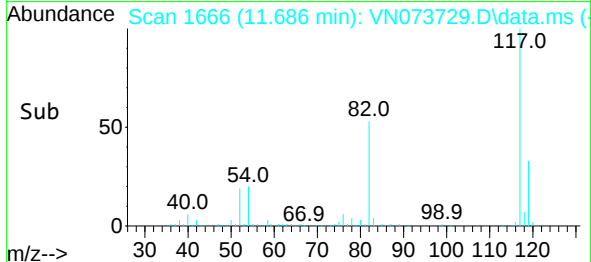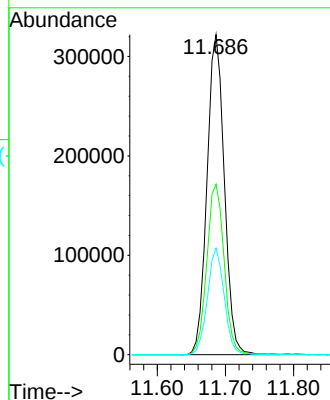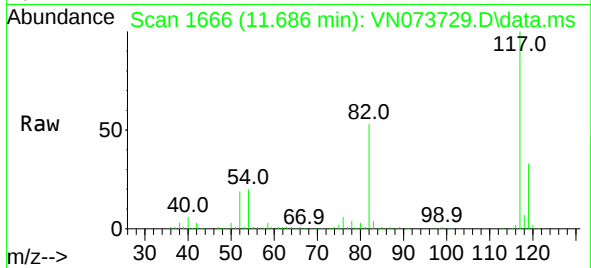

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. -0.000 min
Lab File: VN073729.D
Acq: 04 Aug 2022 12:03

Tgt Ion:152 Resp: 266911
Ion Ratio Lower Upper
152 100
115 56.6 28.9 86.7
150 157.9 0.0 356.2

