
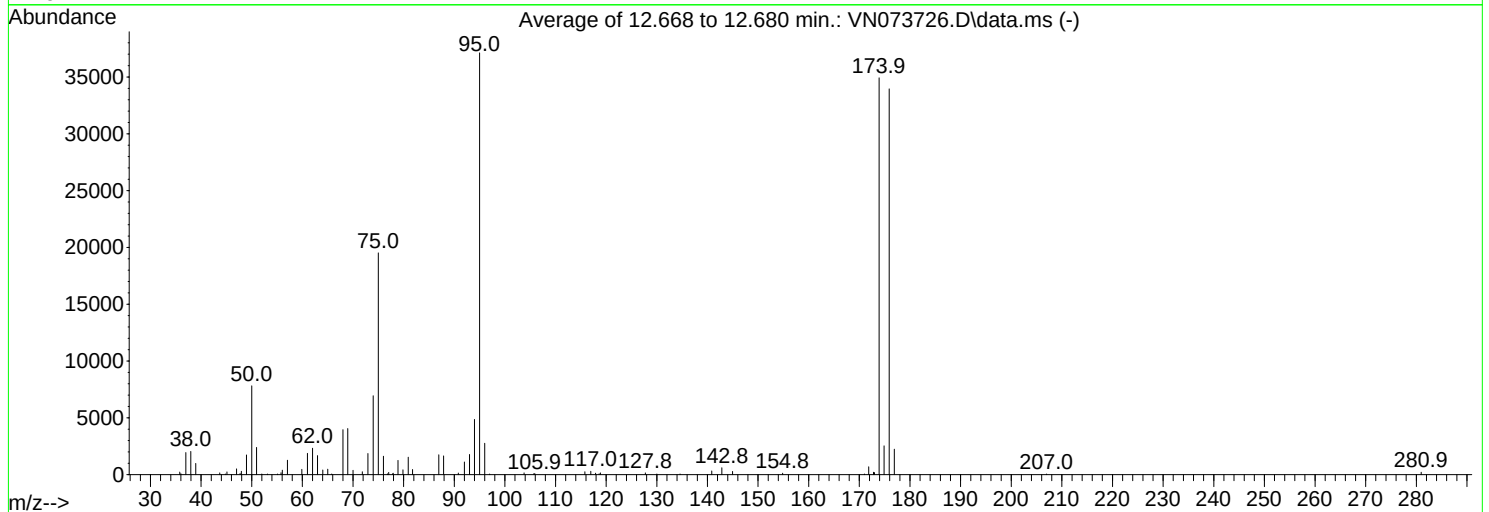


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080422\
Data File : VN073726.D
Acq On : 04 Aug 2022 09:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Title : SW846 8260
Last Update : Fri Jul 29 02:20:25 2022

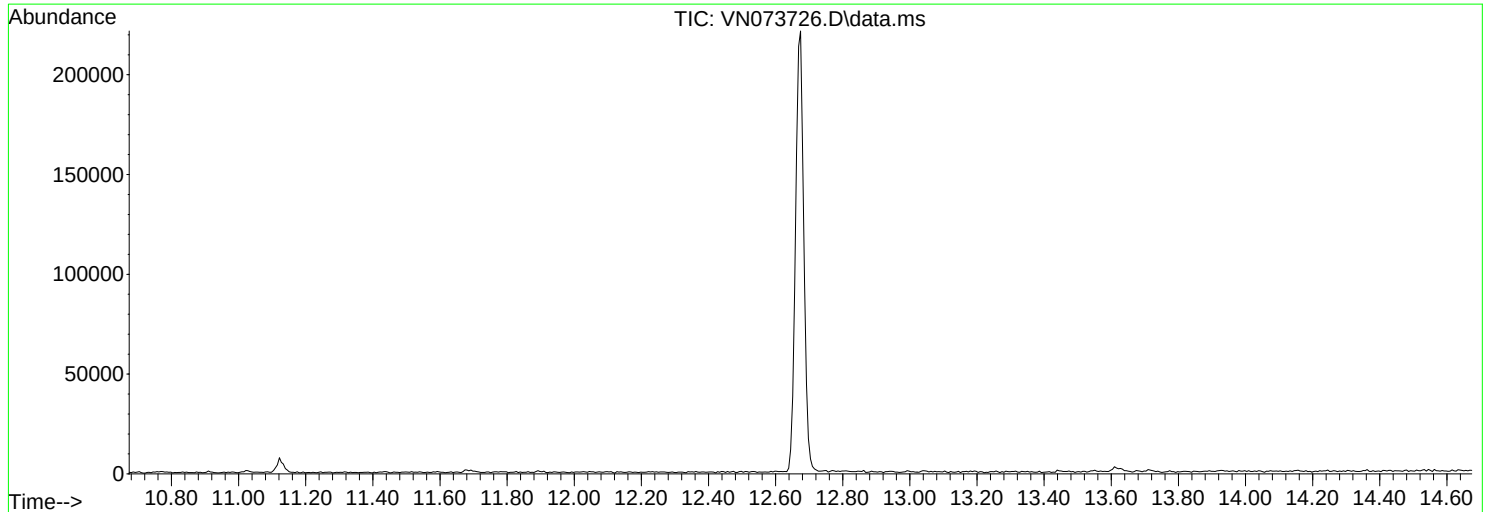

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	7814	PASS
75	95	30	60	52.6	19512	PASS
95	95	100	100	100.0	37123	PASS
96	95	5	9	7.5	2766	PASS
173	174	0.00	2	0.6	212	PASS
174	95	50	100	94.1	34923	PASS
175	174	5	9	7.3	2536	PASS
176	174	95	101	97.2	33947	PASS
177	176	5	9	6.6	2237	PASS