


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN080519\
Data File : VN057069.D
Acq On : 5 Aug 2019 8:53
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Title : SW846 8260
Last Update : Sat Jul 27 01:33:29 2019

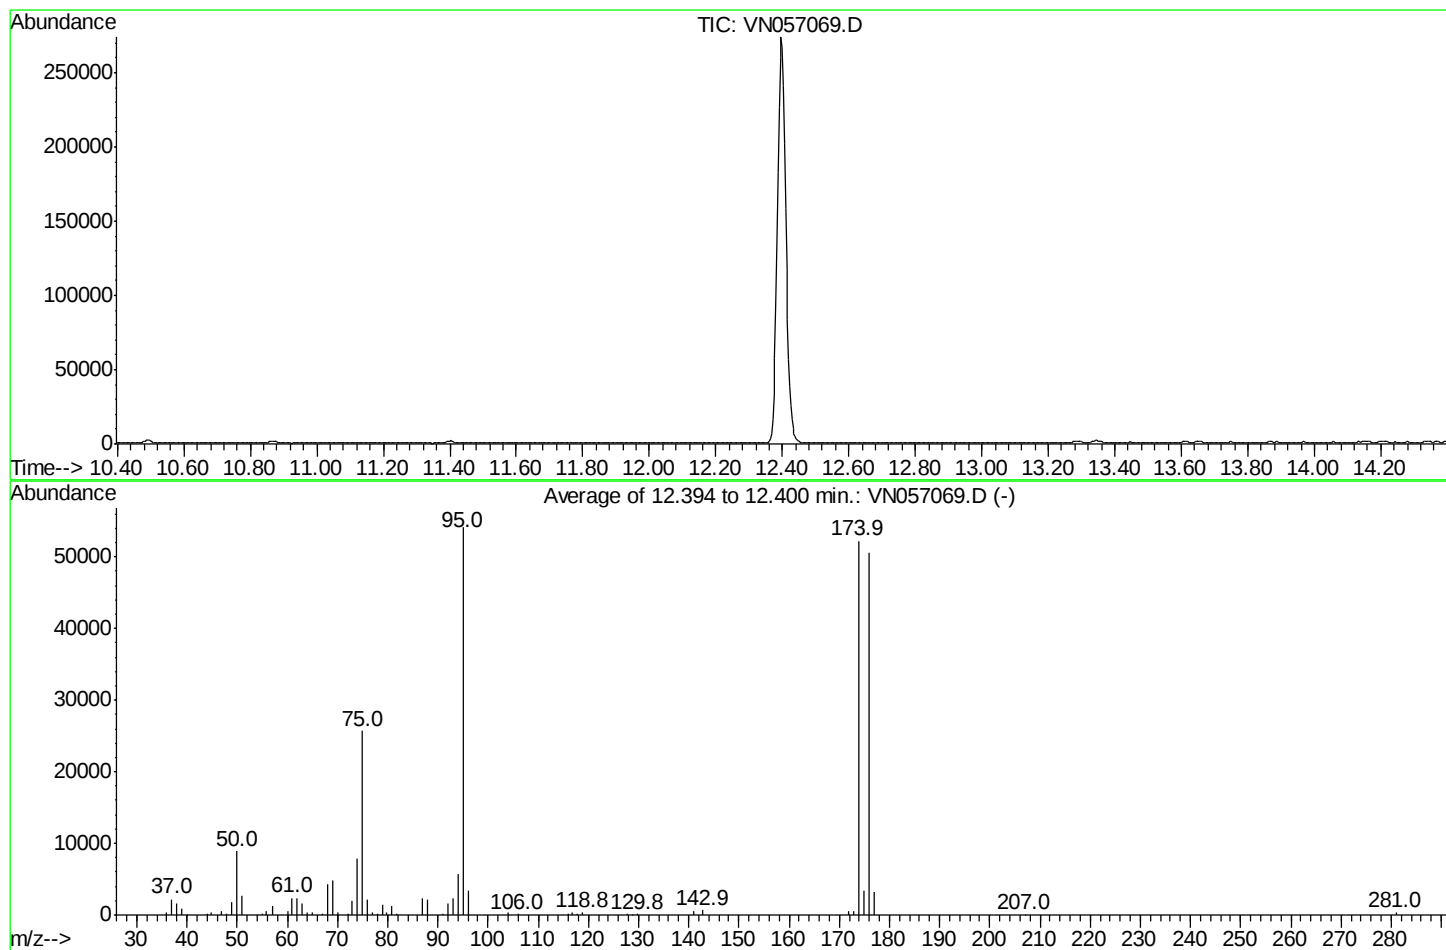

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	8900	PASS
75	95	30	60	47.5	25712	PASS
95	95	100	100	100.0	54122	PASS
96	95	5	9	6.3	3434	PASS
173	174	0.00	2	1.0	517	PASS
174	95	50	100	96.4	52184	PASS
175	174	5	9	6.4	3349	PASS
176	174	95	101	97.0	50605	PASS
177	176	5	9	6.4	3258	PASS