

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080521\
 Data File : VN068017.D
 Acq On : 5 Aug 2021 15:43
 Operator : JC/MD
 Sample : PB138172TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 06 01:23:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 29 15:02:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	306703	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.971	114	594110	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	620174	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	216196	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	236510	54.471	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 108.940%			
35) Dibromofluoromethane	8.024	113	180211	52.048	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 104.100%			
50) Toluene-d8	10.443	98	789602	49.460	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 98.920%			
62) 4-Bromofluorobenzene	12.734	95	261938	45.304	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 90.600%			
Target Compounds						
						Qvalue
11) Tert butyl alcohol	5.382	59	127	0.218	ug/l	# 71
13) Acrolein	4.039	56	197	0.499	ug/l	# 29
16) Acetone	4.296	43	37577	23.719	ug/l	94
18) Methyl Acetate	4.859	43	1835	0.380	ug/l	# 75
20) Methylene Chloride	5.090	84	14905	3.812	ug/l	91
23) Vinyl Acetate	6.308	43	184	8.818	ug/l	# 75
25) 2-Butanone	7.345	43	3429	1.492	ug/l	97
29) Tetrahydrofuran	7.691	42	944	0.641	ug/l	# 58
31) Cyclohexane	8.088	56	7632	1.192	ug/l	# 10
36) 1,1-Dichloropropene	8.086	75	26542	4.830	ug/l	# 46
38) Carbon Tetrachloride	8.088	117	32983	6.103	ug/l	# 17
43) Isopropyl Acetate	8.568	43	37288	4.327	ug/l	# 92
45) 1,2-Dichloropropane	9.628	63	2411	0.595	ug/l	# 44
48) Methyl methacrylate	9.550	41	7693	4.013	ug/l	# 12
49) 1,4-Dioxane	9.628	88	185	2.699	ug/l	# 1
51) 4-Methyl-2-Pentanone	10.336	43	8069	13.787	ug/l	# 85
53) t-1,3-Dichloropropene	10.717	75	58	2.841	ug/l	# 3
54) cis-1,3-Dichloropropene	10.247	75	56956	9.737	ug/l	# 62
56) Ethyl methacrylate	10.883	69	450	3.156	ug/l	# 1
57) 1,3-Dichloropropane	11.095	76	34100	5.102	ug/l	# 43
59) 2-Hexanone	11.095	43	502348	119.548	ug/l	# 54
60) Dibromochloromethane	11.486	129	49	3.311	ug/l	# 11
68) m/p-Xylenes	11.953	106	186	4.080	ug/l	# 47
70) Styrene	12.302	104	151	2.640	ug/l	# 22
71) Bromoform	12.717	173	325	4.106	ug/l	# 1
74) N-amyl acetate	12.200	43	15563	2.538	ug/l	# 58
76) 1,2,3-Trichloropropane	12.734	75	143331	33.011	ug/l	# 100
81) trans-1,4-Dichloro-2-b...	12.734	75	143331	88.596	ug/l	# 6
93) 1,2,4-Trichlorobenzene	15.271	180	163	2.516	ug/l	# 12
95) Naphthalene	15.509	128	2645	3.395	ug/l	# 75
96) 1,2,3-Trichlorobenzene	15.700	180	381	2.489	ug/l	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080521\
Data File : VN068017.D
Acq On : 5 Aug 2021 15:43
Operator : JC/MD
Sample : PB138172TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Aug 06 01:23:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 29 15:02:35 2021
Response via : Initial Calibration




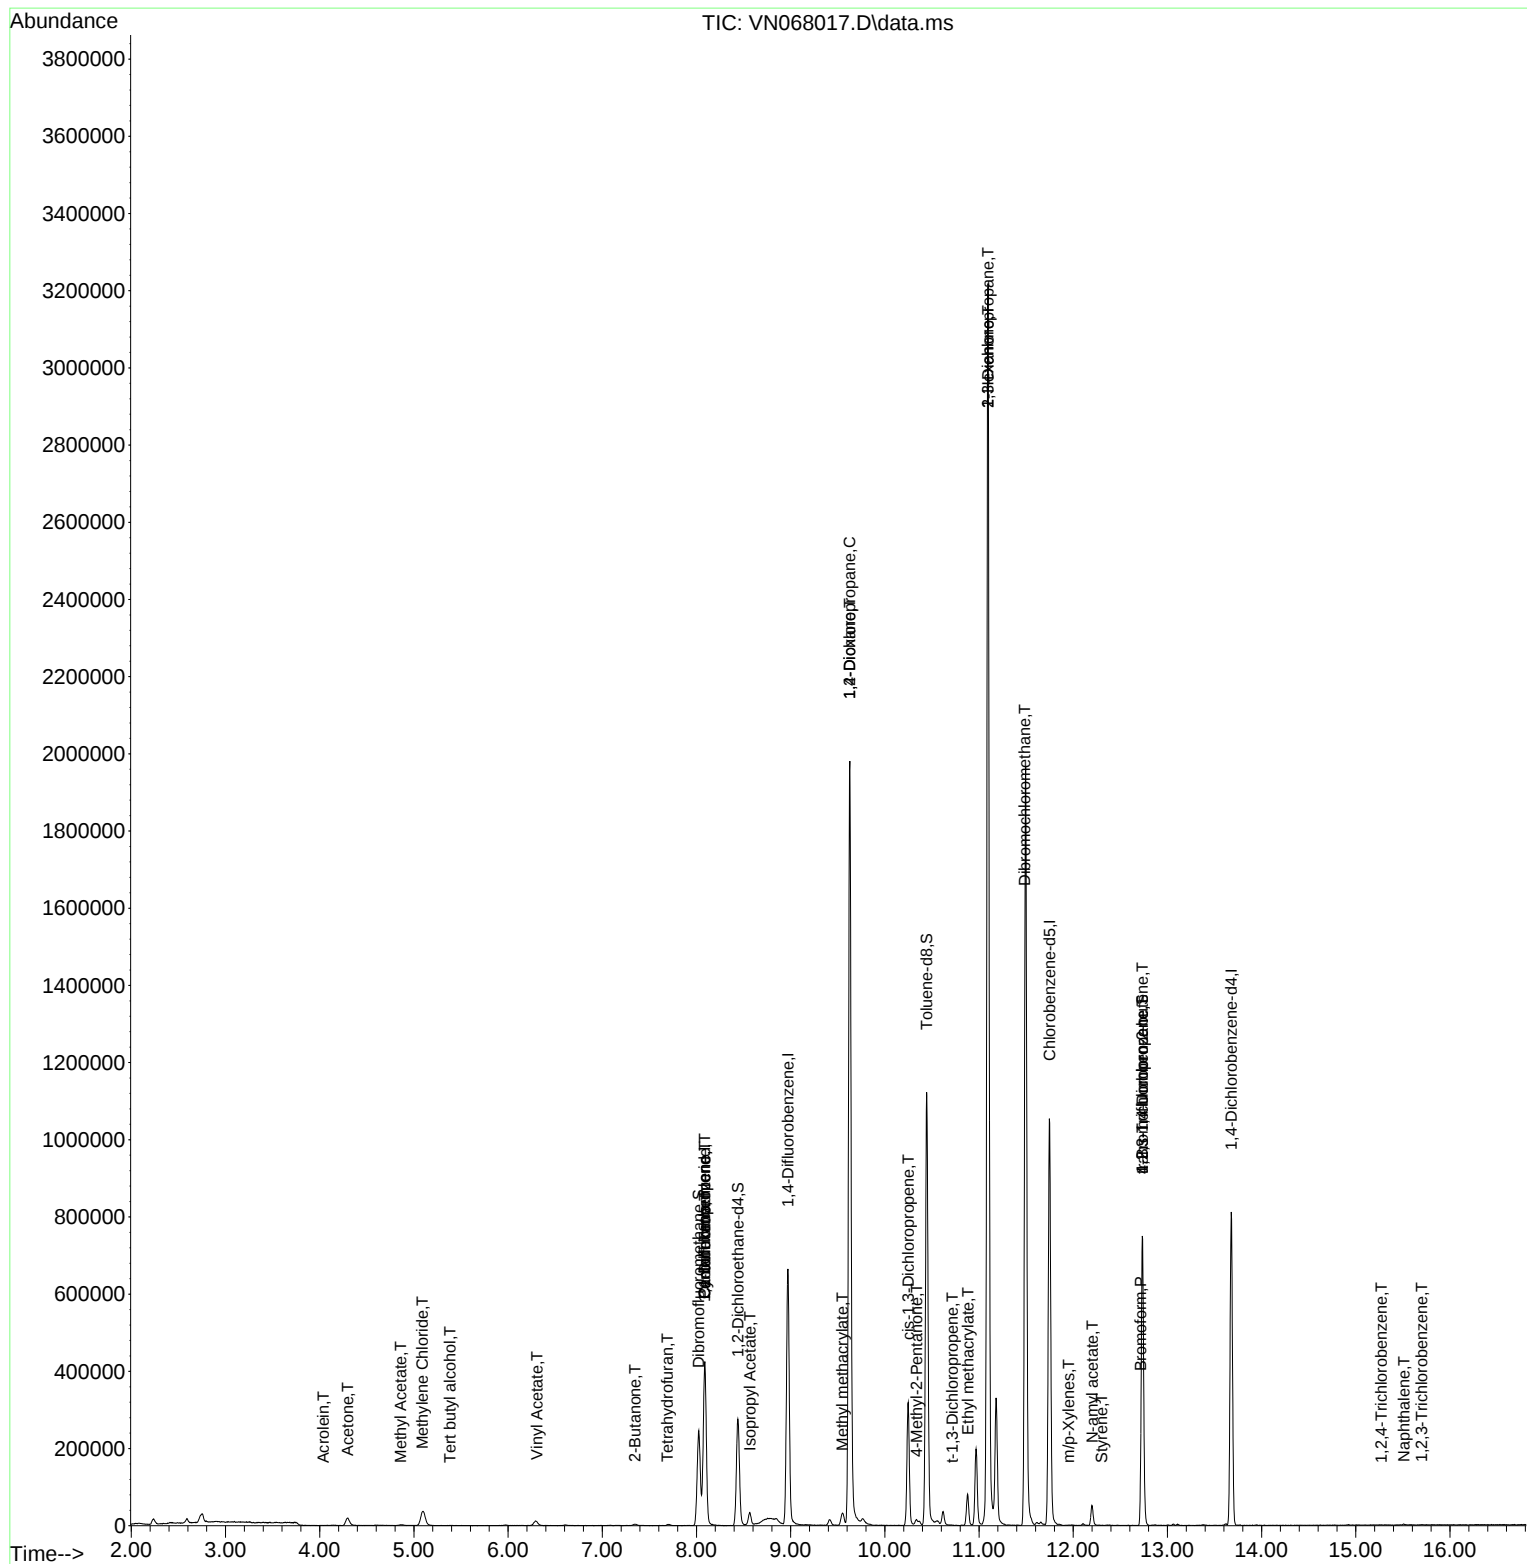




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 306703
Ion Ratio Lower Upper
168 100
99 61.2 62.9 94.3#

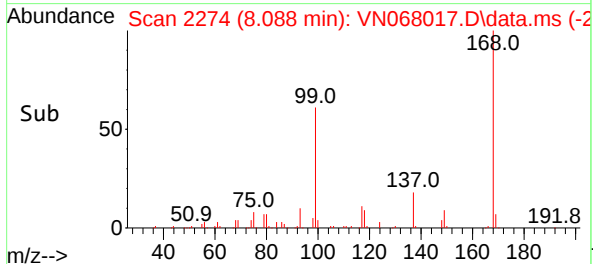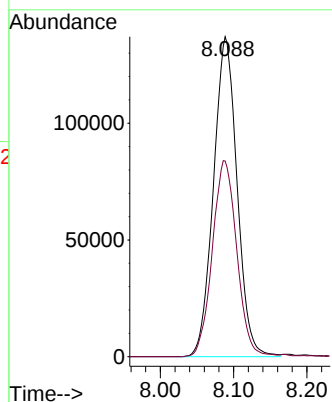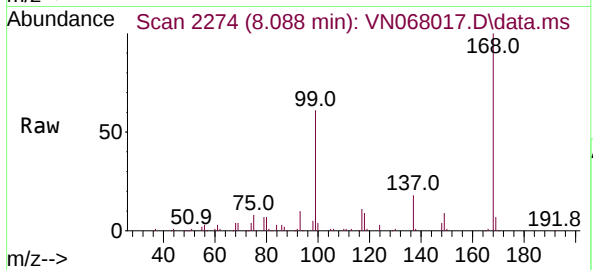

#11
Tert butyl alcohol
Concen: 0.218 ug/l
RT: 5.382 min Scan# 1265
Delta R.T. -0.008 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

Tgt Ion: 59 Resp: 127
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


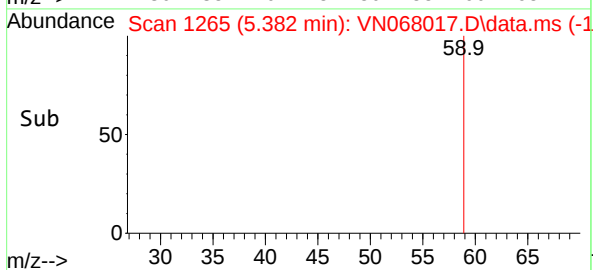
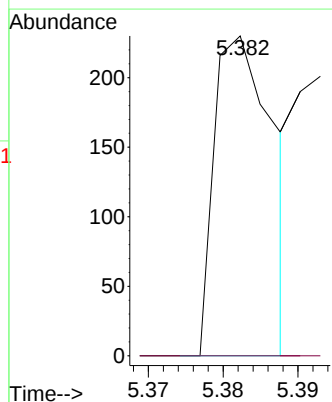
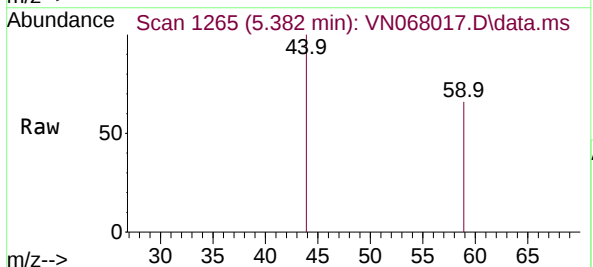




#13
Acrolein
Concen: 0.499 ug/l
RT: 4.039 min Scan# 764
Delta R.T. -0.002 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 197
Ion Ratio Lower Upper
56 100
55 12.7 57.4 86.0#

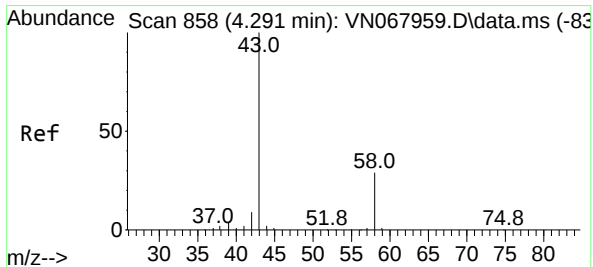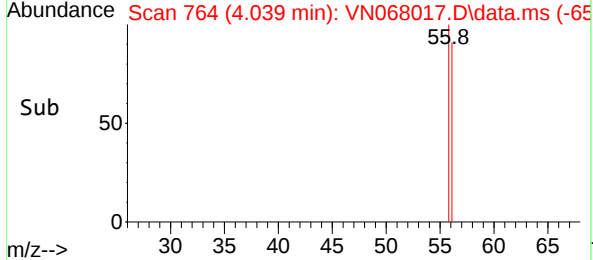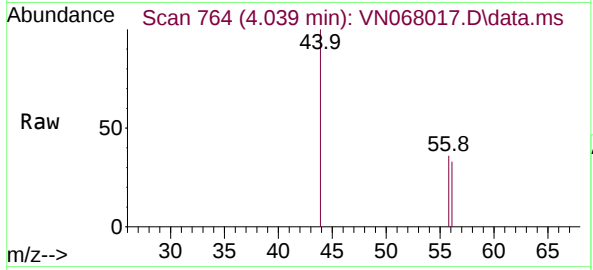

#16
Acetone
Concen: 23.719 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.005 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

Tgt Ion: 43 Resp: 37577
Ion Ratio Lower Upper
43 100
58 29.6 21.2 31.8


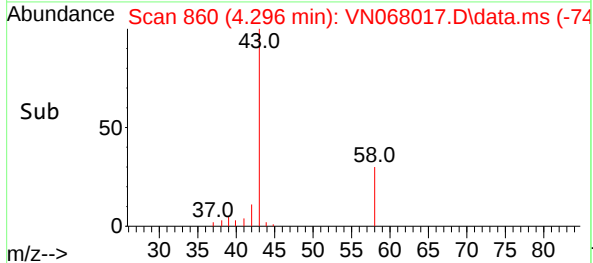
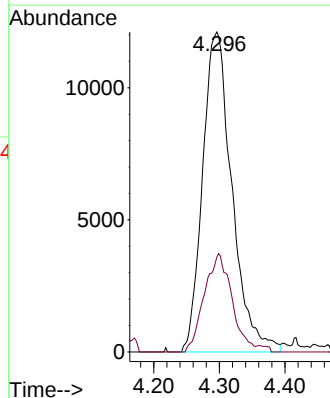
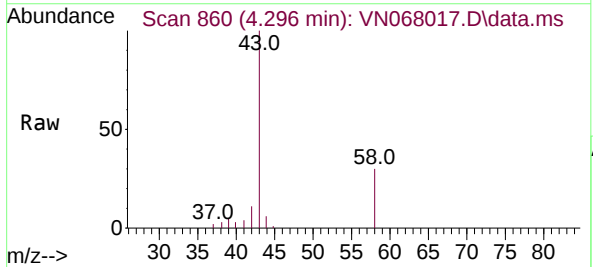




#18
Methyl Acetate
Concen: 0.380 ug/l
RT: 4.859 min Scan# 1070
Delta R.T. 0.002 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 1835
Ion Ratio Lower Upper
43 100
74 10.0 17.4 26.0#

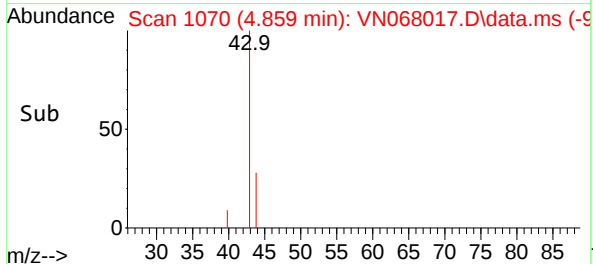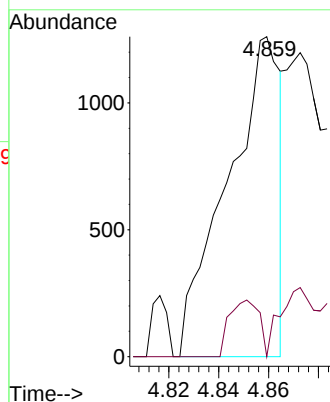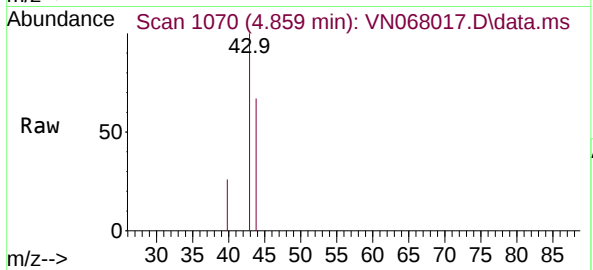

#20
Methylene Chloride
Concen: 3.812 ug/l
RT: 5.090 min Scan# 1156
Delta R.T. -0.003 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

Tgt Ion: 84 Resp: 14905
Ion Ratio Lower Upper
84 100
49 124.4 110.9 166.3
51 35.4 32.6 49.0
86 63.2 51.6 77.4


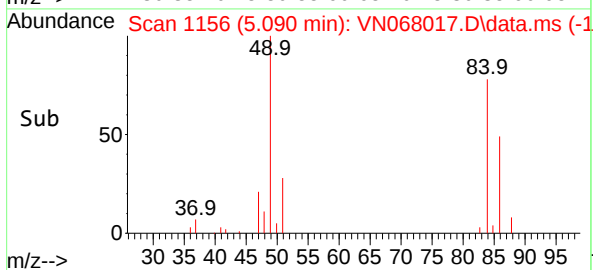

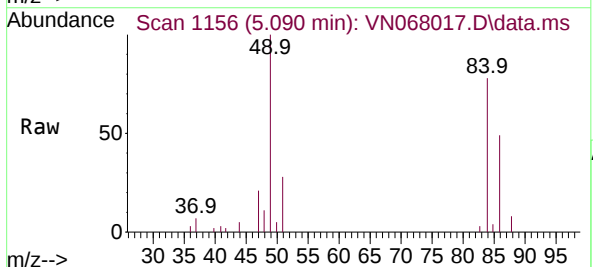


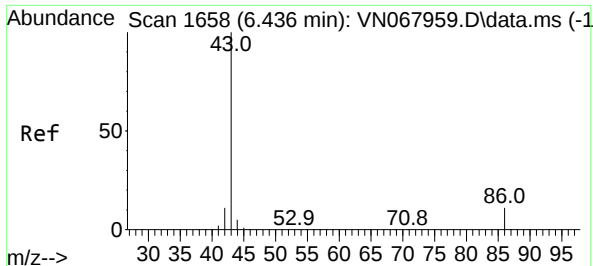

#23
 Vinyl Acetate
 Concen: 8.818 ug/l
 RT: 6.308 min Scan# 1610
 Delta R.T. -0.128 min
 Lab File: VN068017.D
 Acq: 5 Aug 2021 15:43




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 43 Resp: 184
 Ion Ratio Lower Upper
 43 100
 86 0.0 7.3 10.9#

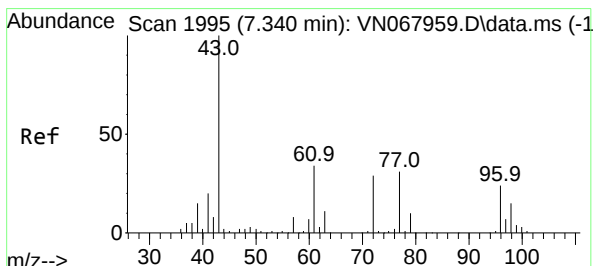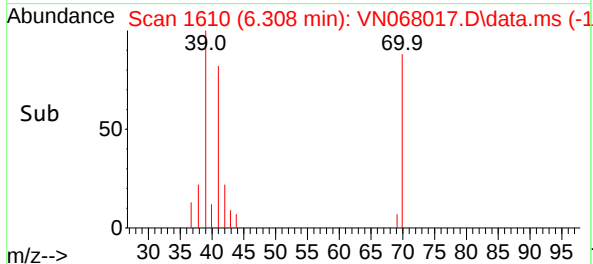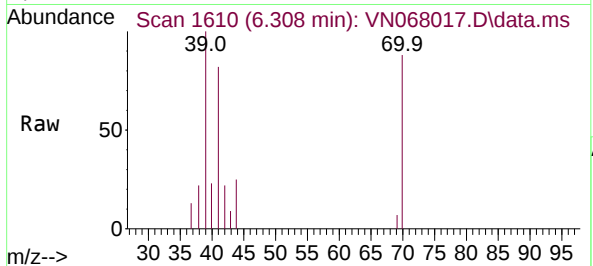

#25
 2-Butanone
 Concen: 1.492 ug/l
 RT: 7.345 min Scan# 1997
 Delta R.T. 0.005 min
 Lab File: VN068017.D
 Acq: 5 Aug 2021 15:43

Tgt Ion: 43 Resp: 3429
 Ion Ratio Lower Upper
 43 100
 72 23.2 19.7 29.5

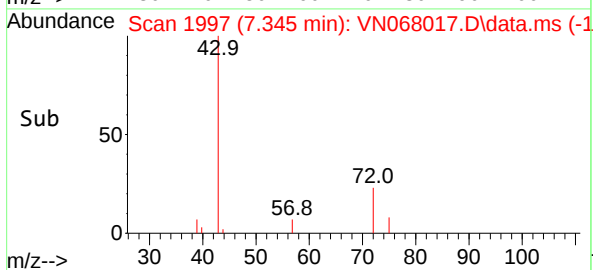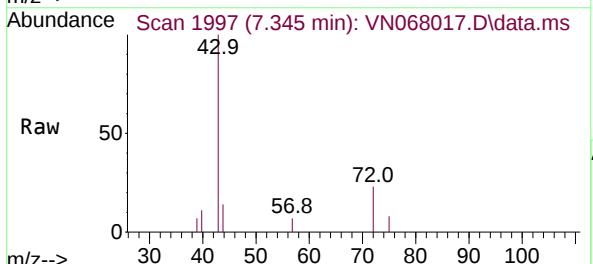

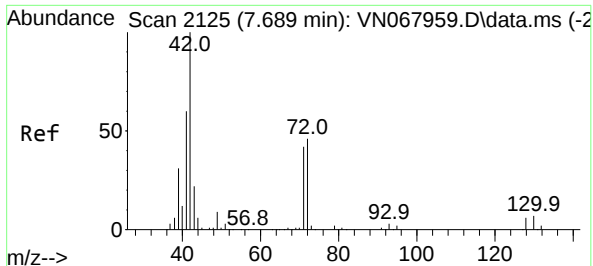

#29

Tetrahydrofuran

Concen: 0.641 ug/l

RT: 7.691 min Scan# 2126





Delta R.T. 0.002 min

Lab File: VN068017.D

Acq: 5 Aug 2021 15:43

Tgt Ion: 42 Resp: 944

Ion	Ratio	Lower	Upper
42	100		
72	48.2	32.8	49.2
71	83.7	31.2	46.8#

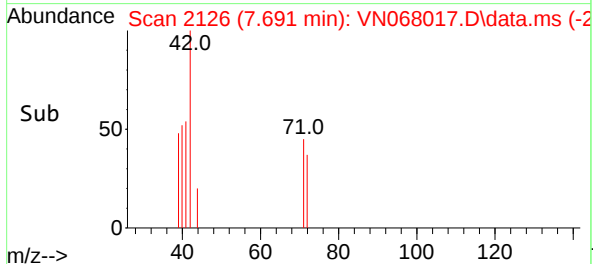

#31

Cyclohexane

Concen: 1.192 ug/l

RT: 8.088 min Scan# 2274




Delta R.T. -0.008 min

Lab File: VN068017.D


Acq: 5 Aug 2021 15:43

Tgt Ion: 56 Resp: 7632

Ion	Ratio	Lower	Upper
56	100		
69	155.3	27.3	40.9#
84	116.2	64.9	97.3#

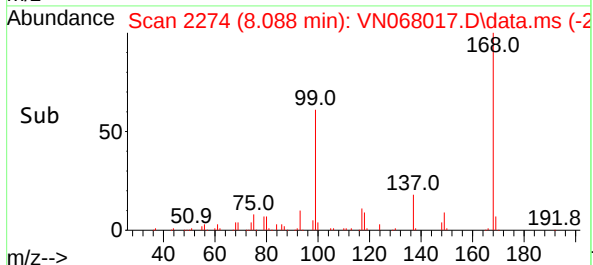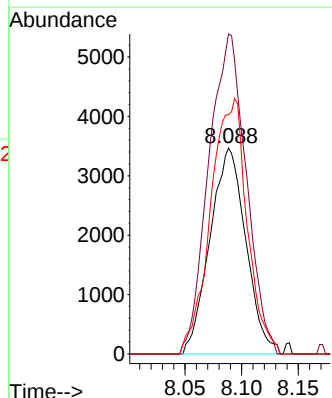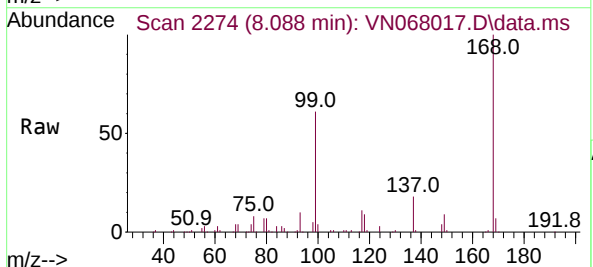





Instrument :
MSVOA_N
ClientSampled :



#33
 1,2-Dichloroethane-d4
 Concen: 54.471 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. 0.003 min
 Lab File: VN068017.D
 Acq: 5 Aug 2021 15:43




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 65 Resp: 236510
 Ion Ratio Lower Upper
 65 100
 67 49.9 0.0 98.6

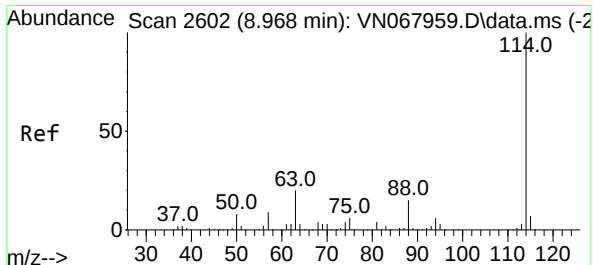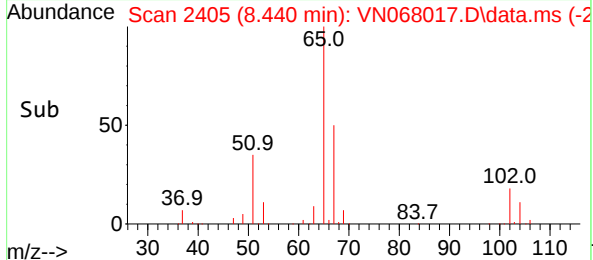

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.971 min Scan# 2603
 Delta R.T. 0.003 min
 Lab File: VN068017.D
 Acq: 5 Aug 2021 15:43

Tgt Ion: 114 Resp: 594110
 Ion Ratio Lower Upper
 114 100
 63 20.5 0.0 49.0
 88 14.7 0.0 36.6


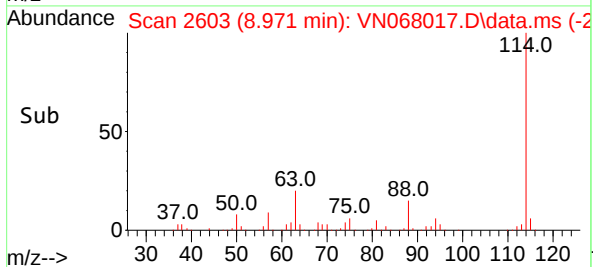

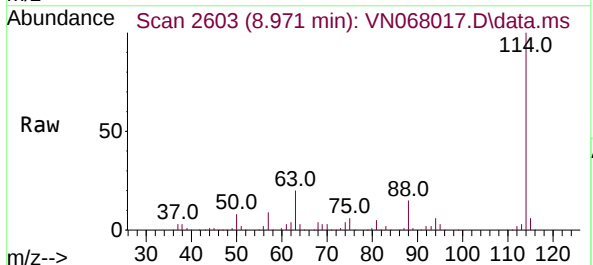




#35
Dibromofluoromethane
Concen: 52.048 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 180211
Ion Ratio Lower Upper
113 100
111 102.1 83.8 125.8
192 15.8 13.4 20.0

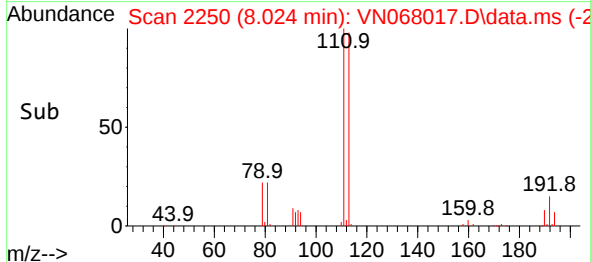

#36
1,1-Dichloropropene
Concen: 4.830 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.136 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43


Tgt Ion: 75 Resp: 26542
Ion Ratio Lower Upper
75 100
110 2.9 15.7 47.0#
77 0.0 24.6 37.0#

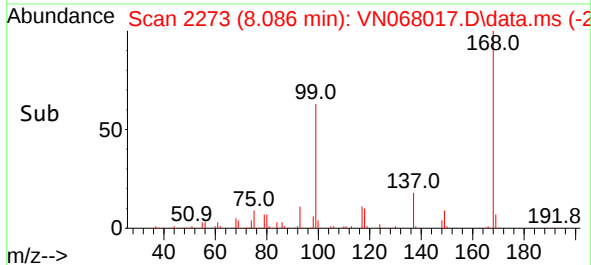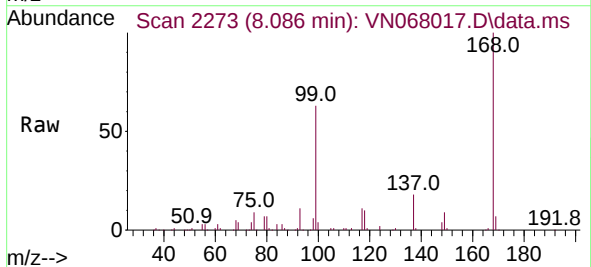






#38
Carbon Tetrachloride
Concen: 6.103 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.116 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:117 Resp: 32983
Ion Ratio Lower Upper
117 100
119 5.6 75.4 113.2#
121 0.0 23.5 35.3#

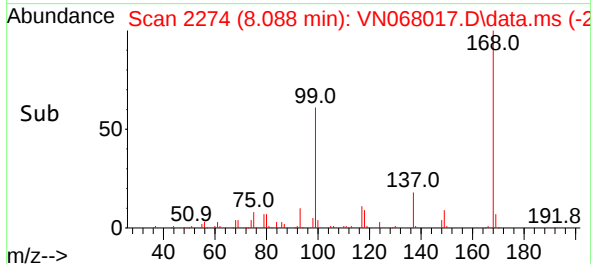


#43
Isopropyl Acetate
Concen: 4.327 ug/l
RT: 8.568 min Scan# 2453
Delta R.T. 0.005 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

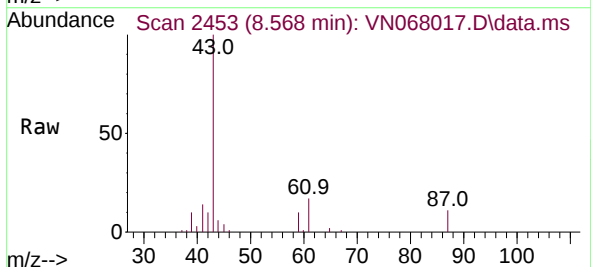

Tgt Ion: 43 Resp: 37288
Ion Ratio Lower Upper
43 100
61 17.6 19.0 28.4#
87 12.0 9.5 14.3

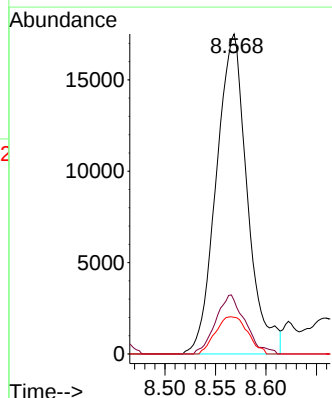




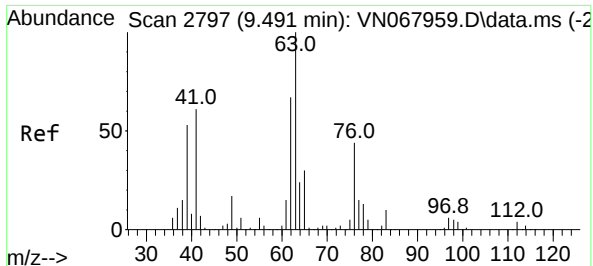


#45

1,2-Dichloropropane
Concen: 0.595 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.137 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 63 Resp: 2411
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#

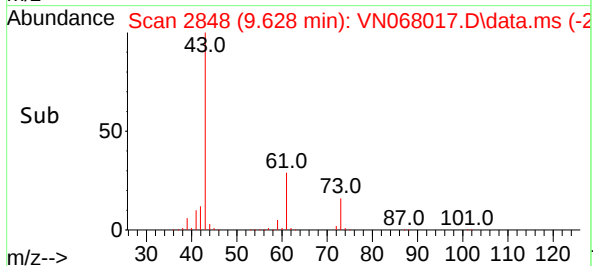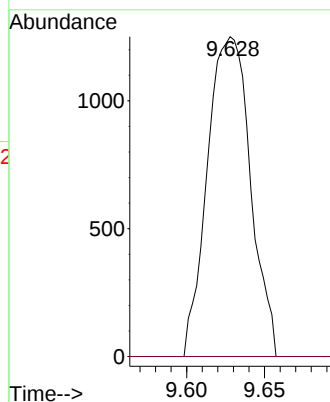


#48

Methyl methacrylate
Concen: 4.013 ug/l
RT: 9.550 min Scan# 2819
Delta R.T. -0.013 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

Tgt Ion: 41 Resp: 7693
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

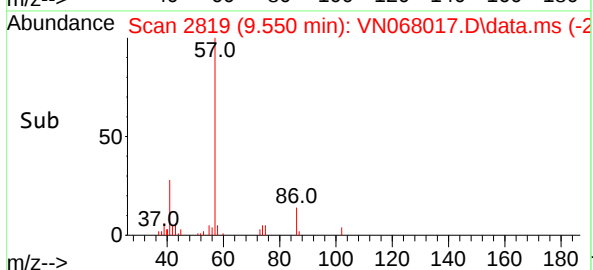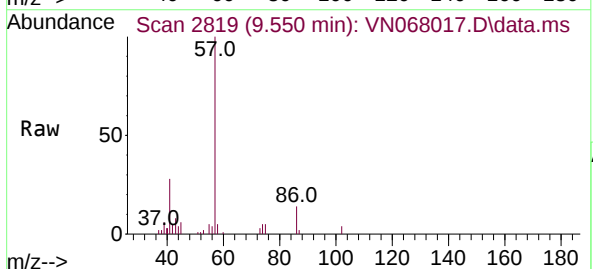

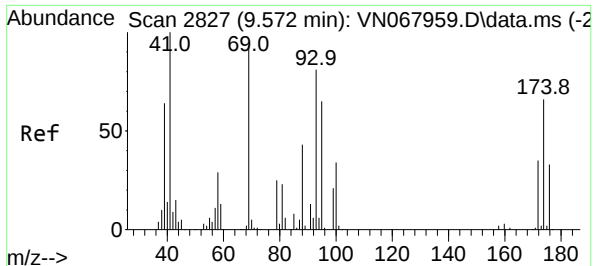

#49

1,4-Dioxane

Concen: 2.699 ug/l

RT: 9.628 min Scan# 2848

Delta R.T. 0.056 min

Lab File: VN068017.D

Acq: 5 Aug 2021 15:43

Tgt Ion: 88 Resp: 185

Ion Ratio Lower Upper

88 100





43 1070896.2 28.8 43.2#

58 5247.6 60.4 90.6#

Instrument :

MSVOA_N

ClientSampled :

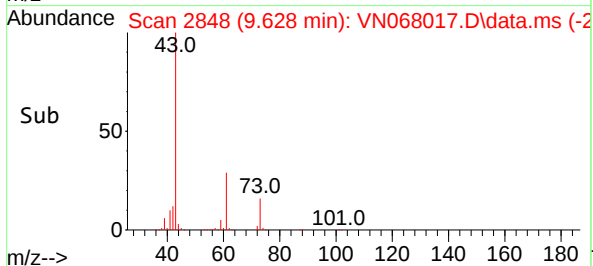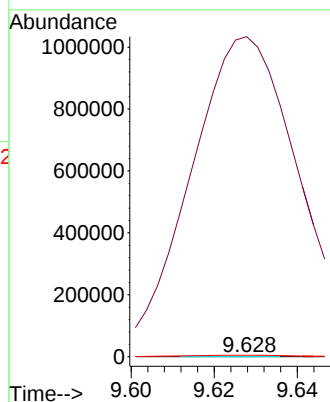

#50

Toluene-d8

Concen: 49.460 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. 0.000 min

Lab File: VN068017.D




Acq: 5 Aug 2021 15:43


Tgt Ion: 98 Resp: 789602

Ion Ratio Lower Upper

98 100

100 63.1 51.7 77.5


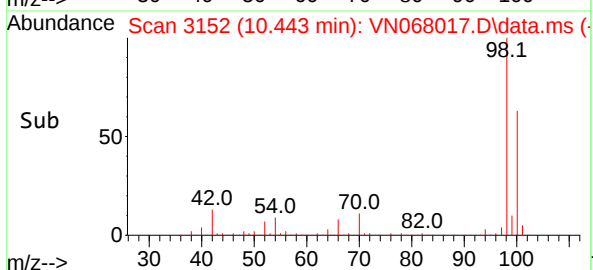

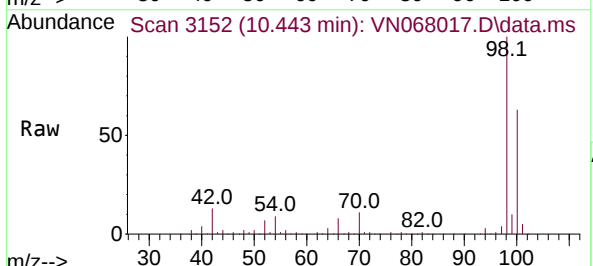




#51
4-Methyl-2-Pentanone
Concen: 13.787 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 8069
Ion Ratio Lower Upper
43 100
58 44.5 28.6 43.0#

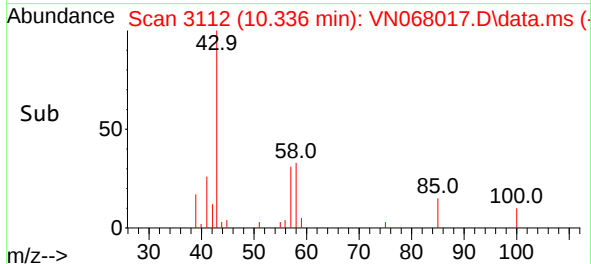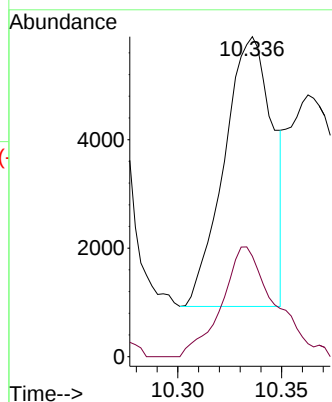

#53
t-1,3-Dichloropropene
Concen: 2.841 ug/l
RT: 10.717 min Scan# 3254
Delta R.T. -0.005 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

Tgt Ion: 75 Resp: 58
Ion Ratio Lower Upper
75 100
77 85.1 25.1 37.7#


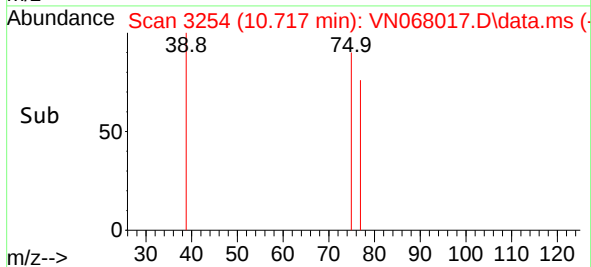
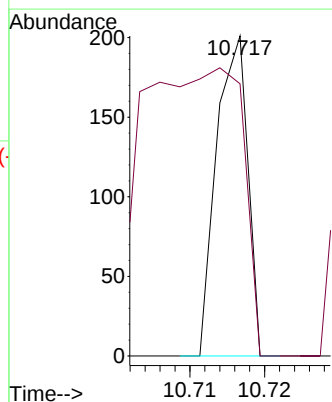
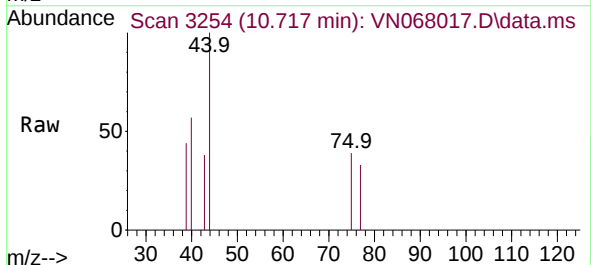


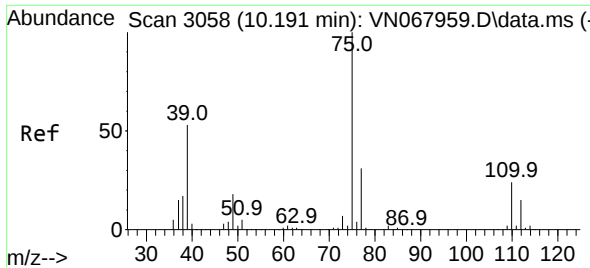

#54
 cis-1,3-Dichloropropene
 Concen: 9.737 ug/l
 RT: 10.247 min Scan# 3079
 Delta R.T. 0.056 min
 Lab File: VN068017.D
 Acq: 5 Aug 2021 15:43




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 56956
 Ion Ratio Lower Upper
 75 100
 77 0.0 24.6 37.0#
 39 40.5 50.7 76.1#

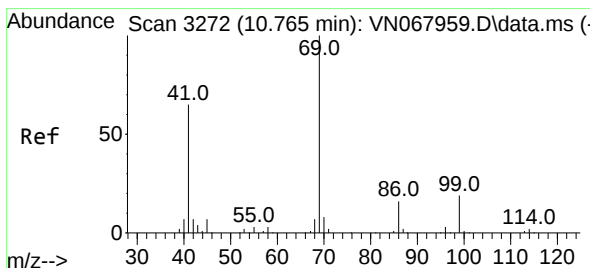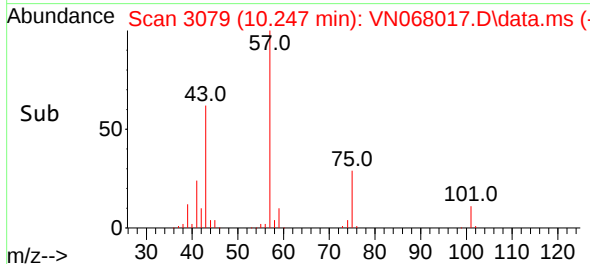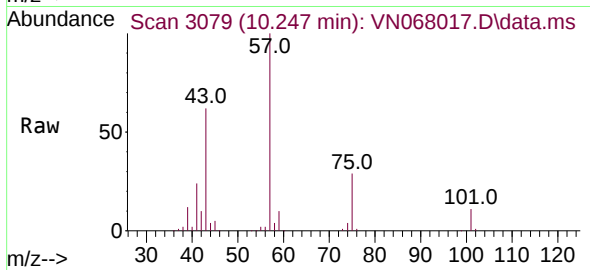

#56
 Ethyl methacrylate
 Concen: 3.156 ug/l
 RT: 10.883 min Scan# 3316
 Delta R.T. 0.118 min
 Lab File: VN068017.D
 Acq: 5 Aug 2021 15:43

Tgt Ion: 69 Resp: 450
 Ion Ratio Lower Upper
 69 100
 41 3917.1 58.6 88.0#
 39 1792.7 38.3 57.5#


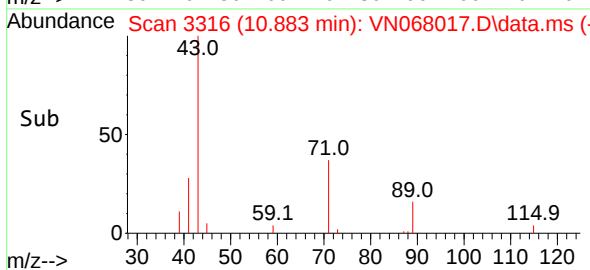

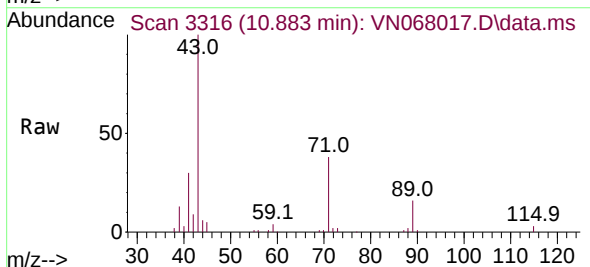




#57
1,3-Dichloropropane
Concen: 5.102 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 34100
Ion Ratio Lower Upper
76 100
78 0.3 25.7 38.5#

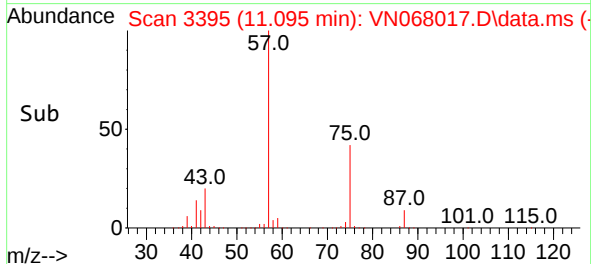

#59
2-Hexanone
Concen: 119.548 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

Tgt Ion: 43 Resp: 502348
Ion Ratio Lower Upper
43 100
58 18.0 24.7 74.1#


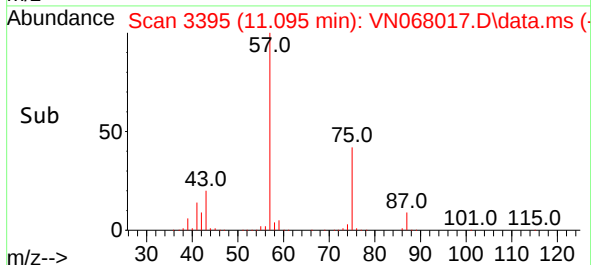

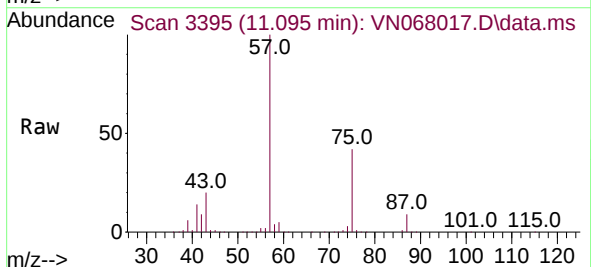




#60
Dibromochloromethane
Concen: 3.311 ug/l
RT: 11.486 min Scan# 3541
Delta R.T. 0.246 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:129 Resp: 49
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

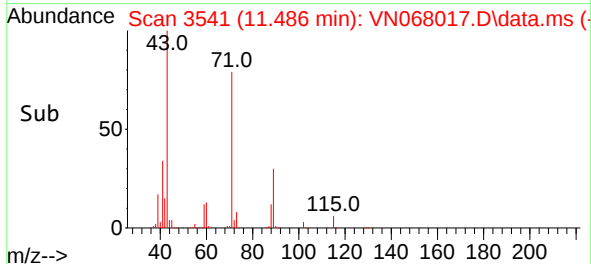

#62
4-Bromofluorobenzene
Concen: 45.304 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.000 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

Tgt Ion: 95 Resp: 261938
Ion Ratio Lower Upper
95 100
174 73.6 0.0 122.0
176 69.8 0.0 117.6


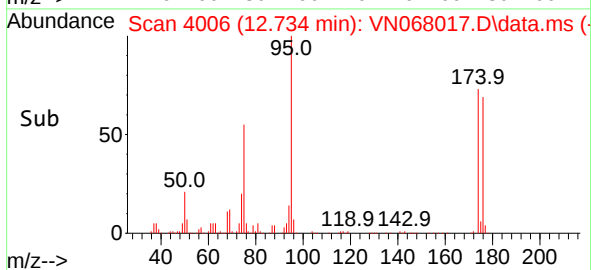

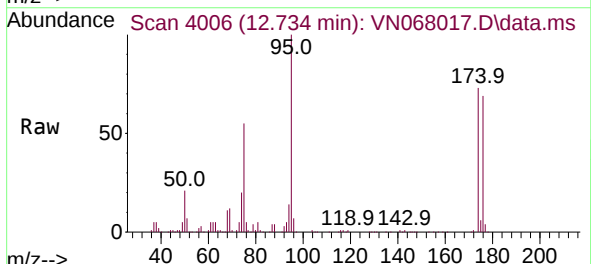




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.002 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 620174
Ion Ratio Lower Upper
117 100
82 54.8 53.1 79.7
119 32.2 25.5 38.3

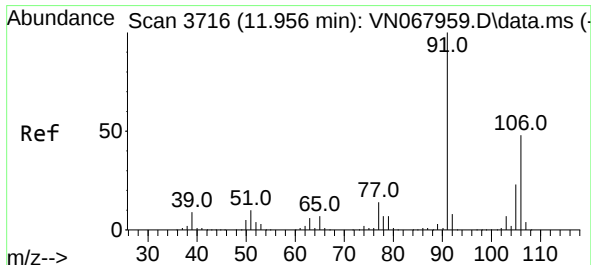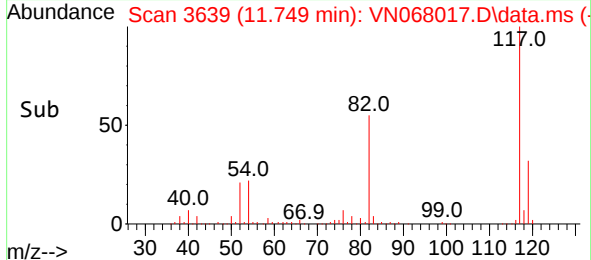

#68
m/p-Xylenes
Concen: 4.080 ug/l
RT: 11.953 min Scan# 3715
Delta R.T. -0.003 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43


Tgt Ion:106 Resp: 186
Ion Ratio Lower Upper
106 100
91 312.4 180.6 270.8#

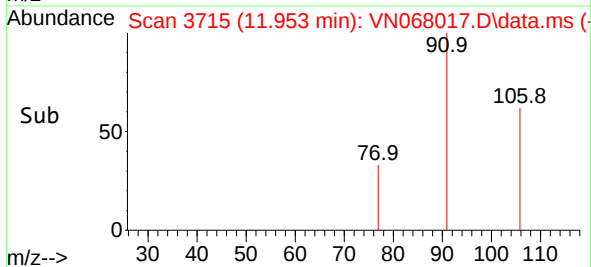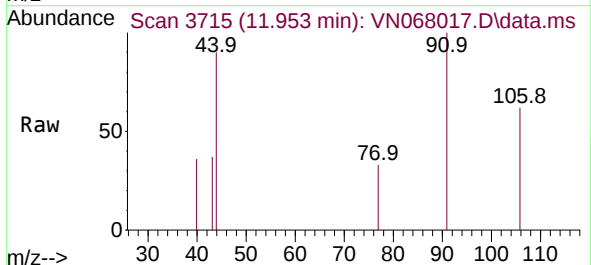



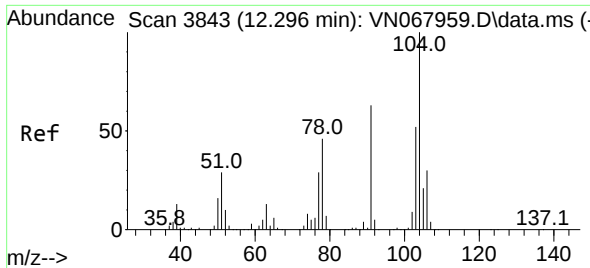


#70
Styrene
Concen: 2.640 ug/l
RT: 12.302 min Scan# 3845
Delta R.T. 0.006 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43


Instrument :
MSVOA_N
ClientSampled :

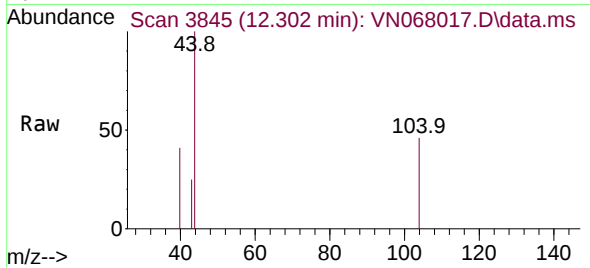



Tgt Ion:104 Resp: 151
Ion Ratio Lower Upper
104 100
78 0.0 48.2 72.2#
103 0.0 44.5 66.7#

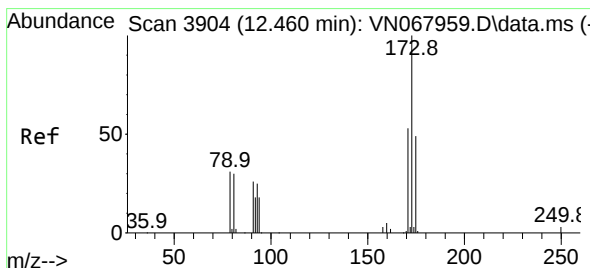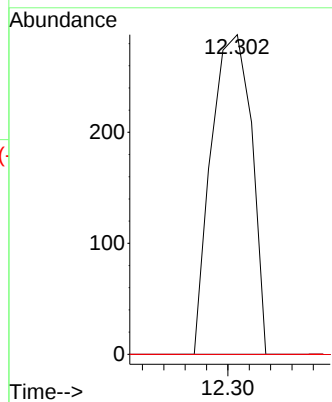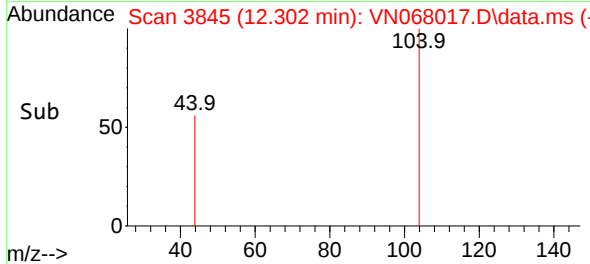


#71
Bromoform
Concen: 4.106 ug/l
RT: 12.717 min Scan# 4000
Delta R.T. 0.257 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

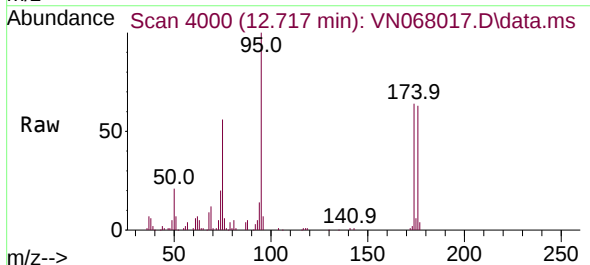

Tgt Ion:173 Resp: 325
Ion Ratio Lower Upper
173 100
175 4379.1 23.9 71.8#
254 0.0 0.0 0.0




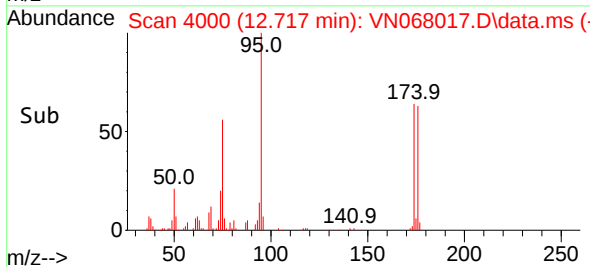




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:152 Resp: 216196
Ion Ratio Lower Upper
152 100
115 61.4 36.1 108.5
150 158.3 0.0 351.8

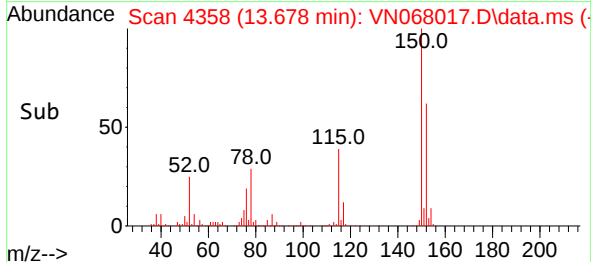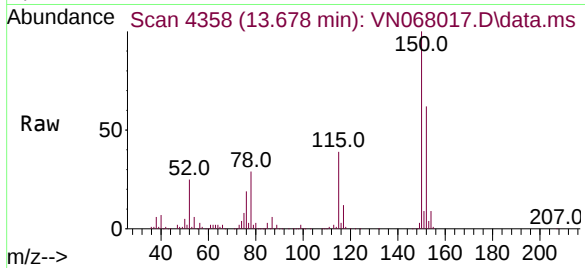

#74
N-ethyl acetate
Concen: 2.538 ug/l
RT: 12.200 min Scan# 3807
Delta R.T. -0.190 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

Tgt Ion: 43 Resp: 15563
Ion Ratio Lower Upper
43 100
70 2.1 29.4 44.2#
55 5.6 17.0 25.4#
61 10.9 17.6 26.4#


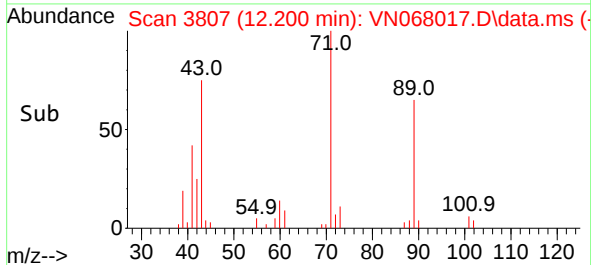
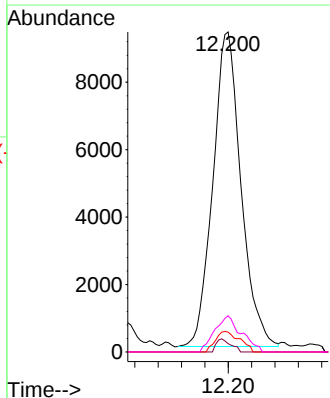
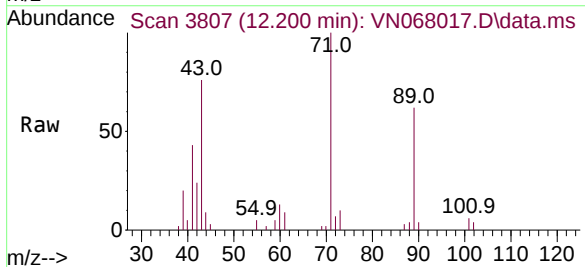




#76
1,2,3-Trichloropropane
Concen: 33.011 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.150 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 143331
Ion Ratio Lower Upper
75 100
77 1.1 0.0 0.0#

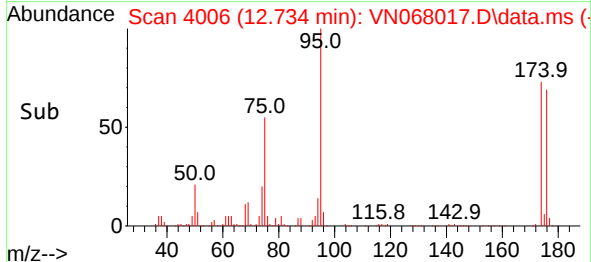

#81
trans-1,4-Dichloro-2-butene
Concen: 88.596 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43


Tgt Ion: 75 Resp: 143331
Ion Ratio Lower Upper
75 100
53 0.1 87.6 131.4#
89 0.0 37.8 56.8#

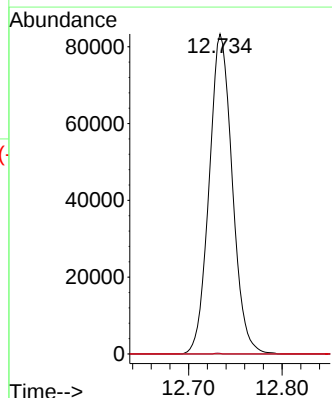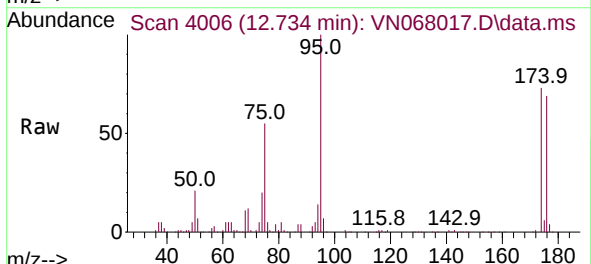






#93
1,2,4-Trichlorobenzene
Concen: 2.516 ug/l
RT: 15.271 min Scan# 4952
Delta R.T. 0.006 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:180 Resp: 163
Ion Ratio Lower Upper
180 100
182 0.0 47.5 142.5#
145 0.0 17.2 51.6#

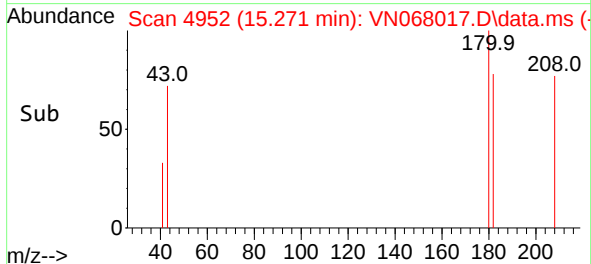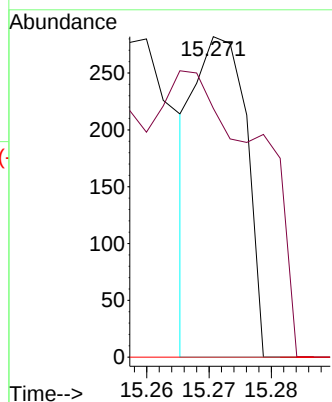


#95
Naphthalene
Concen: 3.395 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.000 min
Lab File: VN068017.D
Acq: 5 Aug 2021 15:43

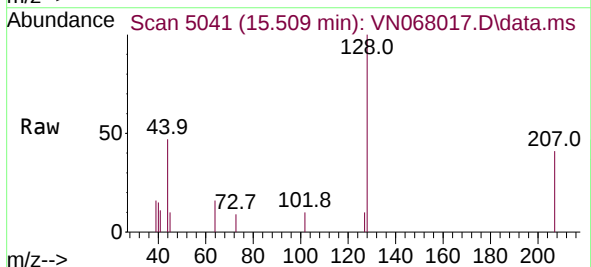


Tgt Ion:128 Resp: 2645
Ion Ratio Lower Upper
128 100
127 4.6 10.6 15.8#
129 0.0 8.6 12.8#

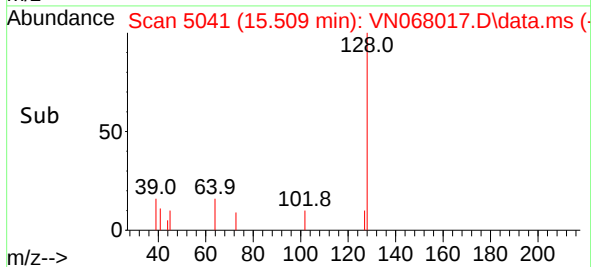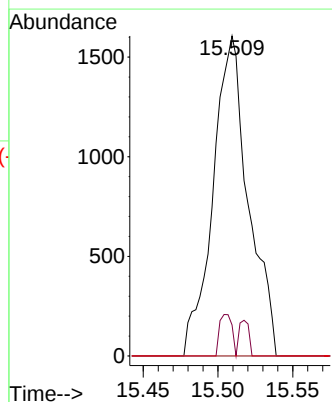



#96
 1,2,3-Trichlorobenzene
 Concen: 2.489 ug/l
 RT: 15.700 min Scan# 5112
 Delta R.T. -0.002 min
 Lab File: VN068017.D
 Acq: 5 Aug 2021 15:43

Instrument :
 MSVOA_N
 ClientSampleId :

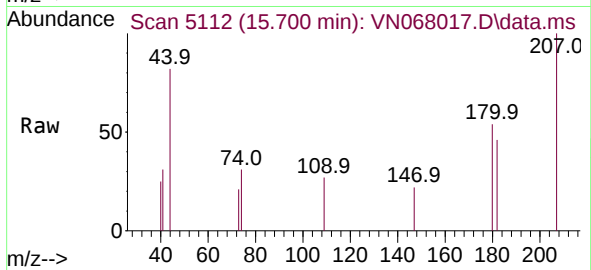

Tgt Ion:180 Resp: 381
 Ion Ratio Lower Upper
 180 100
 182 114.2 47.8 143.3
 145 0.0 18.2 54.6#

