

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080521\
 Data File : VN068022.D
 Acq On : 5 Aug 2021 17:45
 Operator : JC/MD
 Sample : M2940-09 .5PPB MDL
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 06 02:09:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 06 02:07:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	335017	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	665836	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	595834	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	201461	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	279177	58.864	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 117.720%			
35) Dibromofluoromethane	8.024	113	202746	52.249	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 104.500%			
50) Toluene-d8	10.443	98	792338	50.452	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 100.900%			
62) 4-Bromofluorobenzene	12.733	95	243006	44.669	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 89.340%			
Target Compounds					Qvalue	
3) Chloromethane	2.301	50	1408	0.330	ug/l #	57
5) Bromomethane	2.842	94	2486	0.419	ug/l #	72
6) Chloroethane	3.006	64	1203	0.233	ug/l #	56
11) Tert butyl alcohol	5.398	59	141	0.222	ug/l #	71
13) Acrolein	4.033	56	742	1.721	ug/l #	51
15) Acrylonitrile	5.559	53	398	0.223	ug/l #	49
16) Acetone	4.293	43	2337	1.350	ug/l	93
17) Carbon Disulfide	4.527	76	2154	0.234	ug/l #	74
18) Methyl Acetate	4.864	43	7817	1.752	ug/l #	65
20) Methylene Chloride	5.090	84	6607	1.487	ug/l #	84
23) Vinyl Acetate	6.436	43	6730	0.675	ug/l #	84
25) 2-Butanone	7.345	43	1392	0.554	ug/l #	80
28) Bromochloromethane	7.654	49	953	0.288	ug/l #	67
29) Tetrahydrofuran	7.694	42	1035	0.644	ug/l #	65
30) Chloroform	7.828	83	1859	0.242	ug/l	97
31) Cyclohexane	8.088	56	10102	1.444	ug/l #	32
36) 1,1-Dichloropropene	8.086	75	29425	4.778	ug/l #	51
38) Carbon Tetrachloride	8.088	117	37253	6.150	ug/l #	17
43) Isopropyl Acetate	8.598	43	5252	0.544	ug/l #	58
48) Methyl methacrylate	9.563	41	949	0.228	ug/l #	83
49) 1,4-Dioxane	9.574	88	167	2.174	ug/l #	12
51) 4-Methyl-2-Pentanone	10.336	43	5265	0.884	ug/l	98
58) 2-Chloroethyl Vinyl ether	10.043	63	1867	1.688	ug/l	95
59) 2-Hexanone	11.089	43	4175	0.976	ug/l	91
68) m/p-Xylenes	11.961	106	2294	0.284	ug/l	89
74) N-amyl acetate	12.387	43	1328	0.232	ug/l #	68
75) 1,1,2,2-Tetrachloroethane	12.827	83	1042	0.210	ug/l #	96
76) 1,2,3-Trichloropropane	12.733	75	136058	33.628	ug/l #	100
79) 2-Chlorotoluene	13.010	91	2416	0.214	ug/l	89
81) trans-1,4-Dichloro-2-b...	12.733	75	136058	106.161	ug/l #	6
82) 4-Chlorotoluene	13.109	91	2289	0.202	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080521\
Data File : VN068022.D
Acq On : 5 Aug 2021 17:45
Operator : JC/MD
Sample : M2940-09 .5PPB MDL
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Aug 06 02:09:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 06 02:07:57 2021
Response via : Initial Calibration




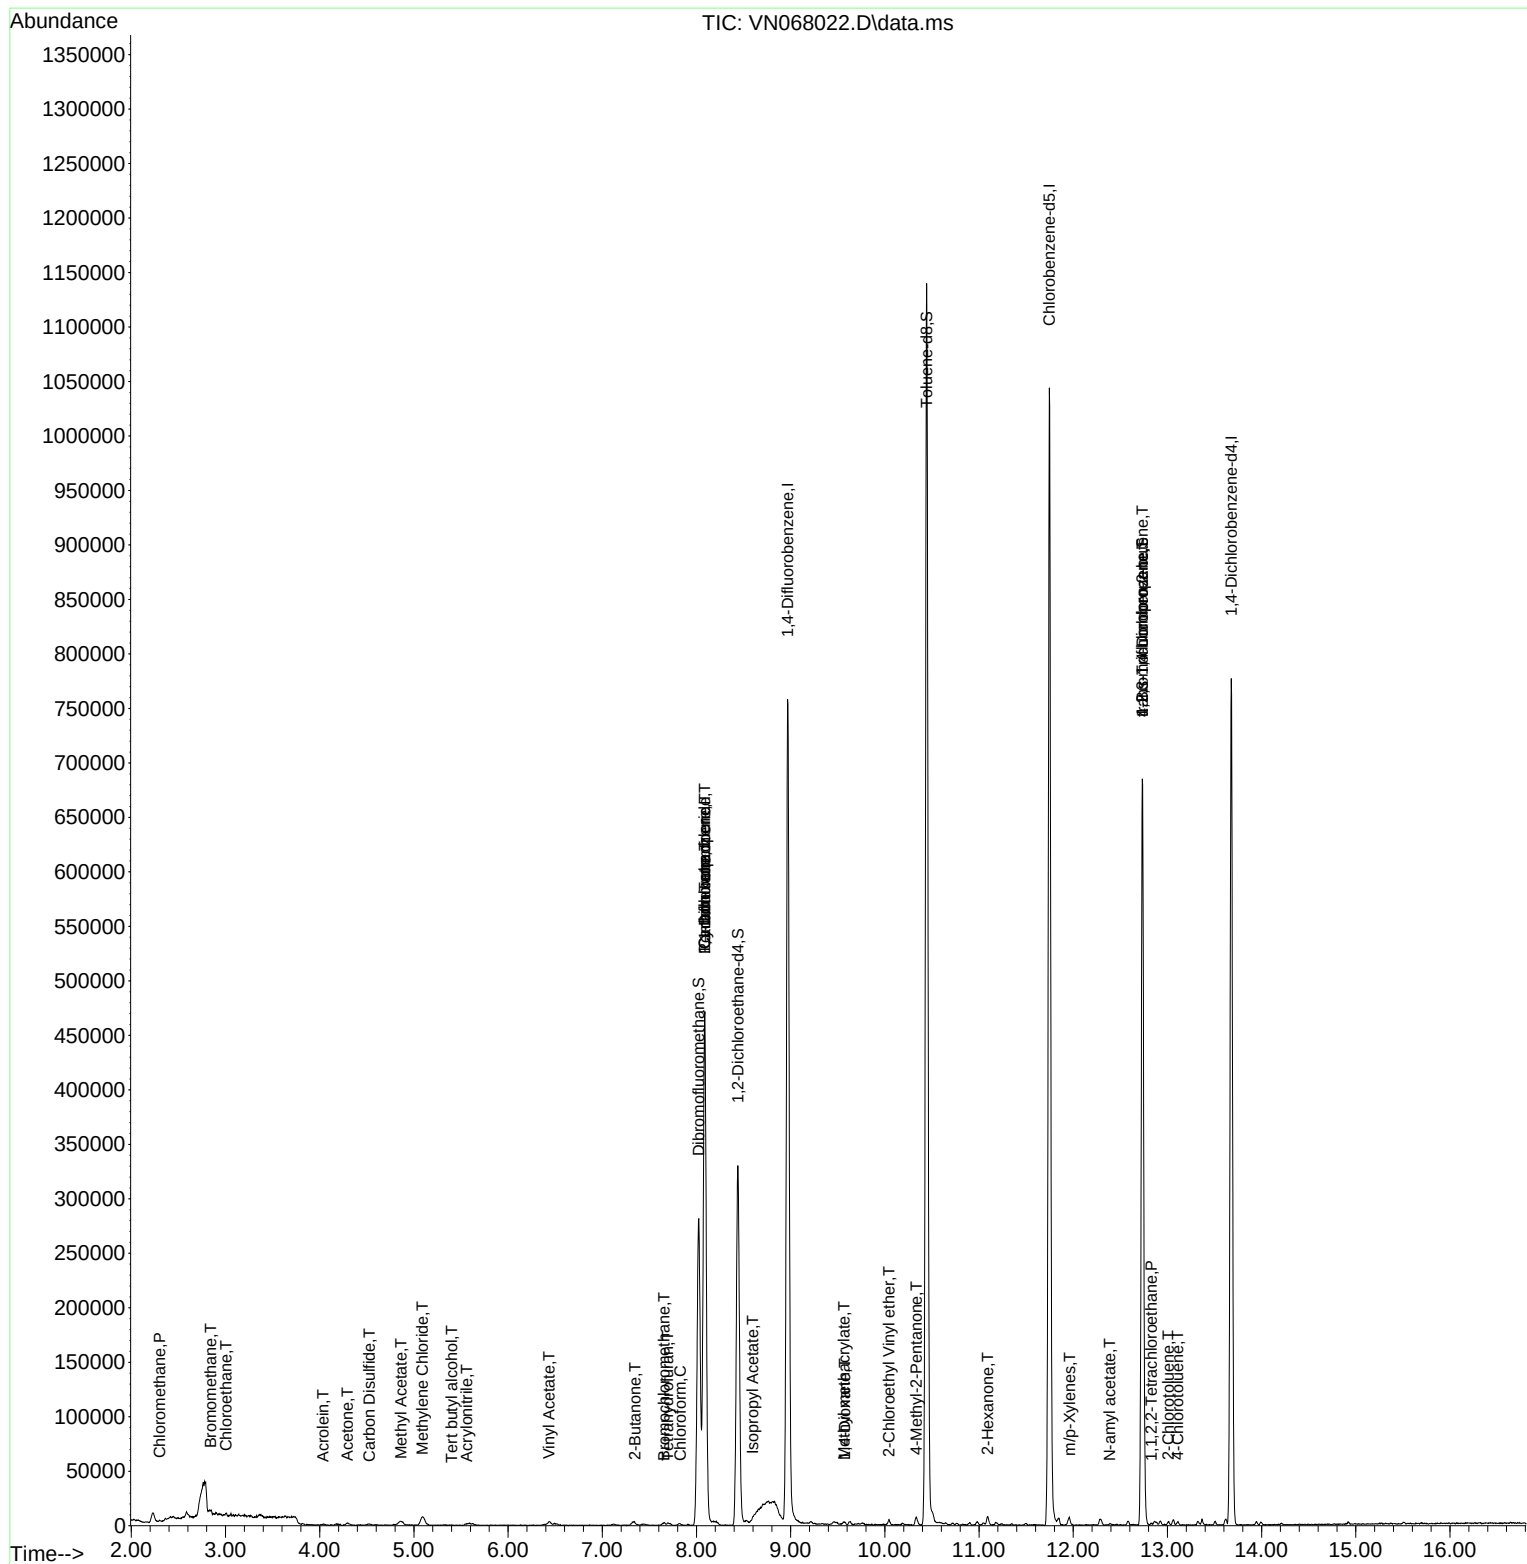




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 335017
Ion Ratio Lower Upper
168 100
99 63.9 62.9 94.3

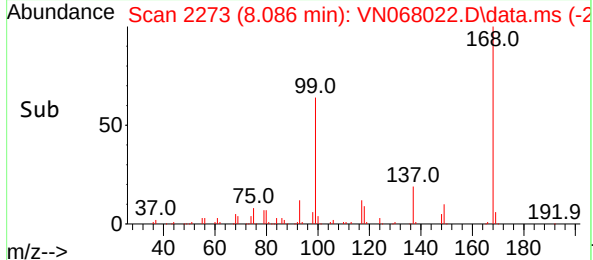

#3
Chloromethane
Concen: 0.330 ug/l
RT: 2.301 min Scan# 116
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45


Tgt Ion: 50 Resp: 1408
Ion Ratio Lower Upper
50 100
52 56.0 25.6 38.4#

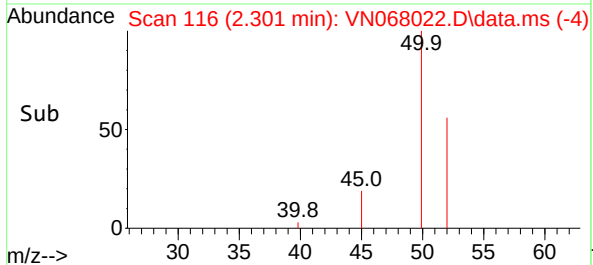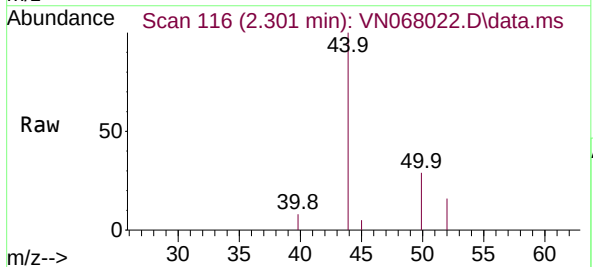



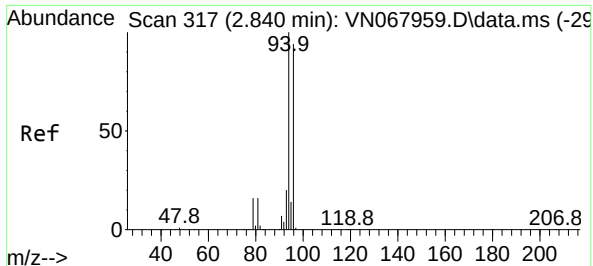


#5
Bromomethane
Concen: 0.419 ug/l
RT: 2.842 min Scan# 318
Delta R.T. 0.002 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Instrument :
MSVOA_N
ClientSampled :



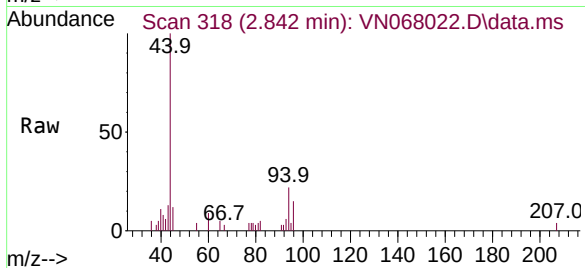



Tgt Ion: 94 Resp: 2486
Ion Ratio Lower Upper
94 100
96 65.2 73.7 110.5#

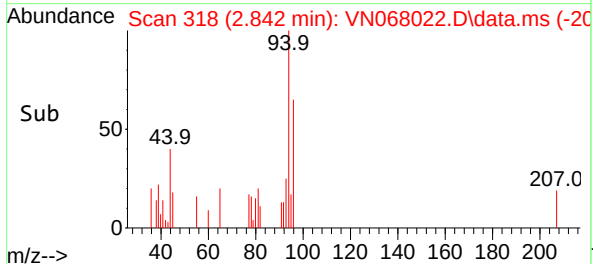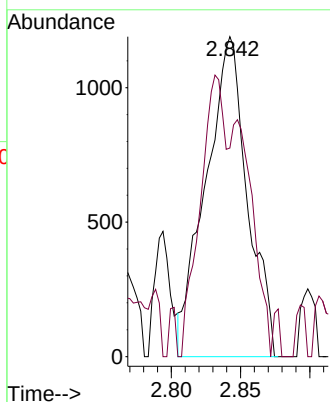

#6
Chloroethane
Concen: 0.233 ug/l
RT: 3.006 min Scan# 379
Delta R.T. -0.005 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 64 Resp: 1203
Ion Ratio Lower Upper
64 100
66 55.3 24.7 37.1#

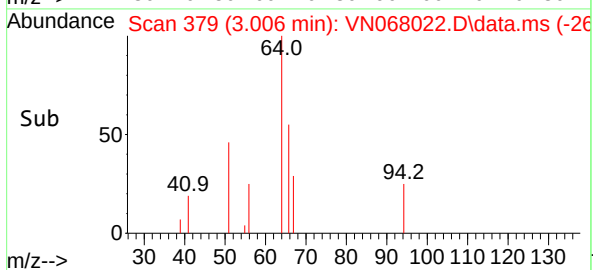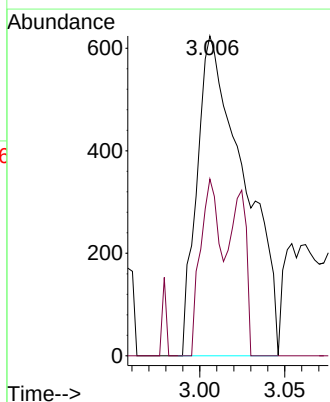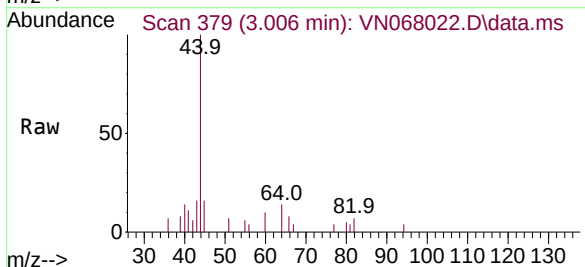







#11

Tert butyl alcohol
Concen: 0.222 ug/l
RT: 5.398 min Scan# 1271
Delta R.T. 0.008 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 59 Resp: 141
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

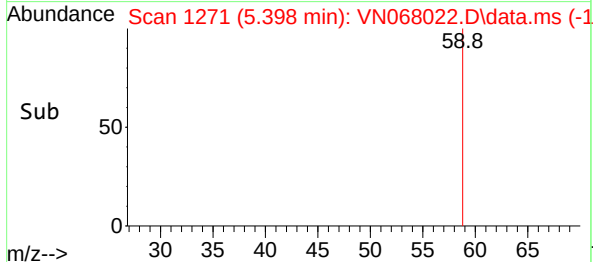


#13

Acrolein
Concen: 1.721 ug/l
RT: 4.033 min Scan# 762
Delta R.T. -0.008 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 56 Resp: 742
Ion Ratio Lower Upper
56 100
55 30.7 57.4 86.0#


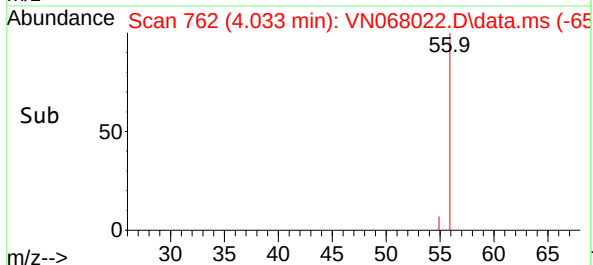

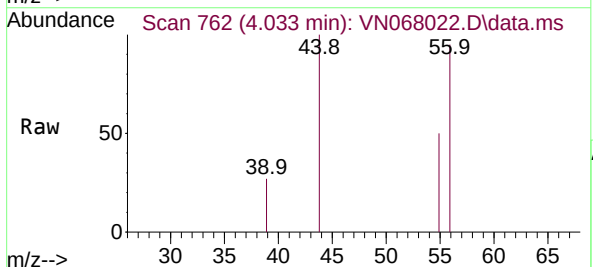




#15
Acrylonitrile
Concen: 0.223 ug/l
RT: 5.559 min Scan# 1331
Delta R.T. 0.002 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 53 Resp: 398
Ion Ratio Lower Upper
53 100
52 39.4 66.2 99.2#
51 72.4 30.2 45.4#

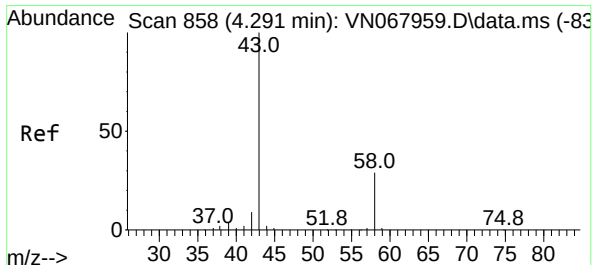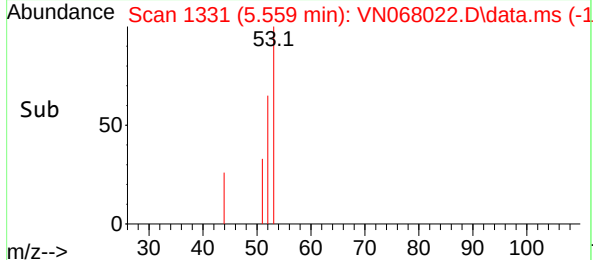

#16
Acetone
Concen: 1.350 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.002 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 43 Resp: 2337
Ion Ratio Lower Upper
43 100
58 30.2 21.2 31.8


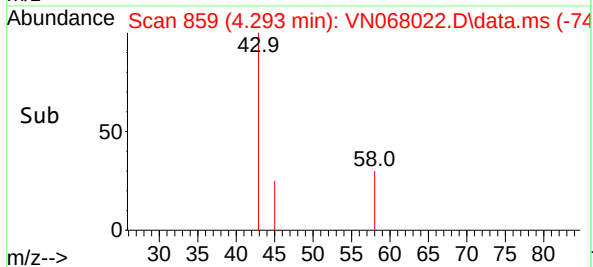

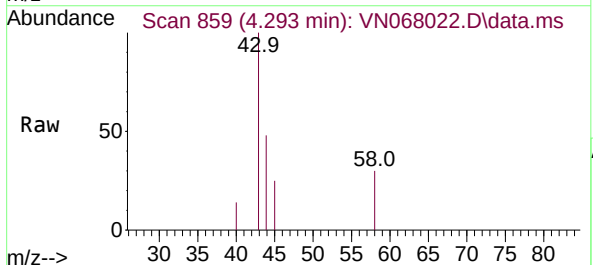




#17
Carbon Disulfide
Concen: 0.234 ug/l
RT: 4.527 min Scan# 946
Delta R.T. 0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 2154
Ion Ratio Lower Upper
76 100
78 0.0 7.7 11.5#

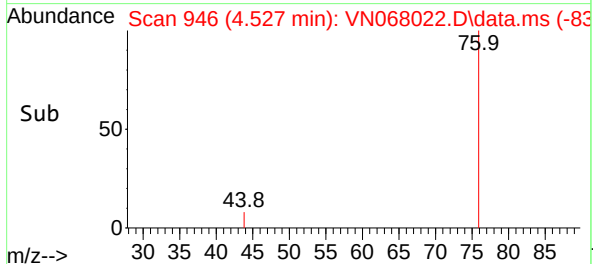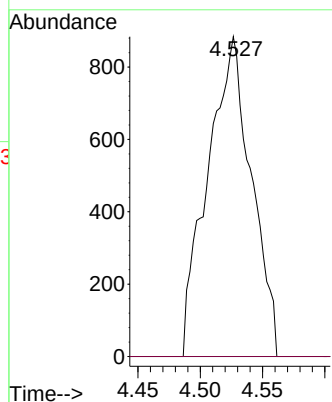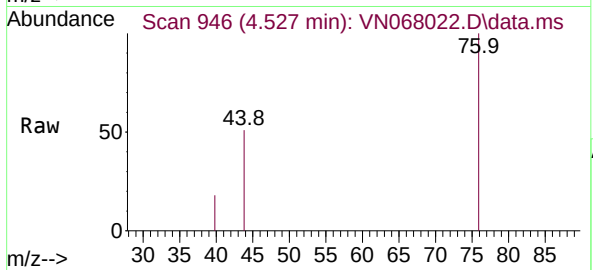

#18
Methyl Acetate
Concen: 1.752 ug/l
RT: 4.864 min Scan# 1072
Delta R.T. 0.007 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45


Tgt Ion: 43 Resp: 7817
Ion Ratio Lower Upper
43 100
74 5.2 17.4 26.0#

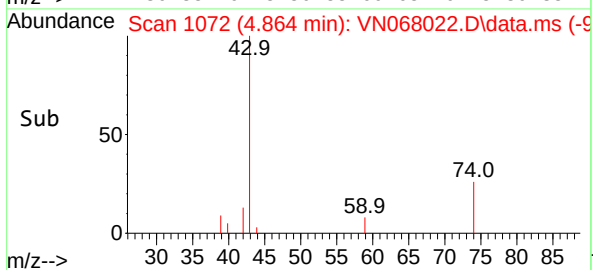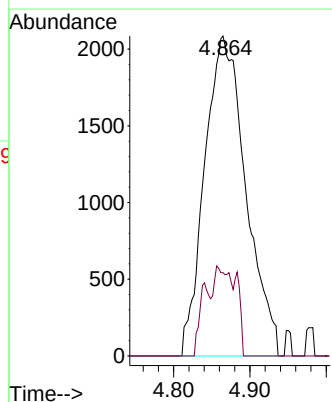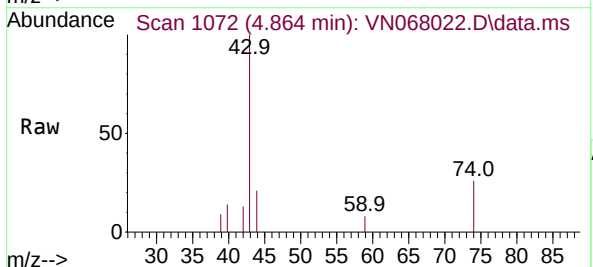






#20
Methylene Chloride
Concen: 1.487 ug/l
RT: 5.090 min Scan# 1156
Delta R.T. -0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Instrument :
MSVOA_N
ClientSampleId :

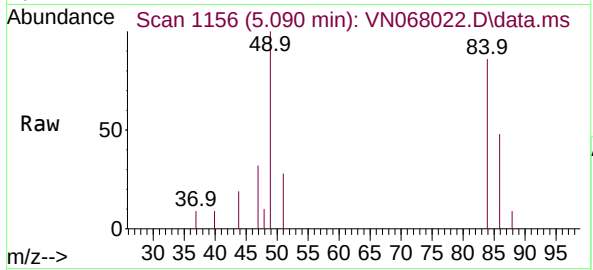

Tgt Ion: 84 Resp: 6607




Ion	Ratio	Lower	Upper
84	100		
49	116.0	110.9	166.3
51	32.4	32.6	49.0#
86	55.8	51.6	77.4

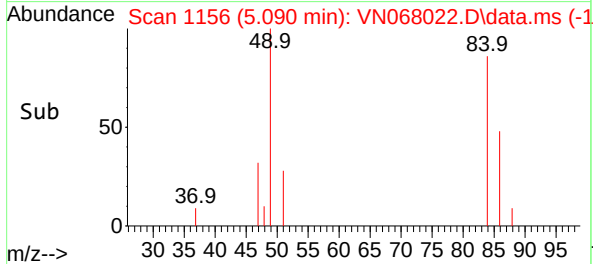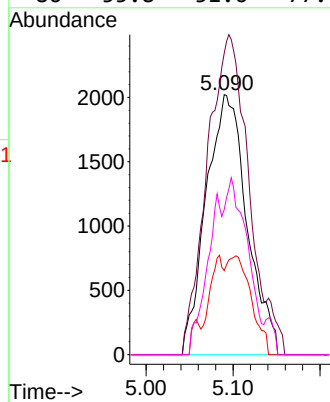


#23
Vinyl Acetate
Concen: 0.675 ug/l
RT: 6.436 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 43 Resp: 6730

Ion	Ratio	Lower	Upper
43	100		
86	14.8	7.3	10.9#

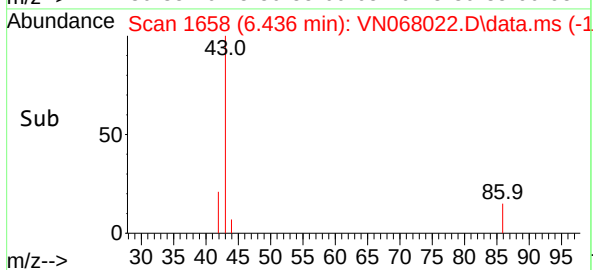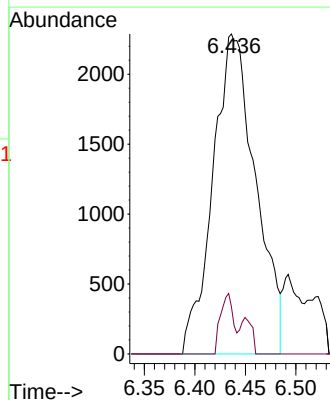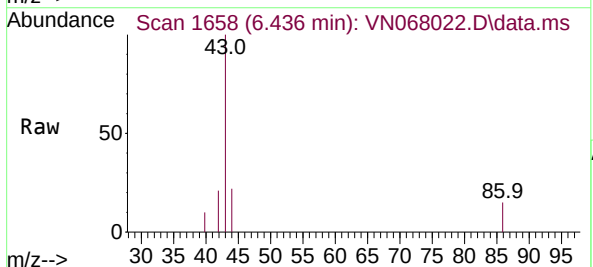



#25

2-Butanone

Concen: 0.554 ug/l

RT: 7.345 min Scan# 1997

Delta R.T. 0.005 min

Lab File: VN068022.D





Acq: 5 Aug 2021 17:45

Tgt Ion: 43 Resp: 1392

Ion Ratio Lower Upper

43 100

72 34.8 19.7 29.5#

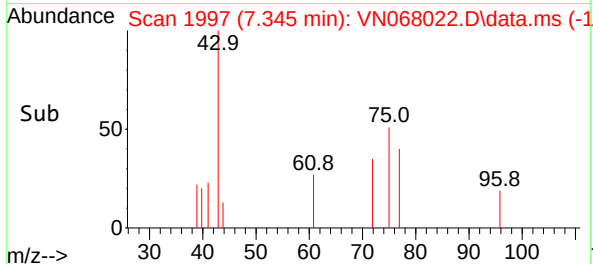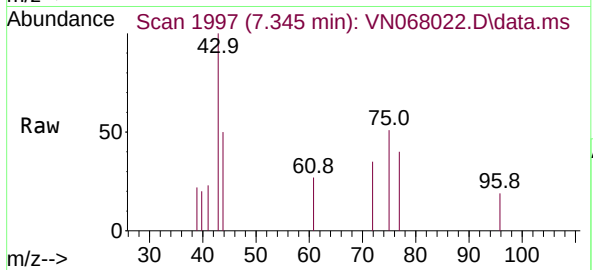

#28

Bromochloromethane

Concen: 0.288 ug/l

RT: 7.654 min Scan# 2112

Delta R.T. -0.003 min

Lab File: VN068022.D

Acq: 5 Aug 2021 17:45




Tgt Ion: 49 Resp: 953


Ion Ratio Lower Upper

49 100

129 0.0 0.0 3.8

130 87.8 49.7 74.5#

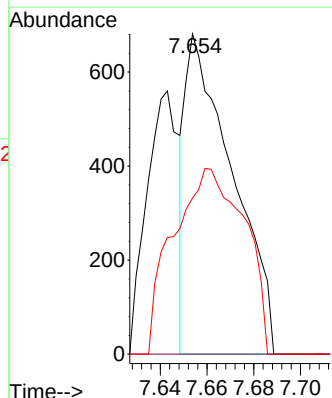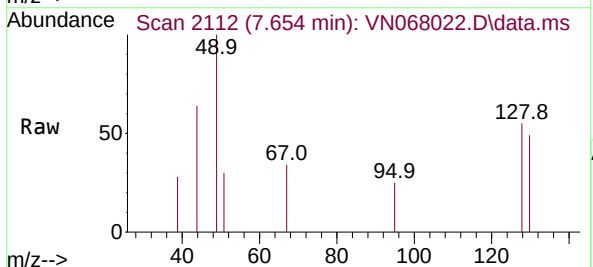

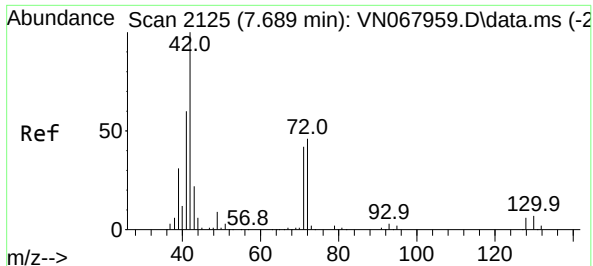

#29

Tetrahydrofuran

Concen: 0.644 ug/l

RT: 7.694 min Scan# 2127





Delta R.T. 0.005 min

Lab File: VN068022.D

Acq: 5 Aug 2021 17:45

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion: 42	Resp: 1035
Ion Ratio	Lower Upper
42	100
72	46.2 32.8 49.2
71	0.0 31.2 46.8#

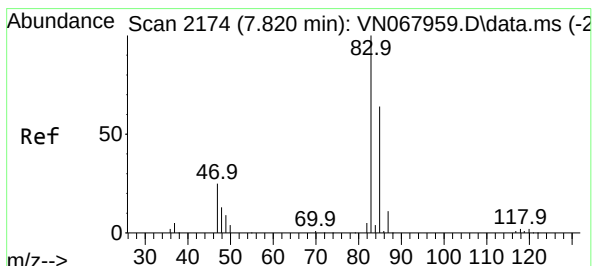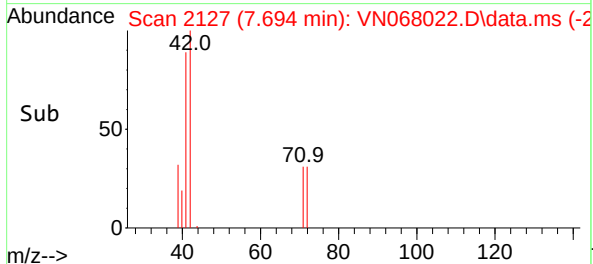

#30

Chloroform

Concen: 0.242 ug/l




RT: 7.828 min Scan# 2177


Delta R.T. 0.008 min

Lab File: VN068022.D

Acq: 5 Aug 2021 17:45

Tgt Ion: 83	Resp: 1859
Ion Ratio	Lower Upper
83	100
85	62.1 51.5 77.3



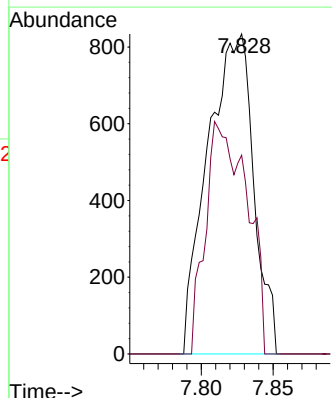
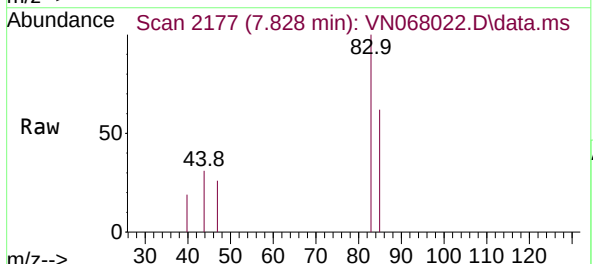


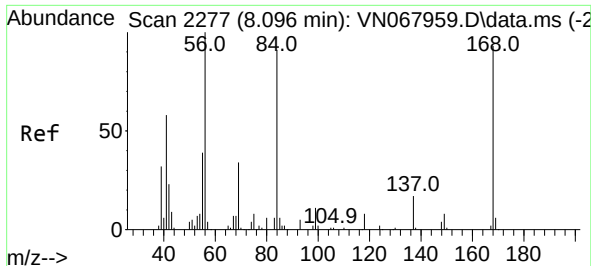

#31
Cyclohexane
Concen: 1.444 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.008 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 10102
Ion Ratio Lower Upper
56 100
69 130.0 27.3 40.9#
84 104.8 64.9 97.3#

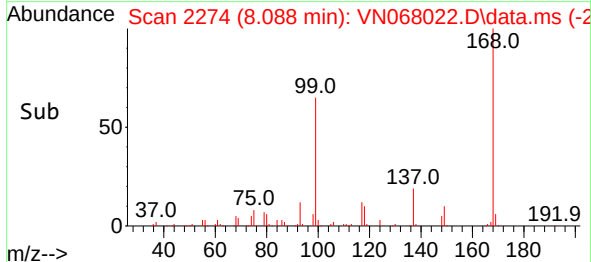

#33
1,2-Dichloroethane-d4
Concen: 58.864 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 65 Resp: 279177
Ion Ratio Lower Upper
65 100
67 51.4 0.0 98.6


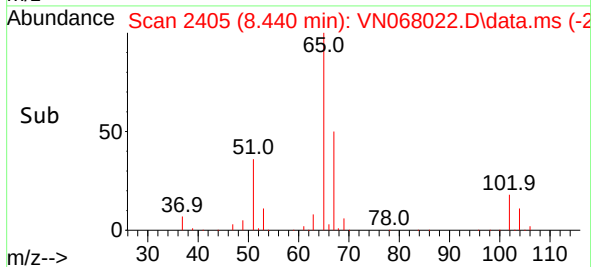

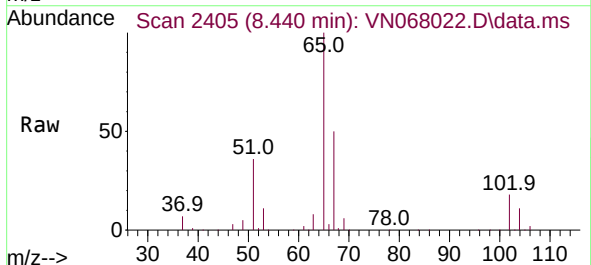


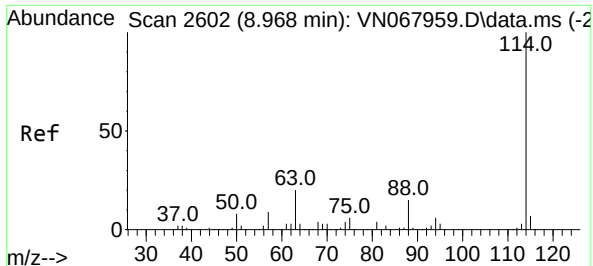

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:114 Resp: 665836
Ion Ratio Lower Upper
114 100
63 20.4 0.0 49.0
88 14.8 0.0 36.6

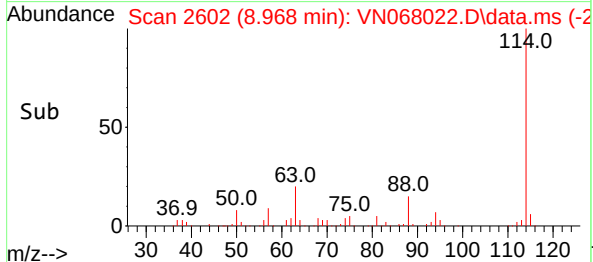

#35
Dibromofluoromethane
Concen: 52.249 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion:113 Resp: 202746
Ion Ratio Lower Upper
113 100
111 104.1 83.8 125.8
192 15.9 13.4 20.0


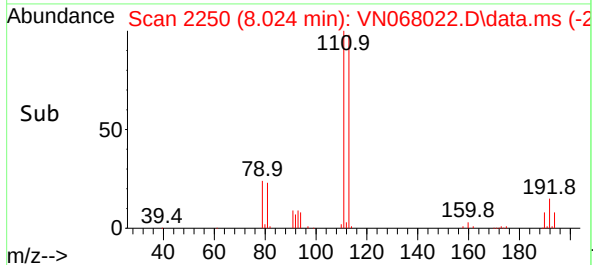

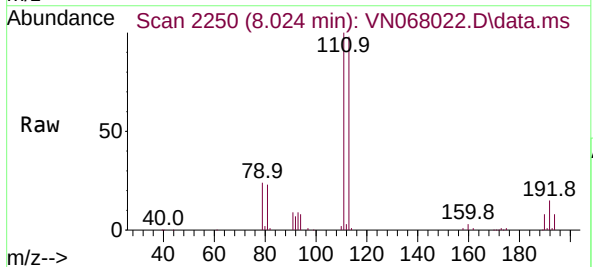


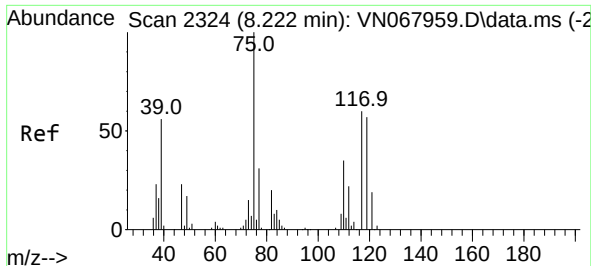

#36
 1,1-Dichloropropene
 Concen: 4.778 ug/l
 RT: 8.086 min Scan# 2273
 Delta R.T. -0.136 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 75 Resp: 29425
 Ion Ratio Lower Upper
 75 100
 110 7.6 15.7 47.0#
 77 0.0 24.6 37.0#

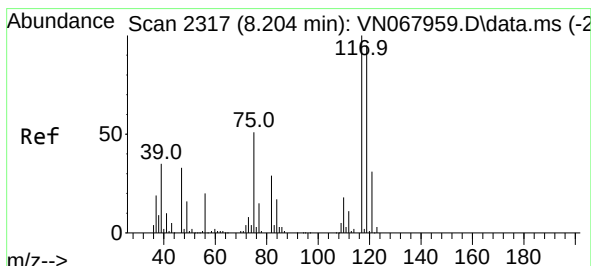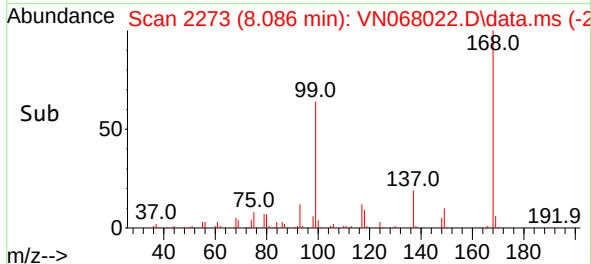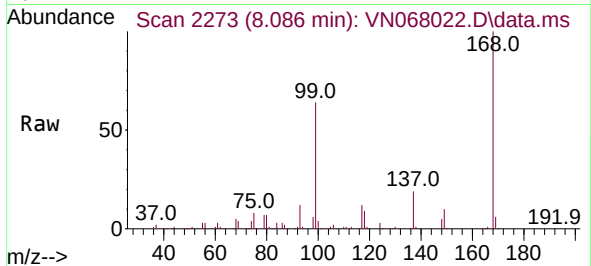

#38
 Carbon Tetrachloride
 Concen: 6.150 ug/l
 RT: 8.088 min Scan# 2274
 Delta R.T. -0.116 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45

Tgt Ion: 117 Resp: 37253
 Ion Ratio Lower Upper
 117 100
 119 5.1 75.4 113.2#
 121 0.0 23.5 35.3#


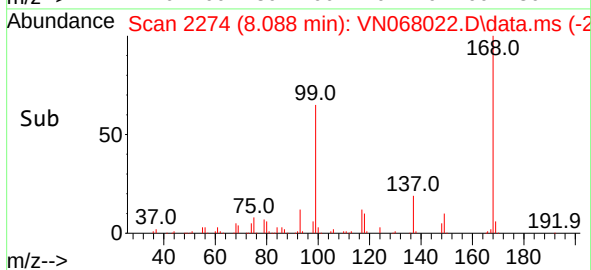

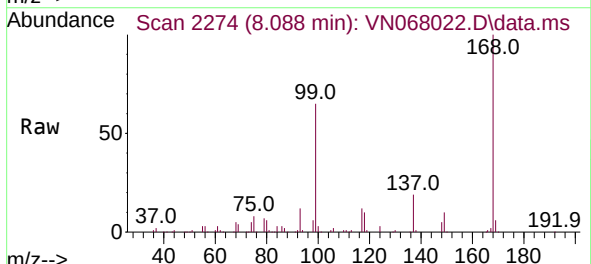


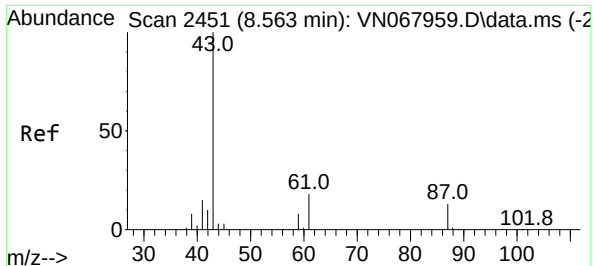

#43
Isopropyl Acetate
Concen: 0.544 ug/l
RT: 8.598 min Scan# 2464
Delta R.T. 0.035 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 5252
Ion Ratio Lower Upper
43 100
61 0.0 19.0 28.4#
87 0.0 9.5 14.3#

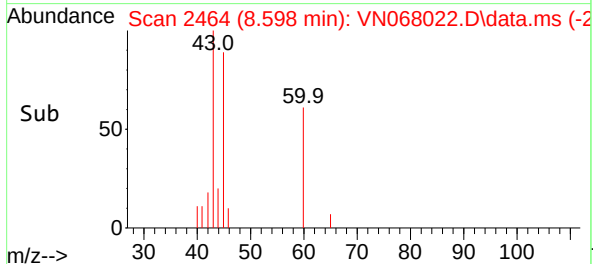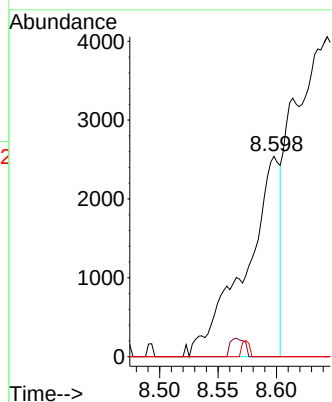

#48
Methyl methacrylate
Concen: 0.228 ug/l
RT: 9.563 min Scan# 2824
Delta R.T. 0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 41 Resp: 949
Ion Ratio Lower Upper
41 100
69 66.8 64.6 96.8
39 51.2 53.3 79.9#

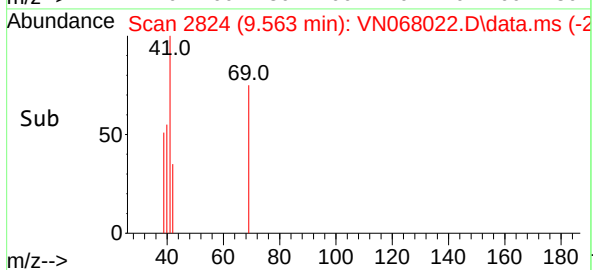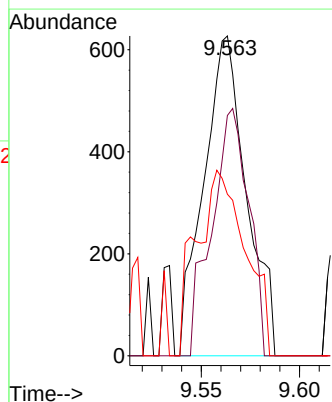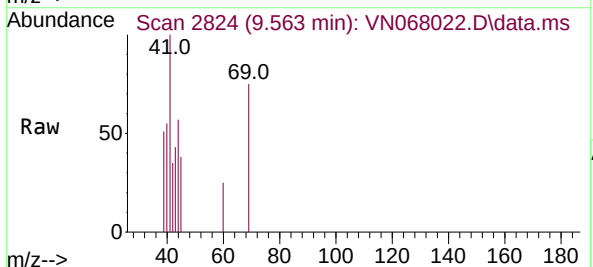

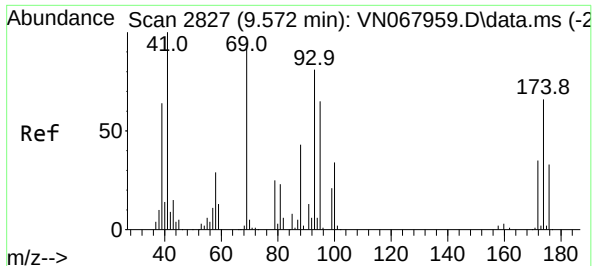

#49

1,4-Dioxane

Concen: 2.174 ug/l

RT: 9.574 min Scan# 2828

Delta R.T. 0.002 min

Lab File: VN068022.D

Acq: 5 Aug 2021 17:45

Tgt Ion: 88 Resp: 167

Ion Ratio Lower Upper

88 100





43 86.8 28.8 43.2#

58 0.0 60.4 90.6#

Instrument :

MSVOA_N

ClientSampled :

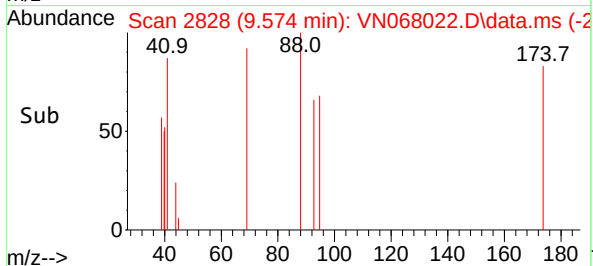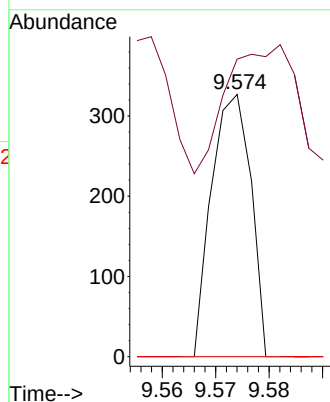

#50

Toluene-d8

Concen: 50.452 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. -0.000 min

Lab File: VN068022.D




Acq: 5 Aug 2021 17:45


Tgt Ion: 98 Resp: 792338

Ion Ratio Lower Upper

98 100

100 64.0 51.7 77.5


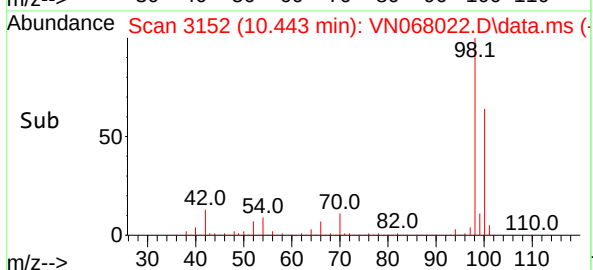
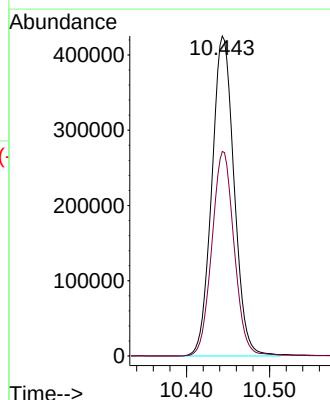
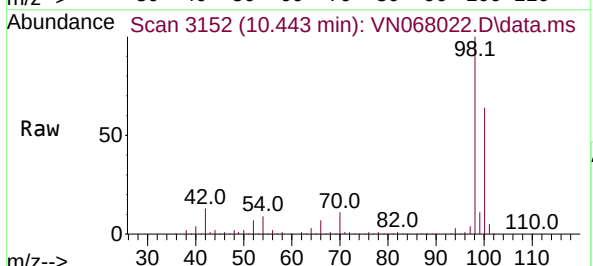




#51
4-Methyl-2-Pentanone
Concen: 0.884 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 5265
Ion Ratio Lower Upper
43 100
58 37.0 28.6 43.0

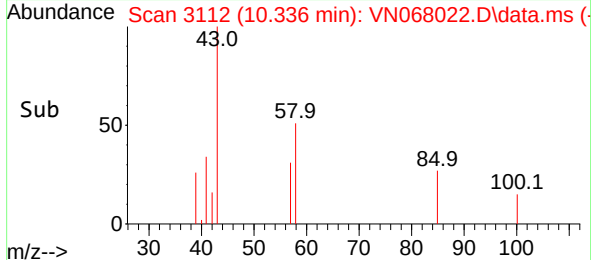

#58
2-Chloroethyl Vinyl ether
Concen: 1.688 ug/l
RT: 10.043 min Scan# 3003
Delta R.T. -0.001 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 63 Resp: 1867
Ion Ratio Lower Upper
63 100
106 22.2 19.8 29.8


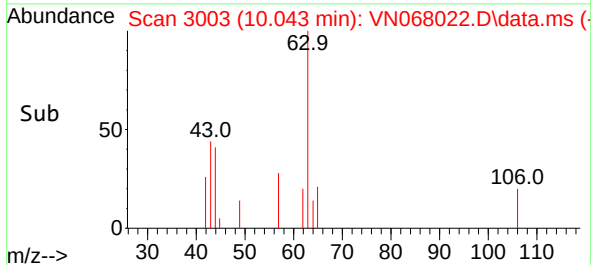

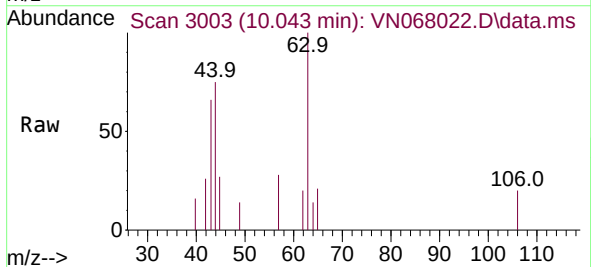




#59
2-Hexanone
Concen: 0.976 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. 0.002 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 4175
Ion Ratio Lower Upper
43 100
58 43.5 24.7 74.1

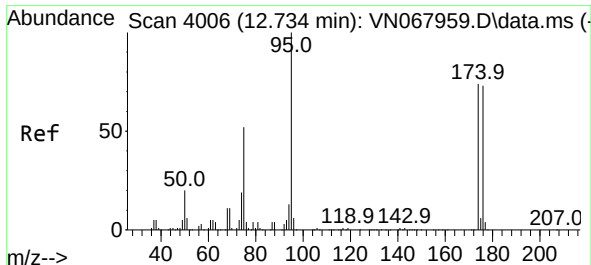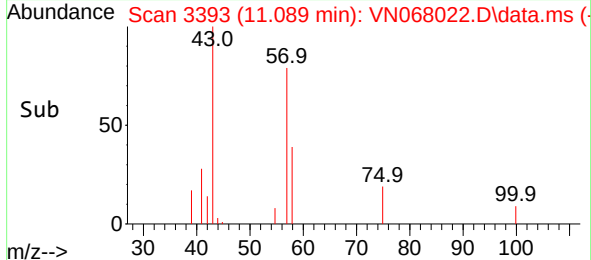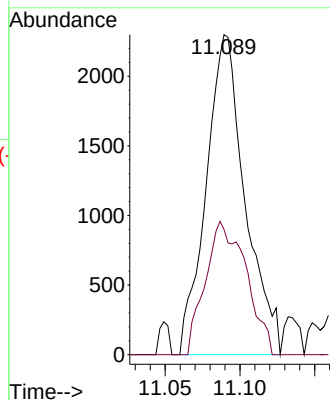

#62
4-Bromofluorobenzene
Concen: 44.669 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.001 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 95 Resp: 243006
Ion Ratio Lower Upper
95 100
174 72.9 0.0 122.0
176 69.3 0.0 117.6


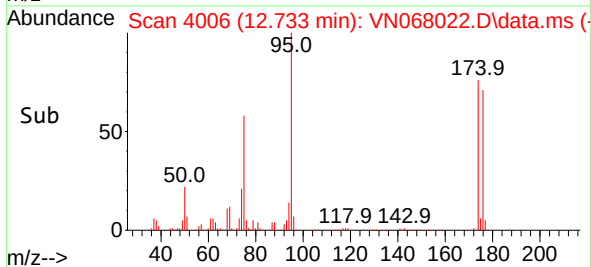
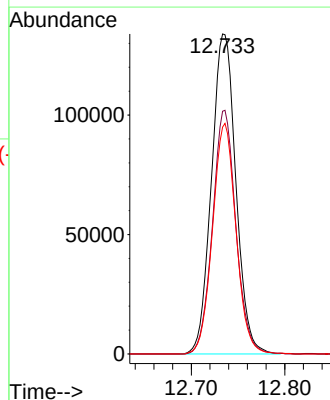
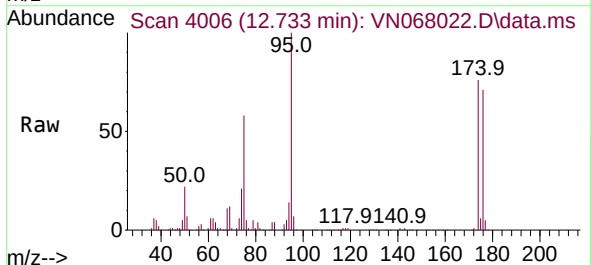




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.001 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 595834
Ion Ratio Lower Upper
117 100
82 57.1 53.1 79.7
119 32.7 25.5 38.3

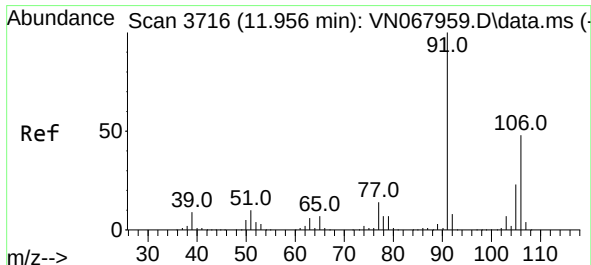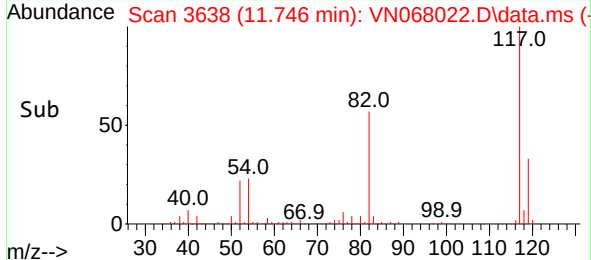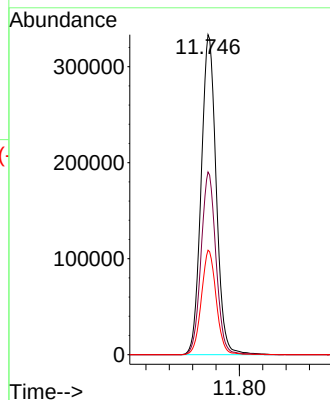

#68
m/p-Xylenes
Concen: 0.284 ug/l
RT: 11.961 min Scan# 3718
Delta R.T. 0.005 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion:106 Resp: 2294
Ion Ratio Lower Upper
106 100
91 207.2 180.6 270.8


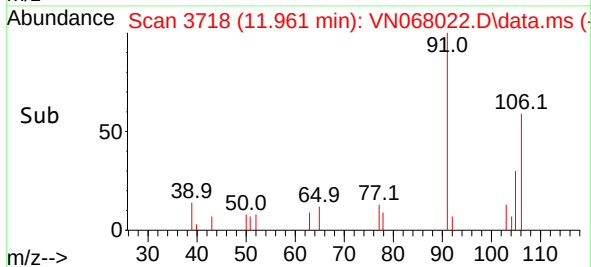
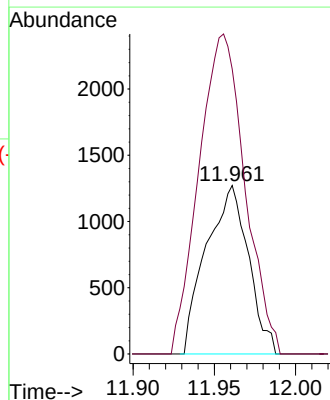
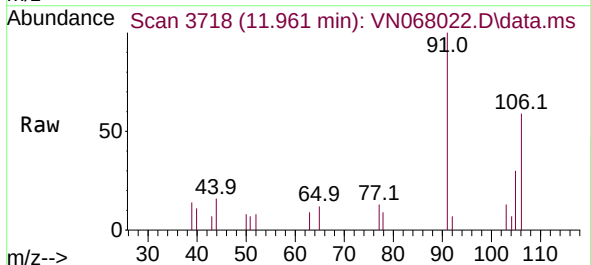


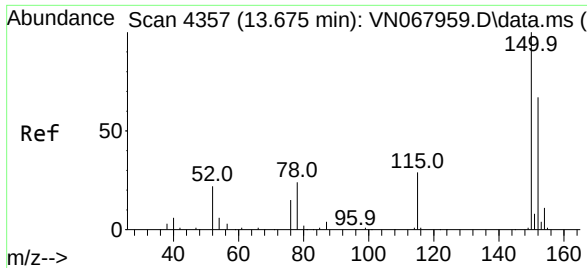

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.677 min Scan# 4358
 Delta R.T. 0.002 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion:152 Resp: 201461
 Ion Ratio Lower Upper
 152 100
 115 63.8 36.1 108.5
 150 159.1 0.0 351.8

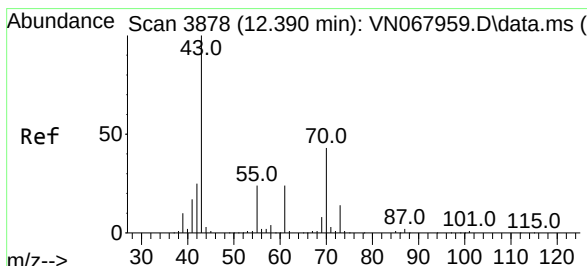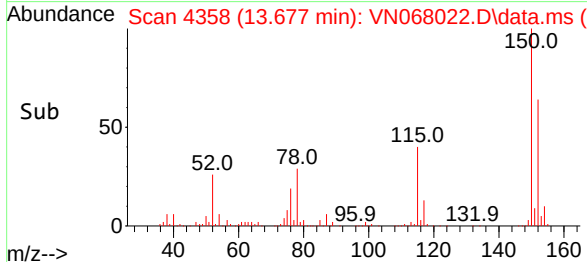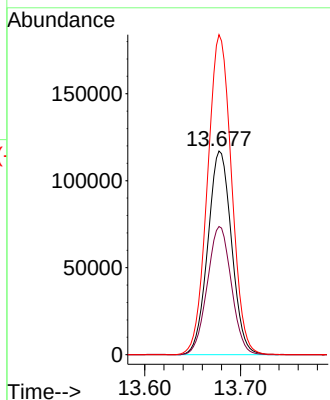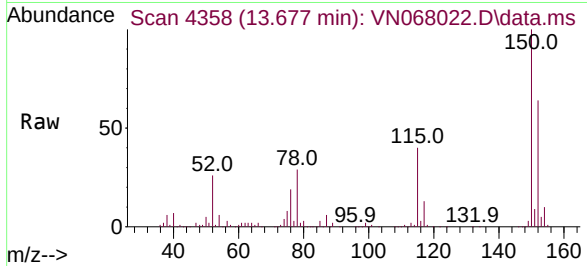

#74
 N-ethyl acetate
 Concen: 0.232 ug/l
 RT: 12.387 min Scan# 3877
 Delta R.T. -0.003 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45

Tgt Ion: 43 Resp: 1328
 Ion Ratio Lower Upper
 43 100
 70 19.9 29.4 44.2#
 55 11.0 17.0 25.4#
 61 0.0 17.6 26.4#


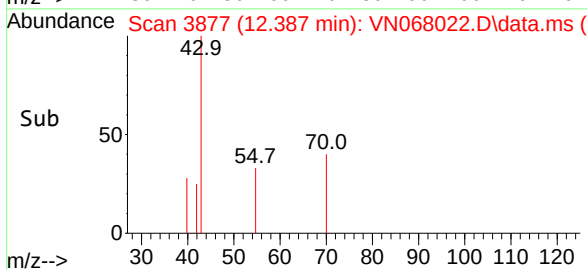
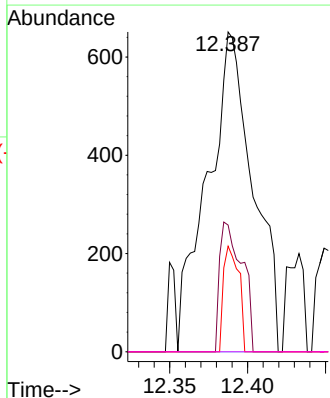
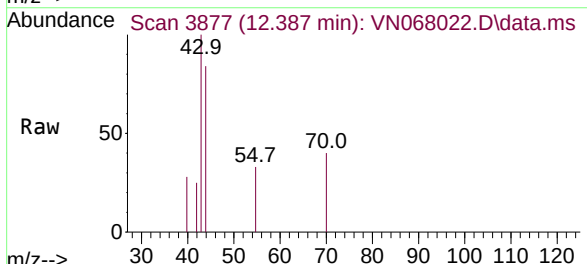




#75
 1,1,2,2-Tetrachloroethane
 Concen: 0.210 ug/l
 RT: 12.827 min Scan# 4041
 Delta R.T. -0.003 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 83 Resp: 1042
 Ion Ratio Lower Upper
 83 100
 131 0.0 4.8 14.4#
 85 63.7 32.2 96.6

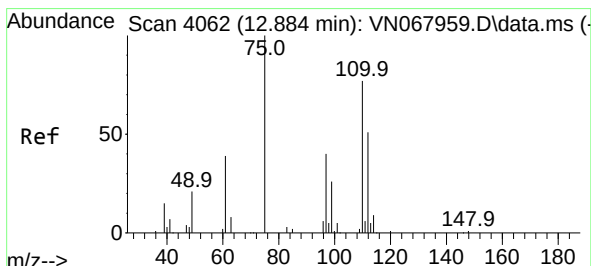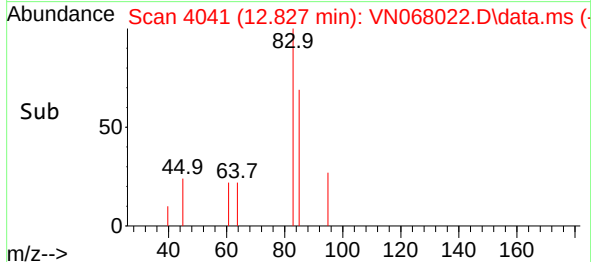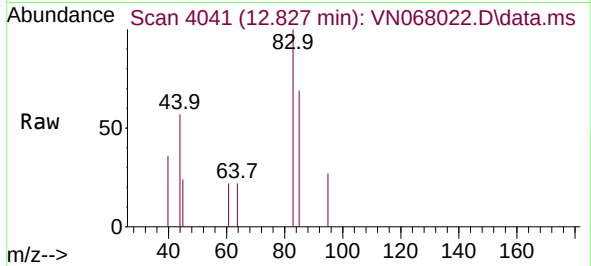

#76
 1,2,3-Trichloropropane
 Concen: 33.628 ug/l
 RT: 12.733 min Scan# 4006
 Delta R.T. -0.151 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45

Tgt Ion: 75 Resp: 136058
 Ion Ratio Lower Upper
 75 100
 77 0.9 0.0 0.0#


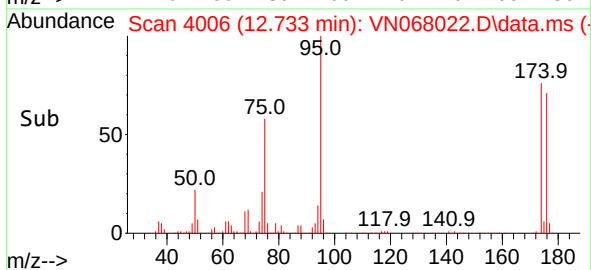

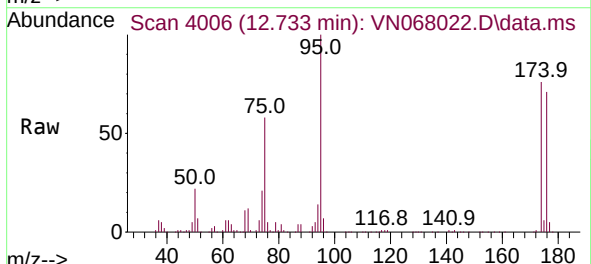


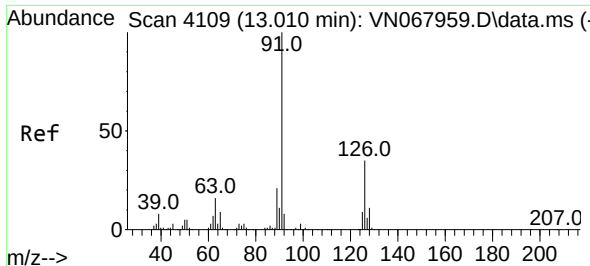

#79
2-Chlorotoluene
Concen: 0.214 ug/l
RT: 13.010 min Scan# 4109
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 2416
Ion Ratio Lower Upper
91 100
126 35.1 14.5 43.5

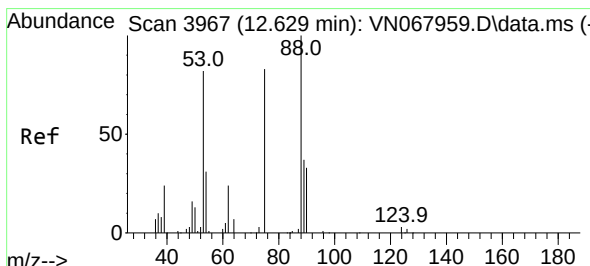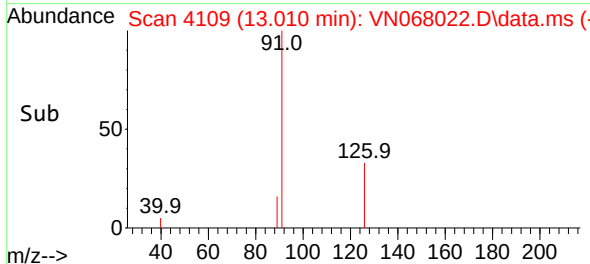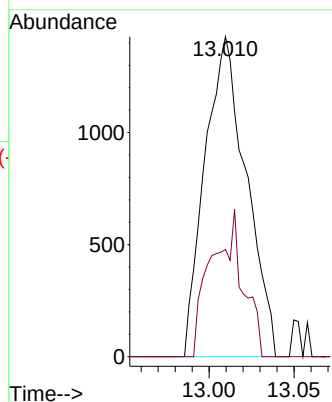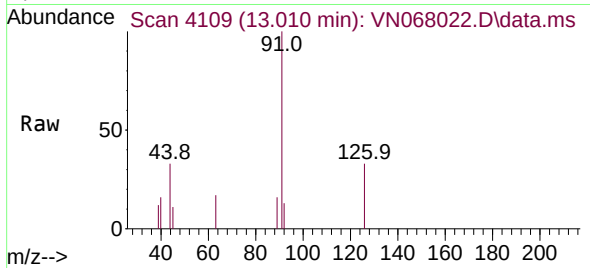

#81
trans-1,4-Dichloro-2-butene
Concen: 106.161 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45


Tgt Ion: 75 Resp: 136058
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

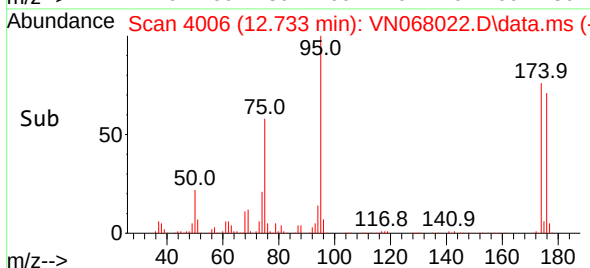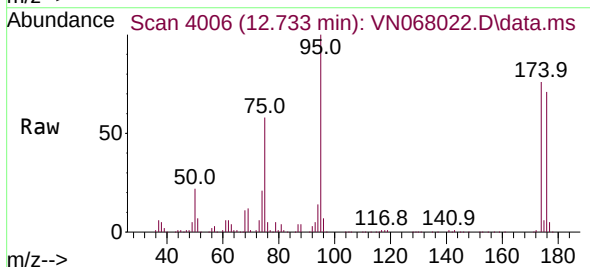



#82
 4-Chlorotoluene
 Concen: 0.202 ug/l
 RT: 13.109 min Scan# 4146
 Delta R.T. 0.003 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45

Instrument :
 MSVOA_N
 ClientSampleId :

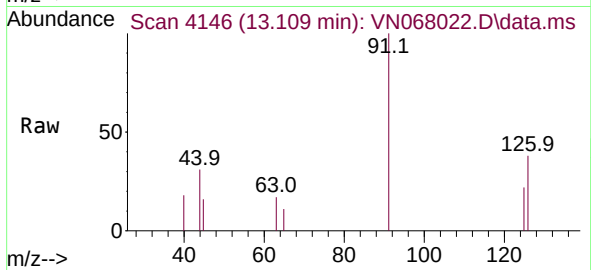

Tgt Ion: 91 Resp: 2289
 Ion Ratio Lower Upper
 91 100
 126 30.8 14.8 44.4

