

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080521\
 Data File : VN068031.D
 Acq On : 5 Aug 2021 21:24
 Operator : JC/MD
 Sample : M3291-04
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 06 01:27:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 29 15:02:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	296999	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	591653	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	623063	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	214002	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	235618	56.039	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 112.080%			
35) Dibromofluoromethane	8.024	113	179529	52.067	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 104.140%			
50) Toluene-d8	10.443	98	773011	48.687	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 97.380%			
62) 4-Bromofluorobenzene	12.733	95	260181	45.200	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 90.400%			
Target Compounds					Qvalue	
3) Chloromethane	2.300	50	781	0.207	ug/l	91
11) Tert butyl alcohol	5.385	59	793	1.408	ug/l #	71
13) Acrolein	4.052	56	114	0.298	ug/l #	74
16) Acetone	4.288	43	28848	18.804	ug/l	96
18) Methyl Acetate	4.862	43	5089	1.280	ug/l #	90
20) Methylene Chloride	5.095	84	32934	9.064	ug/l #	84
23) Vinyl Acetate	6.594	43	55	8.806	ug/l #	75
25) 2-Butanone	7.351	43	20607	9.259	ug/l	96
29) Tetrahydrofuran	7.694	42	1425	1.000	ug/l #	87
31) Cyclohexane	8.088	56	7652	1.234	ug/l #	17
36) 1,1-Dichloropropene	8.085	75	26220	4.791	ug/l #	52
37) Ethyl Acetate	7.351	43	20607	4.001	ug/l #	70
38) Carbon Tetrachloride	8.091	117	33688	6.259	ug/l #	17
41) Methacrylonitrile	7.691	41	518	0.211	ug/l #	33
43) Isopropyl Acetate	8.568	43	40857	4.760	ug/l #	91
45) 1,2-Dichloropropane	9.628	63	2644	0.655	ug/l #	44
48) Methyl methacrylate	9.547	41	10699	4.690	ug/l #	12
49) 1,4-Dioxane	9.625	88	246	3.603	ug/l #	1
51) 4-Methyl-2-Pentanone	10.341	43	5934	13.468	ug/l #	64
53) t-1,3-Dichloropropene	10.623	75	24	2.837	ug/l #	48
54) cis-1,3-Dichloropropene	10.247	75	63514	10.621	ug/l #	60
56) Ethyl methacrylate	10.872	69	401	3.150	ug/l #	1
57) 1,3-Dichloropropane	11.095	76	40421	6.073	ug/l #	43
59) 2-Hexanone	11.095	43	595364	139.746	ug/l #	55
60) Dibromochloromethane	11.489	129	321	3.361	ug/l #	11
68) m/p-Xylenes	11.956	106	54	4.067	ug/l #	1
74) N-amyl acetate	12.355	43	3008	0.496	ug/l #	50
76) 1,2,3-Trichloropropane	12.733	75	139857	32.542	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.733	75	139857	87.386	ug/l #	6
95) Naphthalene	15.509	128	451	3.167	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080521\
Data File : VN068031.D
Acq On : 5 Aug 2021 21:24
Operator : JC/MD
Sample : M3291-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Aug 06 01:27:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 29 15:02:35 2021
Response via : Initial Calibration




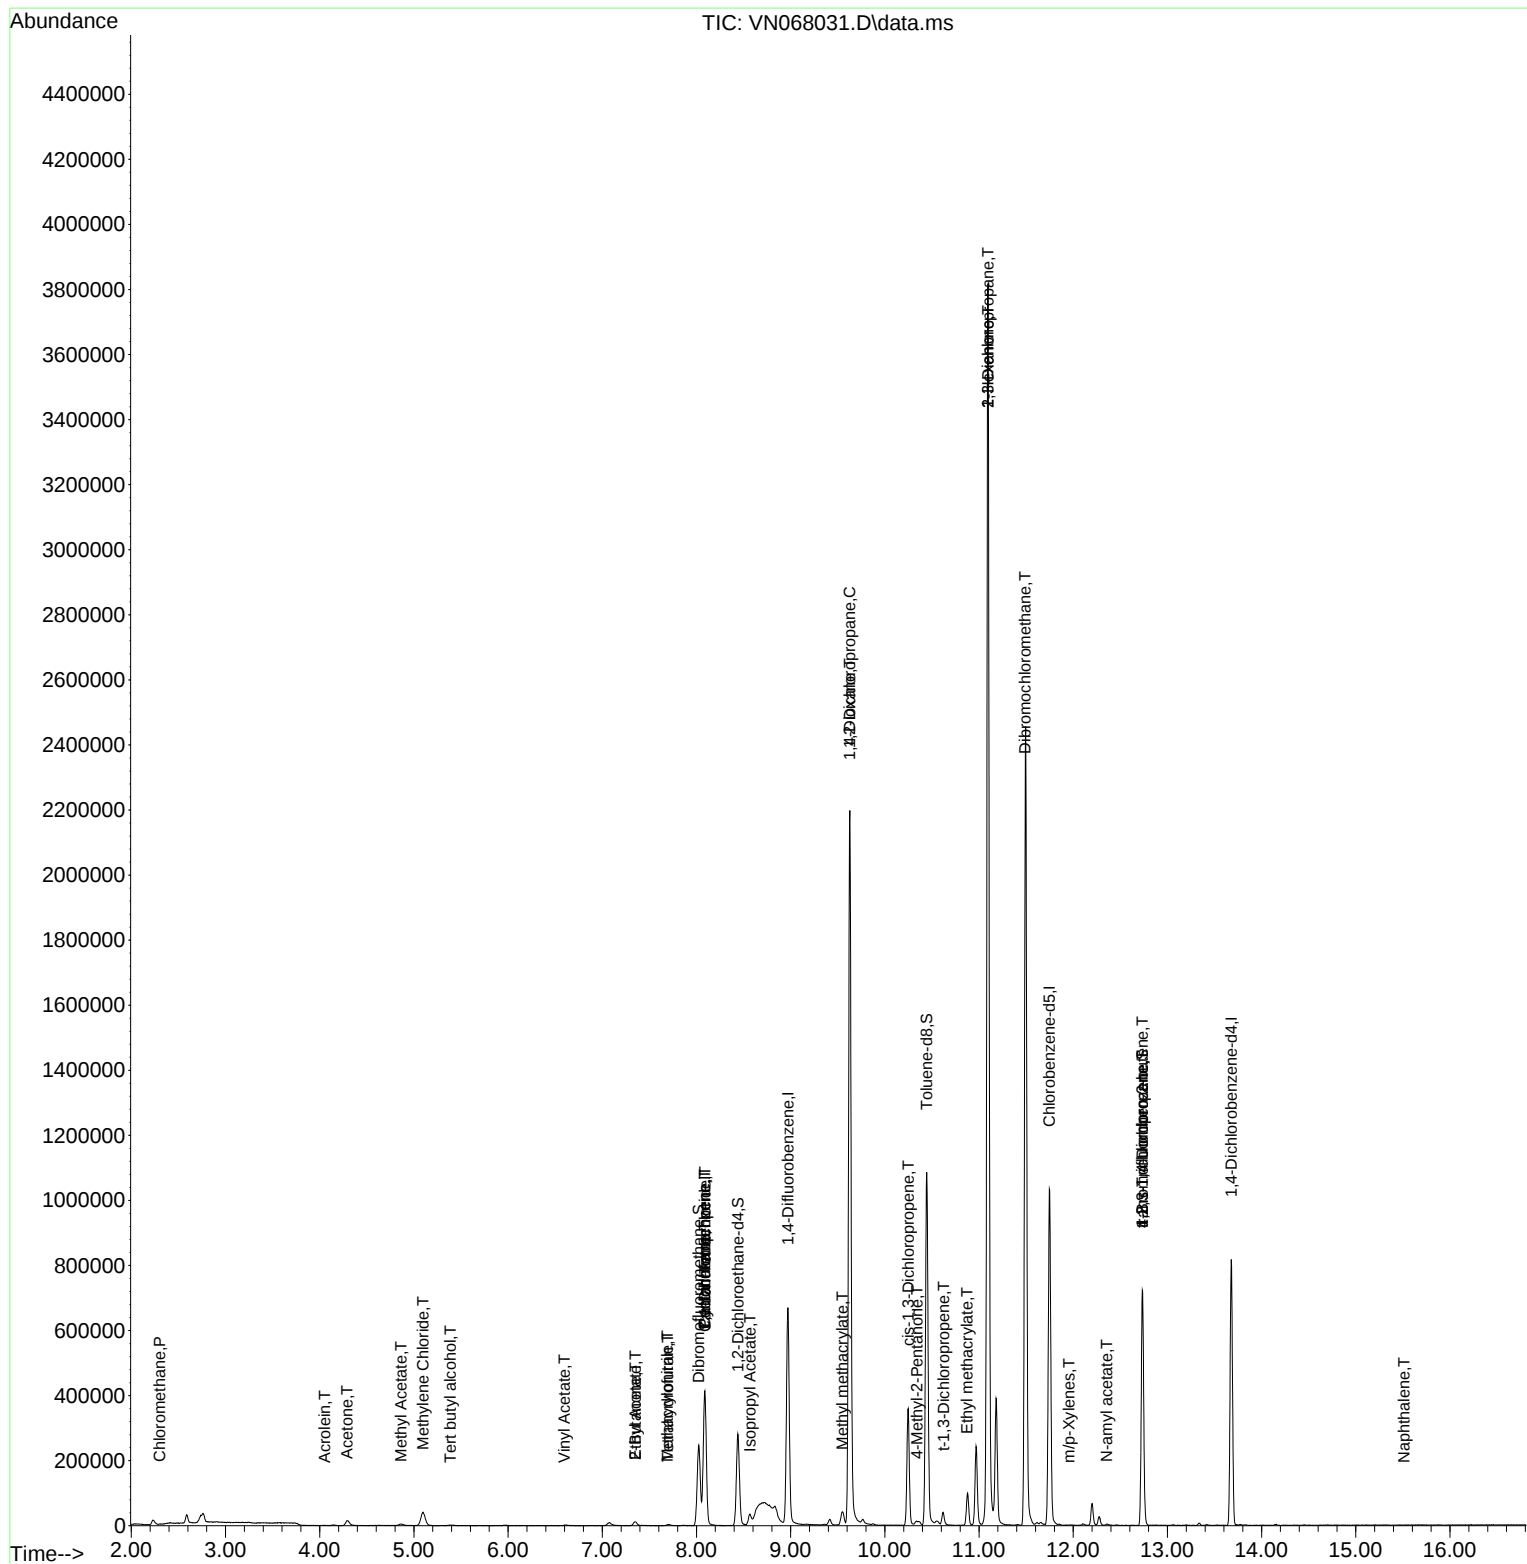




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 296999
Ion Ratio Lower Upper
168 100
99 65.6 62.9 94.3

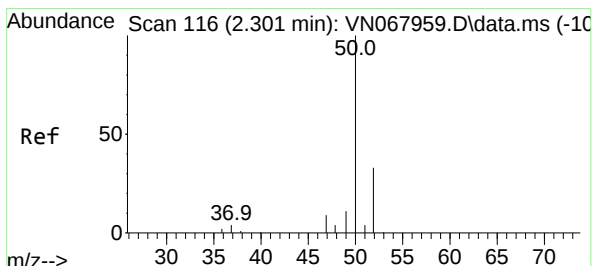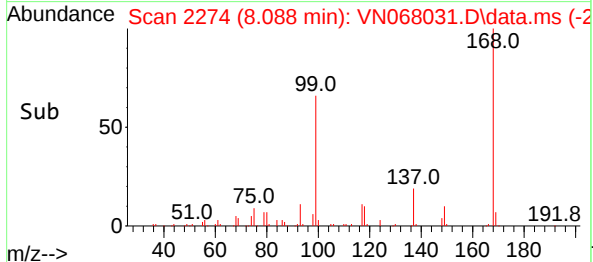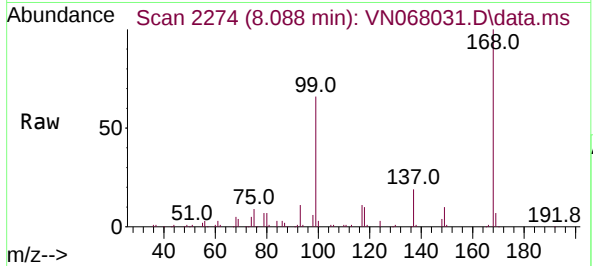

#3
Chloromethane
Concen: 0.207 ug/l
RT: 2.300 min Scan# 116
Delta R.T. -0.001 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 50 Resp: 781
Ion Ratio Lower Upper
50 100
52 36.8 25.6 38.4






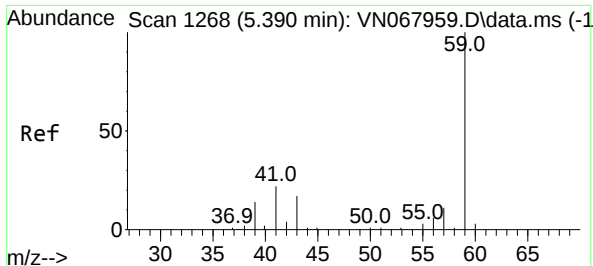


#11

Tert butyl alcohol
Concen: 1.408 ug/l
RT: 5.385 min Scan# 1266
Delta R.T. -0.005 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 59 Resp: 793
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

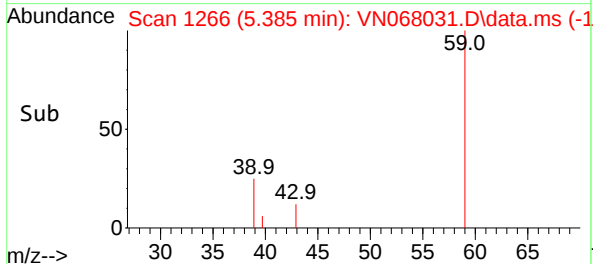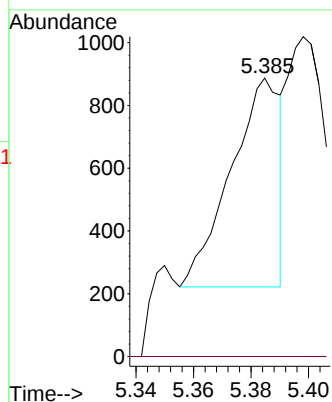


#13

Acrolein
Concen: 0.298 ug/l
RT: 4.052 min Scan# 769
Delta R.T. 0.011 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 56 Resp: 114
Ion Ratio Lower Upper
56 100
55 50.0 57.4 86.0#



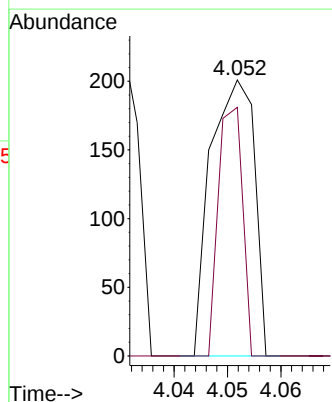



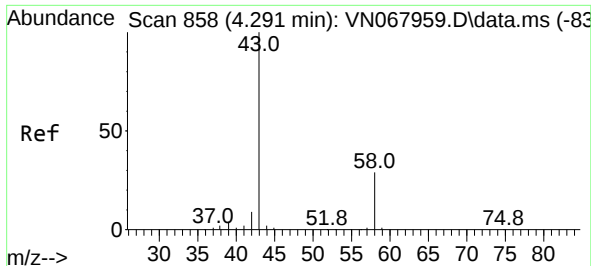

#16
Acetone
Concen: 18.804 ug/l
RT: 4.288 min Scan# 857
Delta R.T. -0.003 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 28848
Ion Ratio Lower Upper
43 100
58 28.6 21.2 31.8

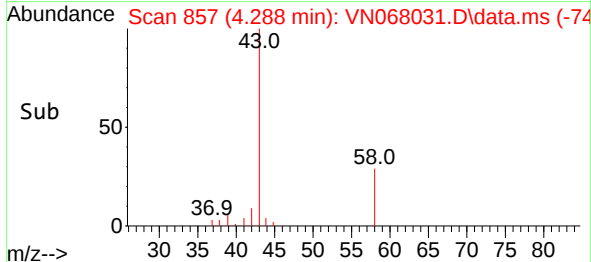

#18
Methyl Acetate
Concen: 1.280 ug/l
RT: 4.862 min Scan# 1071
Delta R.T. 0.005 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 43 Resp: 5089
Ion Ratio Lower Upper
43 100
74 26.2 17.4 26.0#


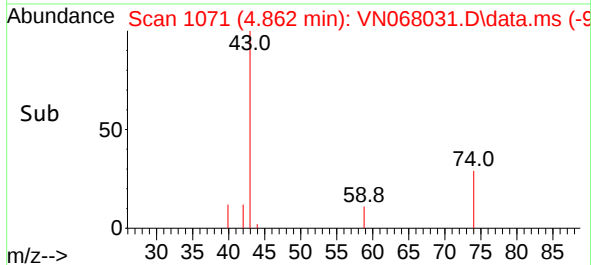

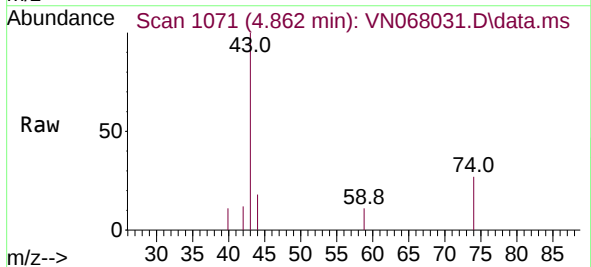


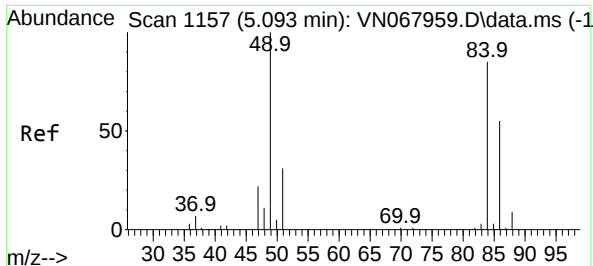

#20
Methylene Chloride
Concen: 9.064 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.002 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 84 Resp: 32934
Ion Ratio Lower Upper
84 100
49 116.7 110.9 166.3
51 32.5 32.6 49.0#
86 55.5 51.6 77.4

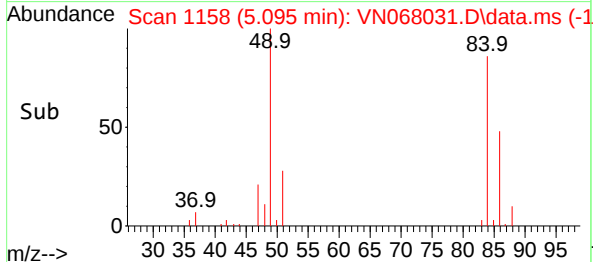

#23
Vinyl Acetate
Concen: 8.806 ug/l
RT: 6.594 min Scan# 1717
Delta R.T. 0.158 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 43 Resp: 55
Ion Ratio Lower Upper
43 100
86 0.0 7.3 10.9#




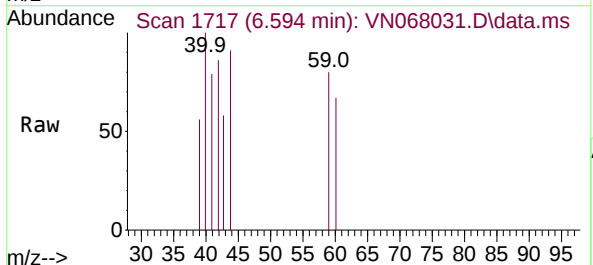




#25
2-Butanone
Concen: 9.259 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. 0.011 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 20607
Ion Ratio Lower Upper
43 100
72 26.6 19.7 29.5

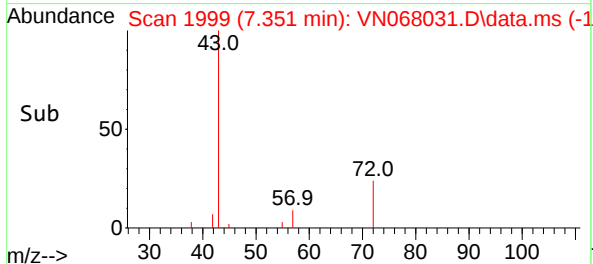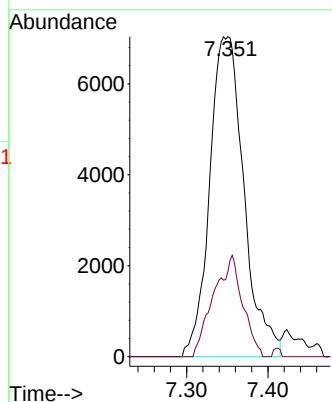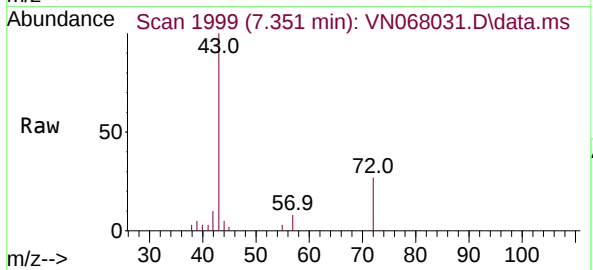

#29
Tetrahydrofuran
Concen: 1.000 ug/l
RT: 7.694 min Scan# 2127
Delta R.T. 0.005 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 42 Resp: 1425
Ion Ratio Lower Upper
42 100
72 53.4 32.8 49.2#
71 43.2 31.2 46.8


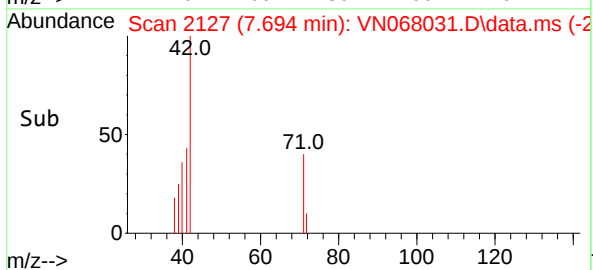
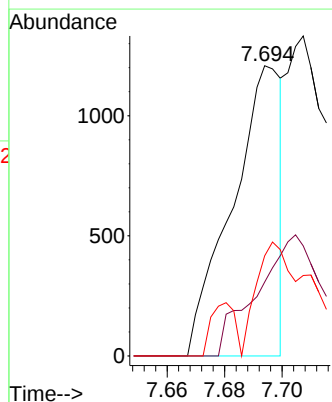



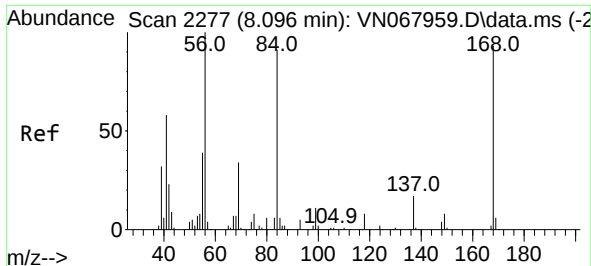

#31
Cyclohexane
Concen: 1.234 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.008 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 7652
Ion Ratio Lower Upper
56 100
69 147.6 27.3 40.9#
84 112.4 64.9 97.3#

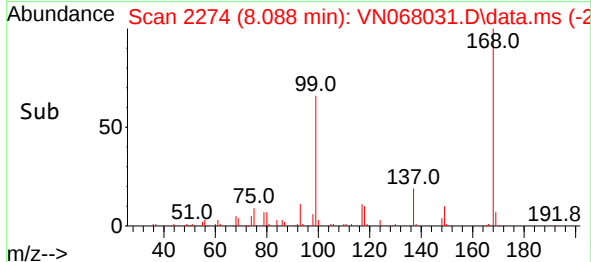

#33
1,2-Dichloroethane-d4
Concen: 56.039 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 65 Resp: 235618
Ion Ratio Lower Upper
65 100
67 51.1 0.0 98.6


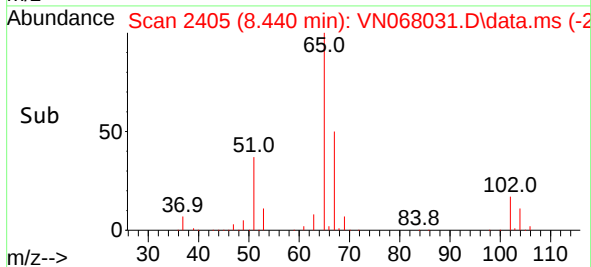

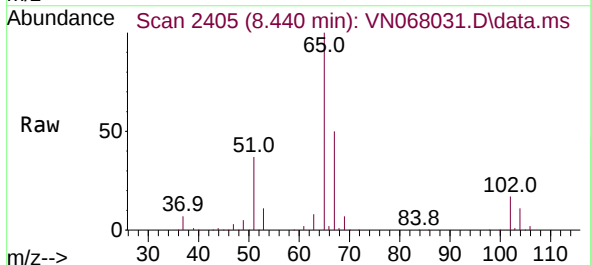


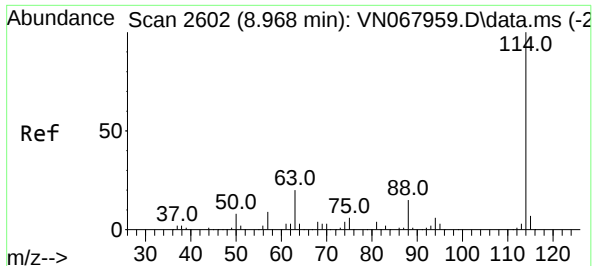

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:114 Resp: 591653
Ion Ratio Lower Upper
114 100
63 20.1 0.0 49.0
88 15.6 0.0 36.6

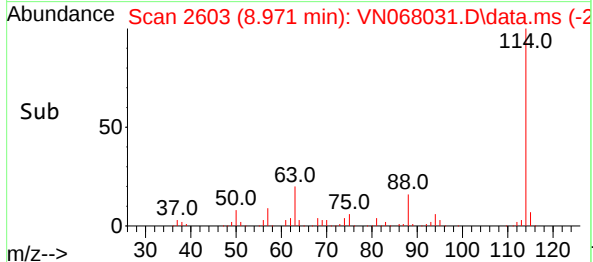

#35
Dibromofluoromethane
Concen: 52.067 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24


Tgt Ion:113 Resp: 179529
Ion Ratio Lower Upper
113 100
111 104.6 83.8 125.8
192 16.1 13.4 20.0

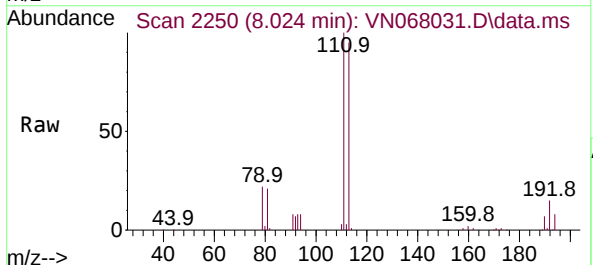



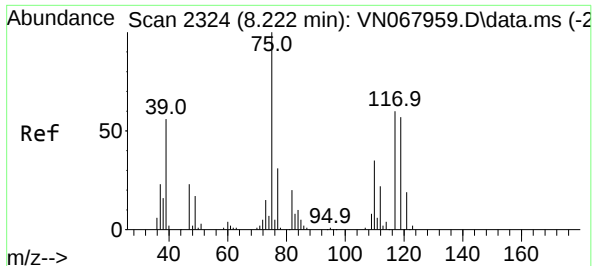


#36
1,1-Dichloropropene
Concen: 4.791 ug/l
RT: 8.085 min Scan# 2273
Delta R.T. -0.136 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 75 Resp: 26220
Ion Ratio Lower Upper
75 100
110 9.6 15.7 47.0#
77 0.0 24.6 37.0#

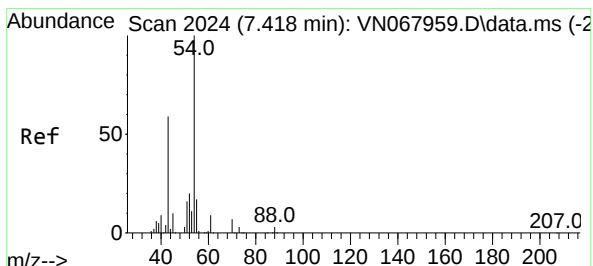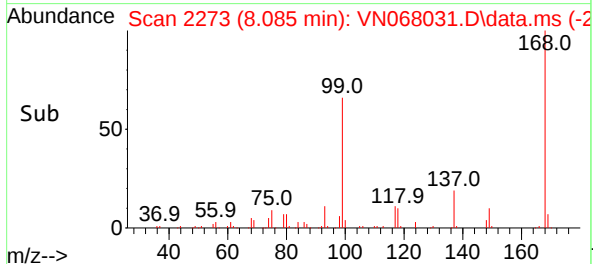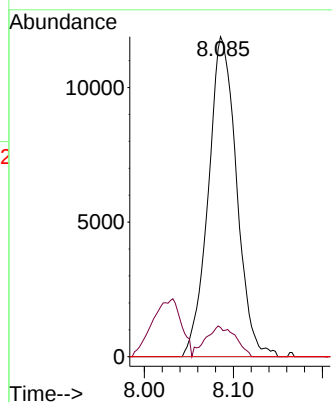

#37
Ethyl Acetate
Concen: 4.001 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. -0.067 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24


Tgt Ion: 43 Resp: 20607
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.1 8.1 12.1#





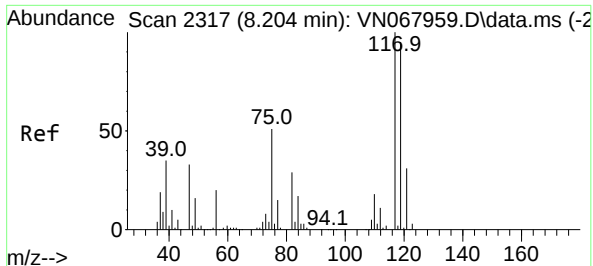


#38
Carbon Tetrachloride
Concen: 6.259 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.113 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion:117 Resp: 33688
Ion Ratio Lower Upper
117 100
119 5.2 75.4 113.2#
121 0.0 23.5 35.3#

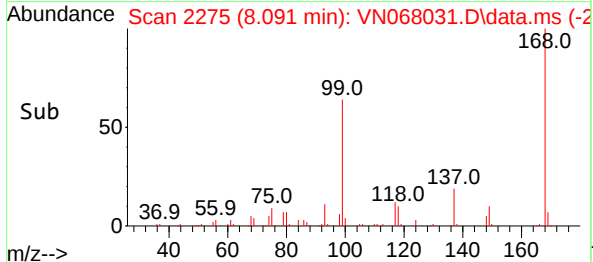

#41
Methacrylonitrile
Concen: 0.211 ug/l
RT: 7.691 min Scan# 2126
Delta R.T. 0.053 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 41 Resp: 518
Ion Ratio Lower Upper
41 100
39 96.3 47.6 71.4#
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#




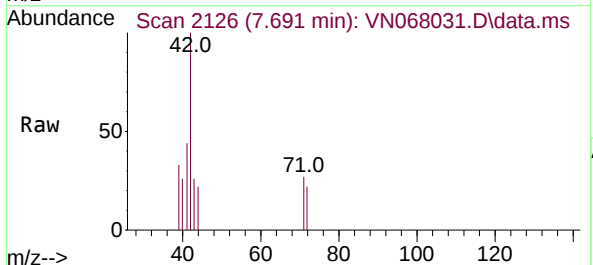


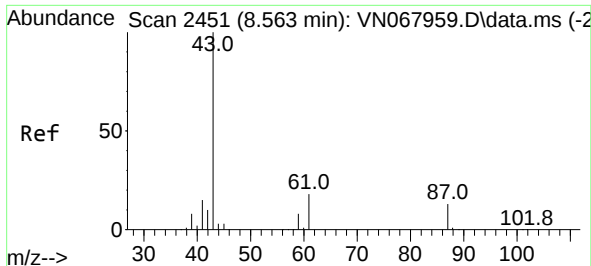

#43
Isopropyl Acetate
Concen: 4.760 ug/l
RT: 8.568 min Scan# 2453
Delta R.T. 0.005 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 40857
Ion Ratio Lower Upper
43 100
61 17.3 19.0 28.4#
87 12.2 9.5 14.3

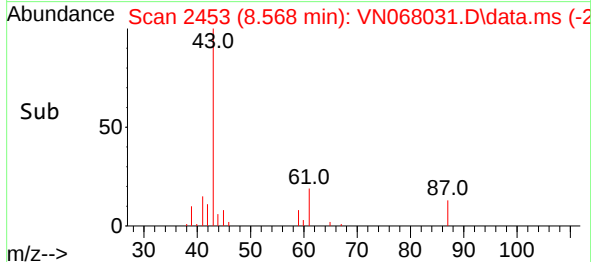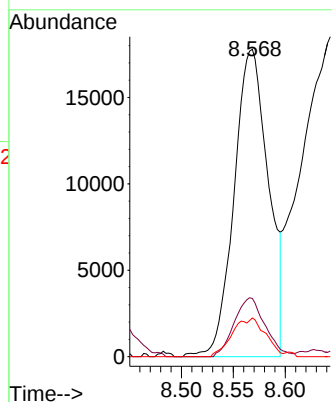

#45
1,2-Dichloropropane
Concen: 0.655 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.137 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 63 Resp: 2644
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#

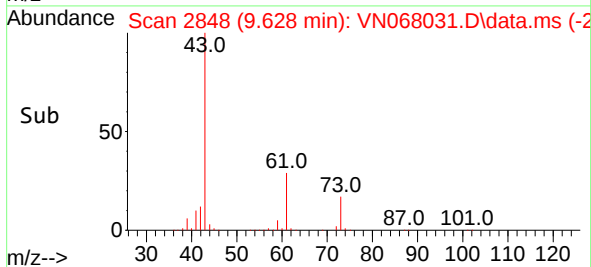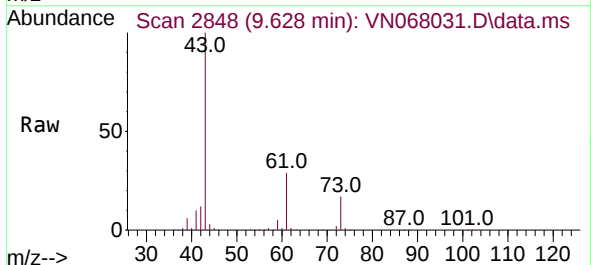

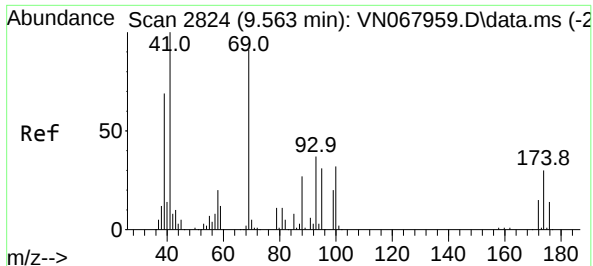

#48

Methyl methacrylate

Concen: 4.690 ug/l

RT: 9.547 min Scan# 2818

Delta R.T. -0.016 min

Lab File: VN068031.D

Acq: 5 Aug 2021 21:24





Tgt Ion: 41 Resp: 10699

Ion Ratio Lower Upper

41 100

69 0.0 64.6 96.8#

39 0.0 53.3 79.9#

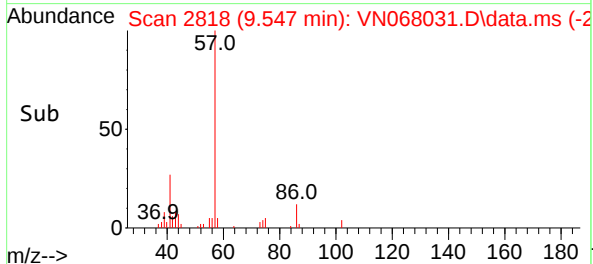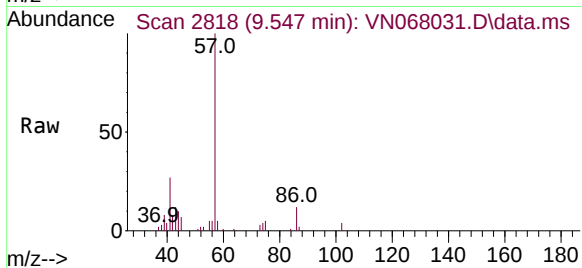

#49

1,4-Dioxane

Concen: 3.603 ug/l

RT: 9.625 min Scan# 2847

Delta R.T. 0.053 min

Lab File: VN068031.D

Acq: 5 Aug 2021 21:24




Tgt Ion: 88 Resp: 246


Ion Ratio Lower Upper

88 100

43 875811.0 28.8 43.2#

58 4247.6 60.4 90.6#


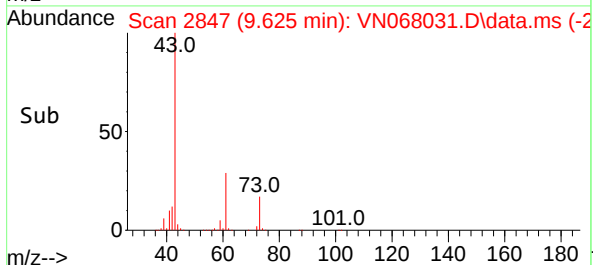
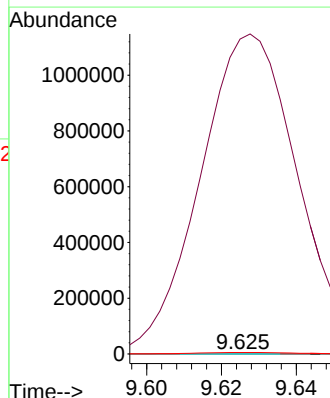
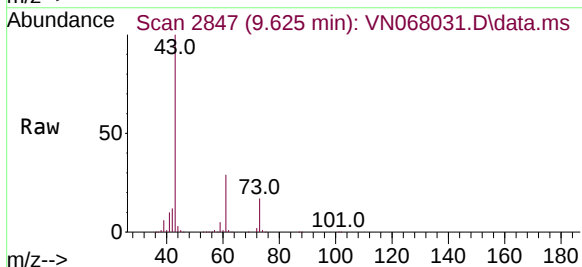




#50
Toluene-d8
Concen: 48.687 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 773011
Ion Ratio Lower Upper
98 100
100 64.1 51.7 77.5

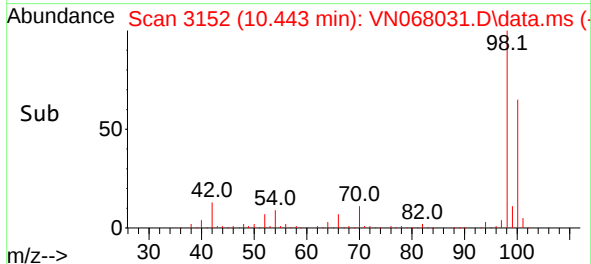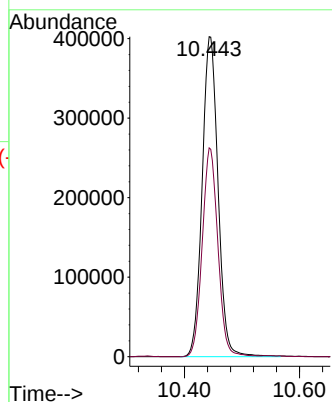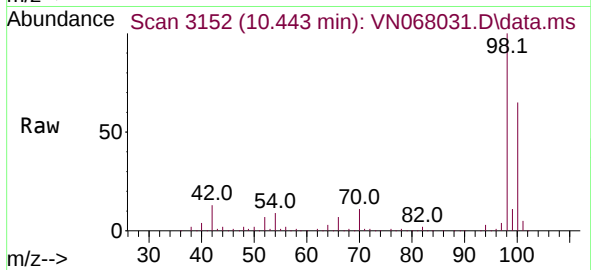

#51
4-Methyl-2-Pentanone
Concen: 13.468 ug/l
RT: 10.341 min Scan# 3114
Delta R.T. 0.008 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 43 Resp: 5934
Ion Ratio Lower Upper
43 100
58 56.6 28.6 43.0#


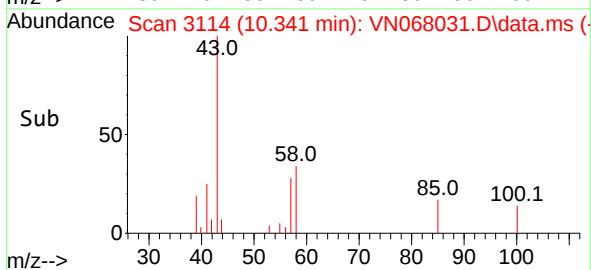
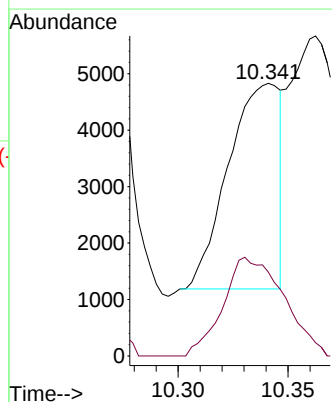
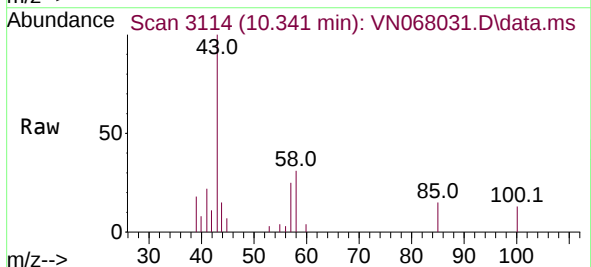


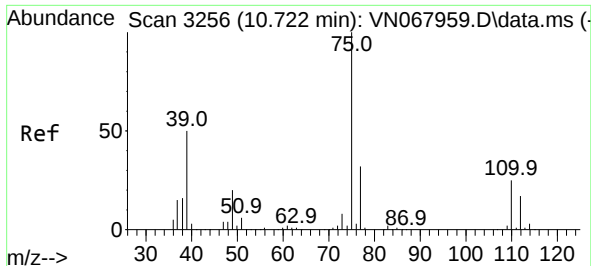

#53
t-1,3-Dichloropropene
Concen: 2.837 ug/l
RT: 10.623 min Scan# 3219
Delta R.T. -0.099 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 24
Ion Ratio Lower Upper
75 100
77 2.6 25.1 37.7#

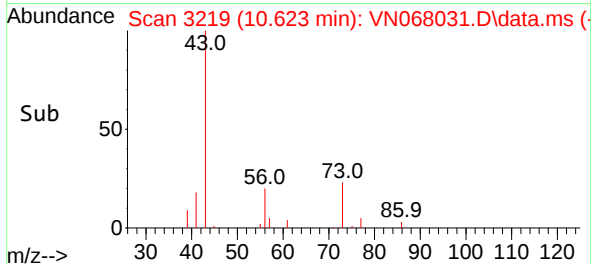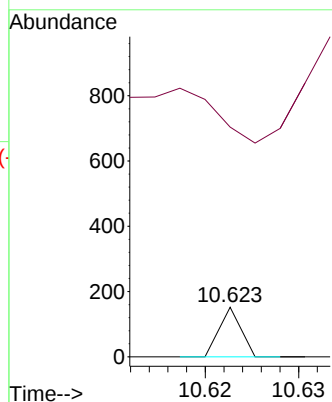

#54
cis-1,3-Dichloropropene
Concen: 10.621 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 75 Resp: 63514
Ion Ratio Lower Upper
75 100
77 0.7 24.6 37.0#
39 37.4 50.7 76.1#


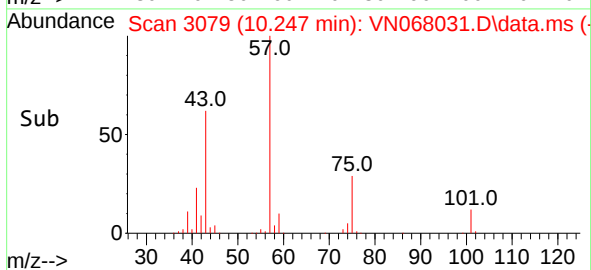

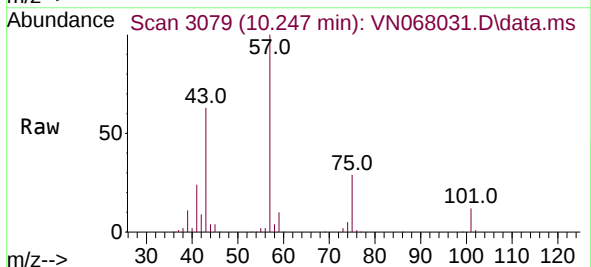




#56
Ethyl methacrylate
Concen: 3.150 ug/l
RT: 10.872 min Scan# 3312
Delta R.T. 0.107 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 69 Resp: 401
Ion Ratio Lower Upper
69 100
41 5353.4 58.6 88.0#
39 2664.8 38.3 57.5#

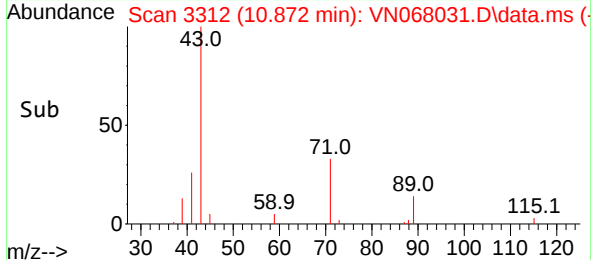

#57
1,3-Dichloropropane
Concen: 6.073 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 76 Resp: 40421
Ion Ratio Lower Upper
76 100
78 0.4 25.7 38.5#


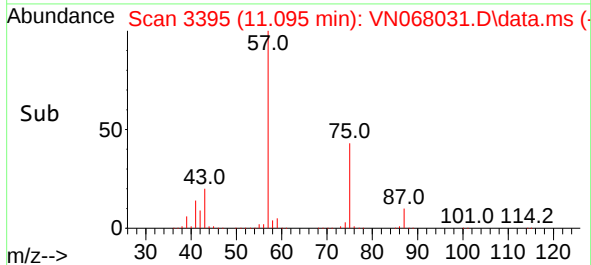

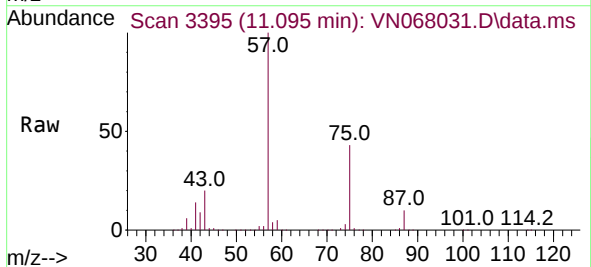




#59
2-Hexanone
Concen: 139.746 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 595364
Ion Ratio Lower Upper
43 100
58 18.7 24.7 74.1#

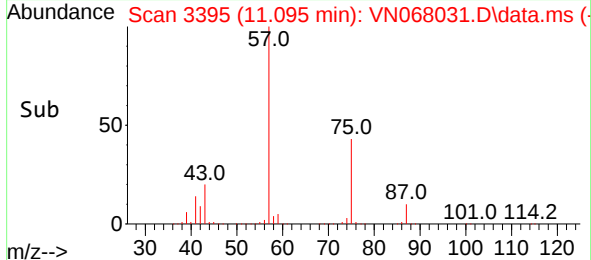

#60
Dibromochloromethane
Concen: 3.361 ug/l
RT: 11.489 min Scan# 3542
Delta R.T. 0.249 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion:129 Resp: 321
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#


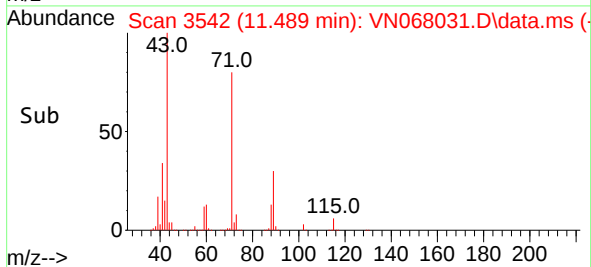

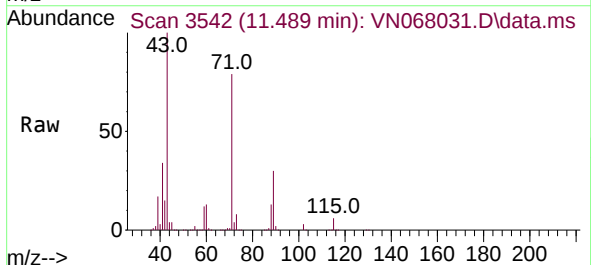


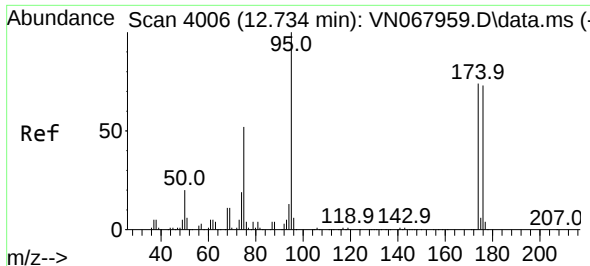

#62
4-Bromofluorobenzene
Concen: 45.200 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.001 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 260181
Ion Ratio Lower Upper
95 100
174 73.1 0.0 122.0
176 69.3 0.0 117.6

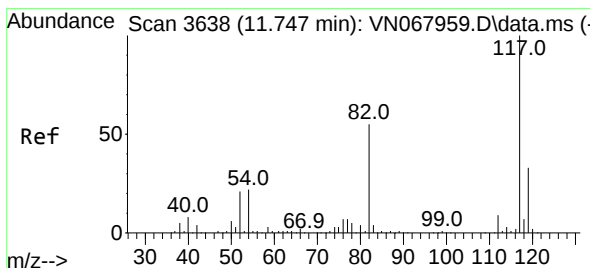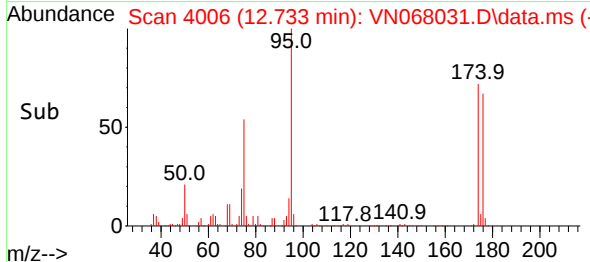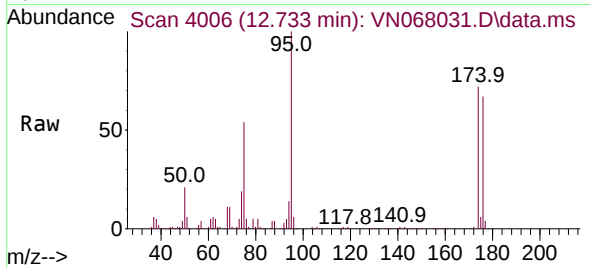

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.001 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion: 117 Resp: 623063
Ion Ratio Lower Upper
117 100
82 54.3 53.1 79.7
119 31.1 25.5 38.3


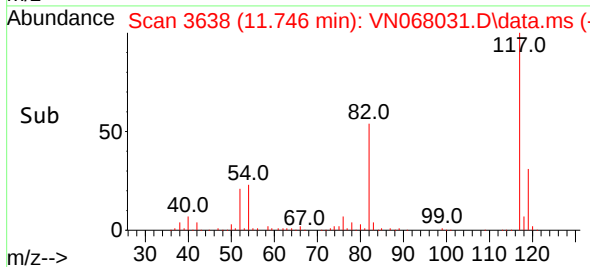

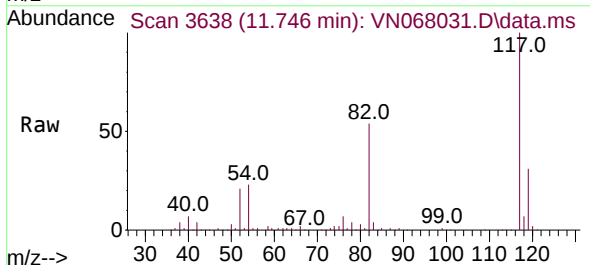




#68
m/p-Xylenes
Concen: 4.067 ug/l
RT: 11.956 min Scan# 3716
Delta R.T. -0.000 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 54
Ion Ratio Lower Upper
106 100
91 540.7 180.6 270.8#

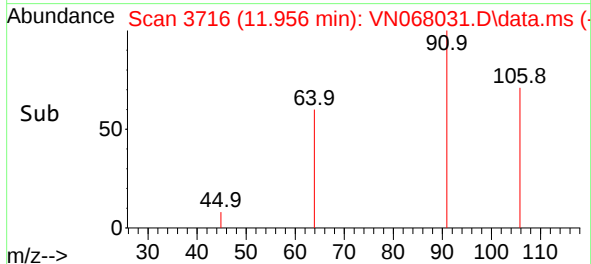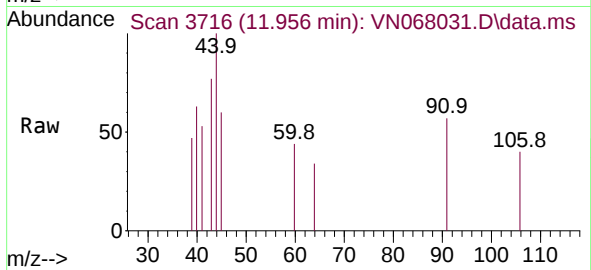

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.002 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

Tgt Ion:152 Resp: 214002
Ion Ratio Lower Upper
152 100
115 62.4 36.1 108.5
150 161.1 0.0 351.8


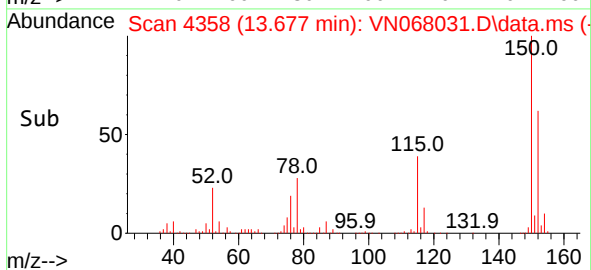

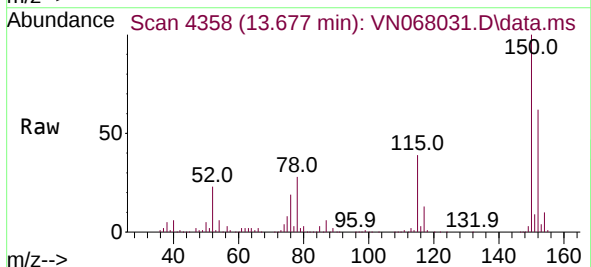


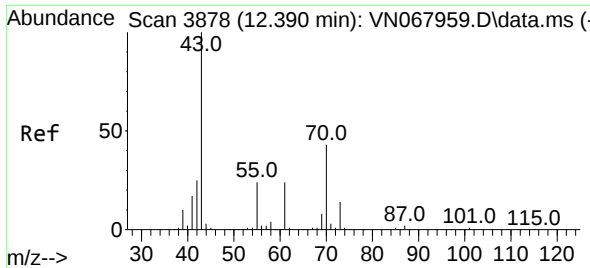

#74
N-amy1 acetate
Concen: 0.496 ug/l
RT: 12.355 min Scan# 3865
Delta R.T. -0.035 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43	Resp: 3008
Ion Ratio	Lower Upper
43 100	
70 0.0	29.4 44.2#
55 5.6	17.0 25.4#
61 0.0	17.6 26.4#

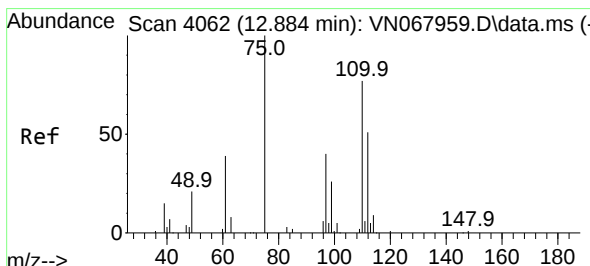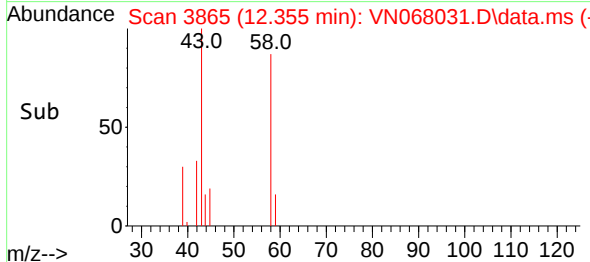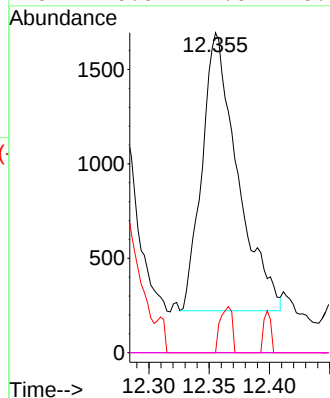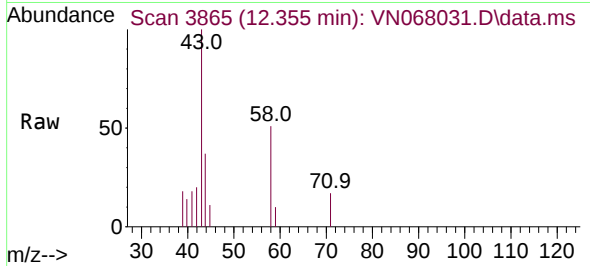

#76
1,2,3-Trichloropropane
Concen: 32.542 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24


Tgt Ion: 75	Resp: 139857
Ion Ratio	Lower Upper
75 100	
77 1.0	0.0 0.0#

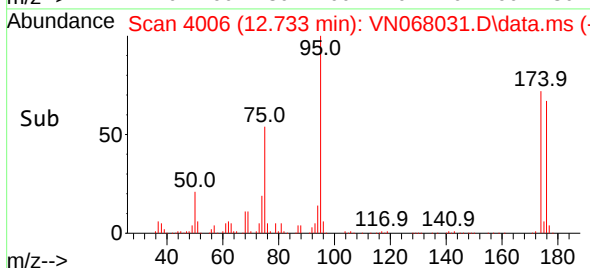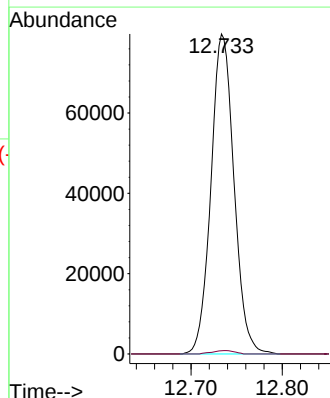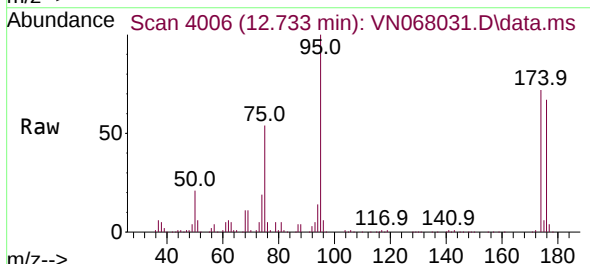



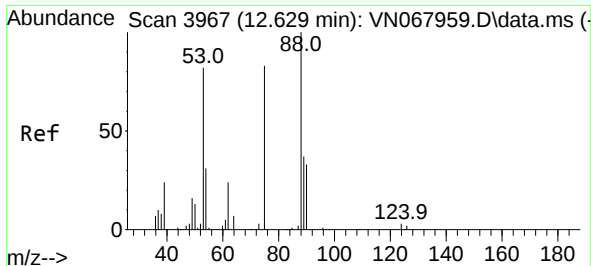


#81
trans-1,4-Dichloro-2-butene
Concen: 87.386 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24


Instrument :
MSVOA_N
ClientSampled :

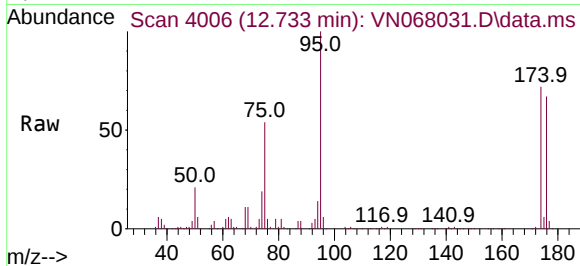

Tgt Ion: 75 Resp: 139857
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

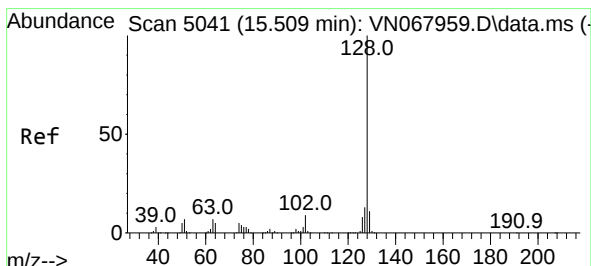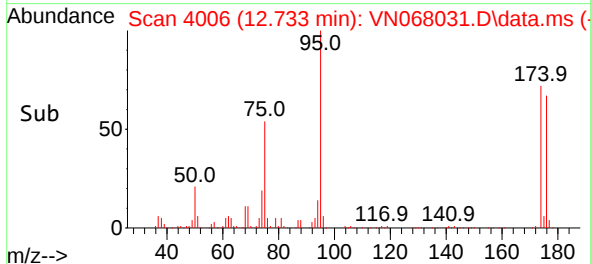

#95
Naphthalene
Concen: 3.167 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.000 min
Lab File: VN068031.D
Acq: 5 Aug 2021 21:24

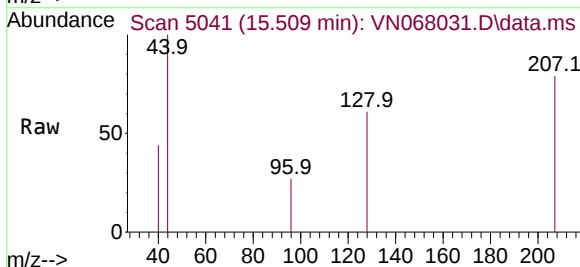

Tgt Ion:128 Resp: 451
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.6 12.8#

