

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080521\
 Data File : VN068022.D
 Acq On : 5 Aug 2021 17:45
 Operator : JC/MD
 Sample : M2940-09 .5PPB MDL
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MDL-WATER-03-QT3-2021DL

Manual Integrations
 APPROVED

MMDadoda
 8/6/2021 5:42:53 PM

Quant Time: Aug 06 02:09:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 06 02:07:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	335017	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	665836	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	595834	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	201461	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	279177	58.864	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 117.720%			
35) Dibromofluoromethane	8.024	113	202746	52.249	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 104.500%			
50) Toluene-d8	10.443	98	792338	50.452	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 100.900%			
62) 4-Bromofluorobenzene	12.733	95	243006	44.669	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 89.340%			
Target Compounds					Qvalue	
3) Chloromethane	2.301	50	1408	0.330	ug/l #	57
5) Bromomethane	2.842	94	2486	0.419	ug/l #	72
6) Chloroethane	3.006	64	1203	0.233	ug/l #	56
11) Tert butyl alcohol	5.398	59	141	0.222	ug/l #	71
13) Acrolein	4.033	56	1036m	2.402	ug/l	
14) Allyl chloride	4.832	41	1452m	0.269	ug/l	
15) Acrylonitrile	5.559	53	1584m	0.889	ug/l	
16) Acetone	4.293	43	3383m	1.955	ug/l	
17) Carbon Disulfide	4.527	76	2154	0.234	ug/l #	74
18) Methyl Acetate	4.864	43	7817	1.752	ug/l #	65
20) Methylene Chloride	5.090	84	6607	1.487	ug/l #	84
23) Vinyl Acetate	6.436	43	6730	0.675	ug/l #	84
25) 2-Butanone	7.345	43	2331m	0.928	ug/l	
28) Bromochloromethane	7.654	49	1485m	0.450	ug/l	
29) Tetrahydrofuran	7.694	42	1493m	0.929	ug/l	
30) Chloroform	7.828	83	1859	0.242	ug/l	97
31) Cyclohexane	8.088	56	10102	1.444	ug/l #	32
38) Carbon Tetrachloride	8.193	117	1223m	0.202	ug/l	
42) 1,2-Dichloroethane	8.536	62	1767m	0.262	ug/l	
48) Methyl methacrylate	9.563	41	949	0.228	ug/l #	83
49) 1,4-Dioxane	9.574	88	167	2.174	ug/l #	12
51) 4-Methyl-2-Pentanone	10.336	43	5265	0.884	ug/l	98
58) 2-Chloroethyl Vinyl ether	10.043	63	1867	1.688	ug/l	95
59) 2-Hexanone	11.089	43	4175	0.976	ug/l	91
68) m/p-Xylenes	11.961	106	2294	0.284	ug/l	89
74) N-amyl acetate	12.387	43	1328	0.232	ug/l #	68
75) 1,1,2,2-Tetrachloroethane	12.827	83	1042	0.210	ug/l #	96
76) 1,2,3-Trichloropropane	12.884	75	1099m	0.272	ug/l	
79) 2-Chlorotoluene	13.010	91	2416	0.214	ug/l	89
82) 4-Chlorotoluene	13.109	91	2289	0.202	ug/l	98
88) 1,4-Dichlorobenzene	13.696	146	1483m	0.217	ug/l	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080521\
Data File : VN068022.D
Acq On : 5 Aug 2021 17:45
Operator : JC/MD
Sample : M2940-09 .5PPB MDL
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL

Manual Integrations
APPROVED

MMDadoda
8/6/2021 5:42:53 PM

Quant Time: Aug 06 02:09:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 06 02:07:57 2021
Response via : Initial Calibration

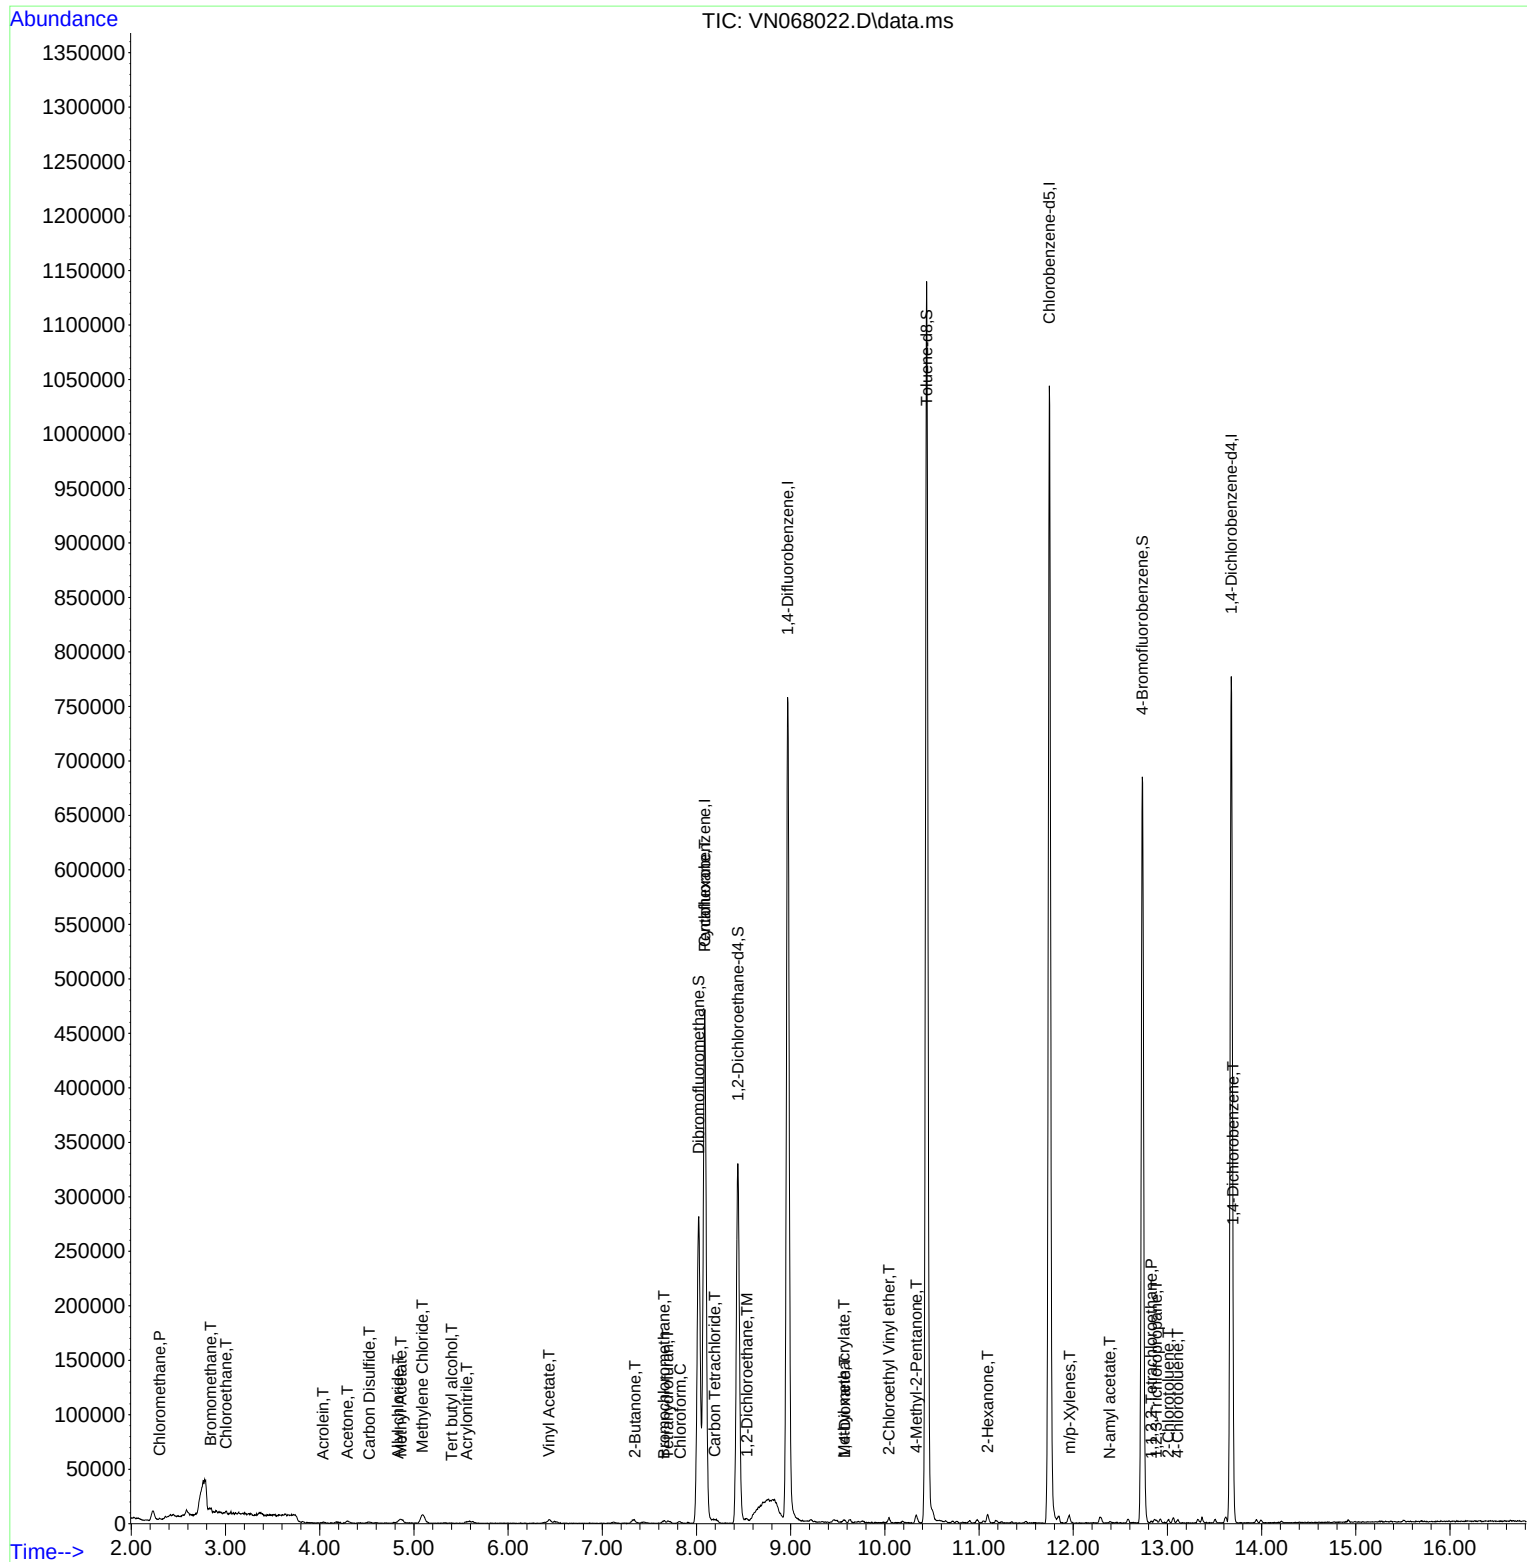







#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 168 Resp: 335017
Ion Ratio Lower Upper
168 100
99 63.9 62.9 94.3

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:42:53 PM

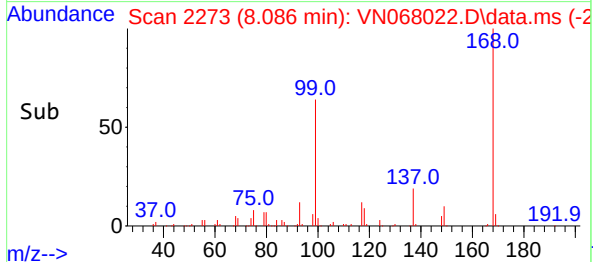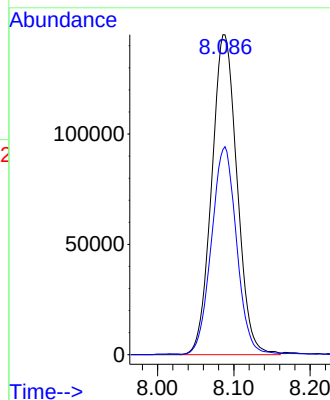

#3
Chloromethane
Concen: 0.330 ug/l
RT: 2.301 min Scan# 116
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45


Tgt Ion: 50 Resp: 1408
Ion Ratio Lower Upper
50 100
52 56.0 25.6 38.4#

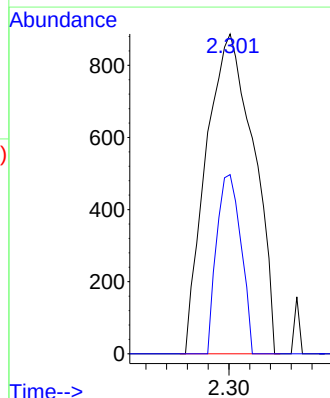



#5
Bromomethane
Concen: 0.419 ug/l
RT: 2.842 min Scan# 318
Delta R.T. 0.002 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL



Tgt Ion: 94 Resp: 2486
Ion Ratio Lower Upper
94 100
96 65.2 73.7 110.5#




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:42:53 PM

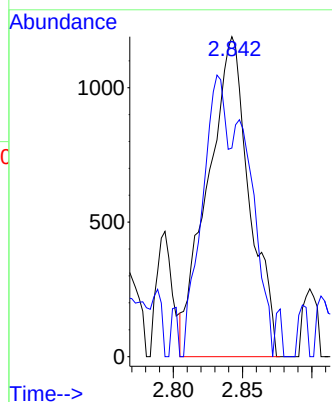

#6
Chloroethane
Concen: 0.233 ug/l
RT: 3.006 min Scan# 379
Delta R.T. -0.005 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 64 Resp: 1203
Ion Ratio Lower Upper
64 100
66 55.3 24.7 37.1#

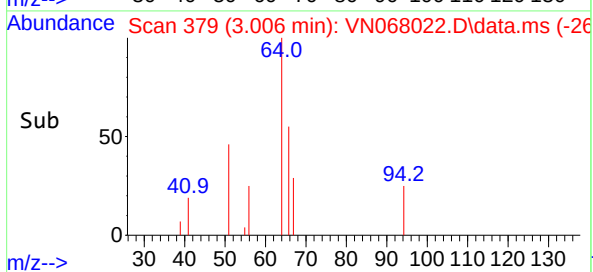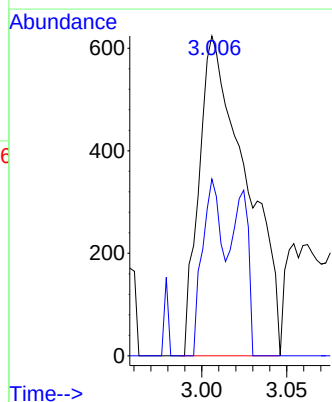







#11
Tert butyl alcohol
Concen: 0.222 ug/l
RT: 5.398 min Scan# 1271
Delta R.T. 0.008 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 59 Resp: 141
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:42:53 PM

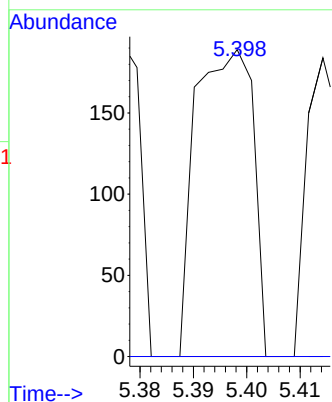

#13
Acrolein
Concen: 2.402 ug/l m
RT: 4.033 min Scan# 762
Delta R.T. -0.008 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 56 Resp: 1036
Ion Ratio Lower Upper
56 100
55 22.0 57.4 86.0#

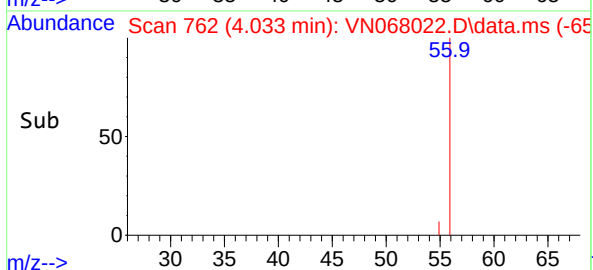



#14





Allyl chloride
Concen: 0.269 ug/l m
RT: 4.832 min Scan# 1060
Delta R.T. -0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion:	41	Resp:	1452
Ion	Ratio	Lower	Upper
41	100		
39	20.0	60.9	91.3#
76	0.0	24.3	36.5#

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL

Manual Integrations
APPROVED




MMDadoda
8/6/2021 5:42:53 PM

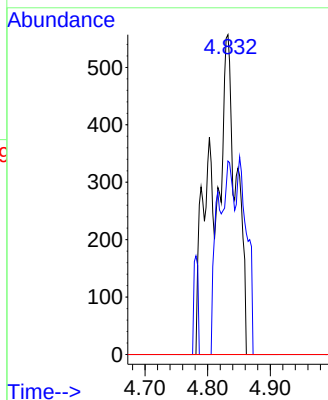


#15

Acrylonitrile
Concen: 0.889 ug/l m
RT: 5.559 min Scan# 1331
Delta R.T. 0.002 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45


Tgt Ion:	53	Resp:	1584
Ion	Ratio	Lower	Upper
53	100		
52	9.9	66.2	99.2#
51	18.2	30.2	45.4#

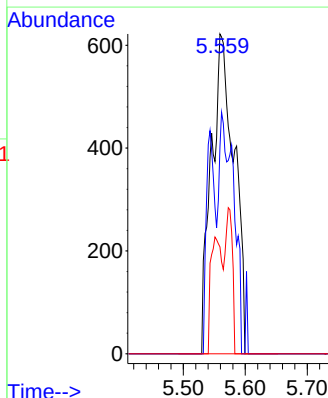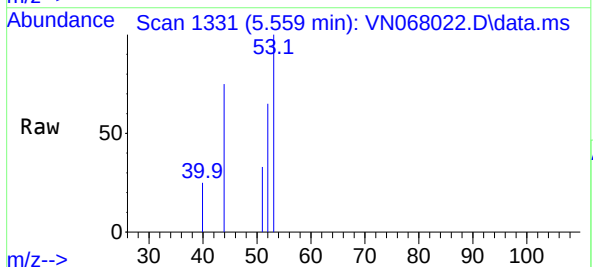



#16
Acetone
Concen: 1.955 ug/l m
RT: 4.293 min Scan# 859
Delta R.T. 0.002 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL




Tgt Ion: 43 Resp: 3383
Ion Ratio Lower Upper
43 100
58 30.2 21.2 31.8

Manual Integrations
APPROVED



MMDadoda
8/6/2021 5:42:53 PM

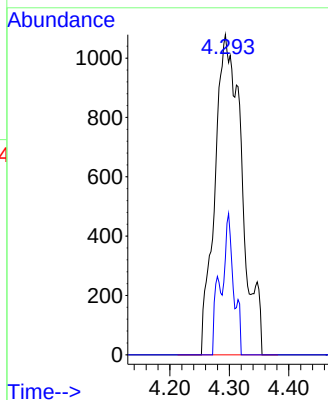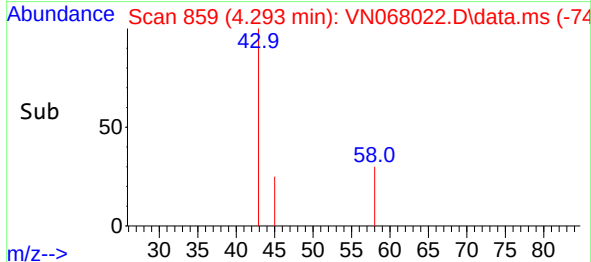


#17
Carbon Disulfide
Concen: 0.234 ug/l
RT: 4.527 min Scan# 946
Delta R.T. 0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

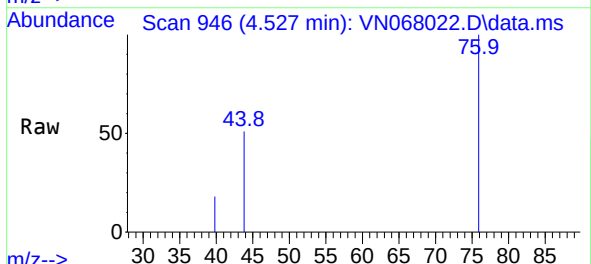

Tgt Ion: 76 Resp: 2154
Ion Ratio Lower Upper
76 100
78 0.0 7.7 11.5#

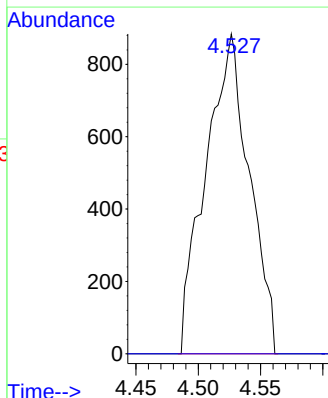







#18
Methyl Acetate
Concen: 1.752 ug/l
RT: 4.864 min Scan# 1072
Delta R.T. 0.007 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 43 Resp: 7817
Ion Ratio Lower Upper
43 100
74 5.2 17.4 26.0#

Instrument :
MSVOA_N
ClientSampleID :
MDL-WATER-03-QT3-2021DL




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:42:53 PM



#20
Methylene Chloride
Concen: 1.487 ug/l
RT: 5.090 min Scan# 1156
Delta R.T. -0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45


Tgt Ion: 84 Resp: 6607
Ion Ratio Lower Upper
84 100
49 116.0 110.9 166.3
51 32.4 32.6 49.0#
86 55.8 51.6 77.4

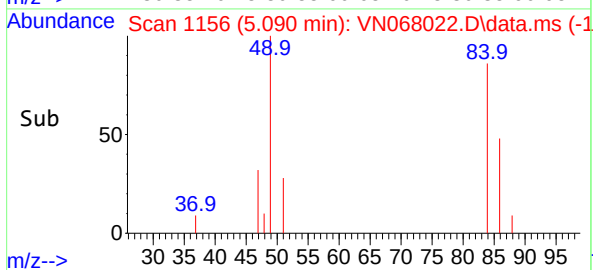



#23
 Vinyl Acetate
 Concen: 0.675 ug/l
 RT: 6.436 min Scan# 1658
 Delta R.T. 0.000 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45




Instrument :
 MSVOA_N
 ClientSampleId :
 MDL-WATER-03-QT3-2021DL



Tgt Ion: 43 Resp: 6730
 Ion Ratio Lower Upper
 43 100
 86 14.8 7.3 10.9#




Manual Integrations
 APPROVED


MMDadoda
 8/6/2021 5:42:53 PM

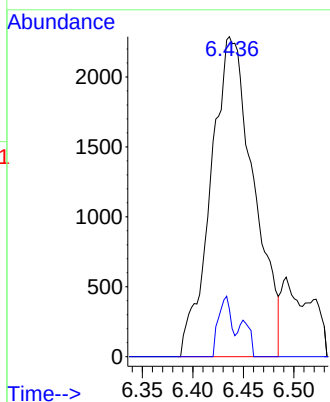

#25
 2-Butanone
 Concen: 0.928 ug/l m
 RT: 7.345 min Scan# 1997
 Delta R.T. 0.005 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45


Tgt Ion: 43 Resp: 2331
 Ion Ratio Lower Upper
 43 100
 72 34.8 19.7 29.5#

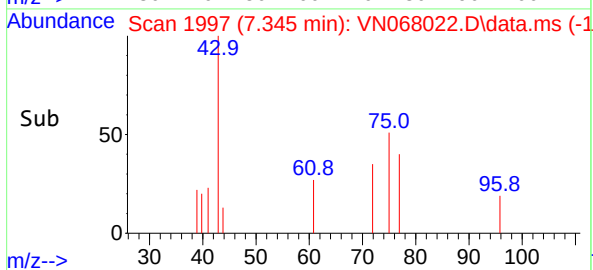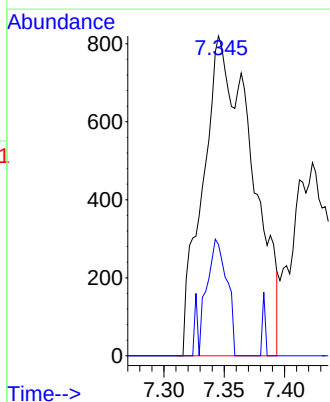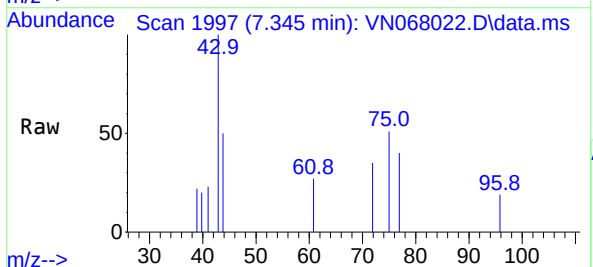

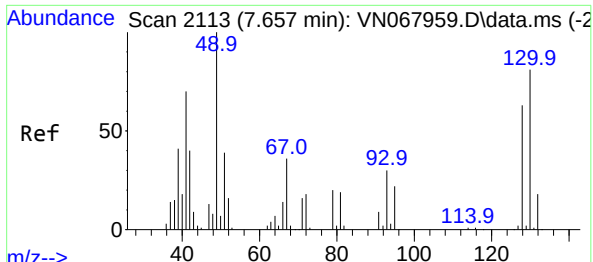

#28
Bromochloromethane
Concen: 0.450 ug/l m
RT: 7.654 min Scan# 2112
Delta R.T. -0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45




Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL

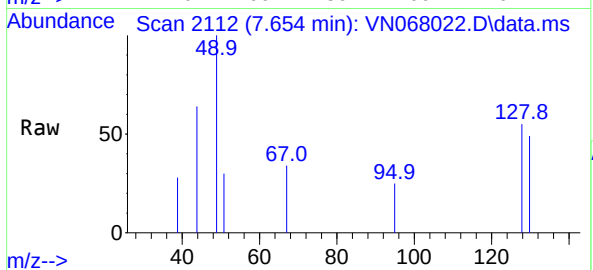


Tgt Ion: 49 Resp: 1485
Ion Ratio Lower Upper
49 100
129 0.0 0.0 3.8
130 56.4 49.7 74.5

Manual Integrations
APPROVED



MMDadoda
8/6/2021 5:42:53 PM

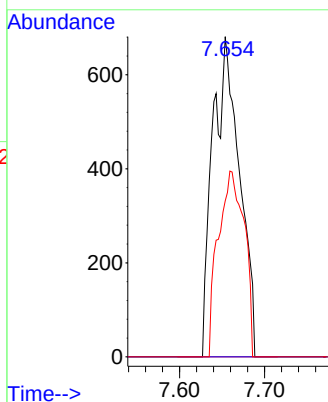


#29
Tetrahydrofuran
Concen: 0.929 ug/l m
RT: 7.694 min Scan# 2127
Delta R.T. 0.005 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

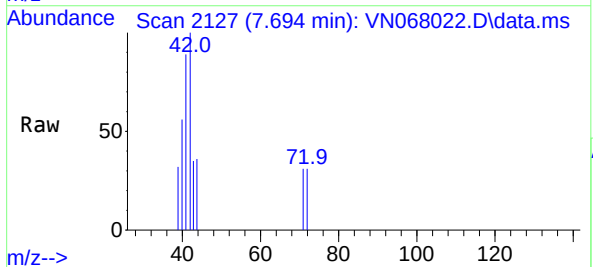

Tgt Ion: 42 Resp: 1493
Ion Ratio Lower Upper
42 100
72 32.0 32.8 49.2#
71 0.0 31.2 46.8#

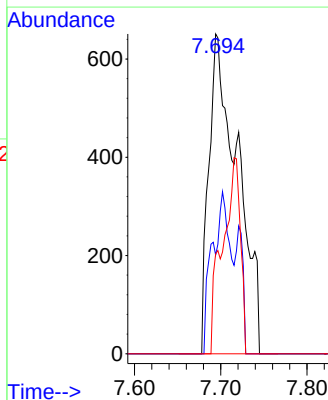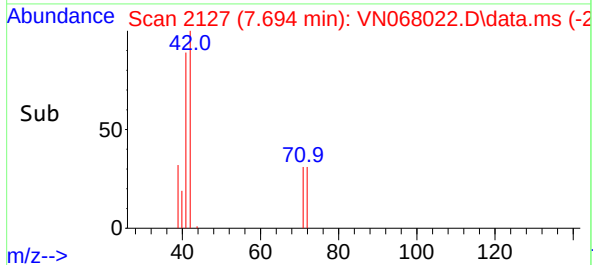



#30





Chloroform
Concen: 0.242 ug/l
RT: 7.828 min Scan# 2177
Delta R.T. 0.008 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 83 Resp: 1859
Ion Ratio Lower Upper
83 100
85 62.1 51.5 77.3

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL

Manual Integrations
APPROVED




MMDadoda
8/6/2021 5:42:53 PM

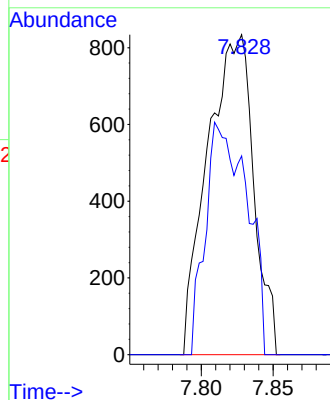


#31

Cyclohexane
Concen: 1.444 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.008 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 56 Resp: 10102
Ion Ratio Lower Upper
56 100
69 130.0 27.3 40.9#
84 104.8 64.9 97.3#

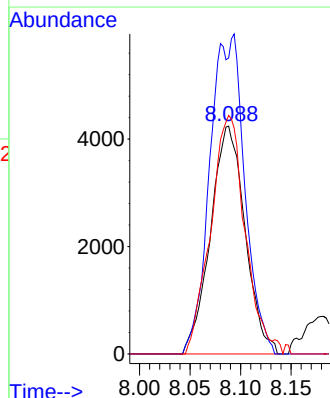







#33
1,2-Dichloroethane-d4
Concen: 58.864 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 65 Resp: 279177
Ion Ratio Lower Upper
65 100
67 51.4 0.0 98.6

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:42:53 PM




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 114 Resp: 665836
Ion Ratio Lower Upper
114 100
63 20.4 0.0 49.0
88 14.8 0.0 36.6






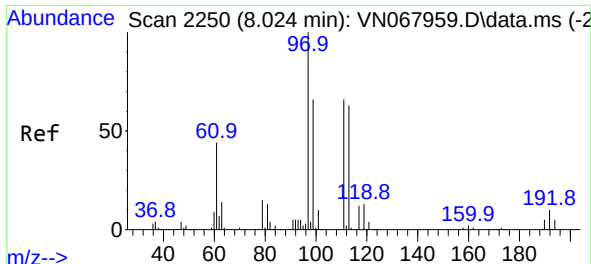


#35
Dibromofluoromethane
Concen: 52.249 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45





Tgt Ion:113 Resp: 202746
Ion Ratio Lower Upper
113 100
111 104.1 83.8 125.8
192 15.9 13.4 20.0



#38
Carbon Tetrachloride
Concen: 0.202 ug/l m
RT: 8.193 min Scan# 2313
Delta R.T. -0.011 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

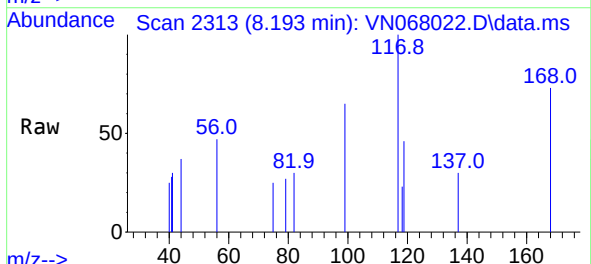


Tgt Ion:117 Resp: 1223
Ion Ratio Lower Upper
117 100
119 46.0 75.4 113.2#
121 0.0 23.5 35.3#

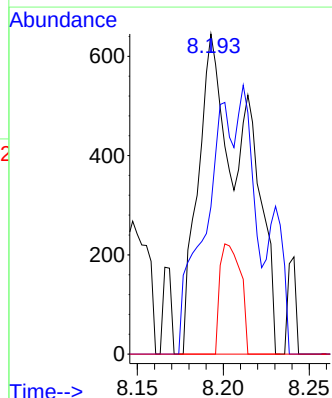

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL

Manual Integrations
APPROVED

MMDadoda
8/6/2021 5:42:53 PM



#42

1,2-Dichloroethane

Concen: 0.262 ug/l m

RT: 8.536 min Scan# 2441

Delta R.T. 0.005 min

Lab File: VN068022.D





Acq: 5 Aug 2021 17:45

Tgt Ion: 62 Resp: 1767

Ion Ratio Lower Upper

62 100

98 0.0 0.0 14.2

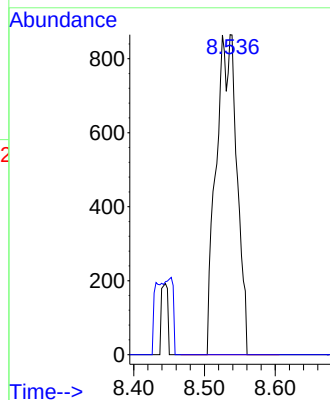

#48

Methyl methacrylate

Concen: 0.228 ug/l

RT: 9.563 min Scan# 2824

Delta R.T. 0.000 min

Lab File: VN068022.D

Acq: 5 Aug 2021 17:45




Tgt Ion: 41 Resp: 949

Ion Ratio Lower Upper

41 100

69 66.8 64.6 96.8

39 51.2 53.3 79.9#

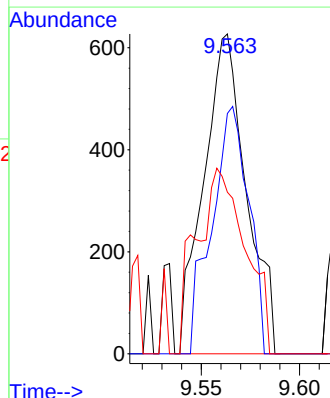

Instrument :

MSVOA_N


ClientSampleID :

MDL-WATER-03-QT3-2021DL

Manual Integrations

APPROVED

MMDadoda
8/6/2021 5:42:53 PM



#49

1,4-Dioxane

Concen: 2.174 ug/l

RT: 9.574 min Scan# 2828

Delta R.T. 0.002 min

Lab File: VN068022.D

Acq: 5 Aug 2021 17:45

Tgt Ion: 88 Resp: 167

Ion Ratio Lower Upper

88 100

43 86.8 28.8 43.2#

58 0.0 60.4 90.6#

Instrument :

MSVOA_N

ClientSampleId :





MDL-WATER-03-QT3-2021DL

Manual Integrations

APPROVED

MMDadoda

8/6/2021 5:42:53 PM

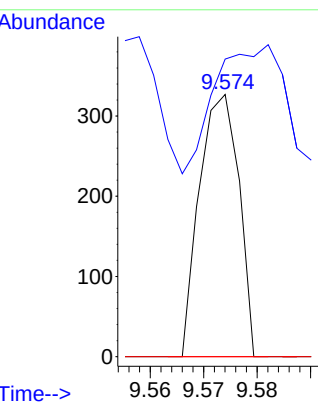

#50

Toluene-d8

Concen: 50.452 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. -0.000 min

Lab File: VN068022.D




Acq: 5 Aug 2021 17:45


Tgt Ion: 98 Resp: 792338

Ion Ratio Lower Upper

98 100

100 64.0 51.7 77.5

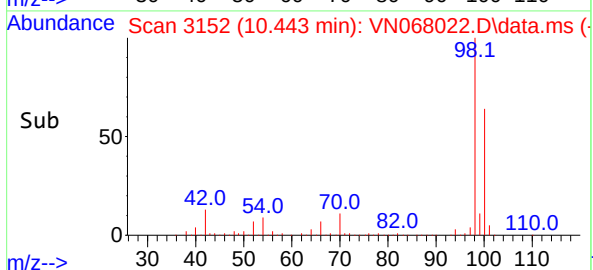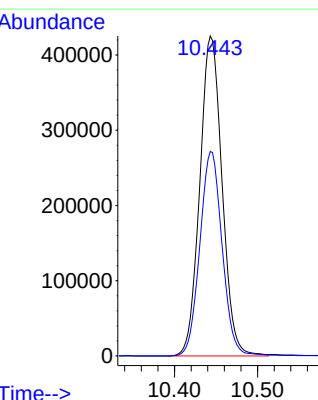







#51
4-Methyl-2-Pentanone
Concen: 0.884 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 43 Resp: 5265
Ion Ratio Lower Upper
43 100
58 37.0 28.6 43.0

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:42:53 PM

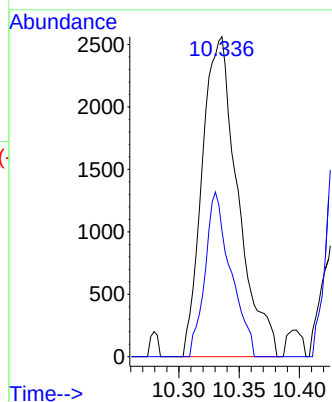


#58
2-Chloroethyl Vinyl ether
Concen: 1.688 ug/l
RT: 10.043 min Scan# 3003
Delta R.T. -0.001 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 63 Resp: 1867
Ion Ratio Lower Upper
63 100
106 22.2 19.8 29.8

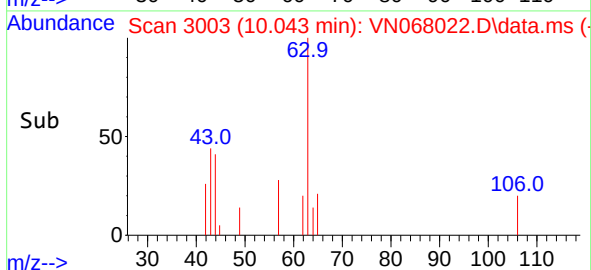







#59
2-Hexanone
Concen: 0.976 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. 0.002 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45





Tgt Ion: 43 Resp: 4175
Ion Ratio Lower Upper
43 100
58 43.5 24.7 74.1

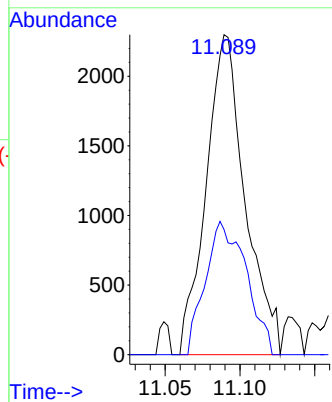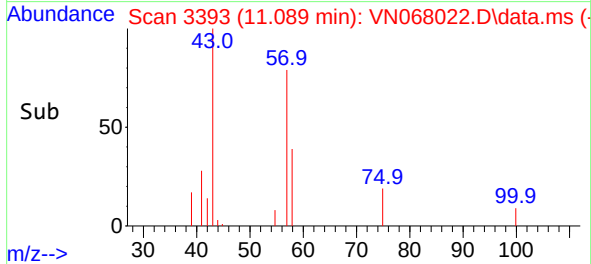

#62
4-Bromofluorobenzene
Concen: 44.669 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.001 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

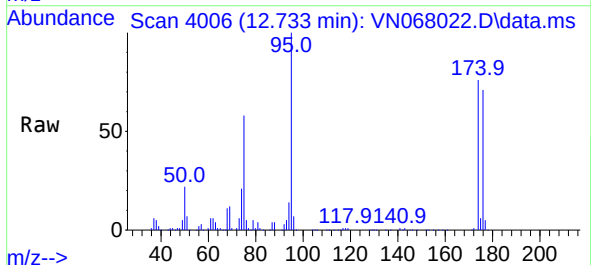


Tgt Ion: 95 Resp: 243006
Ion Ratio Lower Upper
95 100
174 72.9 0.0 122.0
176 69.3 0.0 117.6

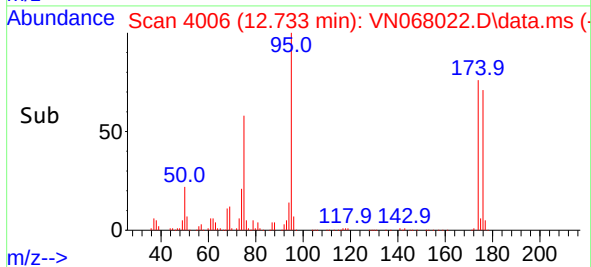

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL

Manual Integrations
APPROVED

MMDadoda
8/6/2021 5:42:53 PM







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.001 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion:117 Resp: 595834
Ion Ratio Lower Upper
117 100
82 57.1 53.1 79.7
119 32.7 25.5 38.3

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:42:53 PM

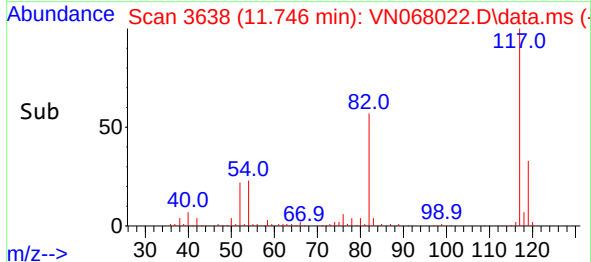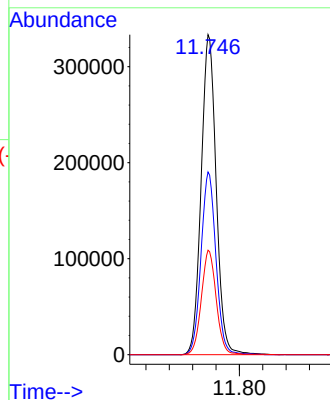


#68
m/p-Xylenes
Concen: 0.284 ug/l
RT: 11.961 min Scan# 3718
Delta R.T. 0.005 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion:106 Resp: 2294
Ion Ratio Lower Upper
106 100
91 207.2 180.6 270.8

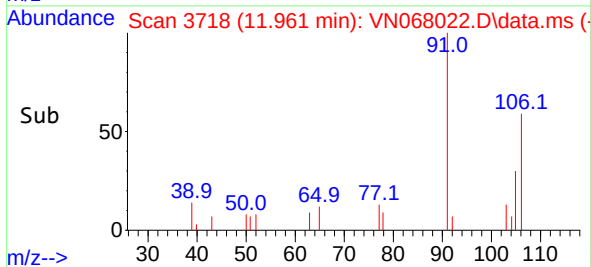
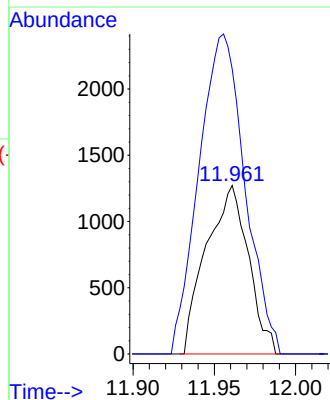
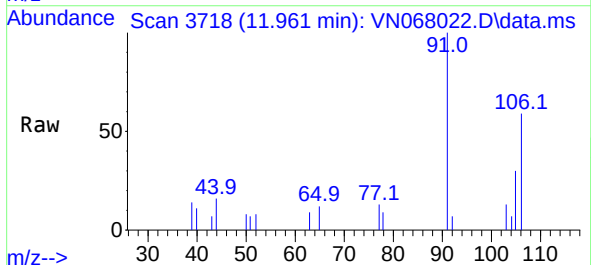


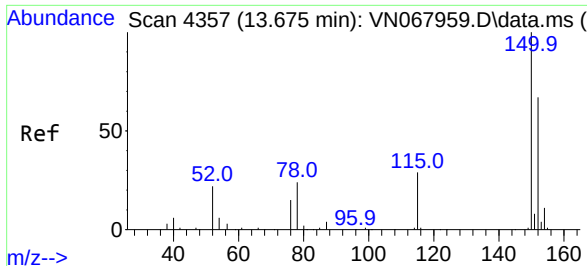


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.002 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

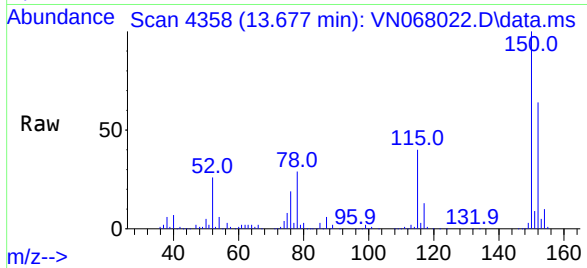



Tgt Ion:152 Resp: 201461
Ion Ratio Lower Upper
152 100
115 63.8 36.1 108.5
150 159.1 0.0 351.8

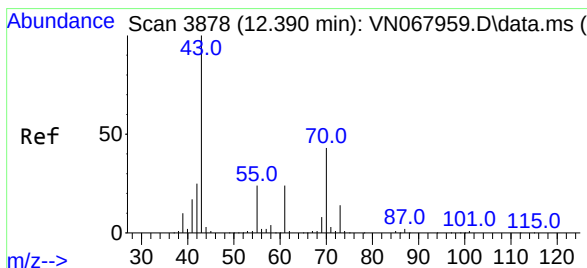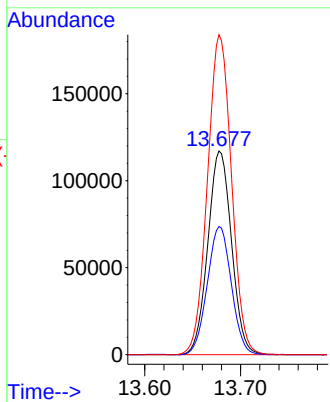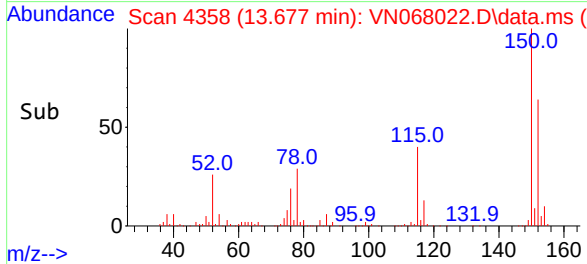

#74
N-ethyl acetate
Concen: 0.232 ug/l
RT: 12.387 min Scan# 3877
Delta R.T. -0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

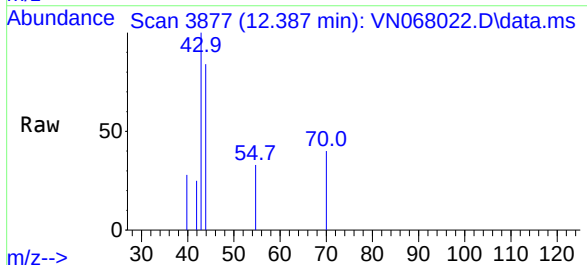


Tgt Ion: 43 Resp: 1328
Ion Ratio Lower Upper
43 100
70 19.9 29.4 44.2#
55 11.0 17.0 25.4#
61 0.0 17.6 26.4#

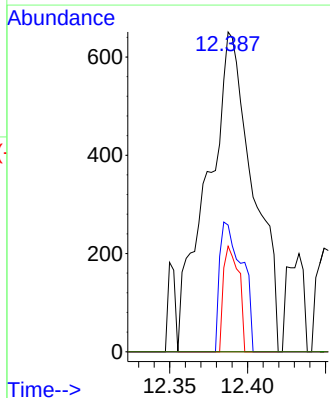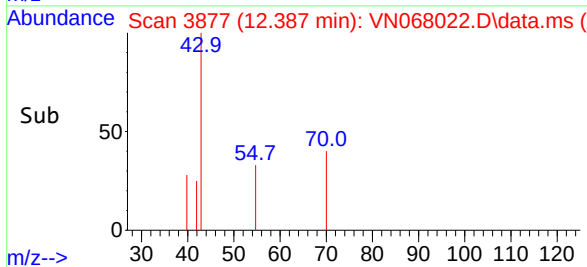

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL

Manual Integrations
APPROVED

MMDadoda
8/6/2021 5:42:53 PM







#75
1,1,2,2-Tetrachloroethane
Concen: 0.210 ug/l
RT: 12.827 min Scan# 4041
Delta R.T. -0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 83 Resp: 1042
Ion Ratio Lower Upper
83 100
131 0.0 4.8 14.4#
85 63.7 32.2 96.6

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT3-2021DL




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:42:53 PM

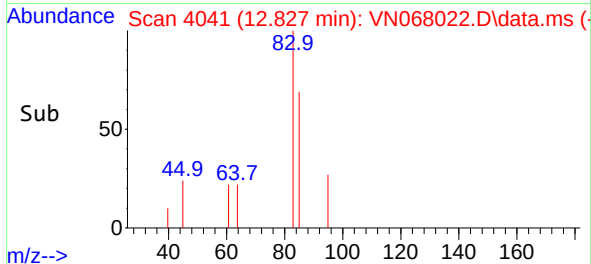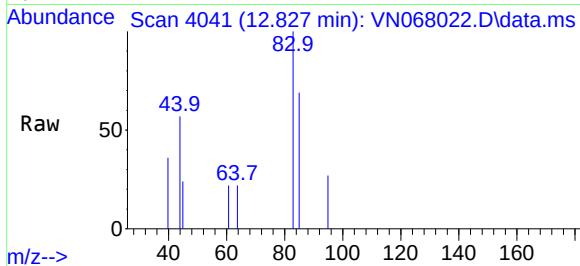

#76
1,2,3-Trichloropropane
Concen: 0.272 ug/l m
RT: 12.884 min Scan# 4062
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 75 Resp: 1099
Ion Ratio Lower Upper
75 100
77 111.5 0.0 0.0#

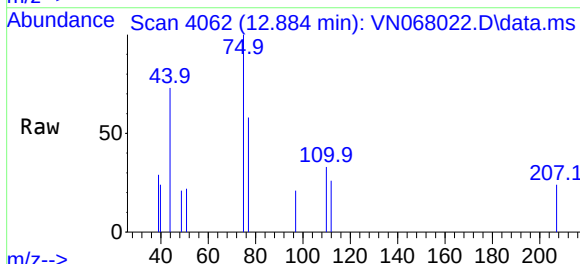

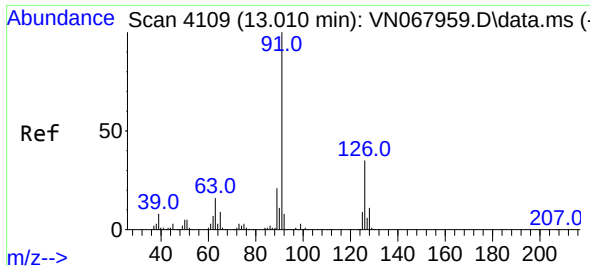





#79
2-Chlorotoluene
Concen: 0.214 ug/l
RT: 13.010 min Scan# 4109
Delta R.T. -0.000 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 91 Resp: 2416
Ion Ratio Lower Upper
91 100
126 35.1 14.5 43.5

Instrument :
MSVOA_N
ClientSampleID :
MDL-WATER-03-QT3-2021DL




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:42:53 PM

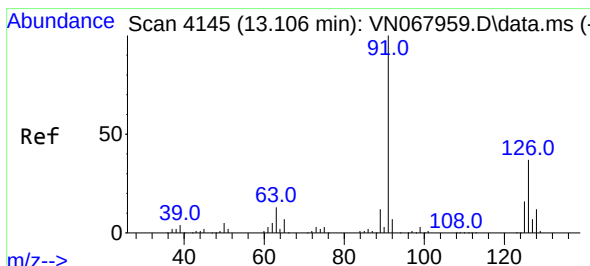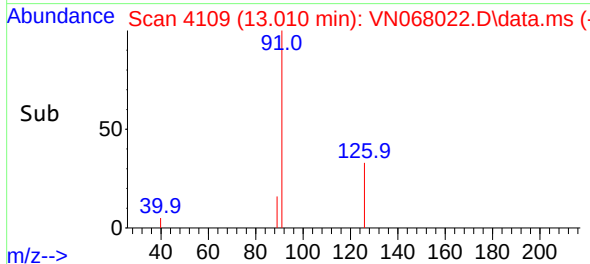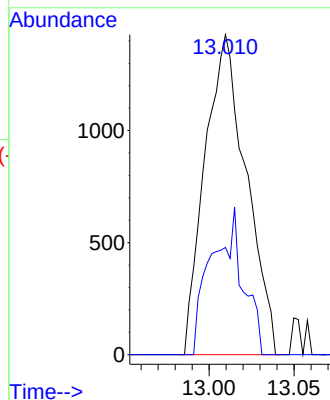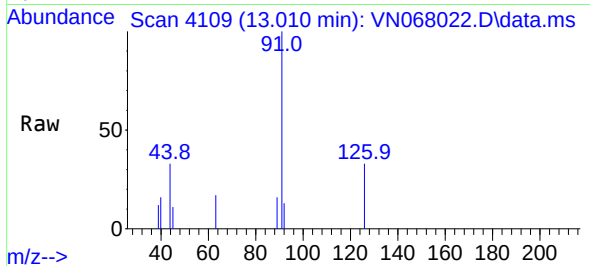


#82
4-Chlorotoluene
Concen: 0.202 ug/l
RT: 13.109 min Scan# 4146
Delta R.T. 0.003 min
Lab File: VN068022.D
Acq: 5 Aug 2021 17:45

Tgt Ion: 91 Resp: 2289
Ion Ratio Lower Upper
91 100
126 30.8 14.8 44.4

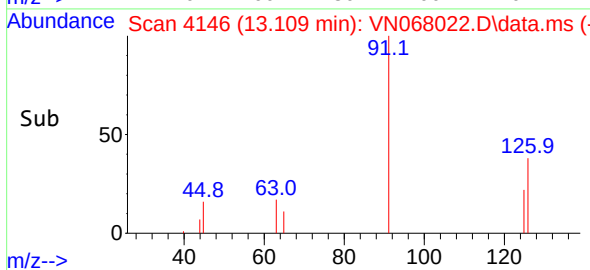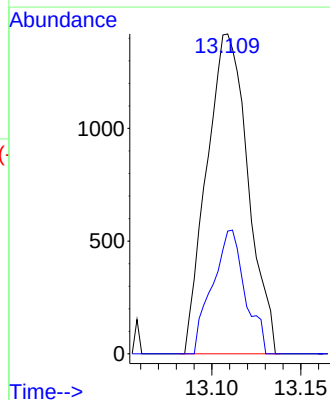
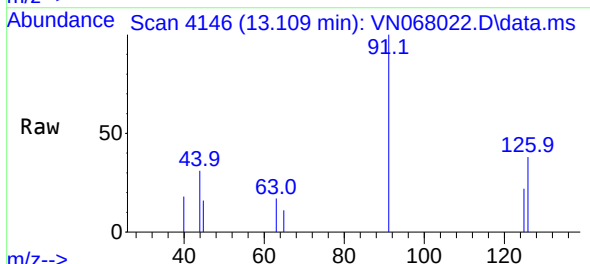




#88
 1,4-Dichlorobenzene
 Concen: 0.217 ug/l m
 RT: 13.696 min Scan# 4365
 Delta R.T. 0.000 min
 Lab File: VN068022.D
 Acq: 5 Aug 2021 17:45



Tgt Ion:	146	Resp:	1483
Ion	Ratio	Lower	Upper
146	100		
111	25.0	23.4	70.2
148	53.0	31.8	95.3

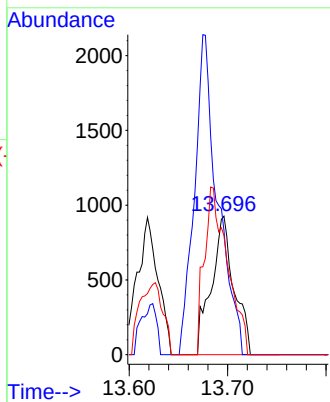

Instrument :
 MSVOA_N
 ClientSampleId :
 MDL-WATER-03-QT3-2021DL

Manual Integrations
 APPROVED

MMDadoda
 8/6/2021 5:42:53 PM