
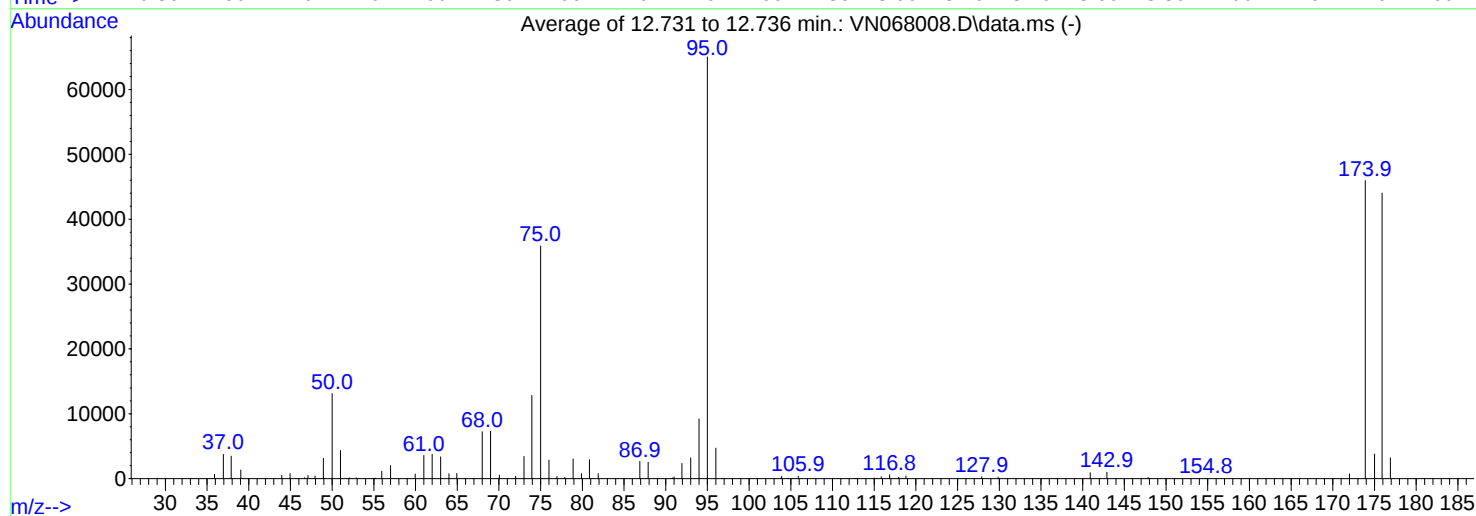


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080521\
Data File : VN068008.D
Acq On : 5 Aug 2021 10:45
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
Title : SW846 8260
Last Update : Thu Jul 29 15:02:35 2021

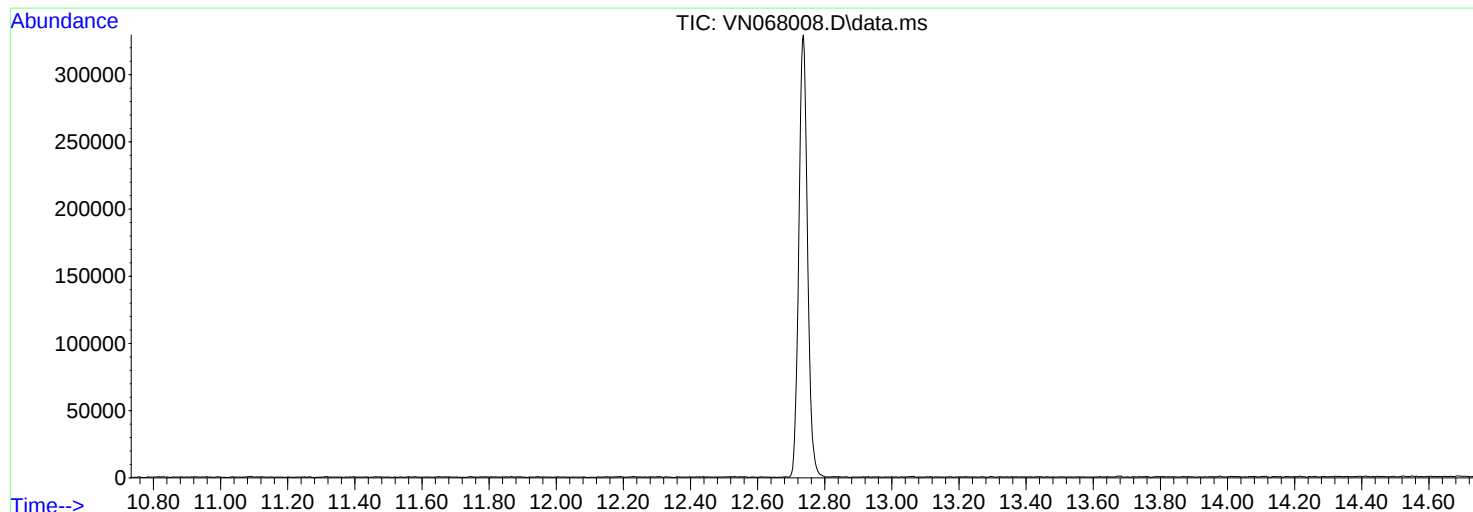

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	13135	PASS
75	95	30	60	55.2	35877	PASS
95	95	100	100	100.0	65032	PASS
96	95	5	9	7.3	4719	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.7	45963	PASS
175	174	5	9	8.3	3809	PASS
176	174	95	101	95.8	44032	PASS
177	176	5	9	7.3	3216	PASS