

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080522\
 Data File : VN073762.D
 Acq On : 05 Aug 2022 15:05
 Operator : JC\MD
 Sample : N4071-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Aug 07 20:51:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 29 02:20:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.022	168	372657	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	594919	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	555332	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	261703	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.375	65	216296	47.627	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	95.260%
35) Dibromofluoromethane	7.951	113	205357	54.971	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	109.940%
50) Toluene-d8	10.381	98	665731	45.286	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	90.580%
62) 4-Bromofluorobenzene	12.675	95	246140	50.097	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080522\
Data File : VN073762.D
Acq On : 05 Aug 2022 15:05
Operator : JC\MD
Sample : N4071-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Aug 07 20:51:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 29 02:20:25 2022
Response via : Initial Calibration




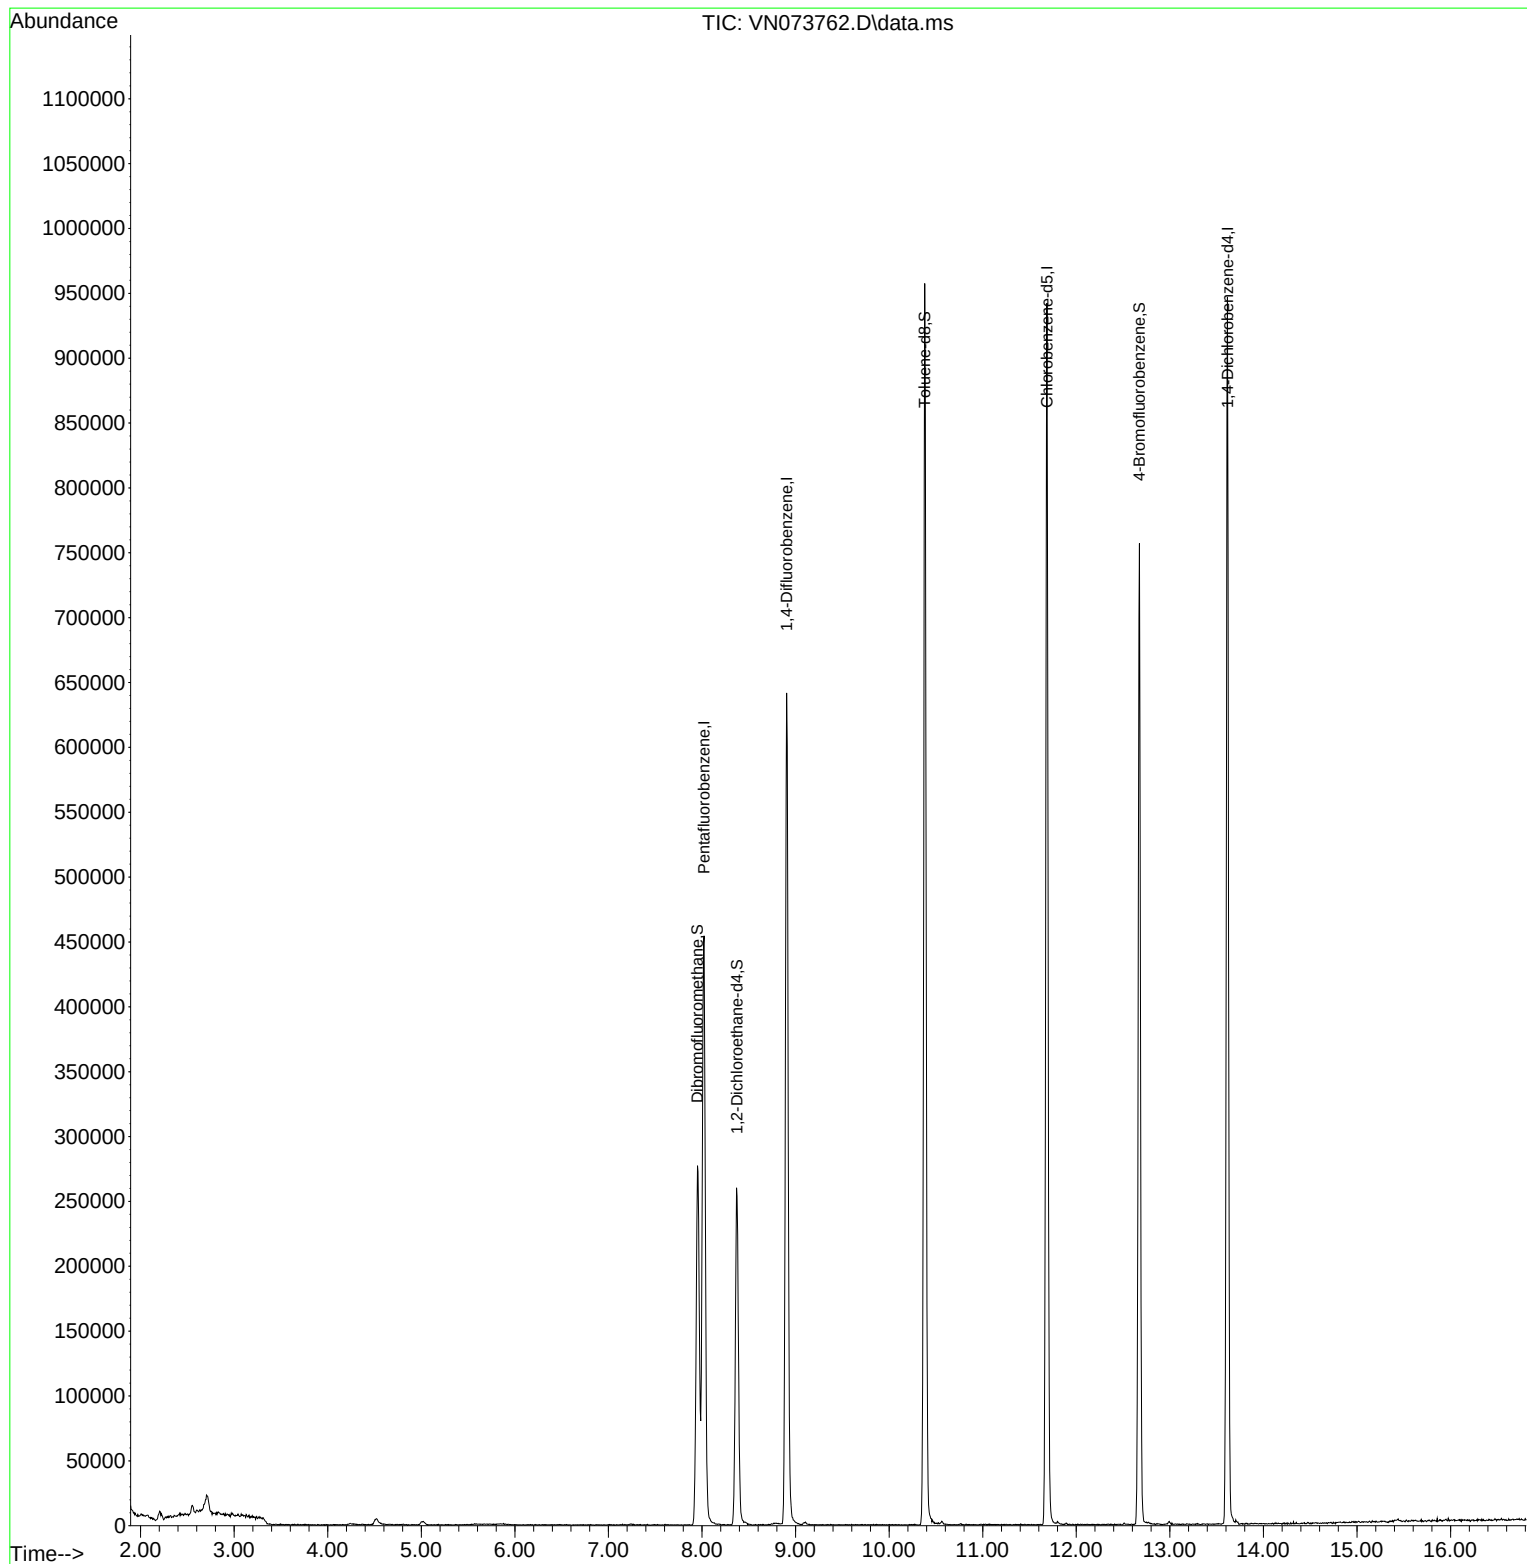


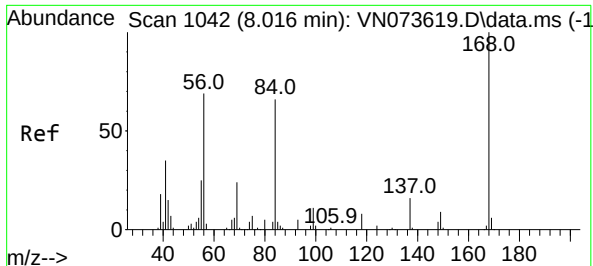

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.022 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VN073762.D
Acq: 05 Aug 2022 15:05




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:168 Resp: 372657
Ion Ratio Lower Upper
168 100
99 50.5 42.3 63.5

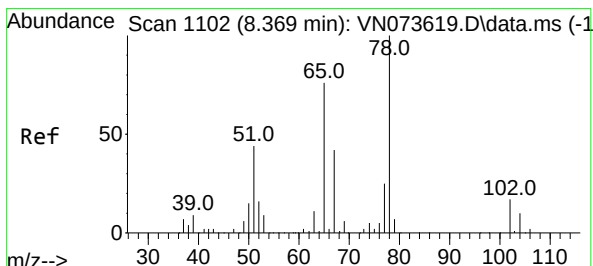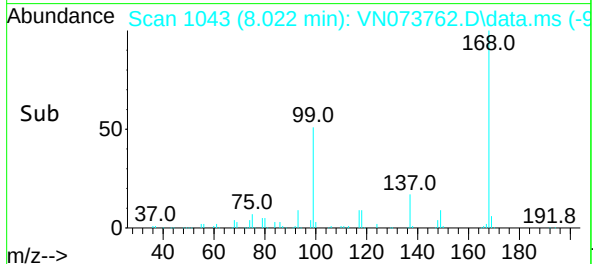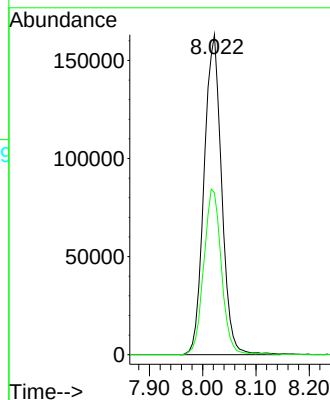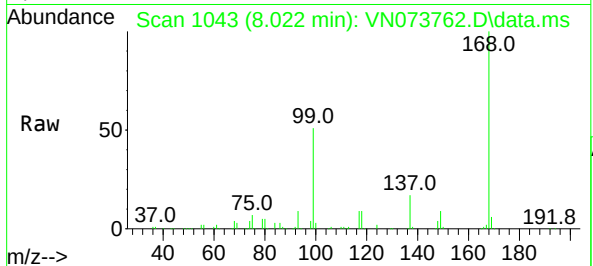

#33
1,2-Dichloroethane-d4
Concen: 47.627 ug/l
RT: 8.375 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VN073762.D
Acq: 05 Aug 2022 15:05

Tgt Ion: 65 Resp: 216296
Ion Ratio Lower Upper
65 100
67 53.3 0.0 104.8

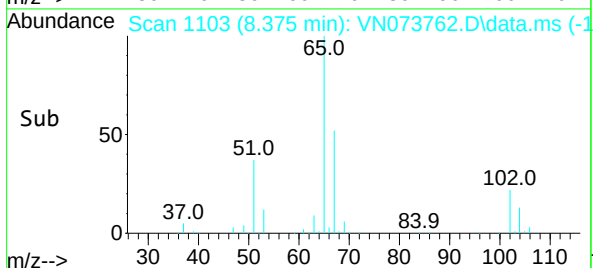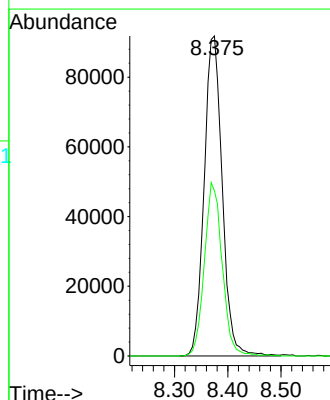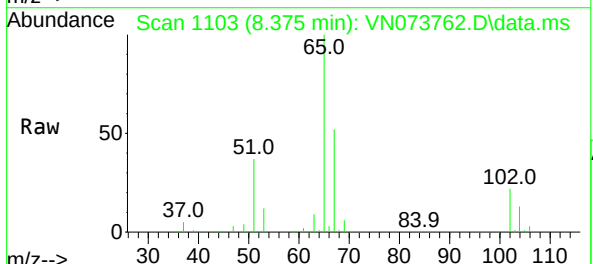

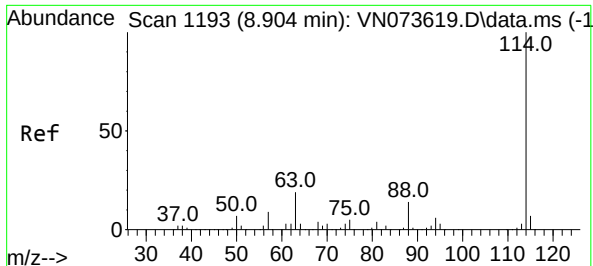

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN073762.D

Acq: 05 Aug 2022 15:05

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-SAMPLE-MANAG





Tgt Ion:114 Resp: 594919

Ion Ratio Lower Upper

114 100

63 20.4 0.0 40.0

88 15.3 0.0 32.6

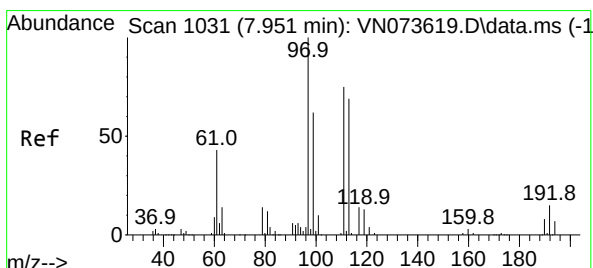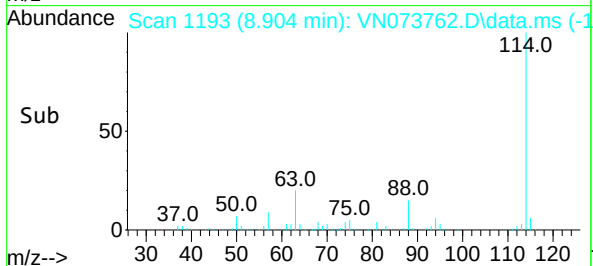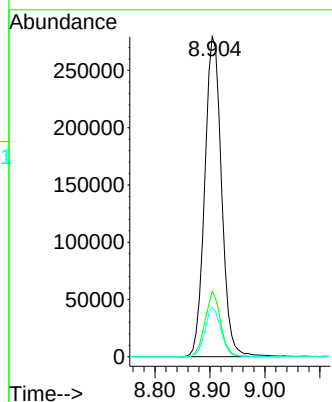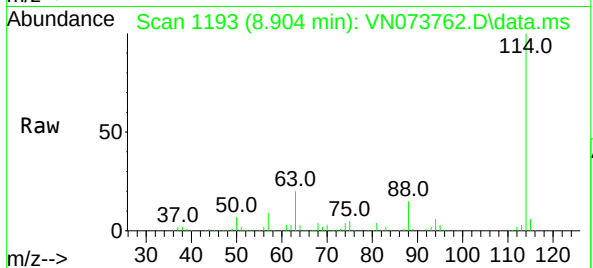

#35

Dibromofluoromethane

Concen: 54.971 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073762.D

Acq: 05 Aug 2022 15:05




Tgt Ion:113 Resp: 205357


Ion Ratio Lower Upper

113 100

111 103.3 81.4 122.0

192 21.0 17.0 25.6


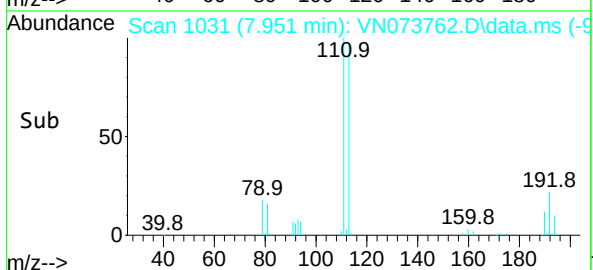
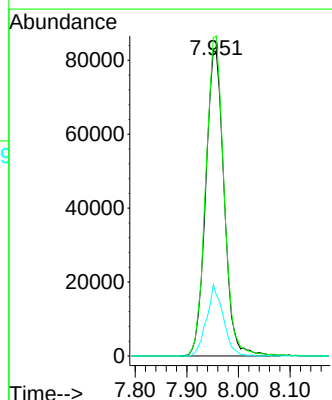
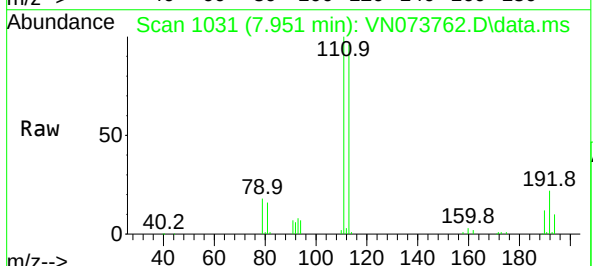


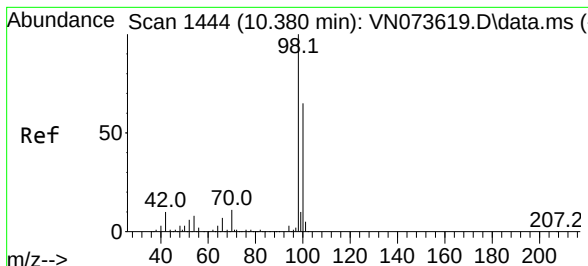

#50
Toluene-d8
Concen: 45.286 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN073762.D
Acq: 05 Aug 2022 15:05




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion: 98 Resp: 665731
Ion Ratio Lower Upper
98 100
100 64.4 52.6 78.8

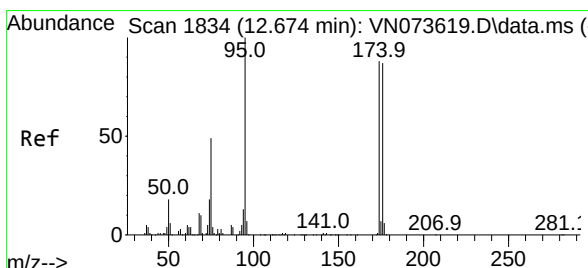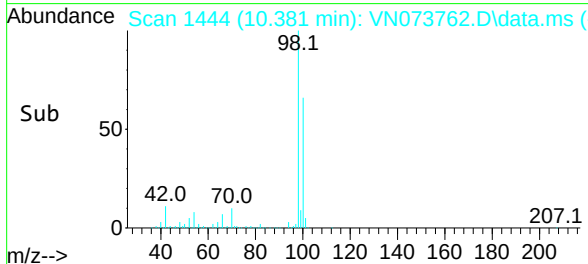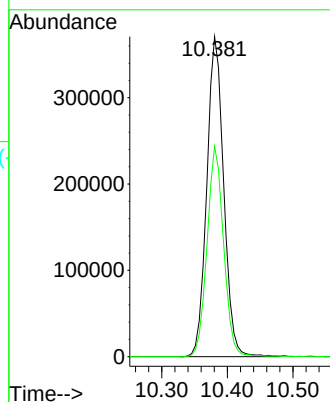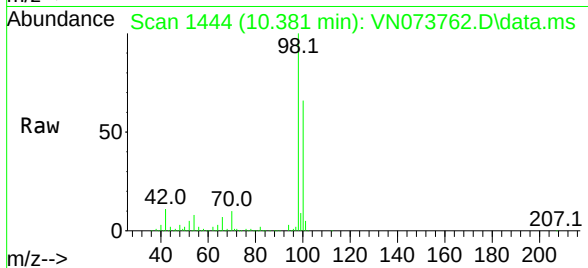

#62
4-Bromofluorobenzene
Concen: 50.097 ug/l
RT: 12.675 min Scan# 1834
Delta R.T. 0.001 min
Lab File: VN073762.D
Acq: 05 Aug 2022 15:05

Tgt Ion: 95 Resp: 246140
Ion Ratio Lower Upper
95 100
174 89.1 0.0 167.6
176 85.5 0.0 163.4


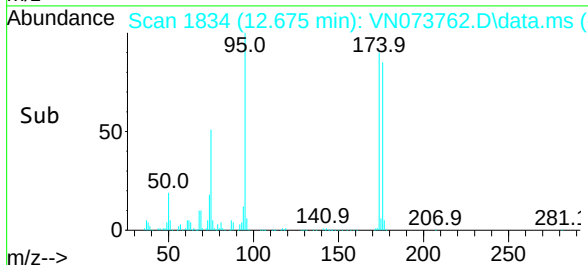
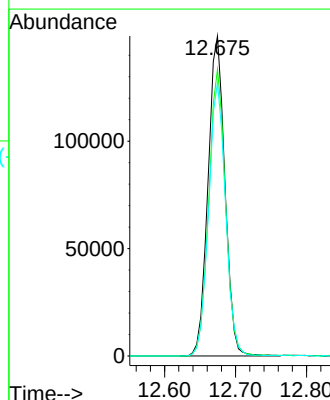
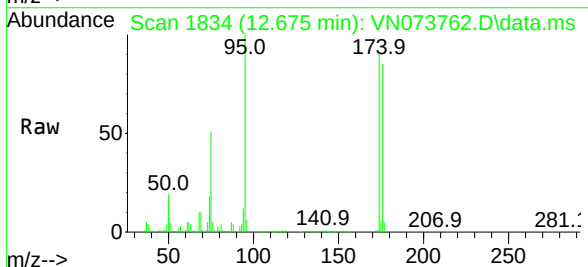


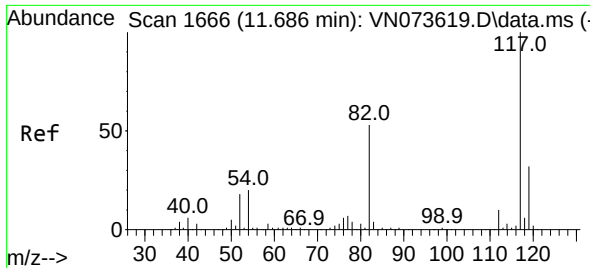

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN073762.D
Acq: 05 Aug 2022 15:05

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:117 Resp: 555332
Ion Ratio Lower Upper
117 100
82 51.9 44.2 66.2
119 32.3 25.4 38.0

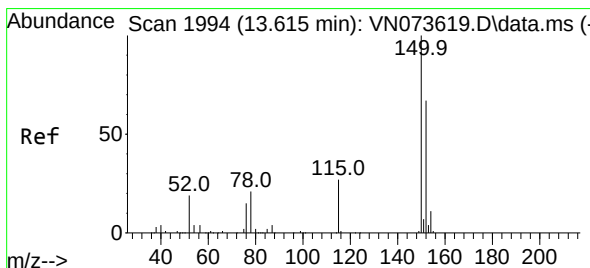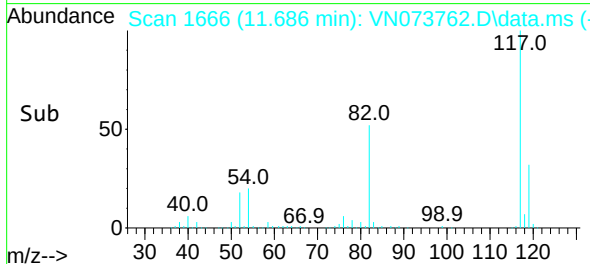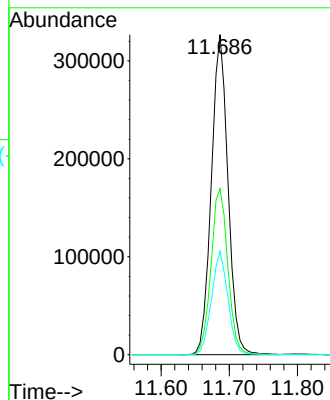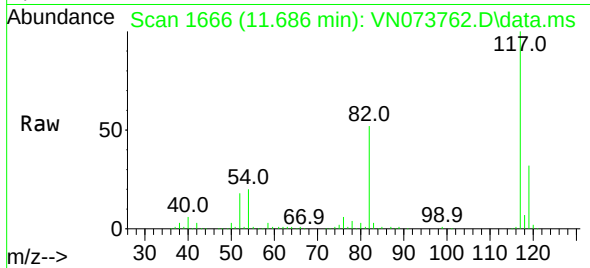

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.616 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN073762.D
Acq: 05 Aug 2022 15:05

Tgt Ion:152 Resp: 261703
Ion Ratio Lower Upper
152 100
115 56.6 28.9 86.7
150 158.4 0.0 356.2

