



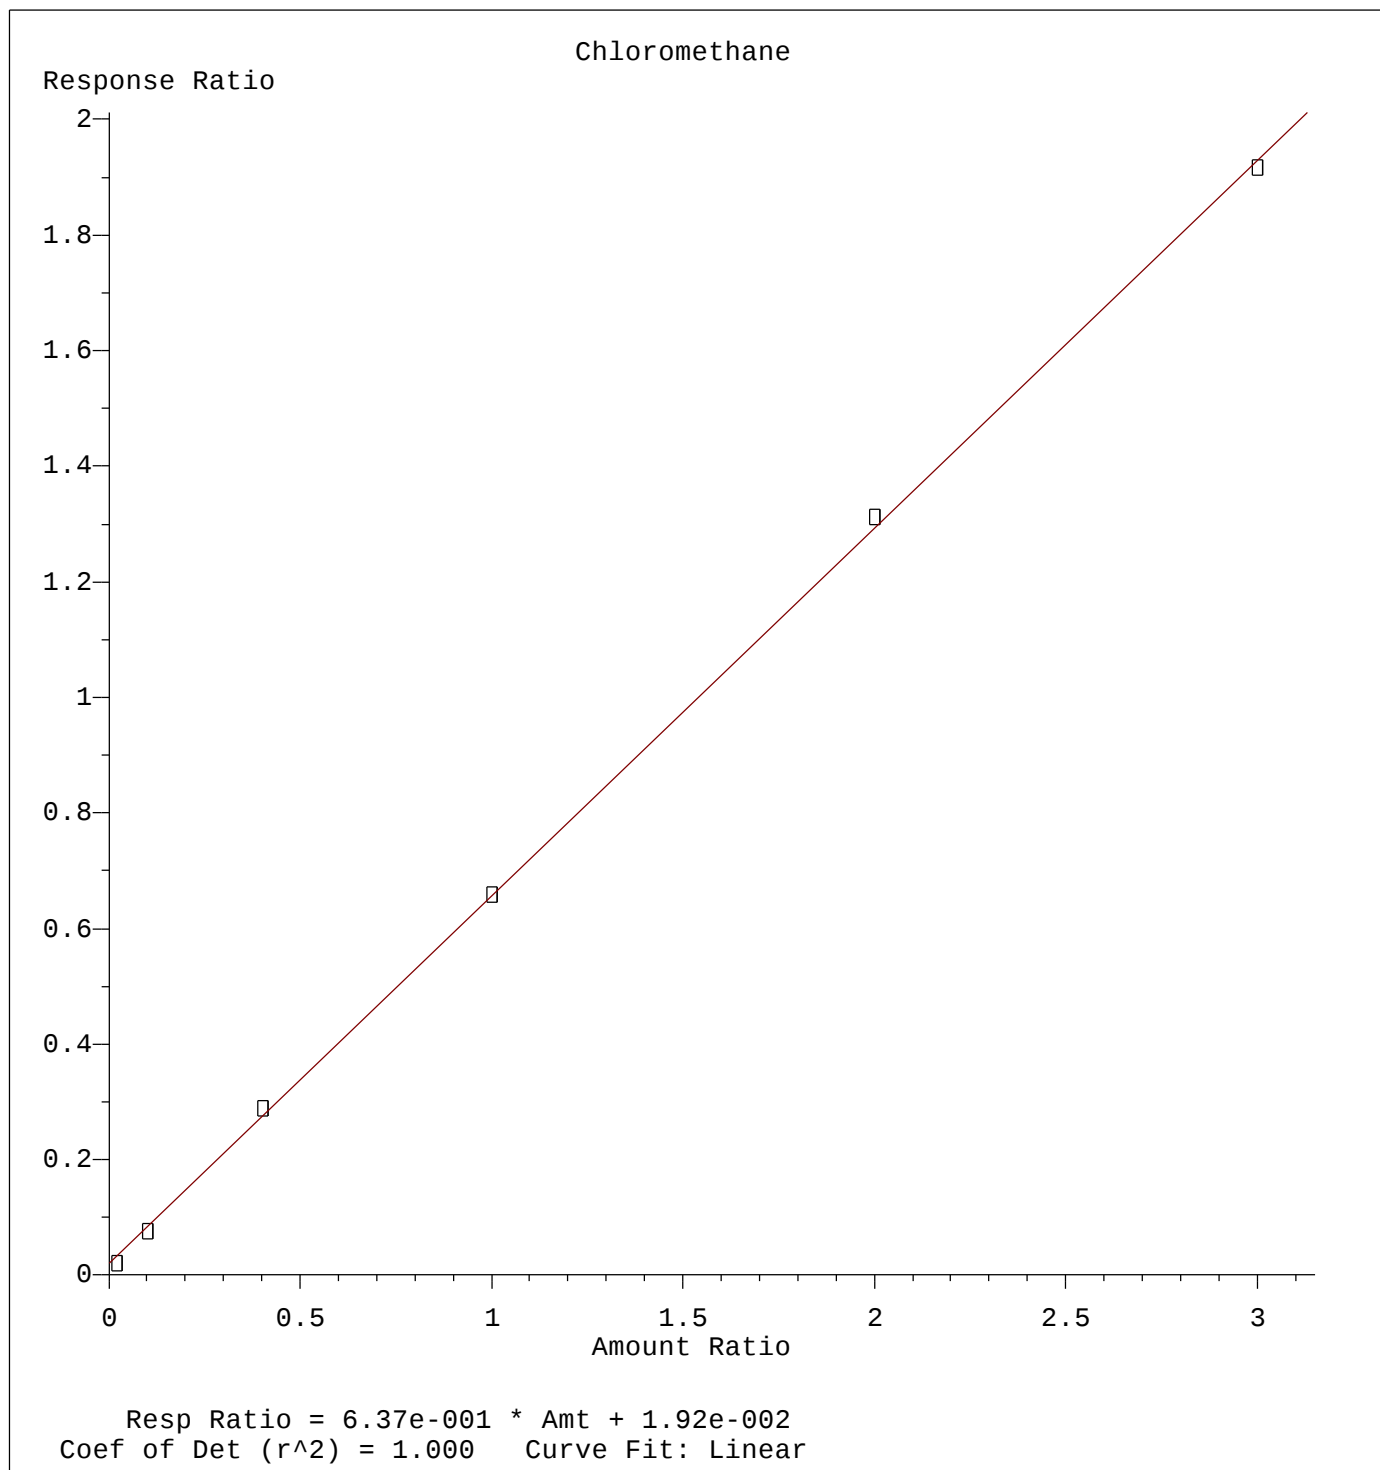

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018


Naphthalene

Response Ratio

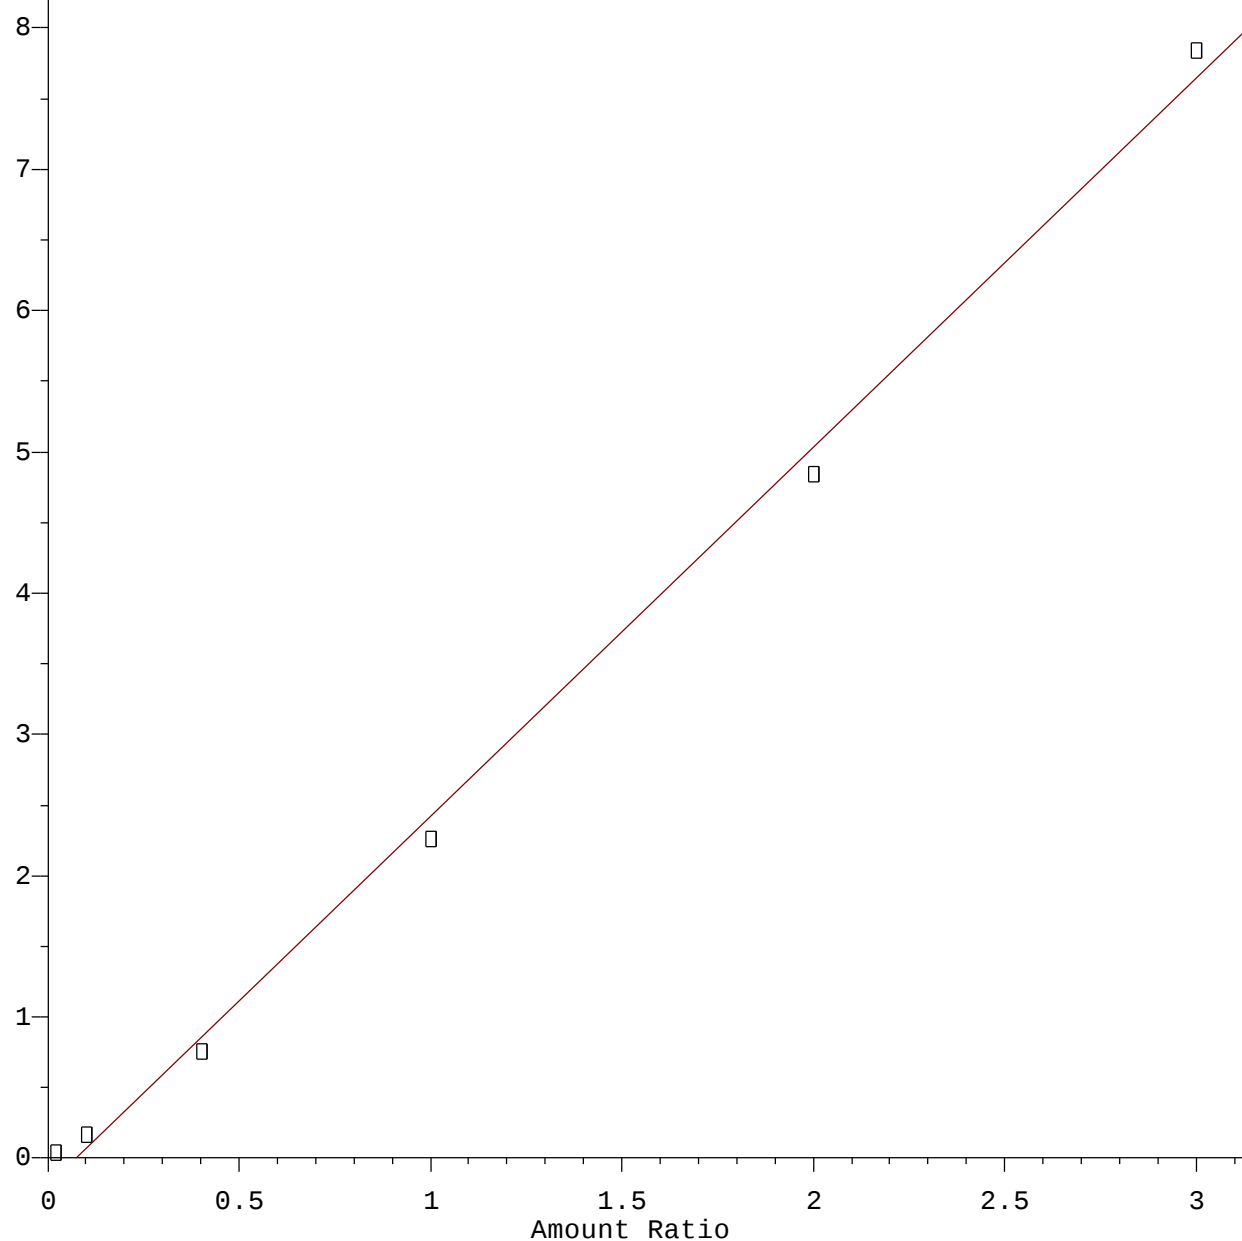

Resp Ratio = 2.61e+000 * Amt - 1.89e-001
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018

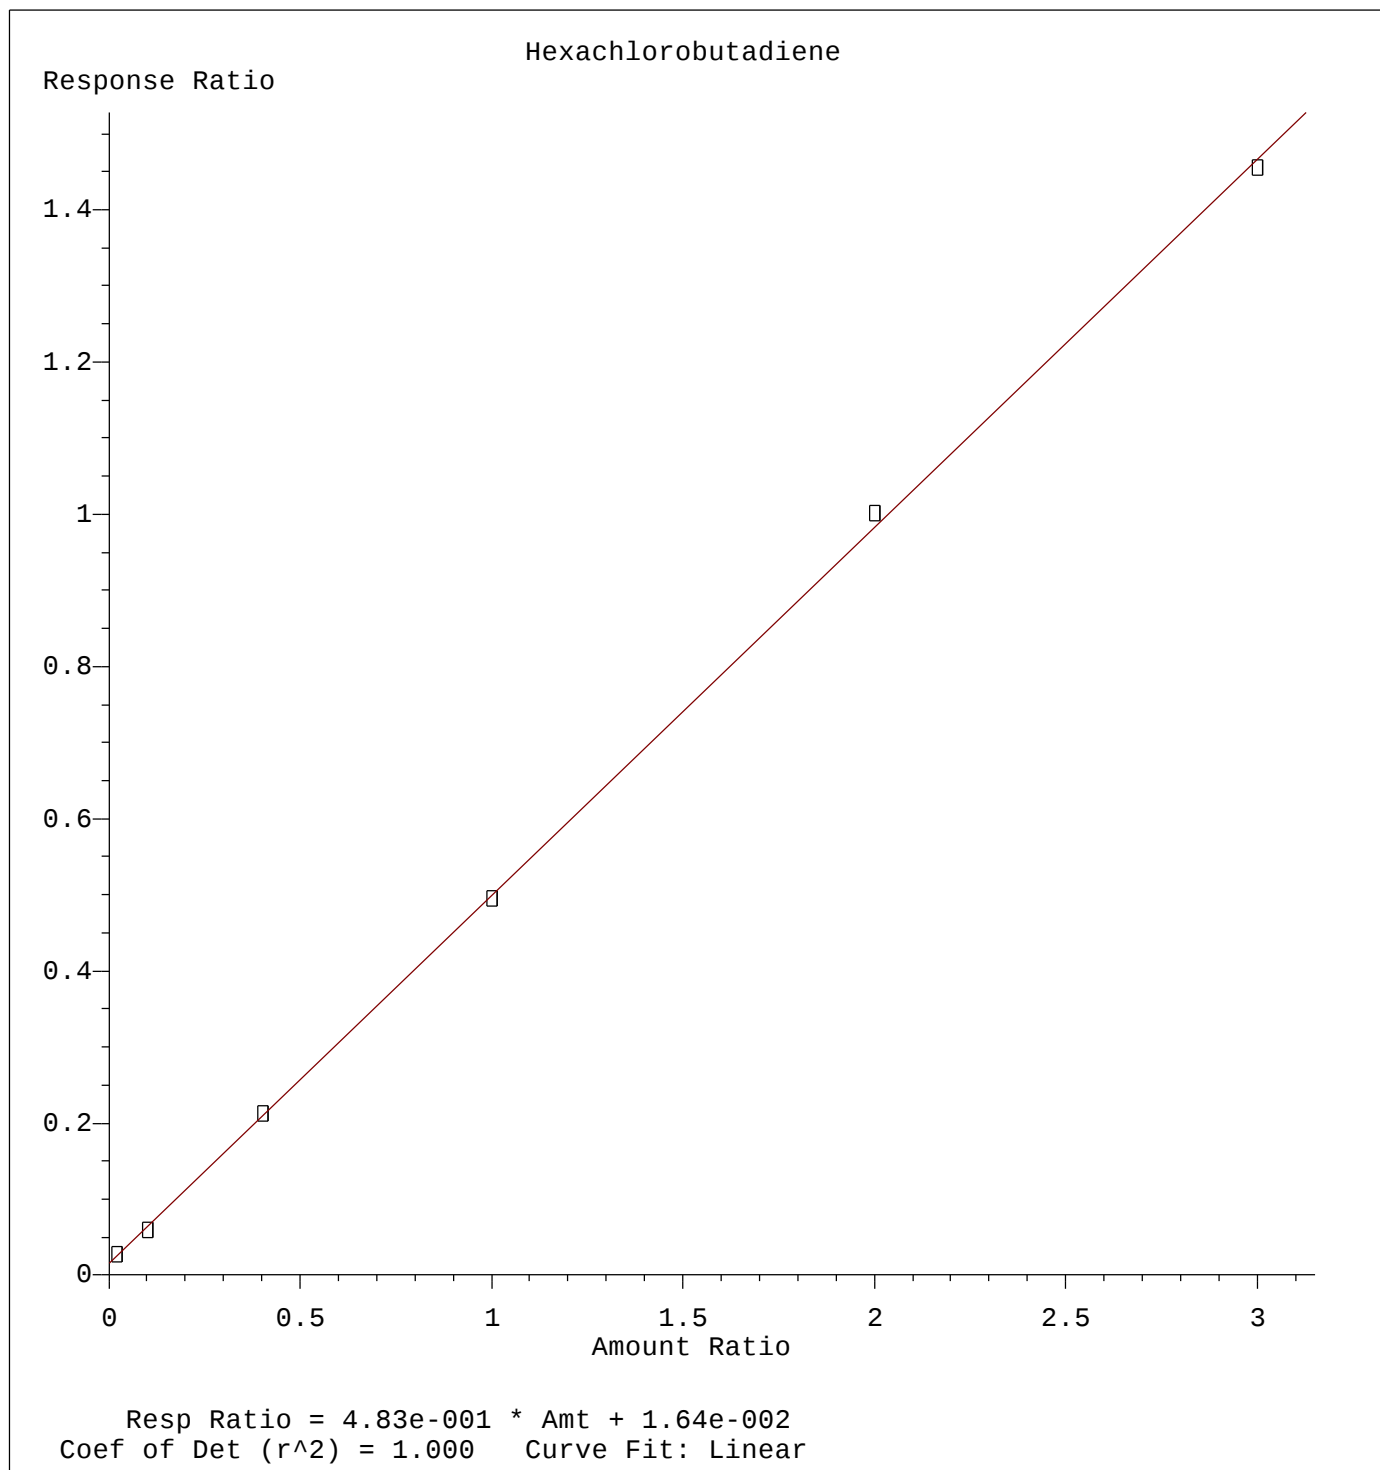

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018

2-Chloroethyl Vinyl ether

Response Ratio

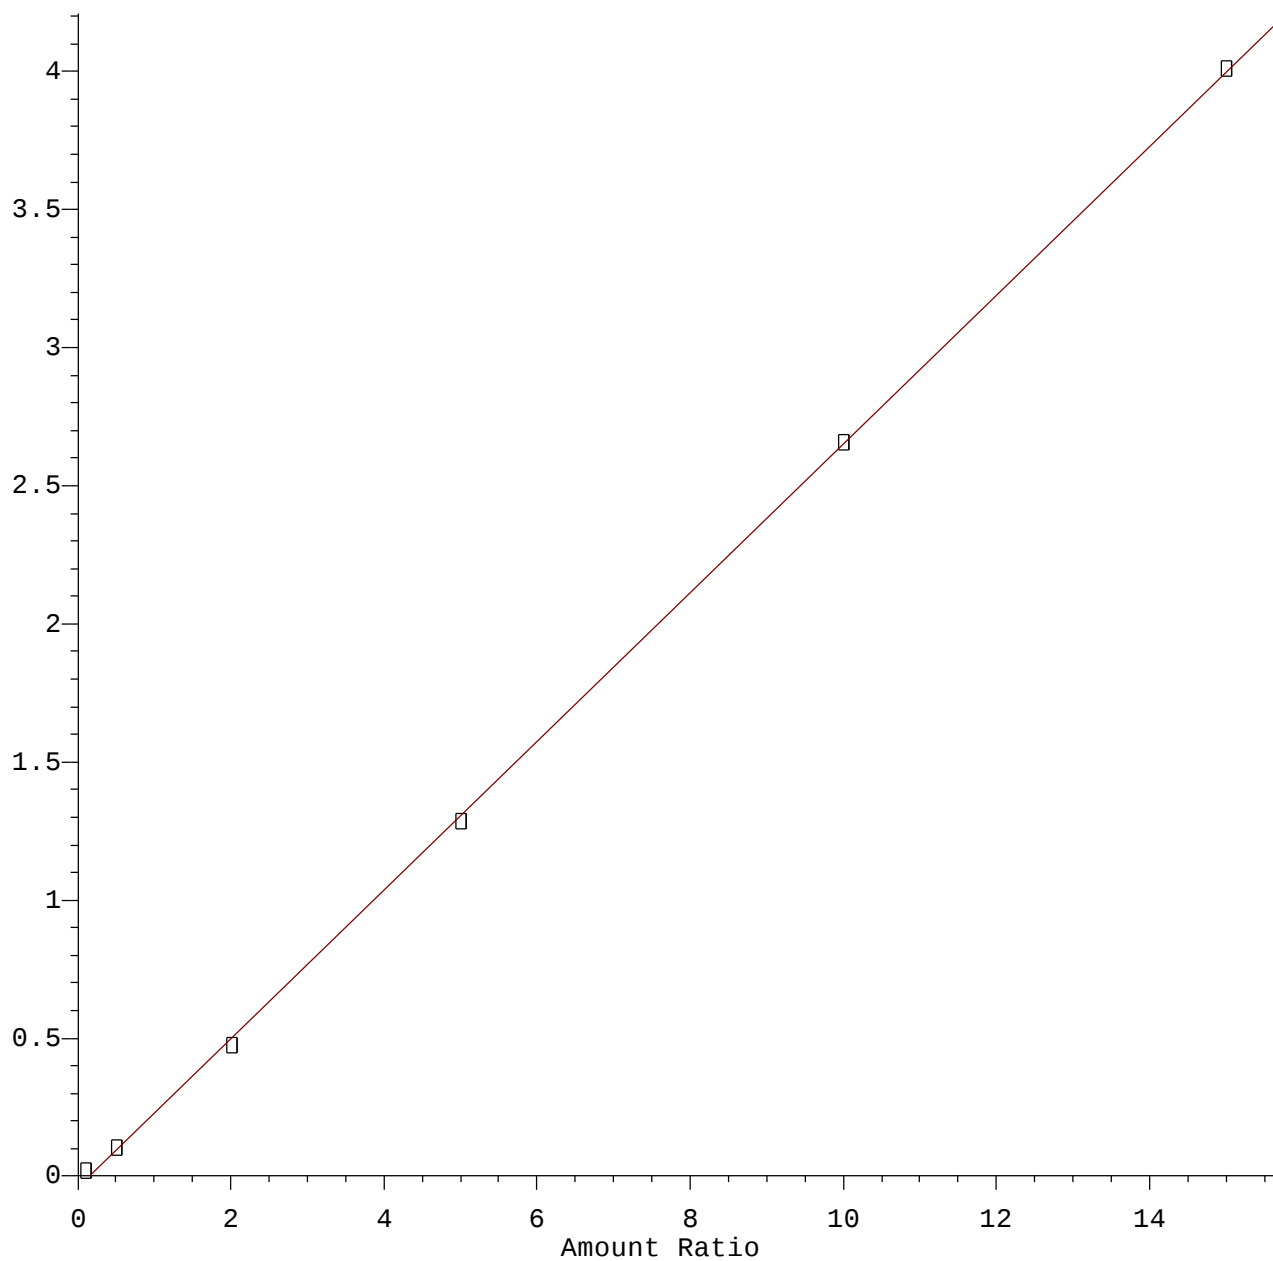


Resp Ratio = $2.69 \times 10^{-1} \times \text{Amt} - 3.98 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018


Ethyl methacrylate

Response Ratio

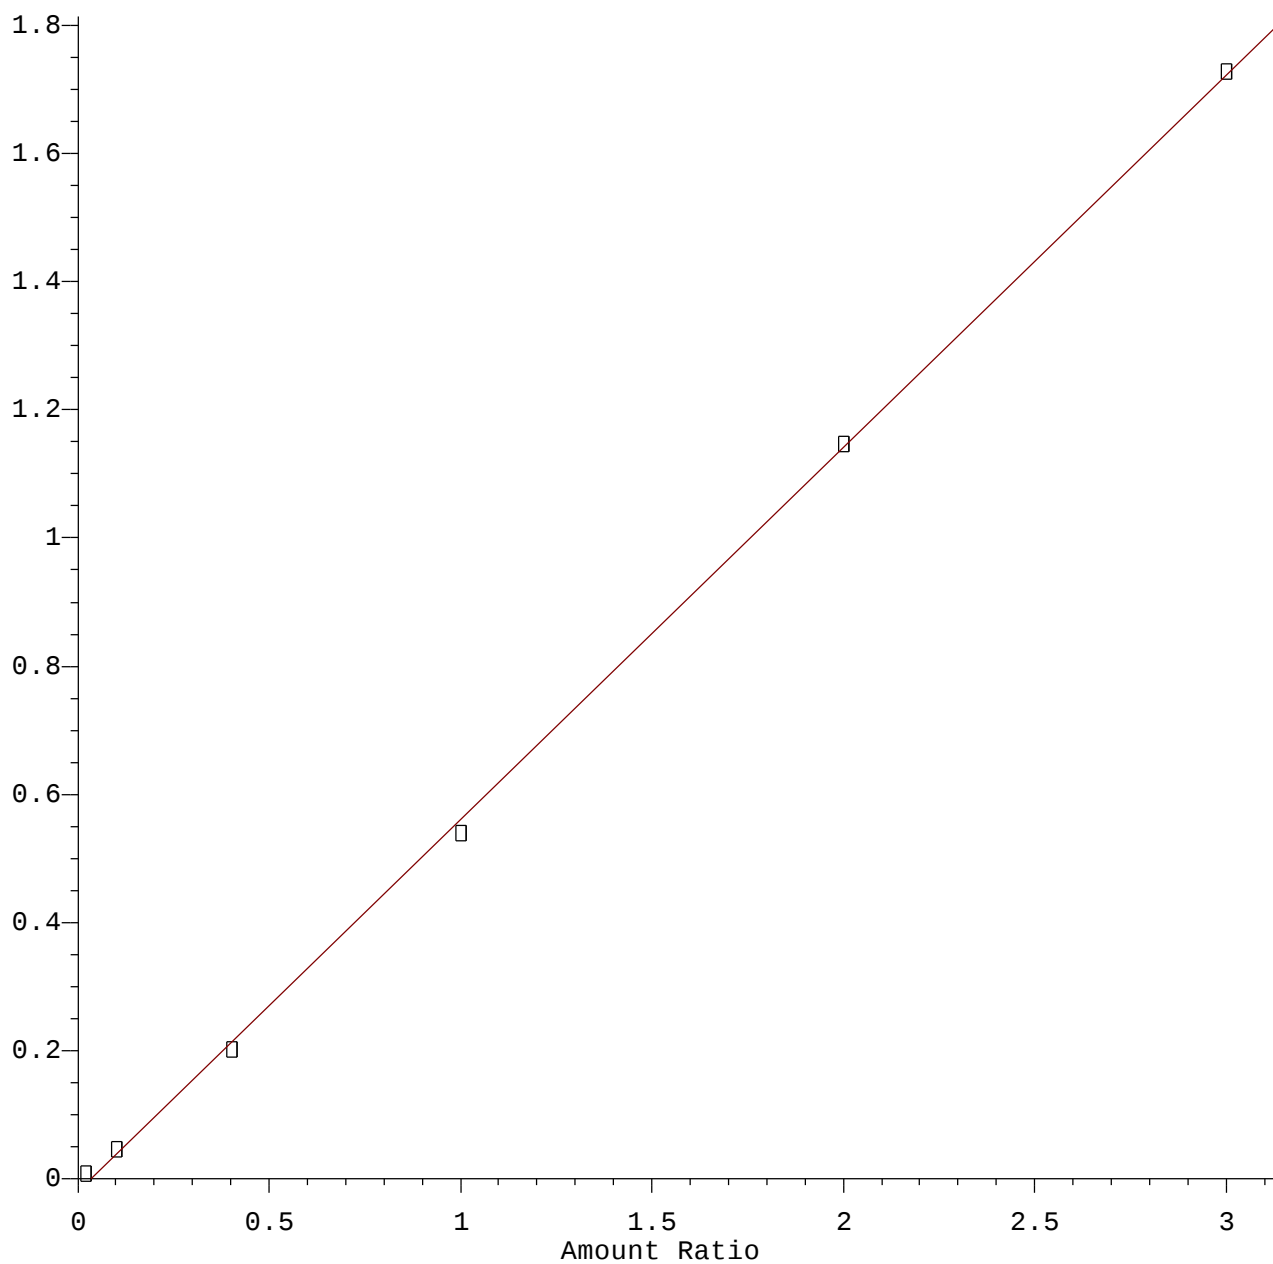

Resp Ratio = 5.80e-001 * Amt - 1.99e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018

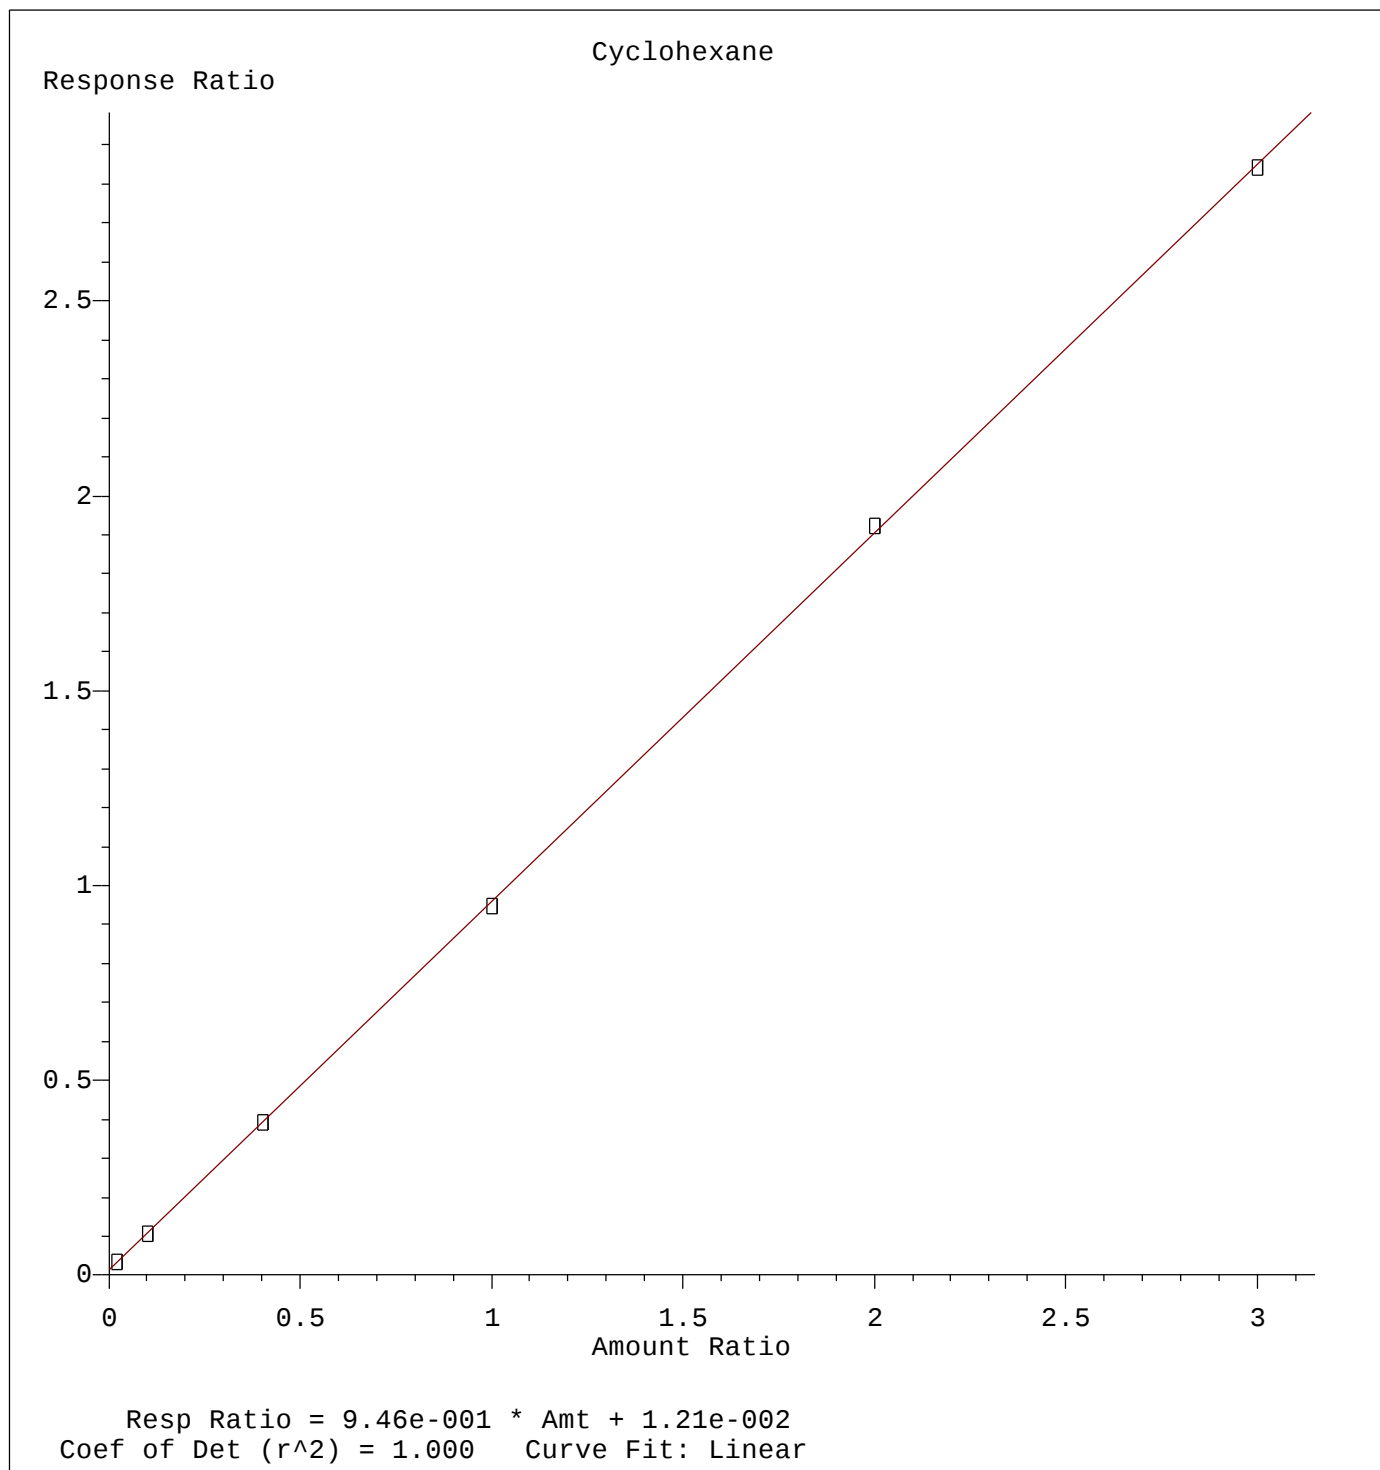

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018


Methylene Chloride

Response Ratio

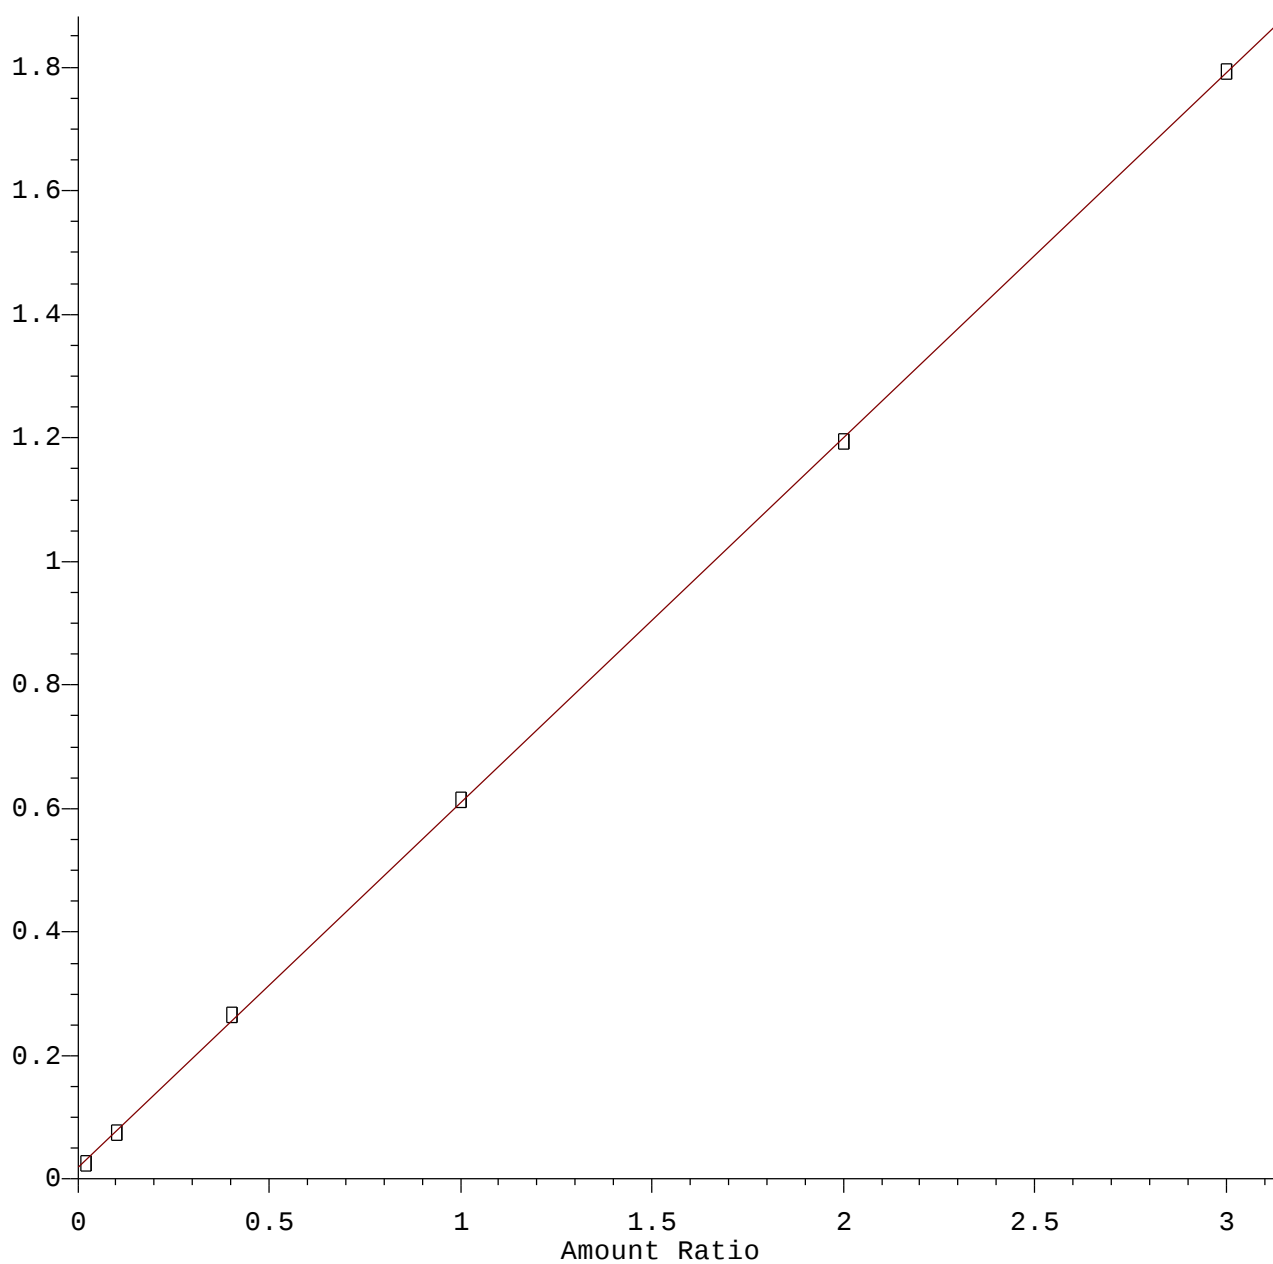


Resp Ratio = 5.90e-001 * Amt + 1.89e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018

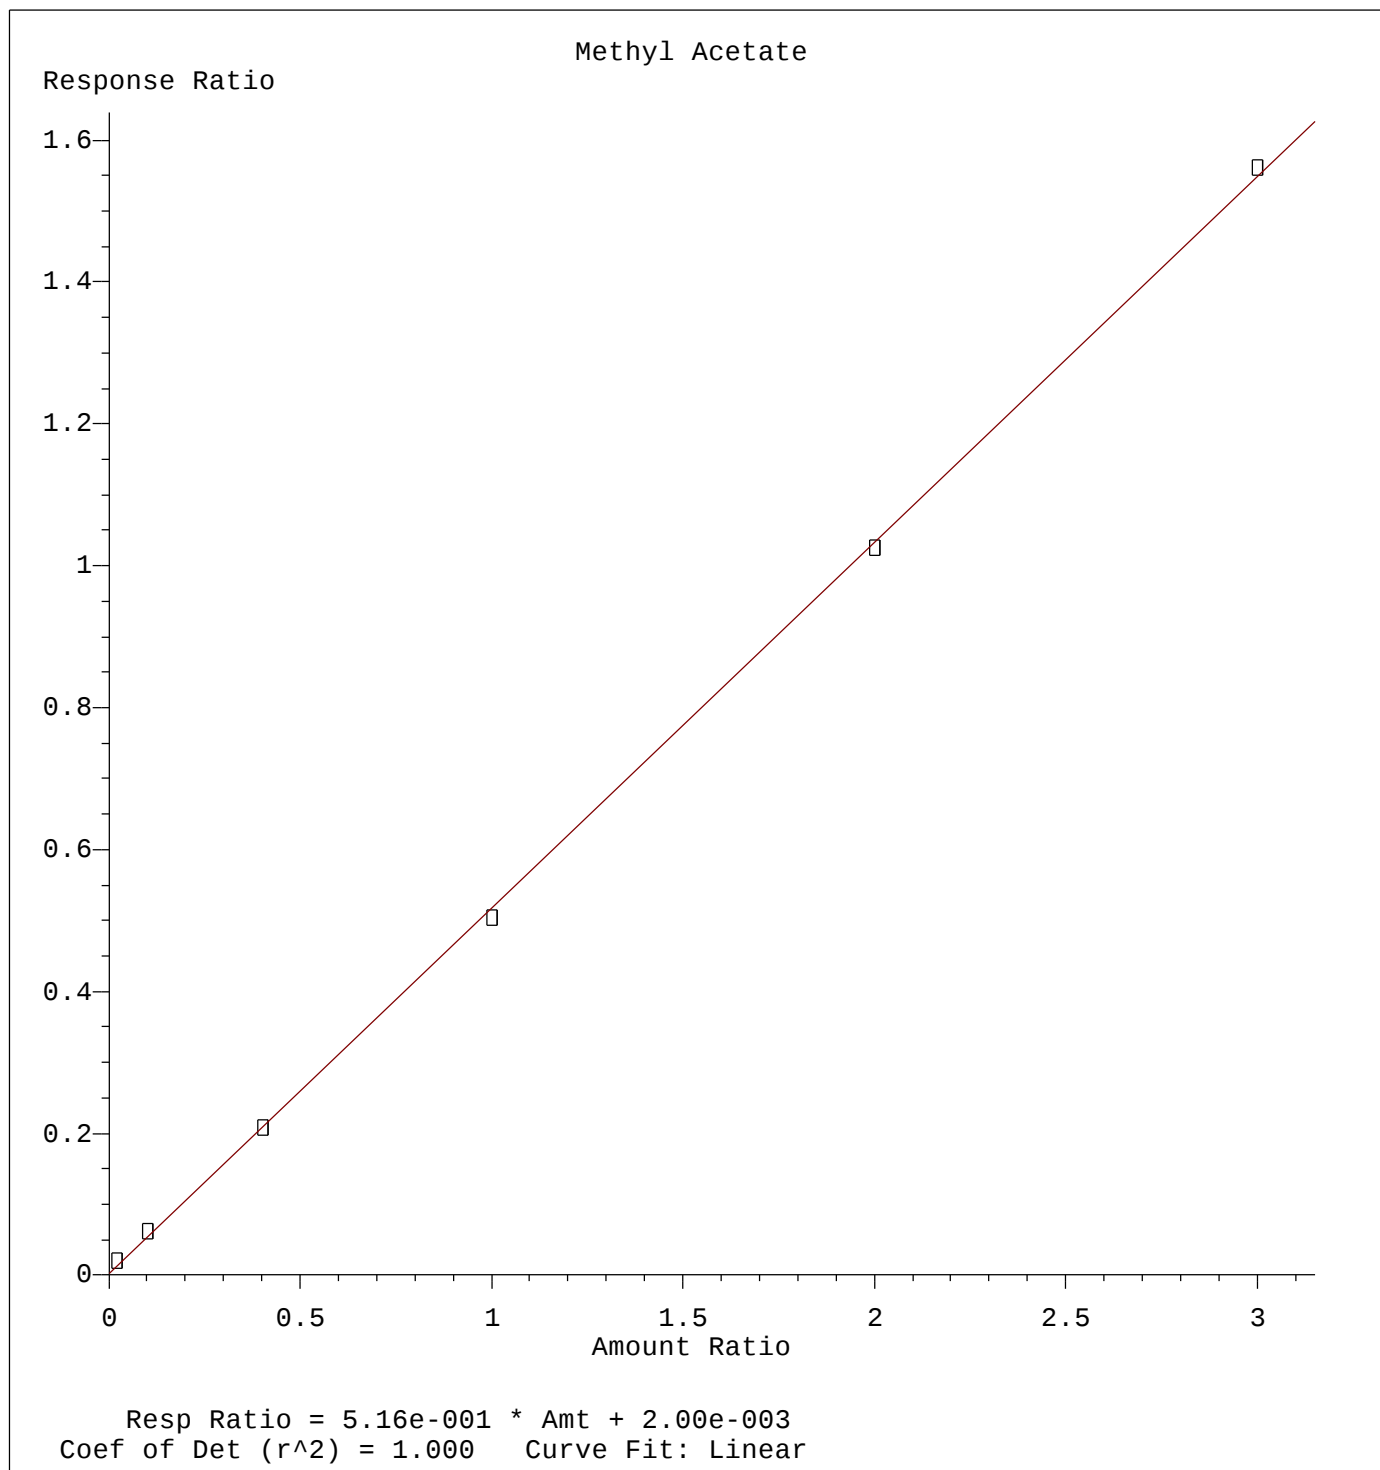


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018

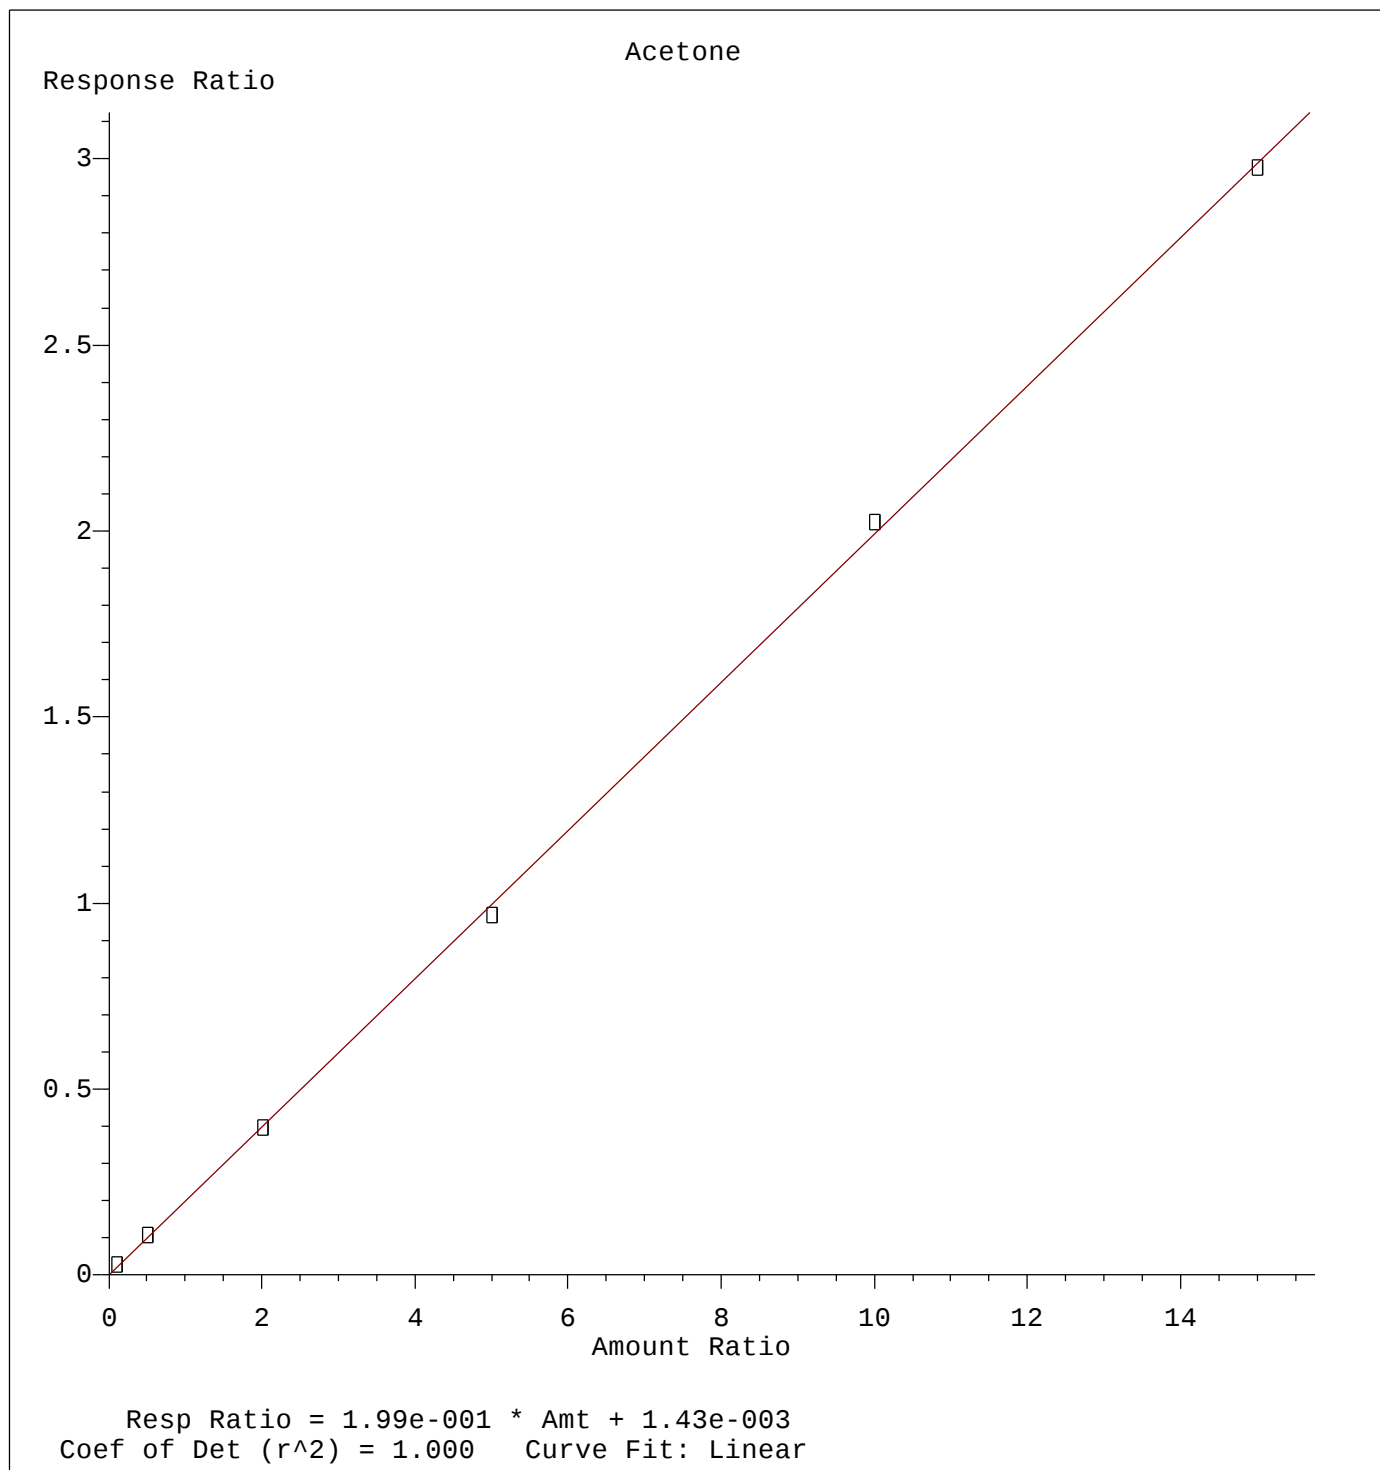

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018


Acrolein

Response Ratio

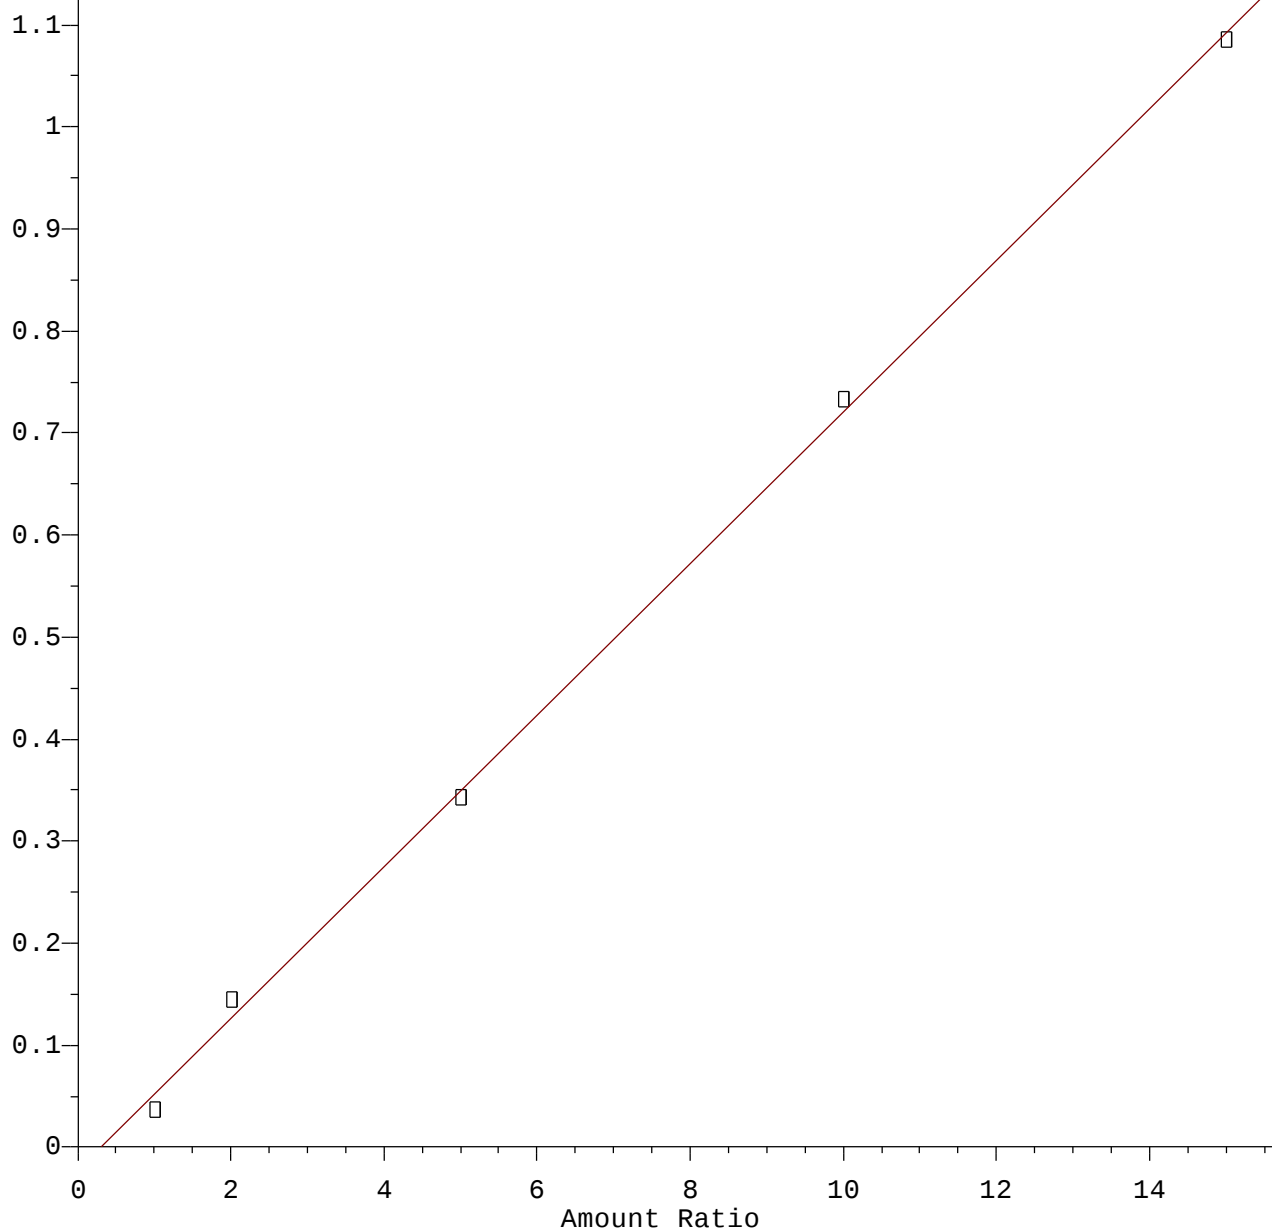

Resp Ratio = 7.43×10^{-2} * Amt - 2.23×10^{-2}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018

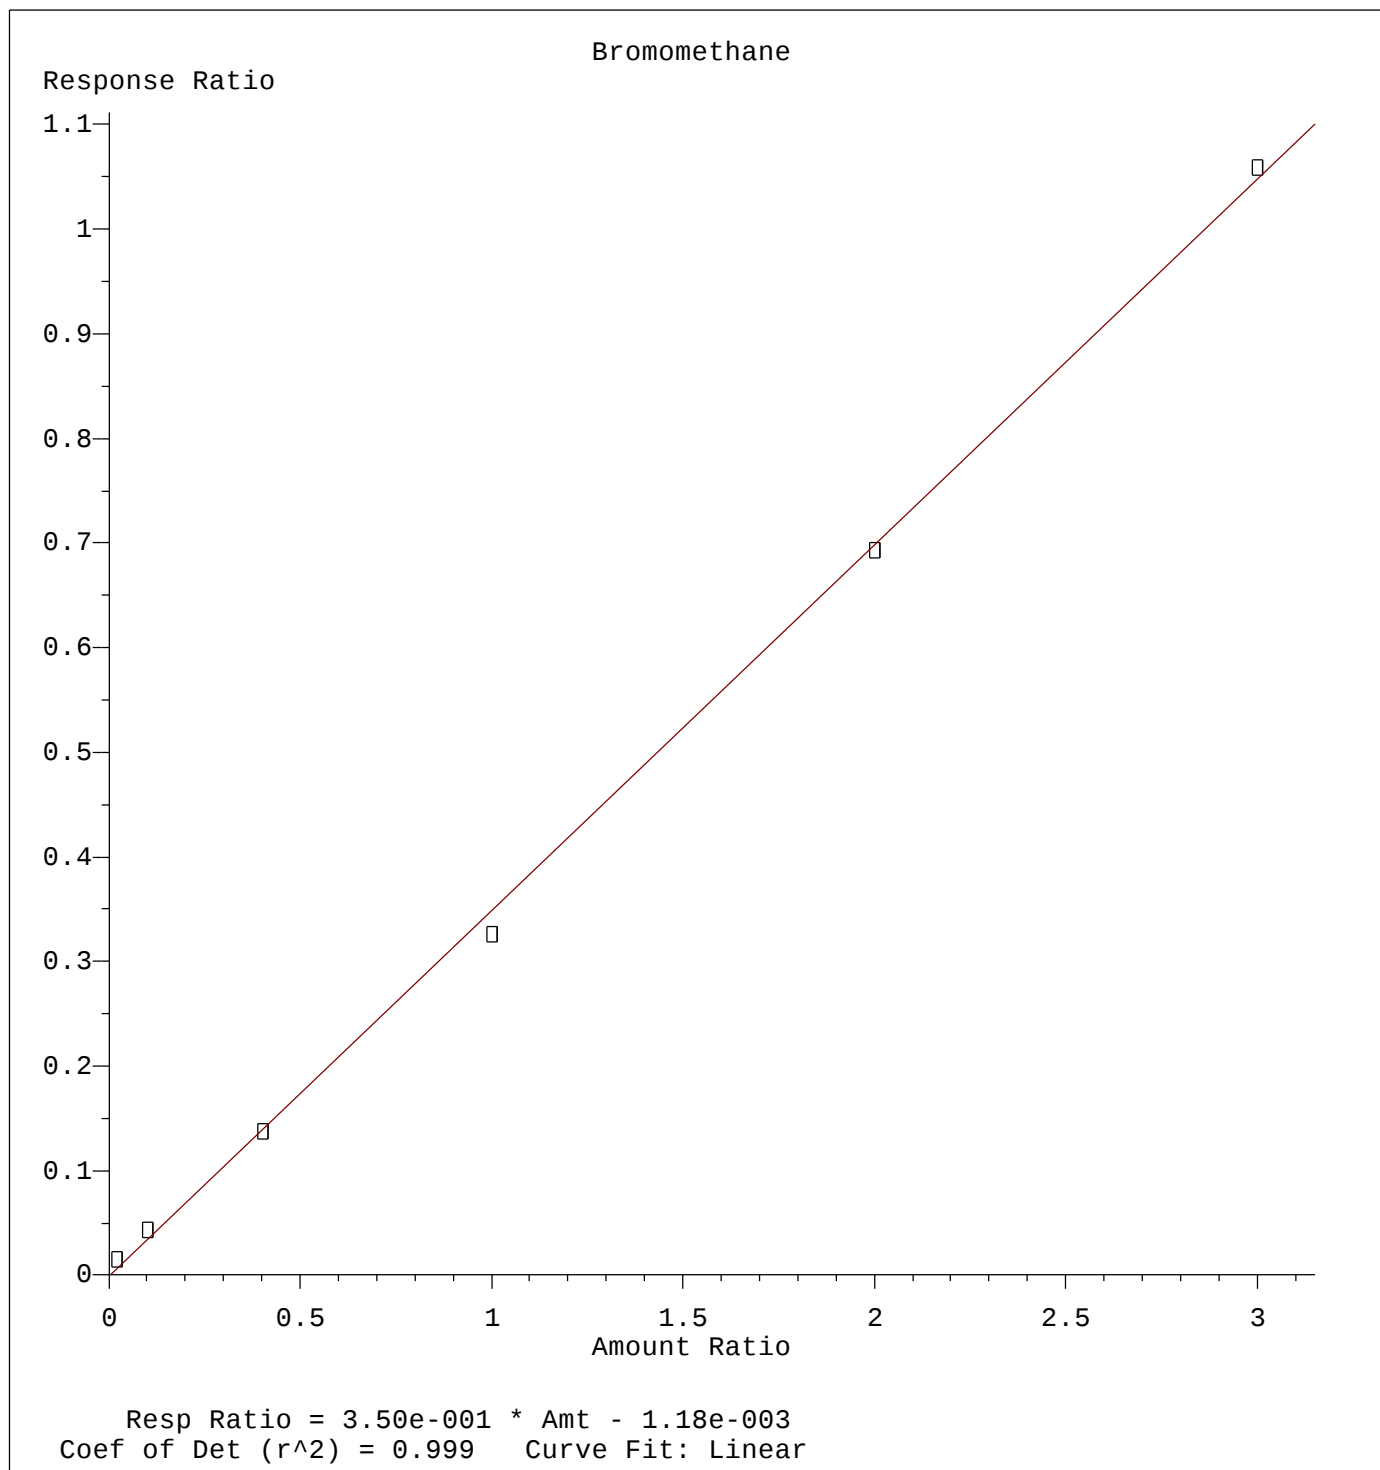

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Calibration Table Last Updated: Tue Aug 07 05:22:15 2018