


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080618\
Data File : VN050374.D
Acq On : 6 Aug 2018 9:43
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Title : SW846 8260
Last Update : Tue Aug 07 05:22:15 2018

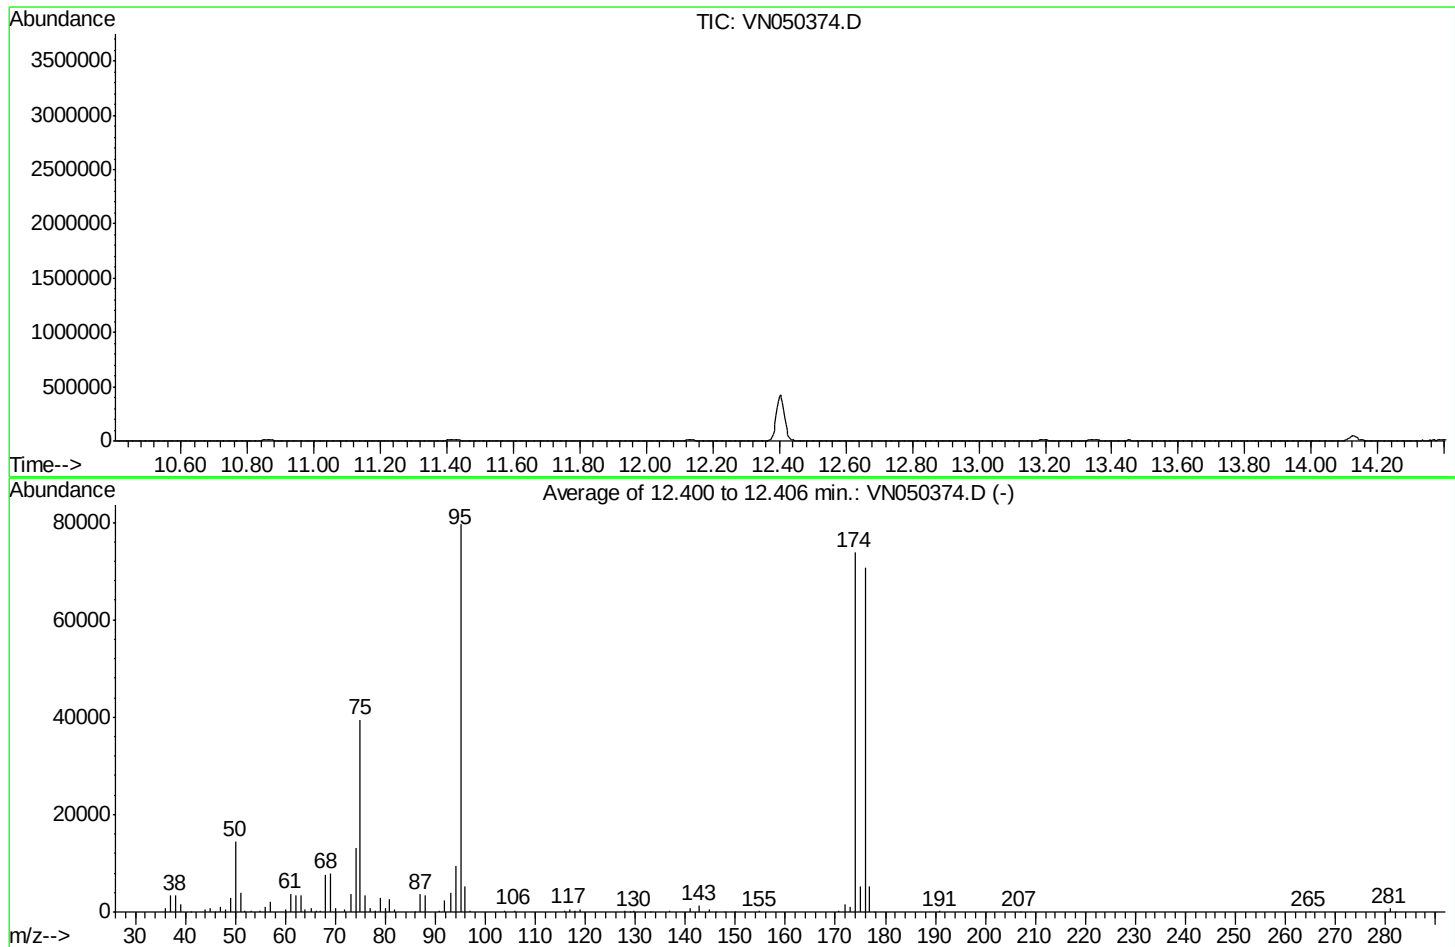

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	14410	PASS
75	95	30	60	49.6	39469	PASS
95	95	100	100	100.0	79586	PASS
96	95	5	9	6.5	5152	PASS
173	174	0.00	2	1.4	1024	PASS
174	95	50	100	92.7	73778	PASS
175	174	5	9	7.2	5281	PASS
176	174	95	101	95.8	70653	PASS
177	176	5	9	7.3	5176	PASS