


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN080620\
Data File : VN062760.D
Acq On : 6 Aug 2020 12:09
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080520W.M
Title : SW846 8260
Last Update : Wed Aug 05 13:26:42 2020

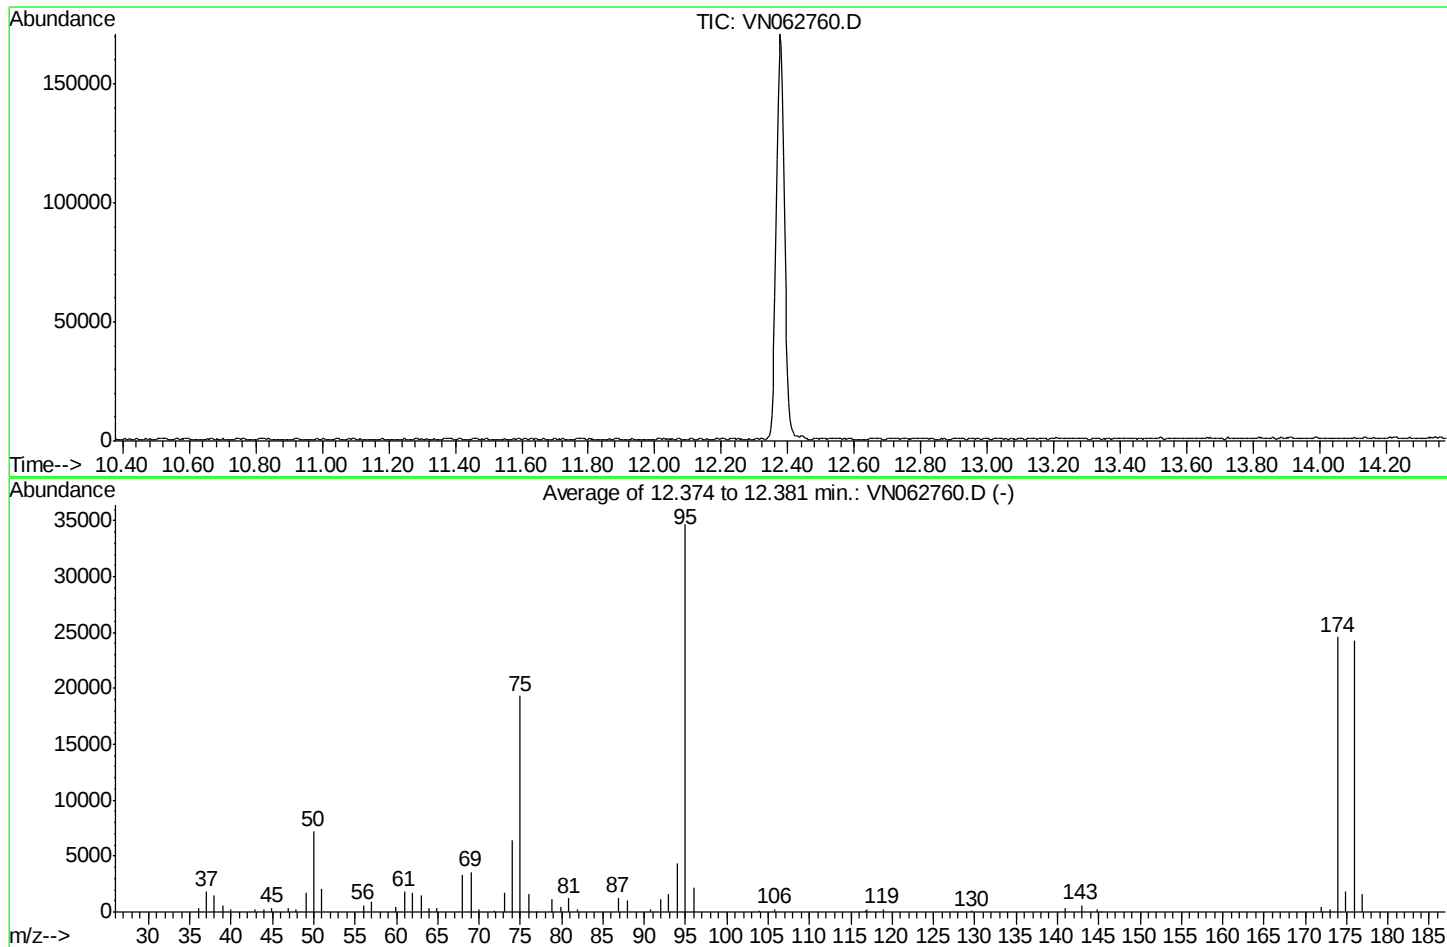

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3283

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	7172	PASS
75	95	30	60	55.7	19298	PASS
95	95	100	100	100.0	34677	PASS
96	95	5	9	6.3	2173	PASS
173	174	0.00	2	1.1	281	PASS
174	95	50	100	70.9	24584	PASS
175	174	5	9	7.5	1855	PASS
176	174	95	101	98.7	24256	PASS
177	176	5	9	6.6	1610	PASS