


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN080718\
Data File : VN050422.D
Acq On : 7 Aug 2018 11:04
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080618W.M
Title : SW846 8260
Last Update : Tue Aug 07 05:22:15 2018

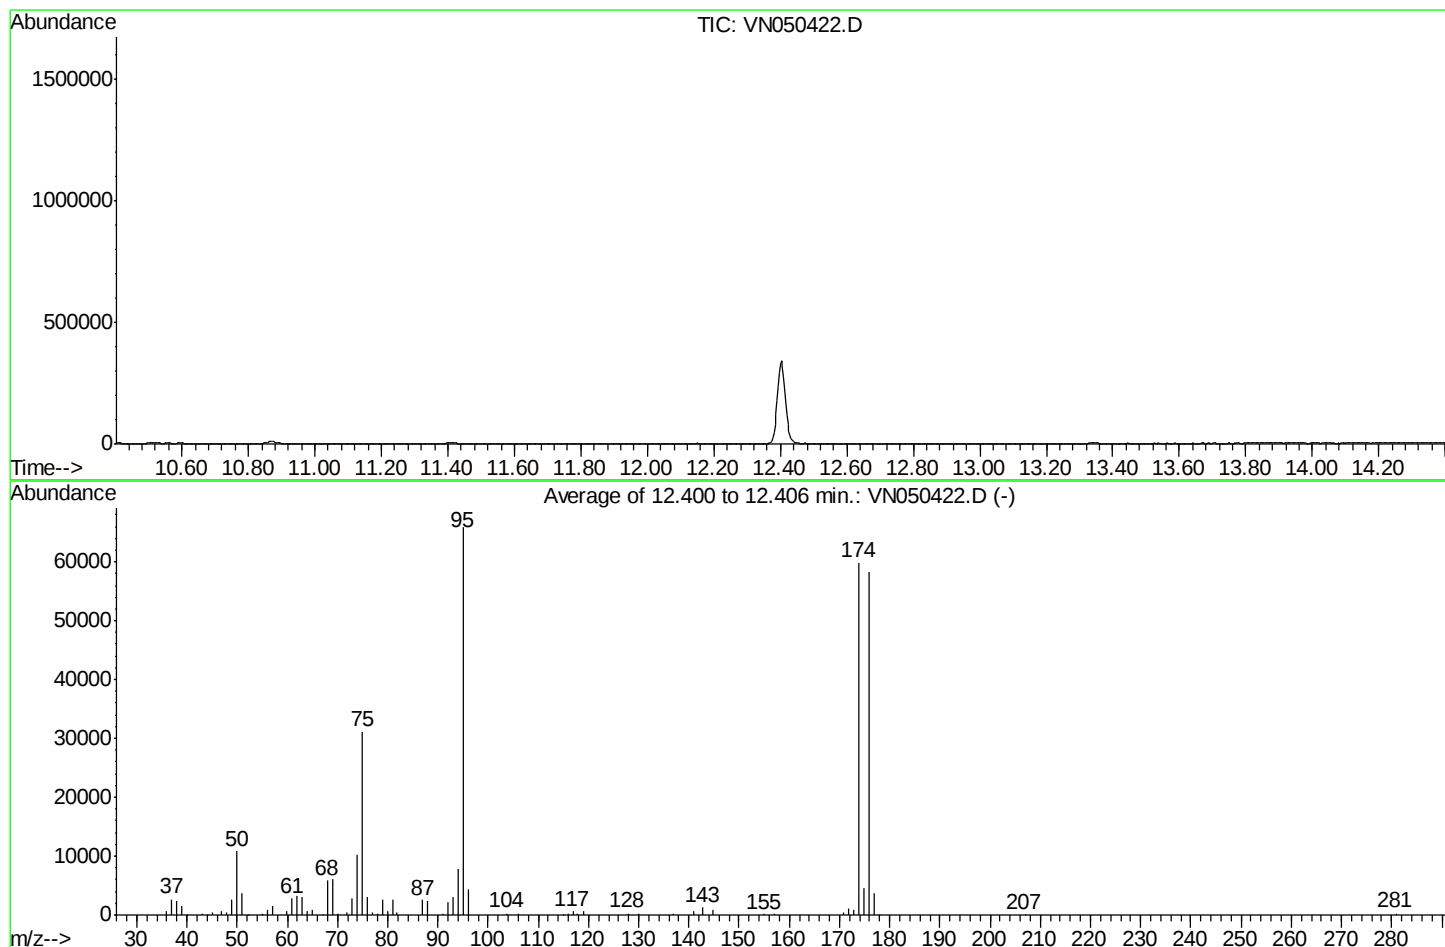

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	10867	PASS
75	95	30	60	47.4	31202	PASS
95	95	100	100	100.0	65861	PASS
96	95	5	9	6.6	4341	PASS
173	174	0.00	2	1.5	922	PASS
174	95	50	100	91.0	59901	PASS
175	174	5	9	7.5	4501	PASS
176	174	95	101	97.2	58197	PASS
177	176	5	9	6.4	3747	PASS