

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080720\
 Data File : VN062787.D
 Acq On : 7 Aug 2020 18:29
 Operator : JC/MD
 Sample : PB130790ZHE#04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130790ZHE#04

Quant Time: Aug 08 02:14:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080520W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 05 13:26:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	131631	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	244984	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	251659	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	88190	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	113932	52.34	ug/l	0.00
Spiked Amount			Recovery	=	104.68%	
35) Dibromofluoromethane	7.55	113	81971	48.91	ug/l	0.00
Spiked Amount			Recovery	=	97.82%	
50) Toluene-d8	10.06	98	320300	48.96	ug/l	0.00
Spiked Amount			Recovery	=	97.92%	
62) 4-Bromofluorobenzene	12.38	95	114806	46.43	ug/l	0.00
Spiked Amount			Recovery	=	92.86%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
8) Diethyl Ether	3.38	74	862	1.012	ug/l	98
11) Tert butyl alcohol	4.69	59	345	0.967	ug/l #	72
16) Acetone	3.78	43	12065	15.339	ug/l	92
17) Carbon Disulfide	4.01	76	77	Below Cal	#	74
18) Methyl Acetate	4.28	43	4289	1.203	ug/l #	61
20) Methylene Chloride	4.51	84	12449	8.010	ug/l	98
25) 2-Butanone	6.80	43	2248	2.018	ug/l	91
29) Tetrahydrofuran	7.17	42	206	0.285	ug/l #	45
31) Cyclohexane	7.63	56	3266	1.238	ug/l #	7
36) 1,1-Dichloropropene	7.63	75	11306	4.740	ug/l #	52
37) Ethyl Acetate	6.80	43	2248	0.902	ug/l #	67
38) Carbon Tetrachloride	7.63	117	14052	4.981	ug/l #	15
43) Isopropyl Acetate	8.13	43	48915	11.769	ug/l	97
45) 1,2-Dichloropropane	9.24	63	1058	0.549	ug/l #	45
48) Methyl methacrylate	9.15	41	3285	1.607	ug/l #	13
51) 4-Methyl-2-Pentanone	9.96	43	5967	2.219	ug/l	93
54) cis-1,3-Dichloropropene	9.88	75	20487	6.543	ug/l #	64
56) Ethyl methacrylate	10.52	69	1395	0.494	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	3890	1.220	ug/l #	43
59) 2-Hexanone	10.74	43	56110	27.972	ug/l #	53
74) N-amyl acetate	12.01	43	2096	0.779	ug/l #	44
76) 1,2,3-Trichloropropane	12.38	75	61461	25.841	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	2690	0.467	ug/l	91
81) trans-1,4-Dichloro-2-buten	12.38	75	61461	78.887	ug/l #	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN080720\
Data File : VN062787.D
Acq On : 7 Aug 2020 18:29
Operator : JC/MD
Sample : PB130790ZHE#04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB130790ZHE#04

Quant Time: Aug 08 02:14:54 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N080520W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 05 13:26:42 2020
Response via : Initial Calibration

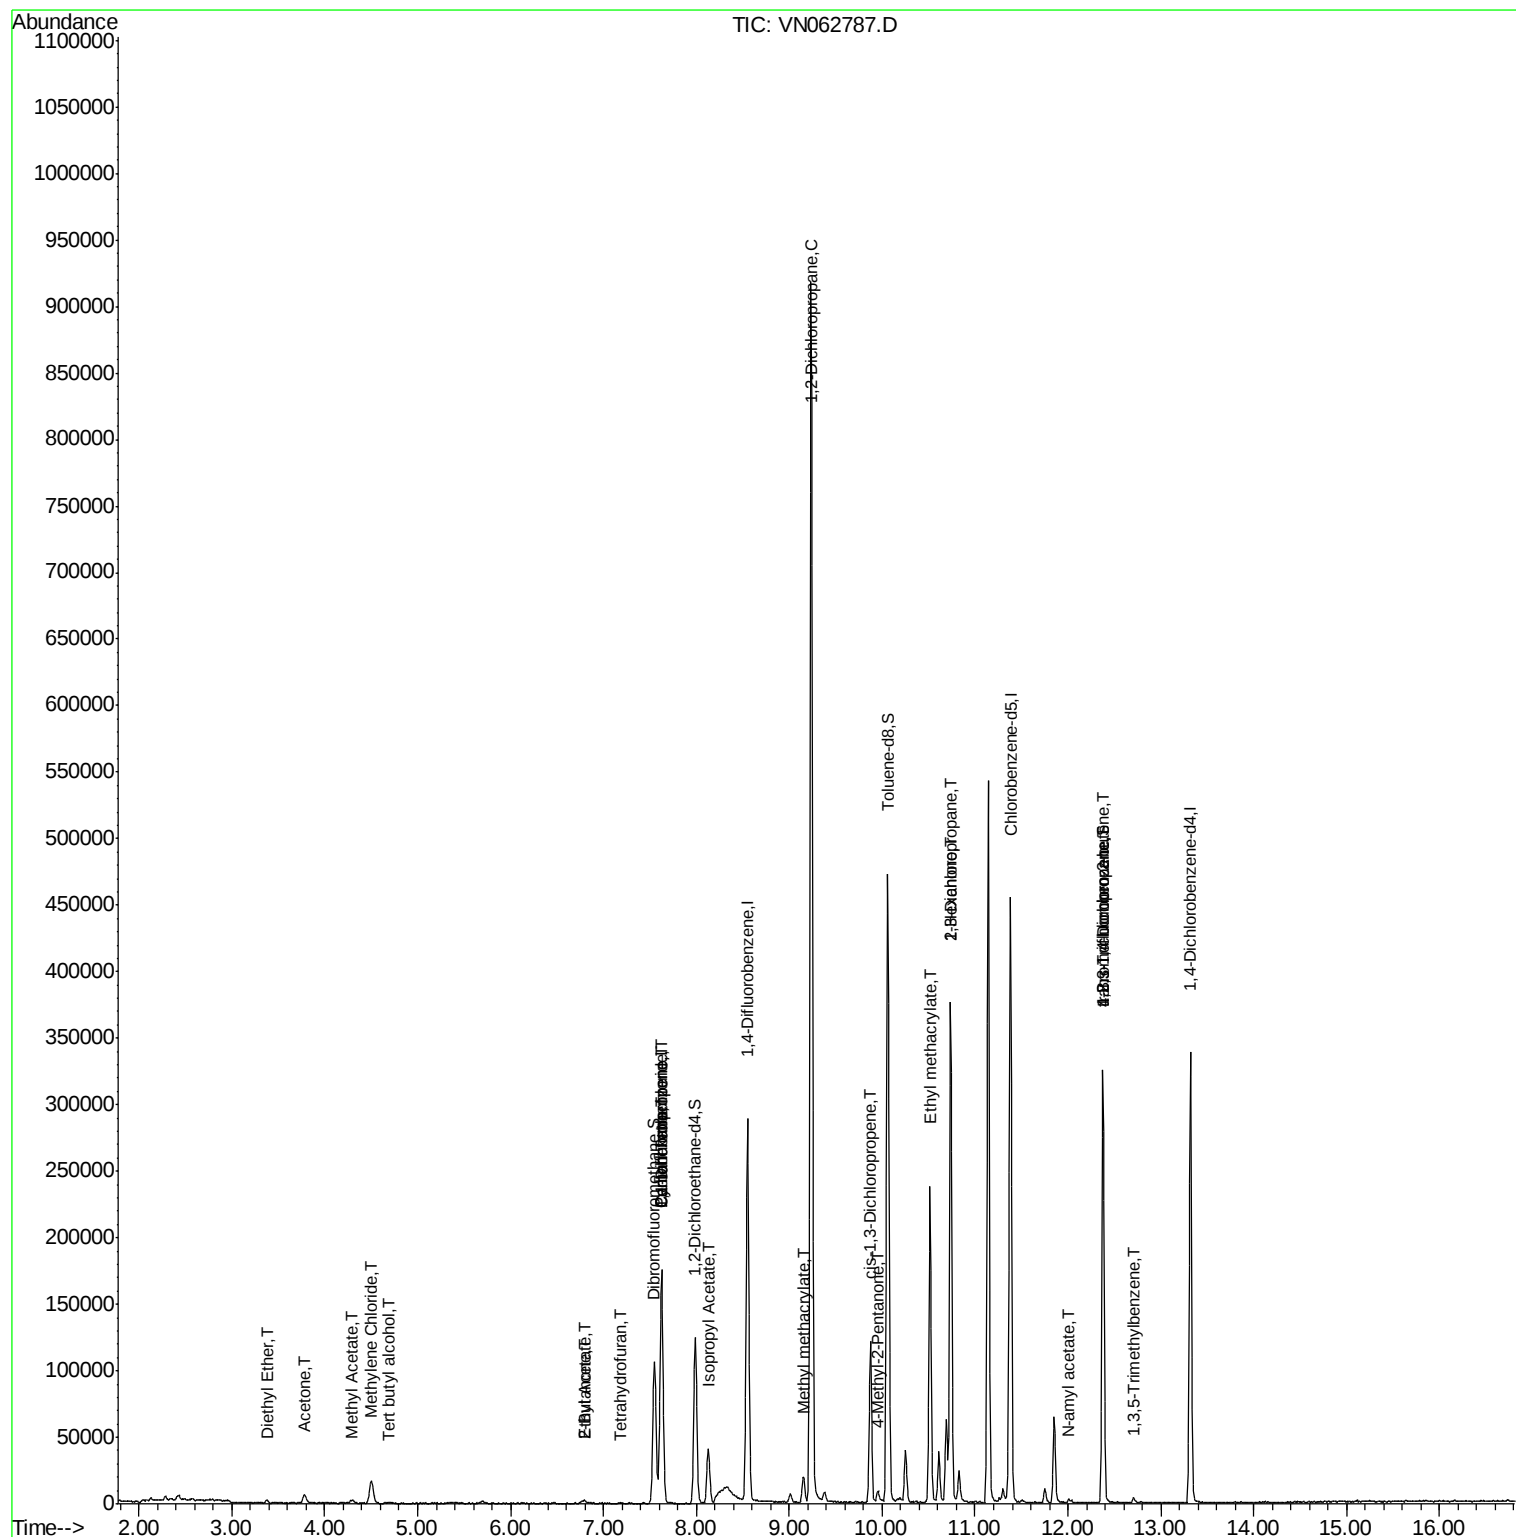

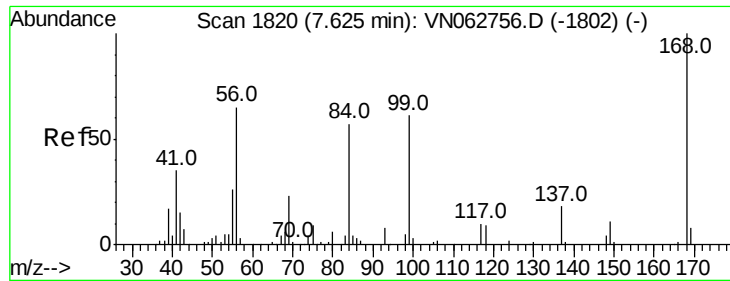

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Instrument :

MSVOA_N

ClientSampleId :


PB130790ZHE#04

Tot Ion:168 Resp: 131631




Ion Ratio Lower Upper

168 100

99 62.5 52.9 79.3

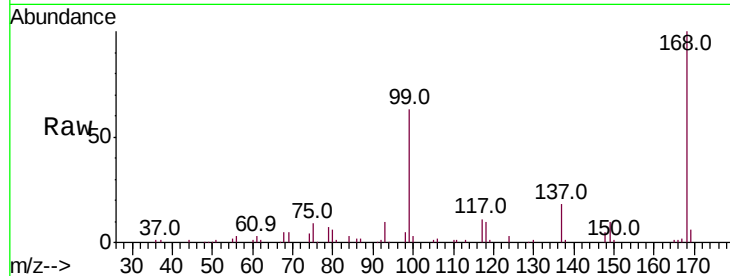

Abundance Ion 167.90 (167.60 to 168.60): VN062756.D (-1802) (-)

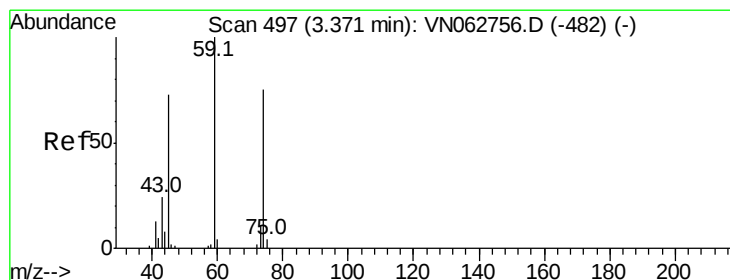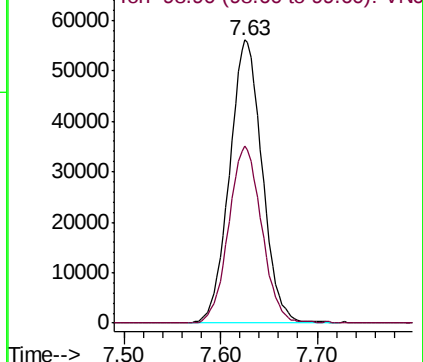

#8

Diethyl Ether

Concen: 1.012 ug/l

RT: 3.38 min Scan# 500

Delta R.T. 0.01 min

Lab File: VN062787.D


Acq: 7 Aug 2020 18:29

Tgt Ion: 74 Resp: 862



Ion Ratio Lower Upper


74 100

45 99.3 48.7 146.1

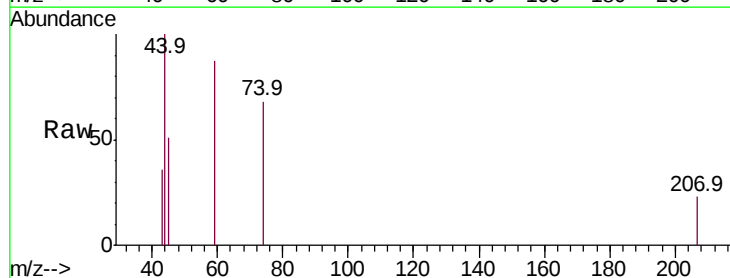

Abundance Ion 74.00 (73.70 to 74.70): VN062756.D (-482) (-)

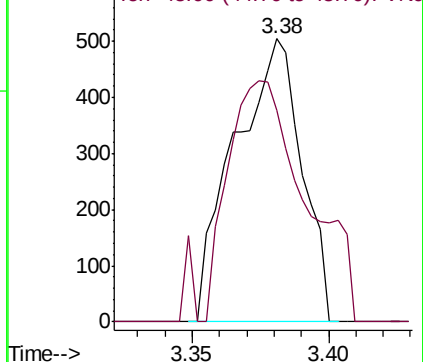




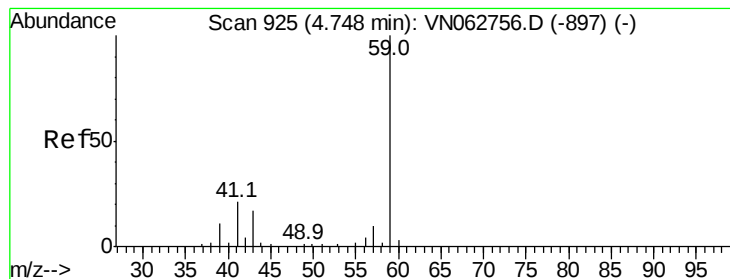


#11

Tert butyl alcohol
 Concen: 0.967 ug/l
 RT: 4.69 min Scan# 907
 Delta R.T. -0.06 min
 Lab File: VN062787.D
 Acq: 7 Aug 2020 18:29

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130790ZHE#04




Tot Ion: 59 Resp: 345
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.3 12.5#

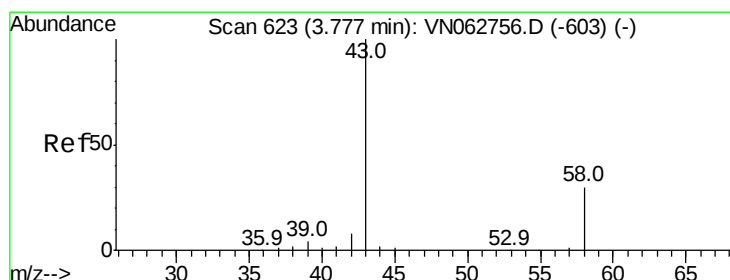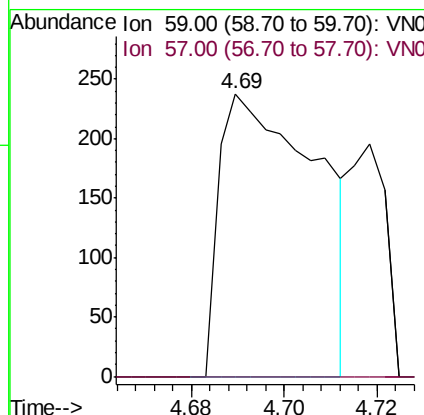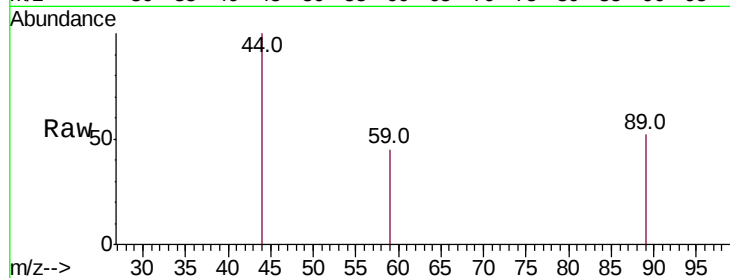


#16

Acetone
 Concen: 15.339 ug/l
 RT: 3.78 min Scan# 625
 Delta R.T. 0.01 min
 Lab File: VN062787.D
 Acq: 7 Aug 2020 18:29

Tgt Ion: 43 Resp: 12065
 Ion Ratio Lower Upper
 43 100
 58 25.8 24.1 36.1

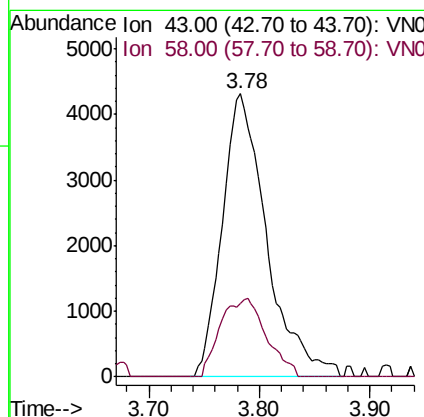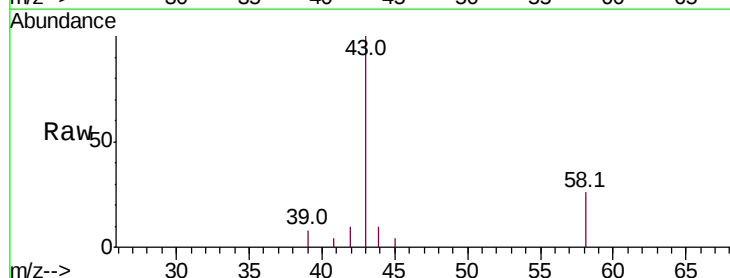

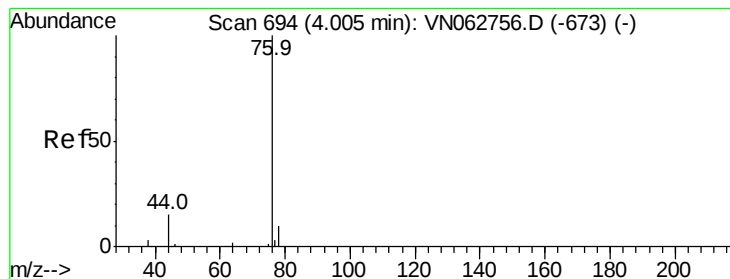

#17

Carbon Disulfide

Concen: Below Cal

RT: 4.01 min Scan# 695

Delta R.T. 0.00 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Instrument :

MSVOA_N

ClientSampleId :


PB130790ZHE#04

Tot Ion: 76 Resp: 77

Ion Ratio Lower Upper




76 100

78 0.0 7.7 11.5#

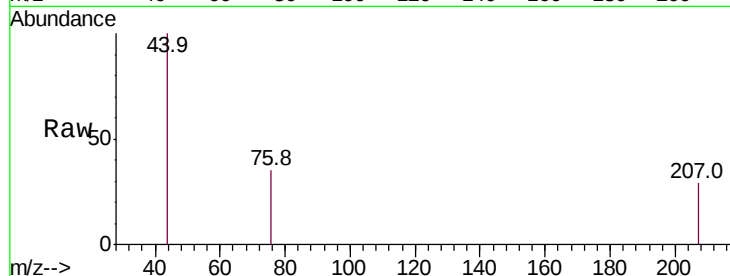

Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

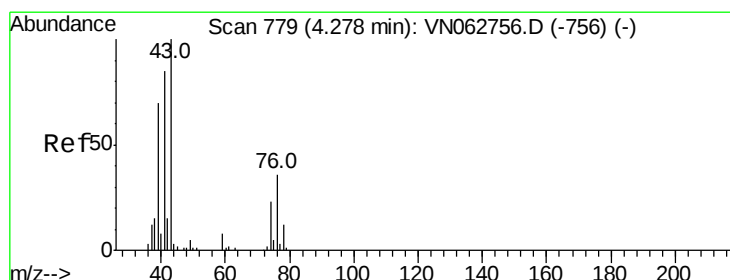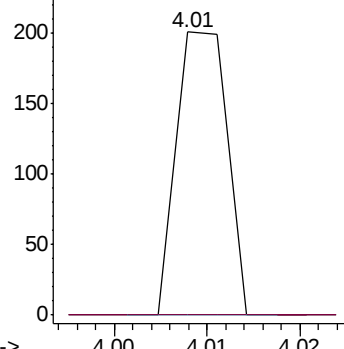

#18

Methyl Acetate

Concen: 1.203 ug/l

RT: 4.28 min Scan# 781

Delta R.T. 0.01 min

Lab File: VN062787.D


Acq: 7 Aug 2020 18:29

Tgt Ion: 43 Resp: 4289

Ion Ratio Lower Upper



43 100


74 4.3 18.6 28.0#

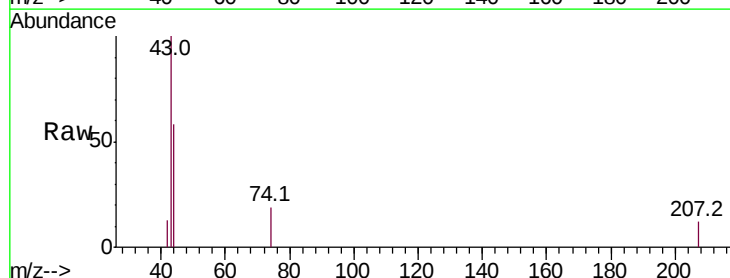

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 74.00 (73.70 to 74.70): VN0

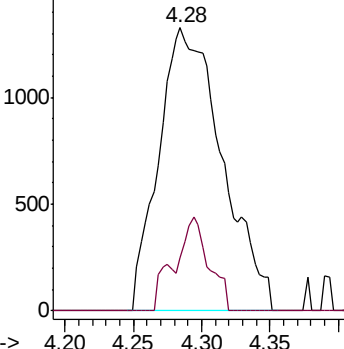

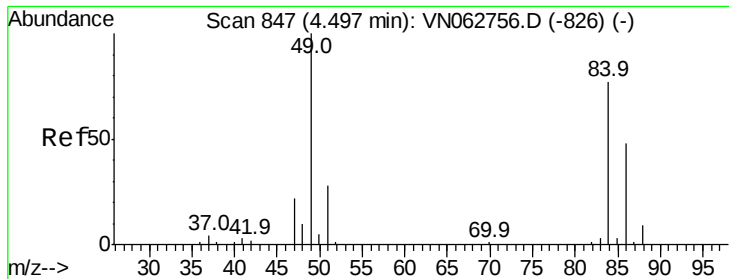

#20

Methvlene Chloride

Concen: 8.010 ug/l

RT: 4.51 min Scan# 850

Delta R.T. 0.01 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#04

Tot Ion: 84 Resp: 12449


Ion Ratio Lower Upper

84 100

49 126.3 103.4 155.2

51 36.1 29.3 43.9

86 64.7 49.9 74.9



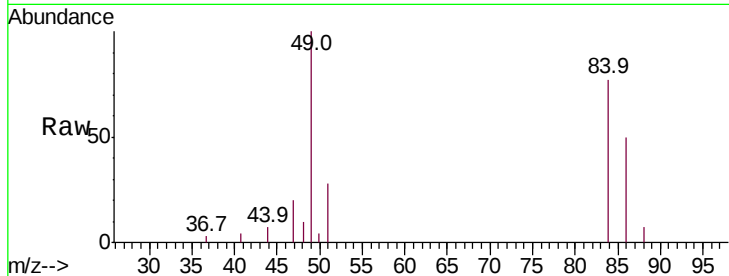


Abundance Ion 83.90 (83.60 to 84.60): VN0

Ion 48.90 (48.60 to 49.60): VN0

Ion 50.90 (50.60 to 51.60): VN0

Ion 85.90 (85.60 to 86.60): VN0

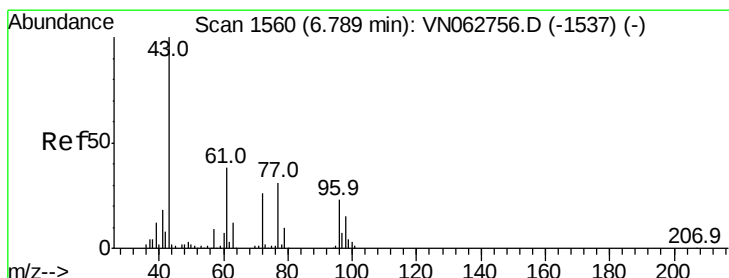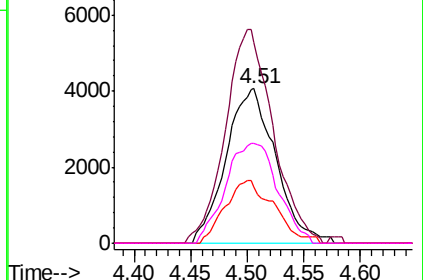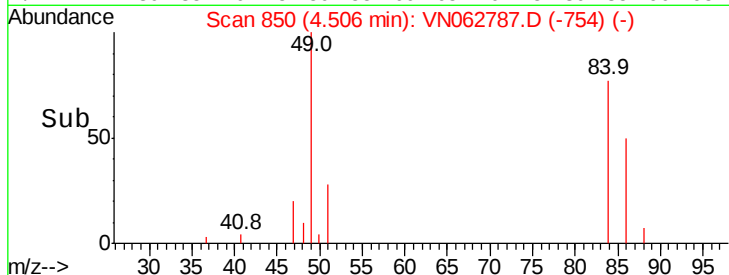

#25

2-Butanone

Concen: 2.018 ug/l

RT: 6.80 min Scan# 1563

Delta R.T. 0.01 min

Lab File: VN062787.D


Acq: 7 Aug 2020 18:29

Tgt Ion: 43 Resp: 2248

Ion Ratio Lower Upper



43 100


72 22.0 21.1 31.7

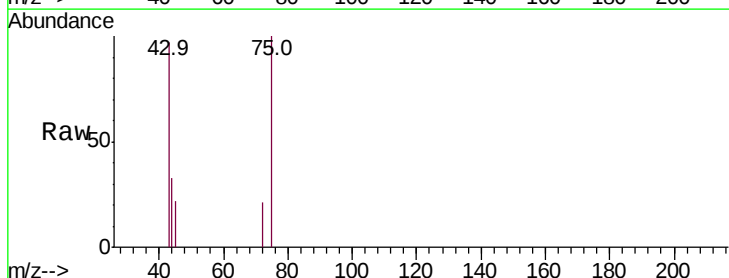

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

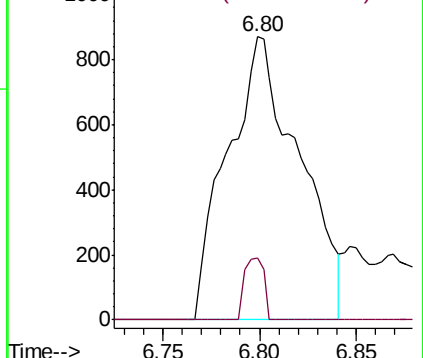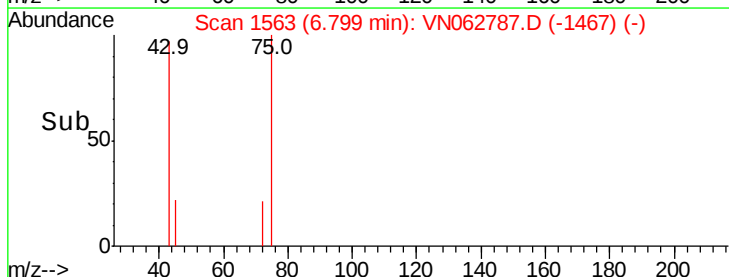



#29

Tetrahydrofuran

Concen: 0.285 ug/l

RT: 7.17 min Scan# 1679

Delta R.T. 0.00 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#04


Tot Ion: 42 Resp: 206

Ion Ratio Lower Upper

42 100

72 14.6 35.0 52.4#


71 0.0 33.2 49.8#





Abundance Ion 42.00 (41.70 to 42.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

Ion 71.00 (70.70 to 71.70): VN0

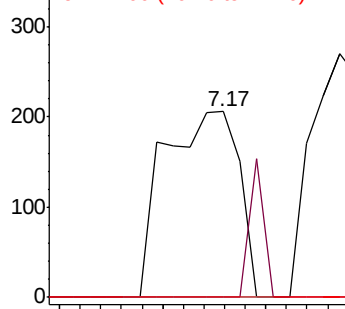

Time--> 7.14 7.16 7.18



#31

Cyclohexane

Concen: 1.238 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.01 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29


Tgt Ion: 56 Resp: 3266

Ion Ratio Lower Upper

56 100

69 189.9 28.1 42.1#


84 101.9 66.8 100.2#




Abundance Ion 56.00 (55.70 to 56.70): VN0


Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

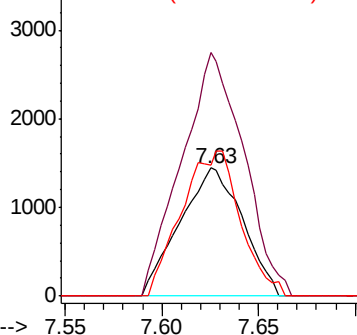

Time--> 7.55 7.60 7.65







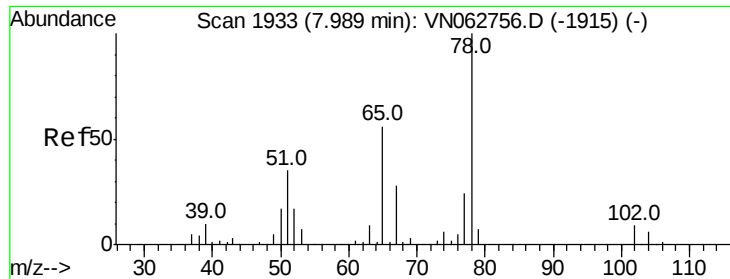

#33
 1,2-Dichloroethane-d4
 Concen: 52.340 ug/l
 RT: 7.99 min Scan# 1933
 Delta R.T. -0.00 min
 Lab File: VN062787.D
 Acq: 7 Aug 2020 18:29




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130790ZHE#04


Tot Ion: 65 Resp: 113932
 Ion Ratio Lower Upper
 65 100
 67 51.2 0.0 101.4

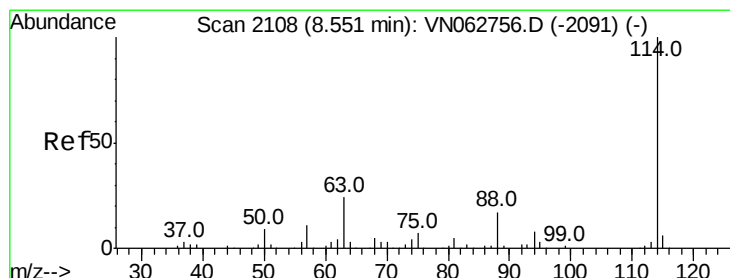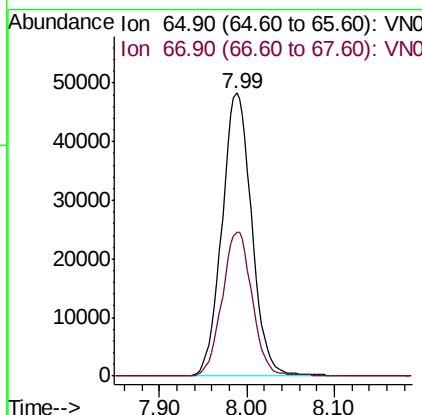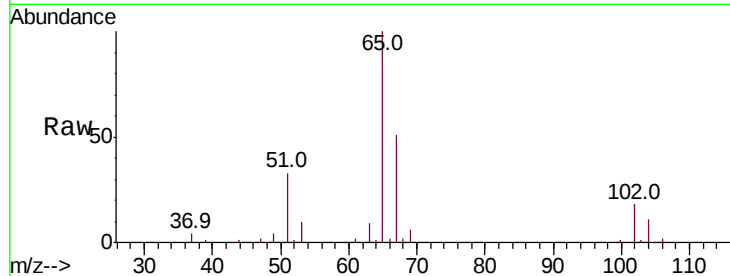

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. -0.00 min
 Lab File: VN062787.D
 Acq: 7 Aug 2020 18:29

Tgt Ion:114 Resp: 244984
 Ion Ratio Lower Upper
 114 100
 63 23.2 0.0 47.6
 88 16.8 0.0 34.4


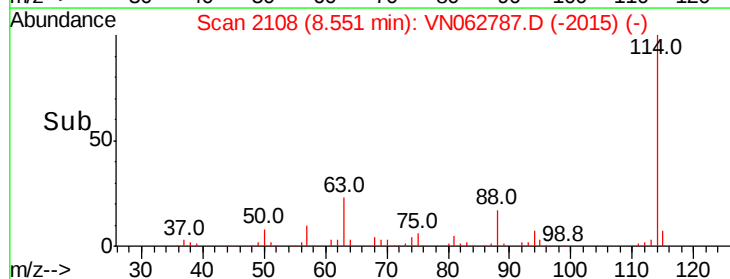
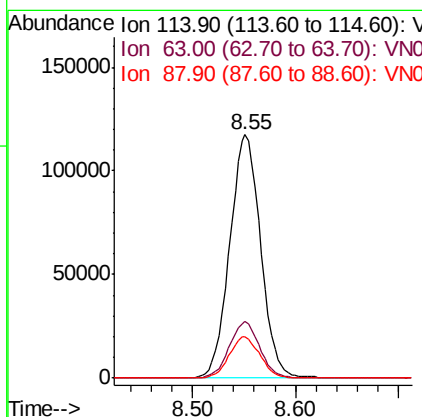
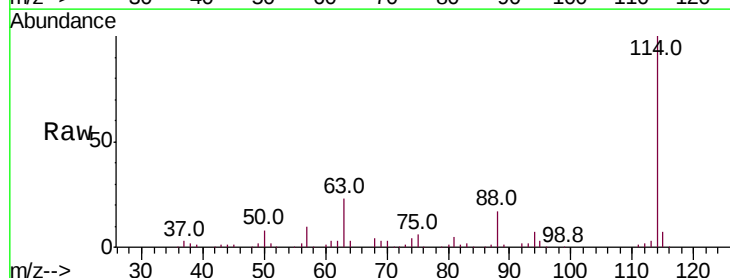




#35
 Dibromofluoromethane
 Concen: 48.914 ug/l
 RT: 7.55 min Scan# 1796
 Delta R.T. -0.00 min
 Lab File: VN062787.D
 Acq: 7 Aug 2020 18:29




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130790ZHE#04


Tot Ion:113 Resp: 81971
 Ion Ratio Lower Upper
 113 100
 111 102.8 81.8 122.6
 192 18.8 15.0 22.4

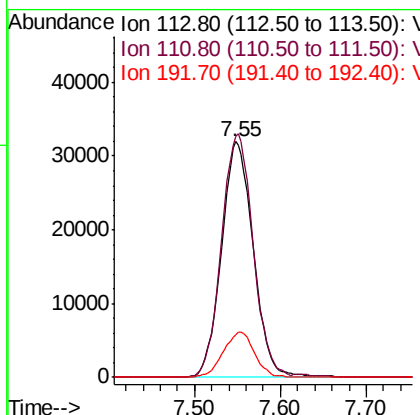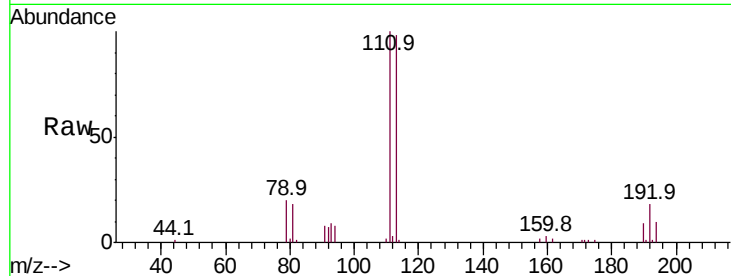

#36
 1,1-Dichloropropene
 Concen: 4.740 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.13 min
 Lab File: VN062787.D
 Acq: 7 Aug 2020 18:29

Tgt Ion: 75 Resp: 11306
 Ion Ratio Lower Upper
 75 100
 110 8.2 15.6 46.7#
 77 0.0 24.1 36.1#

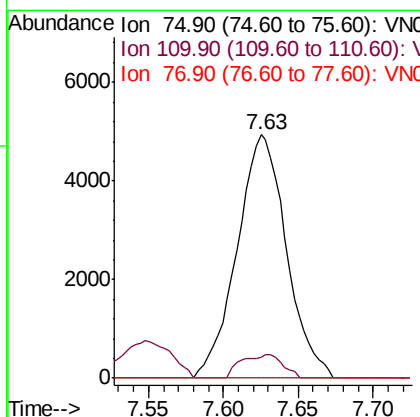



#37

Ethyl Acetate

Concen: 0.902 ug/l

RT: 6.80 min Scan# 1563

Delta R.T. -0.09 min


Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Instrument :
MSVOA_N
ClientSampleId :
PB130790ZHE#04

Tot Ion: 43 Resp: 2248

Ion	Ratio	Lower	Upper
43	100		
61	0.0	12.1	18.1#
70	0.0	8.3	12.5#



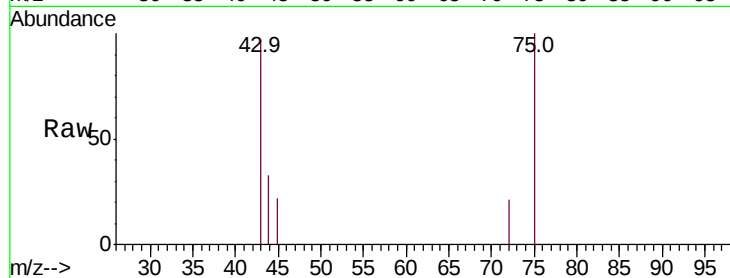


Abundance

Ion 43.00 (42.70 to 43.70): VN062756.D (-1577) (-)

Ion 60.90 (60.60 to 61.60): VN062756.D (-1577) (-)

Ion 70.00 (69.70 to 70.70): VN062756.D (-1577) (-)

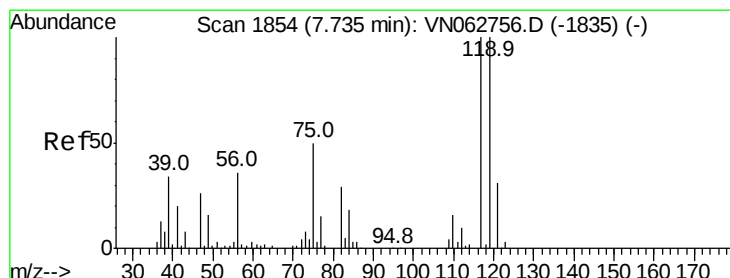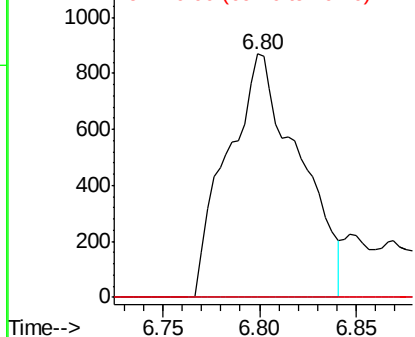

#38

Carbon Tetrachloride

Concen: 4.981 ug/l

RT: 7.63 min Scan# 1820


Delta R.T. -0.11 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Tgt Ion: 117 Resp: 14052

Ion	Ratio	Lower	Upper
117	100		
119	5.5	79.4	119.2#
121	0.0	24.9	37.3#


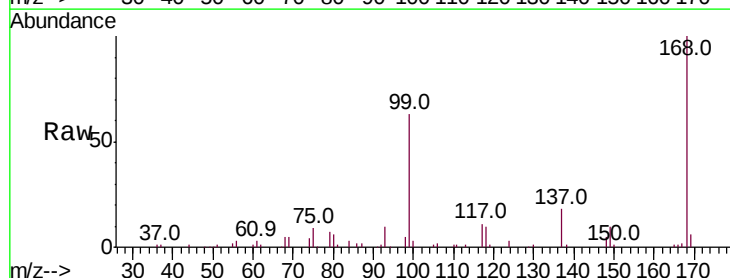



Abundance

Ion 116.80 (116.50 to 117.50): VN062756.D (-1835) (-)

Ion 118.80 (118.50 to 119.50): VN062756.D (-1835) (-)

Ion 120.80 (120.50 to 121.50): VN062756.D (-1835) (-)

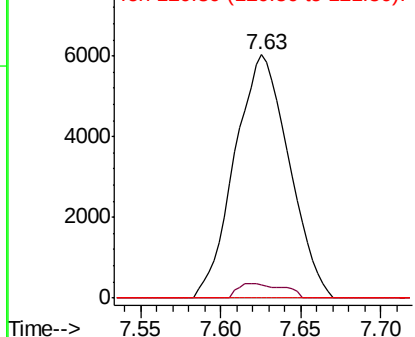



#43

Isopropyl Acetate

Concen: 11.769 ug/l

RT: 8.13 min Scan# 1977

Delta R.T. 0.00 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#04


Tot Ion: 43 Resp: 48915

Ion Ratio Lower Upper

43 100

61 18.1 15.8 23.6




87 11.9 9.9 14.9



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

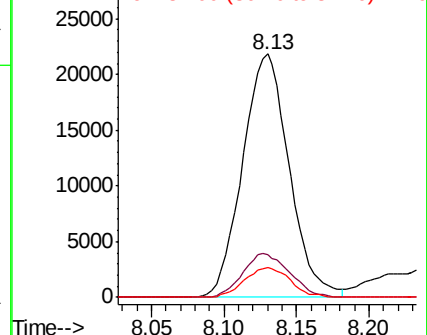

#45

1,2-Dichloropropane

Concen: 0.549 ug/l

RT: 9.24 min Scan# 2321

Delta R.T. 0.15 min

Lab File: VN062787.D


Acq: 7 Aug 2020 18:29

Tgt Ion: 63 Resp: 1058

Ion Ratio Lower Upper



63 100


65 0.0 23.5 35.3#



Abundance Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0




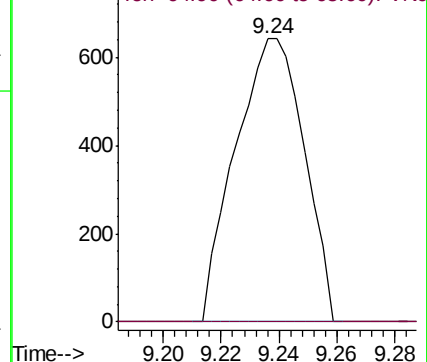




#48
Methvl methacrylate
Concen: 1.607 ug/l
RT: 9.15 min Scan# 2293
Delta R.T. -0.02 min
Lab File: VN062787.D
Acq: 7 Aug 2020 18:29




Instrument :
MSVOA_N
ClientSampleId :
PB130790ZHE#04


Tot Ion: 41 Resp: 3285
Ion Ratio Lower Upper
41 100
69 0.0 67.4 101.2#
39 0.0 47.6 71.4#

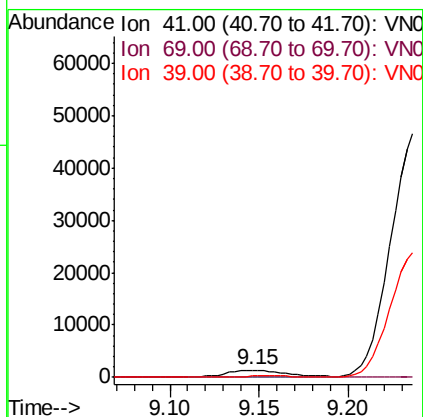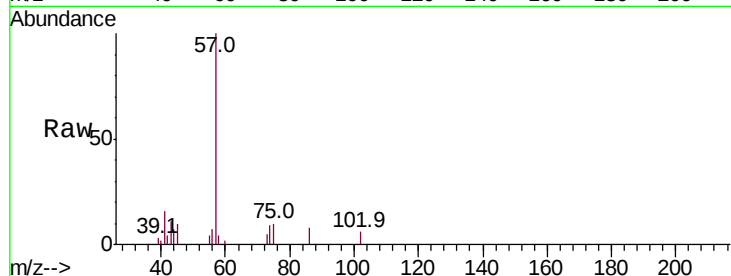

#50
Toluene-d8
Concen: 48.956 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. -0.00 min
Lab File: VN062787.D
Acq: 7 Aug 2020 18:29

Tgt Ion: 98 Resp: 320300
Ion Ratio Lower Upper
98 100
100 64.0 50.9 76.3



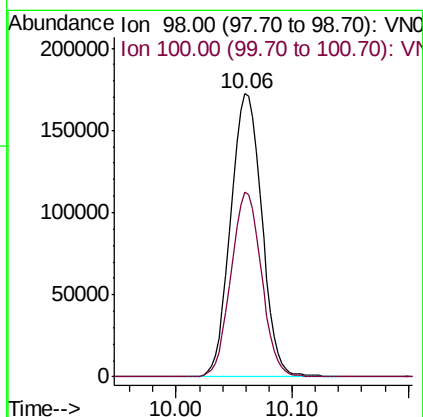





#51
 4-Methyl-2-Pentanone
 Concen: 2.219 ug/l
 RT: 9.96 min Scan# 2545
 Delta R.T. 0.00 min
 Lab File: VN062787.D
 Acq: 7 Aug 2020 18:29




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130790ZHE#04


Tot Ion: 43 Resp: 5967
 Ion Ratio Lower Upper
 43 100
 58 34.8 31.1 46.7

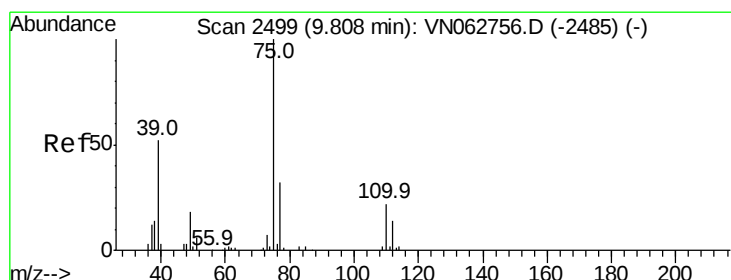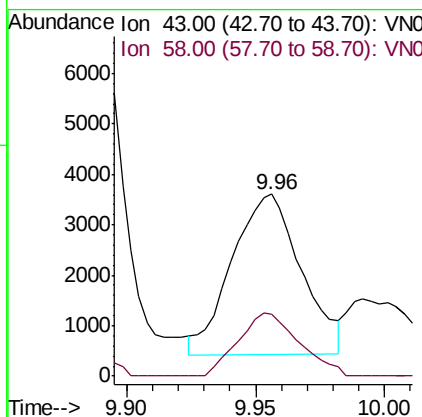

#54
 cis-1,3-Dichloropropene
 Concen: 6.543 ug/l
 RT: 9.88 min Scan# 2520
 Delta R.T. 0.07 min
 Lab File: VN062787.D
 Acq: 7 Aug 2020 18:29

Tgt Ion: 75 Resp: 20487
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.5 38.3#
 39 36.3 41.9 62.9#

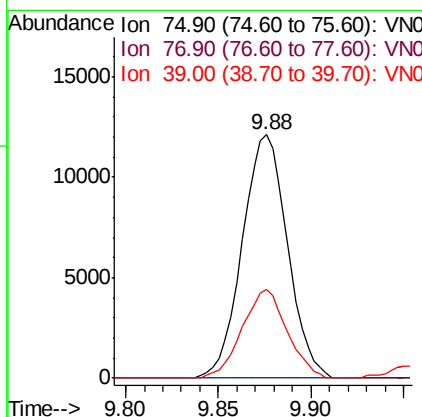



#56

Ethyl methacrylate

Concen: 0.494 ug/l

RT: 10.52 min Scan# 2719

Delta R.T. 0.11 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#04


Tot Ion: 69 Resp: 1395

Ion Ratio Lower Upper

69 100

41 3216.3 52.2 78.2#




39 1430.8 30.9 46.3#

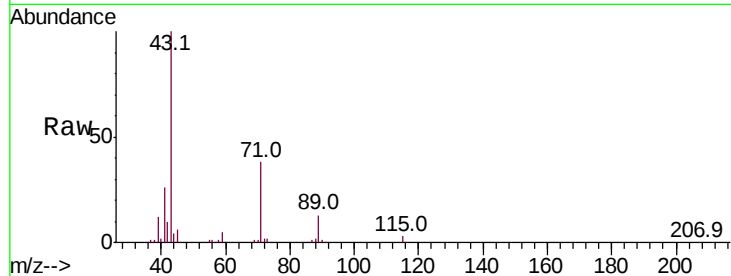

Abundance Ion 69.00 (68.70 to 69.70): VNO

Ion 41.00 (40.70 to 41.70): VNO

Ion 39.00 (38.70 to 39.70): VNO

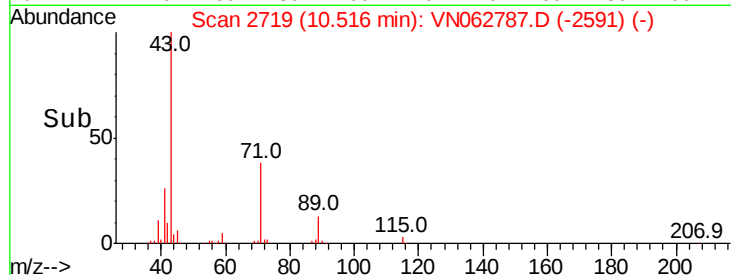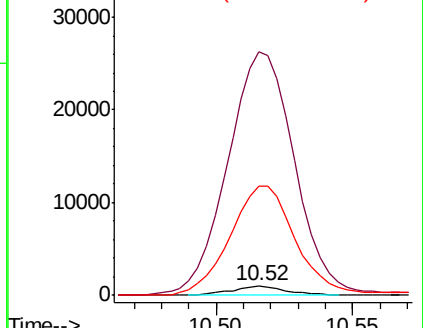

#57

1,3-Dichloropropane

Concen: 1.220 ug/l

RT: 10.74 min Scan# 2789

Delta R.T. 0.06 min

Lab File: VN062787.D


Acq: 7 Aug 2020 18:29

Tgt Ion: 76 Resp: 3890

Ion Ratio Lower Upper



76 100


78 0.0 25.4 38.0#



Abundance Ion 75.90 (75.60 to 76.60): VNO

Ion 77.90 (77.60 to 78.60): VNO




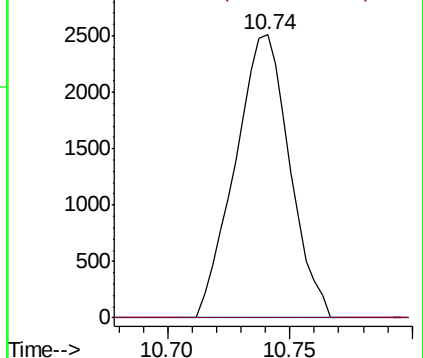




#59
2-Hexanone
Concen: 27.972 ug/l
RT: 10.74 min Scan# 2788
Delta R.T. 0.01 min
Lab File: VN062787.D
Acq: 7 Aug 2020 18:29




Instrument :
MSVOA_N
ClientSampleId :
PB130790ZHE#04


Tot Ion: 43 Resp: 56110
Ion Ratio Lower Upper
43 100
58 19.9 26.7 80.1#

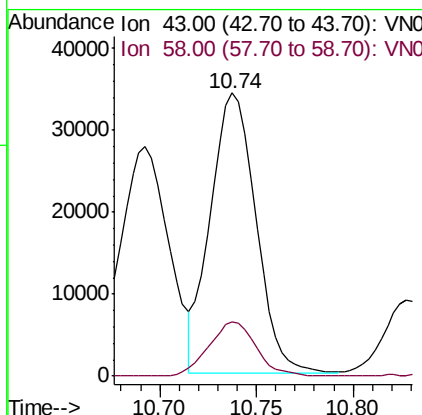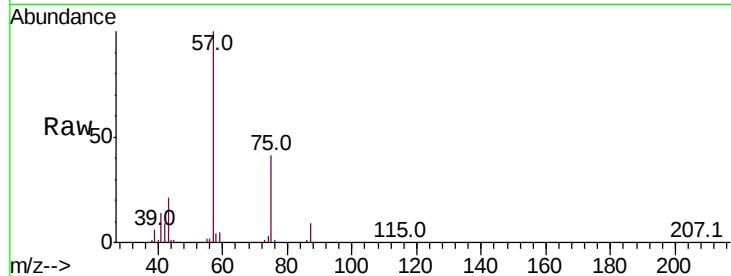

#62
4-Bromofluorobenzene
Concen: 46.434 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. -0.00 min
Lab File: VN062787.D
Acq: 7 Aug 2020 18:29

Tgt Ion: 95 Resp: 114806
Ion Ratio Lower Upper
95 100
174 75.1 0.0 144.8
176 71.8 0.0 142.2

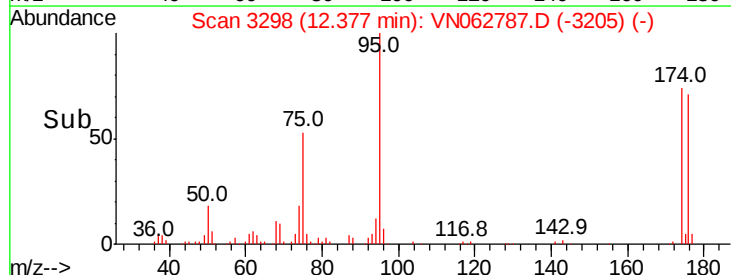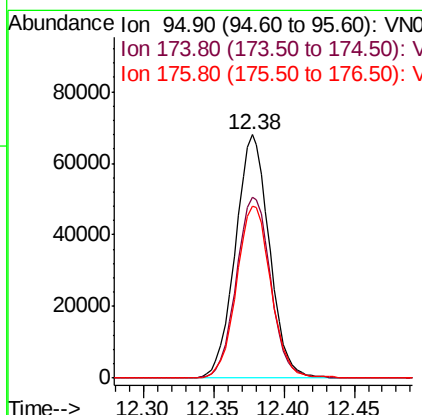



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2988

Delta R.T. -0.00 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#04


Tot Ion:117 Resp: 251659

Ion Ratio Lower Upper

117 100

82 59.5 49.0 73.4

119 33.5 26.2 39.2



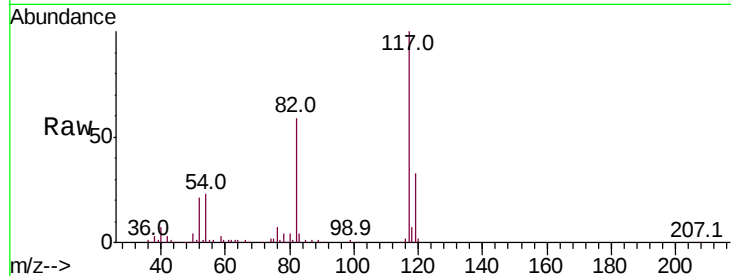


Abundance

Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

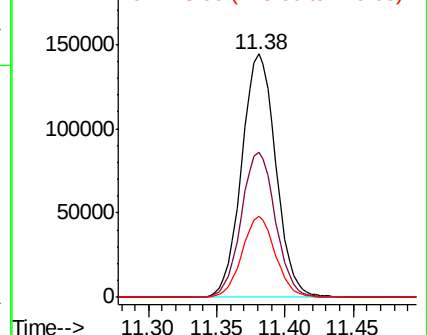

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. -0.00 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29


Tgt Ion:152 Resp: 88190

Ion Ratio Lower Upper

152 100

115 63.5 31.6 94.8

150 159.0 0.0 349.2






Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V




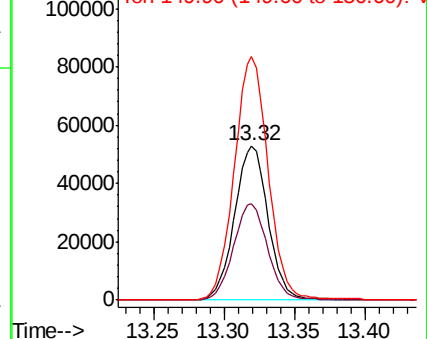




#74
N-amvl acetate
Concen: 0.779 ug/l
RT: 12.01 min Scan# 3183
Delta R.T. -0.04 min
Lab File: VN062787.D
Acq: 7 Aug 2020 18:29




Instrument :
MSVOA_N
ClientSampleId :
PB130790ZHE#04


Tot Ion: 43 Resp: 2096
Ion Ratio Lower Upper
43 100
70 0.0 32.3 48.5#
55 0.0 20.2 30.2#
61 0.0 18.2 27.4#

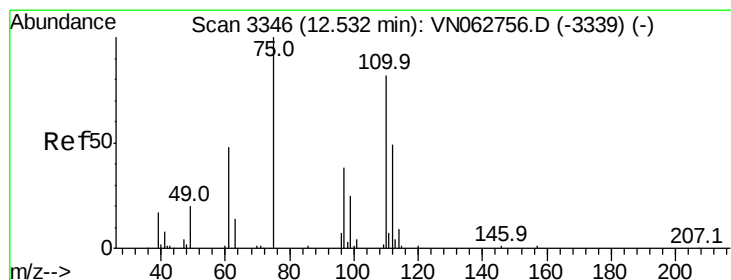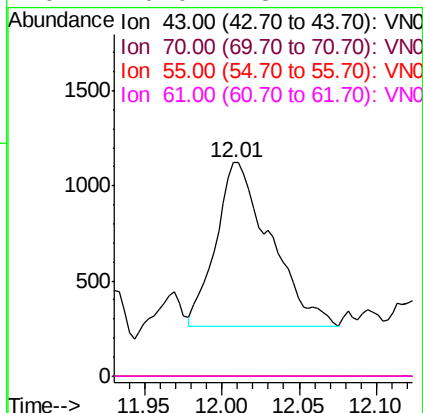

#76
1,2,3-Trichloropropane
Concen: 25.841 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. -0.15 min
Lab File: VN062787.D
Acq: 7 Aug 2020 18:29

Tgt Ion: 75 Resp: 61461
Ion Ratio Lower Upper
75 100
77 1.0 0.0 0.0#

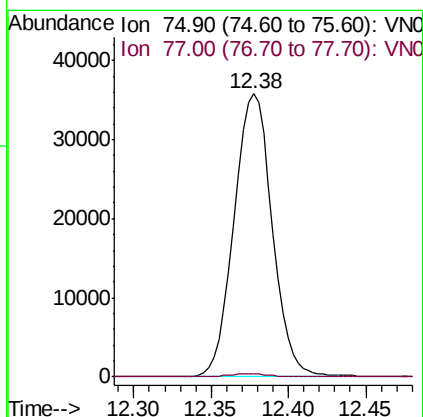



#80

1,3,5-Trimethylbenzene

Concen: 0.467 ug/l

RT: 12.71 min Scan# 3402

Delta R.T. 0.00 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29

Instrument :

MSVOA_N

ClientSampleId :


PB130790ZHE#04

Tot Ion:105 Resp: 2690

Ion Ratio Lower Upper




105 100

120 39.5 22.9 68.5

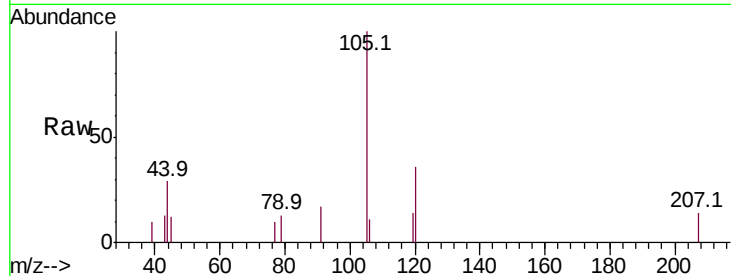

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

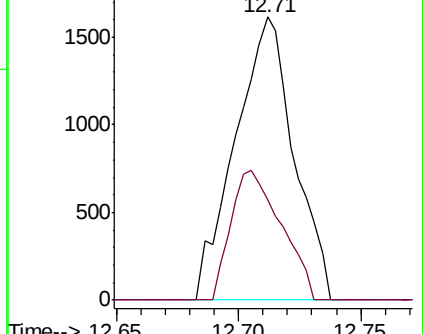

#81

trans-1,4-Dichloro-2-butene

Concen: 78.887 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.10 min

Lab File: VN062787.D

Acq: 7 Aug 2020 18:29


Tgt Ion: 75 Resp: 61461

Ion Ratio Lower Upper

75 100

53 0.0 79.1 118.7#

89 0.0 36.2 54.2#



Abundance Ion 74.90 (74.60 to 75.60): V

Ion 53.00 (52.70 to 53.70): V

Ion 88.90 (88.60 to 89.60): V

