

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN080720\
 Data File : VN062785.D
 Acq On : 7 Aug 2020 17:40
 Operator : JC/MD
 Sample : PB130790ZHE#02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130790ZHE#02

Quant Time: Aug 08 02:45:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080520W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 05 13:26:42 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	129660	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	233606	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	247166	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	85221	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	112465	52.45	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.90%	
35) Dibromofluoromethane	7.55	113	81603	51.07	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.14%	
50) Toluene-d8	10.06	98	312774	50.13	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.26%	
62) 4-Bromofluorobenzene	12.38	95	111730	47.39	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.78%	
Target Compounds						
16) Acetone	3.78	43	12049	15.552	ug/l	98
20) Methylene Chloride	4.50	84	13419	8.838	ug/l	92
43) Isopropyl Acetate	8.13	43	47876	12.080	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN080720\
Data File : VN062785.D
Acq On : 7 Aug 2020 17:40
Operator : JC/MD
Sample : PB130790ZHE#02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB130790ZHE#02

Quant Time: Aug 08 02:45:50 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N080520W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 05 13:26:42 2020
Response via : Initial Calibration

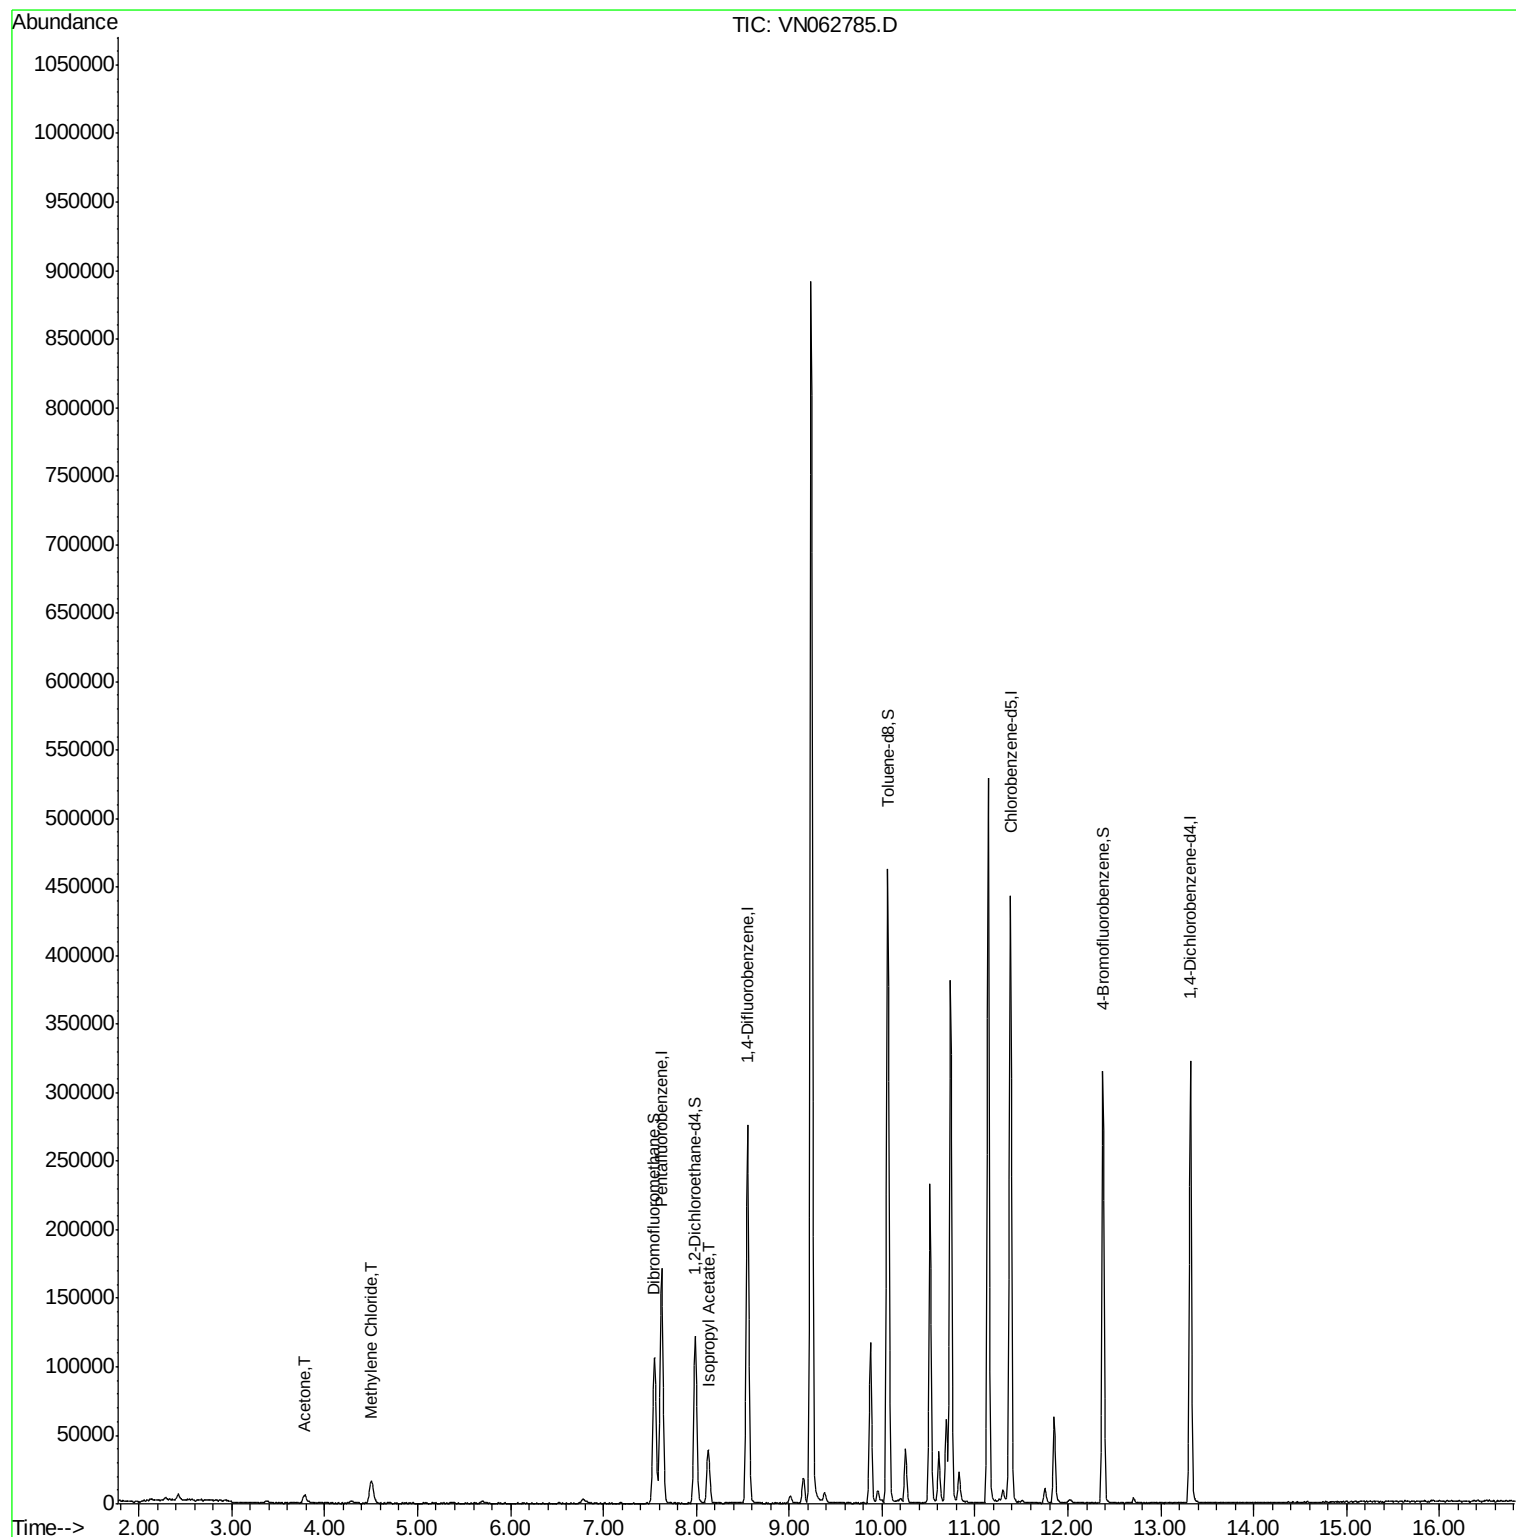

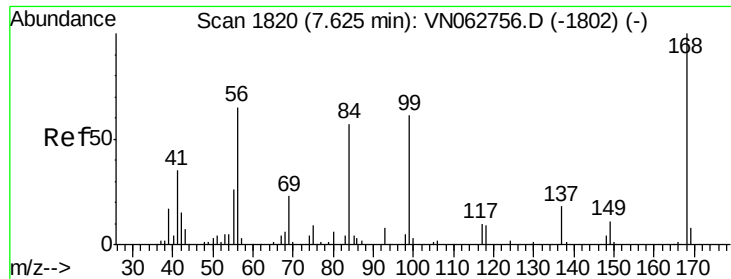

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.00 min

Lab File: VN062785.D

Acq: 7 Aug 2020 17:40

Instrument :

MSVOA_N

ClientSampleId :


PB130790ZHE#02

Tot Ion:168 Resp: 129660

Ion Ratio Lower Upper

168 100

99 63.3 52.9 79.3

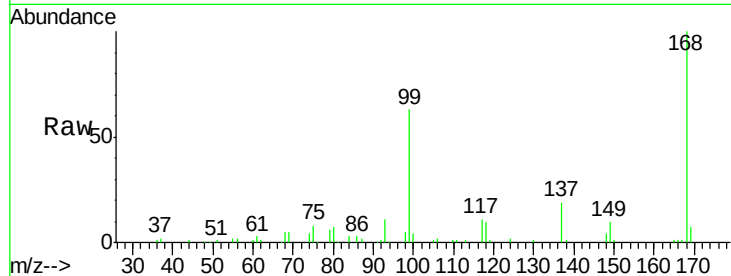

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.63

60000

50000

40000



30000

20000

10000

0

Time-->

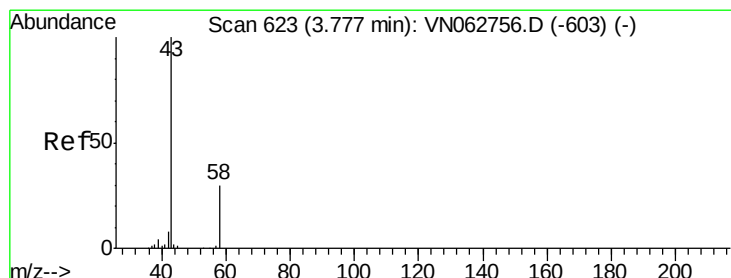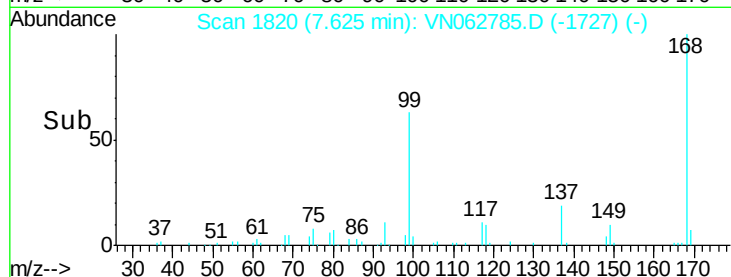

#16

Acetone

Concen: 15.552 ug/l

RT: 3.78 min Scan# 625

Delta R.T. 0.01 min

Lab File: VN062785.D


Acq: 7 Aug 2020 17:40

Tgt Ion: 43 Resp: 12049

Ion Ratio Lower Upper

43 100

58 31.1 24.1 36.1

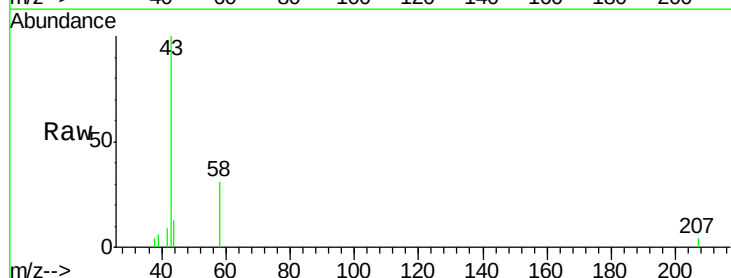

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

3.78

5000

4000


3000




2000

1000

0

Time-->

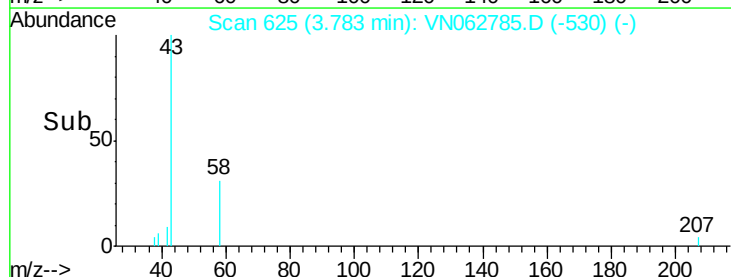

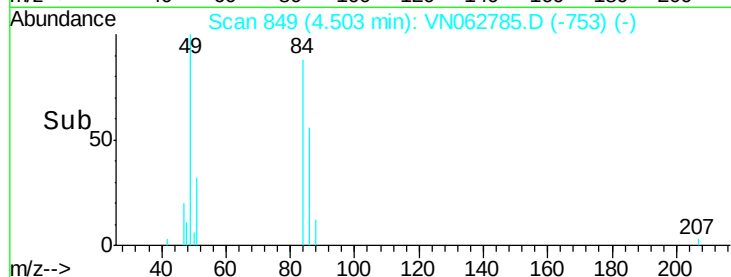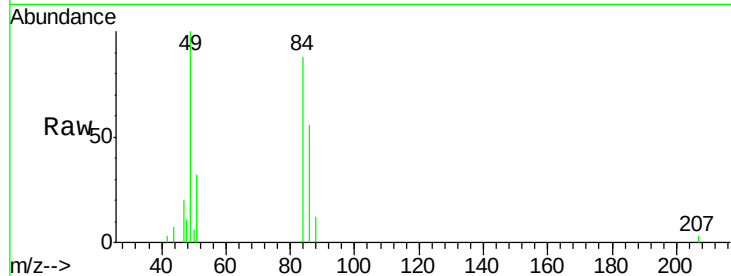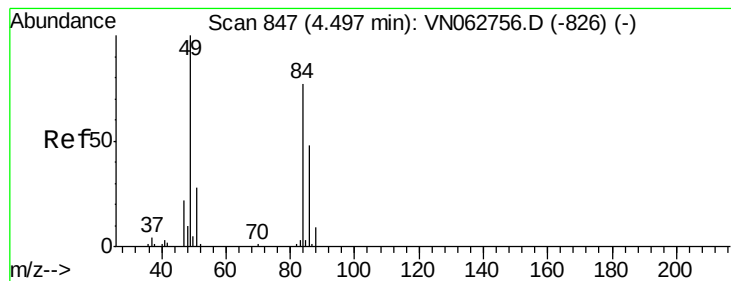

#20

Methylene Chloride

Concen: 8.838 ug/l

RT: 4.50 min Scan# 849

Delta R.T. 0.01 min

Lab File: VN062785.D

Acq: 7 Aug 2020 17:40

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#02

Tot Ion: 84 Resp: 13419

Ion Ratio Lower Upper

84 100

49 113.8 103.4 155.2

51 36.9 29.3 43.9





86 64.0 49.9 74.9

Abundance Ion 83.90 (83.60 to 84.60): VN0

Ion 48.90 (48.60 to 49.60): VN0

Ion 50.90 (50.60 to 51.60): VN0

Ion 85.90 (85.60 to 86.60): VN0

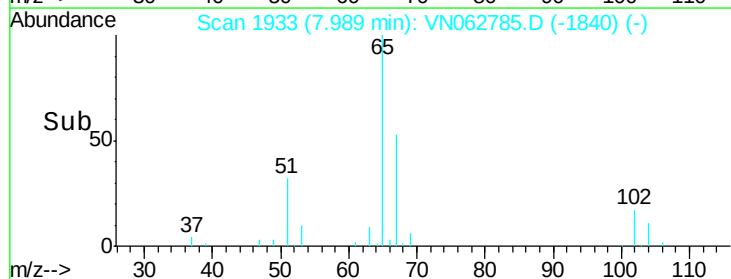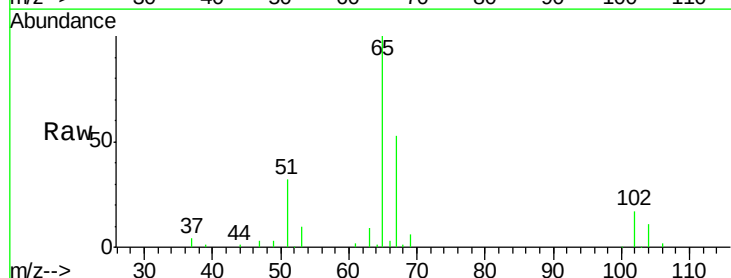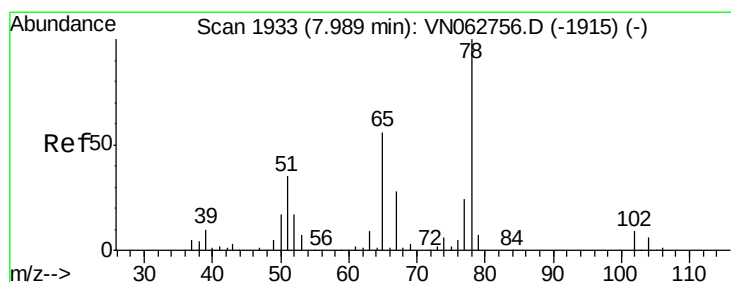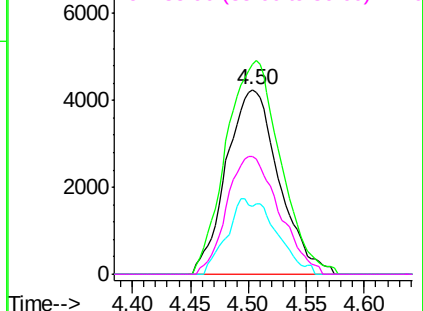

#33

1,2-Dichloroethane-d4

Concen: 52.452 ug/l

RT: 7.99 min Scan# 1933

Delta R.T. 0.00 min

Lab File: VN062785.D

Acq: 7 Aug 2020 17:40

Tgt Ion: 65 Resp: 112465


Ion Ratio Lower Upper


65 100

67 51.1 0.0 101.4

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

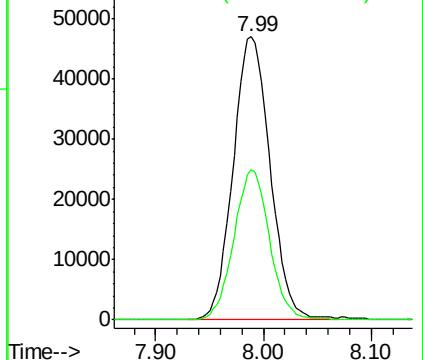

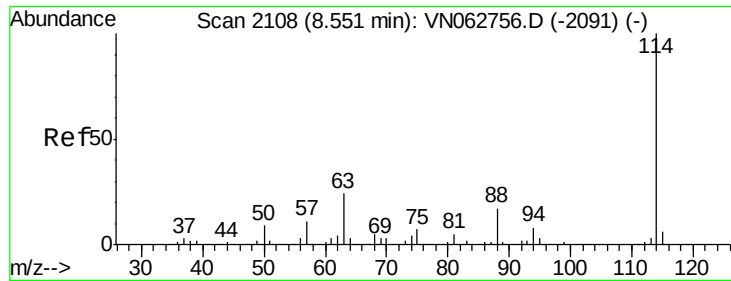

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2108

Delta R.T. 0.00 min

Lab File: VN062785.D

Acq: 7 Aug 2020 17:40

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#02


Tot Ion:114 Resp: 233606

Ion Ratio Lower Upper

114 100

63 22.4 0.0 47.6




88 17.2 0.0 34.4

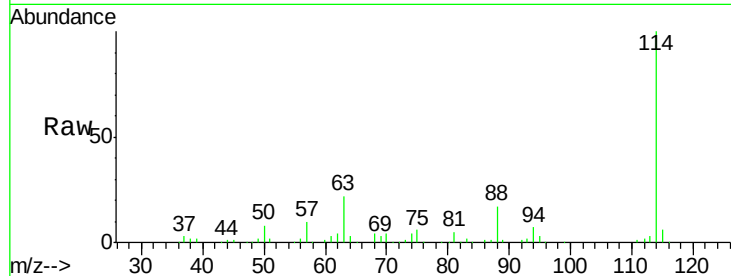

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0

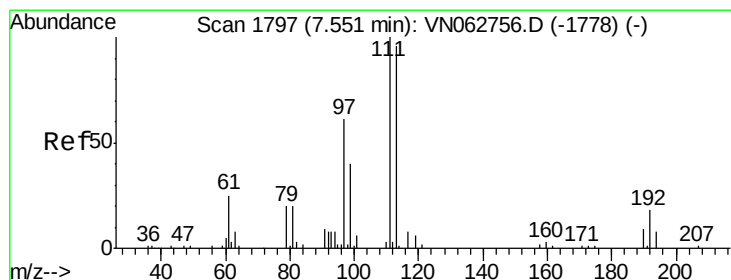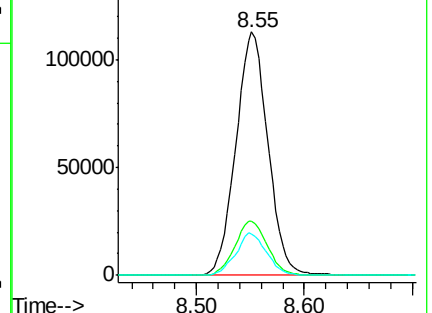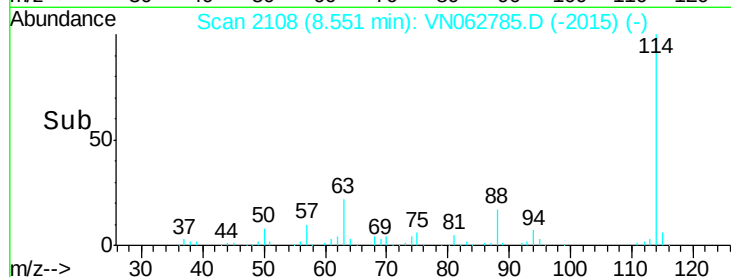

#35

Dibromofluoromethane

Concen: 51.066 ug/l

RT: 7.55 min Scan# 1797

Delta R.T. 0.00 min

Lab File: VN062785.D

Acq: 7 Aug 2020 17:40


Tgt Ion:113 Resp: 81603

Ion Ratio Lower Upper

113 100

111 102.7 81.8 122.6



192 18.4 15.0 22.4

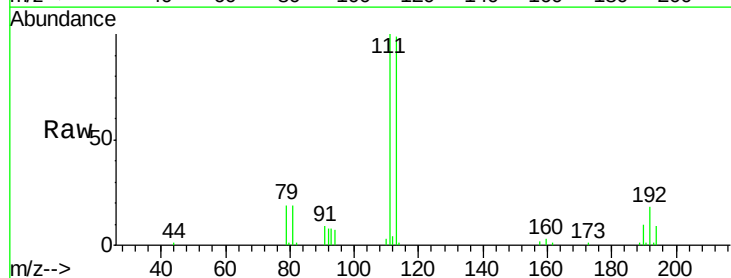


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

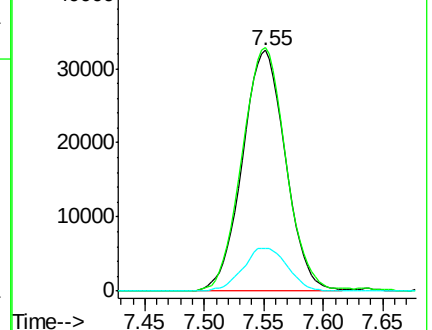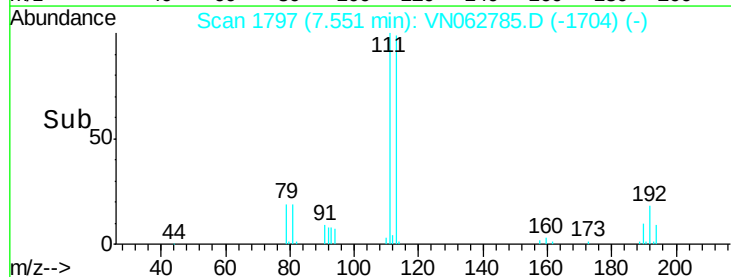

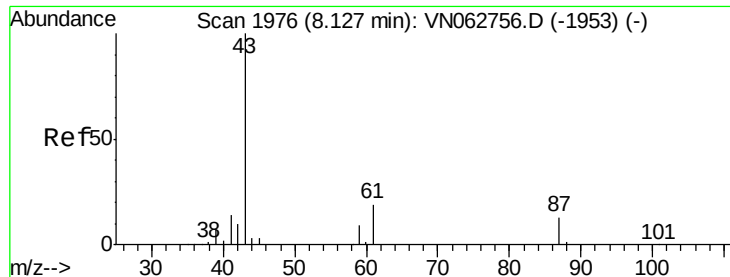

#43

Isopropyl Acetate

Concen: 12.080 ug/l

RT: 8.13 min Scan# 1977

Delta R.T. 0.00 min

Lab File: VN062785.D

Acq: 7 Aug 2020 17:40

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#02


Tot Ion: 43 Resp: 47876

Ion Ratio Lower Upper

43 100

61 18.8 15.8 23.6




87 12.2 9.9 14.9

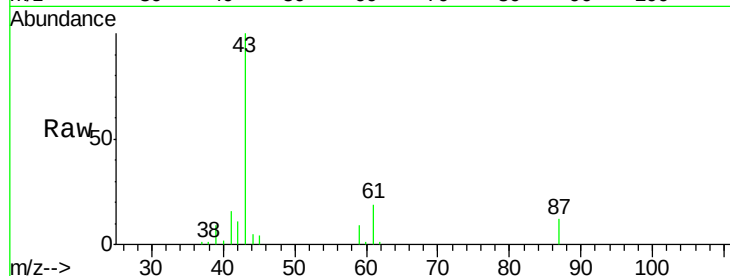

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

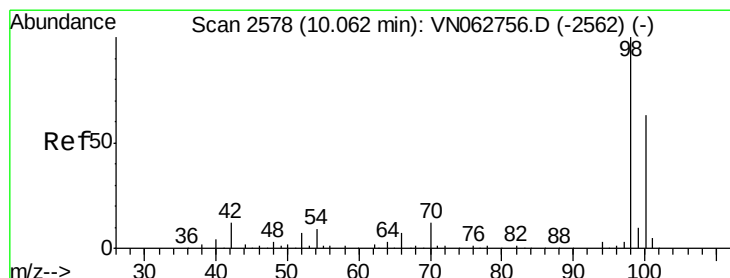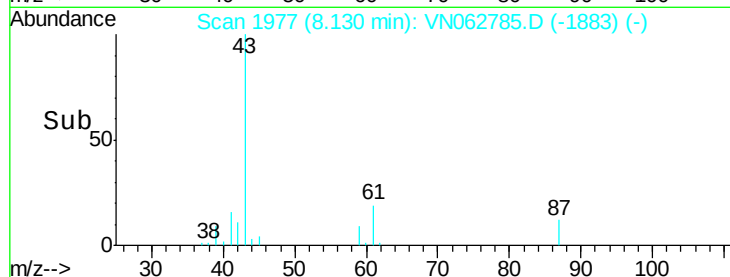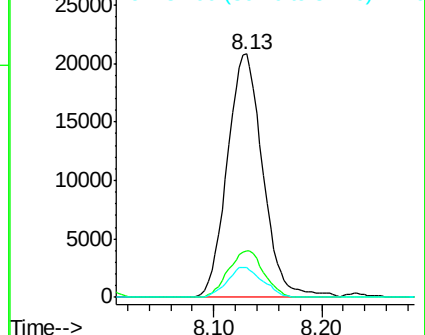

#50

Toluene-d8

Concen: 50.134 ug/l

RT: 10.06 min Scan# 2578

Delta R.T. 0.00 min

Lab File: VN062785.D


Acq: 7 Aug 2020 17:40

Tgt Ion: 98 Resp: 312774

Ion Ratio Lower Upper



98 100


100 64.6 50.9 76.3

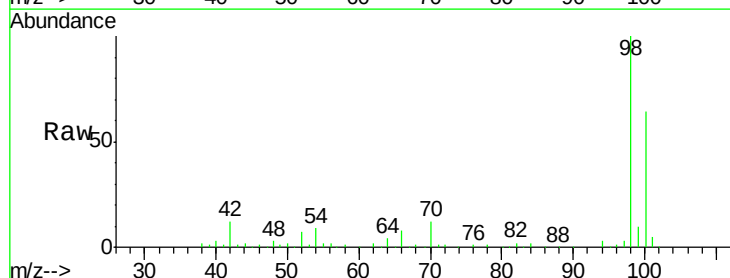

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0

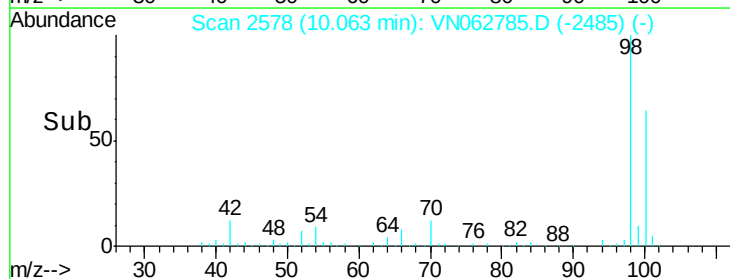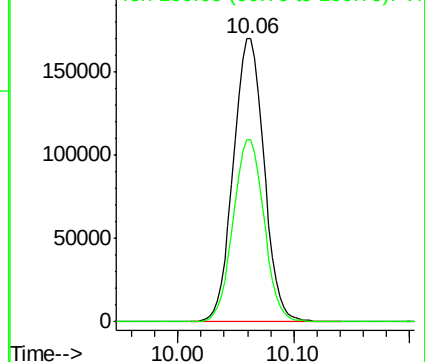

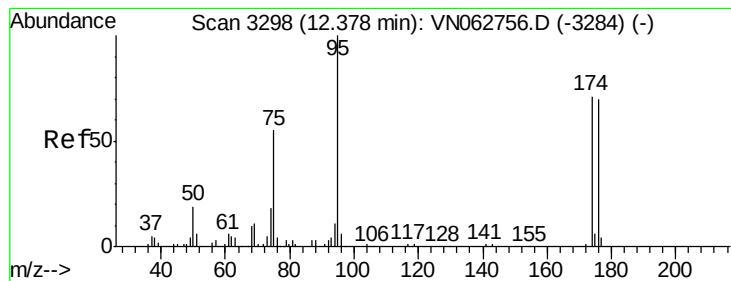

#62

4-Bromofluorobenzene

Concen: 47.391 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.00 min

Lab File: VN062785.D

Acq: 7 Aug 2020 17:40

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#02


Tot Ion: 95 Resp: 111730

Ion Ratio Lower Upper

95 100

174 74.7 0.0 144.8




176 72.0 0.0 142.2

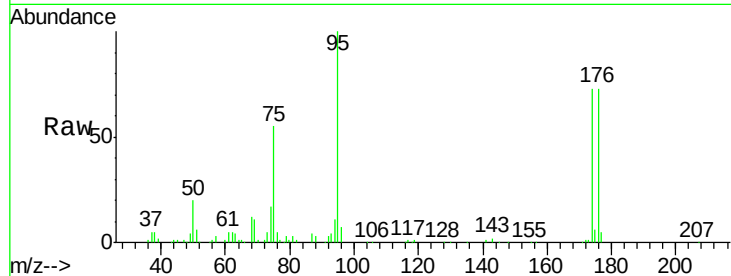

Abundance Ion 94.90 (94.60 to 95.60): VN062785.D (-3205) (-)

Ion 173.80 (173.50 to 174.50): VN062785.D (-3205) (-)

Ion 175.80 (175.50 to 176.50): VN062785.D (-3205) (-)

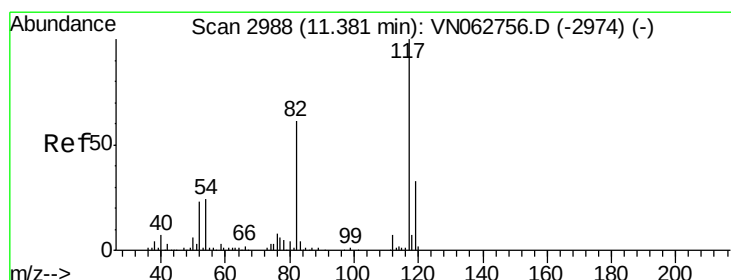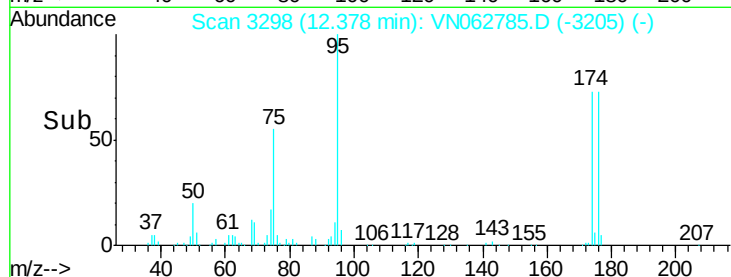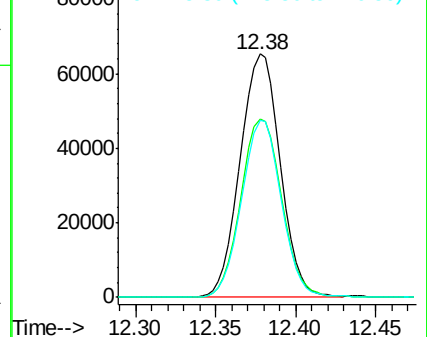

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2988

Delta R.T. 0.00 min

Lab File: VN062785.D

Acq: 7 Aug 2020 17:40


Tgt Ion: 117 Resp: 247166

Ion Ratio Lower Upper

117 100

82 60.9 49.0 73.4



119 32.2 26.2 39.2

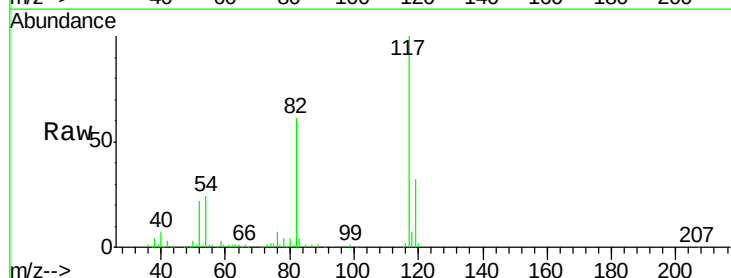


Abundance Ion 116.90 (116.60 to 117.60): VN062785.D (-2895) (-)

Ion 82.00 (81.70 to 82.70): VN062785.D (-2895) (-)

Ion 118.90 (118.60 to 119.60): VN062785.D (-2895) (-)

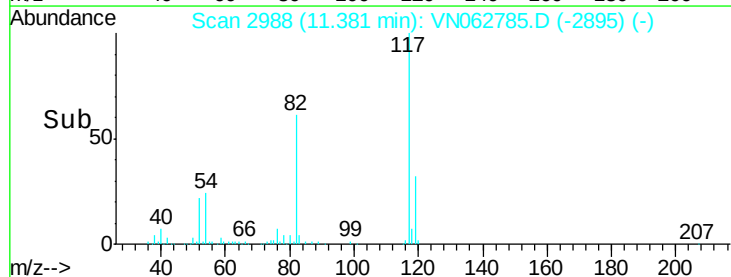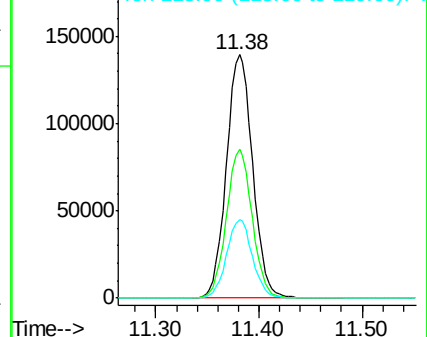

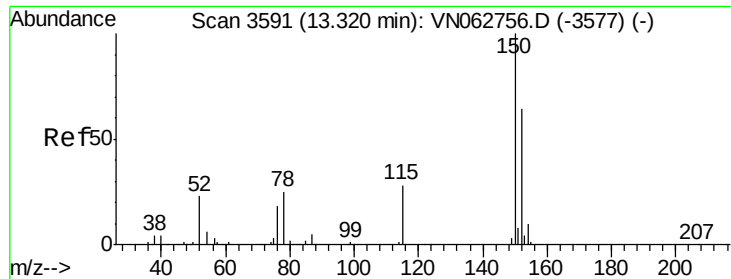

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN062785.D

Acq: 7 Aug 2020 17:40

Instrument :

MSVOA_N

ClientSampleId :

PB130790ZHE#02


Tot Ion:152 Resp: 85221

Ion Ratio Lower Upper

152 100

115 64.1 31.6 94.8

150 159.6 0.0 349.2

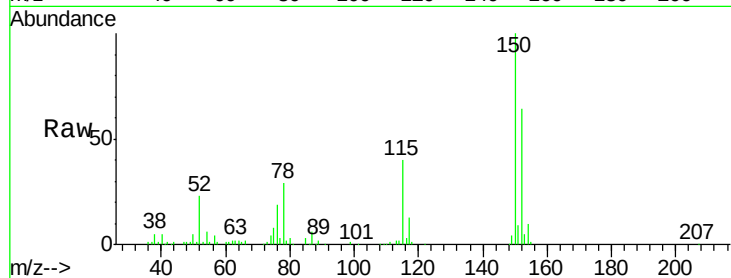

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

