


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN080720\
 Data File : VN062776.D
 Acq On : 7 Aug 2020 9:27
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N080520W.M
 Title : SW846 8260
 Last Update : Wed Aug 05 13:26:42 2020

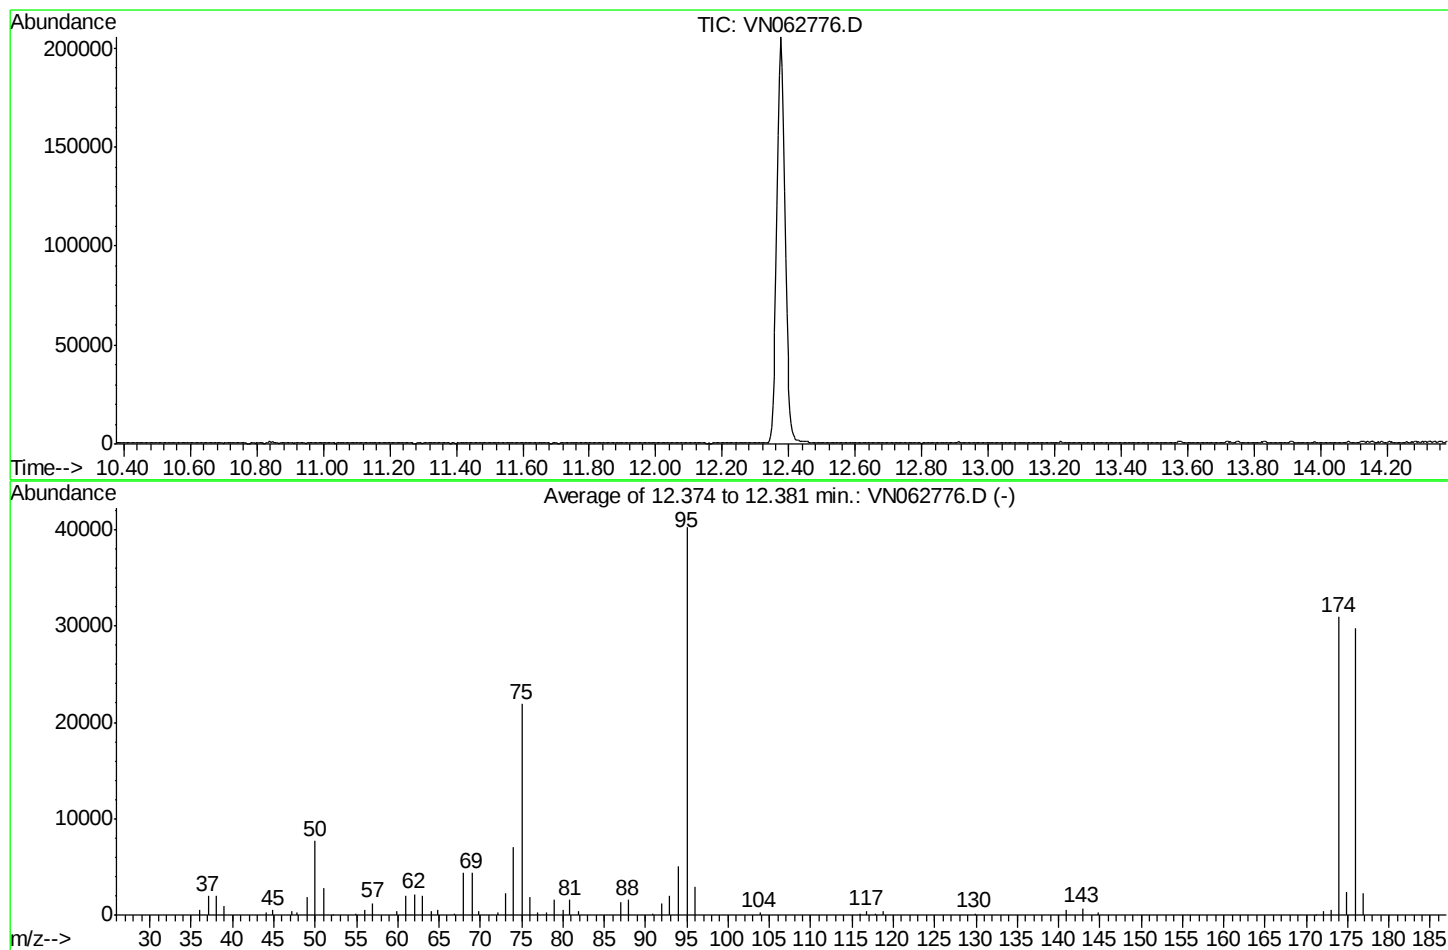

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	7651	PASS
75	95	30	60	54.4	21877	PASS
95	95	100	100	100.0	40248	PASS
96	95	5	9	7.2	2903	PASS
173	174	0.00	2	1.6	504	PASS
174	95	50	100	76.8	30922	PASS
175	174	5	9	7.7	2370	PASS
176	174	95	101	96.4	29821	PASS
177	176	5	9	7.5	2238	PASS