
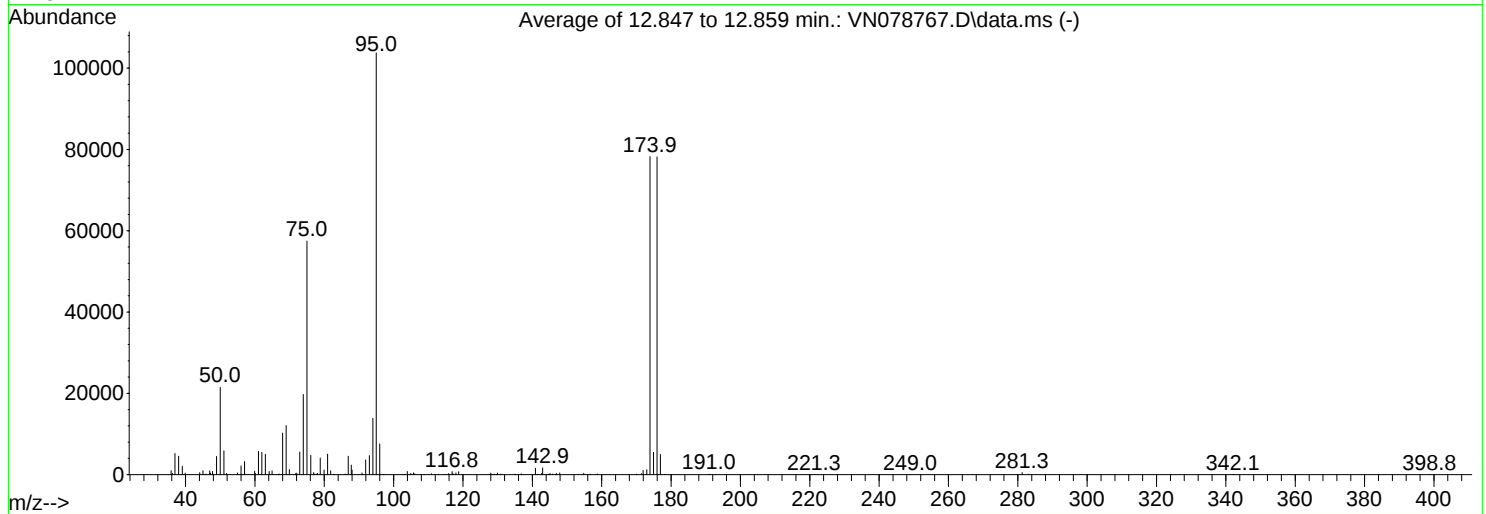


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080723\
Data File : VN078767.D
Acq On : 07 Aug 2023 09:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080723W.M
Title : SW846 8260
Last Update : Tue Aug 08 05:03:52 2023

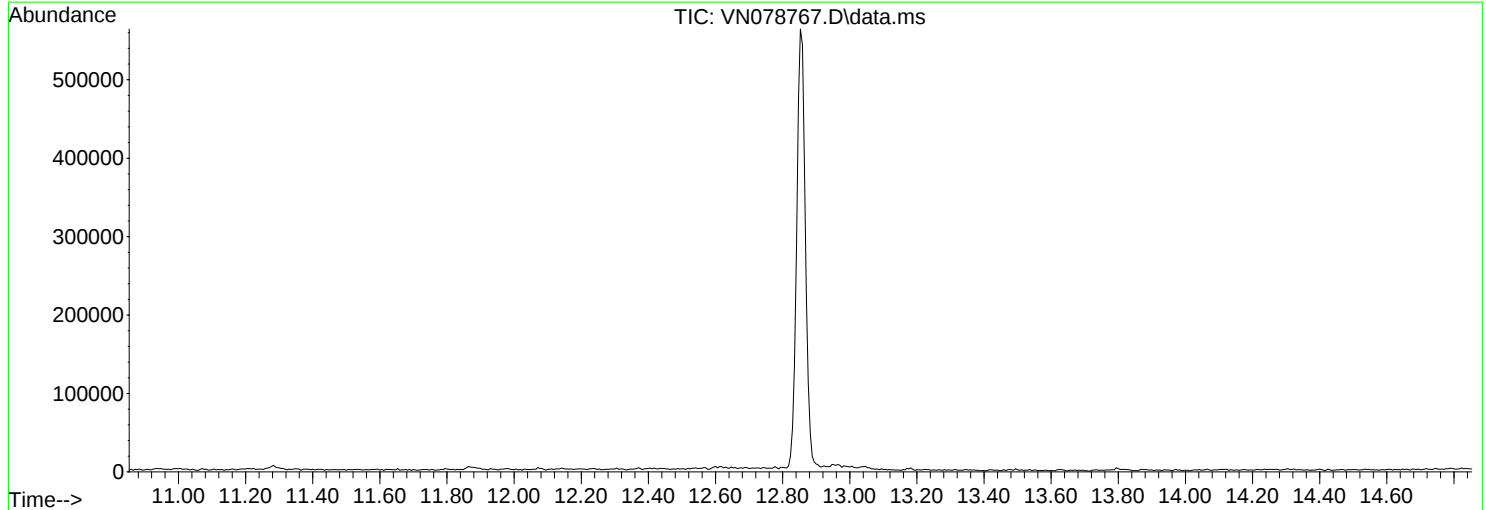

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	21456	PASS
75	95	30	60	55.4	57472	PASS
95	95	100	100	100.0	103763	PASS
96	95	5	9	7.3	7545	PASS
173	174	0.00	2	1.6	1227	PASS
174	95	50	100	75.4	78251	PASS
175	174	5	9	7.0	5507	PASS
176	174	95	101	99.9	78184	PASS
177	176	5	9	6.4	4978	PASS

Average of 12.847 to 12.859 min.: VN078767.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	992	47.80	778	62.00	5466	72.10	411
36.20	335	48.95	4495	63.00	5018	72.95	554
36.95	5200	50.00	21456	64.10	804	73.95	1972
38.00	4517	51.05	5865	64.95	933	75.00	5747
39.05	2045	51.85	296	66.10	55	76.10	4777
39.90	397	55.00	446	66.80	119	76.95	502
44.10	523	56.00	2180	67.00	160	77.20	105
45.00	976	57.00	3250	68.00	10243	77.70	141
45.90	163	59.90	874	69.00	12086	78.05	318
46.95	961	60.10	324	69.95	1268	78.85	4113
47.20	362	61.05	5697	71.80	332	79.95	1144

Average of 12.847 to 12.859 min.: VN078767.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.95	5023	95.00	103763	110.90	255	128.00	395
81.85	964	96.00	7545	113.00	65	128.70	57
82.65	122	97.00	52	114.80	71	129.05	127
86.05	148	97.20	93	115.80	253	129.70	90
86.90	4524	102.70	53	116.00	139	129.95	399
87.80	2344	103.10	71	116.85	739	130.95	166
88.00	1162	103.95	792	117.10	257	134.75	117
90.90	447	104.95	306	117.95	445	135.10	69
91.95	3627	105.75	447	118.75	727	136.85	192
93.00	4697	106.10	184	124.10	56	140.90	1583
94.00	13856	108.80	95	127.50	59	141.60	90

Average of 12.847 to 12.859 min.: VN078767.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
141.80	73	158.75	171	192.80	59		
142.70	309	170.05	123	205.00	74		
142.95	1649	171.50	238	221.30	50		
144.70	127	171.95	1069	249.00	53		
145.10	275	173.00	1227	267.00	58		
145.85	176	173.95	78251	281.25	527		
146.70	111	174.95	5507	283.00	111		
147.00	291	175.95	78184	342.10	68		
147.90	446	176.95	4978	398.80	56		
154.85	349	178.10	64				
156.70	131	191.00	104				