
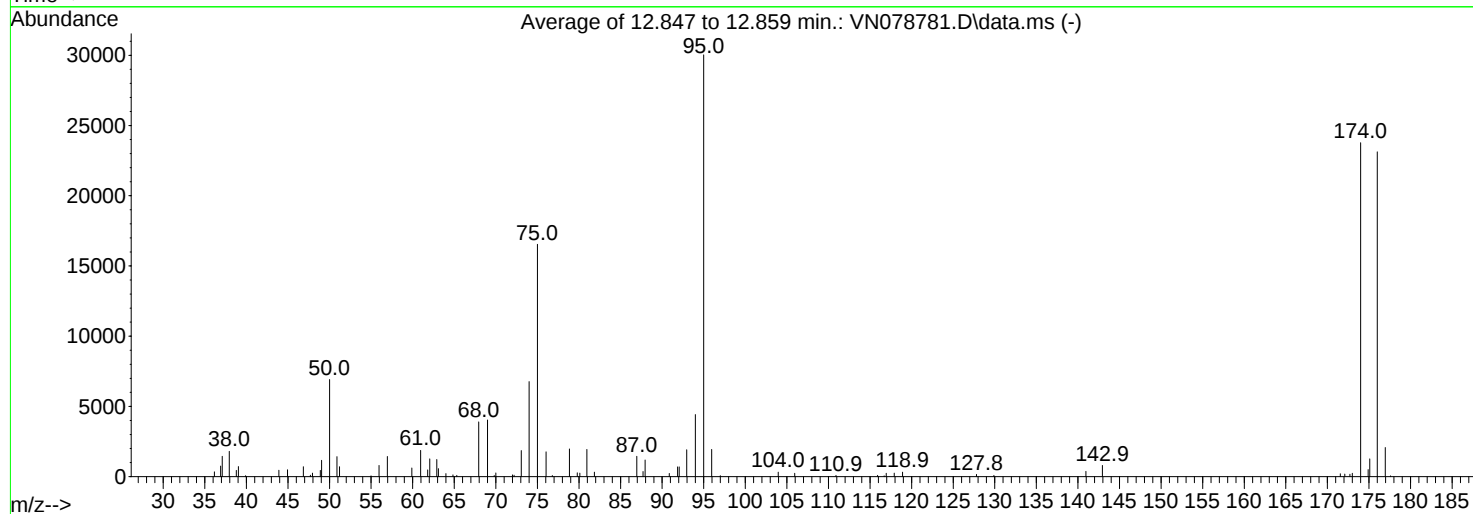


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080723\
Data File : VN078781.D
Acq On : 07 Aug 2023 17:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080723W.M
Title : SW846 8260
Last Update : Tue Aug 08 05:03:52 2023

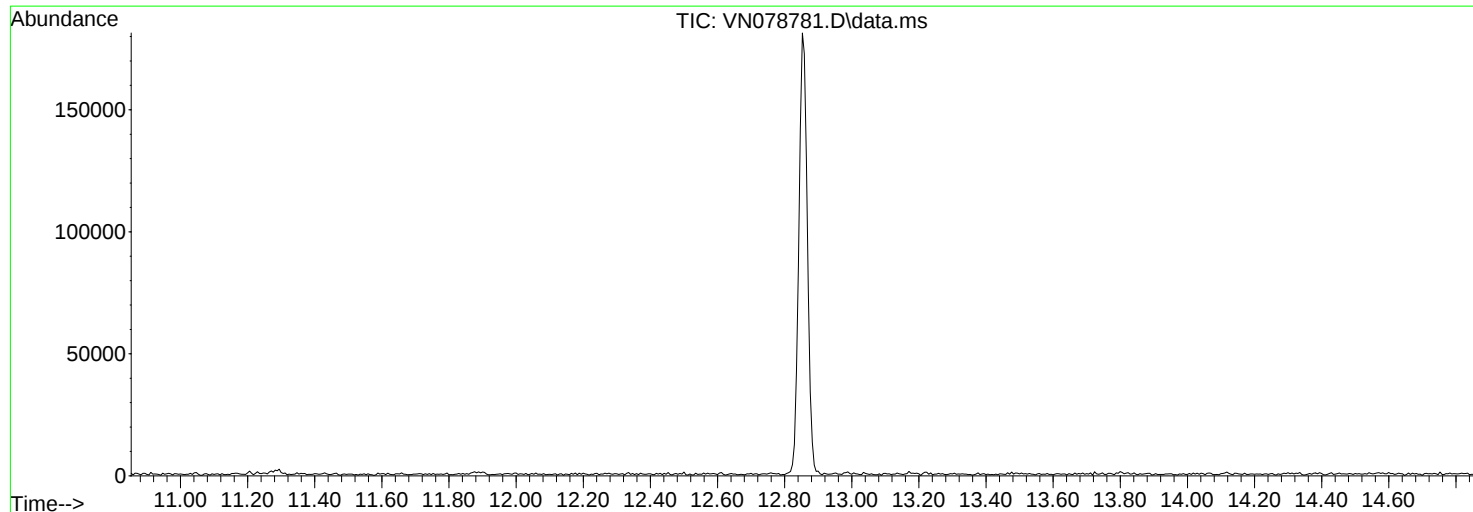

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	6920	PASS
75	95	30	60	55.1	16539	PASS
95	95	100	100	100.0	30032	PASS
96	95	5	9	6.4	1936	PASS
173	174	0.00	2	1.0	236	PASS
174	95	50	100	79.2	23776	PASS
175	174	5	9	5.3	1265	PASS
176	174	95	101	97.3	23128	PASS
177	176	5	9	8.9	2069	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.15	347	47.95	246	61.80	476	72.00	12
36.90	752	48.90	445	62.05	1261	72.20	10
37.10	1446	49.05	1164	62.90	1222	73.05	186
37.95	1804	50.00	6920	63.10	573	74.00	677
38.80	448	50.90	1429	64.00	212	75.00	16539
39.05	719	51.20	710	64.85	126	76.05	1768
39.90	65	55.00	59	65.30	88	76.80	75
43.90	451	55.95	799	67.95	3893	78.85	1969
44.95	489	56.95	1433	69.00	4029	79.80	277
46.85	701	59.90	620	69.80	82	80.10	254
47.70	104	60.95	1871	70.00	264	80.95	1939

Average of 12.847 to 12.859 min.: VN078781.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	314	97.00	71	140.95	374	177.60	56
86.95	1446	103.95	315	142.95	797		
87.70	364	105.95	238	171.55	208		
87.95	1188	110.90	88	172.10	179		
90.85	224	115.90	87	172.70	175		
91.85	700	116.70	59	173.00	236		
92.05	697	116.95	237	174.00	23776		
92.95	1910	117.90	255	174.90	502		
94.00	4426	118.90	324	175.10	1265		
95.00	30032	127.80	158	176.00	23128		
95.95	1936	129.90	91	176.95	2069		

Instrument :

MSVOA_N

ClientSampleId :

BFB