
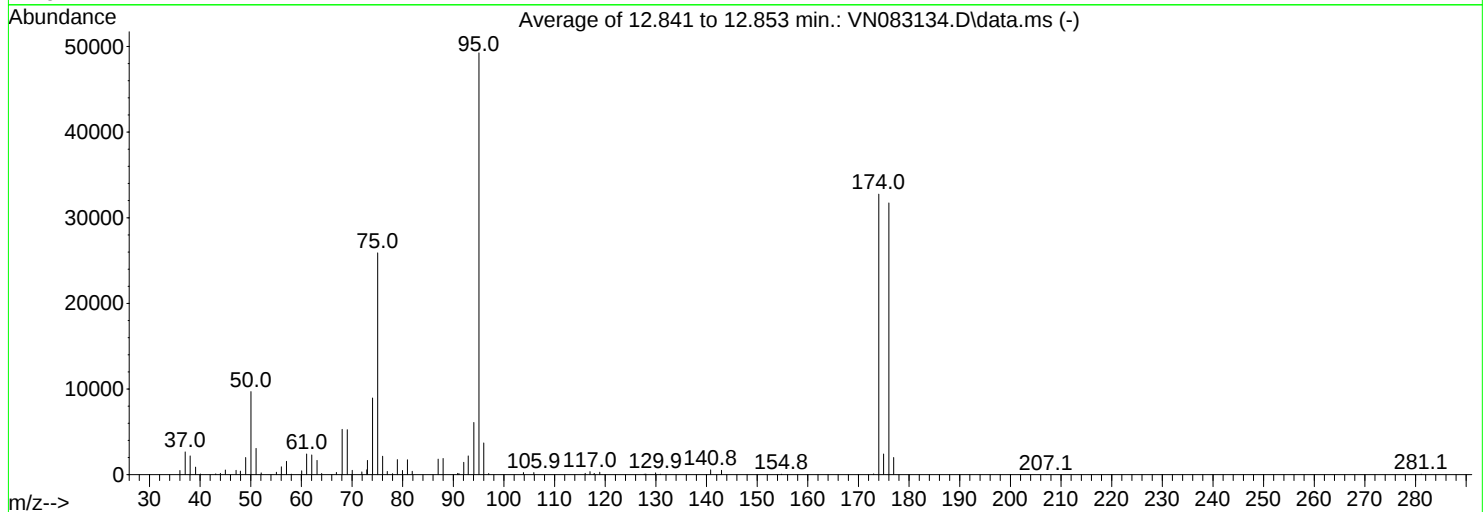


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080724\
Data File : VN083134.D
Acq On : 07 Aug 2024 10:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

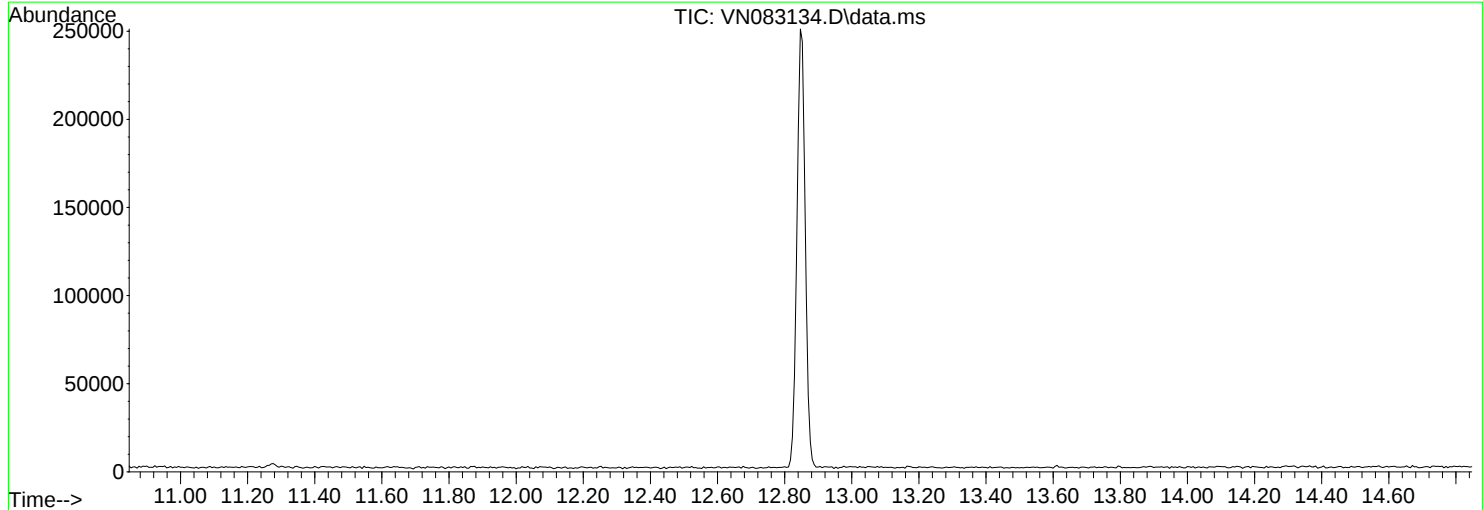

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	9690	PASS
75	95	30	60	52.6	25907	PASS
95	95	100	100	100.0	49259	PASS
96	95	5	9	7.5	3697	PASS
173	174	0.00	2	0.3	99	PASS
174	95	50	100	66.5	32749	PASS
175	174	5	9	7.4	2414	PASS
176	174	95	101	96.9	31720	PASS
177	176	5	9	6.3	1999	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	482	50.05	9690	64.00	127	76.95	379
37.05	2661	51.05	3059	66.90	264	78.00	111
38.05	2186	52.05	203	68.05	5282	78.95	176
39.10	878	55.05	280	69.05	5250	79.95	49
40.05	66	56.05	919	70.05	505	80.95	1731
43.10	90	57.05	1554	71.95	325	81.90	400
44.00	157	58.00	65	72.90	568	87.00	1822
45.00	540	60.05	458	73.05	1669	88.00	1894
47.10	511	61.05	2408	74.05	8942	90.85	148
47.95	415	62.05	2306	75.05	25907	91.10	125
49.00	1997	63.10	1656	76.05	2147	92.05	1444

Average of 12.841 to 12.853 min.: VN083134.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	2196	118.90	274	176.00	31720		
94.05	6092	127.70	54	176.95	1999		
95.05	49259	128.00	79	207.05	13		
96.00	3697	129.95	202	281.10	54		
97.00	129	130.90	61				
103.85	253	140.80	554				
105.90	250	142.95	497				
116.05	155	154.80	55				
117.00	348	173.00	99				
117.70	61	174.00	32749				
117.85	141	174.95	2414				

Instrument :

MSVOA_N

ClientSampleId :

BFB