


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080822\
 Data File : VN073765.D
 Acq On : 08 Aug 2022 12:01
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N072722W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Jul 27 18:07:26 2022

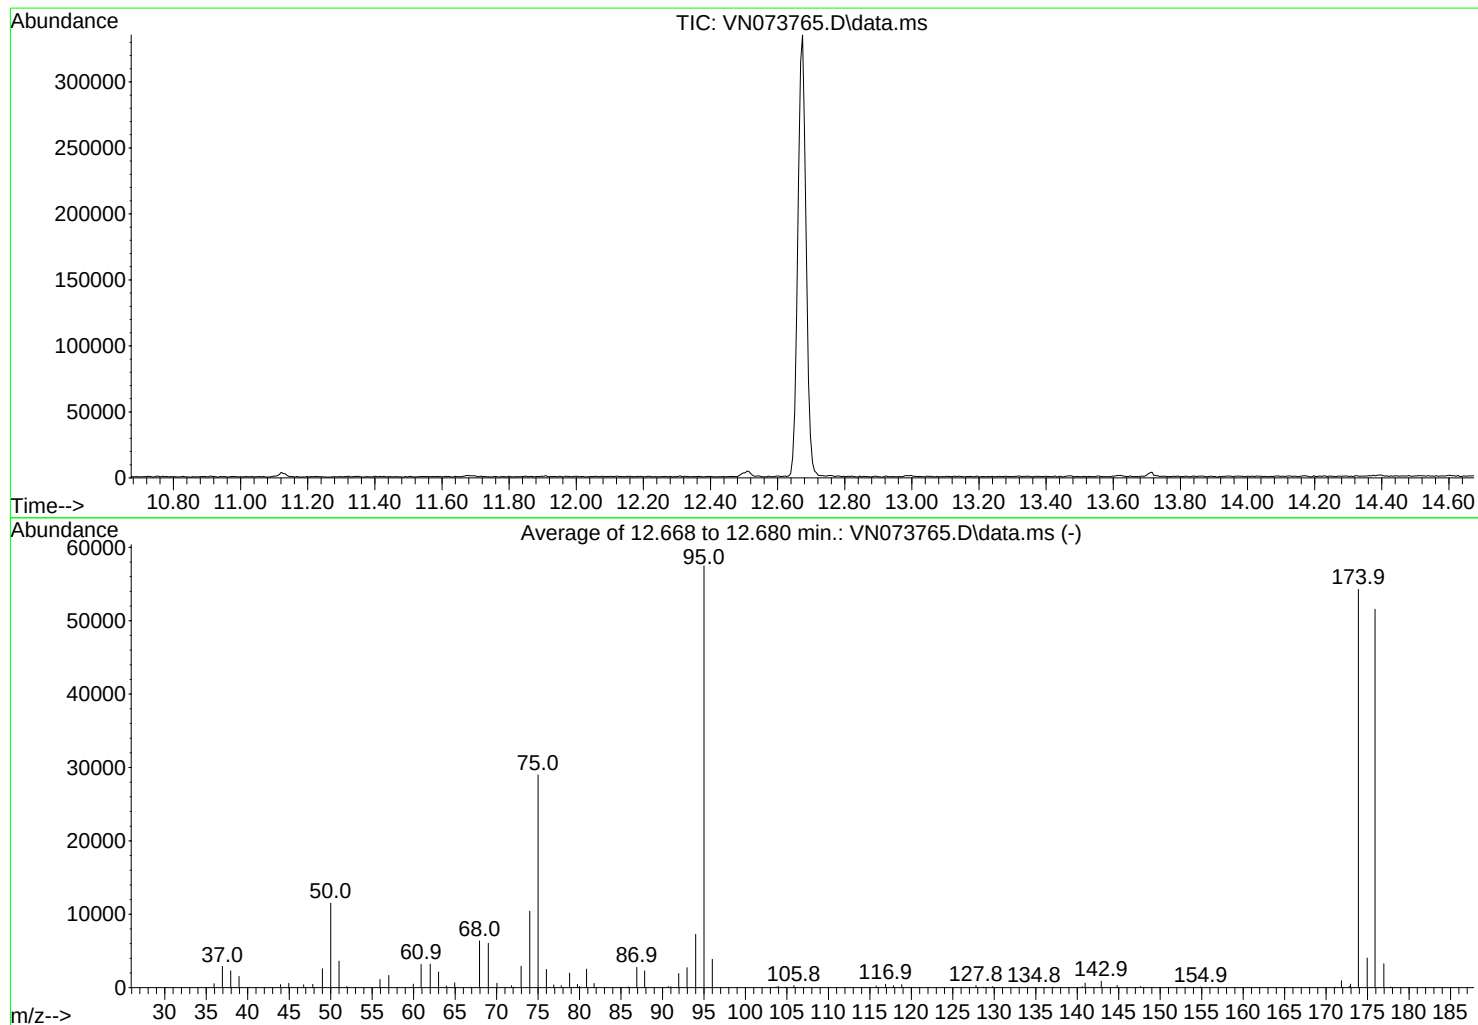

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	11508	PASS
75	95	30	60	50.4	28992	PASS
95	95	100	100	100.0	57475	PASS
96	95	5	9	6.7	3854	PASS
173	174	0.00	2	0.9	484	PASS
174	95	50	100	94.4	54272	PASS
175	174	5	9	7.4	4028	PASS
176	174	95	101	95.0	51573	PASS
177	176	5	9	6.3	3259	PASS