
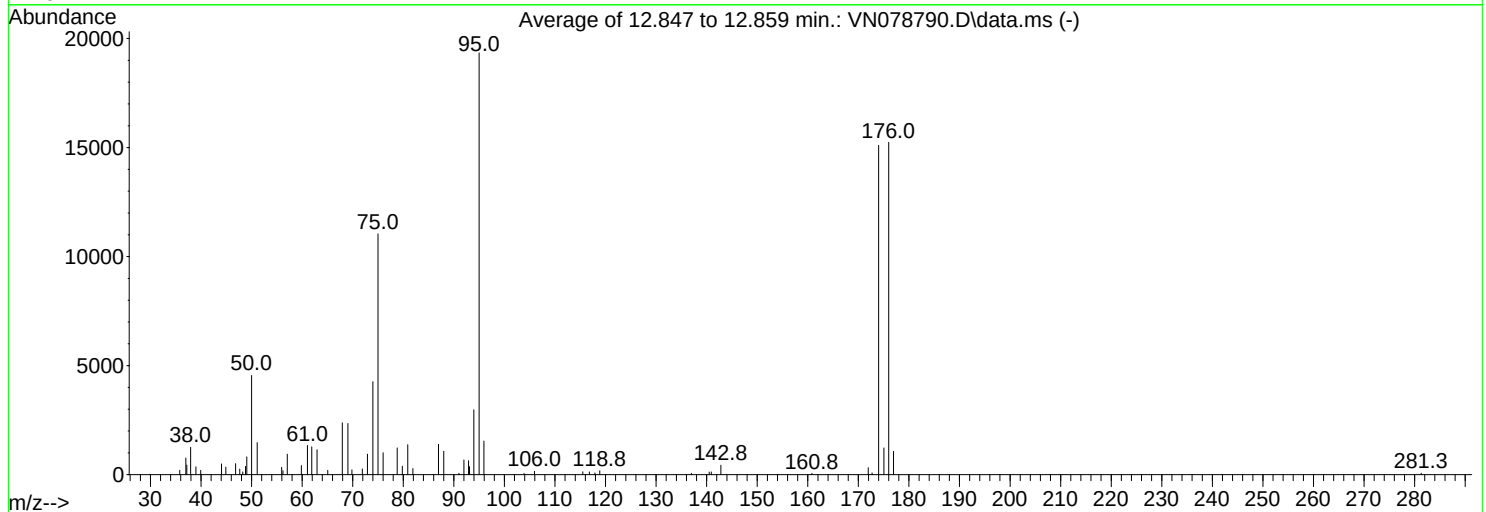


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080823\
Data File : VN078790.D
Acq On : 08 Aug 2023 08:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080723W.M
Title : SW846 8260
Last Update : Tue Aug 08 05:03:52 2023

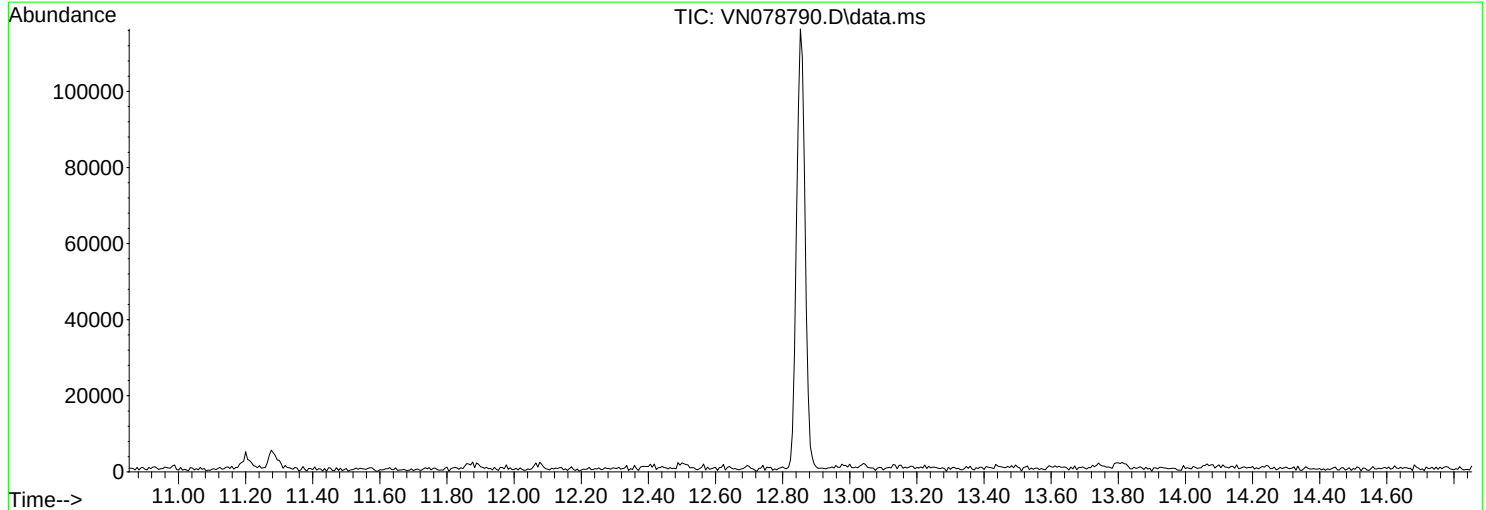

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	4553	PASS
75	95	30	60	57.1	11046	PASS
95	95	100	100	100.0	19344	PASS
96	95	5	9	8.0	1538	PASS
173	174	0.00	2	0.6	84	PASS
174	95	50	100	78.1	15101	PASS
175	174	5	9	8.1	1224	PASS
176	174	95	101	100.9	15239	PASS
177	176	5	9	7.0	1074	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	196	48.80	382	65.05	195	80.90	1377
37.00	763	49.05	813	67.95	2380	81.90	280
37.20	443	50.00	4553	69.05	2345	86.95	139
37.95	1252	51.10	1465	69.85	220	88.00	106
39.00	361	55.95	336	71.90	267	91.00	66
39.95	195	56.20	180	72.90	936	92.00	673
44.05	494	57.05	940	74.00	4265	92.90	641
44.90	347	59.85	416	75.00	11046	93.10	369
46.85	503	61.05	1342	76.00	1007	93.95	2969
47.65	255	61.90	1279	78.80	1222	95.00	19344
48.25	128	62.95	1147	79.80	390	95.95	1538

Average of 12.847 to 12.859 min.: VN078790.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.90	60	171.95	317				
105.95	157	172.70	84				
115.50	130	174.00	15101				
116.80	123	175.05	1224				
117.90	83	176.00	15239				
118.85	179	176.95	1074				
137.00	60	281.30	66				
140.50	121						
140.90	123						
142.80	432						
160.80	58						

Instrument :

MSVOA_N

ClientSampleId :

BFB