
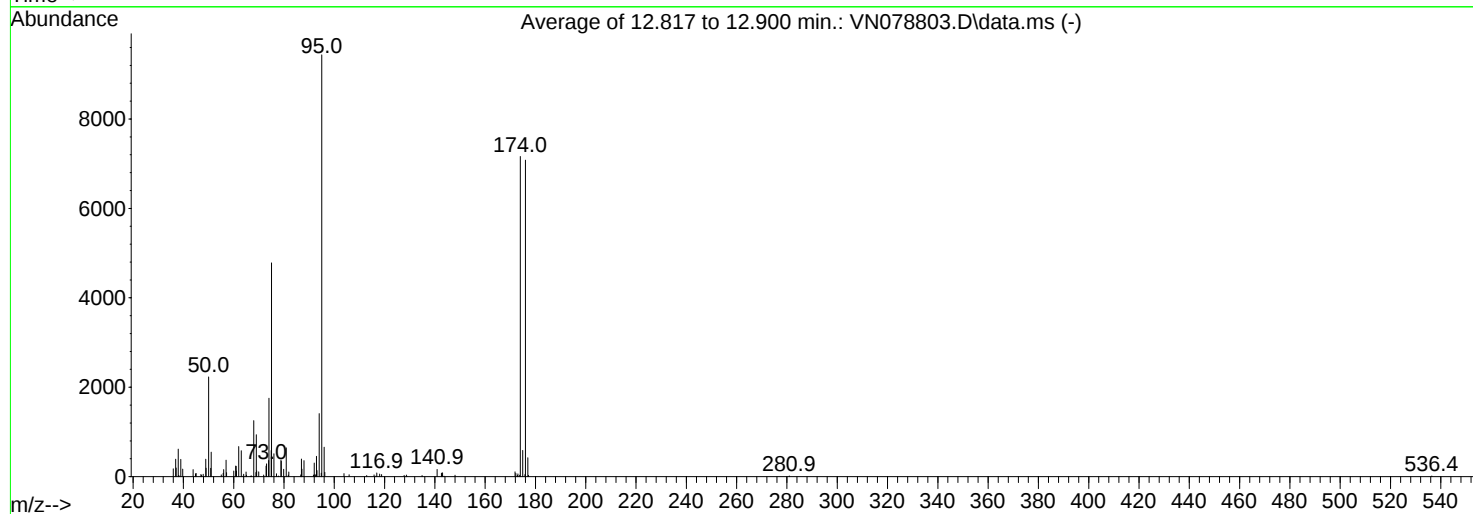


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080823\
 Data File : VN078803.D
 Acq On : 08 Aug 2023 17:18
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080823W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Aug 09 05:05:47 2023

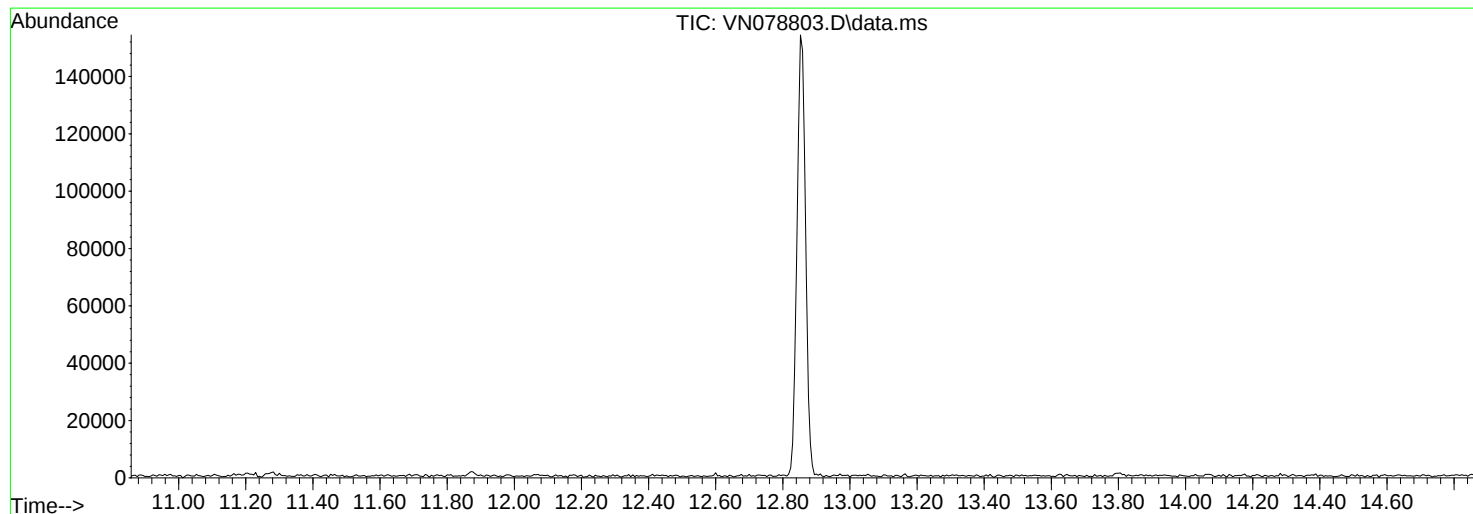

AutoFind: Averaged scan 1847 to 1861; Bkg corrected with scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	2229	PASS
75	95	30	60	50.7	4783	PASS
95	95	100	100	100.0	9435	PASS
96	95	5	9	7.0	657	PASS
173	174	0.00	2	0.9	61	PASS
174	95	50	100	75.9	7161	PASS
175	174	5	9	8.2	587	PASS
176	174	95	101	98.9	7079	PASS
177	176	5	9	6.0	424	PASS