


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080824\
Data File : VN083143.D
Acq On : 08 Aug 2024 08:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

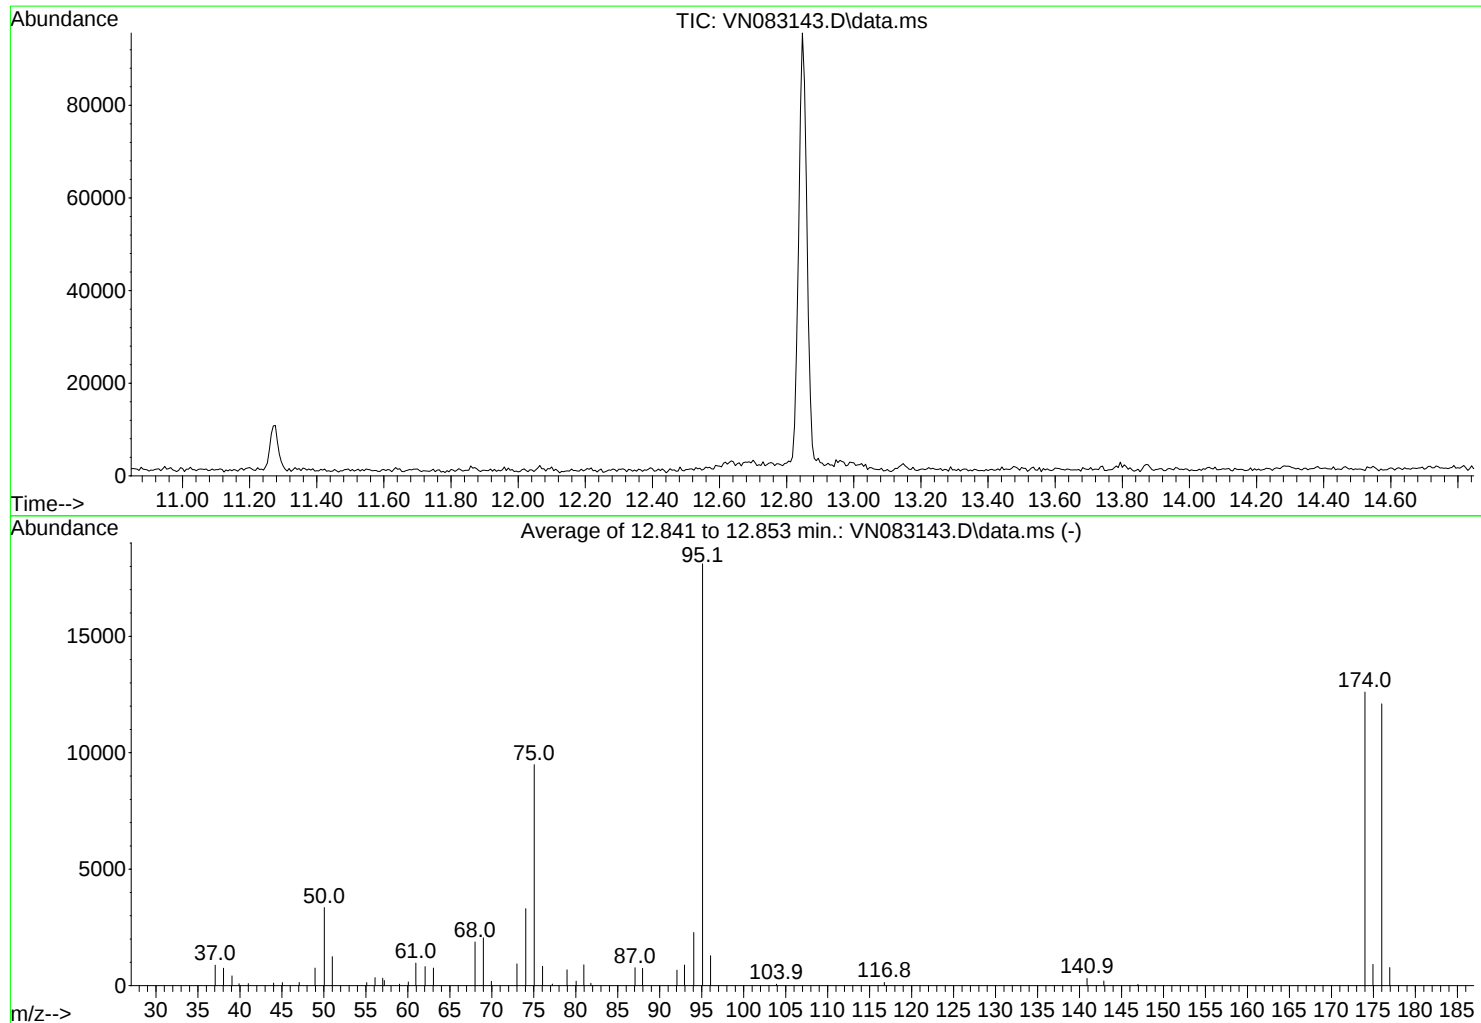

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	3354	PASS
75	95	30	60	52.4	9489	PASS
95	95	100	100	100.0	18110	PASS
96	95	5	9	7.1	1287	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.6	12604	PASS
175	174	5	9	7.3	917	PASS
176	174	95	101	96.0	12097	PASS
177	176	5	9	6.4	777	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
37.05	882	55.10	132	69.95	186	87.95	731
38.05	748	56.10	342	73.00	936	92.05	661
39.05	418	57.00	319	74.05	3308	92.95	881
39.90	82	57.20	221	75.05	9489	94.05	227
41.00	89	59.00	63	76.05	831	95.10	18110
44.00	112	60.05	159	77.20	67	96.05	1287
45.05	133	60.95	968	78.95	683	103.90	60
47.05	140	62.05	821	80.05	190	116.75	138
48.95	756	63.05	754	80.95	892	140.90	310
50.05	3354	68.00	1874	81.80	104	142.90	198
51.00	1242	69.00	2053	87.05	769	146.95	56

Average of 12.841 to 12.853 min.: VN083143.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.00	12604						
174.95	917						
176.00	12097						
176.95	777						

Instrument :

MSVOA_N

ClientSampleId :

BFB